

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
 Data File : PS000937.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2018 12:51
 Operator : UA
 Sample : J3908-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 15:11:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.676	11.089	46561211	47094426	225.675	216.231
Target Compounds							
1) T	Dalapon	3.013	2.449	6792570	769206	25.297	2.855 #
2) T	3,5-DICHL...	0.000	9.175	0	4411661	N.D.	14.998 #
5) T	DICAMBA	0.000	11.333	0	4887815	N.D.	6.227 #
6) T	MCP	12.372	0.000	9602083	0	17.481	N.D. #
8) T	DICHLORPROP	0.000	12.459	0	1690440	N.D.	8.369 #
10) T	Pentachlo...	0.000	13.452	0	3297240	N.D.	1.051 #
11) T	2,4,5-TP ...	0.000	14.069	0	11309513	N.D.	9.012 #
12) T	2,4,5-T	0.000	14.670	0	1415738	N.D.	1.368 #
14) T	DINOSEB	0.000	15.816	0	4746722	N.D.	5.668 #
15) T	Picloram	0.000	16.956	0	2067216	N.D.	1.358 #
16) T	DCPA	0.000	16.956	0	2067216	N.D.	1.202 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
Data File : PS000937.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2018 12:51
Operator : UA
Sample : J3908-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 15:11:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

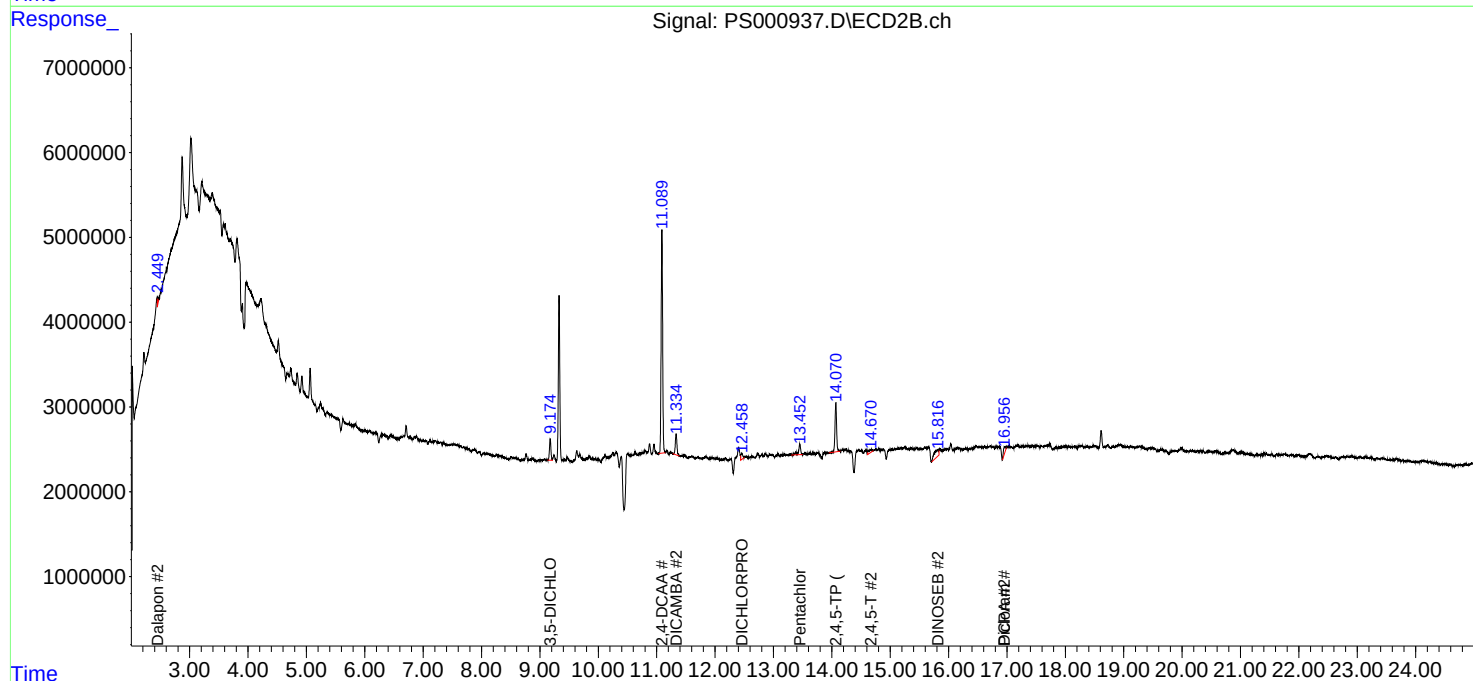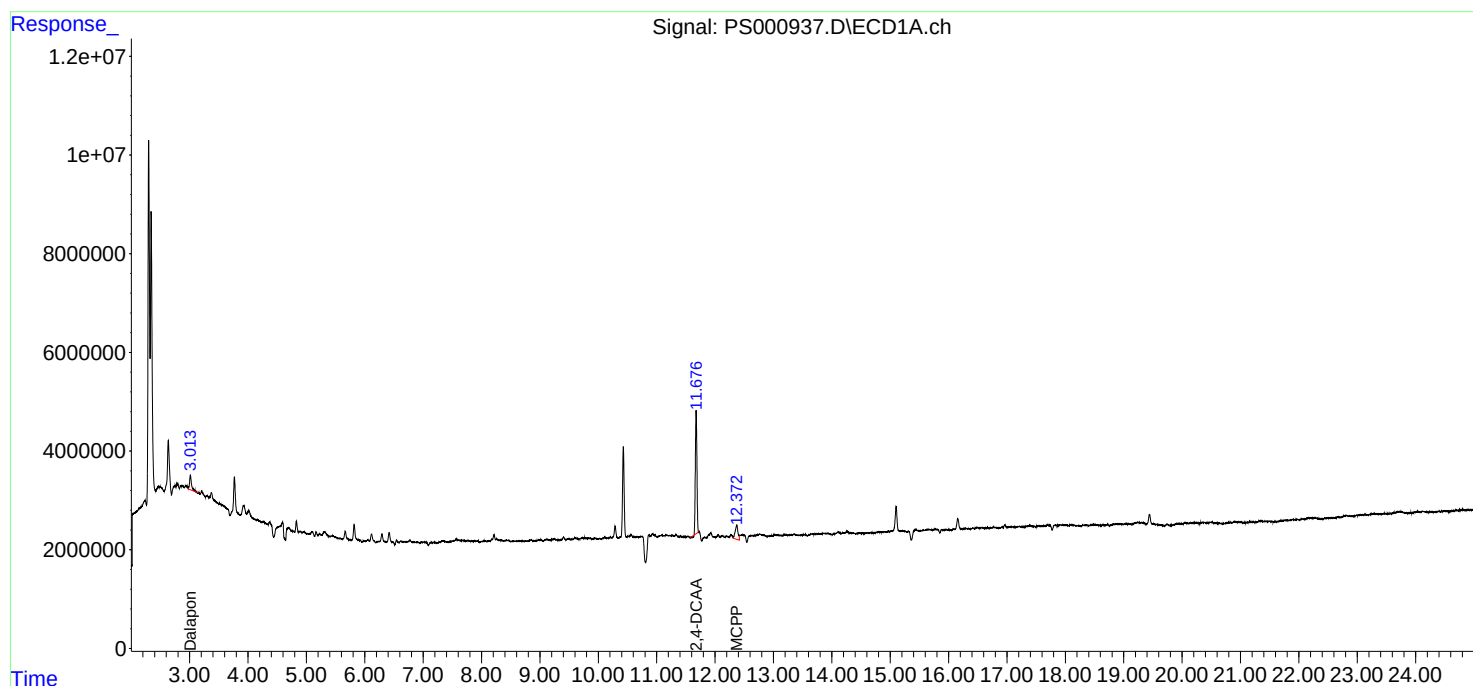


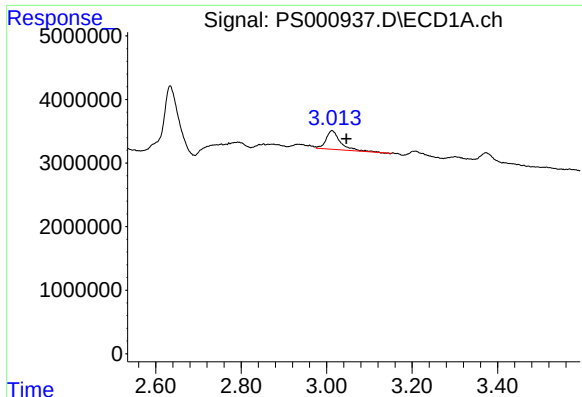

#1 Dalapon


R.T.: 3.013 min
Delta R.T.: -0.033 min
Response: 6792570
Conc: 25.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

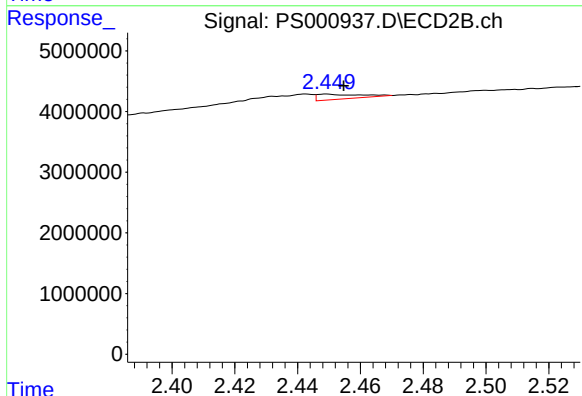


#1 Dalapon

R.T.: 2.449 min
Delta R.T.: -0.005 min
Response: 769206
Conc: 2.85 ng/ml

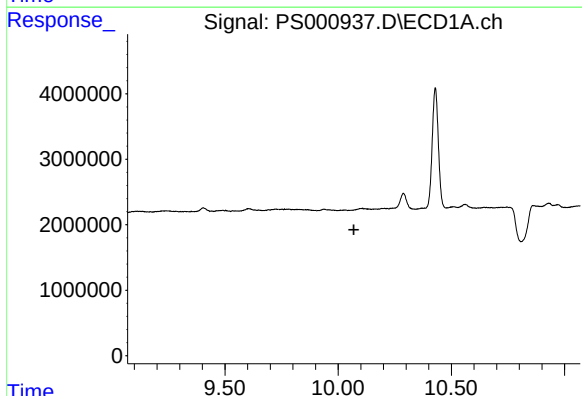


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

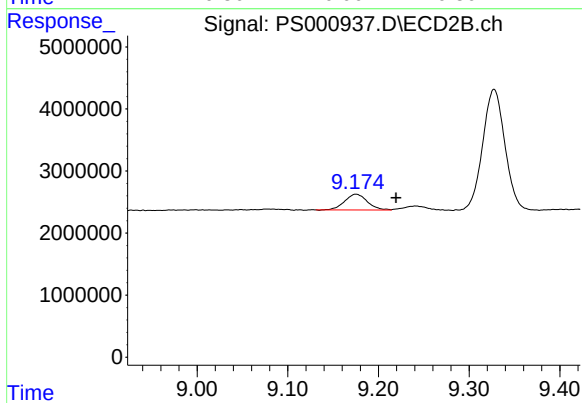

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.175 min
Delta R.T.: -0.044 min
Response: 4411661
Conc: 15.00 ng/ml

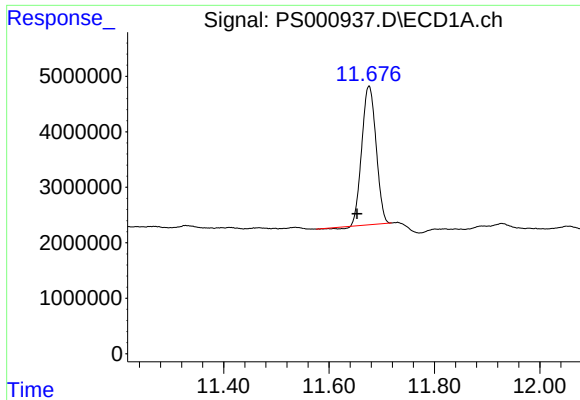

#4 2,4-DCAA


R.T.: 11.676 min
Delta R.T.: 0.022 min
Response: 46561211
Conc: 225.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

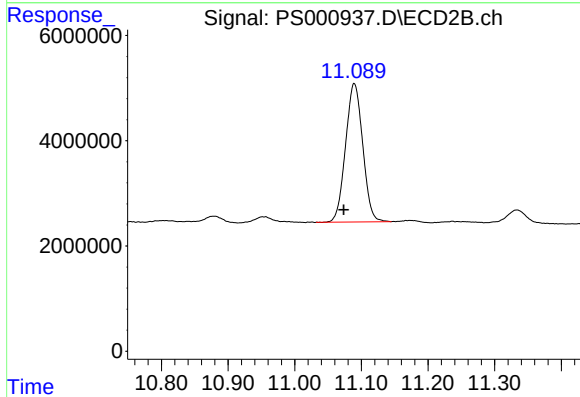


#4 2,4-DCAA

R.T.: 11.089 min
Delta R.T.: 0.016 min
Response: 47094426
Conc: 216.23 ng/ml

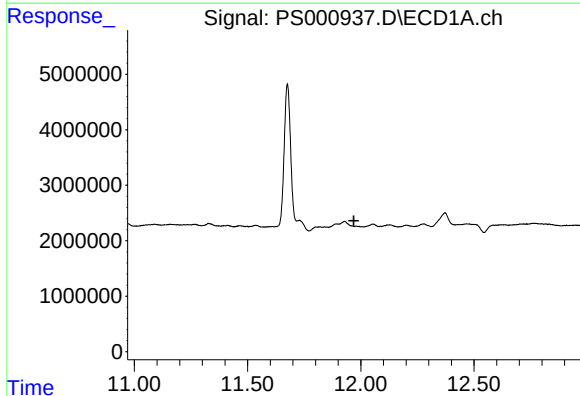


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.970 min
Response: 0
Conc: N.D.

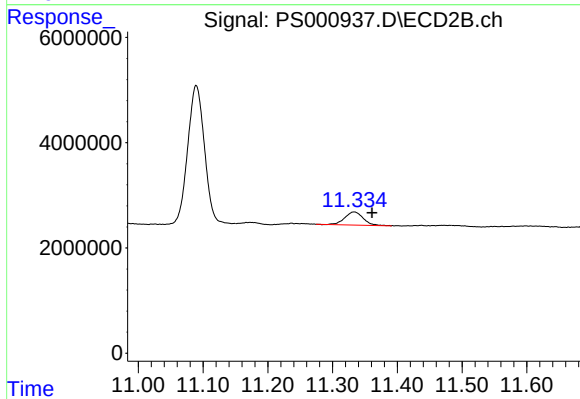

#5 DICAMBA


R.T.: 11.333 min
Delta R.T.: -0.028 min
Response: 4887815
Conc: 6.23 ng/ml

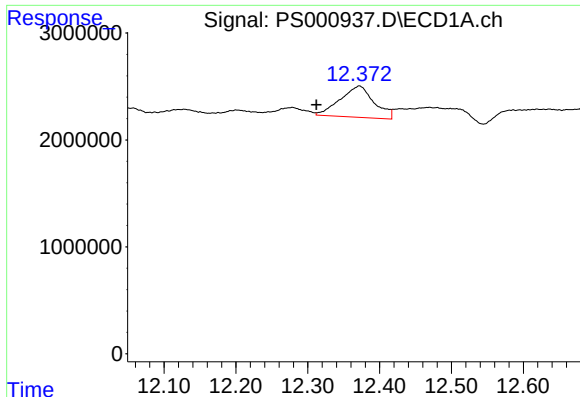

#6 MCP


R.T.: 12.372 min
Delta R.T.: 0.060 min
Response: 9602083
Conc: 17.48 ug/ml

Instrument :
ECD_S
ClientSampleId :

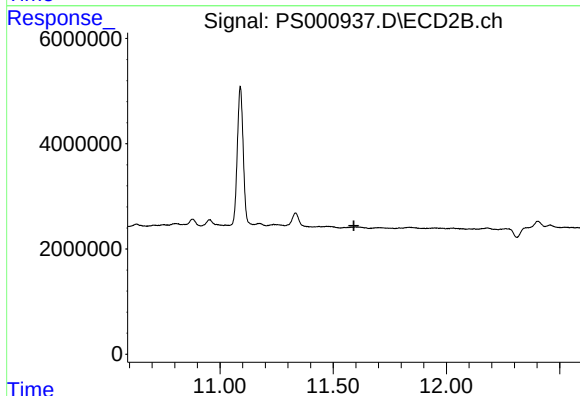


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

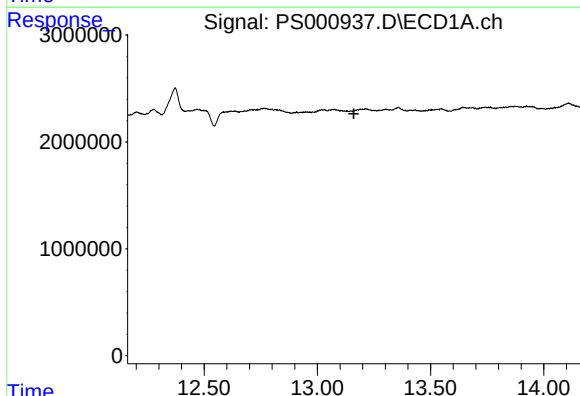


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

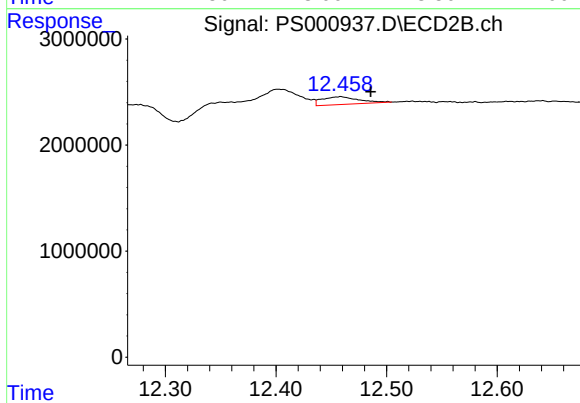

#8 DICHLORPROP


R.T.: 12.459 min
Delta R.T.: -0.027 min
Response: 1690440
Conc: 8.37 ng/ml

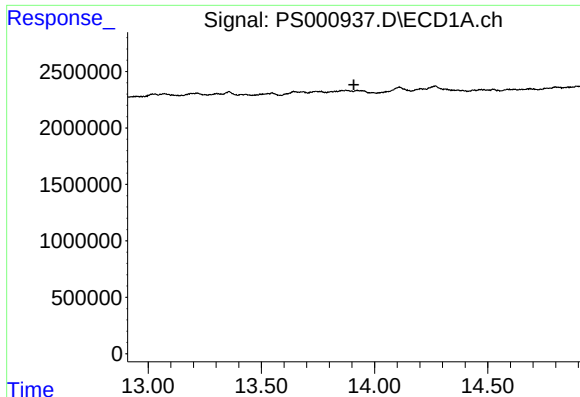

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.908 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

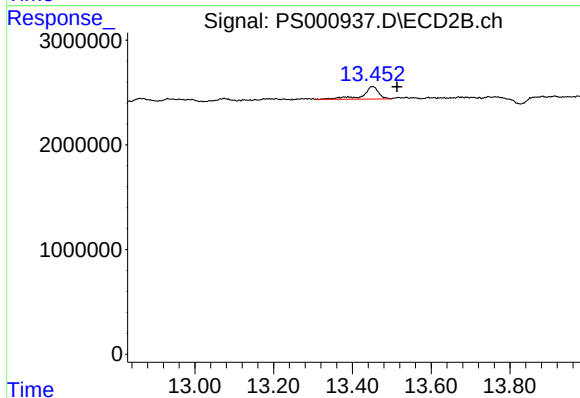


#10 Pentachlorophenol

R.T.: 13.452 min
Delta R.T.: -0.061 min
Response: 3297240
Conc: 1.05 ng/ml

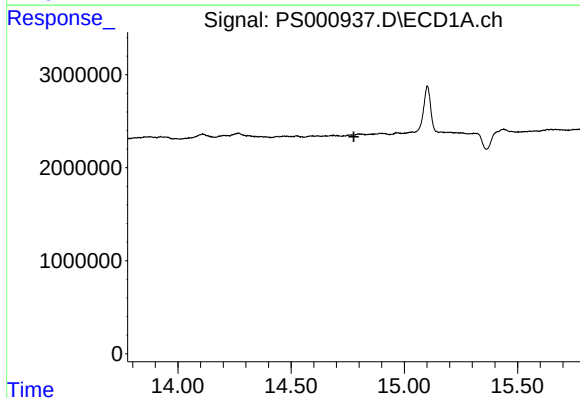


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.777 min
Response: 0
Conc: N.D.

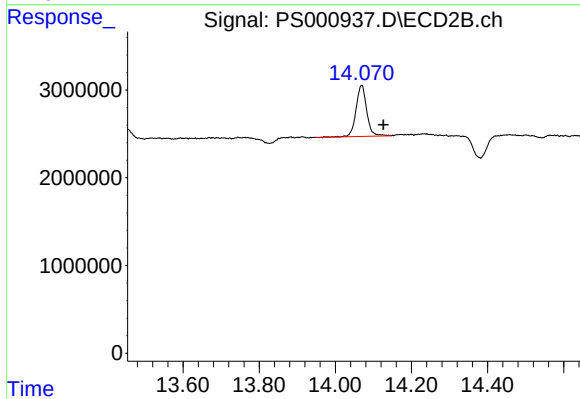

#11 2,4,5-TP (SILVEX)


R.T.: 14.069 min
Delta R.T.: -0.057 min
Response: 11309513
Conc: 9.01 ng/ml

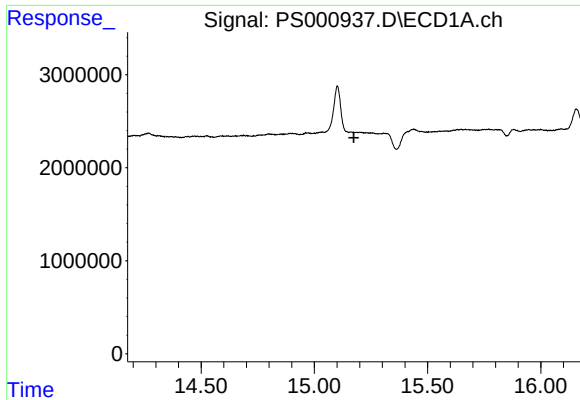

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 15.174 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

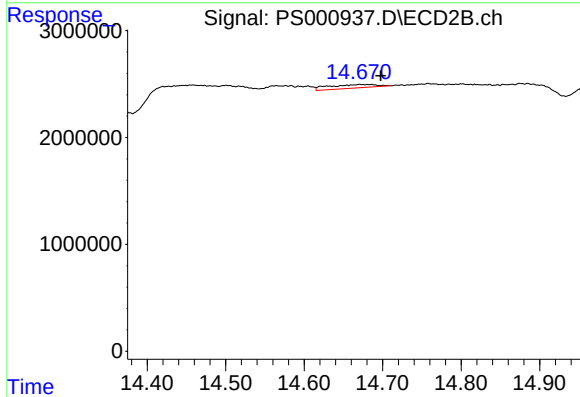


#12 2,4,5-T

R.T.: 14.670 min
Delta R.T.: -0.027 min
Response: 1415738
Conc: 1.37 ng/ml

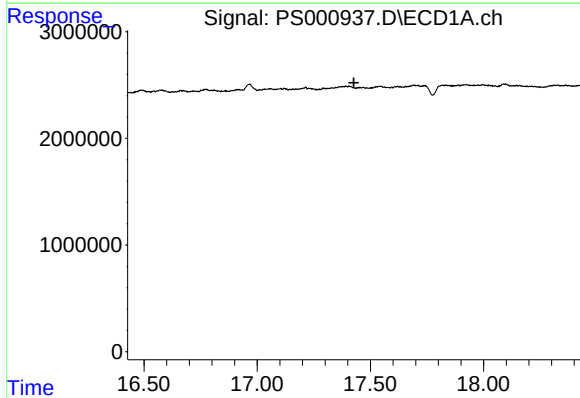


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.427 min
Response: 0
Conc: N.D.

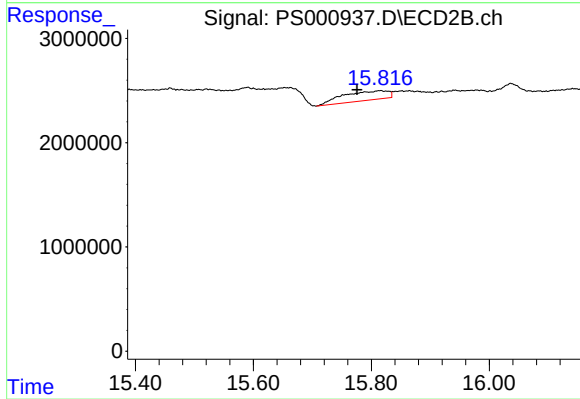

#14 DINOSEB


R.T.: 15.816 min
Delta R.T.: 0.040 min
Response: 4746722
Conc: 5.67 ng/ml

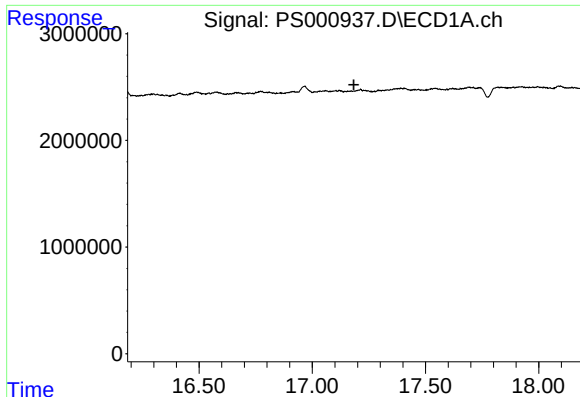

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

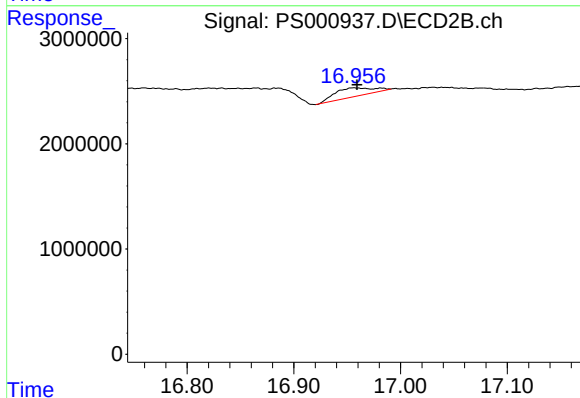


#15 Picloram

R.T.: 16.956 min
Delta R.T.: -0.003 min
Response: 2067216
Conc: 1.36 ng/ml

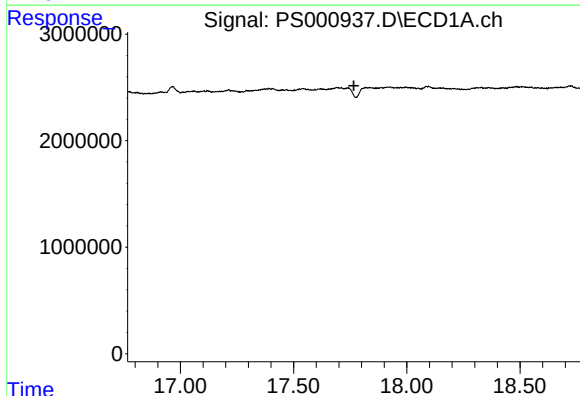

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.766 min
Response: 0
Conc: N.D.

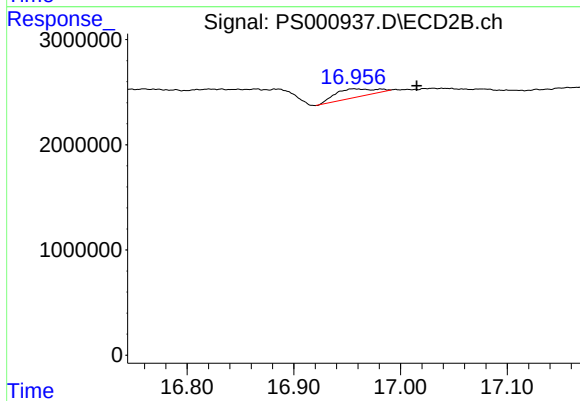

#16 DCPA

R.T.: 16.956 min
Delta R.T.: -0.059 min
Response: 2067216
Conc: 1.20 ng/ml