

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
 Data File : PS000938.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2018 13:22
 Operator : UA
 Sample : J3914-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 15:14:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.654	11.067	56595983	47390478	274.312	217.590
Target Compounds							
1) T	Dalapon	2.990	2.422	6117882	1921812	22.785	7.133 #
2) T	3,5-DICHL...	0.000	9.153	0	5892669	N.D.	20.033 #
5) T	DICAMBA	0.000	11.313	0	5480305	N.D.	6.982 #
6) T	MCP	12.349	0.000	7516653	0	13.684	N.D. #
8) T	DICHLORPROP	0.000	12.438	0	1682877	N.D.	8.332 #
9) T	2,4-D	13.480	0.000	18610900	0	68.375	N.D. #
15) T	Picloram	0.000	16.943	0	1777038	N.D.	1.167 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
Data File : PS000938.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2018 13:22
Operator : UA
Sample : J3914-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 15:14:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

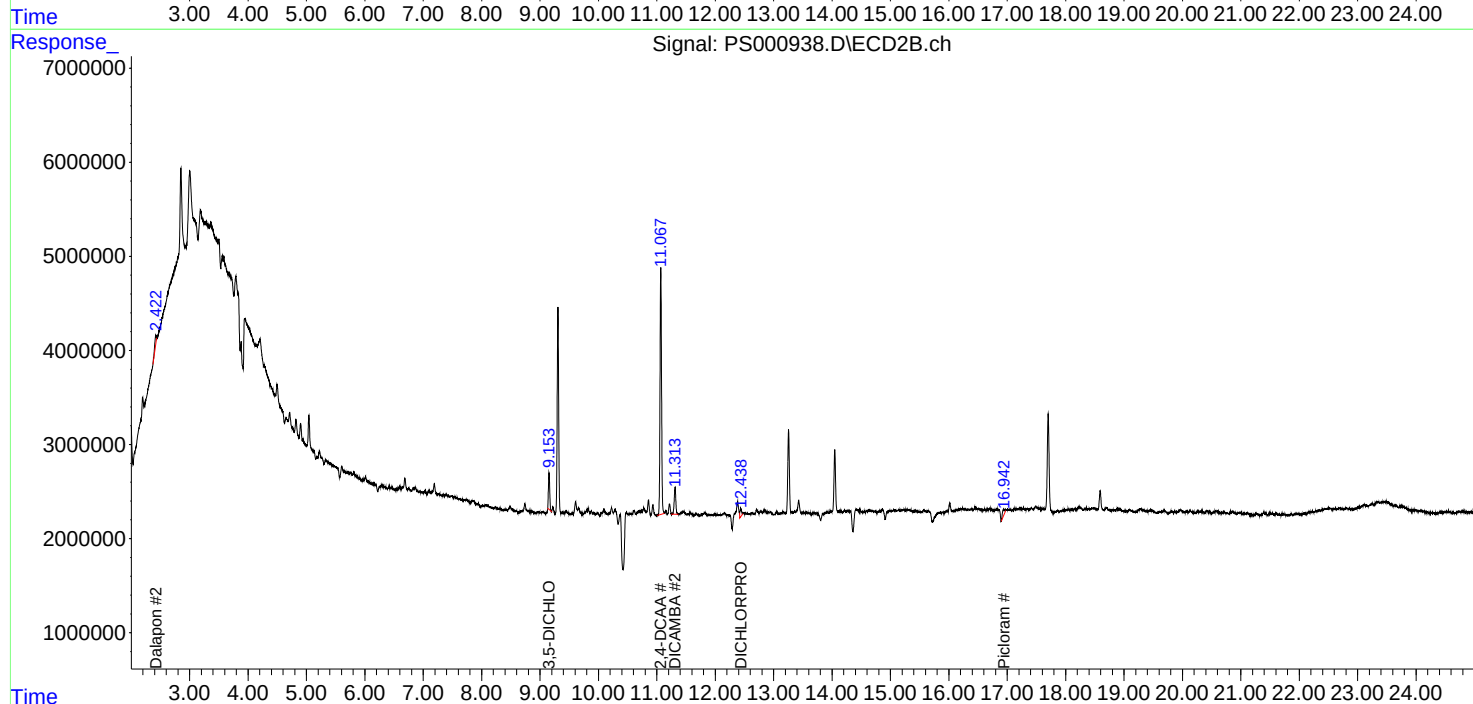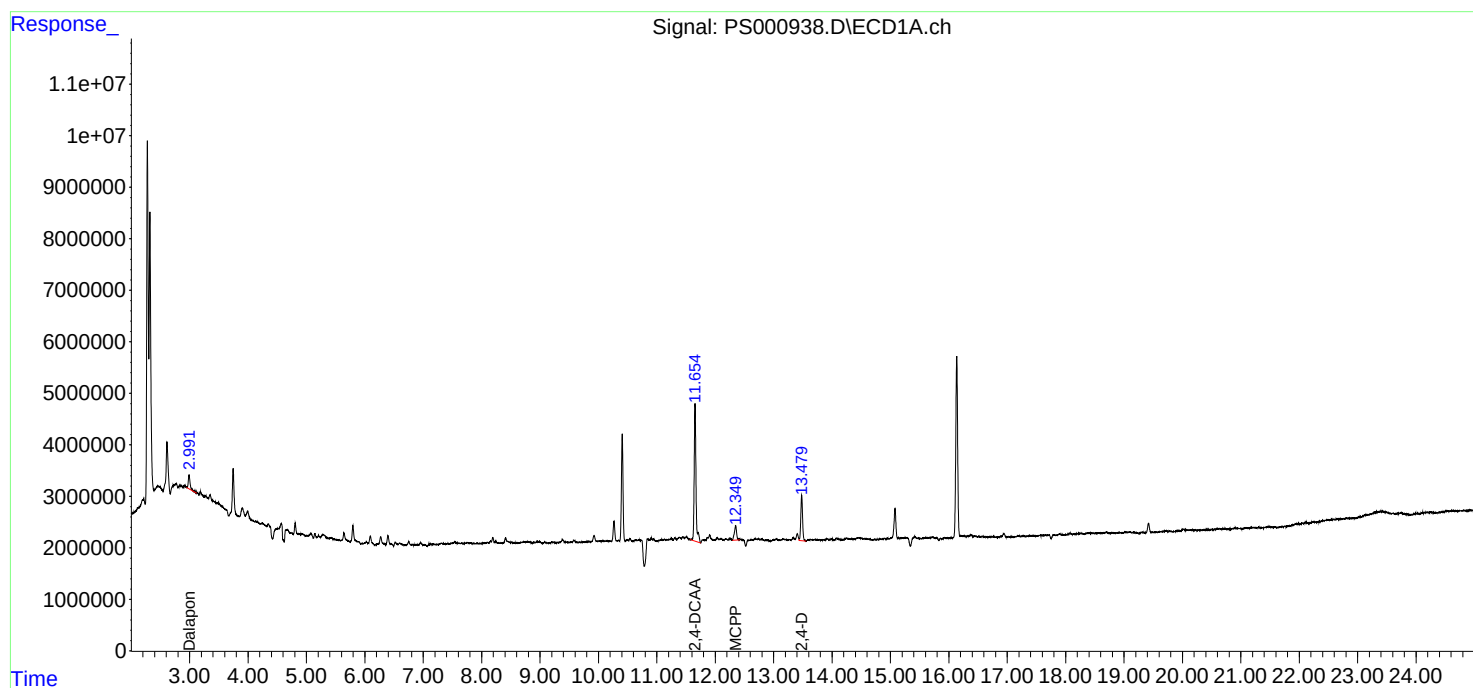


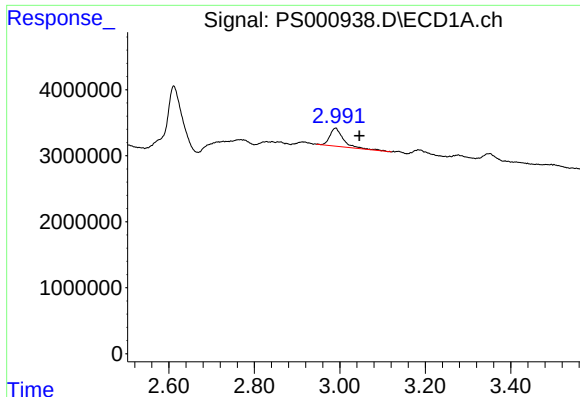

#1 Dalapon


R.T.: 2.990 min
Delta R.T.: -0.056 min
Response: 6117882
Conc: 22.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

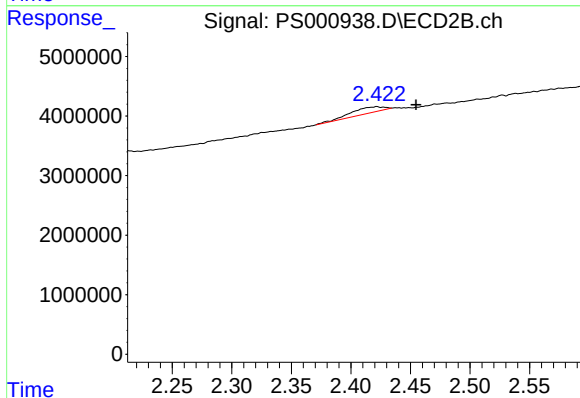


#1 Dalapon

R.T.: 2.422 min
Delta R.T.: -0.033 min
Response: 1921812
Conc: 7.13 ng/ml

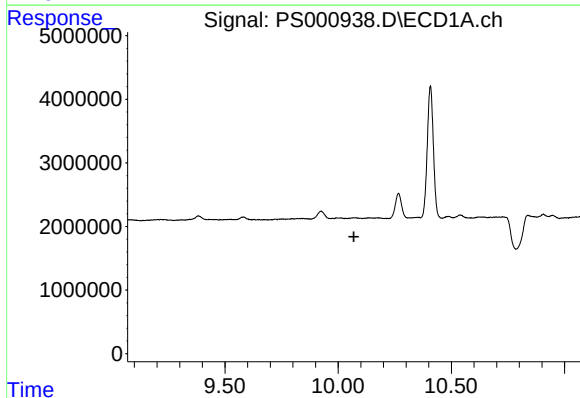


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

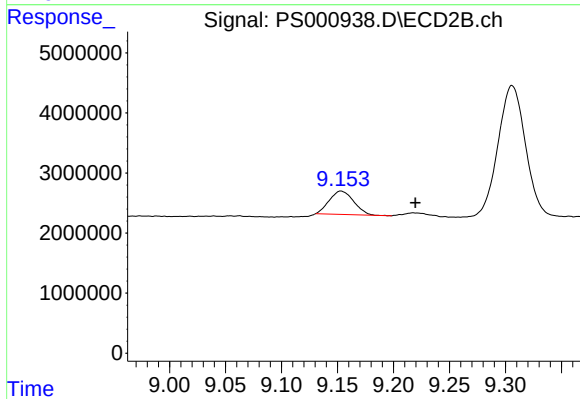

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.153 min
Delta R.T.: -0.066 min
Response: 5892669
Conc: 20.03 ng/ml

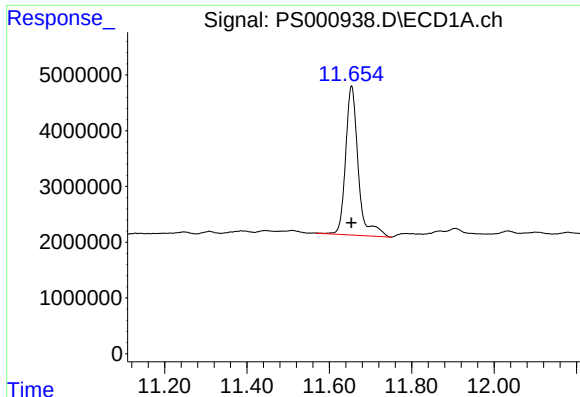

#4 2,4-DCAA


R.T.: 11.654 min
Delta R.T.: 0.000 min
Response: 56595983
Conc: 274.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

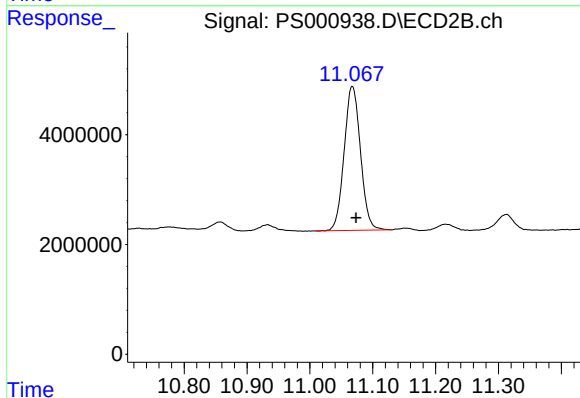


#4 2,4-DCAA

R.T.: 11.067 min
Delta R.T.: -0.006 min
Response: 47390478
Conc: 217.59 ng/ml

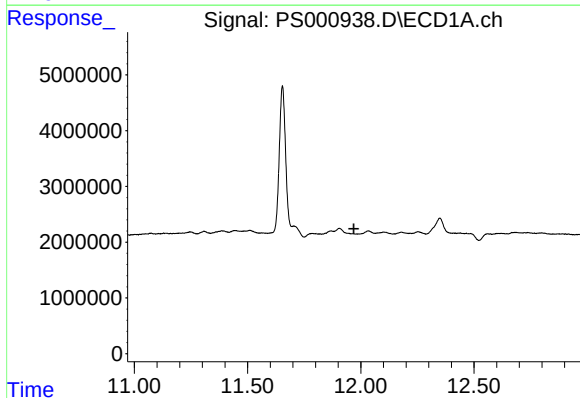


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.970 min
Response: 0
Conc: N.D.

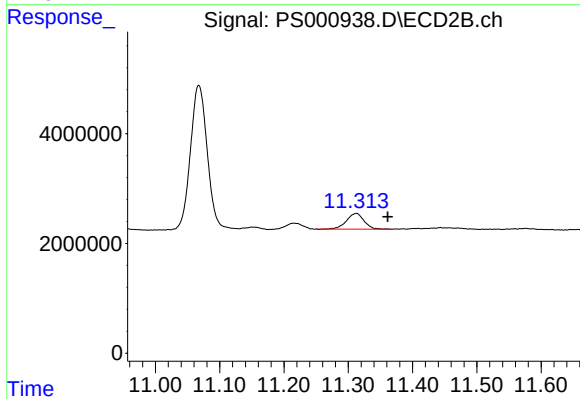

#5 DICAMBA


R.T.: 11.313 min
Delta R.T.: -0.048 min
Response: 5480305
Conc: 6.98 ng/ml

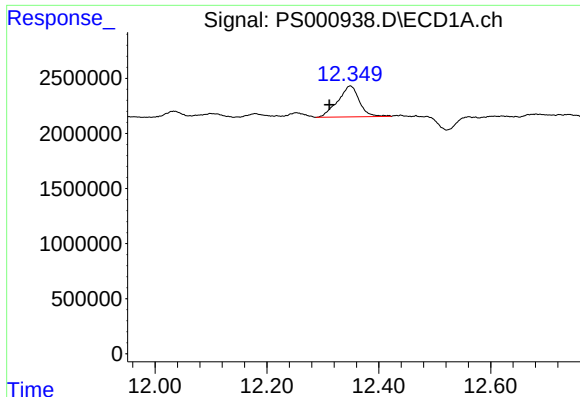

#6 MCP


R.T.: 12.349 min
Delta R.T.: 0.037 min
Response: 7516653
Conc: 13.68 ug/ml

Instrument :
ECD_S
ClientSampleId :

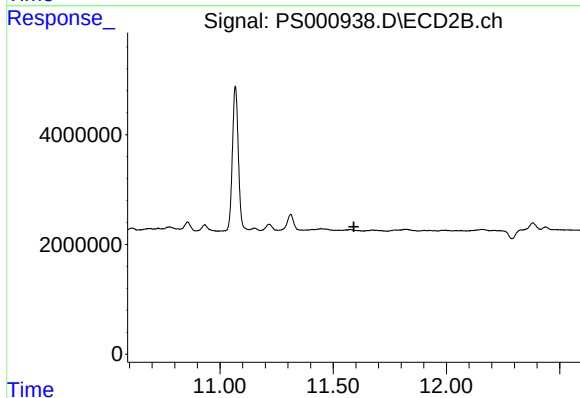


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

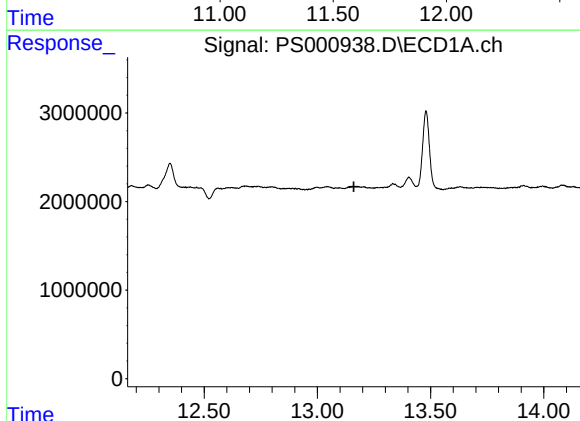


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

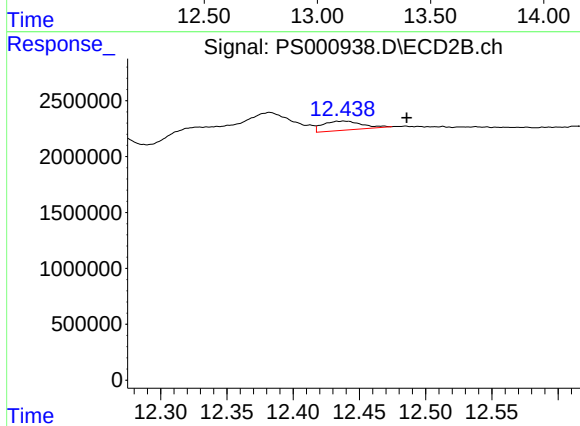

#8 DICHLORPROP


R.T.: 12.438 min
Delta R.T.: -0.047 min
Response: 1682877
Conc: 8.33 ng/ml

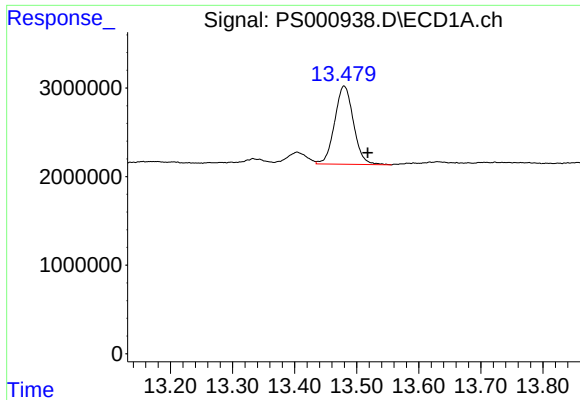

#9 2,4-D


R.T.: 13.480 min
Delta R.T.: -0.038 min
Response: 18610900
Conc: 68.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

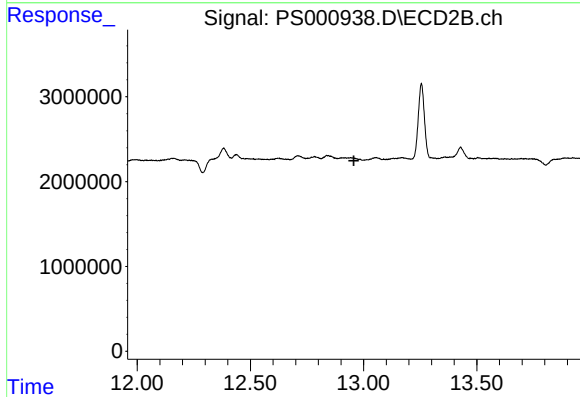


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 12.957 min
Response: 0
Conc: N.D.

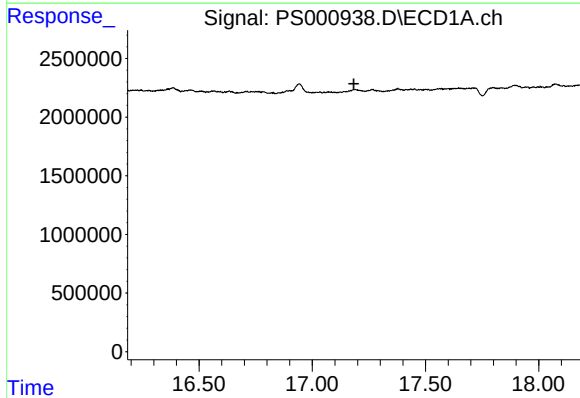

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.184 min
Response: 0
Conc: N.D.

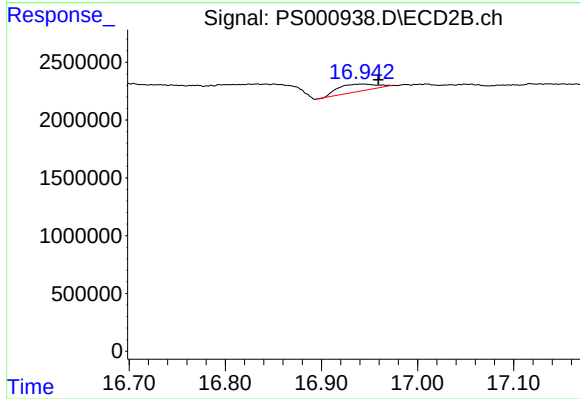

#15 Picloram

R.T.: 16.943 min
Delta R.T.: -0.016 min
Response: 1777038
Conc: 1.17 ng/ml