

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
 Data File : PS000941.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2018 14:54
 Operator : UA
 Sample : J3914-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 00:56:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.676	11.090	47909052	48179473	232.207	221.213
Target Compounds							
1) T	Dalapon	3.011	2.450	5030721	3073441	18.736	11.407 #
2) T	3,5-DICHL...	0.000	9.176	0	10379231	N.D.	35.285 #
5) T	DICAMBA	0.000	11.333	0	5857066	N.D.	7.462 #
6) T	MCP	12.372	0.000	6119599	0	11.141	N.D. #
7) T	MCPA	12.628	0.000	340778	0	0.373	N.D. #
8) T	DICHLORPROP	0.000	12.459	0	1821398	N.D.	9.018 #
10) T	Pentachlo...	0.000	13.453	0	3518630	N.D.	1.121 #
11) T	2,4,5-TP ...	0.000	14.069	0	16538625	N.D.	13.179 #
14) T	DINOSEB	0.000	15.828	0	4641059	N.D.	5.542 #
15) T	Picloram	0.000	16.961	0	2055437	N.D.	1.350 #
16) T	DCPA	0.000	16.970	0	1228908	N.D.	0.715 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
Data File : PS000941.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2018 14:54
Operator : UA
Sample : J3914-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 00:56:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

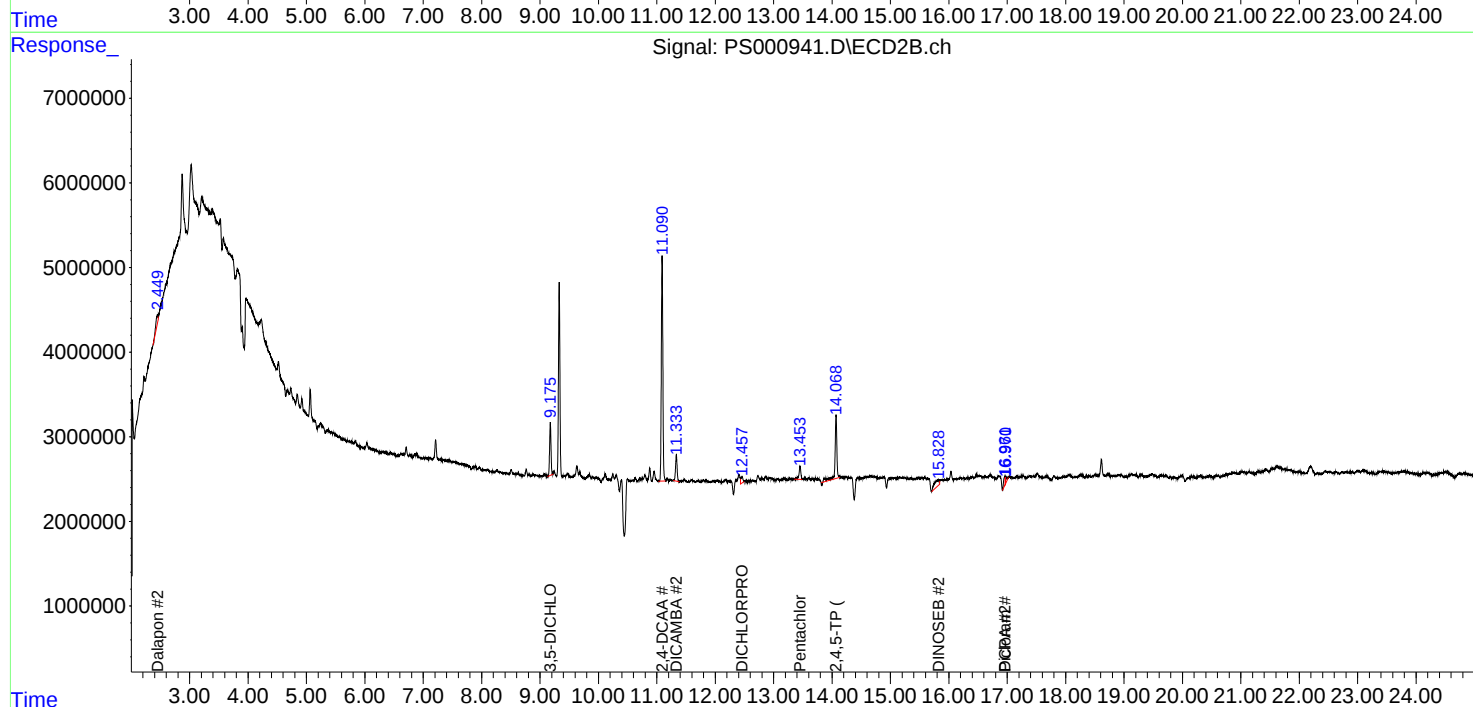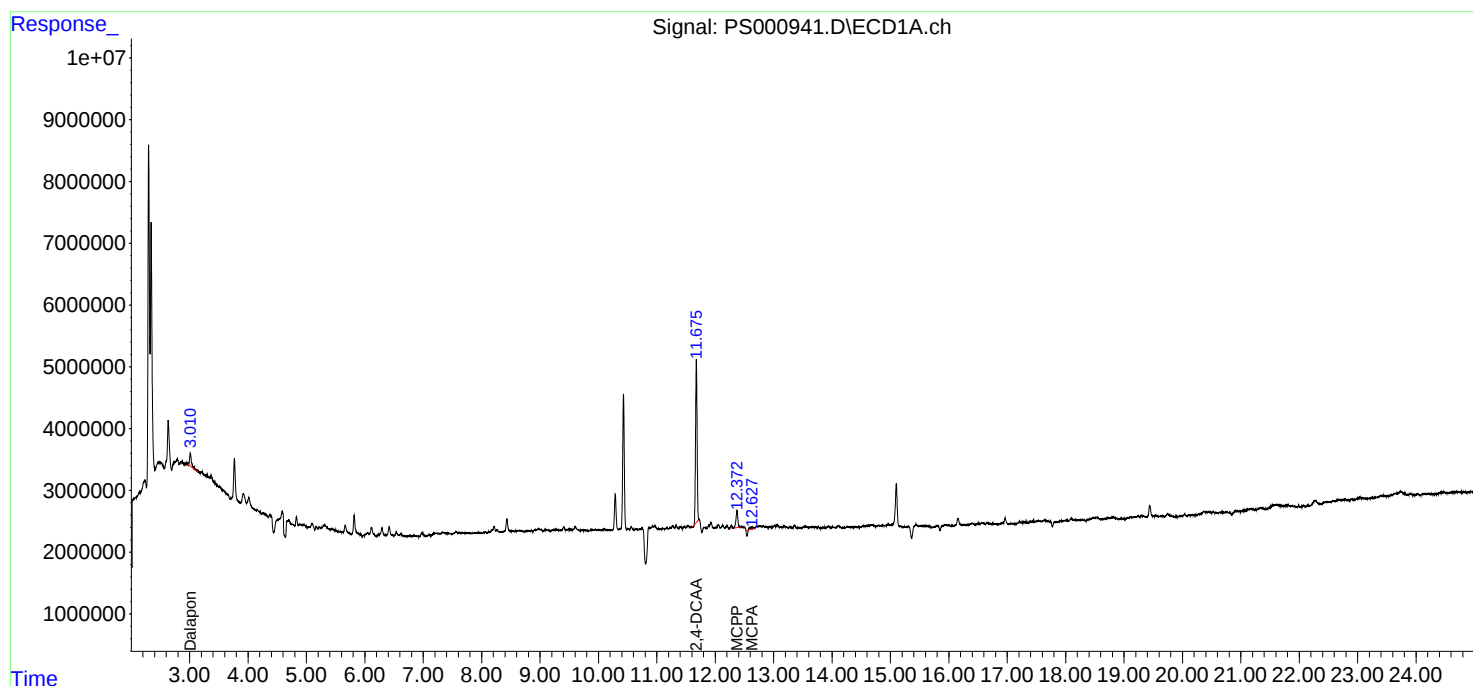


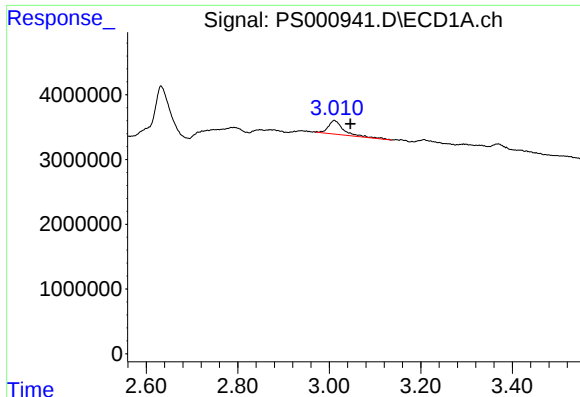

#1 Dalapon


R.T.: 3.011 min
Delta R.T.: -0.035 min
Response: 5030721
Conc: 18.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

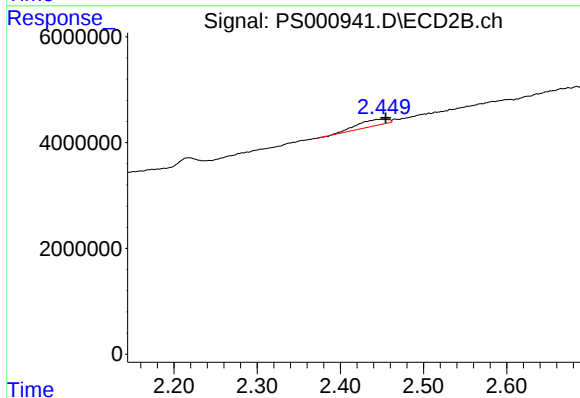


#1 Dalapon

R.T.: 2.450 min
Delta R.T.: -0.005 min
Response: 3073441
Conc: 11.41 ng/ml

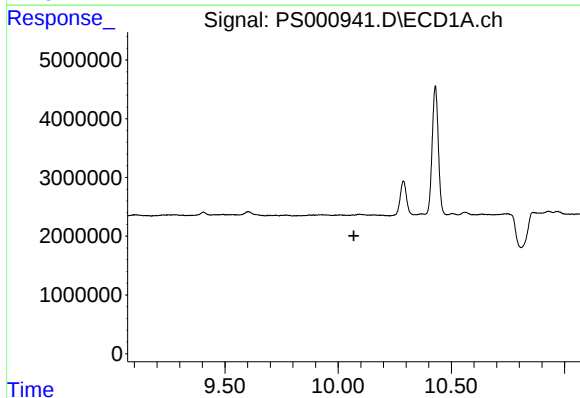


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

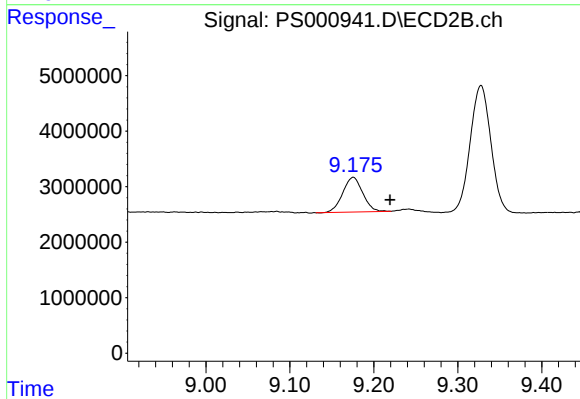

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.176 min
Delta R.T.: -0.044 min
Response: 10379231
Conc: 35.29 ng/ml

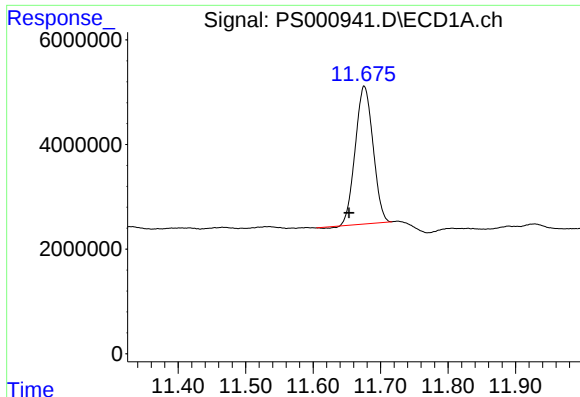

#4 2,4-DCAA


R.T.: 11.676 min
Delta R.T.: 0.022 min
Response: 47909052
Conc: 232.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

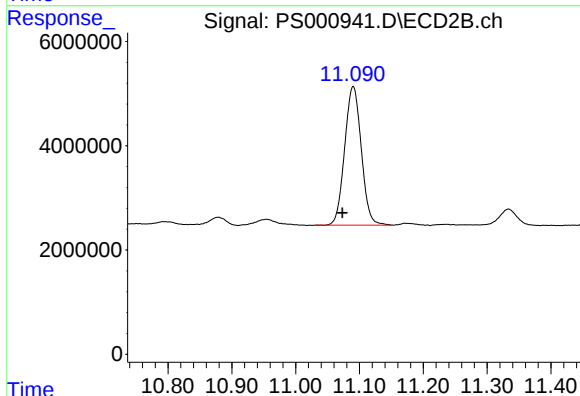


#4 2,4-DCAA

R.T.: 11.090 min
Delta R.T.: 0.017 min
Response: 48179473
Conc: 221.21 ng/ml

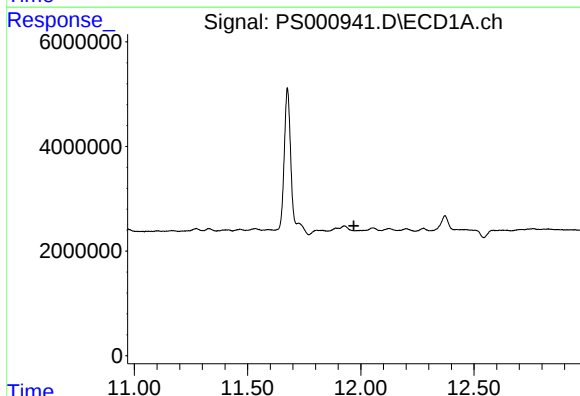


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.970 min
Response: 0
Conc: N.D.

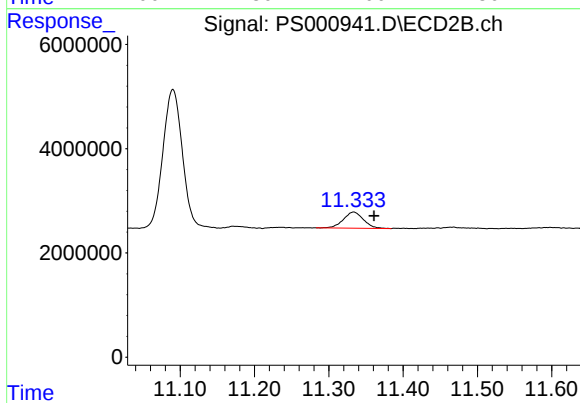

#5 DICAMBA


R.T.: 11.333 min
Delta R.T.: -0.028 min
Response: 5857066
Conc: 7.46 ng/ml

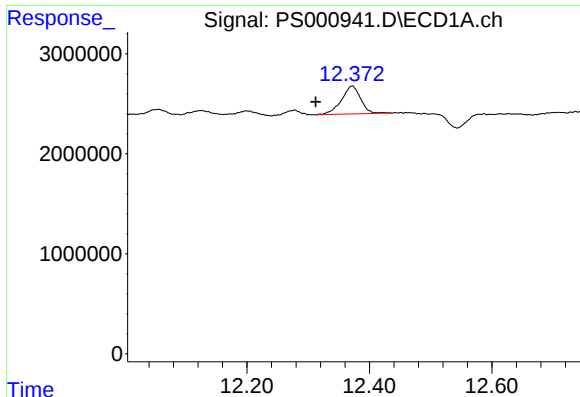

#6 MCPP


R.T.: 12.372 min
Delta R.T.: 0.060 min
Response: 6119599
Conc: 11.14 ug/ml

Instrument :
ECD_S
ClientSampleId :

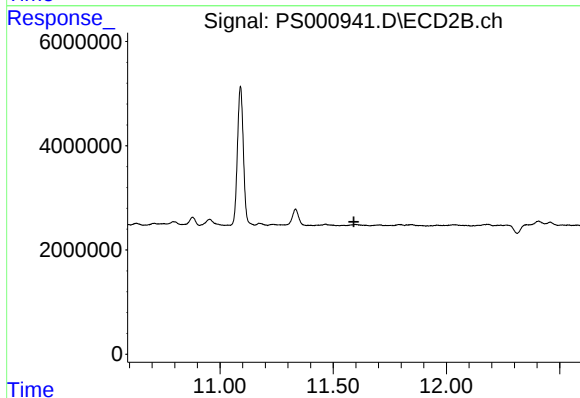


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

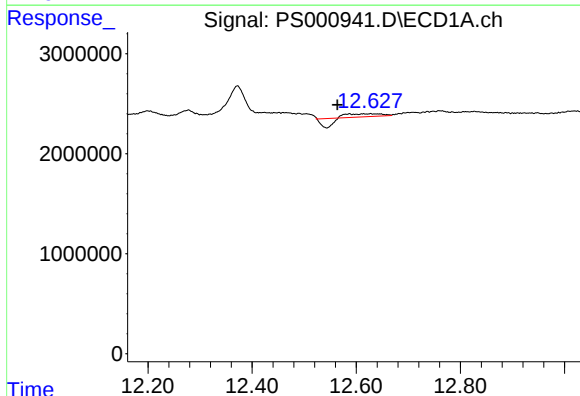


#7 MCPA

R.T.: 12.628 min
Delta R.T.: 0.064 min
Response: 340778
Conc: 0.37 ug/ml

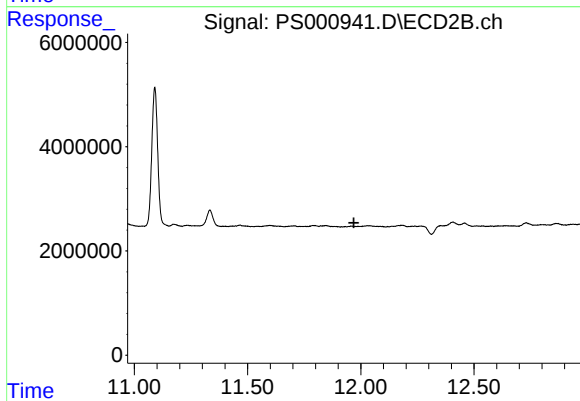

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 11.969 min
Response: 0
Conc: N.D.

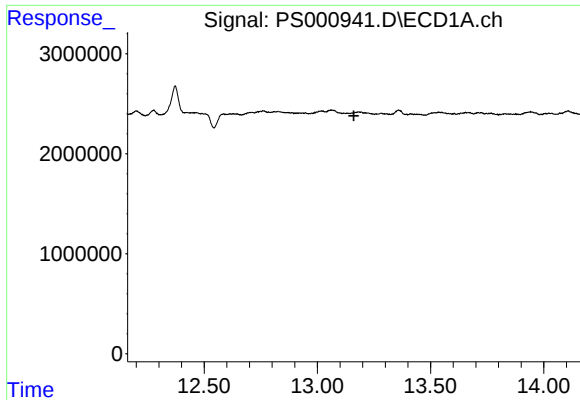

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.161 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

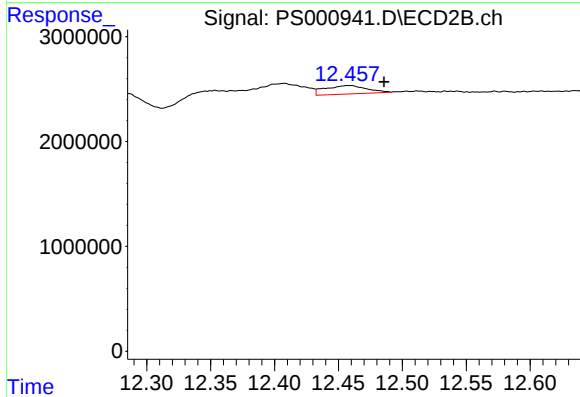


#8 DICHLORPROP

R.T.: 12.459 min
Delta R.T.: -0.027 min
Response: 1821398
Conc: 9.02 ng/ml

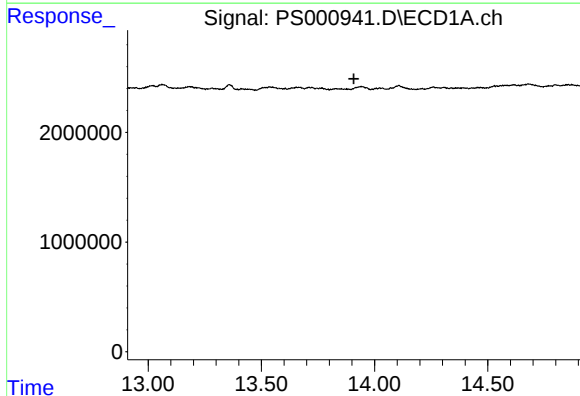


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.908 min
Response: 0
Conc: N.D.

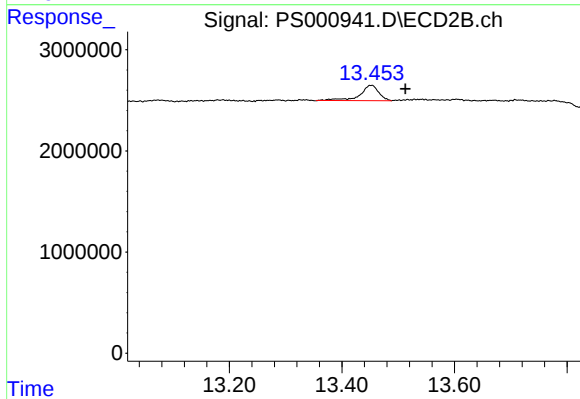

#10 Pentachlorophenol


R.T.: 13.453 min
Delta R.T.: -0.060 min
Response: 3518630
Conc: 1.12 ng/ml

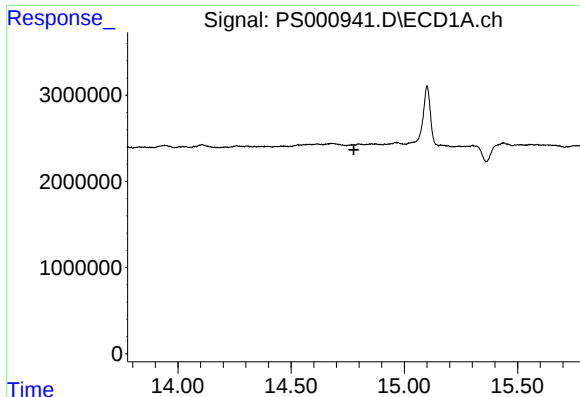

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 14.777 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

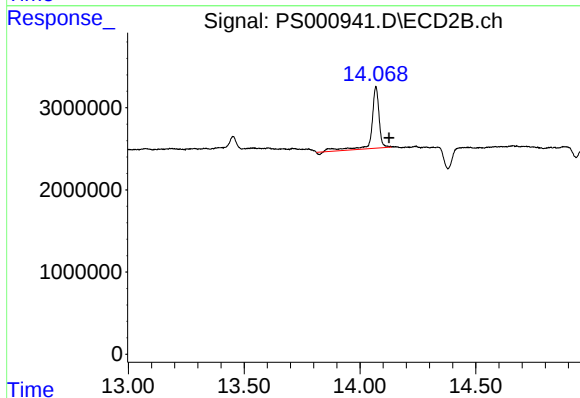


#11 2,4,5-TP (SILVEX)

R.T.: 14.069 min
Delta R.T.: -0.058 min
Response: 16538625
Conc: 13.18 ng/ml

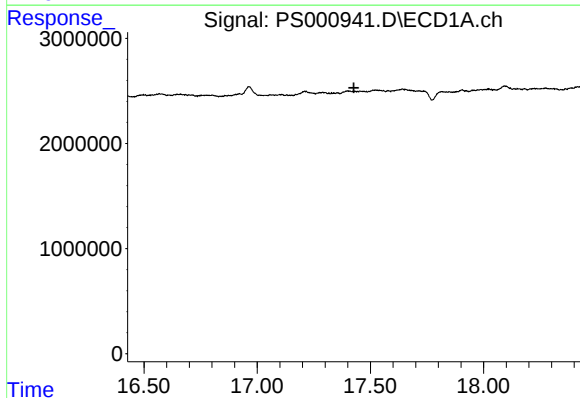


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.427 min
Response: 0
Conc: N.D.

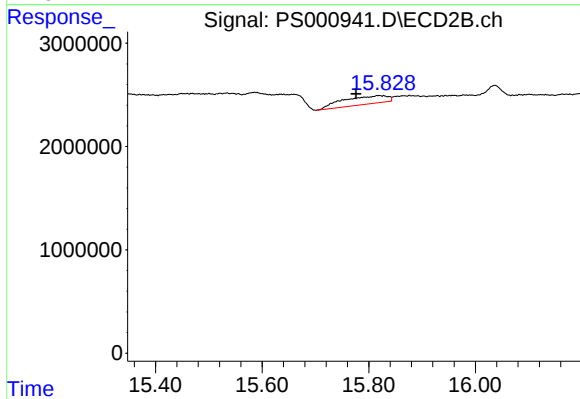

#14 DINOSEB


R.T.: 15.828 min
Delta R.T.: 0.052 min
Response: 4641059
Conc: 5.54 ng/ml

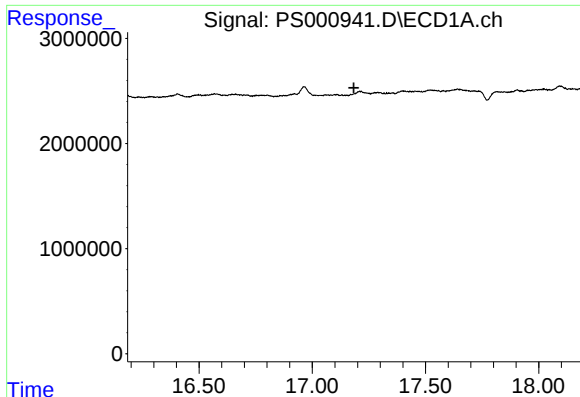

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

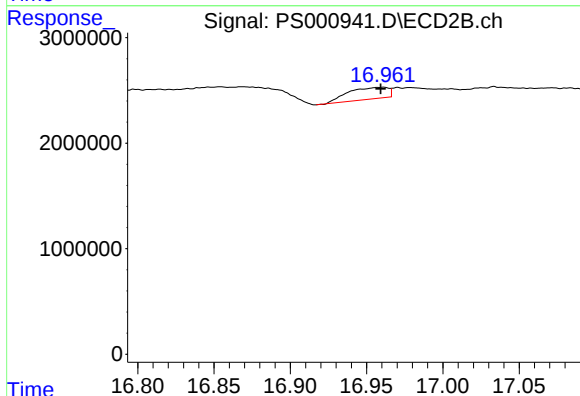


#15 Picloram

R.T.: 16.961 min
Delta R.T.: 0.002 min
Response: 2055437
Conc: 1.35 ng/ml

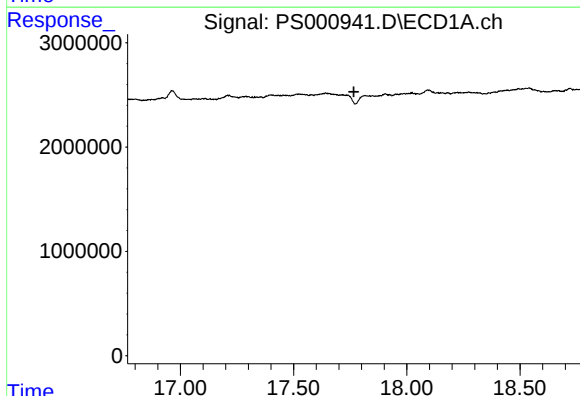

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.766 min
Response: 0
Conc: N.D.

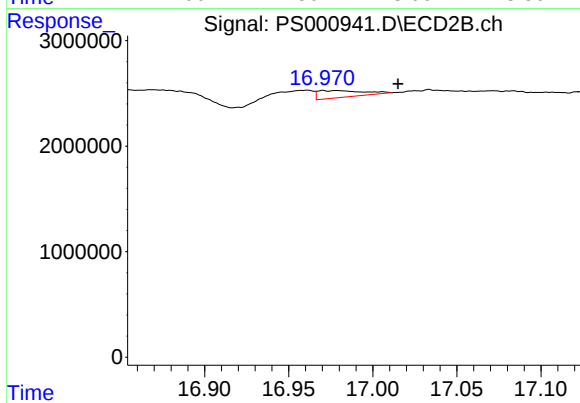

#16 DCPA

R.T.: 16.970 min
Delta R.T.: -0.045 min
Response: 1228908
Conc: 0.71 ng/ml