

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
 Data File : PS000942.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2018 15:25
 Operator : UA
 Sample : J3914-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 00:56:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.656	11.069	68176905	59620193	330.442	273.742
Target Compounds							
1) T	Dalapon	2.992	2.452	9338172	412611	34.778	1.531 #
2) T	3,5-DICHL...	0.000	9.155	0	12072800	N.D.	41.043 #
5) T	DICAMBA	0.000	11.313	0	6570704	N.D.	8.371 #
6) T	MCP	12.352	0.000	6925584	0	12.608	N.D. #
8) T	DICHLORPROP	0.000	12.438	0	1240980	N.D.	6.144 #
15) T	Picloram	0.000	16.955	0	2890096	N.D.	1.898 #
16) T	DCPA	0.000	16.980	0	457648	N.D.	0.266 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
Data File : PS000942.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2018 15:25
Operator : UA
Sample : J3914-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 00:56:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

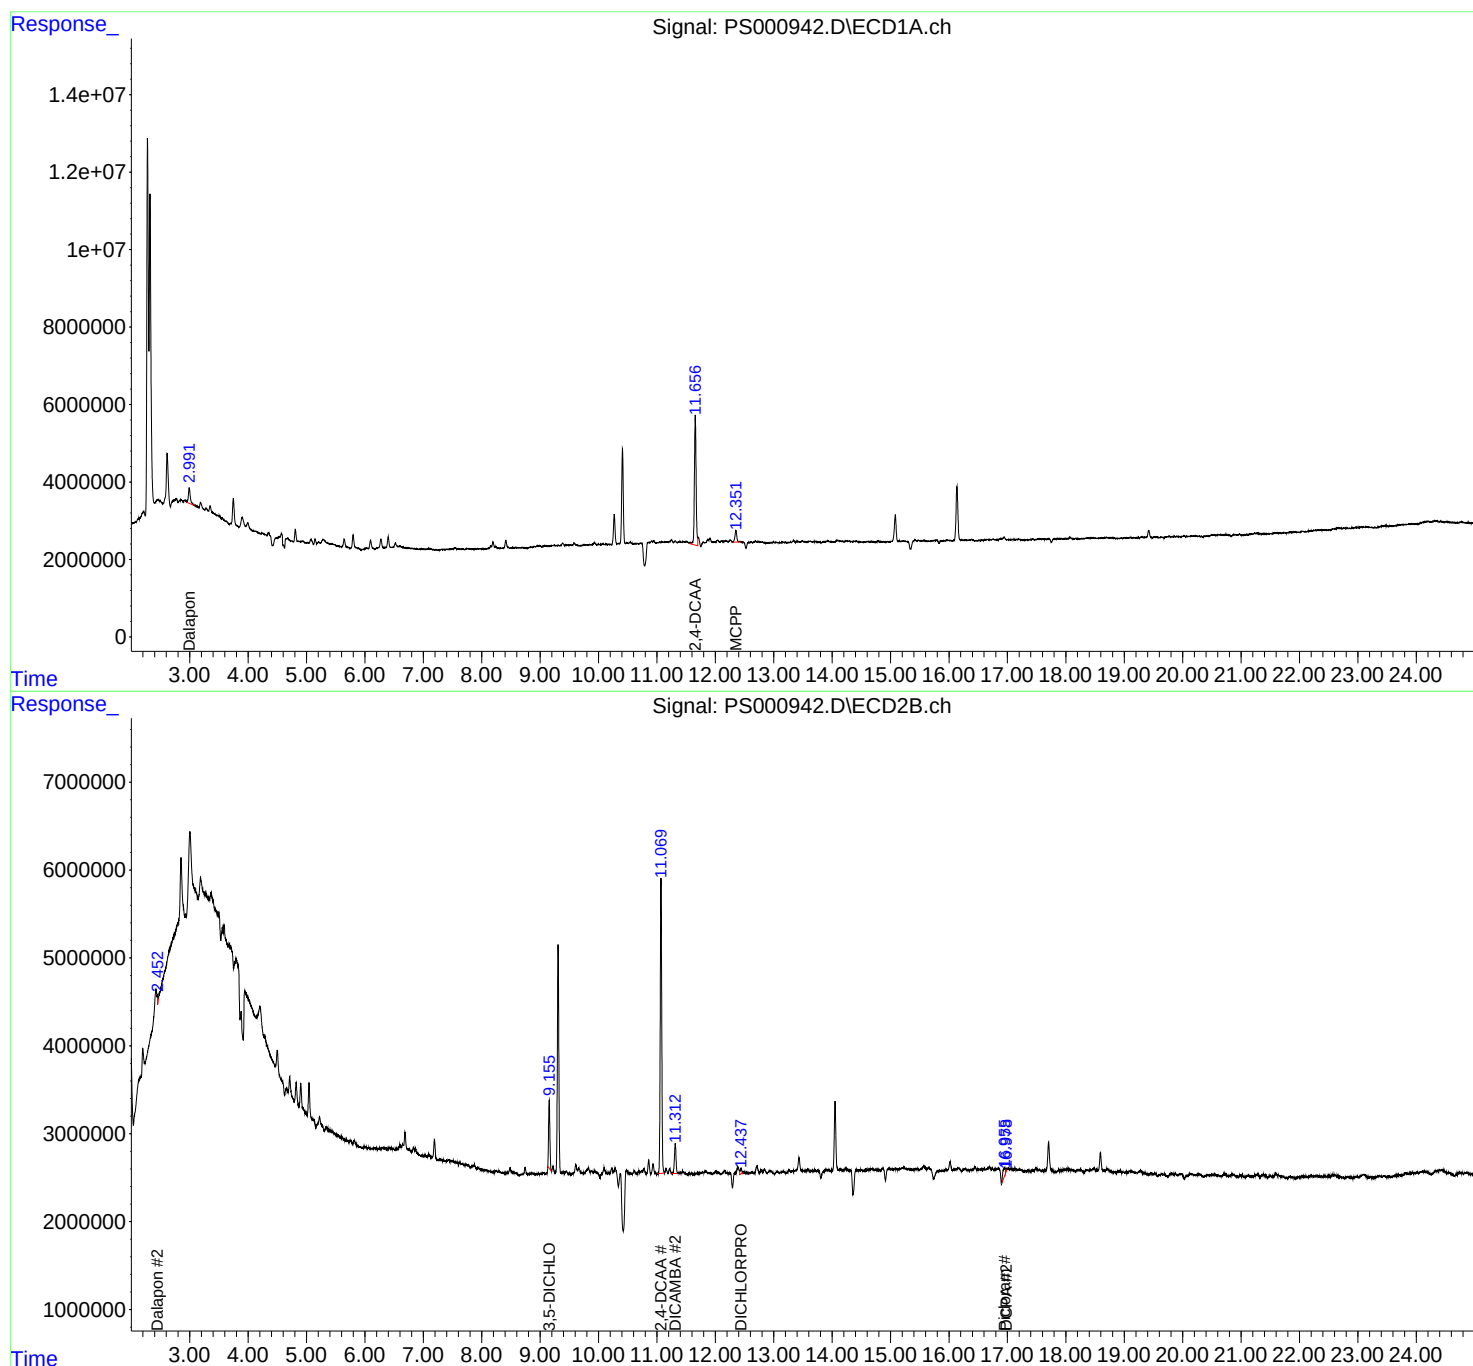


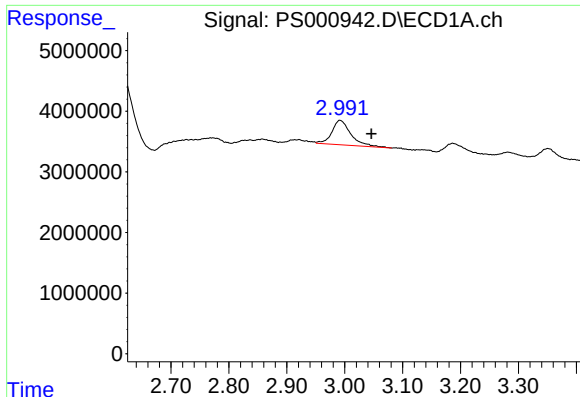

#1 Dalapon


R.T.: 2.992 min
Delta R.T.: -0.054 min
Response: 9338172
Conc: 34.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

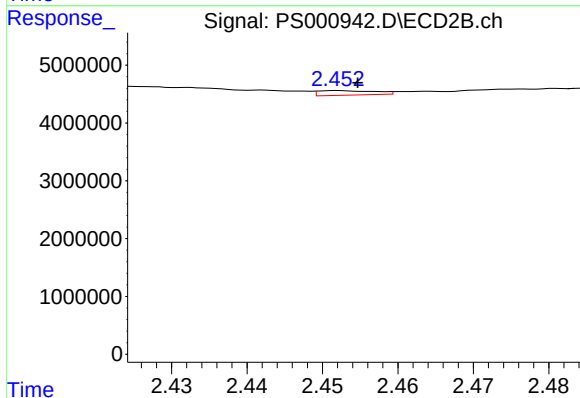


#1 Dalapon

R.T.: 2.452 min
Delta R.T.: -0.002 min
Response: 412611
Conc: 1.53 ng/ml

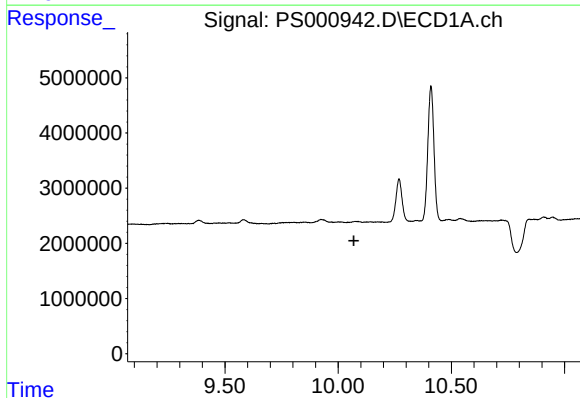


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

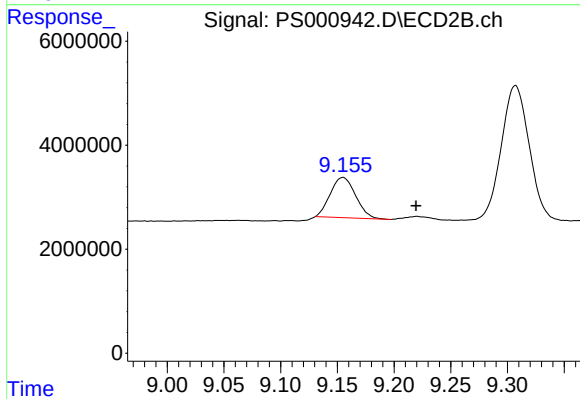

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.155 min
Delta R.T.: -0.064 min
Response: 12072800
Conc: 41.04 ng/ml

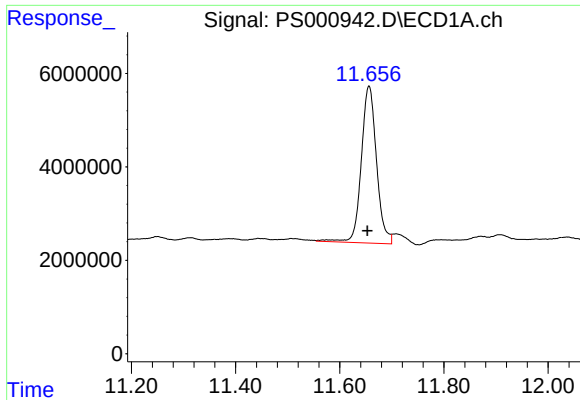

#4 2,4-DCAA


R.T.: 11.656 min
Delta R.T.: 0.003 min
Response: 68176905
Conc: 330.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

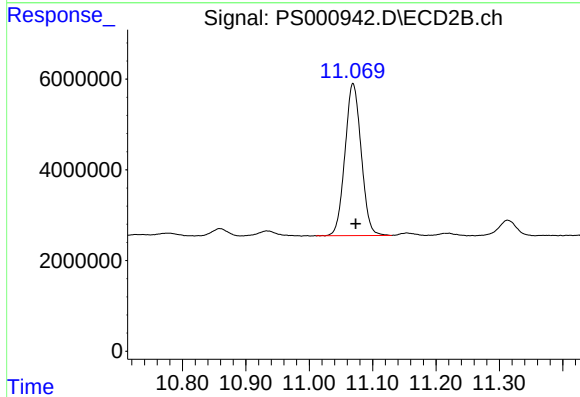


#4 2,4-DCAA

R.T.: 11.069 min
Delta R.T.: -0.004 min
Response: 59620193
Conc: 273.74 ng/ml

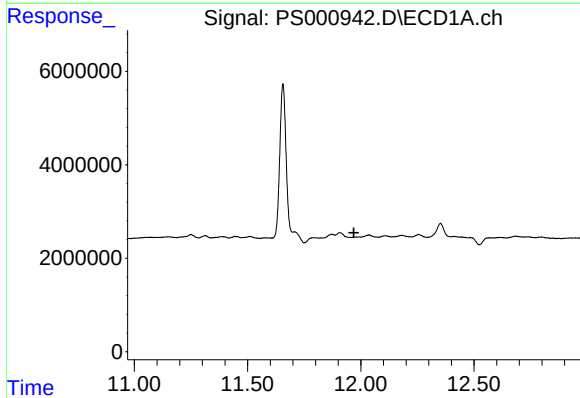


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.970 min
Response: 0
Conc: N.D.

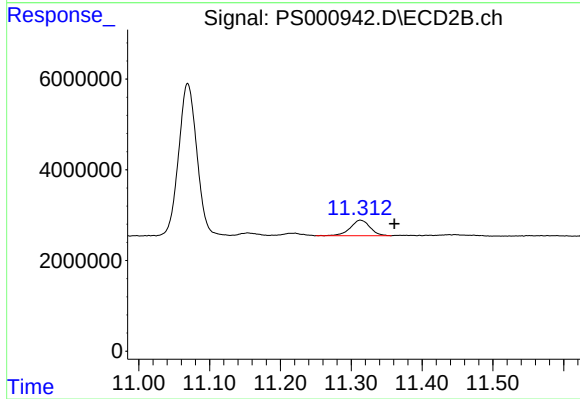

#5 DICAMBA


R.T.: 11.313 min
Delta R.T.: -0.048 min
Response: 6570704
Conc: 8.37 ng/ml

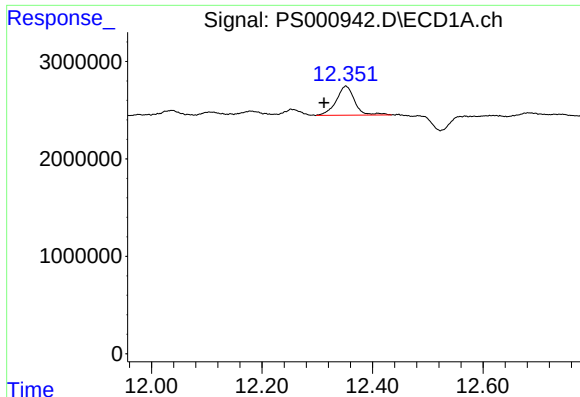

#6 MCP


R.T.: 12.352 min
Delta R.T.: 0.040 min
Response: 6925584
Conc: 12.61 ug/ml

Instrument :
ECD_S
ClientSampleId :

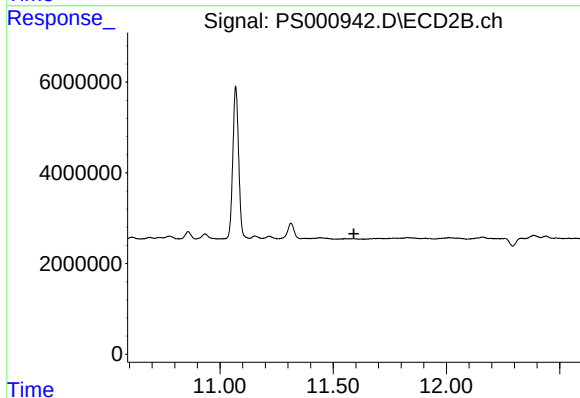


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

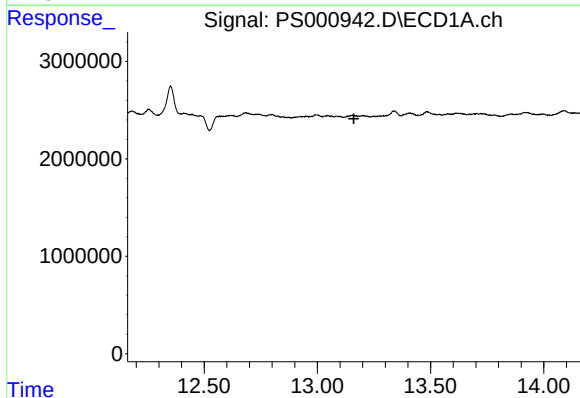


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

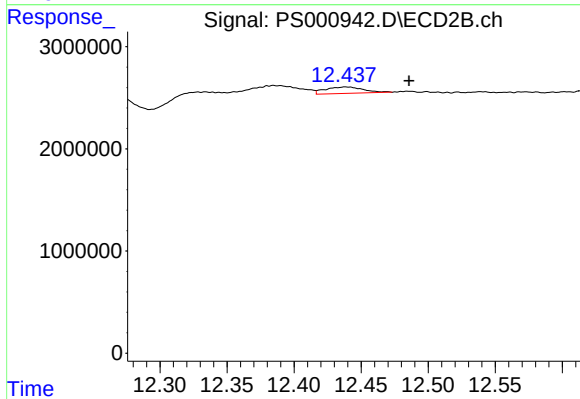

#8 DICHLORPROP


R.T.: 12.438 min
Delta R.T.: -0.047 min
Response: 1240980
Conc: 6.14 ng/ml

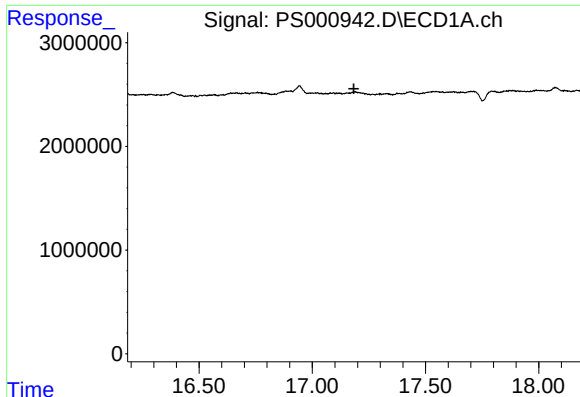

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

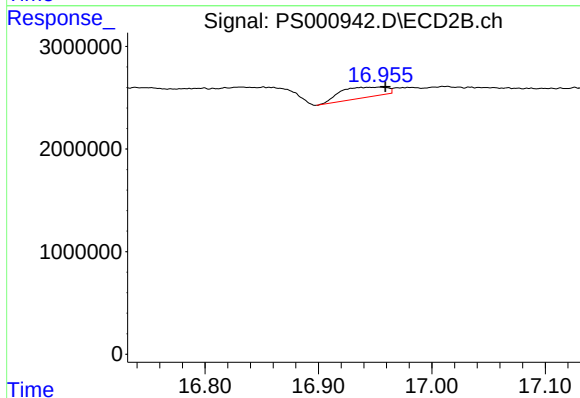


#15 Picloram

R.T.: 16.955 min
Delta R.T.: -0.005 min
Response: 2890096
Conc: 1.90 ng/ml

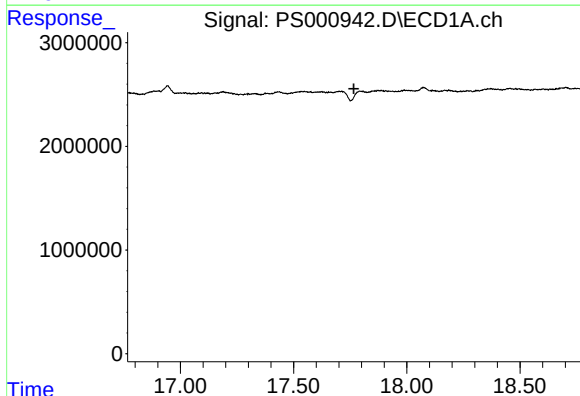

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.766 min
Response: 0
Conc: N.D.

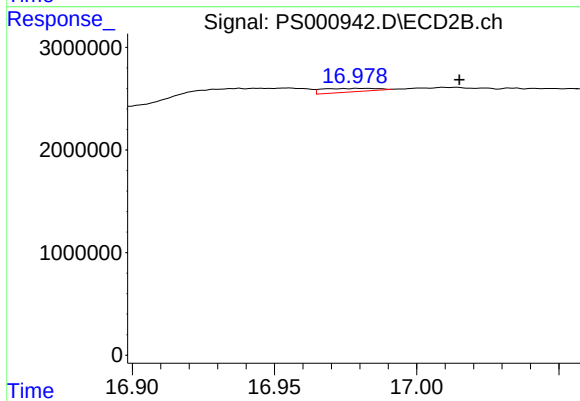

#16 DCPA

R.T.: 16.980 min
Delta R.T.: -0.035 min
Response: 457648
Conc: 0.27 ng/ml