

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
 Data File : PS000943.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2018 15:56
 Operator : UA
 Sample : J3914-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 00:57:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.671	11.086	73742847	60530987	357.420	277.924
Target Compounds							
1) T	Dalapon	3.008	2.440	13370868	12715778	49.797	47.196
2) T	3,5-DICHL...	0.000	9.171	0	14372841	N.D.	48.862 #
5) T	DICAMBA	11.924	11.330	4010116	6820294	5.093	8.689 #
6) T	MCP	12.367	0.000	6918900	0	12.596	N.D. #
8) T	DICHLORPROP	0.000	12.452	0	1530231	N.D.	7.576 #
10) T	Pentachlo...	0.000	13.446	0	3105341	N.D.	0.989 #
11) T	2,4,5-TP ...	0.000	14.064	0	14747009	N.D.	11.751 #
16) T	DCPA	0.000	17.032	0	6573336	N.D.	3.824 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
Data File : PS000943.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2018 15:56
Operator : UA
Sample : J3914-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 00:57:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

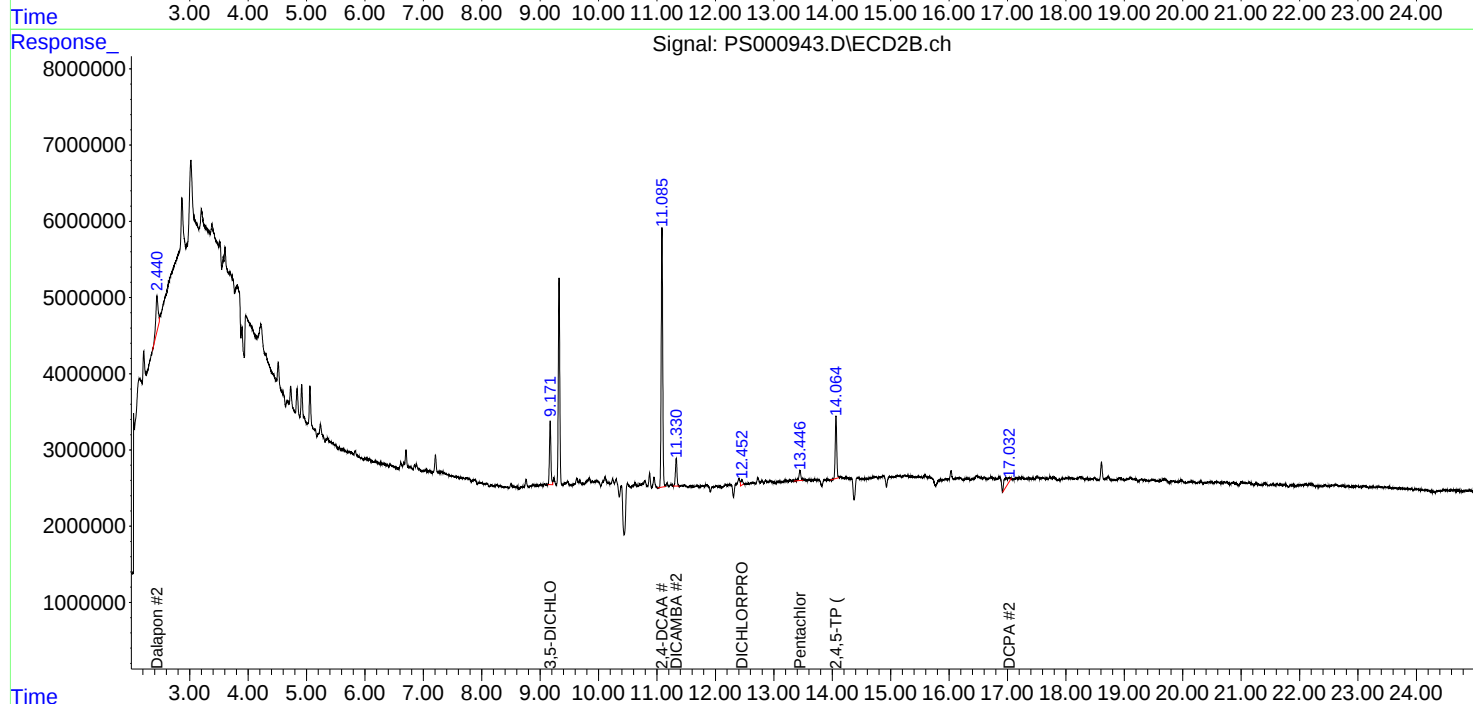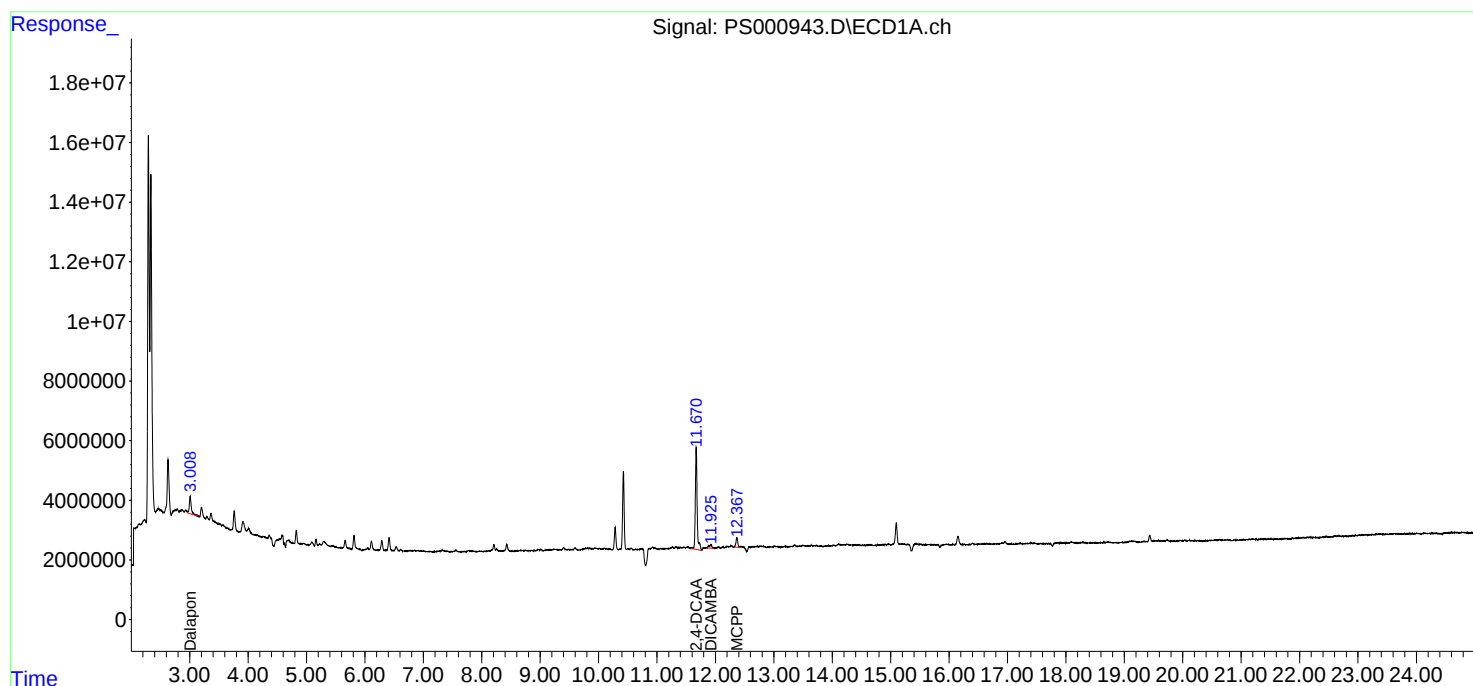


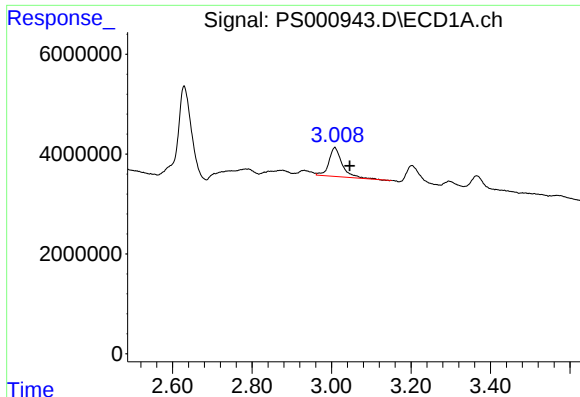

#1 Dalapon


R.T.: 3.008 min
Delta R.T.: -0.038 min
Response: 13370868
Conc: 49.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

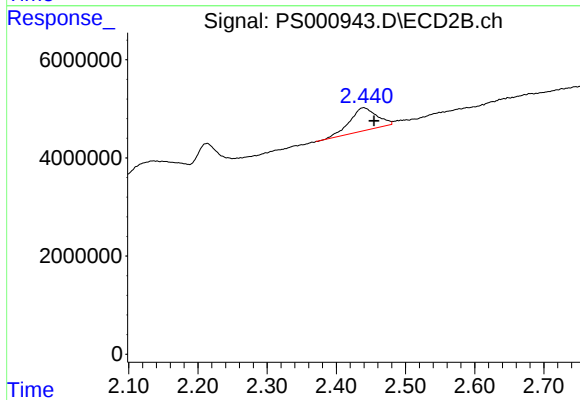


#1 Dalapon

R.T.: 2.440 min
Delta R.T.: -0.015 min
Response: 12715778
Conc: 47.20 ng/ml

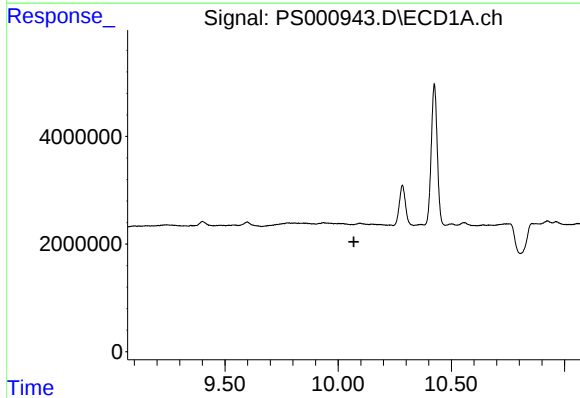


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

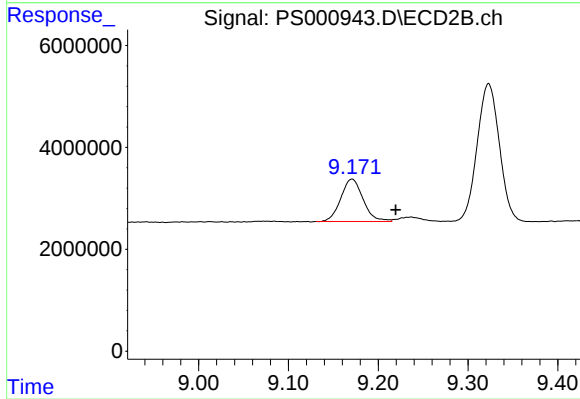

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.171 min
Delta R.T.: -0.048 min
Response: 14372841
Conc: 48.86 ng/ml

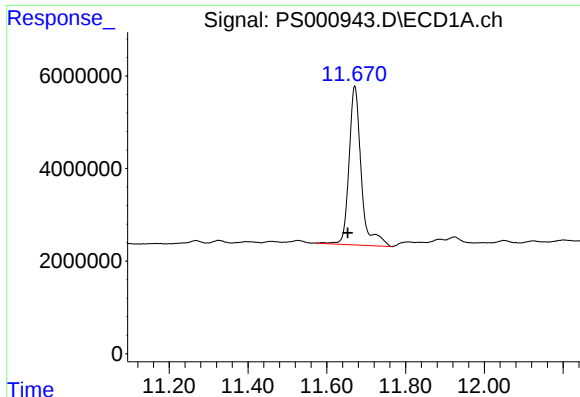

#4 2,4-DCAA


R.T.: 11.671 min
Delta R.T.: 0.018 min
Response: 73742847
Conc: 357.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

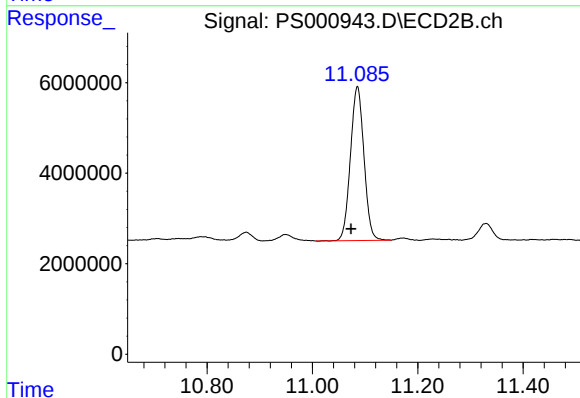


#4 2,4-DCAA

R.T.: 11.086 min
Delta R.T.: 0.012 min
Response: 60530987
Conc: 277.92 ng/ml

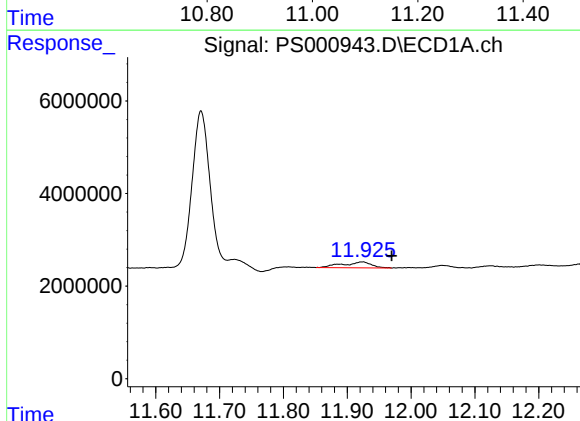


#5 DICAMBA

R.T.: 11.924 min
Delta R.T.: -0.046 min
Response: 4010116
Conc: 5.09 ng/ml

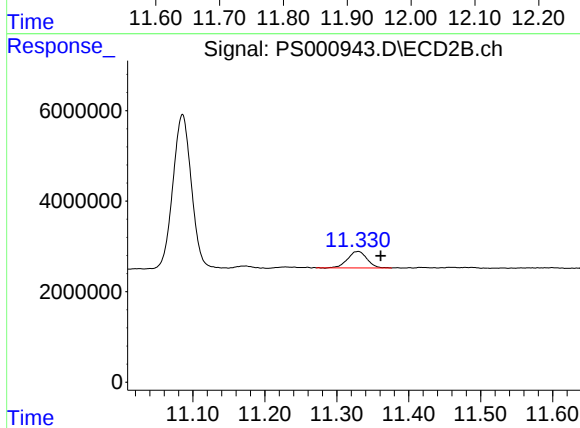

#5 DICAMBA


R.T.: 11.330 min
Delta R.T.: -0.031 min
Response: 6820294
Conc: 8.69 ng/ml

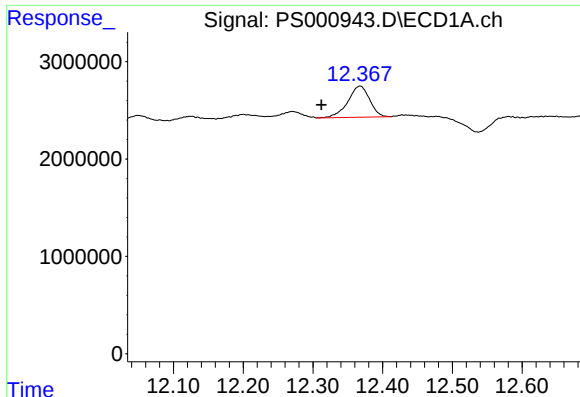

#6 MCP


R.T.: 12.367 min
Delta R.T.: 0.055 min
Response: 6918900
Conc: 12.60 ug/ml

Instrument :
ECD_S
ClientSampleId :

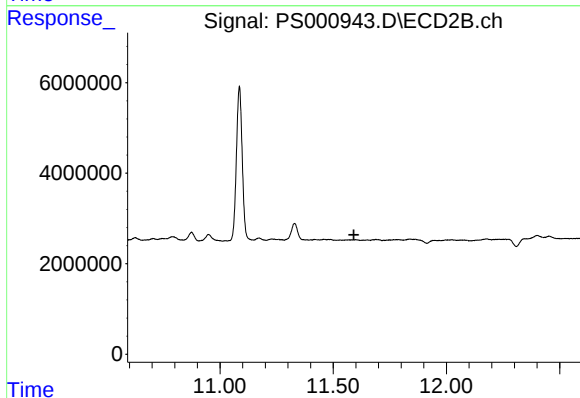


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

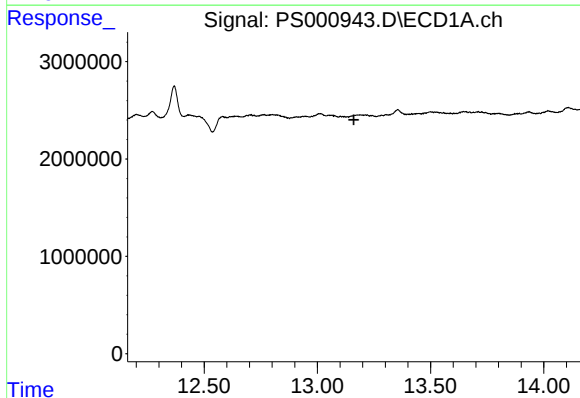


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

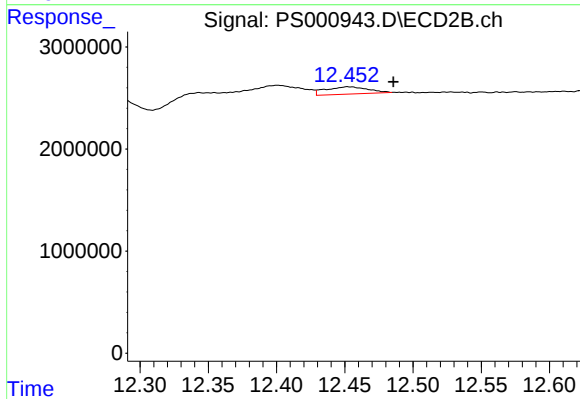

#8 DICHLORPROP


R.T.: 12.452 min
Delta R.T.: -0.033 min
Response: 1530231
Conc: 7.58 ng/ml

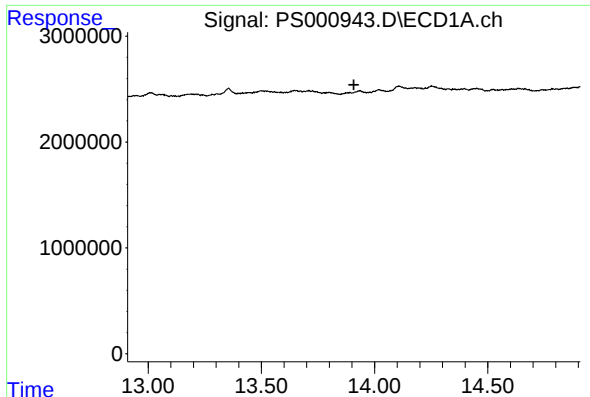

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.908 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

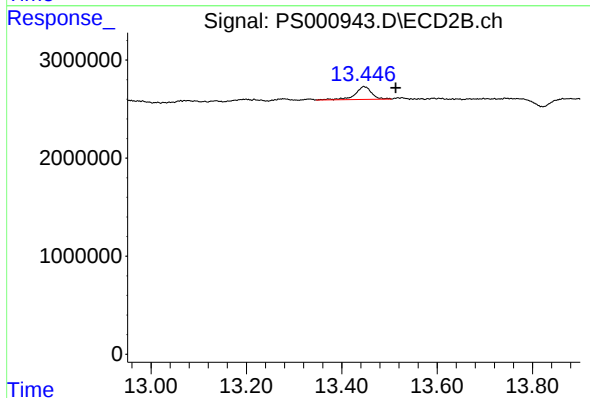


#10 Pentachlorophenol

R.T.: 13.446 min
Delta R.T.: -0.067 min
Response: 3105341
Conc: 0.99 ng/ml

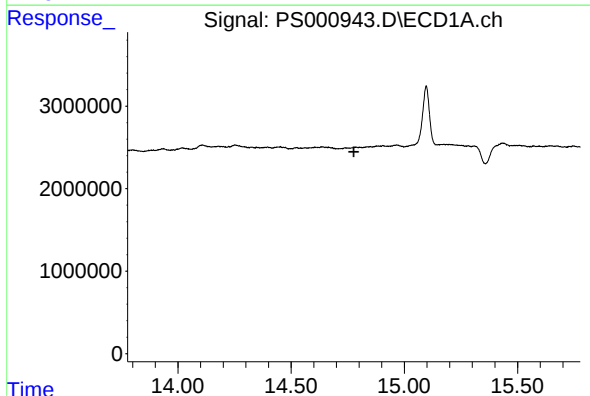


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.777 min
Response: 0
Conc: N.D.

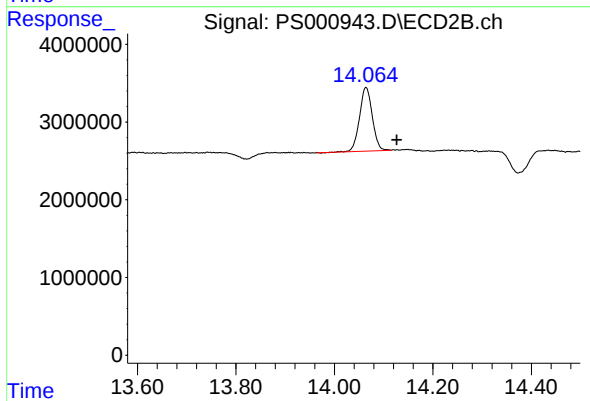

#11 2,4,5-TP (SILVEX)


R.T.: 14.064 min
Delta R.T.: -0.062 min
Response: 14747009
Conc: 11.75 ng/ml

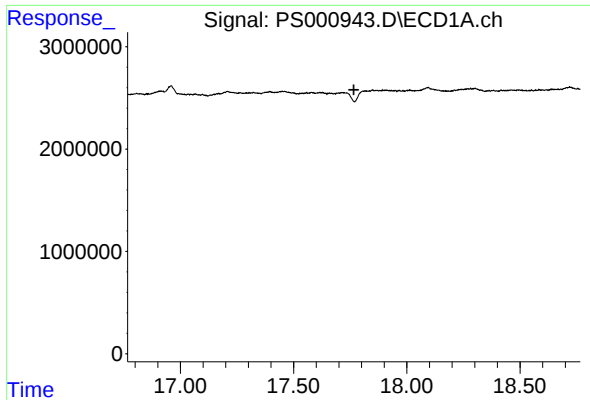

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.766 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

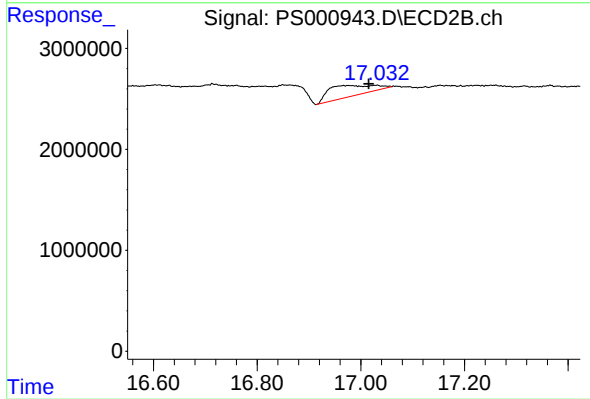

#16 DCPA

R.T.: 17.032 min
Delta R.T.: 0.017 min
Response: 6573336
Conc: 3.82 ng/ml