

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
 Data File : PS000947.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2018 18:00
 Operator : UA
 Sample : J3914-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 00:58:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.634	11.047	52920062	46308168	256.495	212.621
Target Compounds							
1) T	Dalapon	0.000	2.472	0	446575	N.D.	1.657 #
2) T	3,5-DICHL...	0.000	9.286	0	40611851	N.D.	138.063 #
5) T	DICAMBA	0.000	11.291	0	5499902	N.D.	7.007 #
6) T	MCP	12.328	0.000	5145109	0	9.367	N.D. #
7) T	MCPA	12.603	0.000	4119148	0	4.513	N.D. #
15) T	Picloram	0.000	16.937	0	5178125	N.D.	3.401 #
16) T	DCPA	0.000	16.993	0	6450731	N.D.	3.752 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
Data File : PS000947.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2018 18:00
Operator : UA
Sample : J3914-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 00:58:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

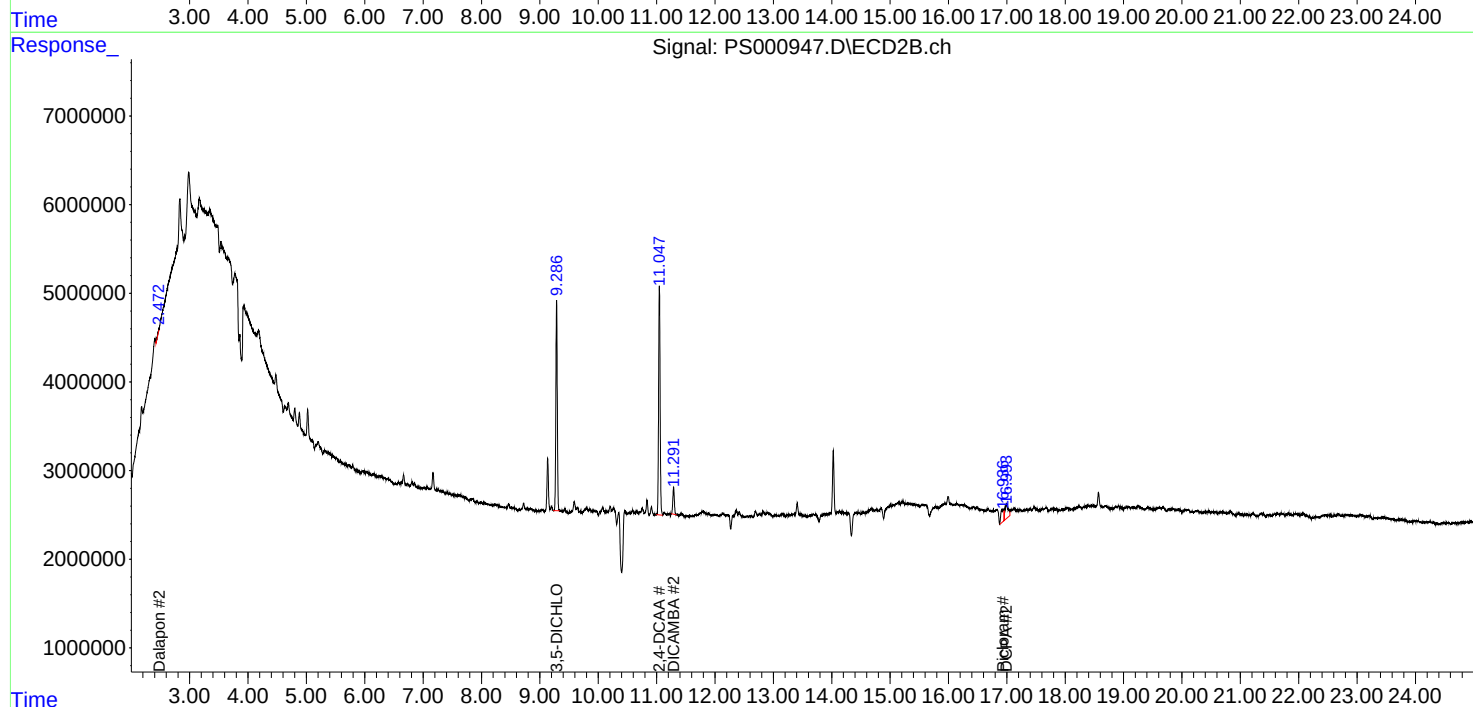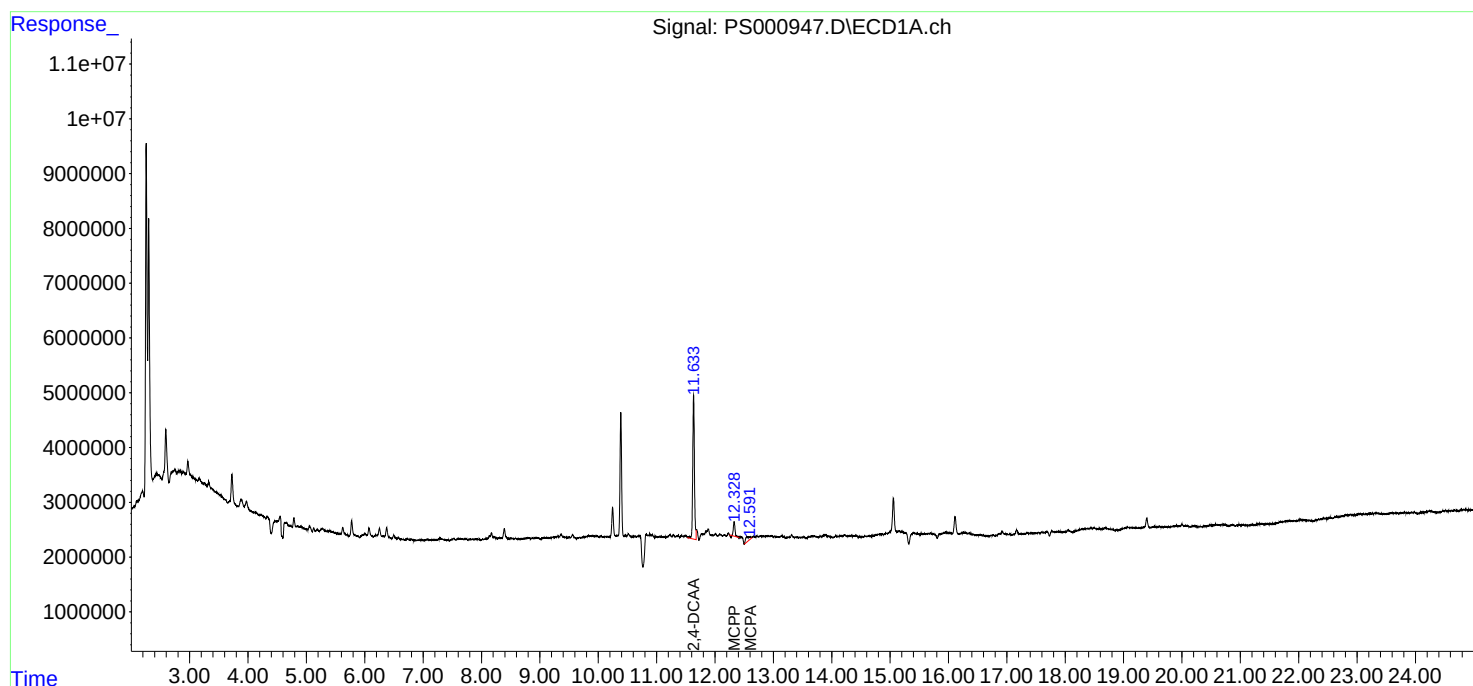


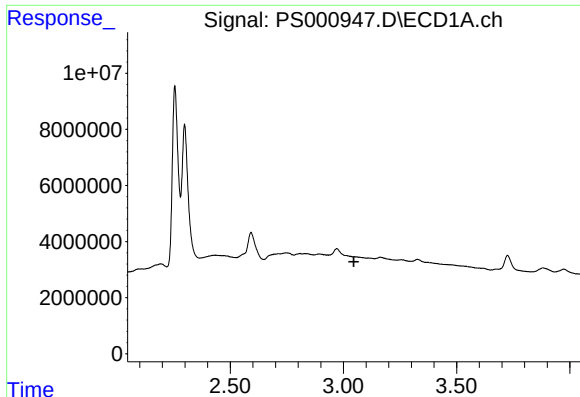

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.046 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

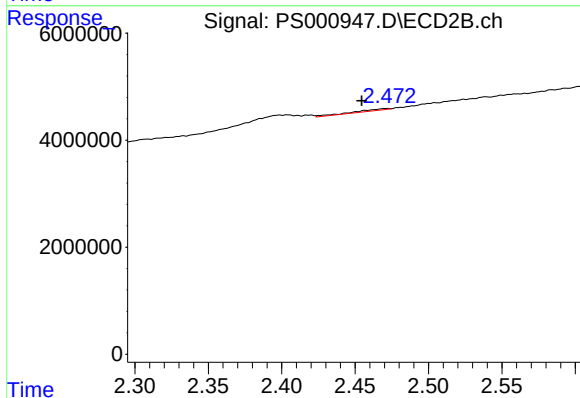


#1 Dalapon

R.T.: 2.472 min
Delta R.T.: 0.018 min
Response: 446575
Conc: 1.66 ng/ml

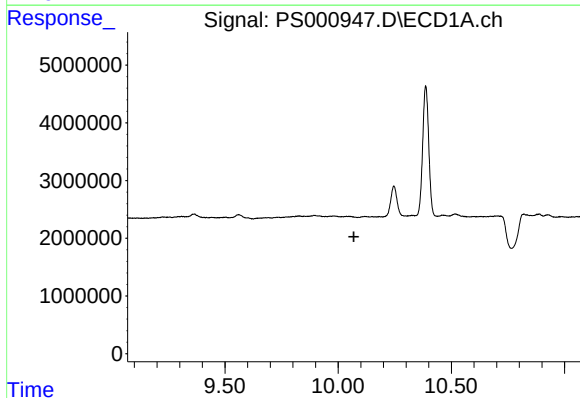


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

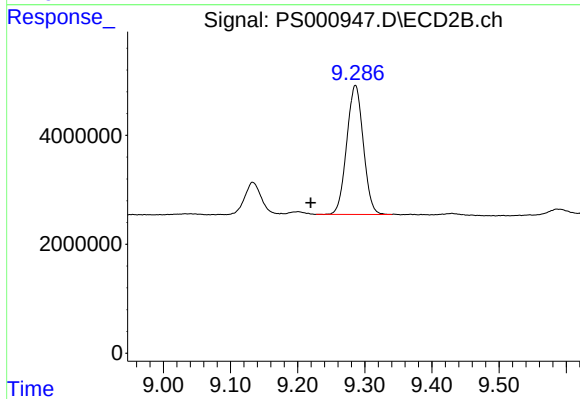

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.286 min
Delta R.T.: 0.067 min
Response: 40611851
Conc: 138.06 ng/ml

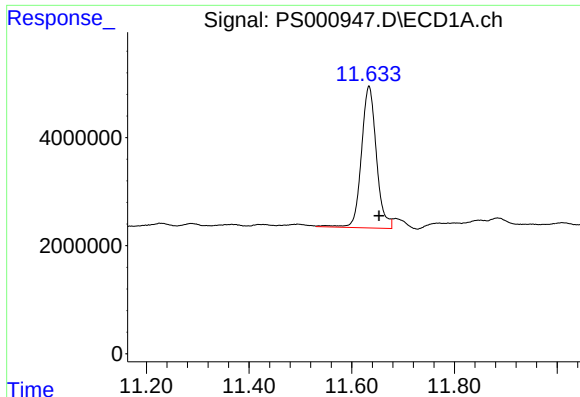

#4 2,4-DCAA


R.T.: 11.634 min
Delta R.T.: -0.020 min
Response: 52920062
Conc: 256.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

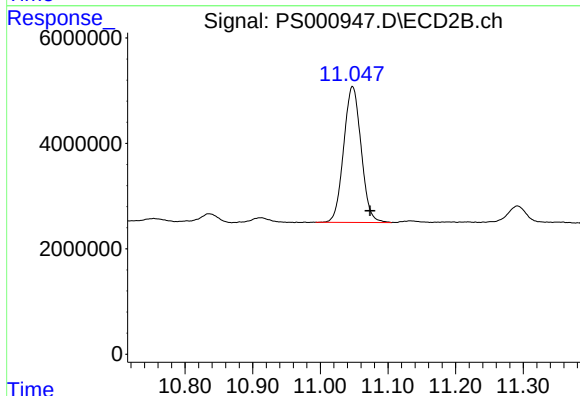


#4 2,4-DCAA

R.T.: 11.047 min
Delta R.T.: -0.026 min
Response: 46308168
Conc: 212.62 ng/ml

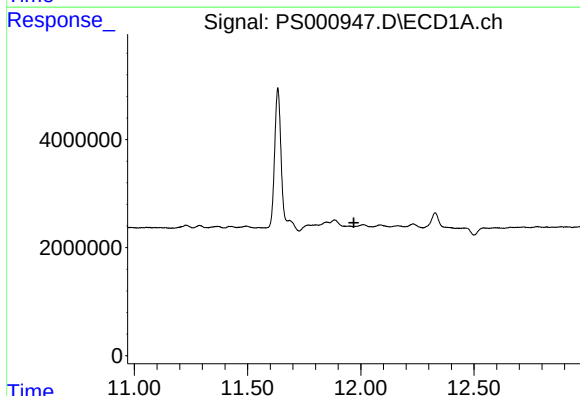


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.970 min
Response: 0
Conc: N.D.

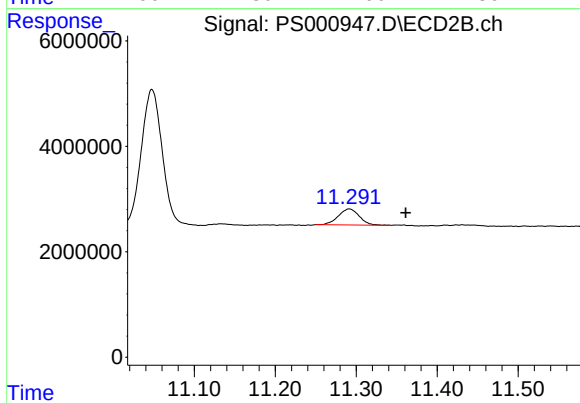

#5 DICAMBA


R.T.: 11.291 min
Delta R.T.: -0.070 min
Response: 5499902
Conc: 7.01 ng/ml

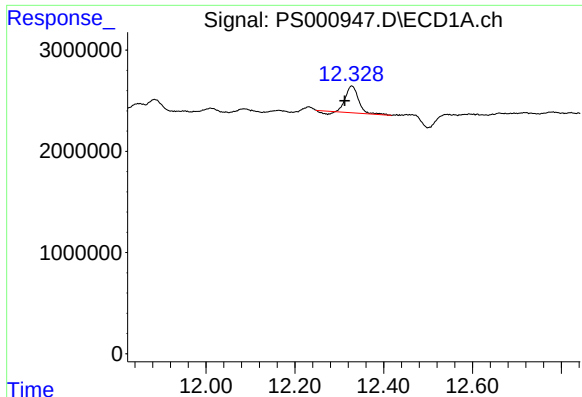

#6 MCPP


R.T.: 12.328 min
Delta R.T.: 0.016 min
Response: 5145109
Conc: 9.37 ug/ml

Instrument :
ECD_S
ClientSampleId :

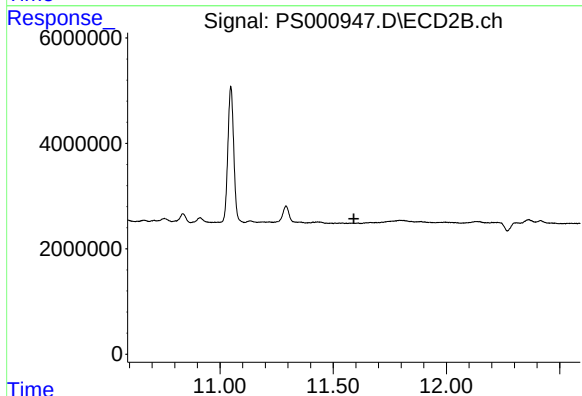


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

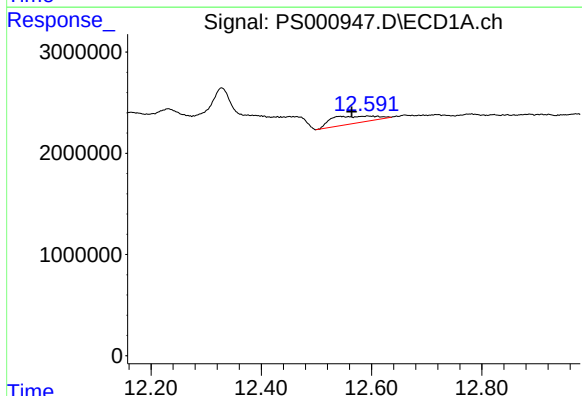


#7 MCPA

R.T.: 12.603 min
Delta R.T.: 0.039 min
Response: 4119148
Conc: 4.51 ug/ml

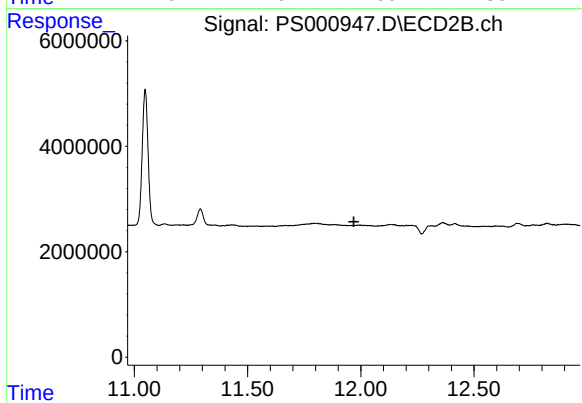

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 11.969 min
Response: 0
Conc: N.D.

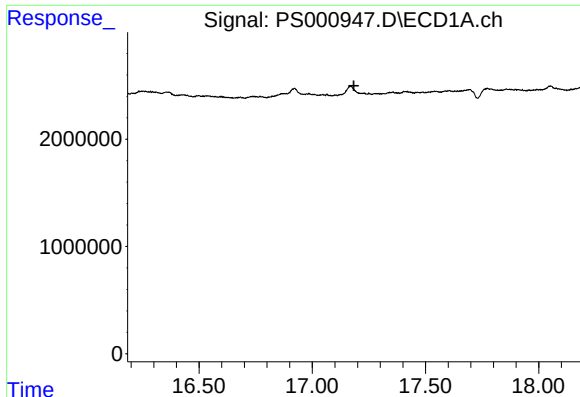

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

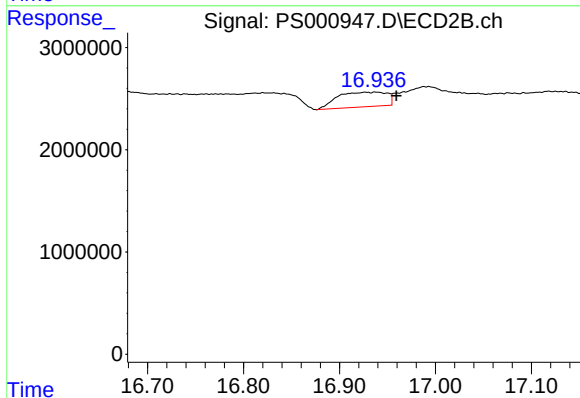


#15 Picloram

R.T.: 16.937 min
Delta R.T.: -0.022 min
Response: 5178125
Conc: 3.40 ng/ml

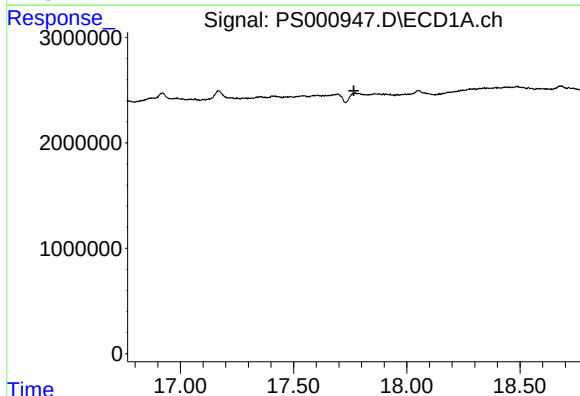

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.766 min
Response: 0
Conc: N.D.

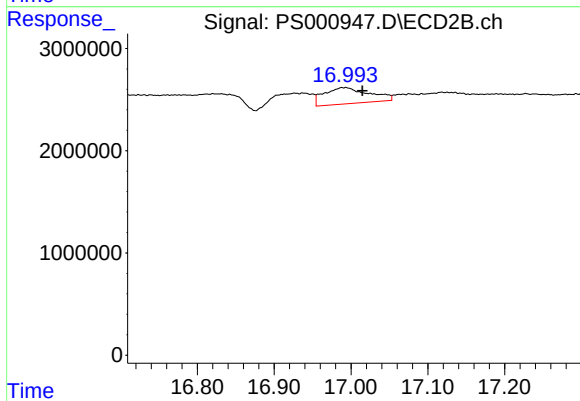

#16 DCPA

R.T.: 16.993 min
Delta R.T.: -0.022 min
Response: 6450731
Conc: 3.75 ng/ml