

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
 Data File : PS000950.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2018 19:33
 Operator : UA
 Sample : PB110958TB
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 00:59:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.687	11.101	63002220	52794097	305.362	242.400
Target Compounds							
2) T	3,5-DICHL...	0.000	9.188	0	15274660	N.D.	51.928 #
5) T	DICAMBA	11.939	11.345	3416736	6870781	4.339	8.753 #
8) T	DICHLORPROP	0.000	12.471	0	5498706	N.D.	27.224 #
11) T	2,4,5-TP ...	0.000	14.081	0	24077321	N.D.	19.186 #
12) T	2,4,5-T	15.111	0.000	22758429	0	18.689	N.D. #
15) T	Picloram	0.000	16.963	0	3589611	N.D.	2.357 #
16) T	DCPA	0.000	17.045	0	1680034	N.D.	0.977 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
Data File : PS000950.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2018 19:33
Operator : UA
Sample : PB110958TB
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 00:59:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

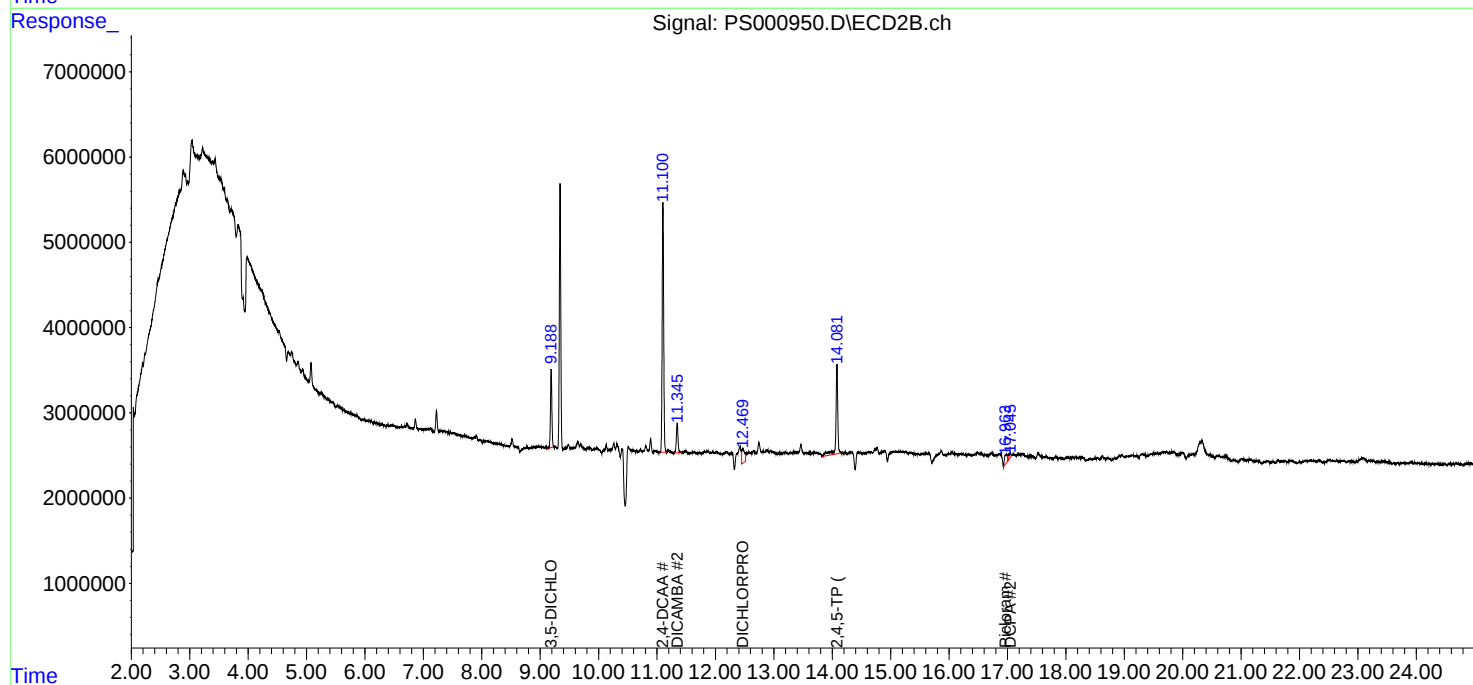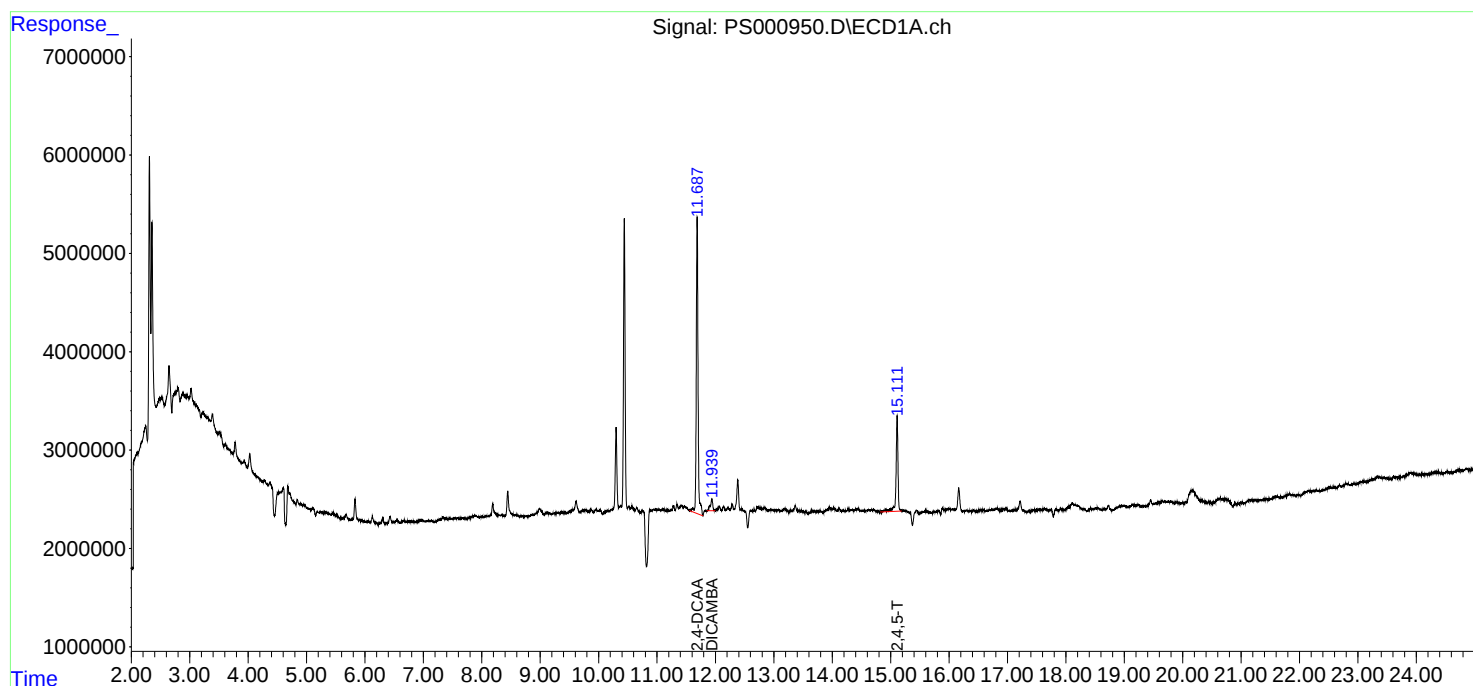


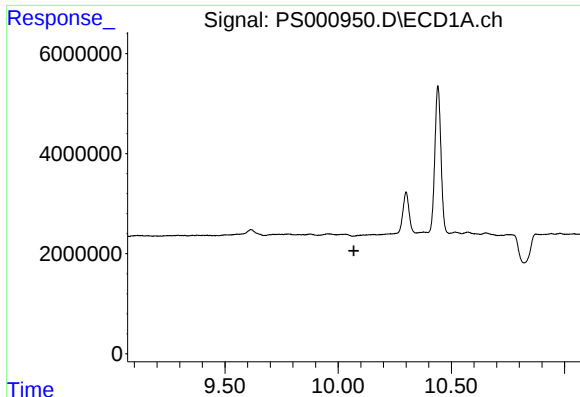

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

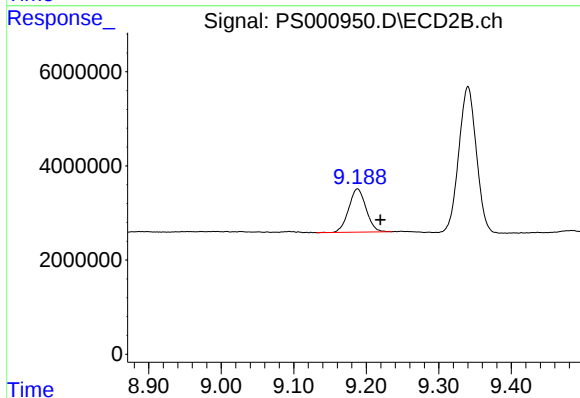


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.188 min
Delta R.T.: -0.031 min
Response: 15274660
Conc: 51.93 ng/ml

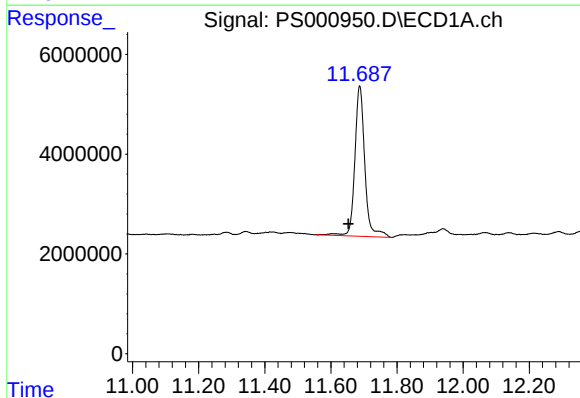


#4 2,4-DCAA

R.T.: 11.687 min
Delta R.T.: 0.034 min
Response: 63002220
Conc: 305.36 ng/ml

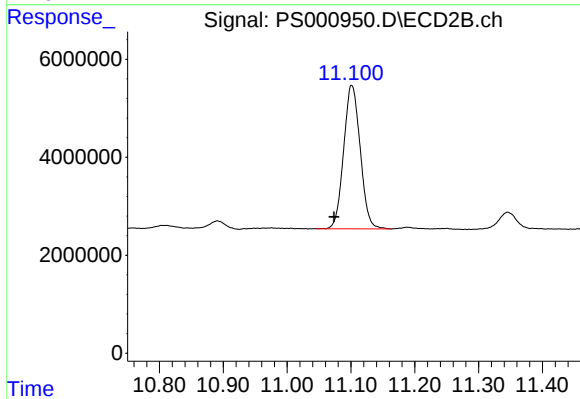

#4 2,4-DCAA


R.T.: 11.101 min
Delta R.T.: 0.028 min
Response: 52794097
Conc: 242.40 ng/ml

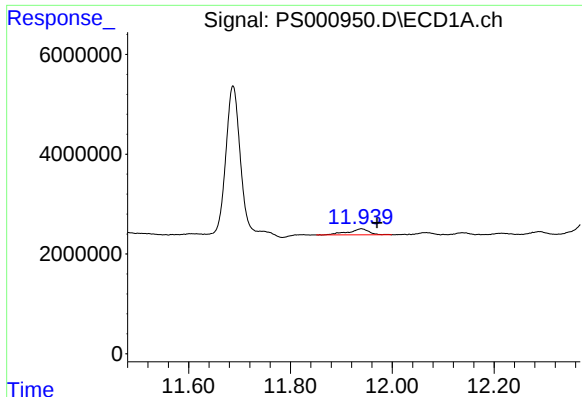

#5 DICAMBA


R.T.: 11.939 min
Delta R.T.: -0.030 min
Response: 3416736
Conc: 4.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

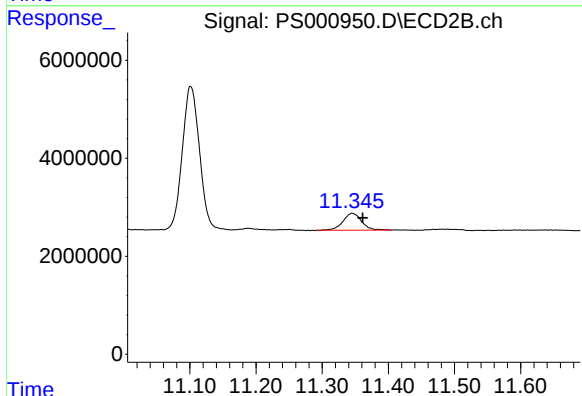


#5 DICAMBA

R.T.: 11.345 min
Delta R.T.: -0.016 min
Response: 6870781
Conc: 8.75 ng/ml

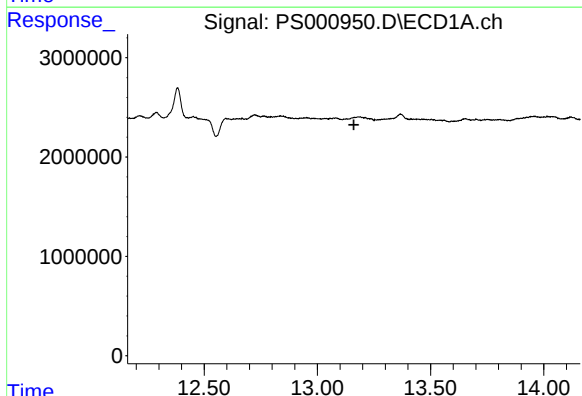


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

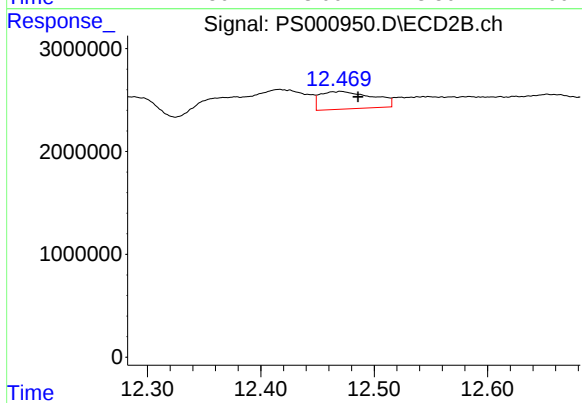

#8 DICHLORPROP


R.T.: 12.471 min
Delta R.T.: -0.015 min
Response: 5498706
Conc: 27.22 ng/ml

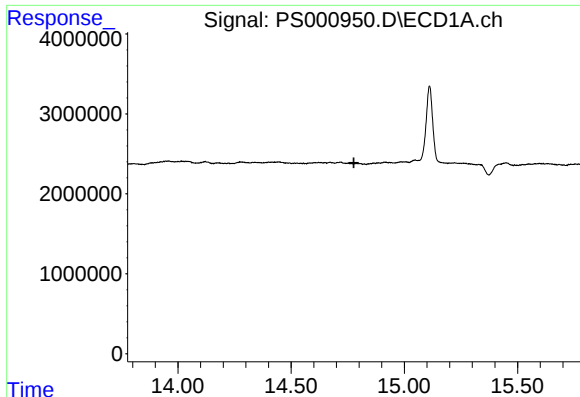

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.777 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

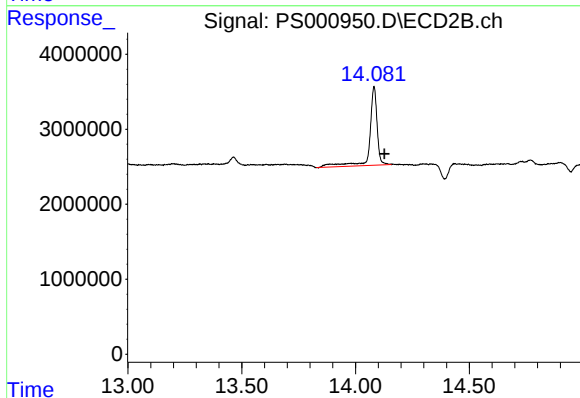


#11 2,4,5-TP (SILVEX)

R.T.: 14.081 min
Delta R.T.: -0.045 min
Response: 24077321
Conc: 19.19 ng/ml

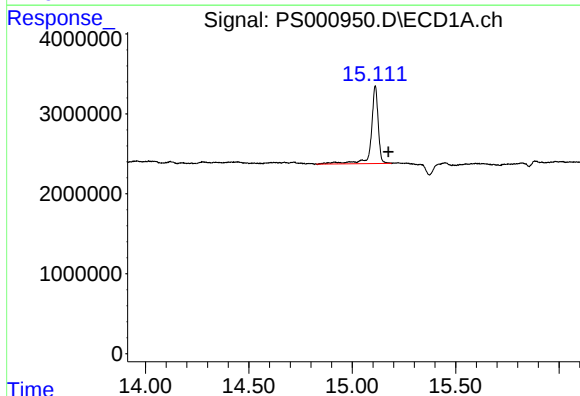


#12 2,4,5-T

R.T.: 15.111 min
Delta R.T.: -0.063 min
Response: 22758429
Conc: 18.69 ng/ml

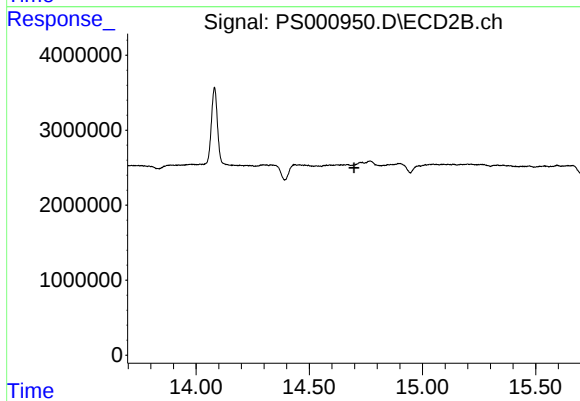

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.697 min
Response: 0
Conc: N.D.

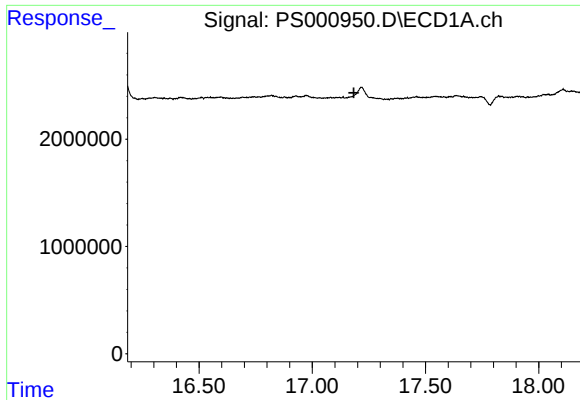

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

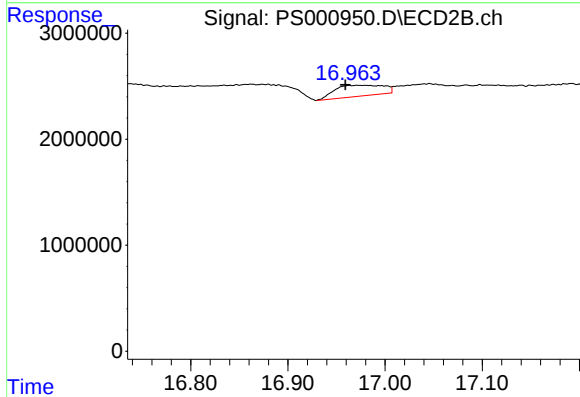


#15 Picloram

R.T.: 16.963 min
Delta R.T.: 0.004 min
Response: 3589611
Conc: 2.36 ng/ml

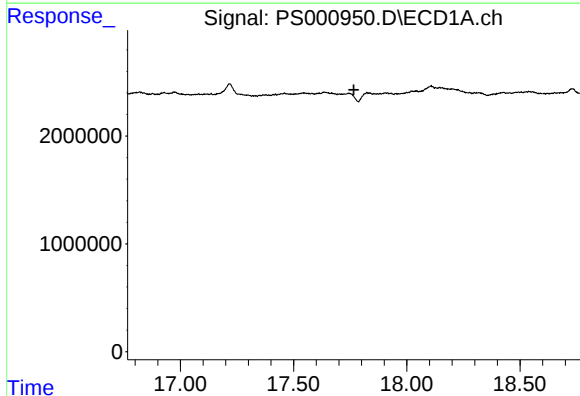

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.766 min
Response: 0
Conc: N.D.

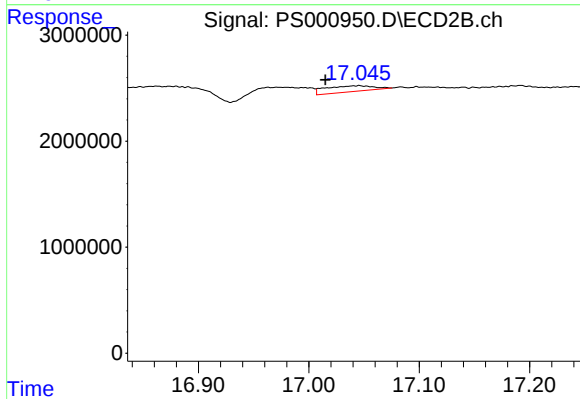

#16 DCPA

R.T.: 17.045 min
Delta R.T.: 0.030 min
Response: 1680034
Conc: 0.98 ng/ml