

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
 Data File : PS000960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2018 00:43
 Operator : UA
 Sample : PB111005BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 02:07:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.659	11.073	102.0E6	86248415	494.184	396.004
Target Compounds							
1) T	Dalapon	2.996	2.430	8364550	5347764	31.152	19.849 #
2) T	3,5-DICHL...	0.000	9.159	0	5239252	N.D.	17.811 #
5) T	DICAMBA	0.000	11.316	0	7157102	N.D.	9.118 #
6) T	MCP	12.354	0.000	10687180	0	19.456	N.D. #
7) T	MCPA	12.629	11.934	6768724	2590640	7.417	3.333 #
8) T	DICHLORPROP	0.000	12.436	0	1638344	N.D.	8.112 #
10) T	Pentachlo...	0.000	13.512	0	2219848	N.D.	0.707 #
14) T	DINOSEB	0.000	15.771	0	7841840	N.D.	9.364 #
15) T	Picloram	17.193	16.957	5024807	13022185	2.775	8.552 #
16) T	DCPA	0.000	17.015	0	10558290	N.D.	6.142 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
Data File : PS000960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2018 00:43
Operator : UA
Sample : PB111005BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 02:07:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

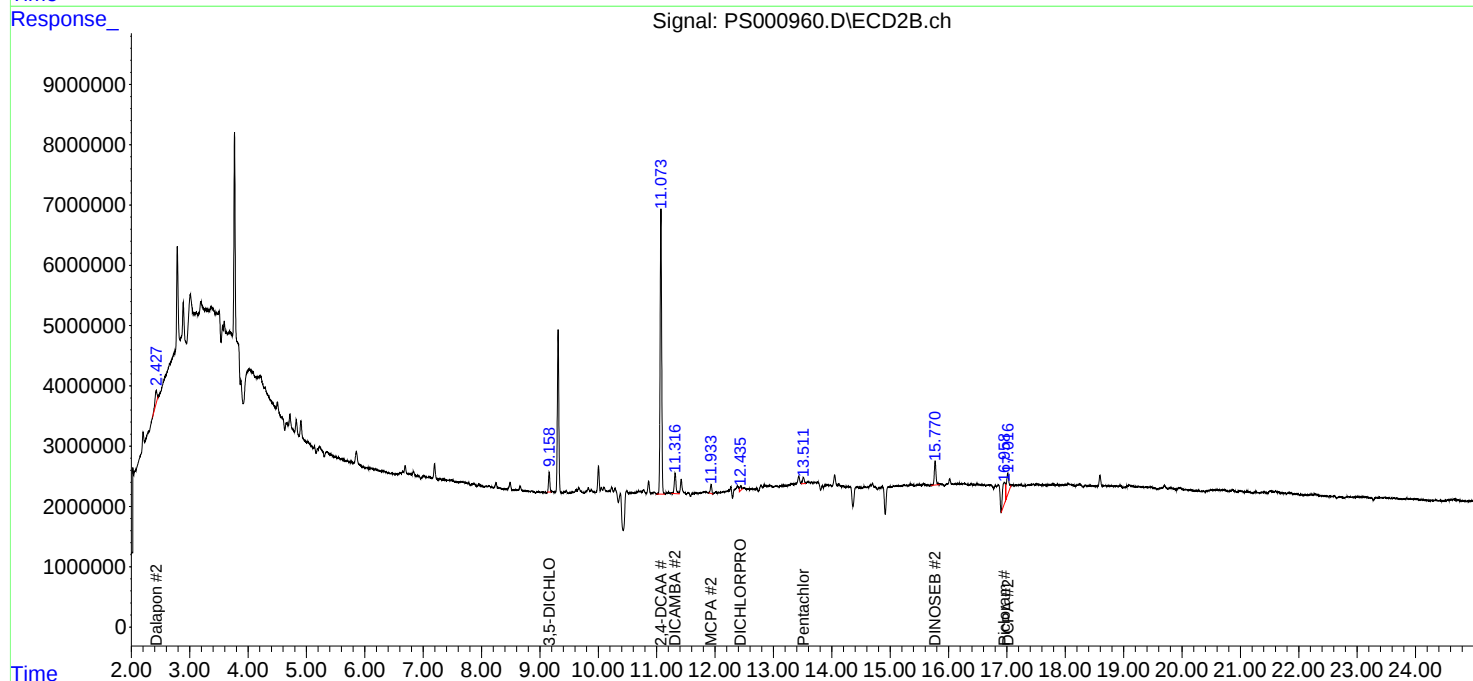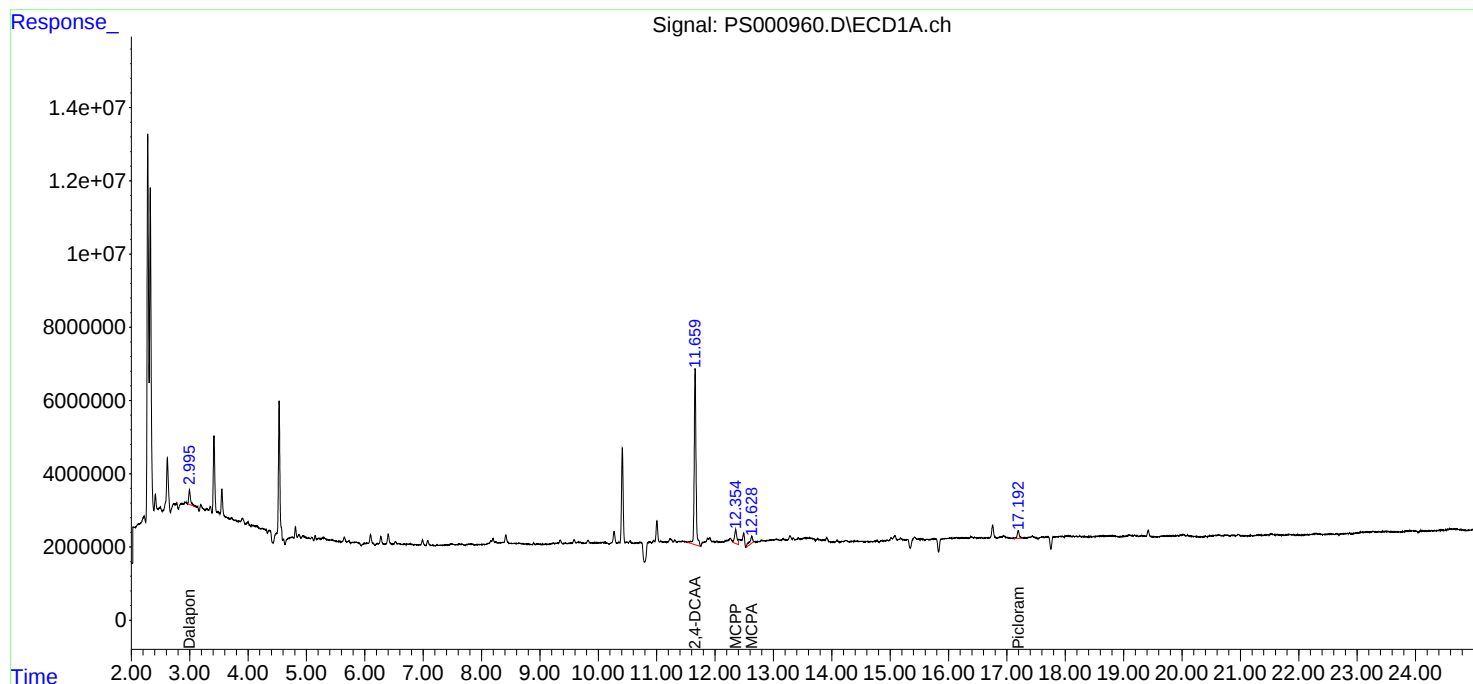


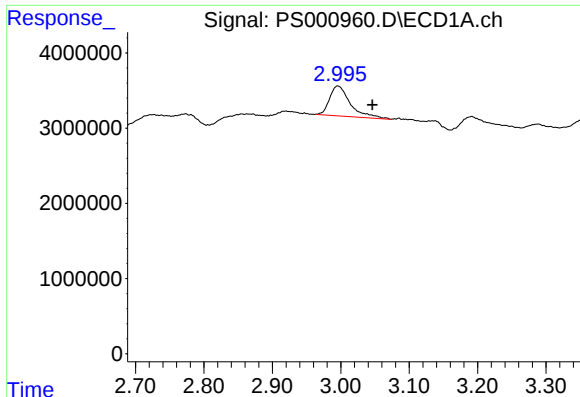

#1 Dalapon


R.T.: 2.996 min
Delta R.T.: -0.050 min
Response: 8364550
Conc: 31.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

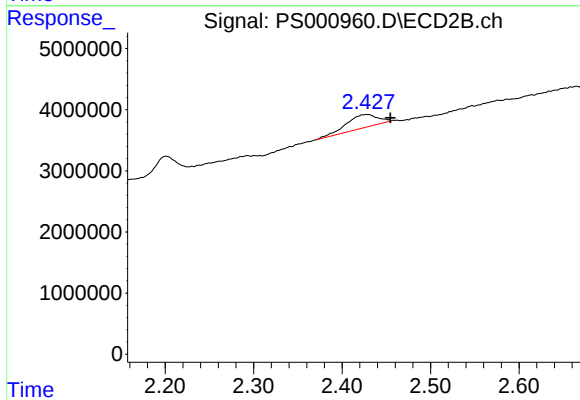


#1 Dalapon

R.T.: 2.430 min
Delta R.T.: -0.024 min
Response: 5347764
Conc: 19.85 ng/ml

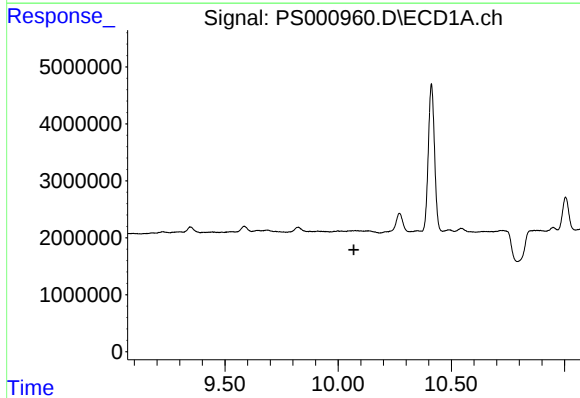


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

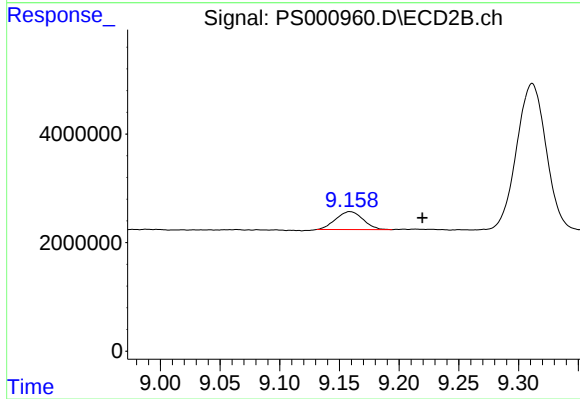

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.159 min
Delta R.T.: -0.061 min
Response: 5239252
Conc: 17.81 ng/ml

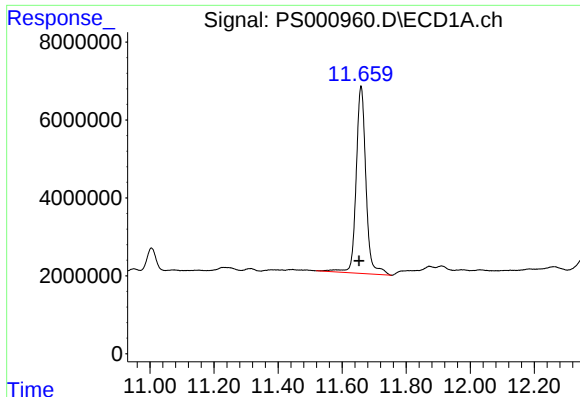

#4 2,4-DCAA


R.T.: 11.659 min
Delta R.T.: 0.006 min
Response: 101960005
Conc: 494.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

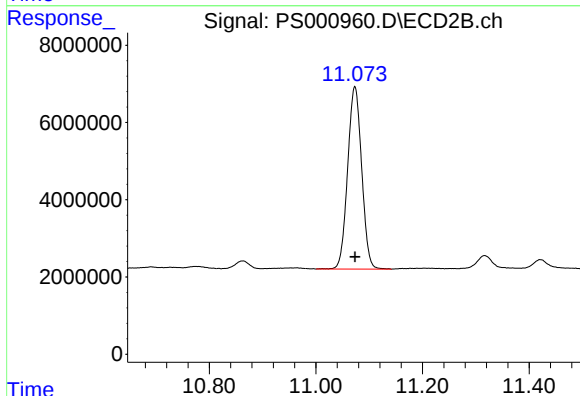


#4 2,4-DCAA

R.T.: 11.073 min
Delta R.T.: 0.000 min
Response: 86248415
Conc: 396.00 ng/ml

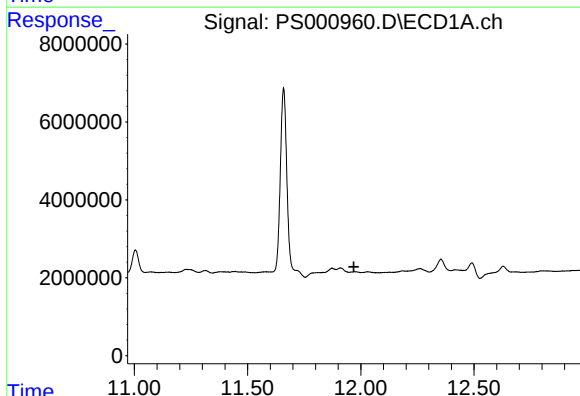


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.970 min
Response: 0
Conc: N.D.

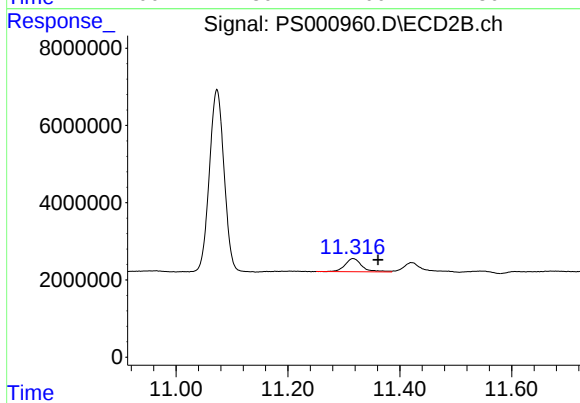

#5 DICAMBA


R.T.: 11.316 min
Delta R.T.: -0.045 min
Response: 7157102
Conc: 9.12 ng/ml

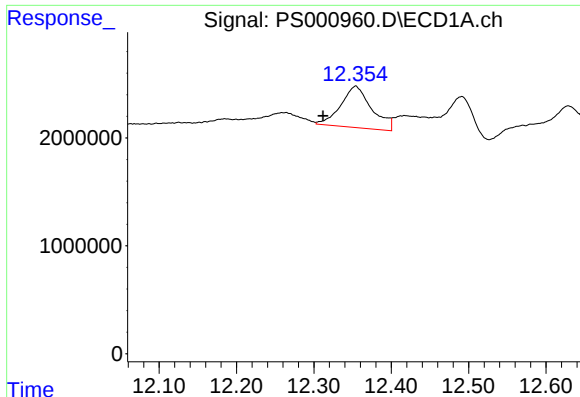

#6 MCPP


R.T.: 12.354 min
Delta R.T.: 0.042 min
Response: 10687180
Conc: 19.46 ug/ml

Instrument :
ECD_S
ClientSampleId :

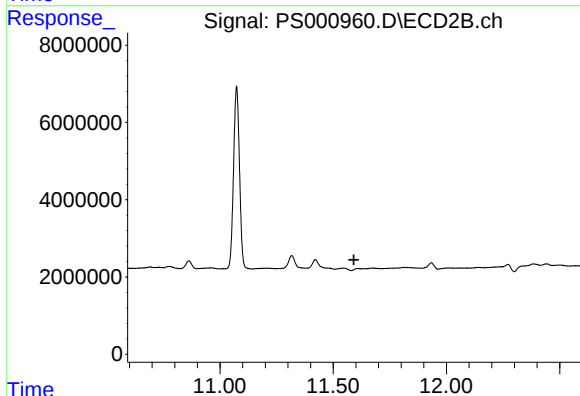


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

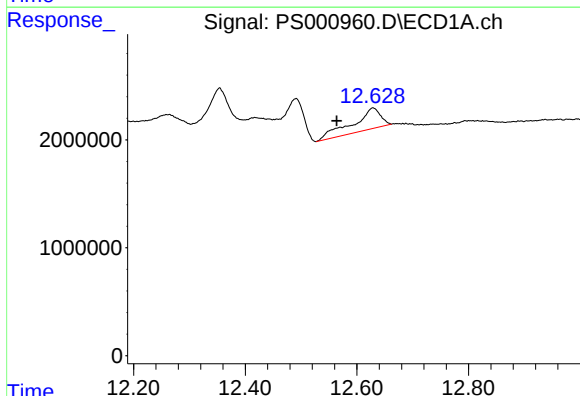


#7 MCPA

R.T.: 12.629 min
Delta R.T.: 0.065 min
Response: 6768724
Conc: 7.42 ug/ml

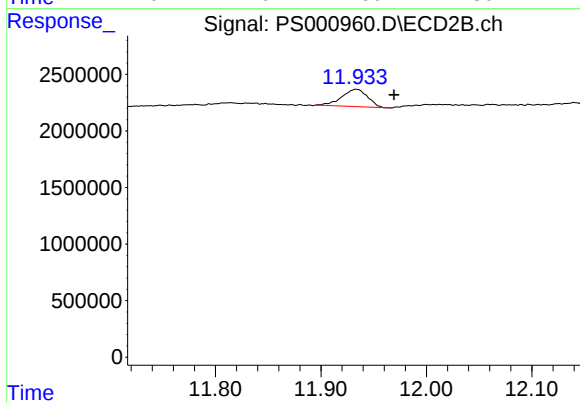

#7 MCPA


R.T.: 11.934 min
Delta R.T.: -0.036 min
Response: 2590640
Conc: 3.33 ug/ml

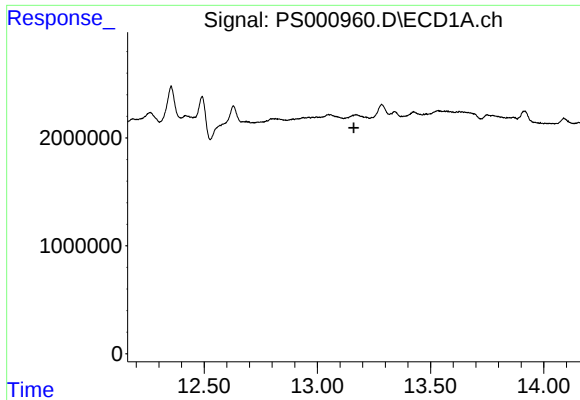

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.161 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

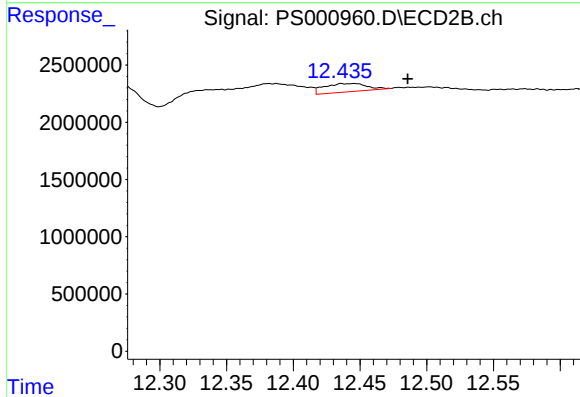


#8 DICHLORPROP

R.T.: 12.436 min
Delta R.T.: -0.050 min
Response: 1638344
Conc: 8.11 ng/ml

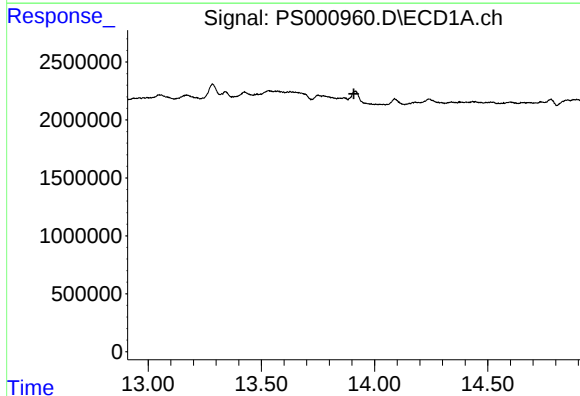


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.908 min
Response: 0
Conc: N.D.

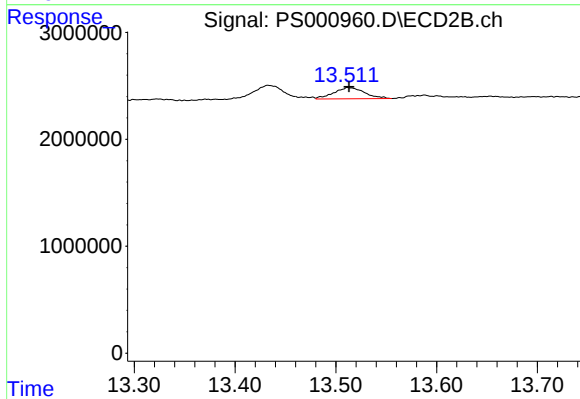

#10 Pentachlorophenol


R.T.: 13.512 min
Delta R.T.: 0.000 min
Response: 2219848
Conc: 0.71 ng/ml

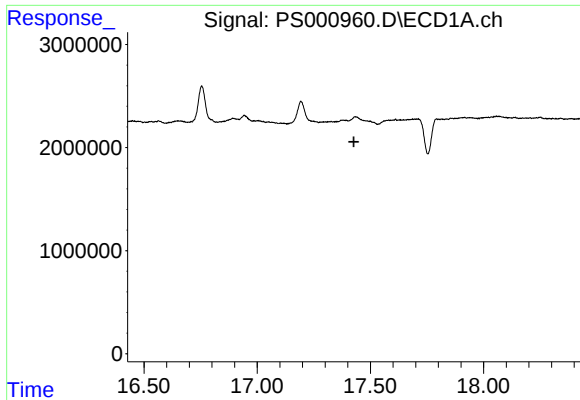

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.427 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

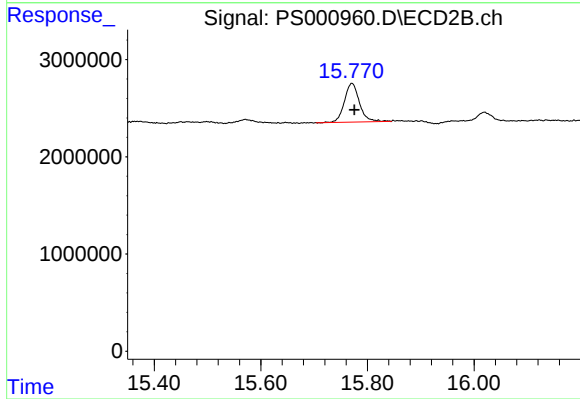


#14 DINOSEB

R.T.: 15.771 min
Delta R.T.: -0.005 min
Response: 7841840
Conc: 9.36 ng/ml

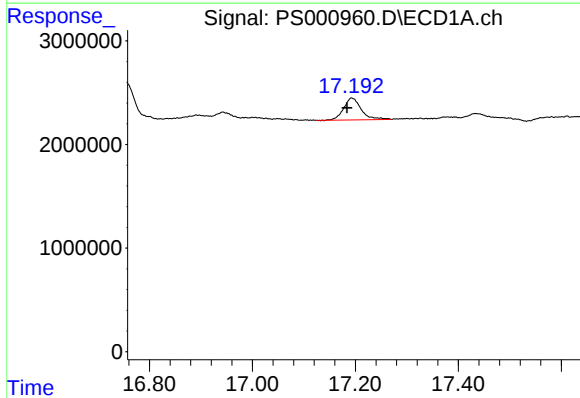


#15 Picloram

R.T.: 17.193 min
Delta R.T.: 0.009 min
Response: 5024807
Conc: 2.77 ng/ml

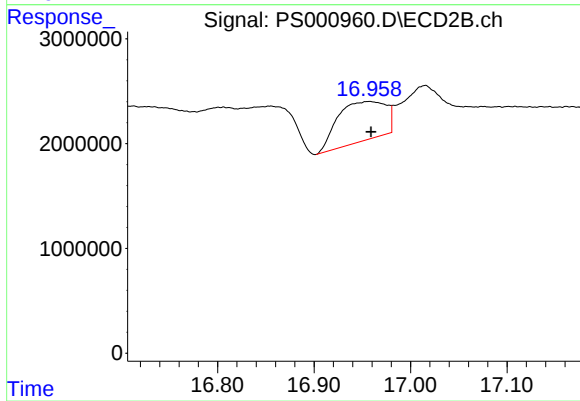

#15 Picloram


R.T.: 16.957 min
Delta R.T.: -0.002 min
Response: 13022185
Conc: 8.55 ng/ml

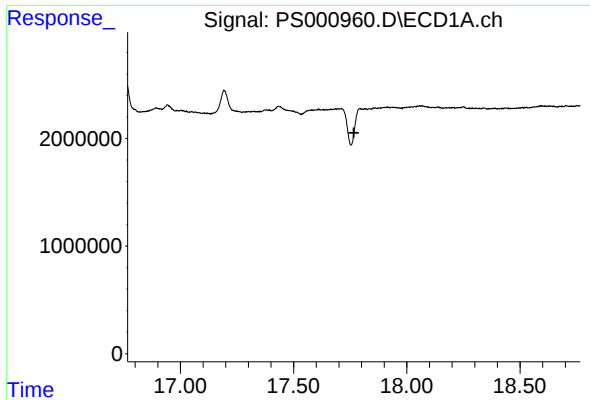

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.766 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

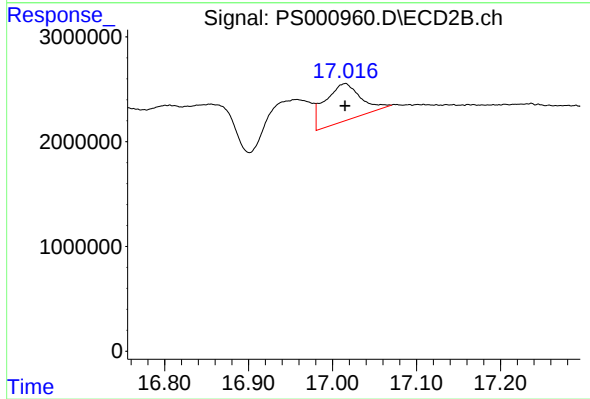

#16 DCPA

R.T.: 17.015 min
Delta R.T.: 0.000 min
Response: 10558290
Conc: 6.14 ng/ml