

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
 Data File : PS000963.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2018 02:15
 Operator : UA
 Sample : J3829-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 04:40:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.632	11.046	71190058	58219686	345.047	267.312
Target Compounds							
1) T	Dalapon	0.000	2.463	0	177666	N.D.	0.659 #
2) T	3,5-DICHL...	0.000	9.284	0	53068548	N.D.	180.411 #
6) T	MCP	12.326	0.000	6978344	0	12.704	N.D. #
14) T	DINOSEB	0.000	15.817	0	1281081	N.D.	1.530 #
15) T	Picloram	0.000	16.995	0	4932434	N.D.	3.239 #
16) T	DCPA	0.000	16.995	0	4932434	N.D.	2.869 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
Data File : PS000963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2018 02:15
Operator : UA
Sample : J3829-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 04:40:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

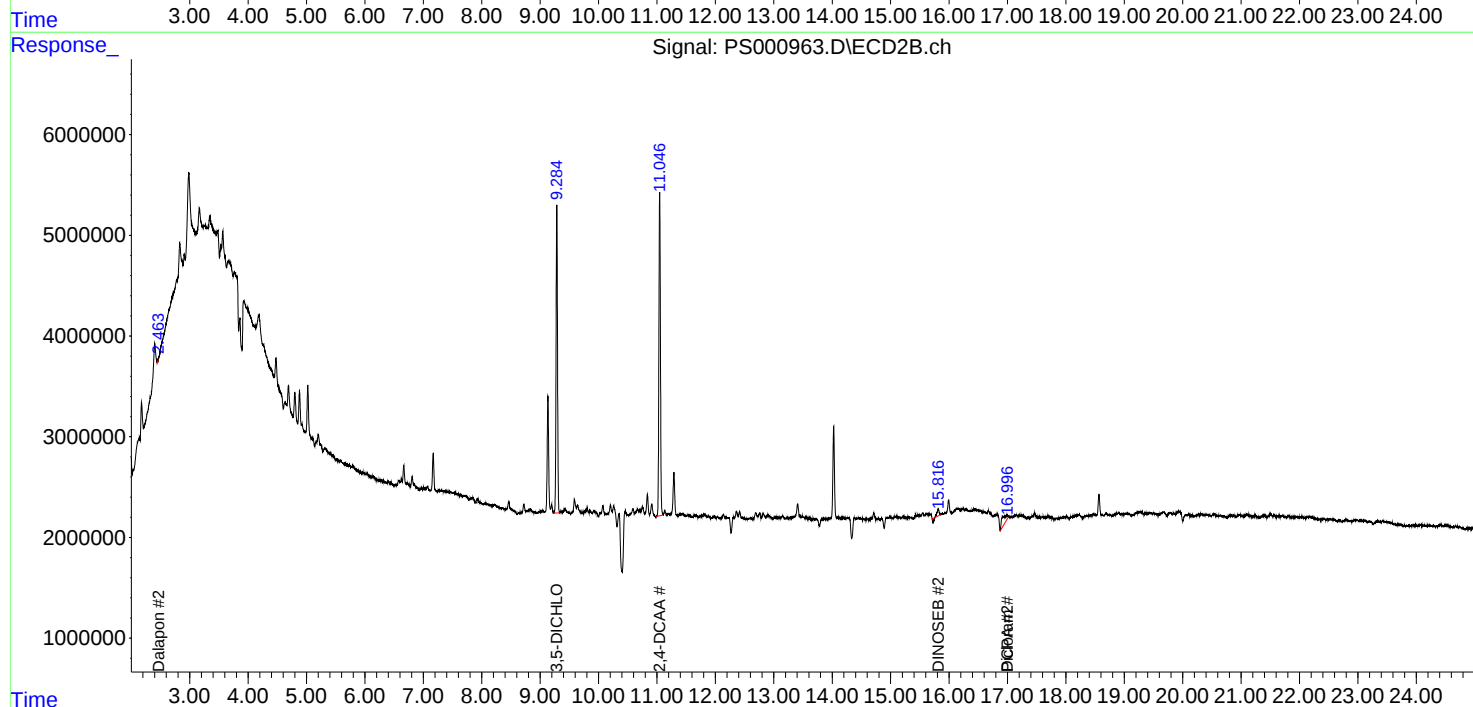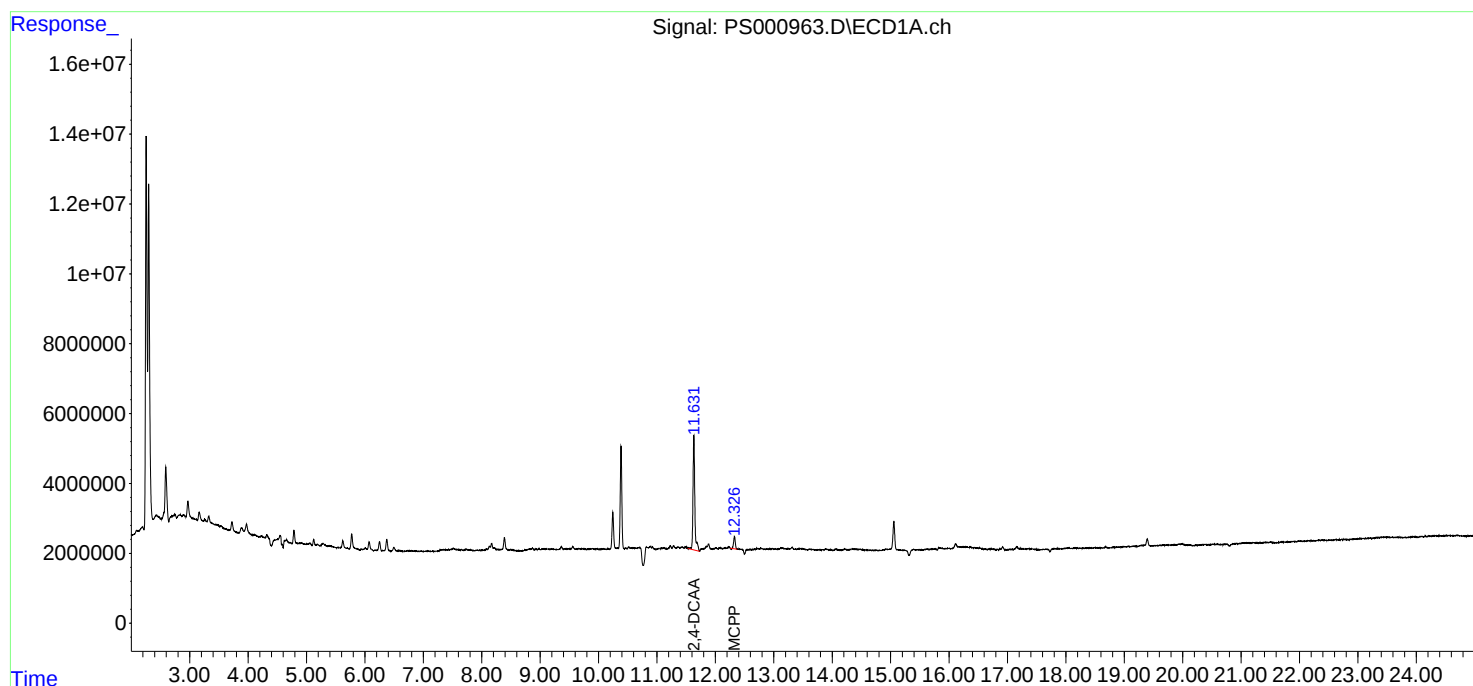


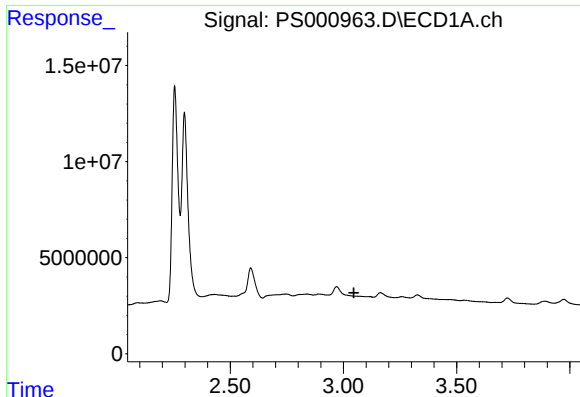

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.046 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

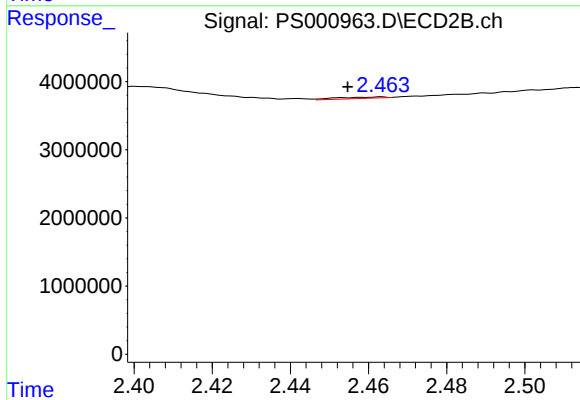


#1 Dalapon

R.T.: 2.463 min
Delta R.T.: 0.009 min
Response: 177666
Conc: 0.66 ng/ml

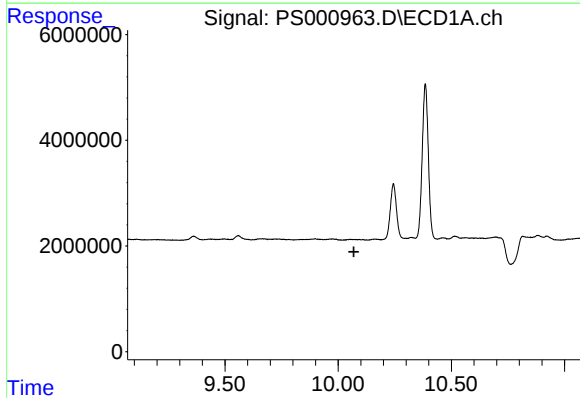


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

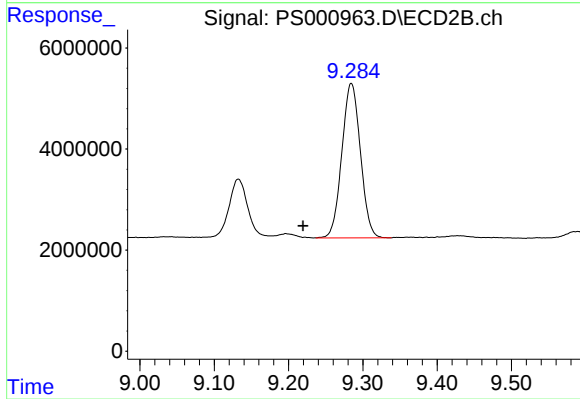

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.284 min
Delta R.T.: 0.065 min
Response: 53068548
Conc: 180.41 ng/ml

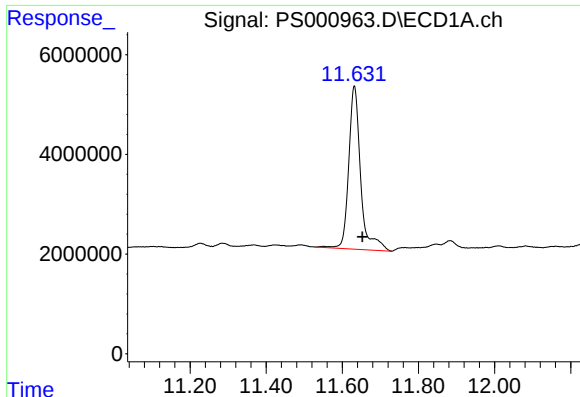

#4 2,4-DCAA


R.T.: 11.632 min
Delta R.T.: -0.022 min
Response: 71190058
Conc: 345.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

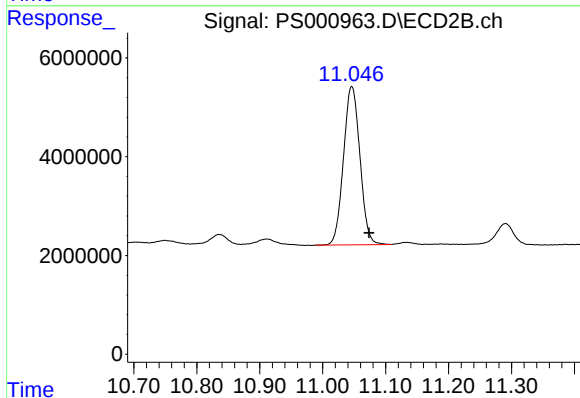


#4 2,4-DCAA

R.T.: 11.046 min
Delta R.T.: -0.027 min
Response: 58219686
Conc: 267.31 ng/ml

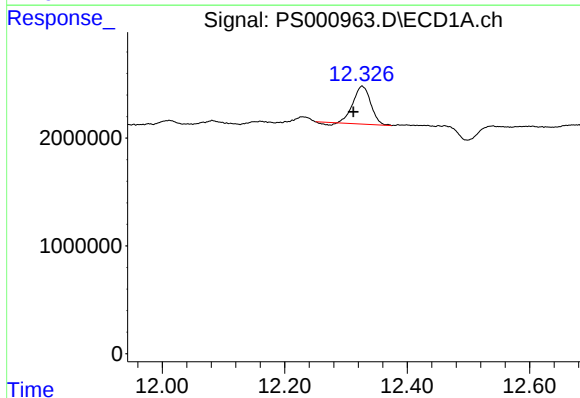


#6 MCP

R.T.: 12.326 min
Delta R.T.: 0.014 min
Response: 6978344
Conc: 12.70 ug/ml

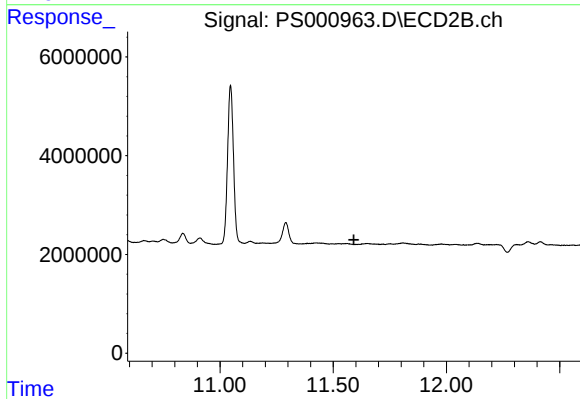

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

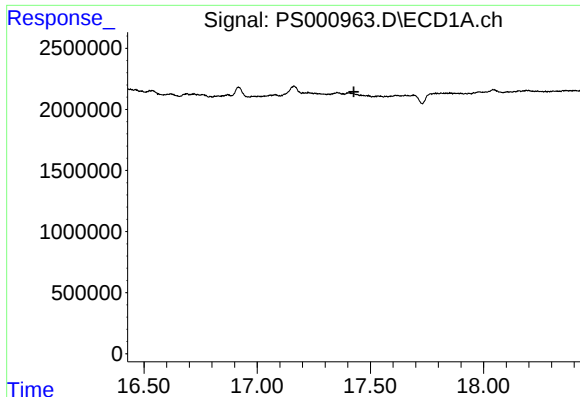

#14 DINoseb


R.T.: 0.000 min
Exp R.T. : 17.427 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

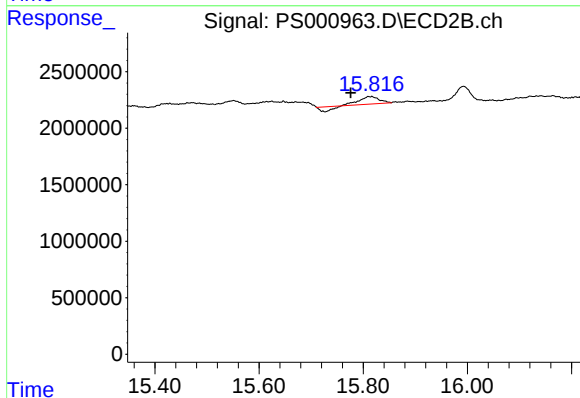


#14 DINoseb

R.T.: 15.817 min
Delta R.T.: 0.041 min
Response: 1281081
Conc: 1.53 ng/ml

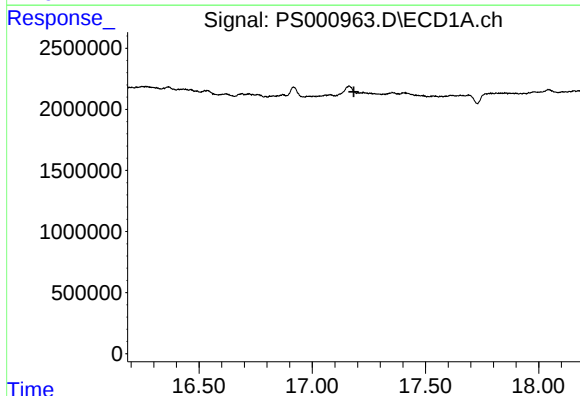


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.184 min
Response: 0
Conc: N.D.

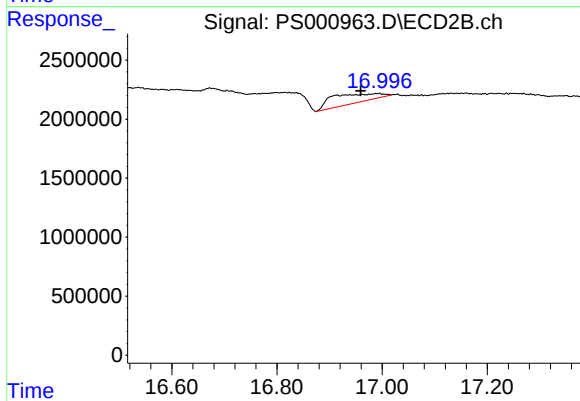

#15 Picloram


R.T.: 16.995 min
Delta R.T.: 0.036 min
Response: 4932434
Conc: 3.24 ng/ml

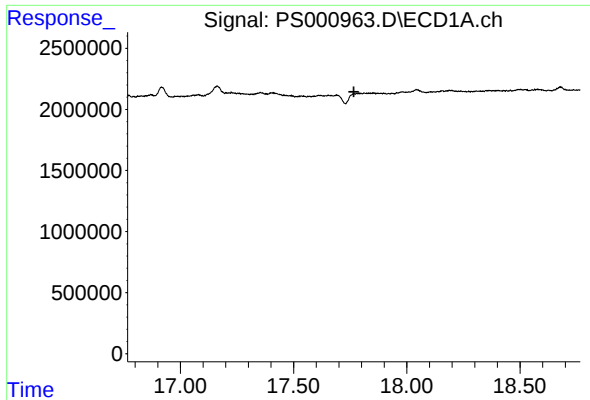

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.766 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

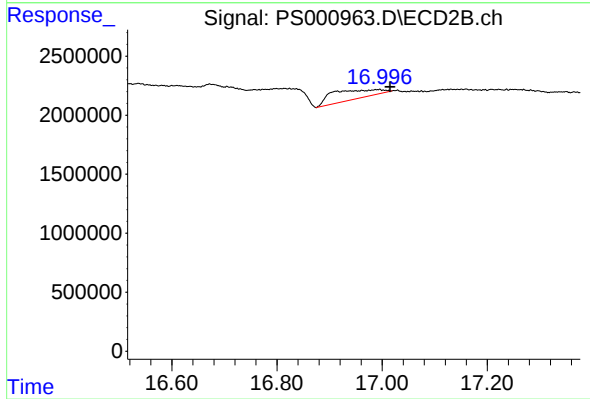

#16 DCPA

R.T.: 16.995 min
Delta R.T.: -0.020 min
Response: 4932434
Conc: 2.87 ng/ml