

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
 Data File : PS000964.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2018 02:46
 Operator : UA
 Sample : J3828-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 04:41:26 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.670	11.083	68625549	56601600	332.617	259.882
Target Compounds							
1) T	Dalapon	3.007	2.443	9094704	4852598	33.871	18.011 #
2) T	3,5-DICHL...	0.000	9.170	0	13739096	N.D.	46.707 #
5) T	DICAMBA	11.922	11.327	3827077	6656087	4.861	8.480 #
6) T	MCP	12.365	0.000	5990047	0	10.905	N.D. #
8) T	DICHLORPROP	0.000	12.452	0	1476327	N.D.	7.309 #
10) T	Pentachlo...	0.000	13.443	0	2849760	N.D.	0.908 #
11) T	2,4,5-TP ...	0.000	14.062	0	13760797	N.D.	10.965 #
15) T	Picloram	17.198	0.000	3370028	0	1.861	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
Data File : PS000964.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2018 02:46
Operator : UA
Sample : J3828-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 04:41:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

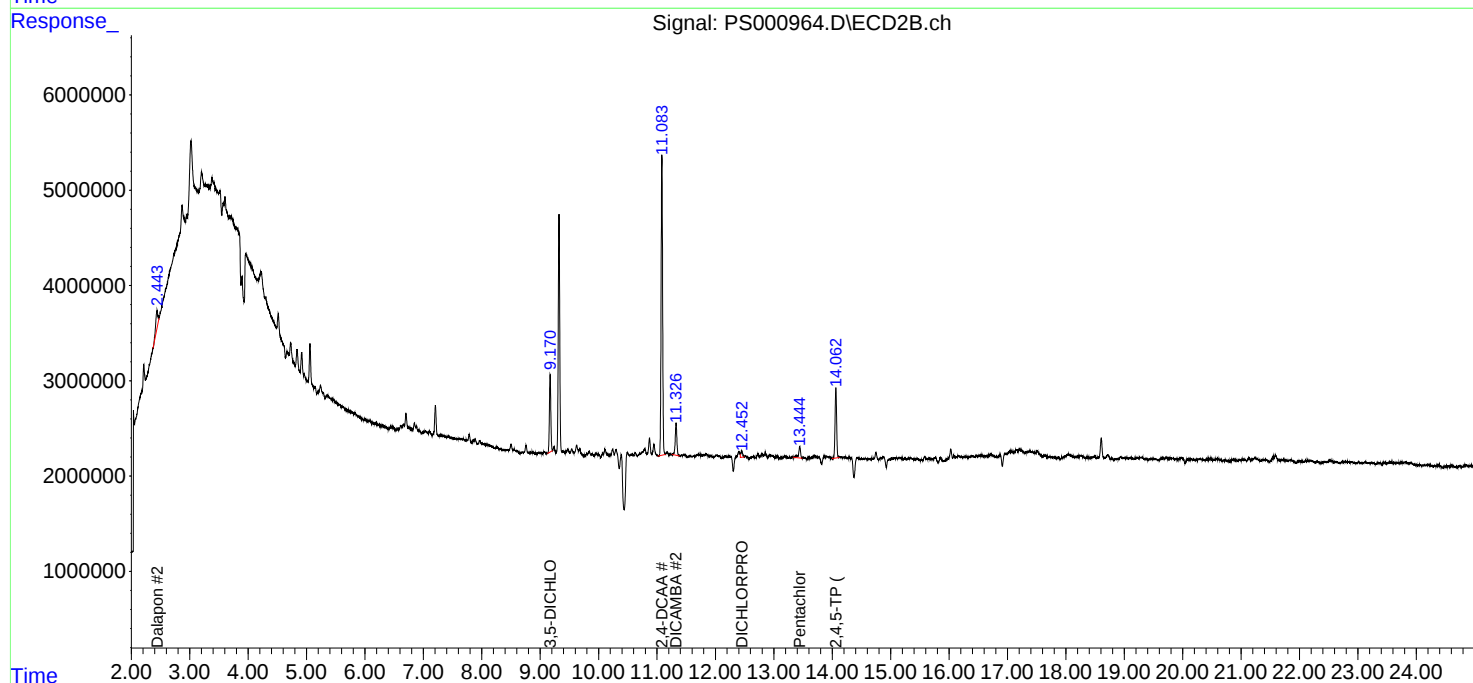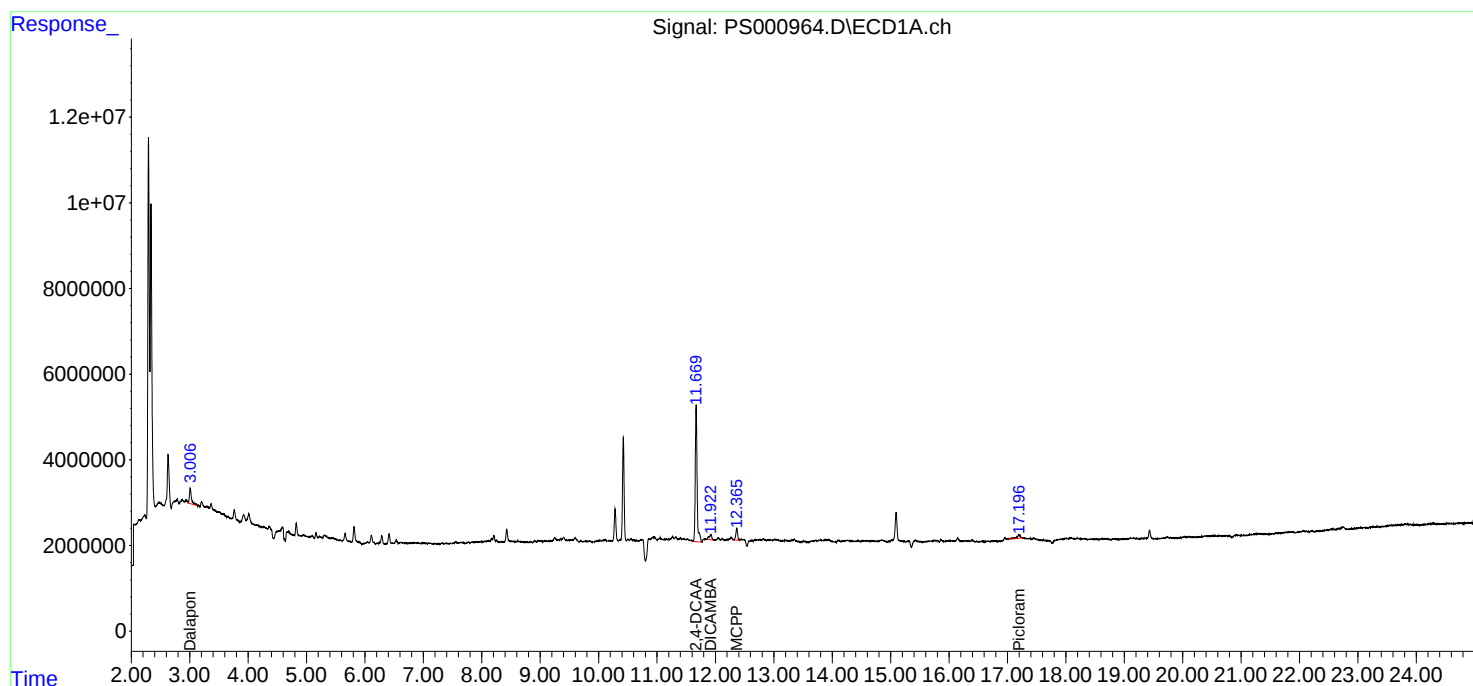


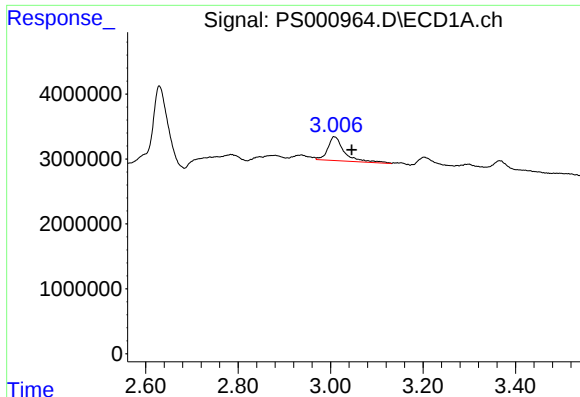

#1 Dalapon


R.T.: 3.007 min
Delta R.T.: -0.038 min
Response: 9094704
Conc: 33.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

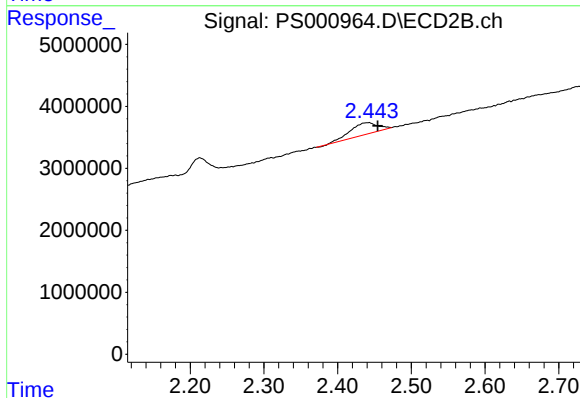


#1 Dalapon

R.T.: 2.443 min
Delta R.T.: -0.012 min
Response: 4852598
Conc: 18.01 ng/ml

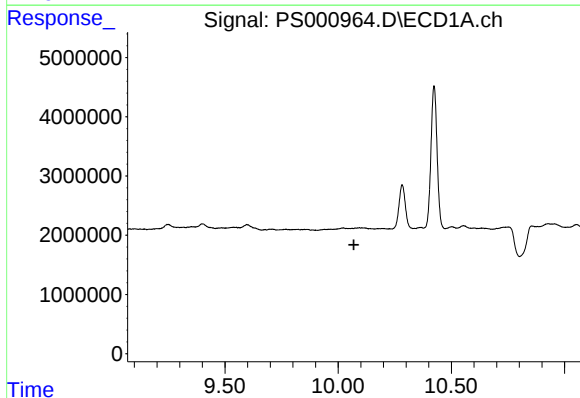


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

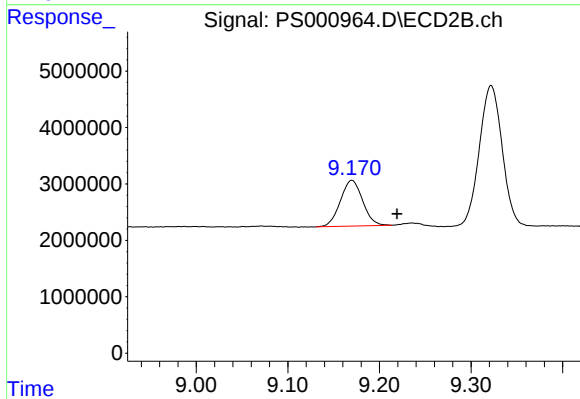

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.170 min
Delta R.T.: -0.049 min
Response: 13739096
Conc: 46.71 ng/ml

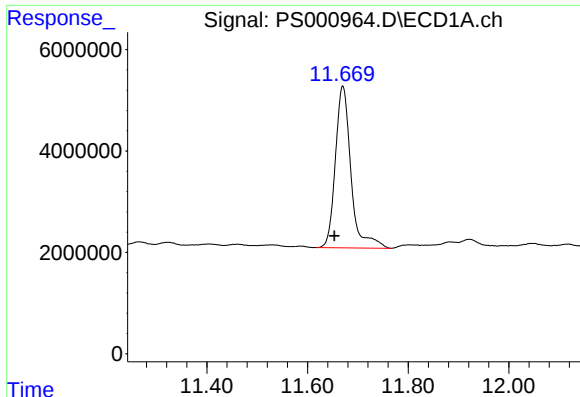

#4 2,4-DCAA


R.T.: 11.670 min
Delta R.T.: 0.017 min
Response: 68625549
Conc: 332.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

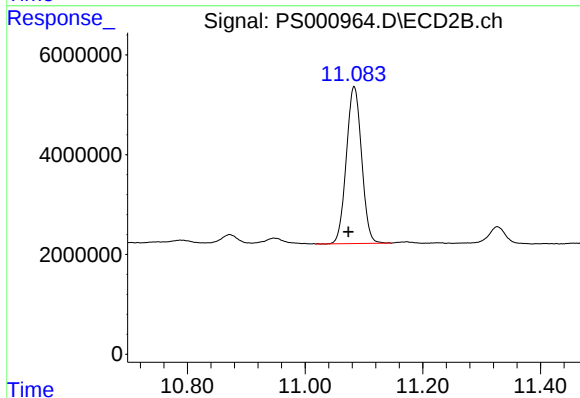


#4 2,4-DCAA

R.T.: 11.083 min
Delta R.T.: 0.010 min
Response: 56601600
Conc: 259.88 ng/ml

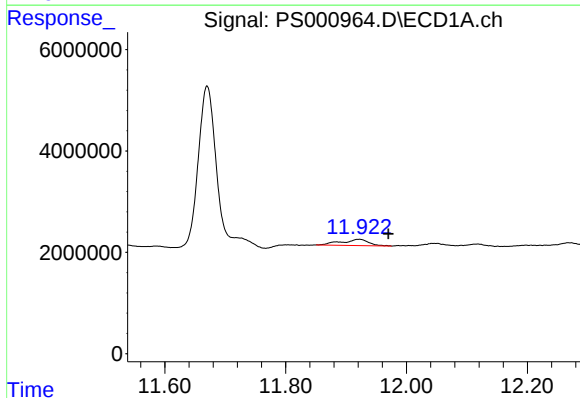


#5 DICAMBA

R.T.: 11.922 min
Delta R.T.: -0.048 min
Response: 3827077
Conc: 4.86 ng/ml

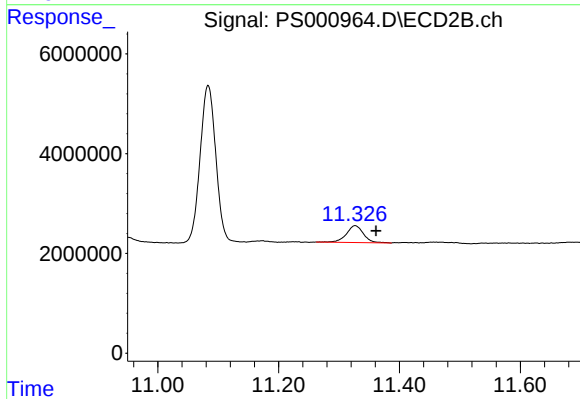

#5 DICAMBA


R.T.: 11.327 min
Delta R.T.: -0.035 min
Response: 6656087
Conc: 8.48 ng/ml

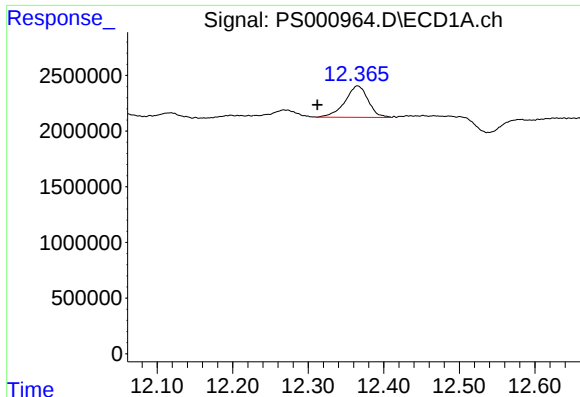

#6 MCP


R.T.: 12.365 min
Delta R.T.: 0.053 min
Response: 5990047
Conc: 10.90 ug/ml

Instrument :
ECD_S
ClientSampleId :

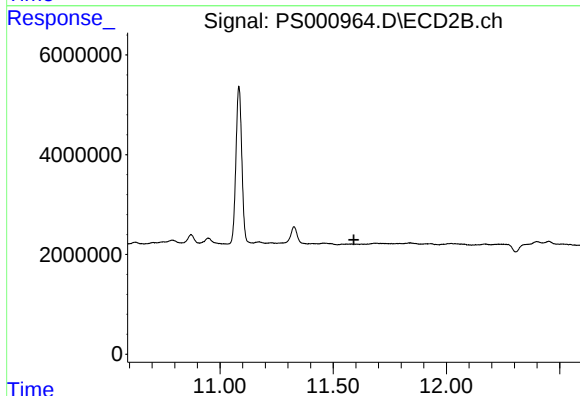


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

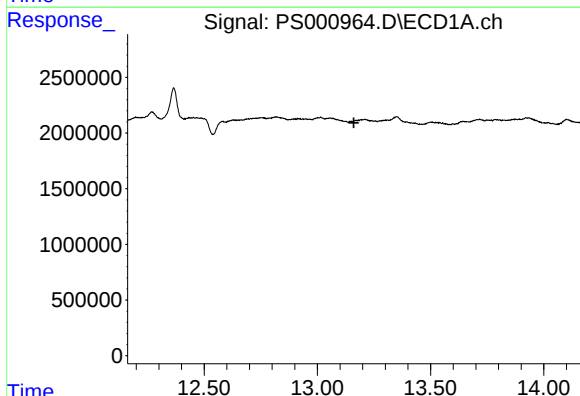


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

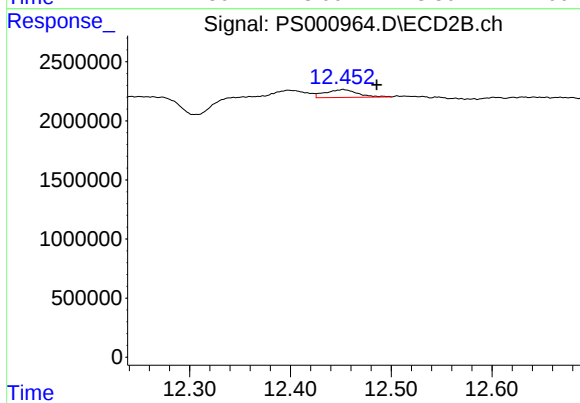

#8 DICHLORPROP


R.T.: 12.452 min
Delta R.T.: -0.034 min
Response: 1476327
Conc: 7.31 ng/ml

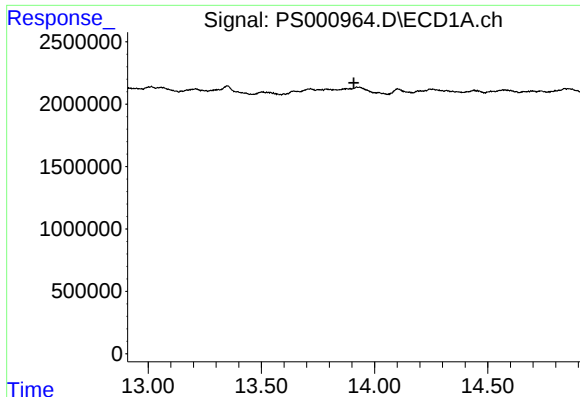

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.908 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

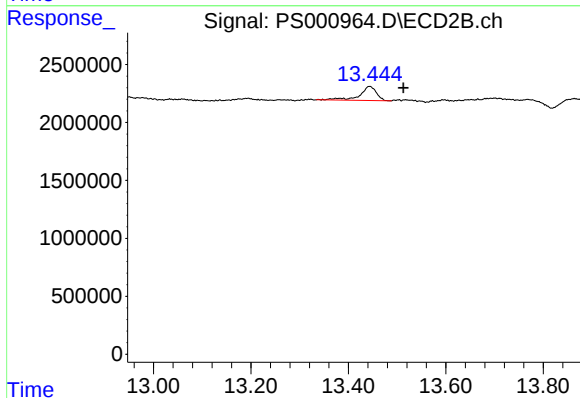


#10 Pentachlorophenol

R.T.: 13.443 min
Delta R.T.: -0.070 min
Response: 2849760
Conc: 0.91 ng/ml

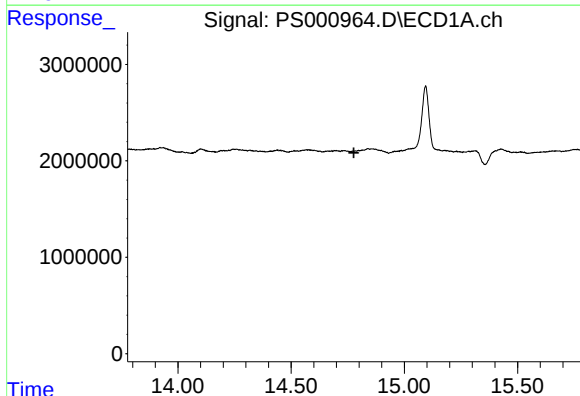


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.777 min
Response: 0
Conc: N.D.

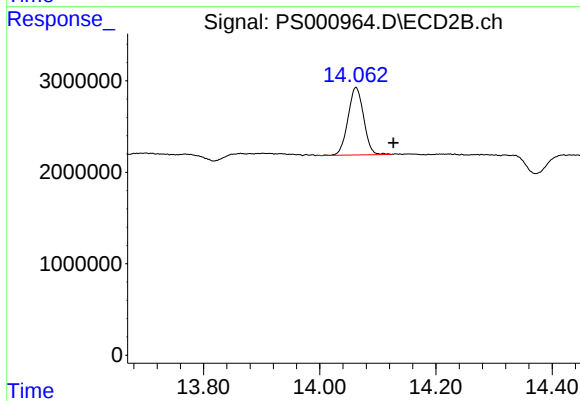

#11 2,4,5-TP (SILVEX)


R.T.: 14.062 min
Delta R.T.: -0.064 min
Response: 13760797
Conc: 10.97 ng/ml

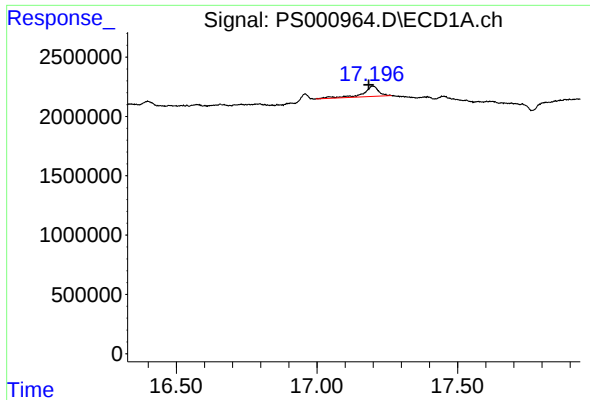

#15 Picloram

R.T.: 17.198 min
Delta R.T.: 0.014 min
Response: 3370028
Conc: 1.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

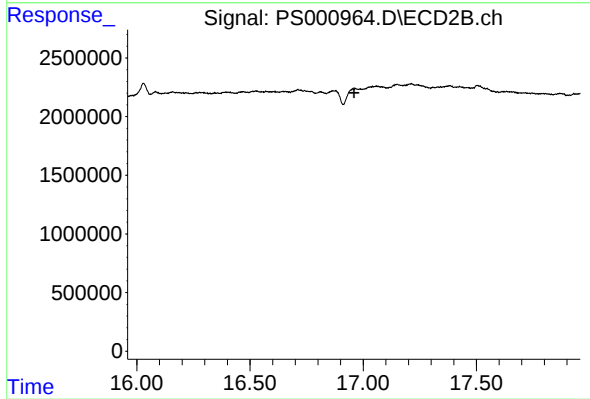

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.959 min
Response: 0
Conc: N.D.