

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
 Data File : PS000965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2018 03:17
 Operator : UA
 Sample : J3828-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 04:41:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.648	11.063	69504732	57003259	336.878	261.726
Target Compounds							
1) T	Dalapon	2.986	2.462	9156055	287325	34.100	1.066 #
5) T	DICAMBA	0.000	11.307	0	7471184	N.D.	9.518 #
6) T	MCPD	12.344	0.000	9468626	0	17.238	N.D. #
7) T	MCPA	12.558	0.000	4232630	0	4.638	N.D. #
8) T	DICHLORPROP	0.000	12.520	0	780417	N.D.	3.864 #
15) T	Picloram	17.179	16.948	3757015	1642985	2.074	1.079 #
16) T	DCPA	0.000	16.948	0	1642985	N.D.	0.956 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
Data File : PS000965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2018 03:17
Operator : UA
Sample : J3828-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 04:41:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

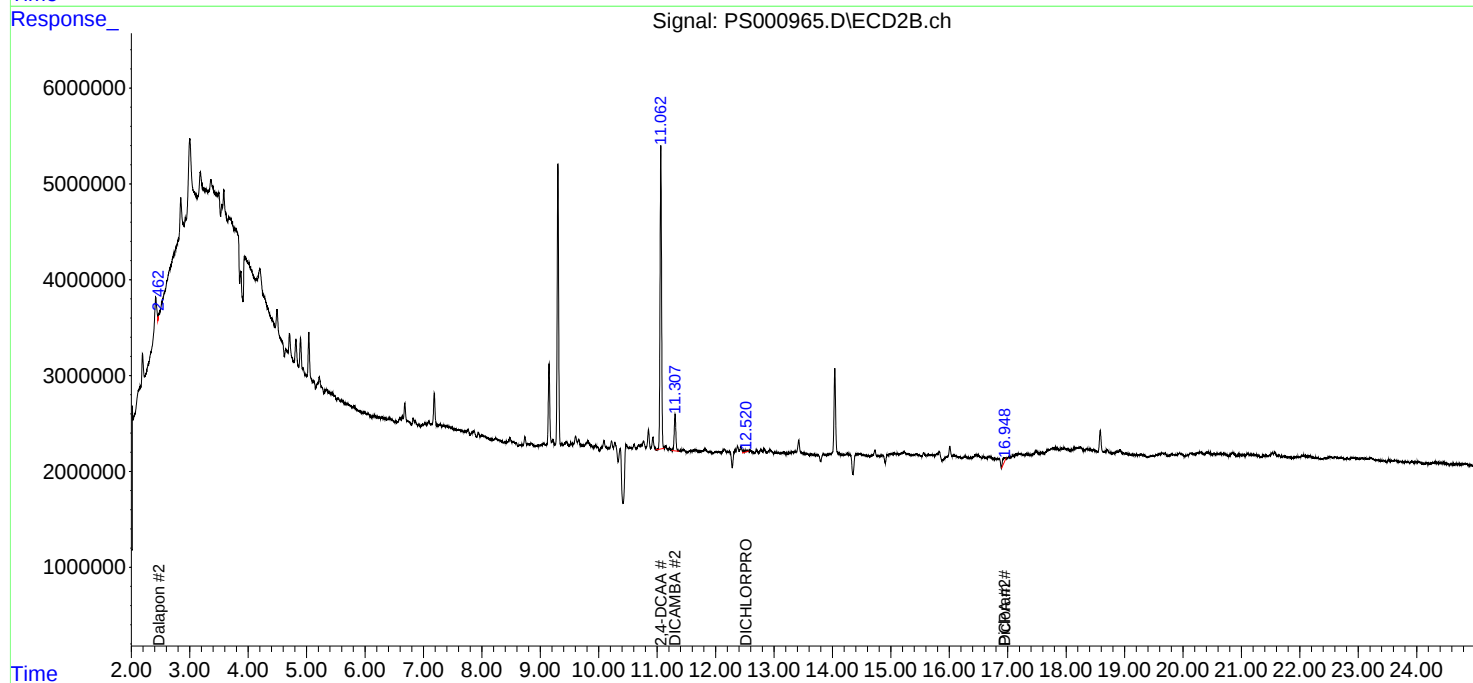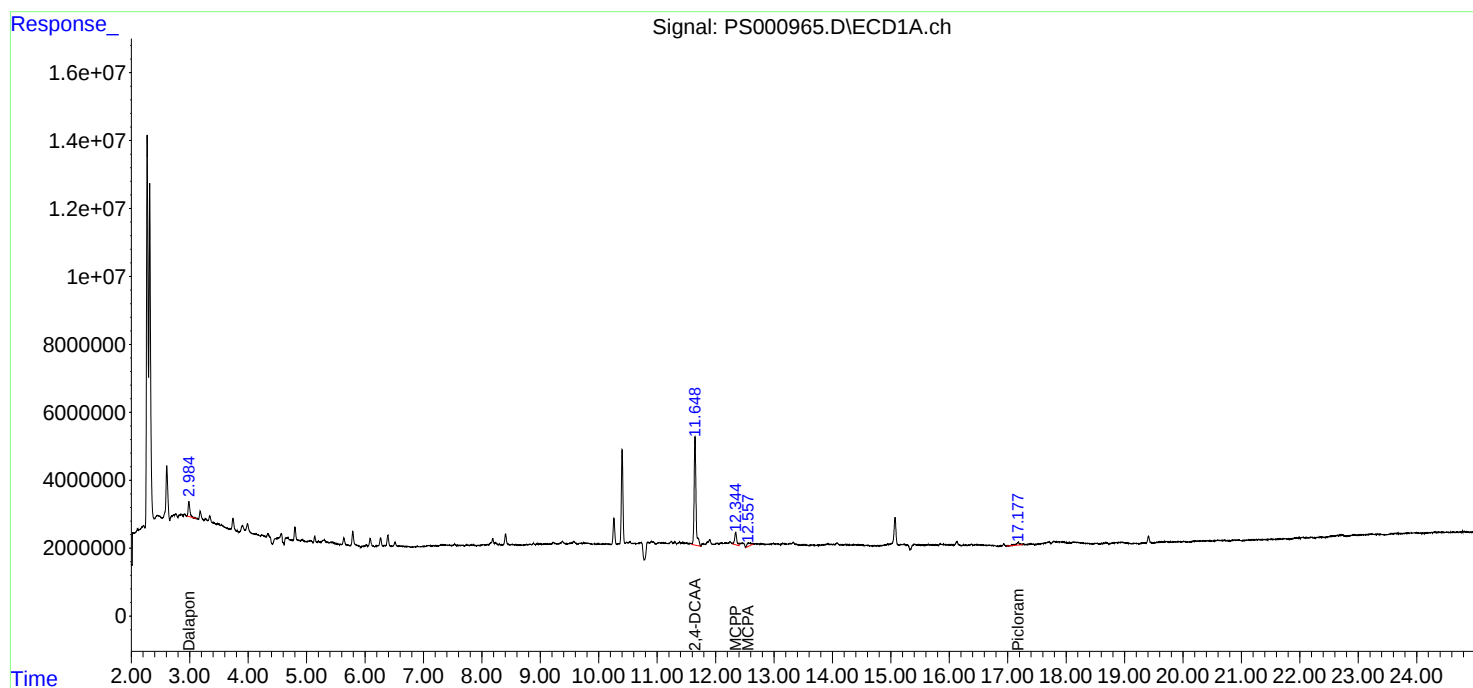


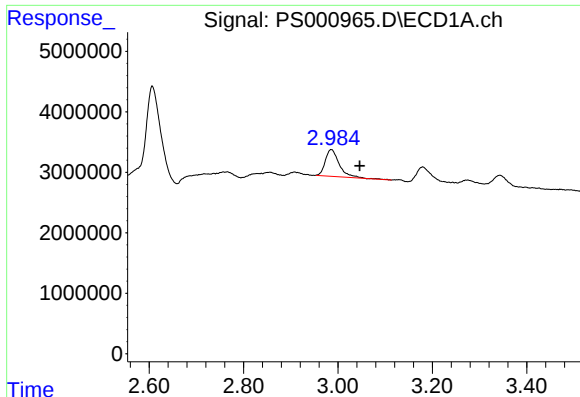

#1 Dalapon


R.T.: 2.986 min
Delta R.T.: -0.060 min
Response: 9156055
Conc: 34.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

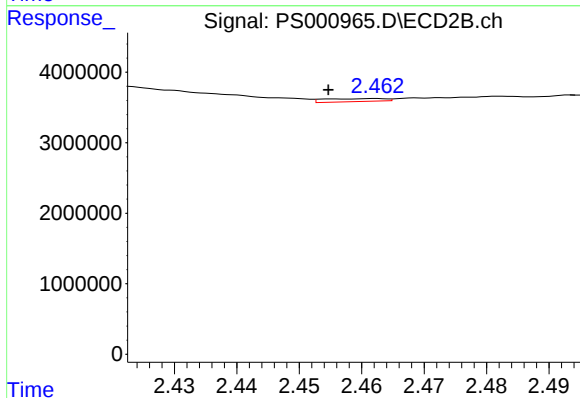


#1 Dalapon

R.T.: 2.462 min
Delta R.T.: 0.008 min
Response: 287325
Conc: 1.07 ng/ml

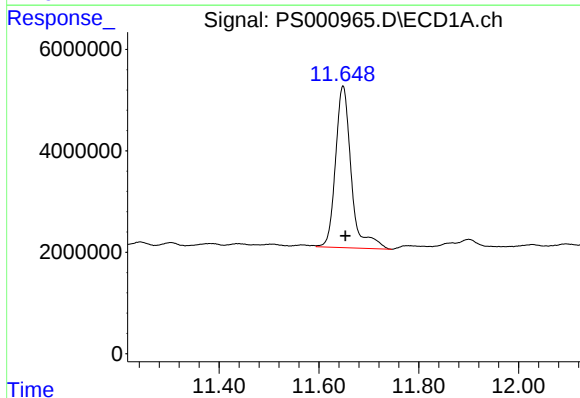


#4 2,4-DCAA

R.T.: 11.648 min
Delta R.T.: -0.005 min
Response: 69504732
Conc: 336.88 ng/ml

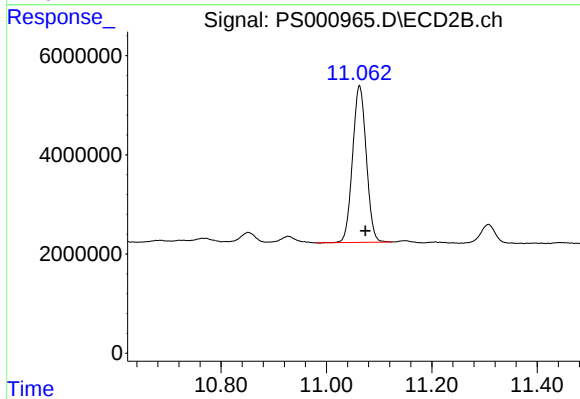

#4 2,4-DCAA


R.T.: 11.063 min
Delta R.T.: -0.011 min
Response: 57003259
Conc: 261.73 ng/ml

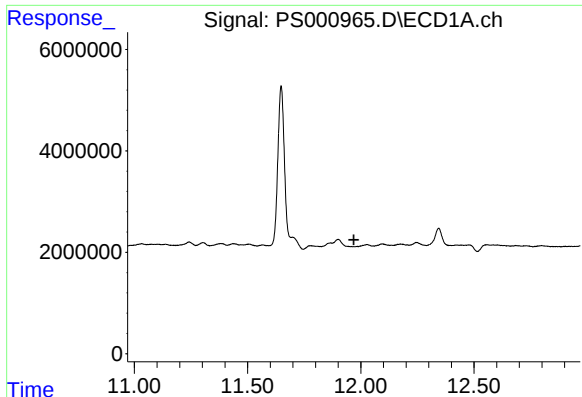

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.970 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

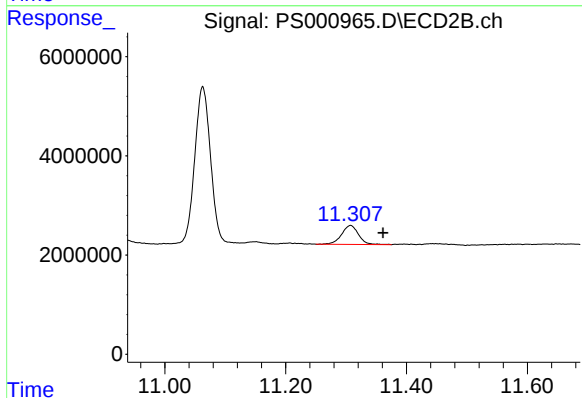


#5 DICAMBA

R.T.: 11.307 min
Delta R.T.: -0.054 min
Response: 7471184
Conc: 9.52 ng/ml

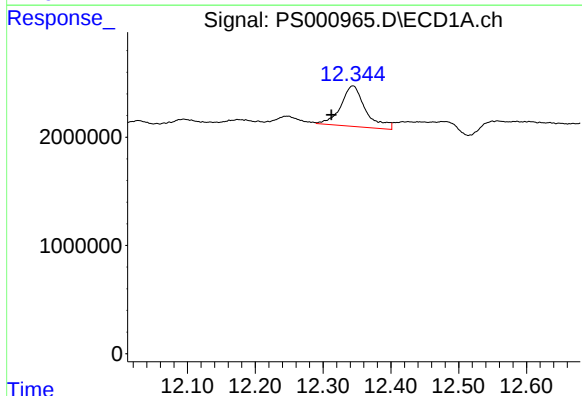


#6 MCP

R.T.: 12.344 min
Delta R.T.: 0.032 min
Response: 9468626
Conc: 17.24 ug/ml

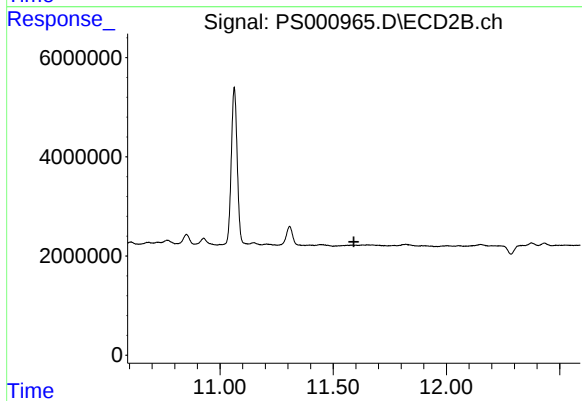

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

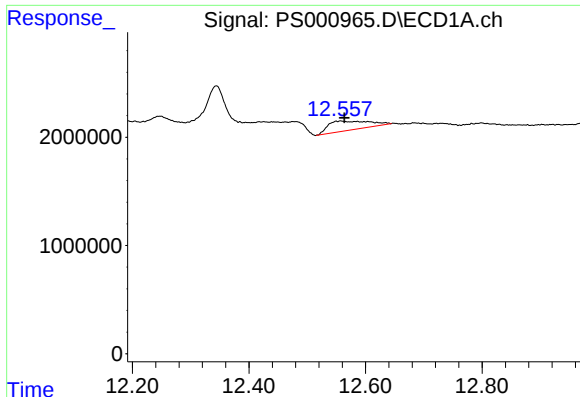

#7 MCPA


R.T.: 12.558 min
Delta R.T.: -0.006 min
Response: 4232630
Conc: 4.64 ug/ml

Instrument :
ECD_S
ClientSampleId :

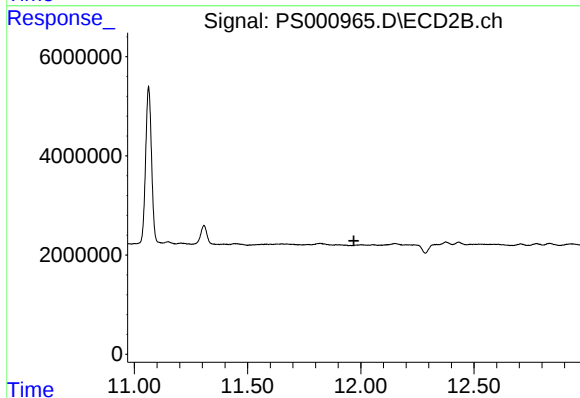


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.969 min
Response: 0
Conc: N.D.

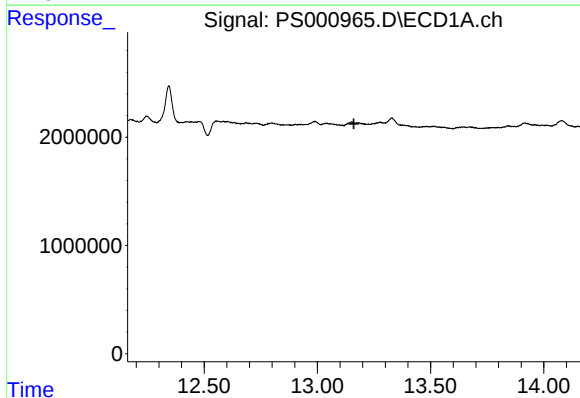


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

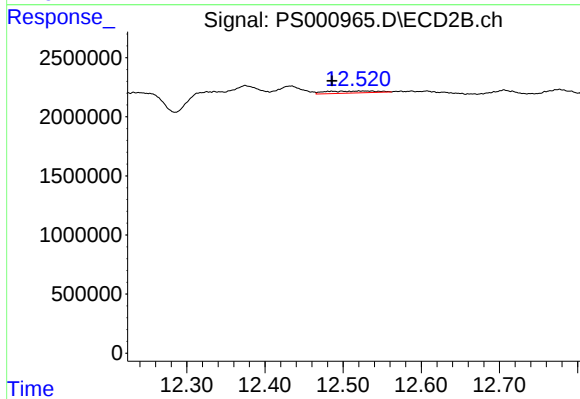

#8 DICHLORPROP


R.T.: 12.520 min
Delta R.T.: 0.035 min
Response: 780417
Conc: 3.86 ng/ml

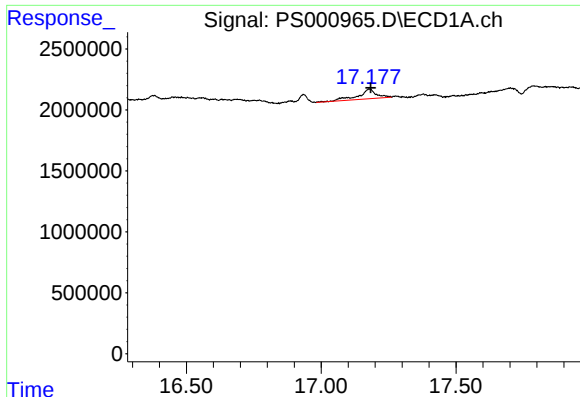

#15 Picloram


R.T.: 17.179 min
Delta R.T.: -0.005 min
Response: 3757015
Conc: 2.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

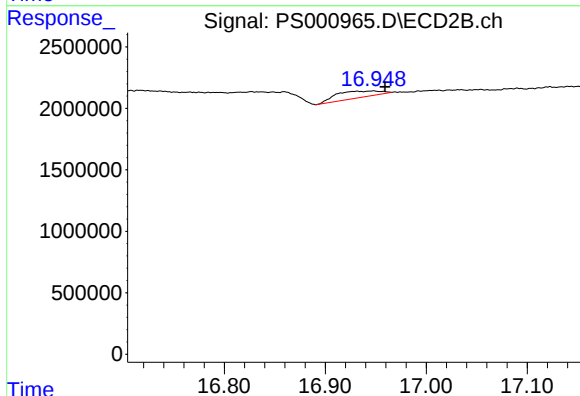


#15 Picloram

R.T.: 16.948 min
Delta R.T.: -0.011 min
Response: 1642985
Conc: 1.08 ng/ml

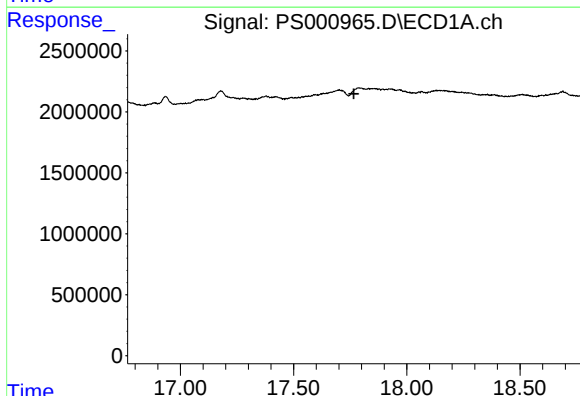

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.766 min
Response: 0
Conc: N.D.

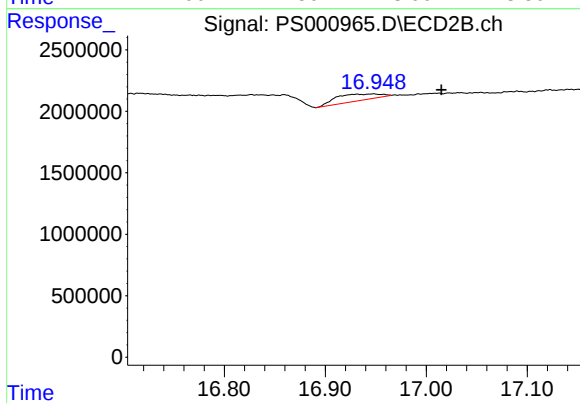

#16 DCPA

R.T.: 16.948 min
Delta R.T.: -0.067 min
Response: 1642985
Conc: 0.96 ng/ml