

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
 Data File : PS000970.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2018 05:52
 Operator : UA
 Sample : J3924-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 07:32:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.618	11.033	53210366	46352546	257.902	212.824
Target Compounds							
2) T	3,5-DICHL...	0.000	9.271	0	33824099	N.D.	114.988 #
6) T	MCP	12.312	0.000	3937669	0	7.169	N.D. #
15) T	Picloram	17.152	16.973	4986055	5478354	2.753	3.598 #
16) T	DCPA	0.000	16.973	0	5478354	N.D.	3.187 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
Data File : PS000970.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2018 05:52
Operator : UA
Sample : J3924-02
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 07:32:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

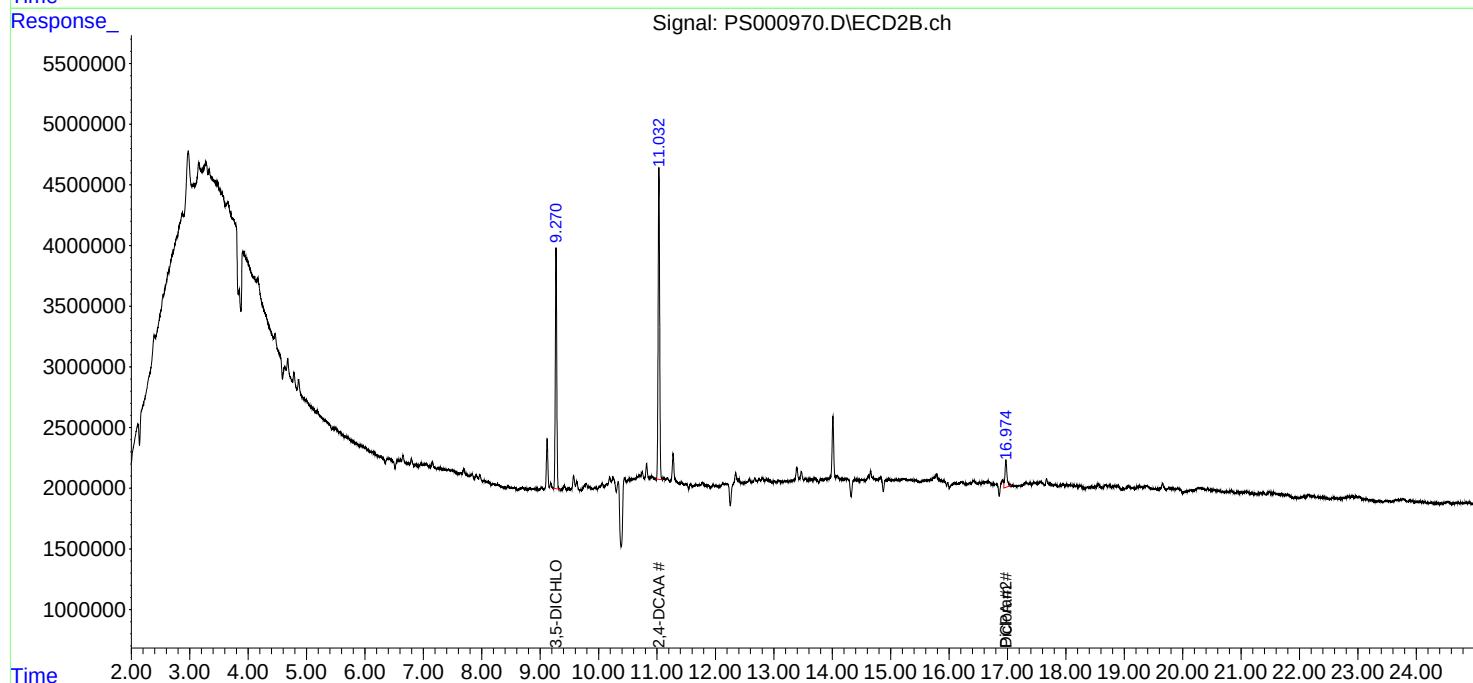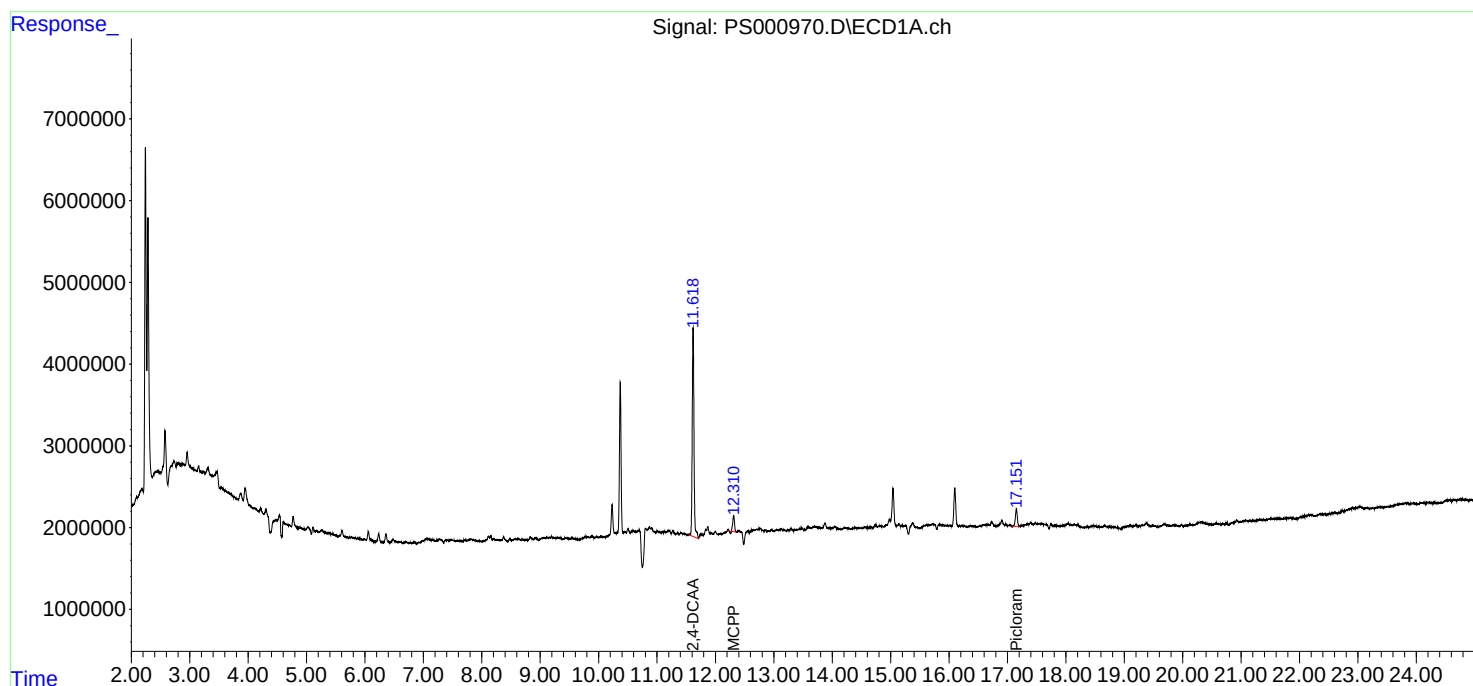


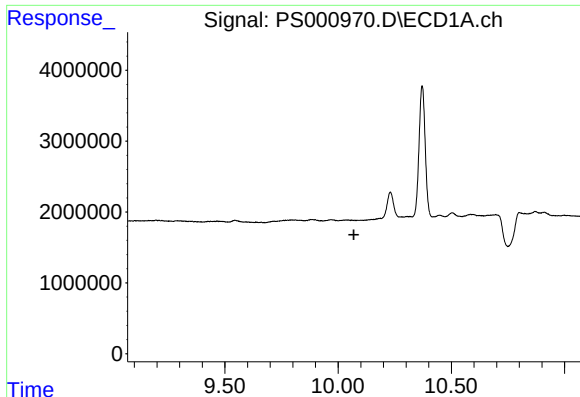

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

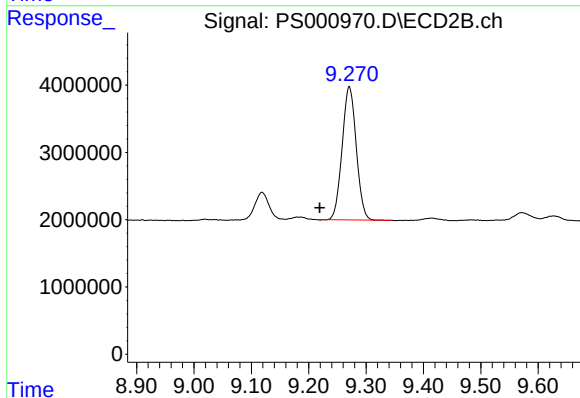


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.271 min
Delta R.T.: 0.051 min
Response: 33824099
Conc: 114.99 ng/ml

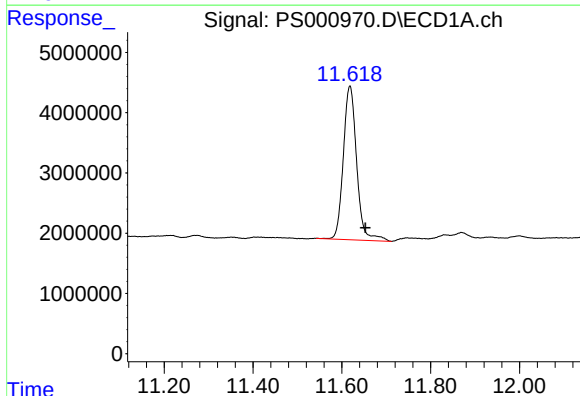


#4 2,4-DCAA

R.T.: 11.618 min
Delta R.T.: -0.035 min
Response: 53210366
Conc: 257.90 ng/ml

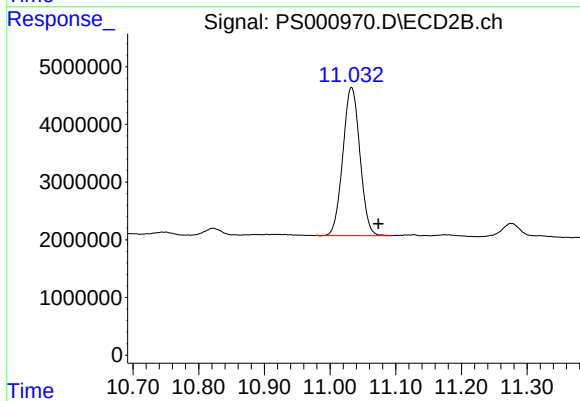

#4 2,4-DCAA


R.T.: 11.033 min
Delta R.T.: -0.041 min
Response: 46352546
Conc: 212.82 ng/ml

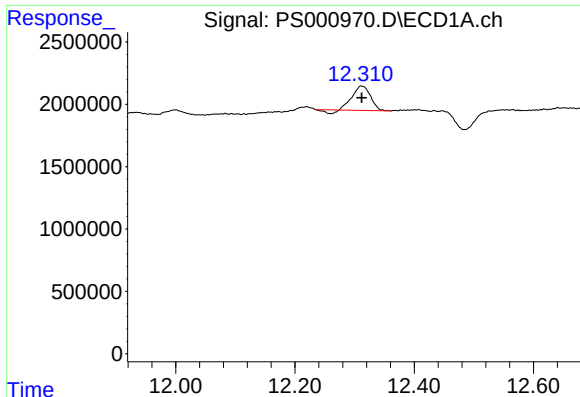

#6 MCP


R.T.: 12.312 min
Delta R.T.: 0.000 min
Response: 3937669
Conc: 7.17 ug/ml

Instrument :
ECD_S
ClientSampleId :

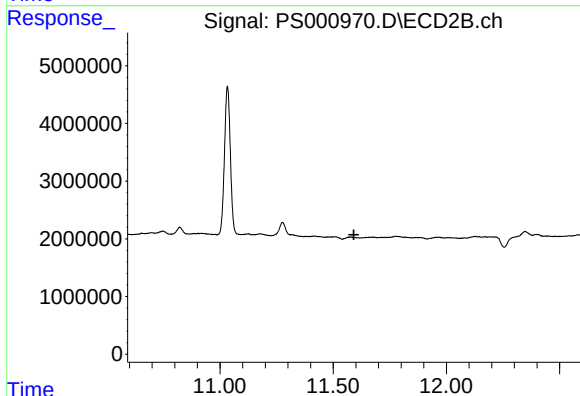


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

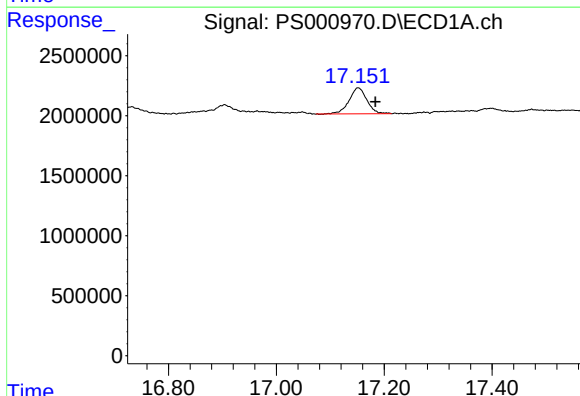


#15 Picloram

R.T.: 17.152 min
Delta R.T.: -0.032 min
Response: 4986055
Conc: 2.75 ng/ml

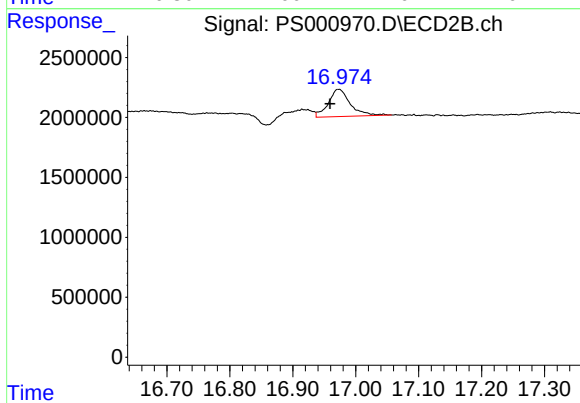

#15 Picloram


R.T.: 16.973 min
Delta R.T.: 0.014 min
Response: 5478354
Conc: 3.60 ng/ml

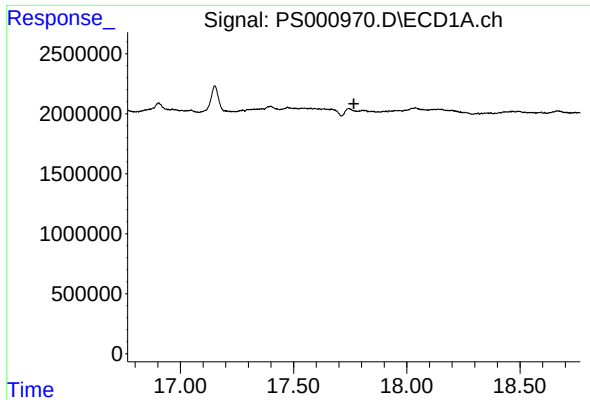

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.766 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

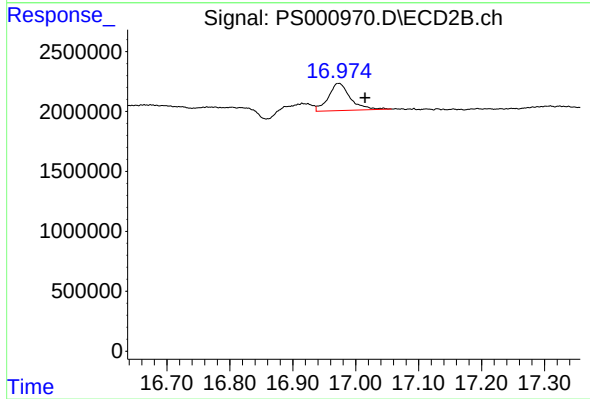

#16 DCPA

R.T.: 16.973 min
Delta R.T.: -0.042 min
Response: 5478354
Conc: 3.19 ng/ml