

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
 Data File : PS000977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2018 09:28
 Operator : UA
 Sample : J3926-02
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 13:35:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.652	11.067	59099928	51030195	286.448	234.302
Target Compounds							
1) T	Dalapon	2.988	2.426	3211851	1850840	11.962	6.870 #
2) T	3,5-DICHL...	0.000	9.153	0	9065976	N.D.	30.821 #
5) T	DICAMBA	0.000	11.311	0	6932244	N.D.	8.832 #
6) T	MCP	12.348	0.000	5910396	0	10.760	N.D. #
8) T	DICHLORPROP	0.000	12.435	0	1103099	N.D.	5.461 #
15) T	Picloram	0.000	16.953	0	3183718	N.D.	2.091 #
16) T	DCPA	0.000	17.009	0	1825822	N.D.	1.062 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071118\
Data File : PS000977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2018 09:28
Operator : UA
Sample : J3926-02
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 13:35:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

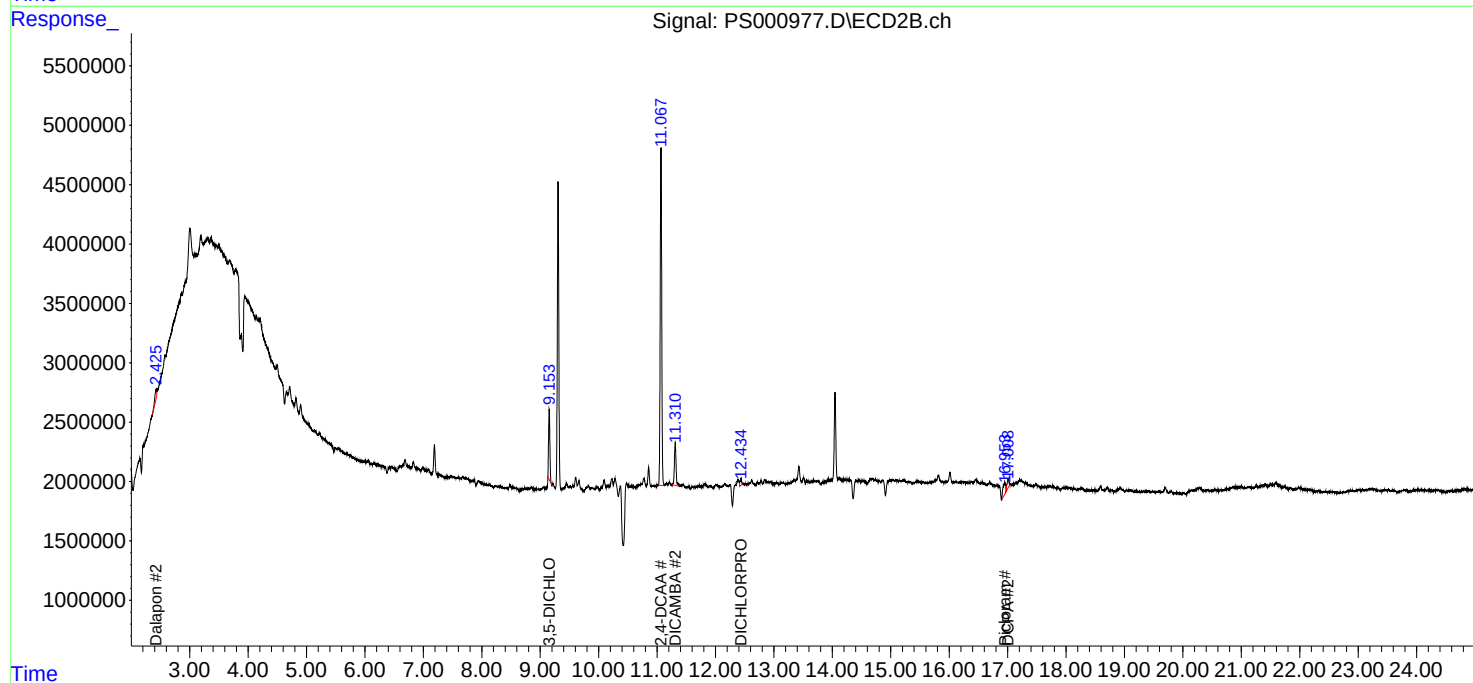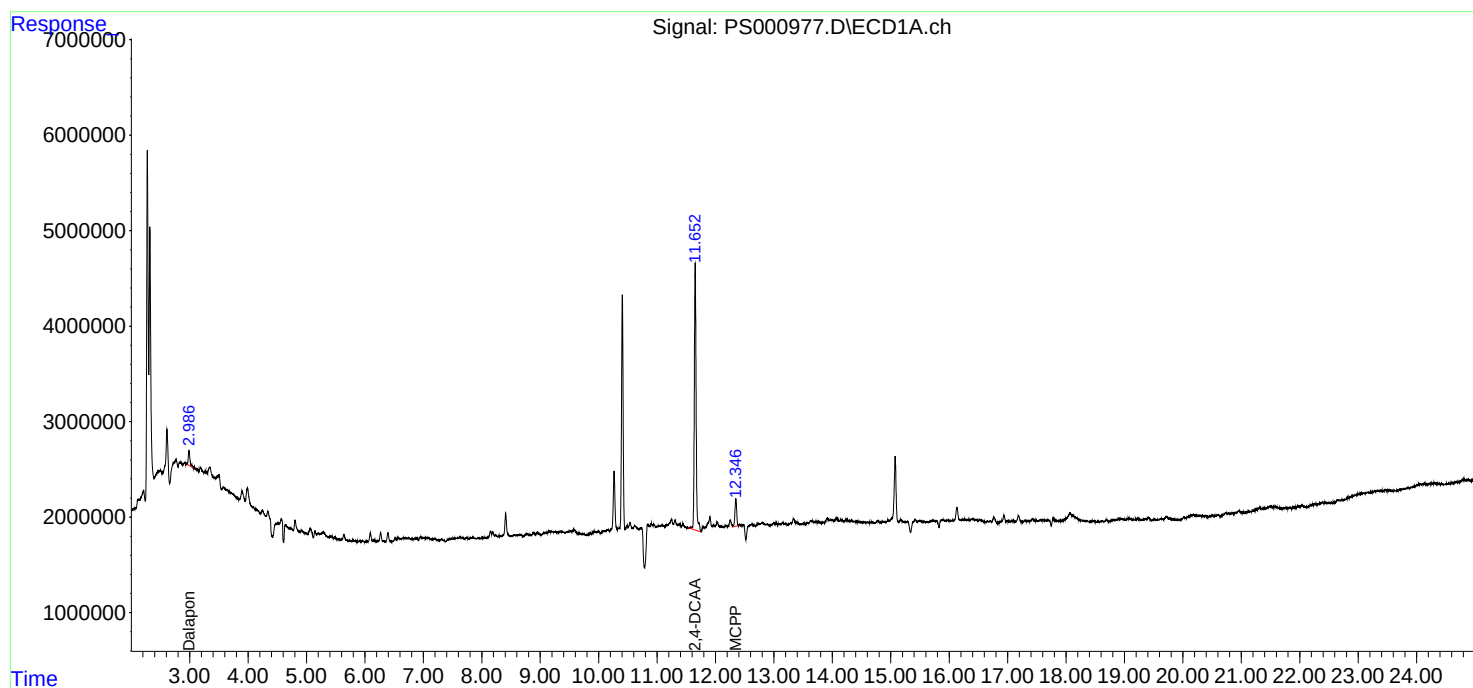


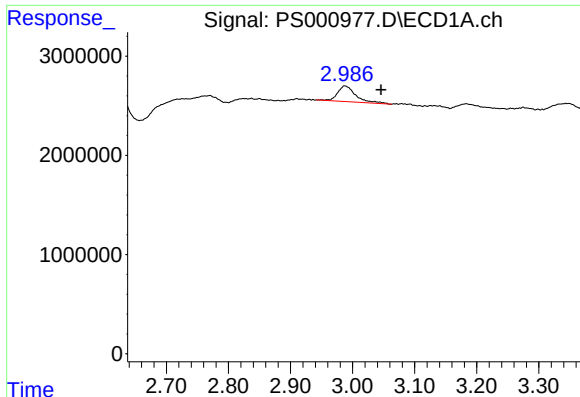

#1 Dalapon


R.T.: 2.988 min
Delta R.T.: -0.058 min
Response: 3211851
Conc: 11.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

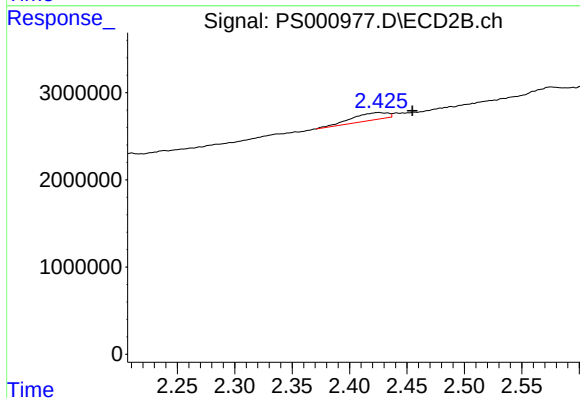


#1 Dalapon

R.T.: 2.426 min
Delta R.T.: -0.029 min
Response: 1850840
Conc: 6.87 ng/ml

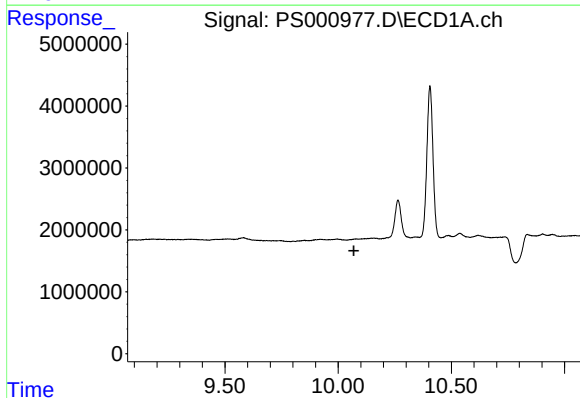


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

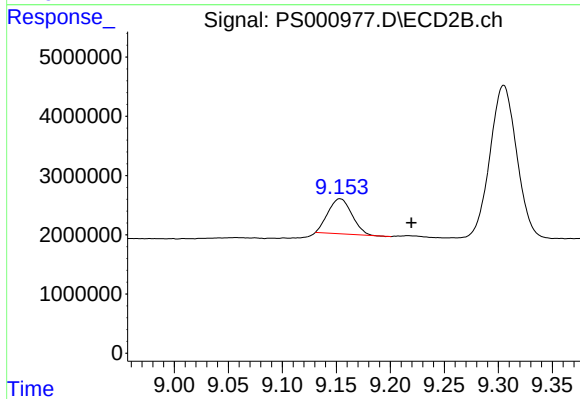

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.153 min
Delta R.T.: -0.066 min
Response: 9065976
Conc: 30.82 ng/ml

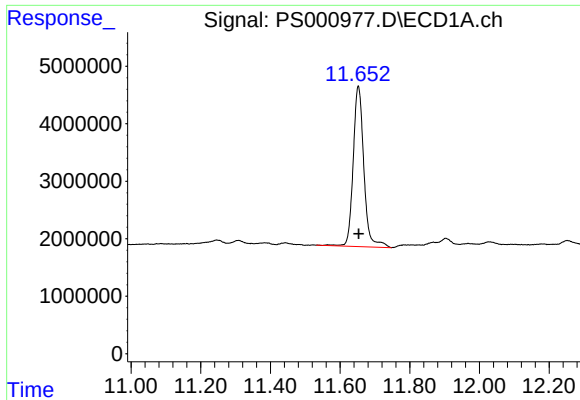

#4 2,4-DCAA


R.T.: 11.652 min
Delta R.T.: -0.001 min
Response: 59099928
Conc: 286.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

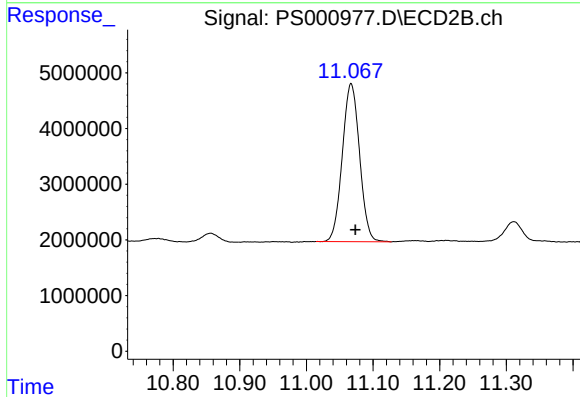


#4 2,4-DCAA

R.T.: 11.067 min
Delta R.T.: -0.006 min
Response: 51030195
Conc: 234.30 ng/ml

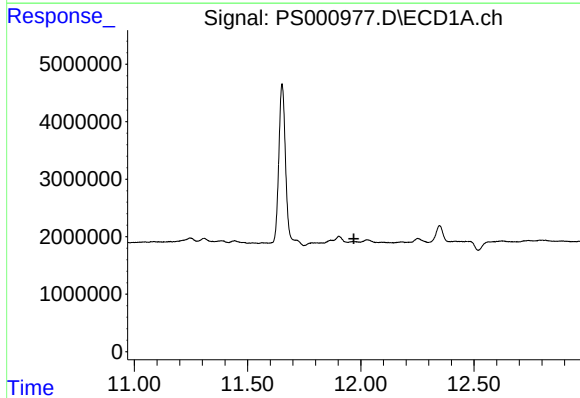


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.970 min
Response: 0
Conc: N.D.

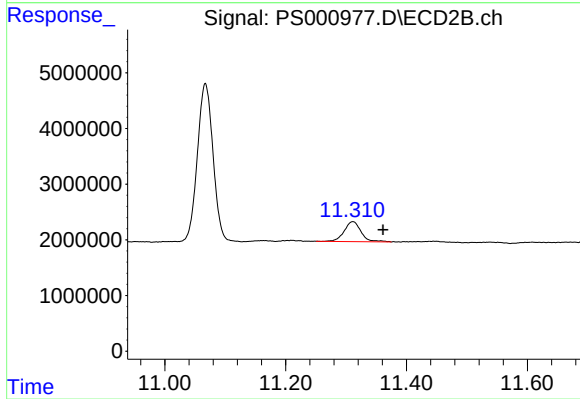

#5 DICAMBA


R.T.: 11.311 min
Delta R.T.: -0.050 min
Response: 6932244
Conc: 8.83 ng/ml

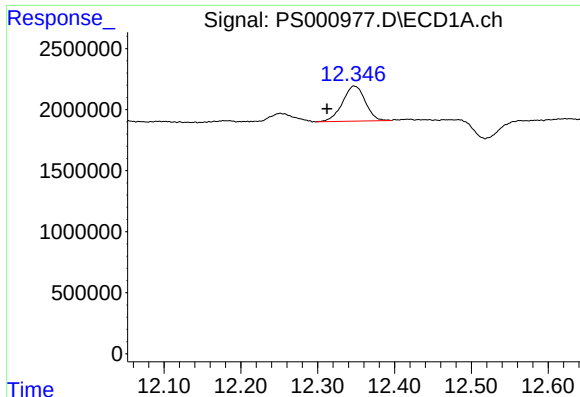

#6 MCP


R.T.: 12.348 min
Delta R.T.: 0.036 min
Response: 5910396
Conc: 10.76 ug/ml

Instrument :
ECD_S
ClientSampleId :

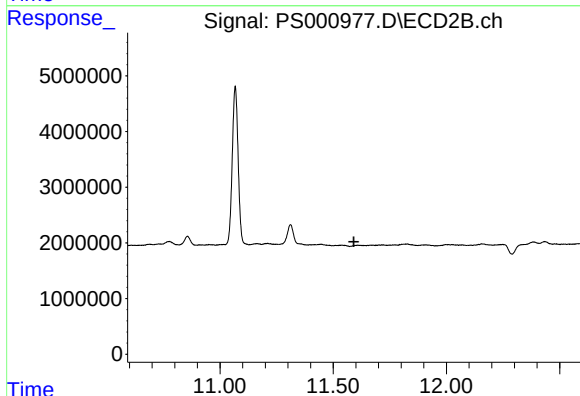


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

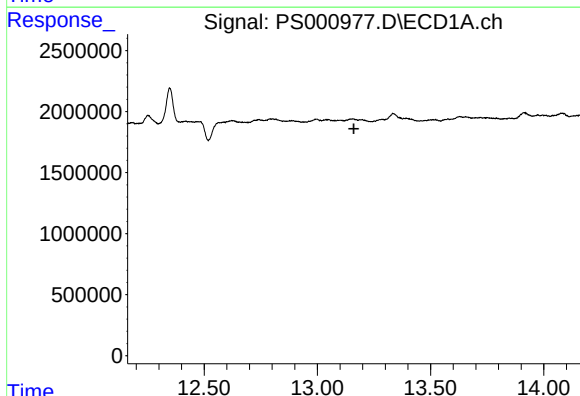


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

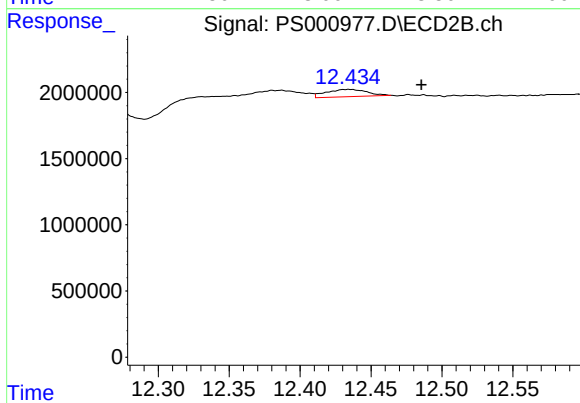

#8 DICHLORPROP


R.T.: 12.435 min
Delta R.T.: -0.051 min
Response: 1103099
Conc: 5.46 ng/ml

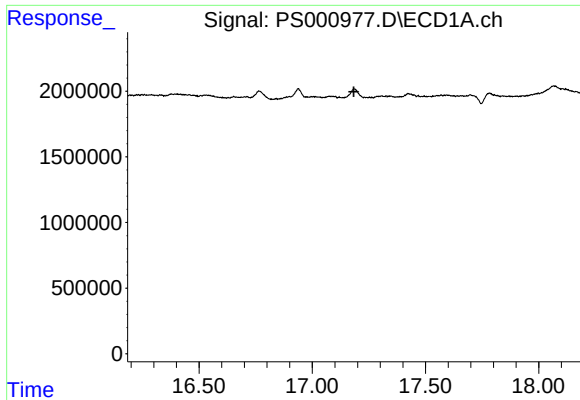

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

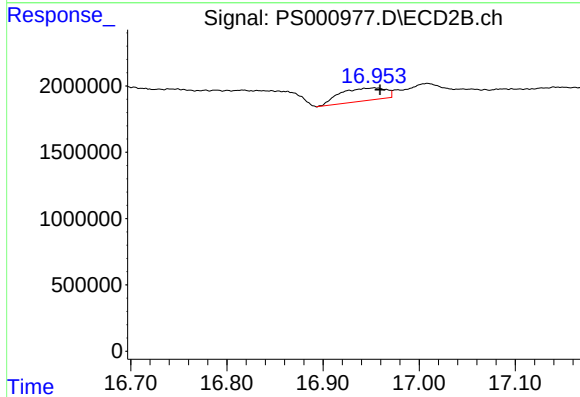


#15 Picloram

R.T.: 16.953 min
Delta R.T.: -0.006 min
Response: 3183718
Conc: 2.09 ng/ml

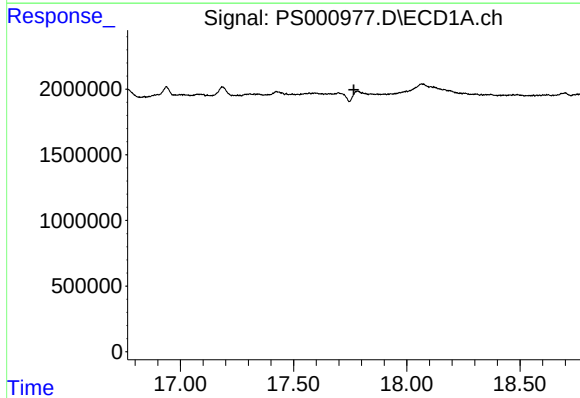

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.766 min
Response: 0
Conc: N.D.

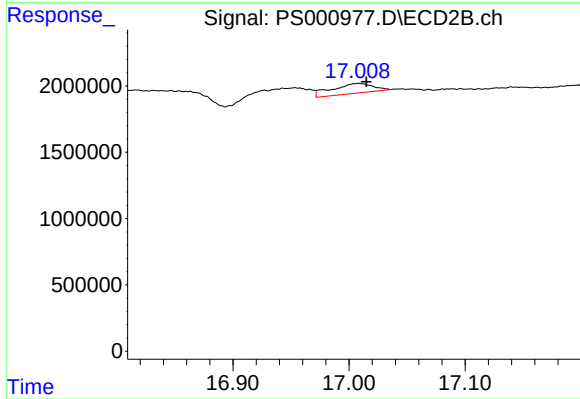

#16 DCPA

R.T.: 17.009 min
Delta R.T.: -0.006 min
Response: 1825822
Conc: 1.06 ng/ml