

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071119\
 Data File : PS005465.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2019 10:03
 Operator : SM\AJ
 Sample : PB121263TB
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 03:12:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.571	5.283	806.0E6	526.4E6	549.090	525.107
Target Compounds							
1) T	Dalapon	2.082	0.000	47250690	0	25.634	N.D. #
2) T	3,5-DICHL...	0.000	4.601	0	103.4E6	N.D.	78.405
3) T	4-Nitroph...	5.376	0.000	15003638	0	20.715	N.D. #
5) T	DICAMBA	5.671	0.000	11558922	0	2.026	N.D. #
7) T	MCPA	6.063	5.674	11210633	17161278	1.785	4.236 #
8) T	DICHLORPROP	0.000	5.977	0	21395185	N.D.	22.159
11) T	2,4,5-TP ...	0.000	6.937	0	20977083	N.D.	3.939
13) T	2,4-DB	8.226	7.853	111.1E6	130.7E6	95.677	200.268 #
15) T	Picloram	9.111	9.102	71945879	103.3E6	6.261	13.691 #
16) T	DCPA	0.000	9.102	0	103.3E6	N.D.	15.177



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071119\
Data File : PS005465.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2019 10:03
Operator : SM\AJ
Sample : PB121263TB
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 03:12:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

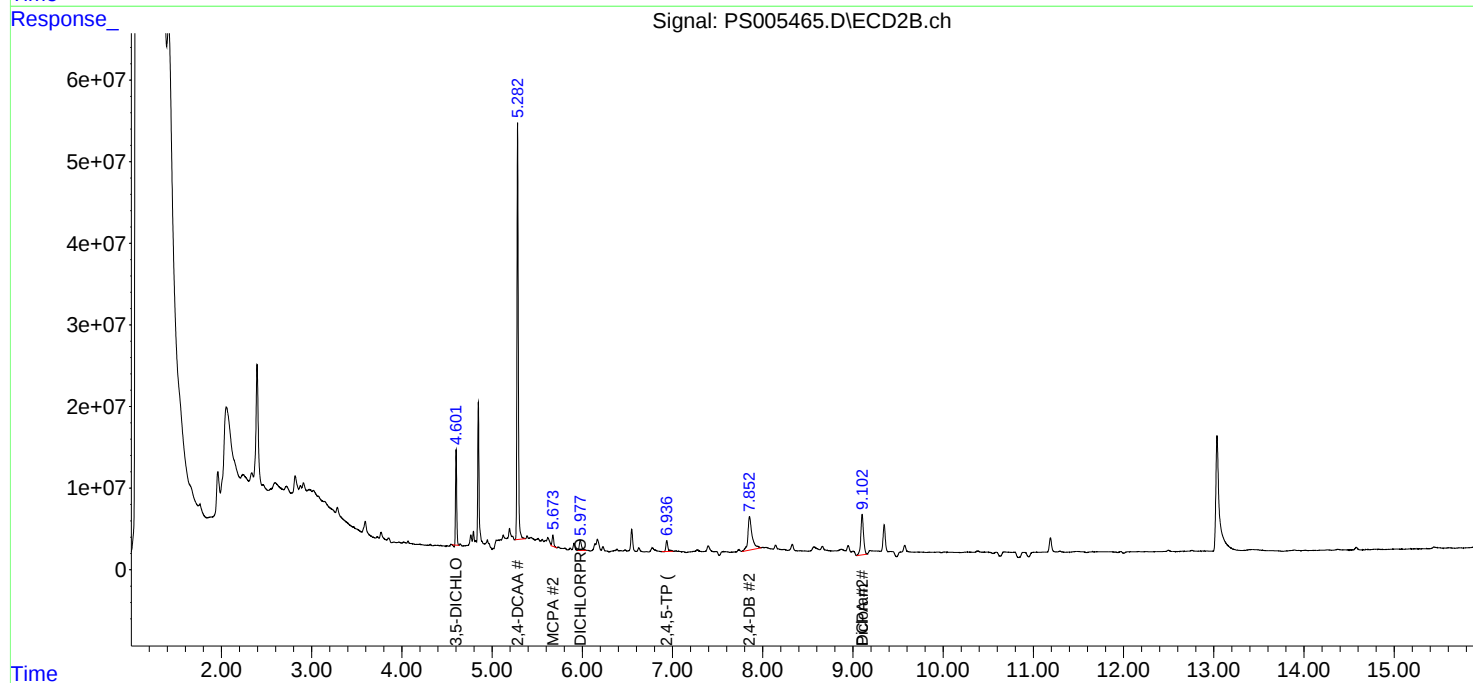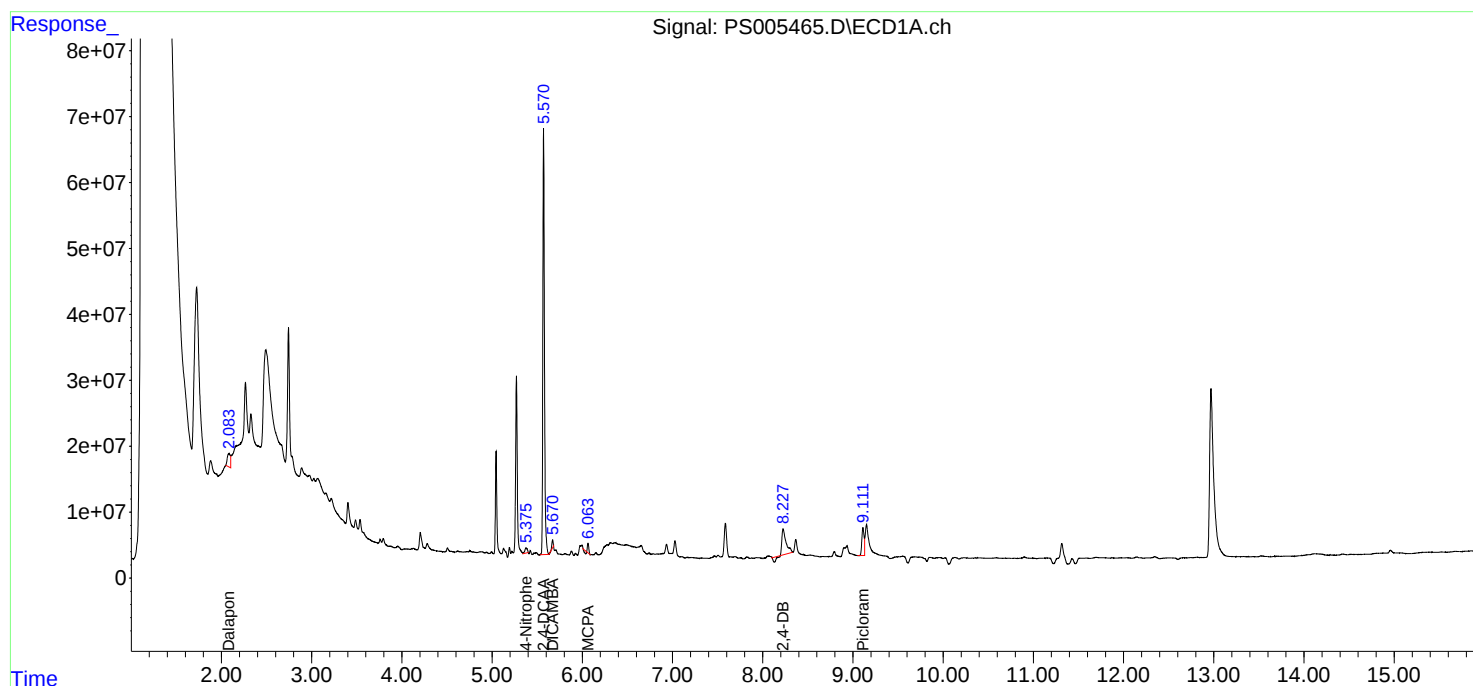


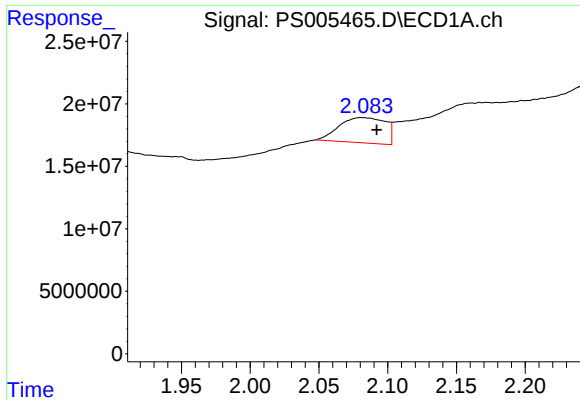

#1 Dalapon


R.T.: 2.082 min
Delta R.T.: -0.010 min
Response: 47250690
Conc: 25.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

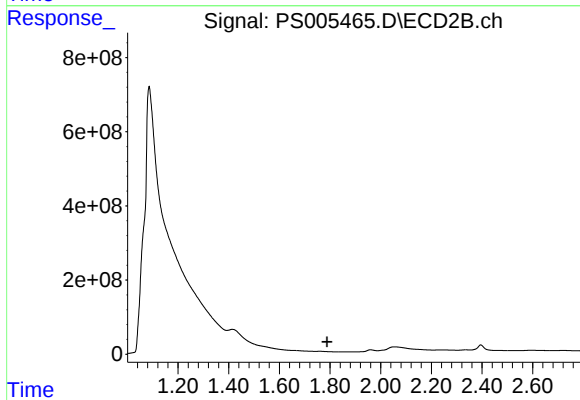


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

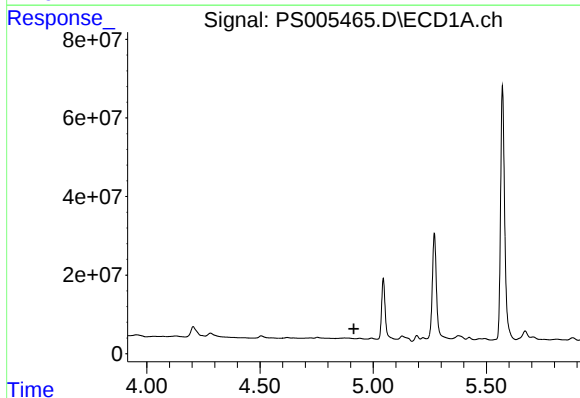


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

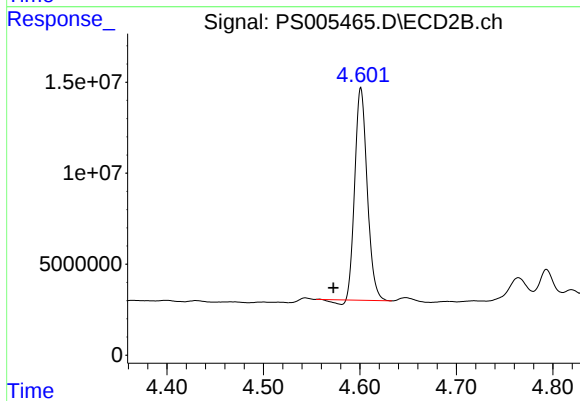

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.601 min
Delta R.T.: 0.029 min
Response: 103393628
Conc: 78.41 ng/ml

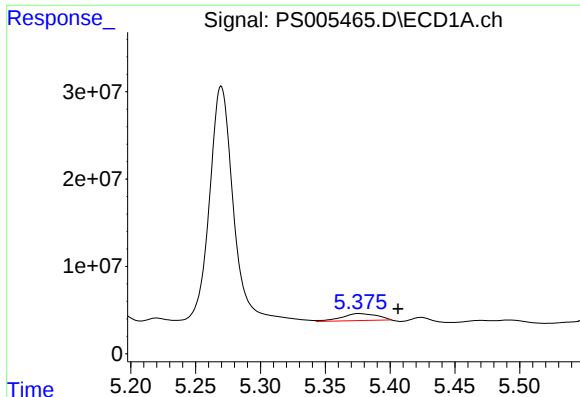

#3 4-Nitrophenol


R.T.: 5.376 min
Delta R.T.: -0.030 min
Response: 15003638
Conc: 20.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

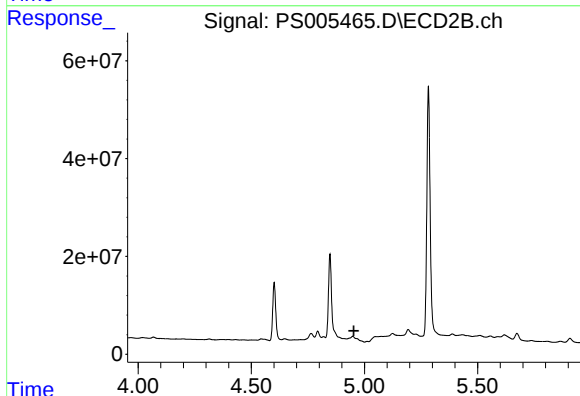


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

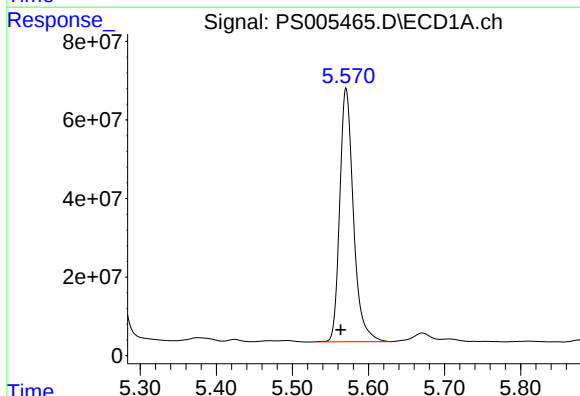


#4 2,4-DCAA

R.T.: 5.571 min
Delta R.T.: 0.007 min
Response: 806004857
Conc: 549.09 ng/ml

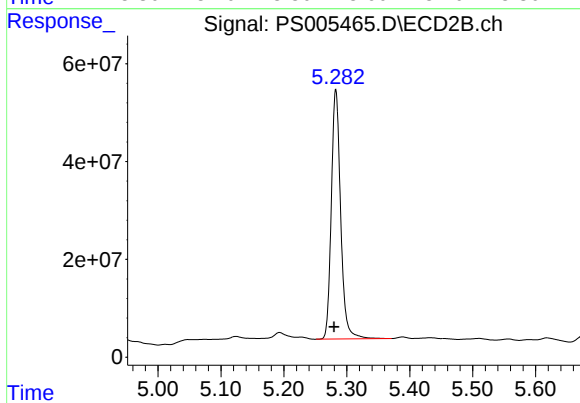

#4 2,4-DCAA


R.T.: 5.283 min
Delta R.T.: 0.003 min
Response: 526350710
Conc: 525.11 ng/ml

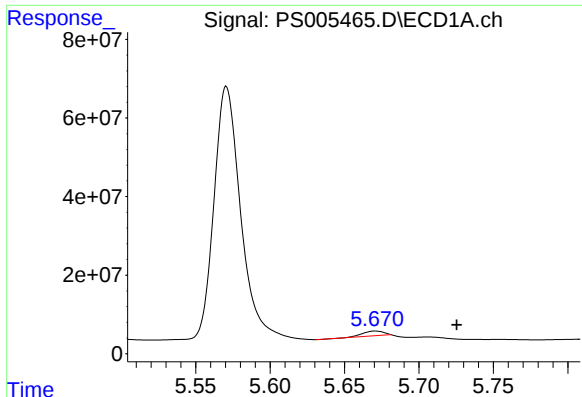

#5 DICAMBA


R.T.: 5.671 min
Delta R.T.: -0.055 min
Response: 11558922
Conc: 2.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

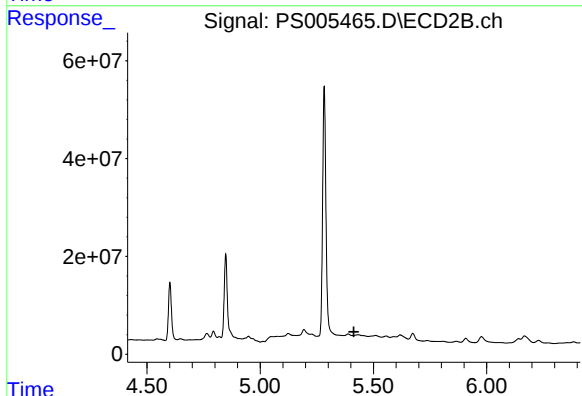


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.414 min
Response: 0
Conc: N.D.

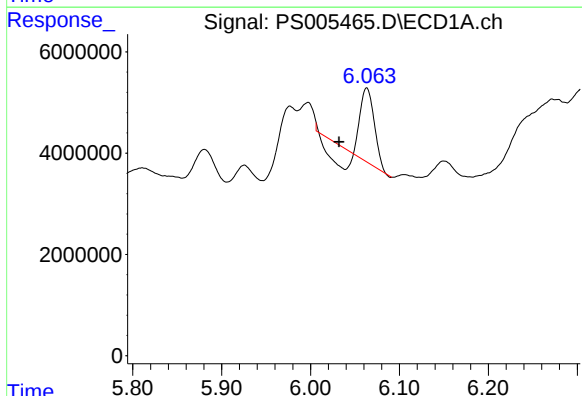


#7 MCPA

R.T.: 6.063 min
Delta R.T.: 0.031 min
Response: 11210633
Conc: 1.79 ug/ml

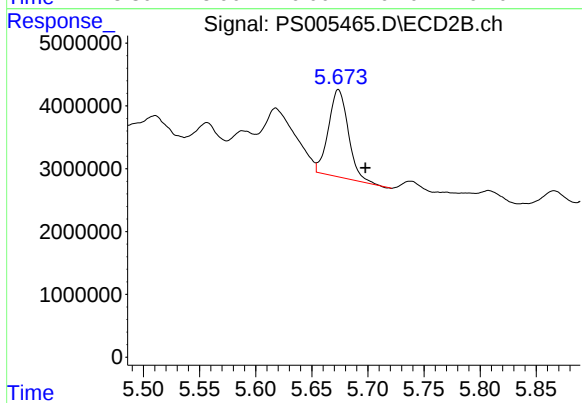

#7 MCPA


R.T.: 5.674 min
Delta R.T.: -0.024 min
Response: 17161278
Conc: 4.24 ug/ml

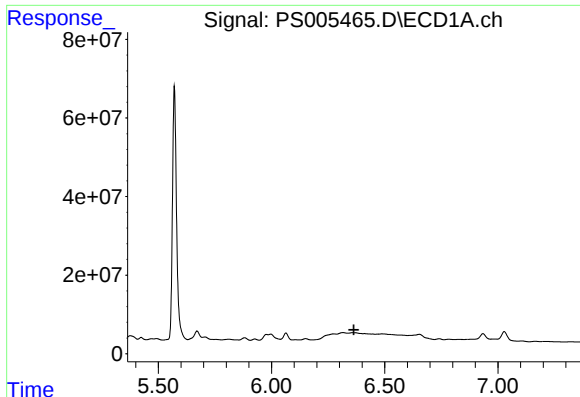

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

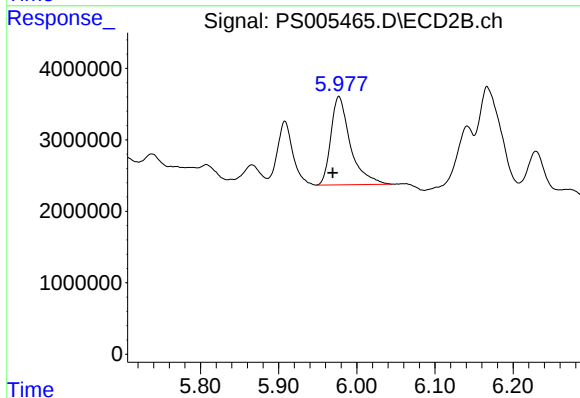


#8 DICHLORPROP

R.T.: 5.977 min
Delta R.T.: 0.008 min
Response: 21395185
Conc: 22.16 ng/ml

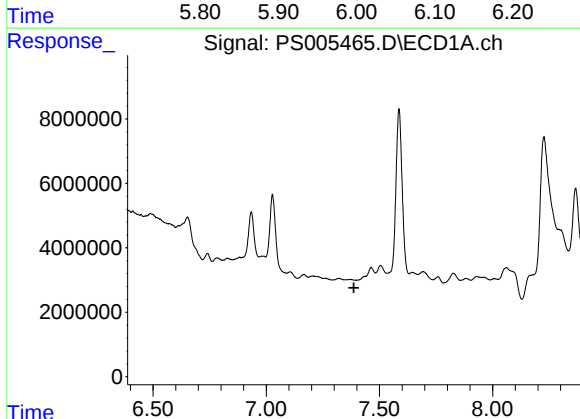


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

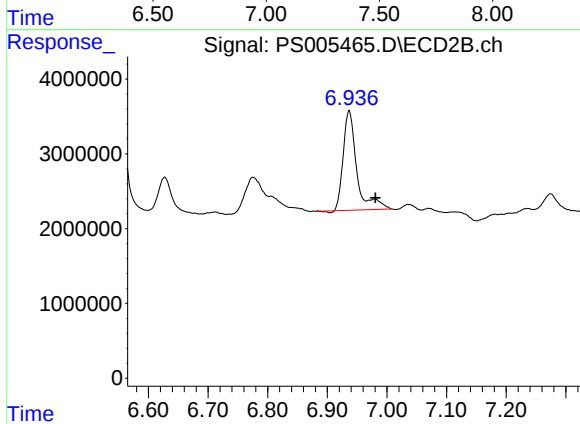

#11 2,4,5-TP (SILVEX)


R.T.: 6.937 min
Delta R.T.: -0.044 min
Response: 20977083
Conc: 3.94 ng/ml

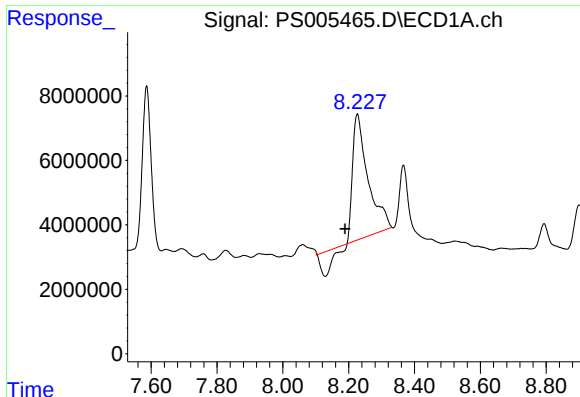

#13 2,4-DB


R.T.: 8.226 min
Delta R.T.: 0.037 min
Response: 111132938
Conc: 95.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

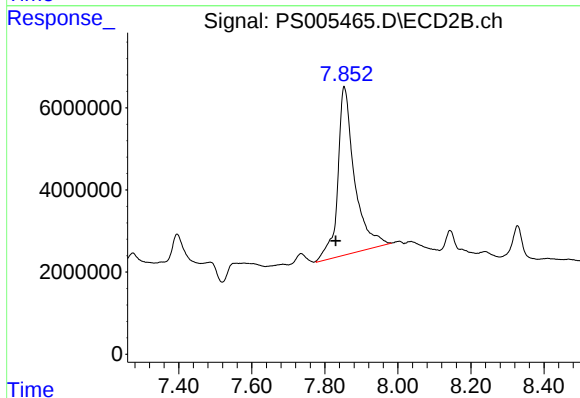


#13 2,4-DB

R.T.: 7.853 min
Delta R.T.: 0.024 min
Response: 130745507
Conc: 200.27 ng/ml

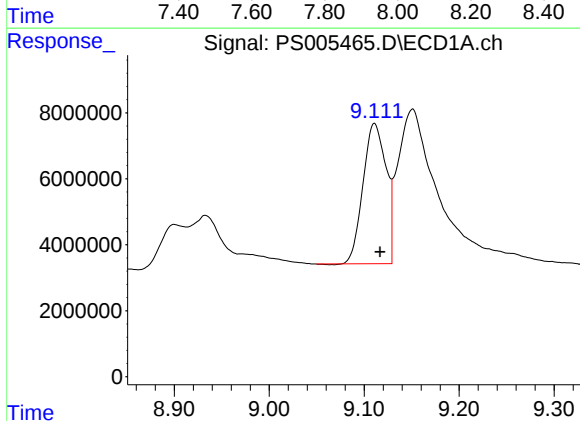


#15 Picloram

R.T.: 9.111 min
Delta R.T.: -0.006 min
Response: 71945879
Conc: 6.26 ng/ml

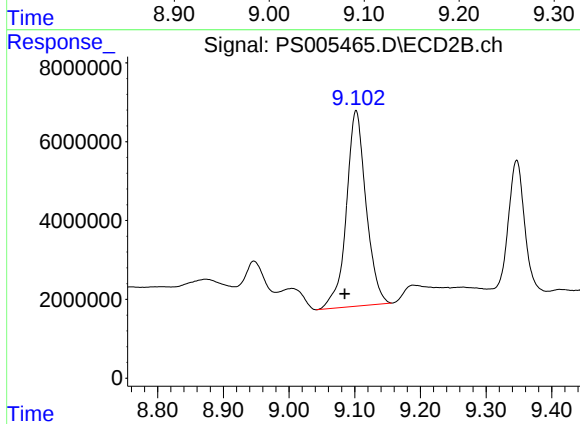

#15 Picloram


R.T.: 9.102 min
Delta R.T.: 0.017 min
Response: 103316320
Conc: 13.69 ng/ml

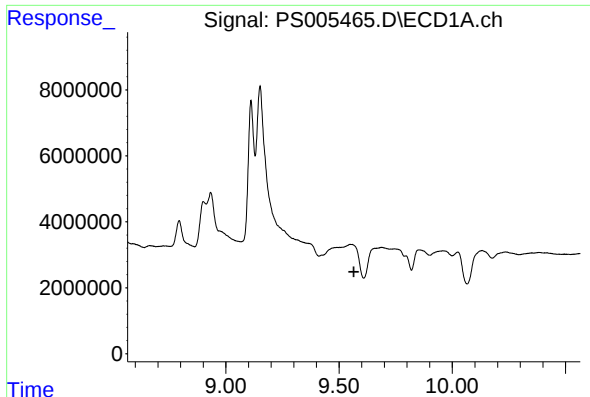

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

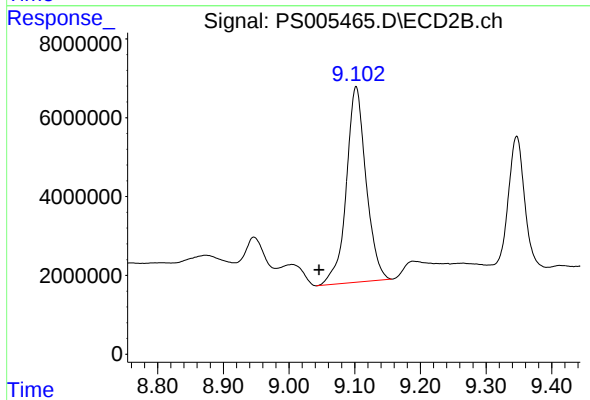

#16 DCPA

R.T.: 9.102 min
Delta R.T.: 0.056 min
Response: 103316320
Conc: 15.18 ng/ml