

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071119\
 Data File : PS005466.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2019 10:25
 Operator : SM\AJ
 Sample : K3632-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 03:13:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.596	5.312	496.4E6	304.8E6	338.203	304.072
Target Compounds							
1) T	Dalapon	2.104	0.000	24649202	0	13.372	N.D. #
2) T	3,5-DICHL...	0.000	4.631	0	139.1E6	N.D.	105.493
7) T	MCPA	5.992	0.000	11986631	0	1.909	N.D. #
8) T	DICHLORPROP	0.000	6.003	0	15378580	N.D.	15.927
9) T	2,4-D	0.000	6.195	0	24708431	N.D.	22.154
10) T	Pentachlo...	0.000	6.576	0	29450072	N.D.	2.291
11) T	2,4,5-TP ...	0.000	6.965	0	46933261	N.D.	8.813
12) T	2,4,5-T	7.615	0.000	130.4E6	0	16.202	N.D. #
15) T	Picloram	9.175	9.130	32210772	13644575	2.803	1.808 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071119\
Data File : PS005466.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2019 10:25
Operator : SM\AJ
Sample : K3632-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 03:13:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

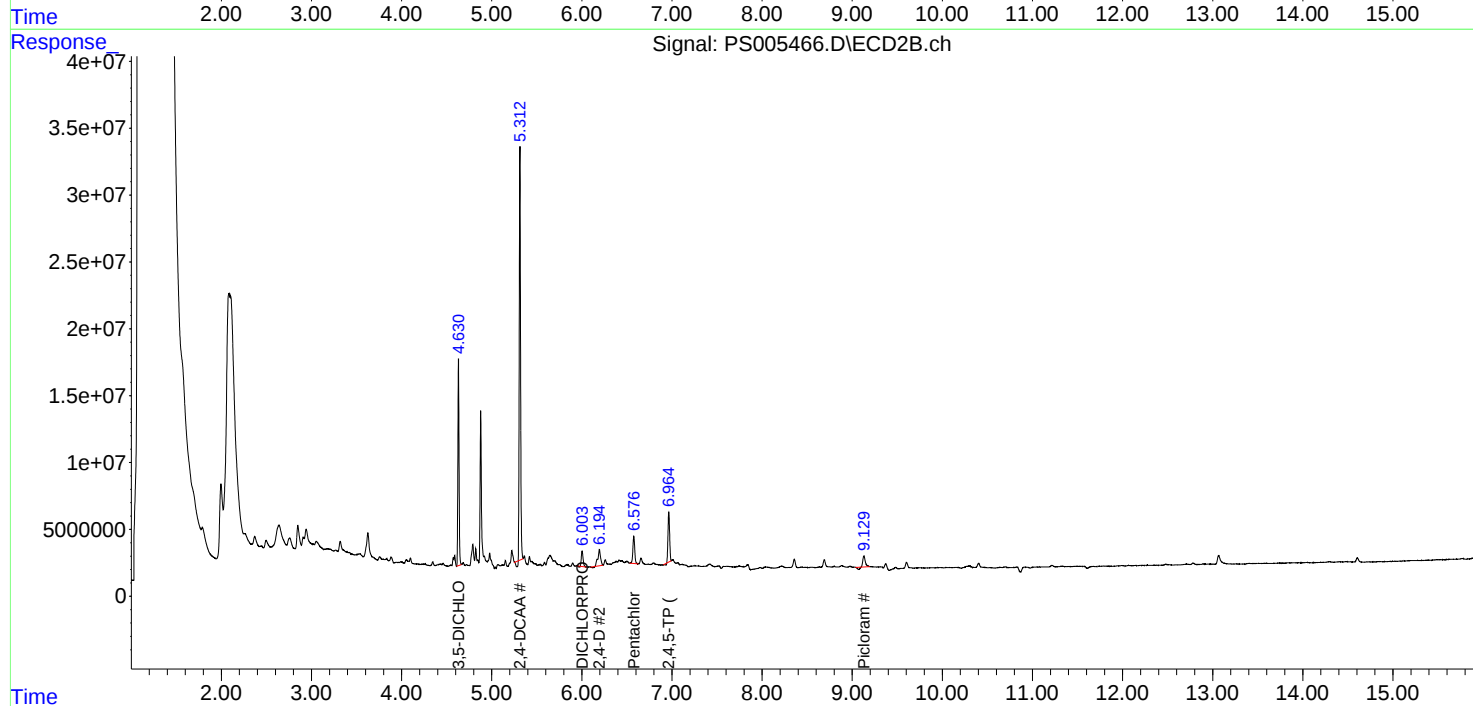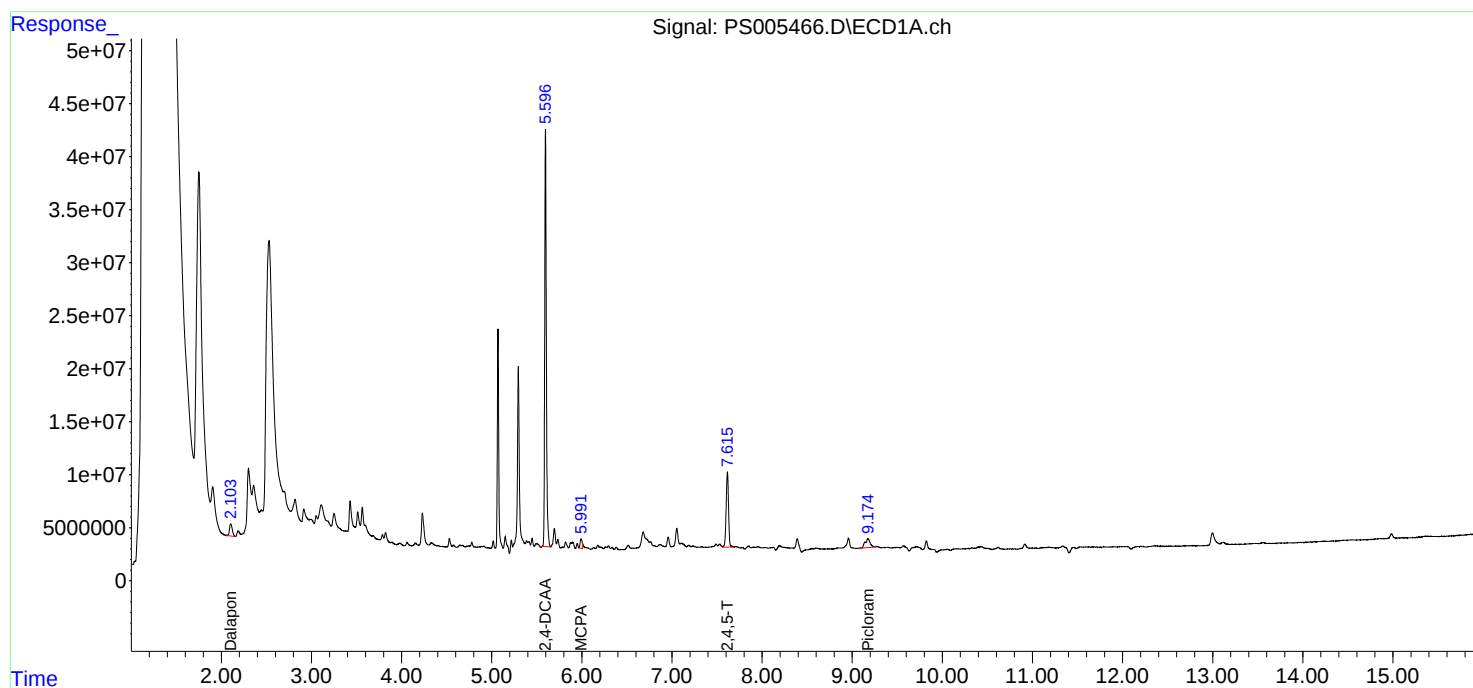


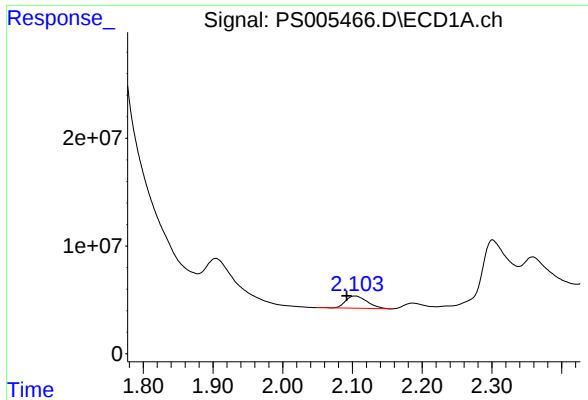

#1 Dalapon


R.T.: 2.104 min
Delta R.T.: 0.012 min
Response: 24649202
Conc: 13.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

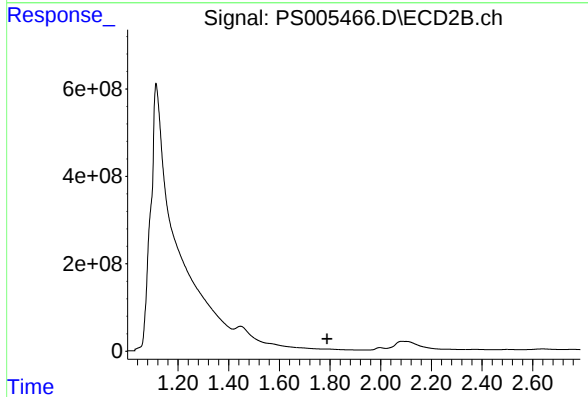


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

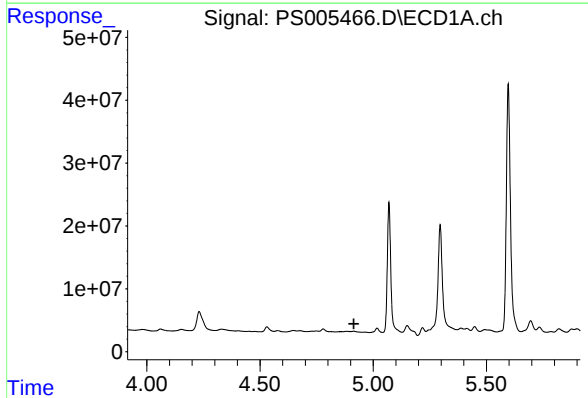


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

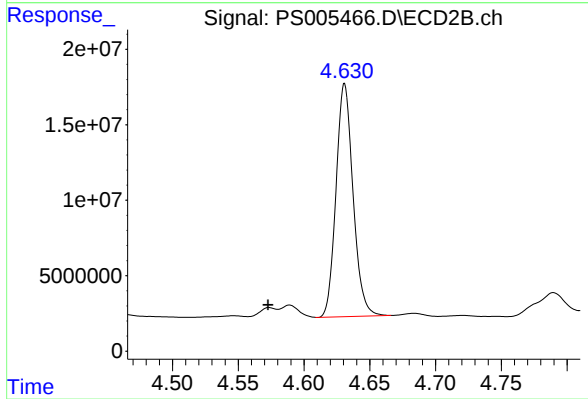

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.631 min
Delta R.T.: 0.058 min
Response: 139114569
Conc: 105.49 ng/ml

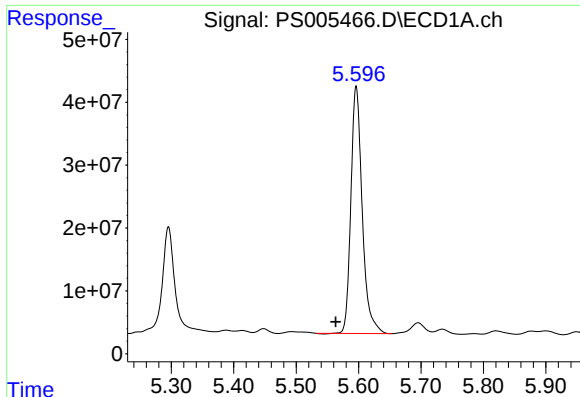

#4 2,4-DCAA


R.T.: 5.596 min
Delta R.T.: 0.033 min
Response: 496445702
Conc: 338.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

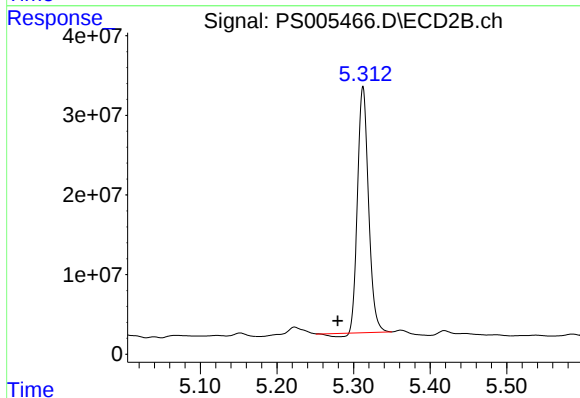


#4 2,4-DCAA

R.T.: 5.312 min
Delta R.T.: 0.033 min
Response: 304792672
Conc: 304.07 ng/ml

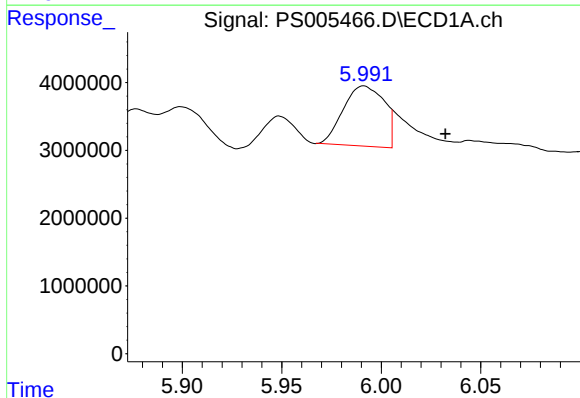


#7 MCPA

R.T.: 5.992 min
Delta R.T.: -0.040 min
Response: 11986631
Conc: 1.91 ug/ml

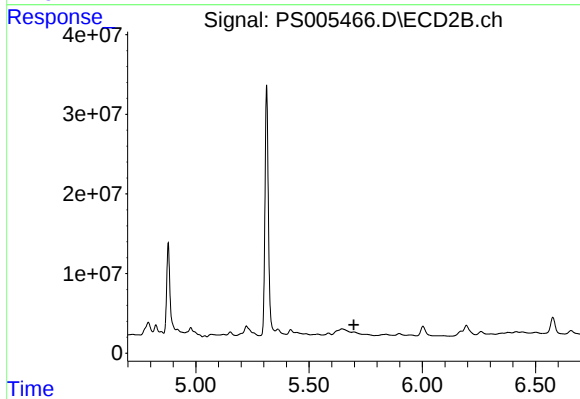

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.698 min
Response: 0
Conc: N.D.

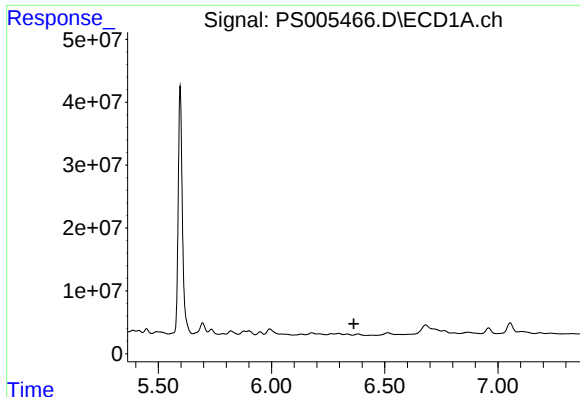

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

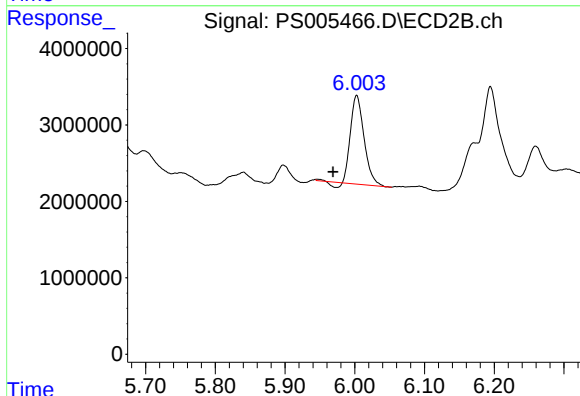


#8 DICHLORPROP

R.T.: 6.003 min
Delta R.T.: 0.034 min
Response: 15378580
Conc: 15.93 ng/ml

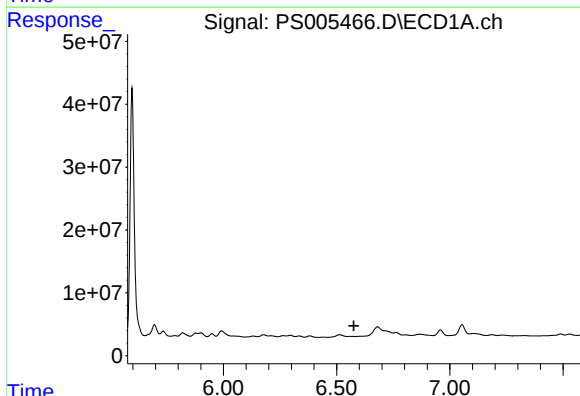


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.576 min
Response: 0
Conc: N.D.

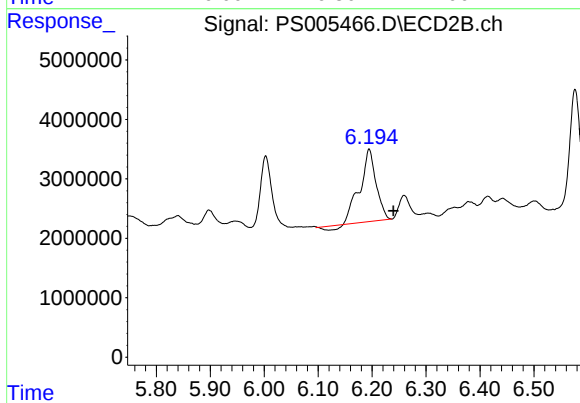

#9 2,4-D


R.T.: 6.195 min
Delta R.T.: -0.045 min
Response: 24708431
Conc: 22.15 ng/ml

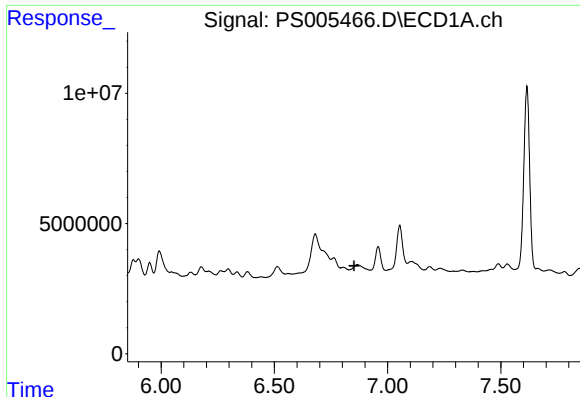

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

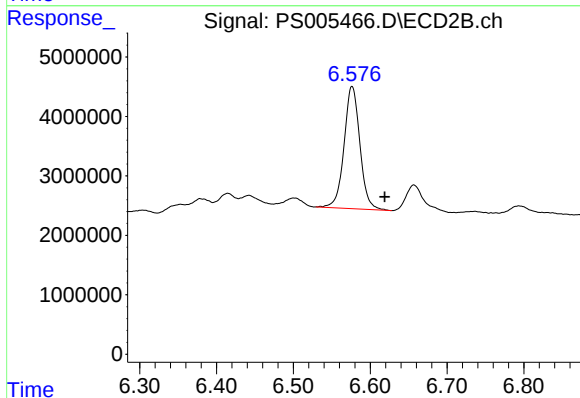


#10 Pentachlorophenol

R.T.: 6.576 min
Delta R.T.: -0.043 min
Response: 29450072
Conc: 2.29 ng/ml

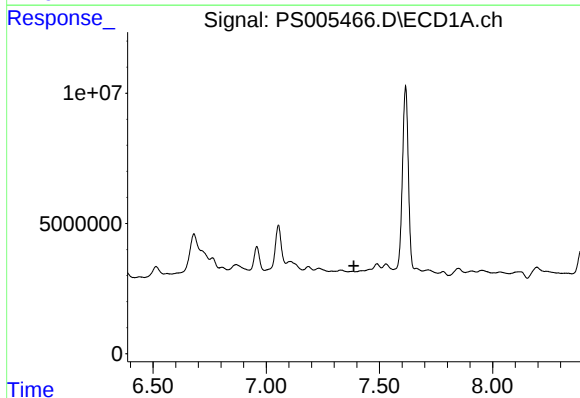


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

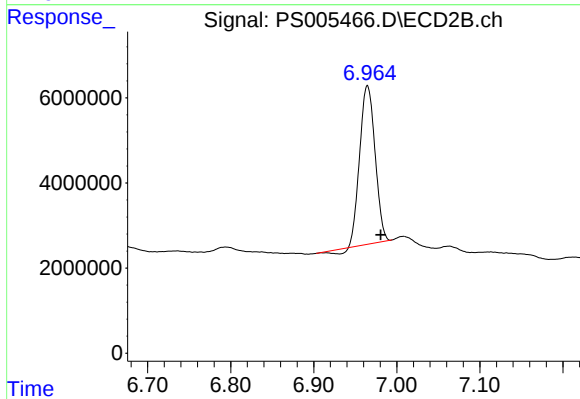

#11 2,4,5-TP (SILVEX)


R.T.: 6.965 min
Delta R.T.: -0.016 min
Response: 46933261
Conc: 8.81 ng/ml

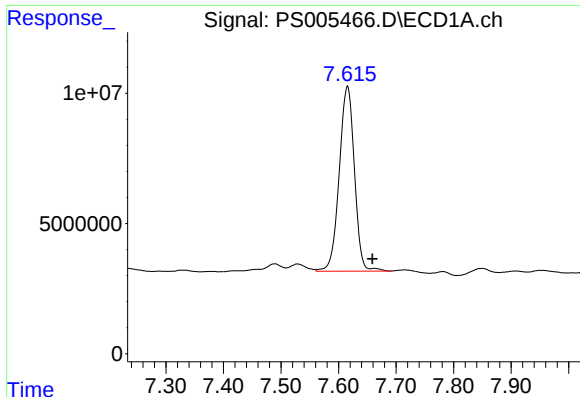

#12 2,4,5-T


R.T.: 7.615 min
Delta R.T.: -0.043 min
Response: 130393533
Conc: 16.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

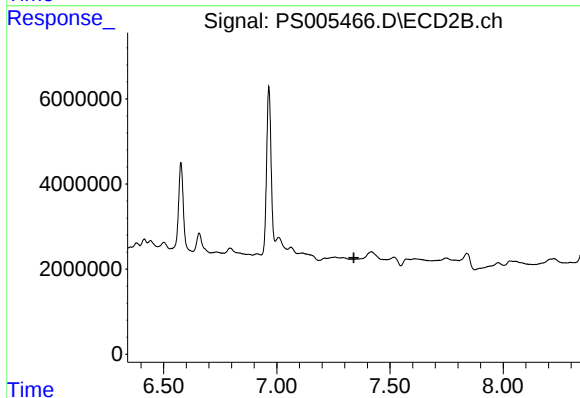


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.

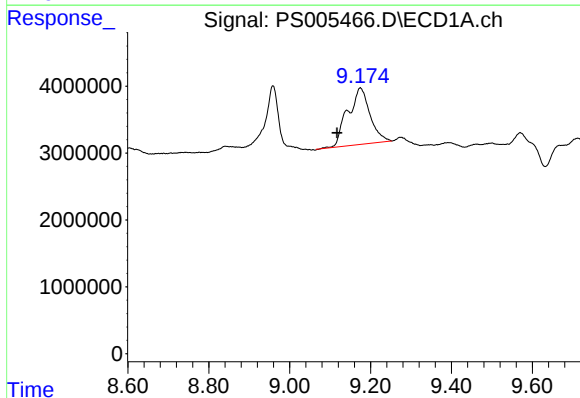

#15 Picloram

R.T.: 9.175 min
Delta R.T.: 0.058 min
Response: 32210772
Conc: 2.80 ng/ml

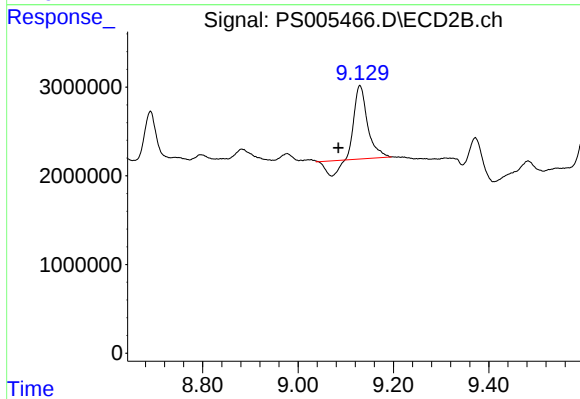

#15 Picloram

R.T.: 9.130 min
Delta R.T.: 0.045 min
Response: 13644575
Conc: 1.81 ng/ml