

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071125\
 Data File : PS031014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2025 20:01
 Operator : AR\AJ
 Sample : Q2517-01RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-14RE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/14/2025
 Supervised By :mohammad ahmed 07/15/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 06:07:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071125.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 14 05:51:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.328	7.767	432.1E6	20628578	109.260	19.911m#

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071125\
Data File : PS031014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2025 20:01
Operator : AR\AJ
Sample : Q2517-01RE
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TP-14RE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/14/2025
Supervised By : mohammad ahmed 07/15/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 06:07:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071125.M
Quant Title : 8080.M
QLast Update : Mon Jul 14 05:51:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

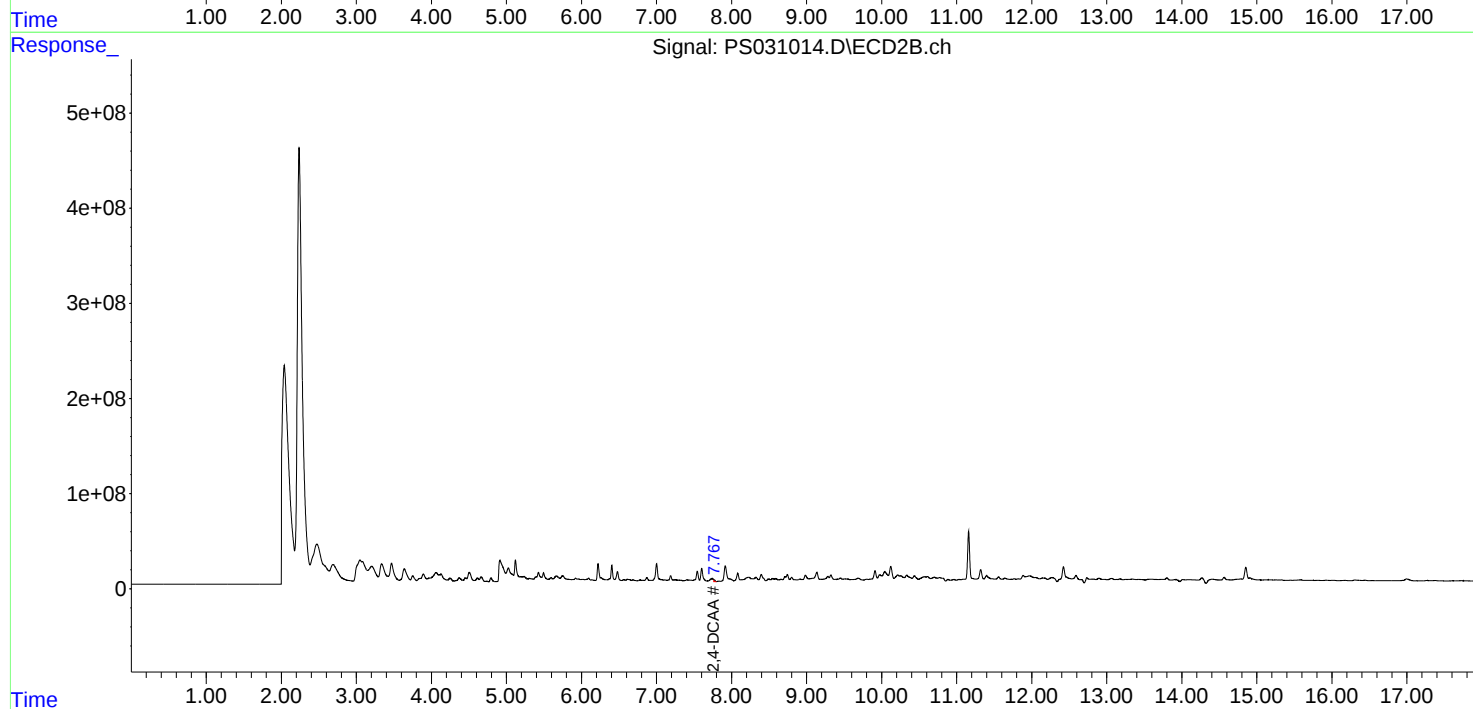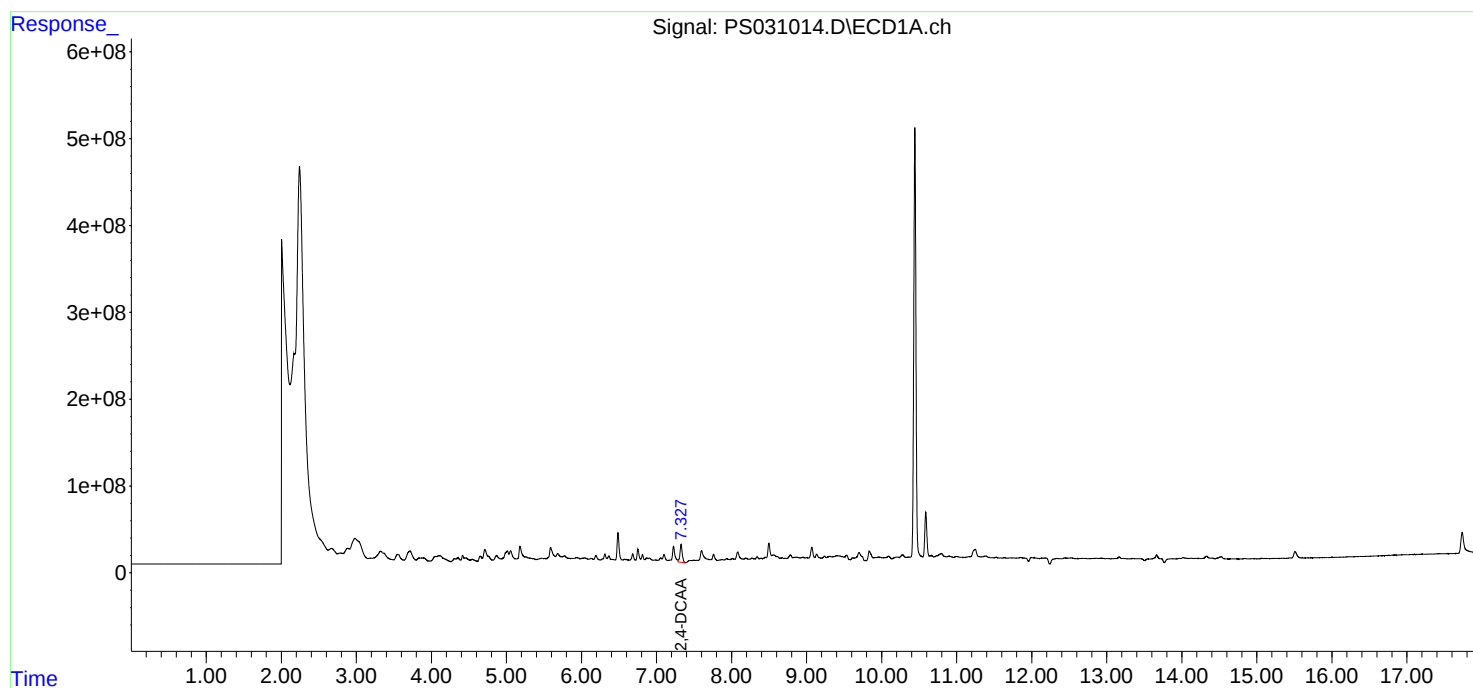

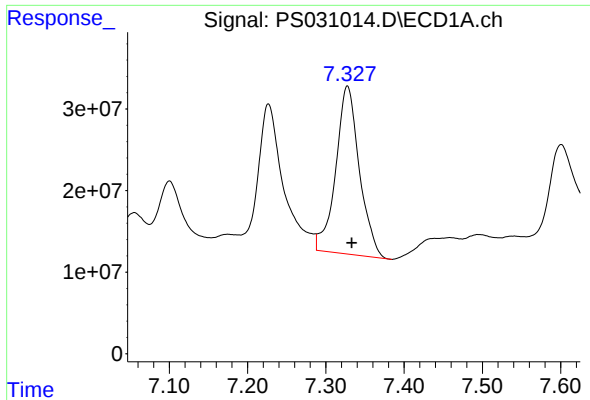


#4 2,4-DCAA

R.T.: 7.328 min
Delta R.T.: -0.005 min
Response: 432129726
Conc: 109.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-14RE

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/14/2025
Supervised By :mohammad ahmed 07/15/2025

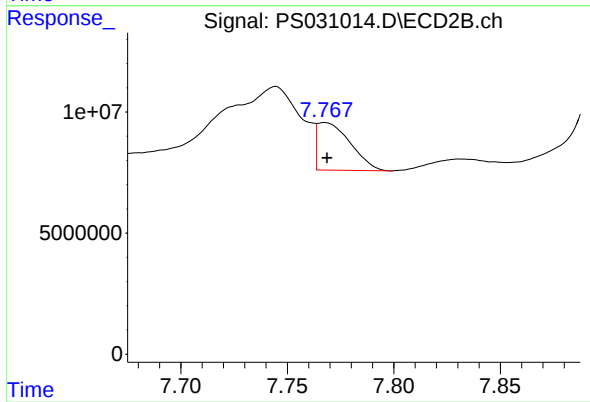

#4 2,4-DCAA

R.T.: 7.767 min
Delta R.T.: -0.002 min
Response: 20628578
Conc: 19.91 ng/ml m