

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071218\
 Data File : PS000983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2018 14:27
 Operator : UA
 Sample : J3914-10RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 15:15:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.664	11.068	63791069	52128092	309.185	239.342
Target Compounds							
1) T	Dalapon	2.998	2.423	5900530	567677	21.975	2.107 #
2) T	3,5-DICHL...	0.000	9.151	0	7282770	N.D.	24.758 #
5) T	DICAMBA	0.000	11.312	0	6190703	N.D.	7.887 #
6) T	MCP	12.360	0.000	7059651	0	12.852	N.D. #
8) T	DICHLORPROP	0.000	12.438	0	1468252	N.D.	7.269 #
15) T	Picloram	17.199	16.941	4394143	2076000	2.426	1.363 #
16) T	DCPA	0.000	17.013	0	6138443	N.D.	3.571 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071218\
Data File : PS000983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2018 14:27
Operator : UA
Sample : J3914-10RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 15:15:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

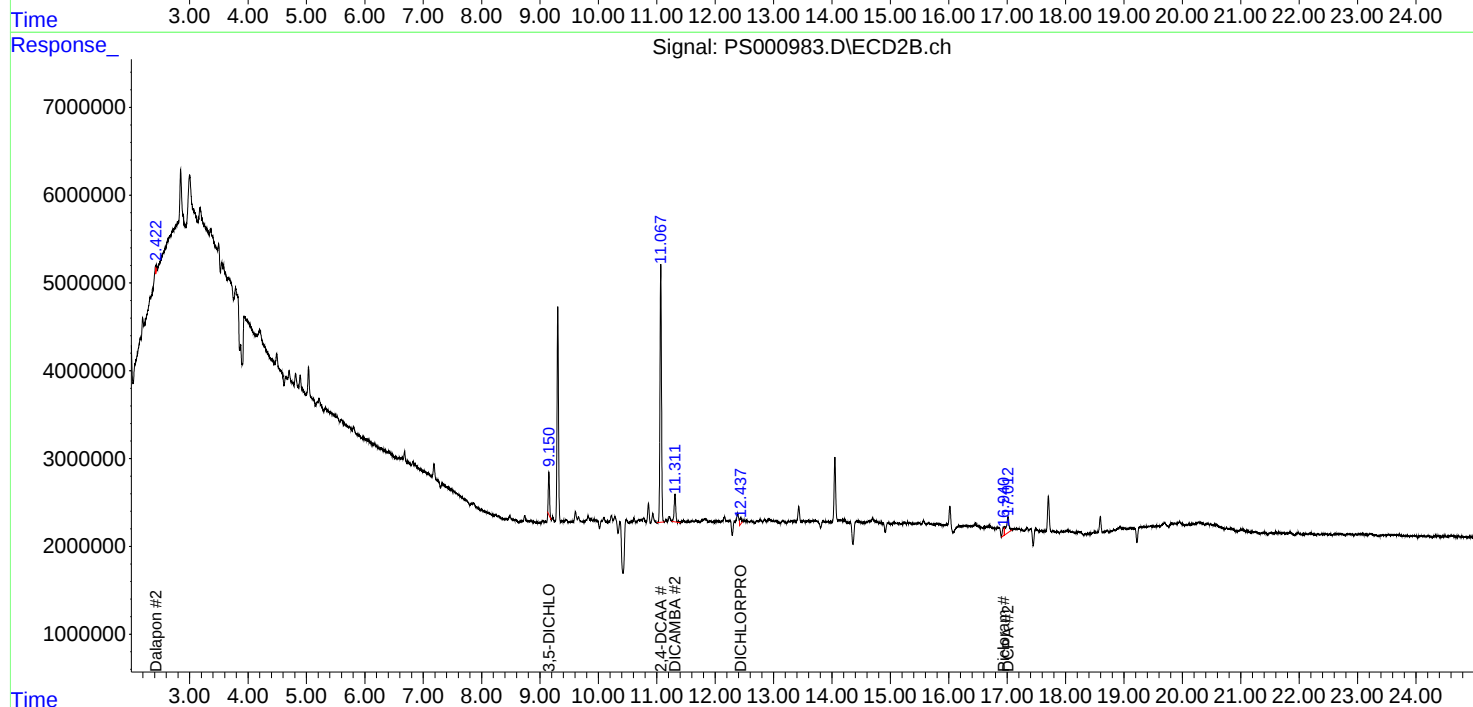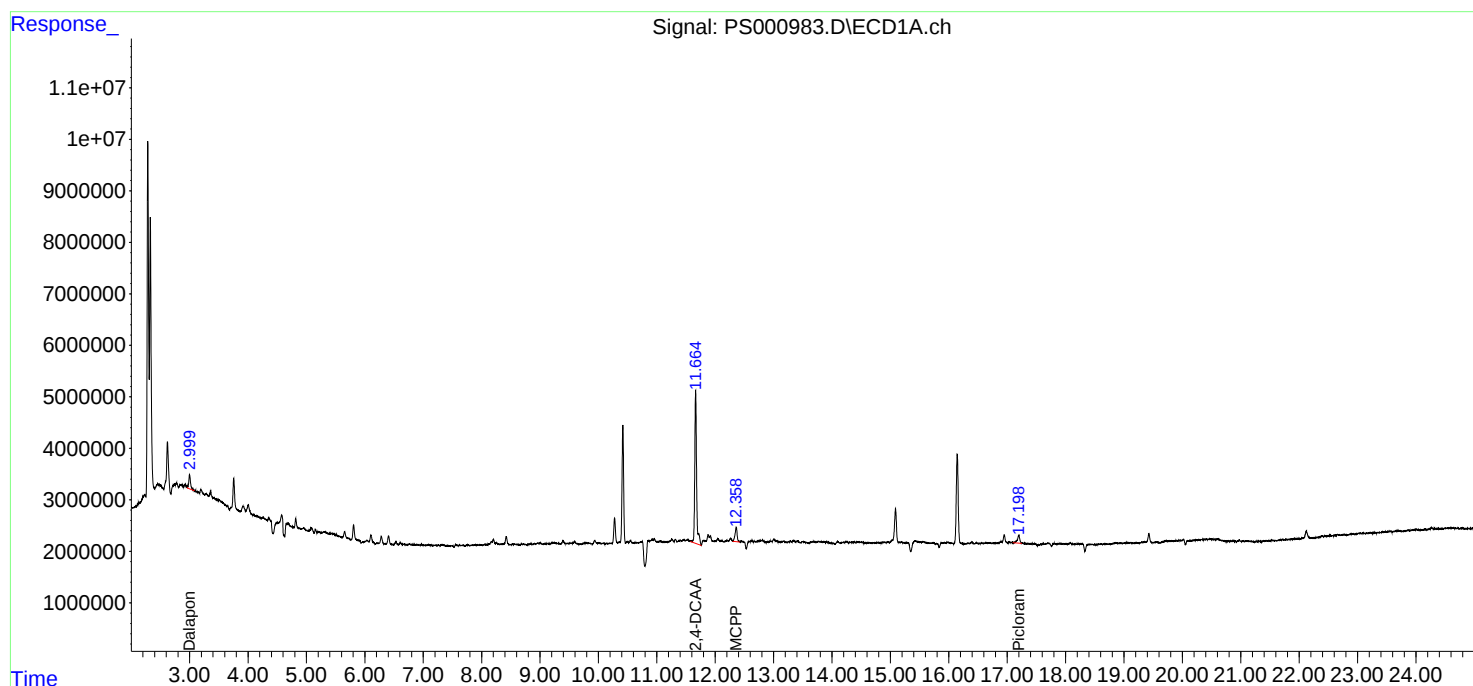


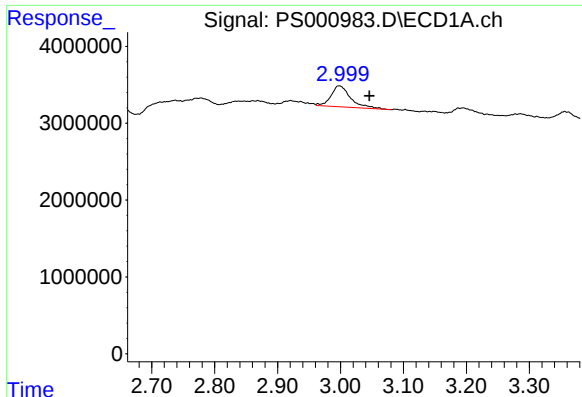

#1 Dalapon


R.T.: 2.998 min
Delta R.T.: -0.048 min
Response: 5900530
Conc: 21.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

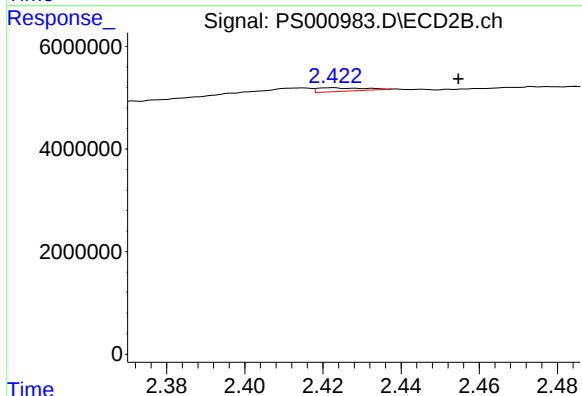


#1 Dalapon

R.T.: 2.423 min
Delta R.T.: -0.032 min
Response: 567677
Conc: 2.11 ng/ml

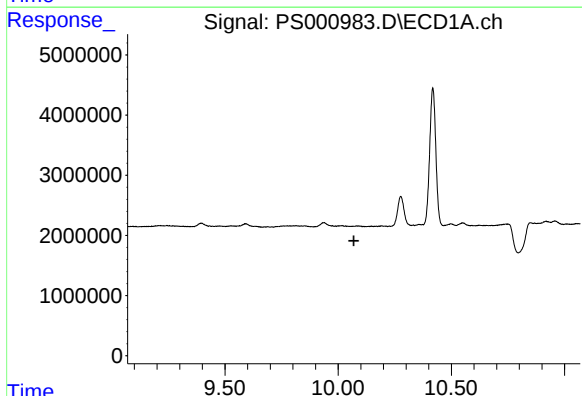


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

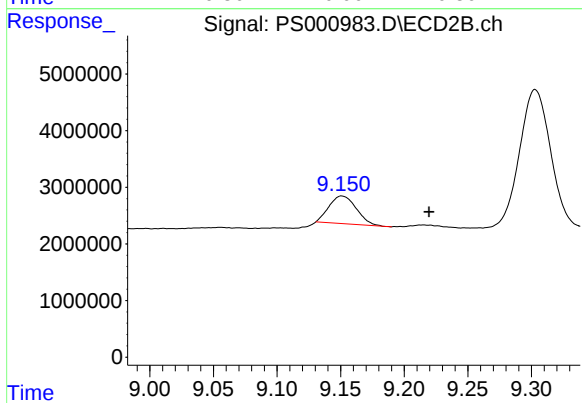

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.151 min
Delta R.T.: -0.069 min
Response: 7282770
Conc: 24.76 ng/ml

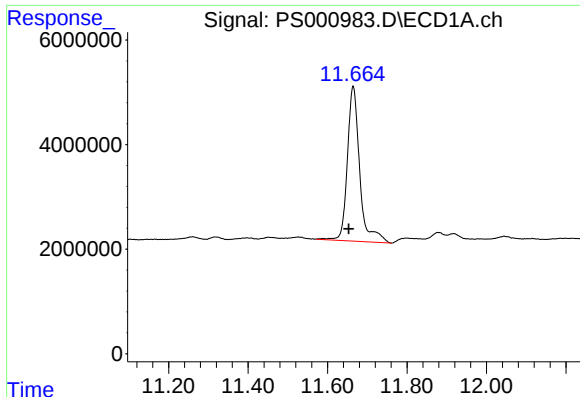

#4 2,4-DCAA


R.T.: 11.664 min
Delta R.T.: 0.011 min
Response: 63791069
Conc: 309.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

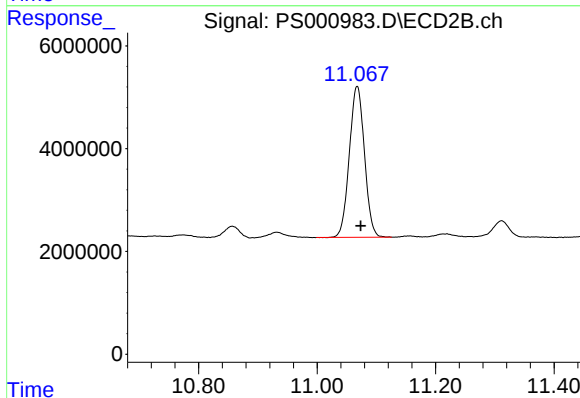


#4 2,4-DCAA

R.T.: 11.068 min
Delta R.T.: -0.006 min
Response: 52128092
Conc: 239.34 ng/ml

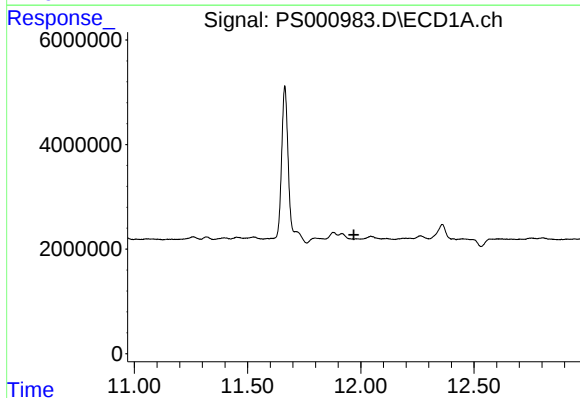


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.970 min
Response: 0
Conc: N.D.

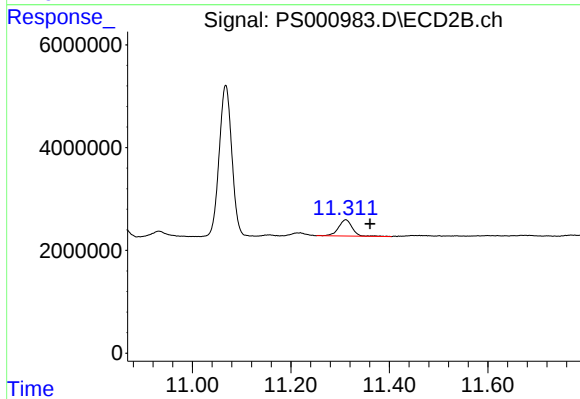

#5 DICAMBA


R.T.: 11.312 min
Delta R.T.: -0.050 min
Response: 6190703
Conc: 7.89 ng/ml

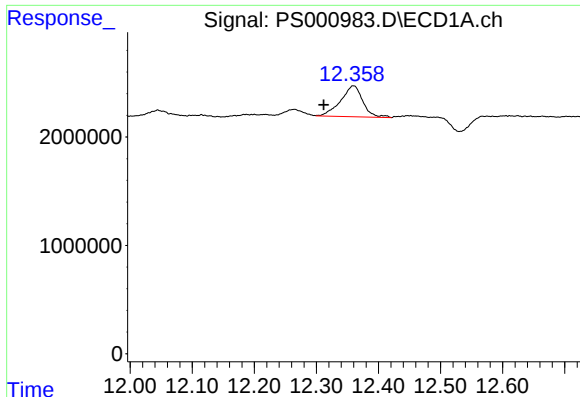

#6 MCP


R.T.: 12.360 min
Delta R.T.: 0.048 min
Response: 7059651
Conc: 12.85 ug/ml

Instrument :
ECD_S
ClientSampleId :

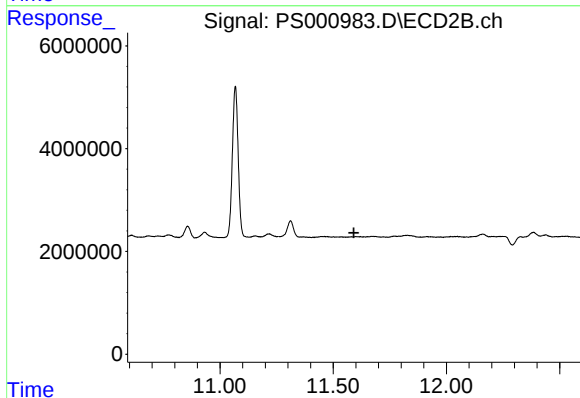


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

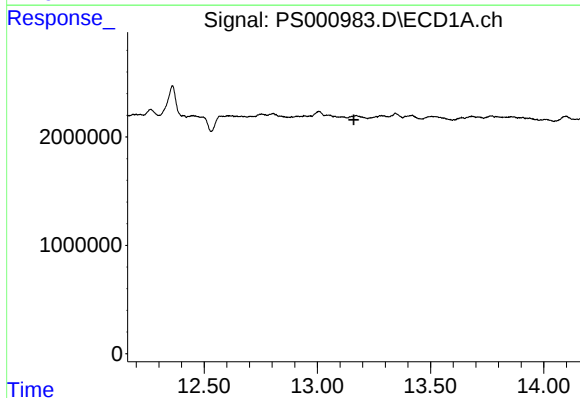


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

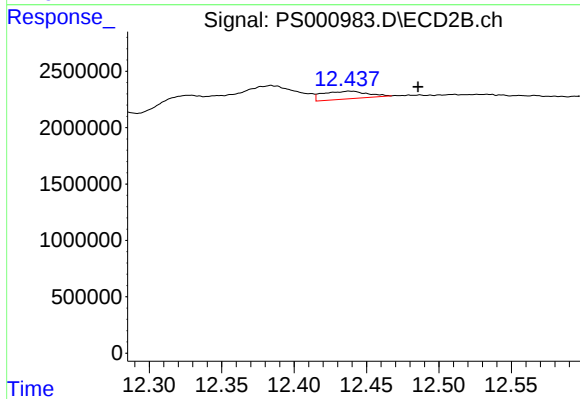

#8 DICHLORPROP


R.T.: 12.438 min
Delta R.T.: -0.047 min
Response: 1468252
Conc: 7.27 ng/ml

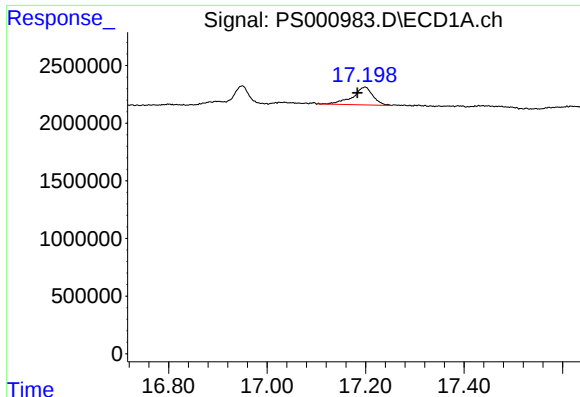

#15 Picloram


R.T.: 17.199 min
Delta R.T.: 0.015 min
Response: 4394143
Conc: 2.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

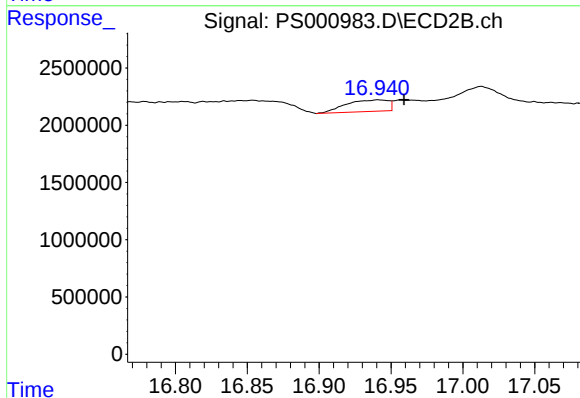


#15 Picloram

R.T.: 16.941 min
Delta R.T.: -0.018 min
Response: 2076000
Conc: 1.36 ng/ml

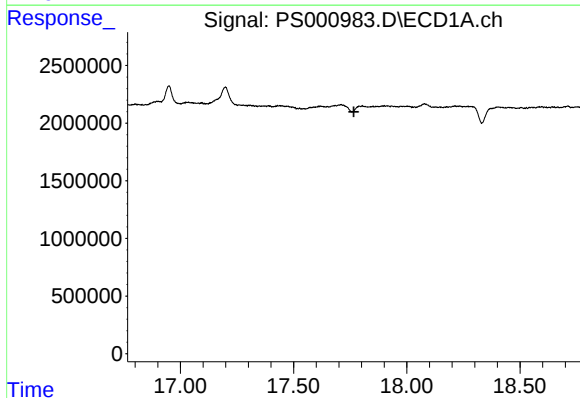

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.766 min
Response: 0
Conc: N.D.

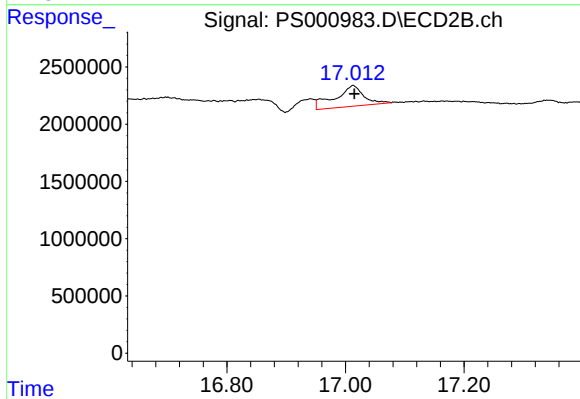

#16 DCPA

R.T.: 17.013 min
Delta R.T.: -0.002 min
Response: 6138443
Conc: 3.57 ng/ml