

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071218\
 Data File : PS000987.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2018 18:46
 Operator : UA
 Sample : J3825-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 00:48:10 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.649	11.063	53728094	43712783	260.411	200.704
Target Compounds							
1) T	Dalapon	2.984	2.425	2738678	961851	10.200	3.570 #
5) T	DICAMBA	0.000	11.306	0	6145401	N.D.	7.829 #
6) T	MCPD	12.344	0.000	6582208	0	11.983	N.D. #
7) T	MCPA	12.590	0.000	5841747	0	6.401	N.D. #
8) T	DICHLORPROP	0.000	12.434	0	1934886	N.D.	9.580 #
15) T	Picloram	0.000	17.010	0	2868976	N.D.	1.884 #
16) T	DCPA	0.000	17.010	0	2868976	N.D.	1.669 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071218\
Data File : PS000987.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2018 18:46
Operator : UA
Sample : J3825-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 00:48:10 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

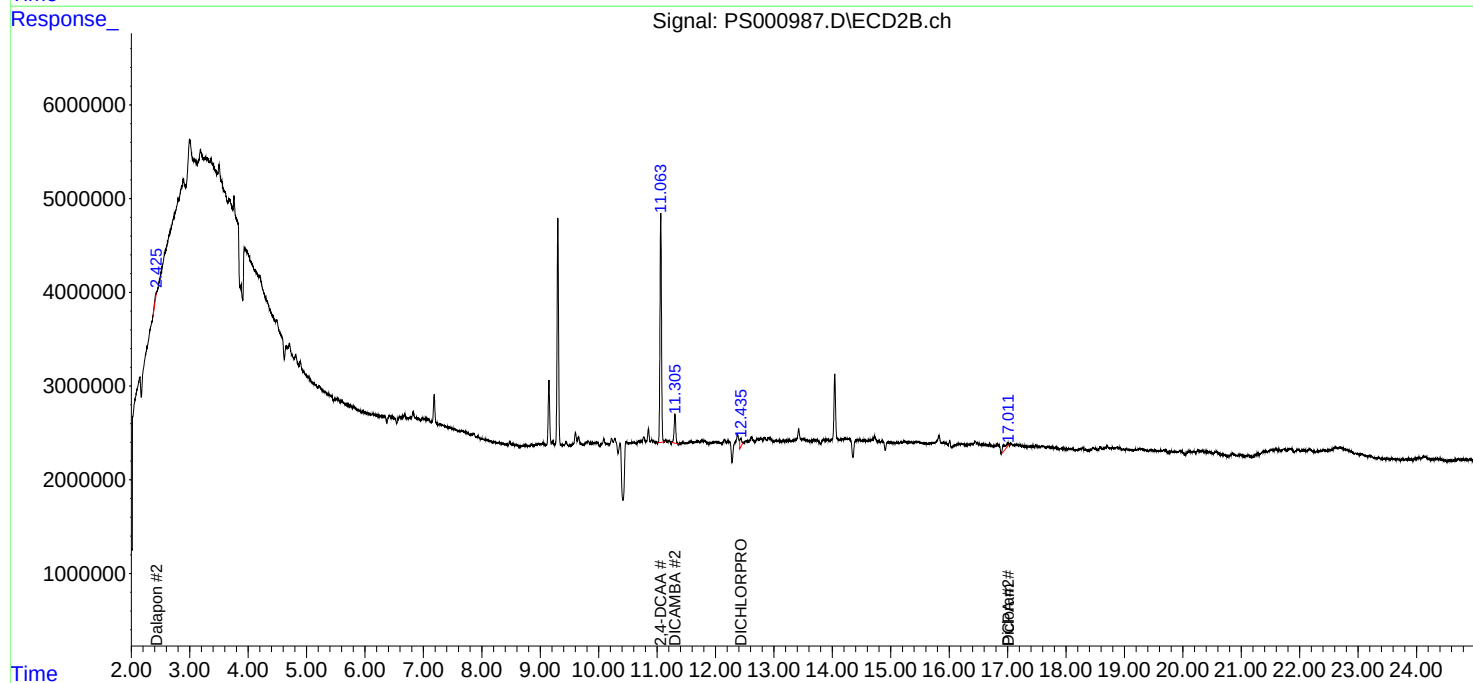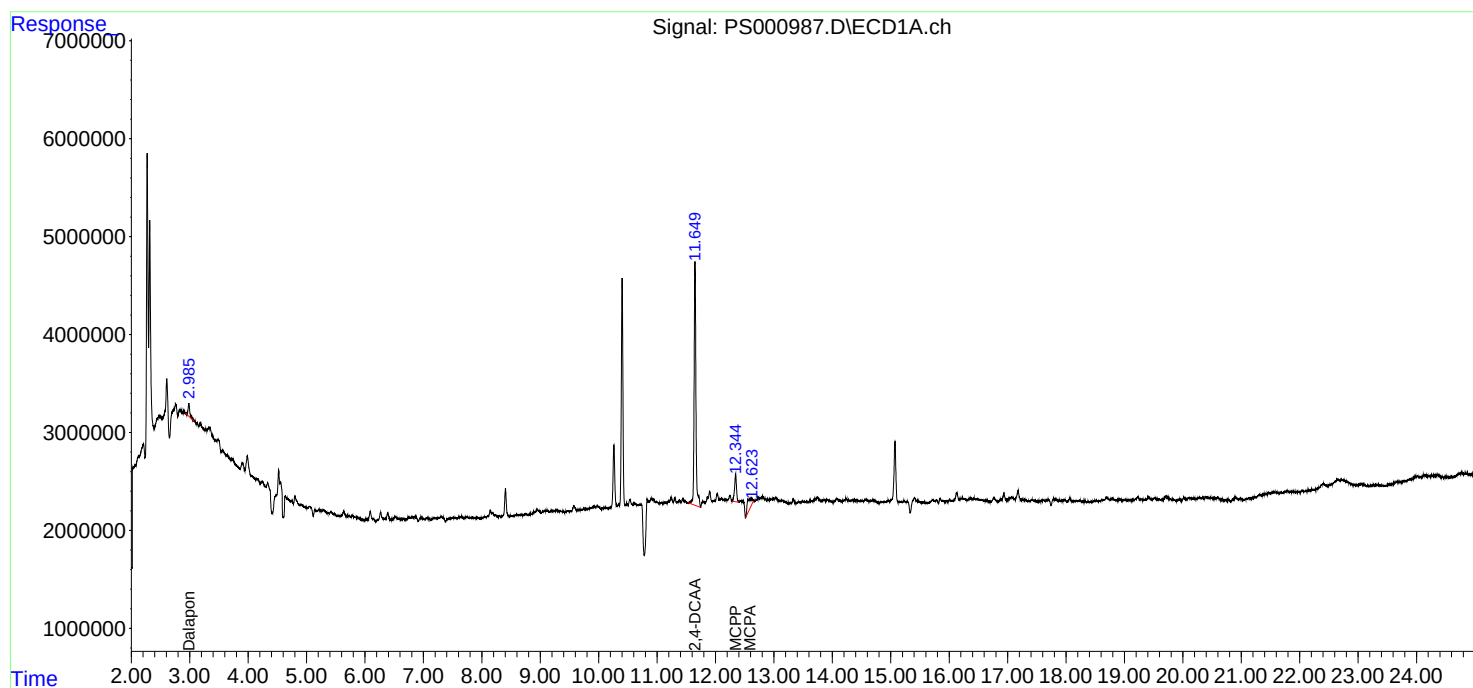


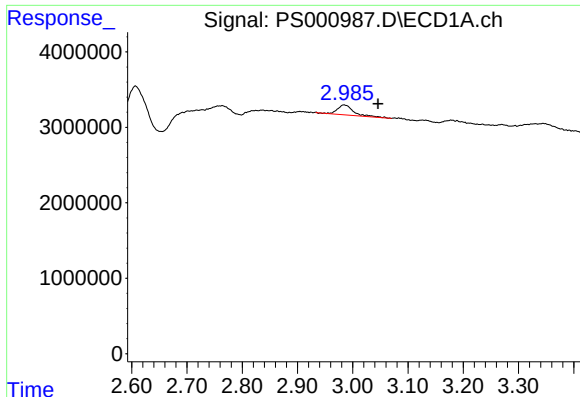

#1 Dalapon


R.T.: 2.984 min
Delta R.T.: -0.062 min
Response: 2738678
Conc: 10.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

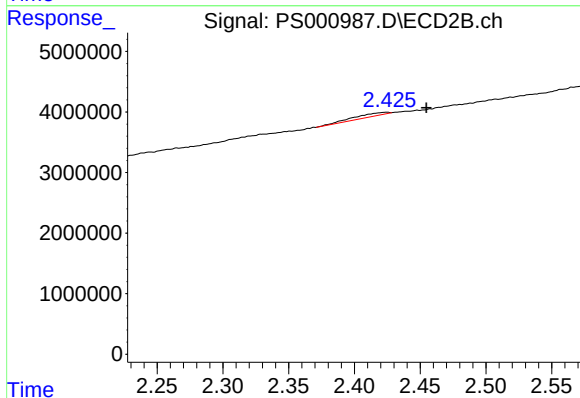


#1 Dalapon

R.T.: 2.425 min
Delta R.T.: -0.030 min
Response: 961851
Conc: 3.57 ng/ml

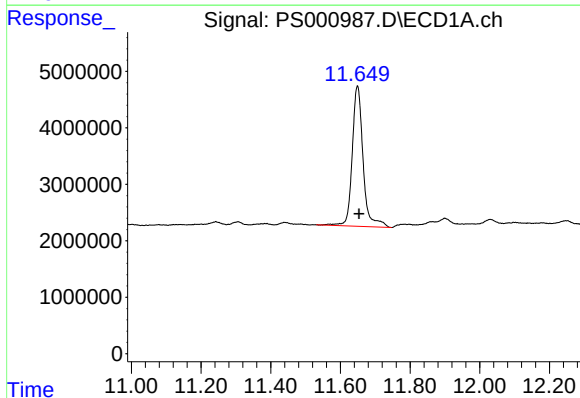


#4 2,4-DCAA

R.T.: 11.649 min
Delta R.T.: -0.004 min
Response: 53728094
Conc: 260.41 ng/ml

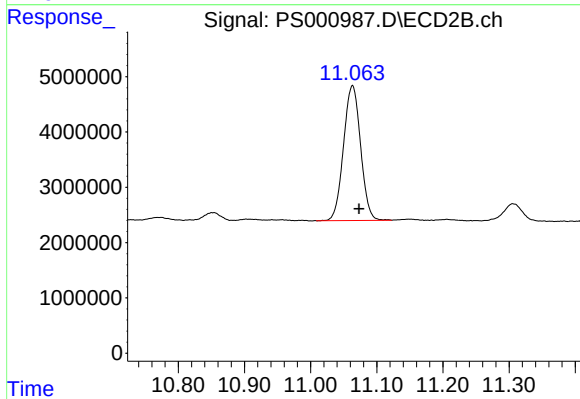

#4 2,4-DCAA


R.T.: 11.063 min
Delta R.T.: -0.010 min
Response: 43712783
Conc: 200.70 ng/ml

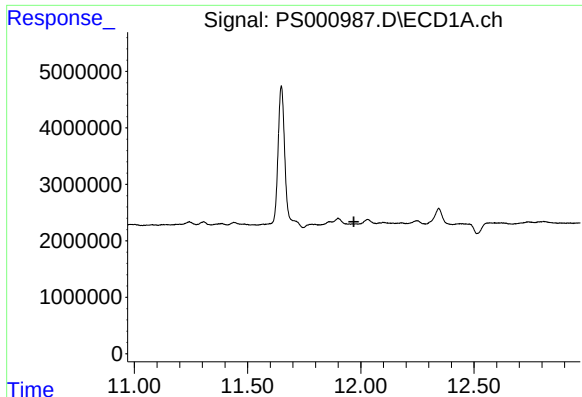

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.970 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

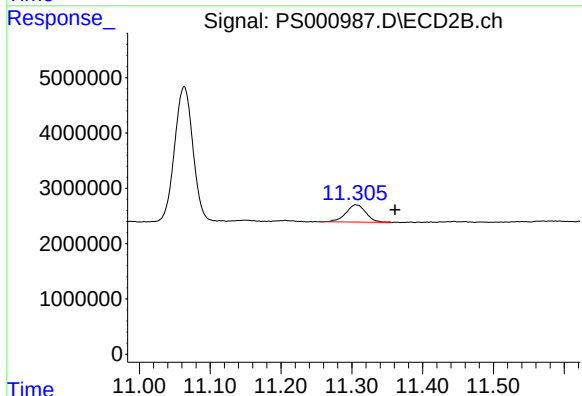


#5 DICAMBA

R.T.: 11.306 min
Delta R.T.: -0.055 min
Response: 6145401
Conc: 7.83 ng/ml

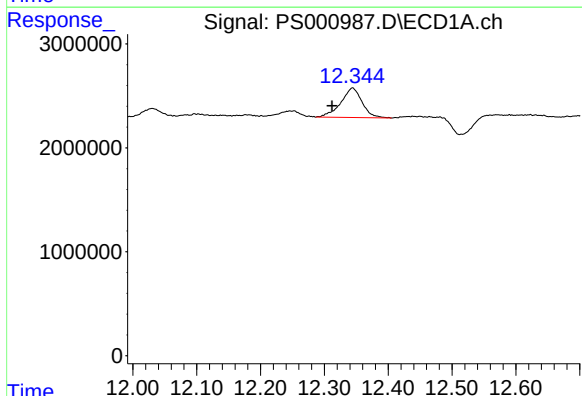


#6 MCPP

R.T.: 12.344 min
Delta R.T.: 0.032 min
Response: 6582208
Conc: 11.98 ug/ml

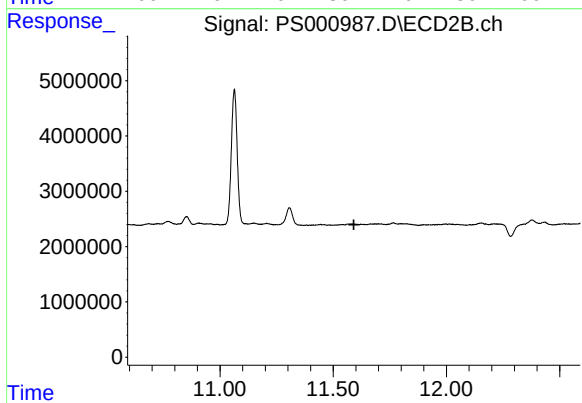

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

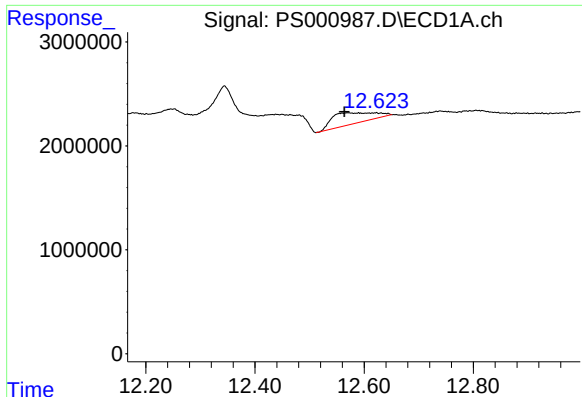

#7 MCPA


R.T.: 12.590 min
Delta R.T.: 0.026 min
Response: 5841747
Conc: 6.40 ug/ml

Instrument :
ECD_S
ClientSampleId :

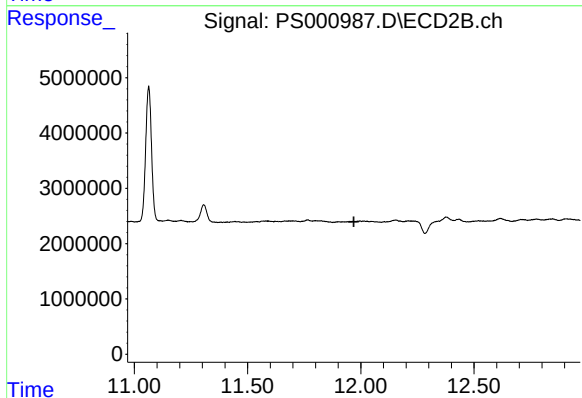


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.969 min
Response: 0
Conc: N.D.

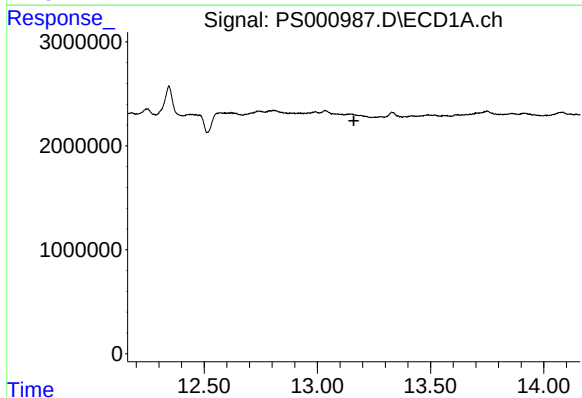


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

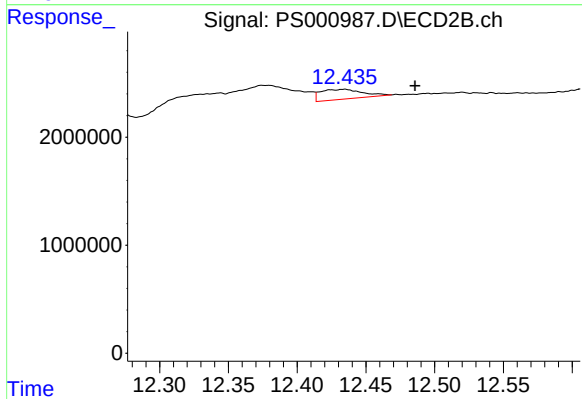

#8 DICHLORPROP


R.T.: 12.434 min
Delta R.T.: -0.051 min
Response: 1934886
Conc: 9.58 ng/ml

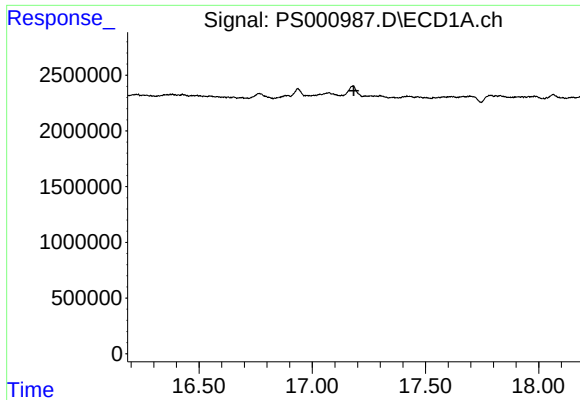

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

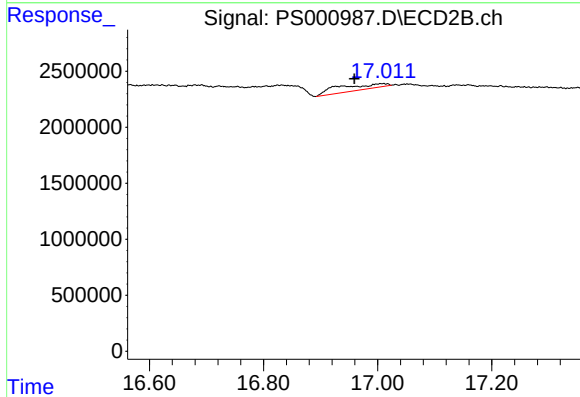


#15 Picloram

R.T.: 17.010 min
Delta R.T.: 0.051 min
Response: 2868976
Conc: 1.88 ng/ml

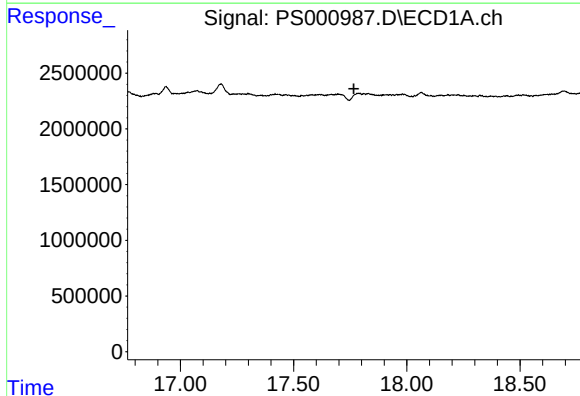

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.766 min
Response: 0
Conc: N.D.

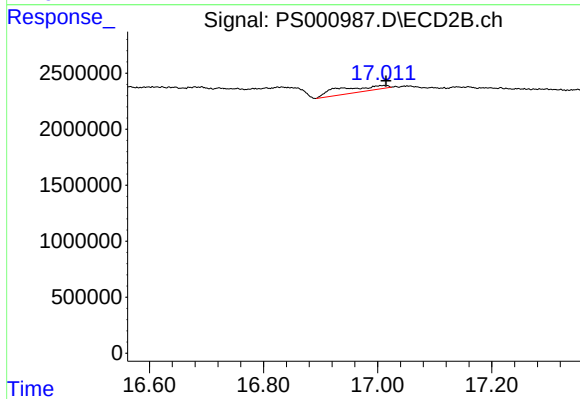

#16 DCPA

R.T.: 17.010 min
Delta R.T.: -0.005 min
Response: 2868976
Conc: 1.67 ng/ml