

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071218\
 Data File : PS000988.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2018 19:17
 Operator : UA
 Sample : J3825-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 00:48:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.633	11.048	55529583	44848908	269.143	205.921
Target Compounds							
2) T	3,5-DICHL...	0.000	9.286	0	45481226	N.D.	154.617 #
5) T	DICAMBA	0.000	11.292	0	7092323	N.D.	9.035 #
6) T	MCP	12.329	0.000	5371566	0	9.779	N.D. #
8) T	DICHLORPROP	0.000	12.417	0	2184800	N.D.	10.817 #
15) T	Picloram	0.000	16.994	0	4605877	N.D.	3.025 #
16) T	DCPA	0.000	16.994	0	4605877	N.D.	2.679 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071218\
Data File : PS000988.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2018 19:17
Operator : UA
Sample : J3825-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 00:48:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

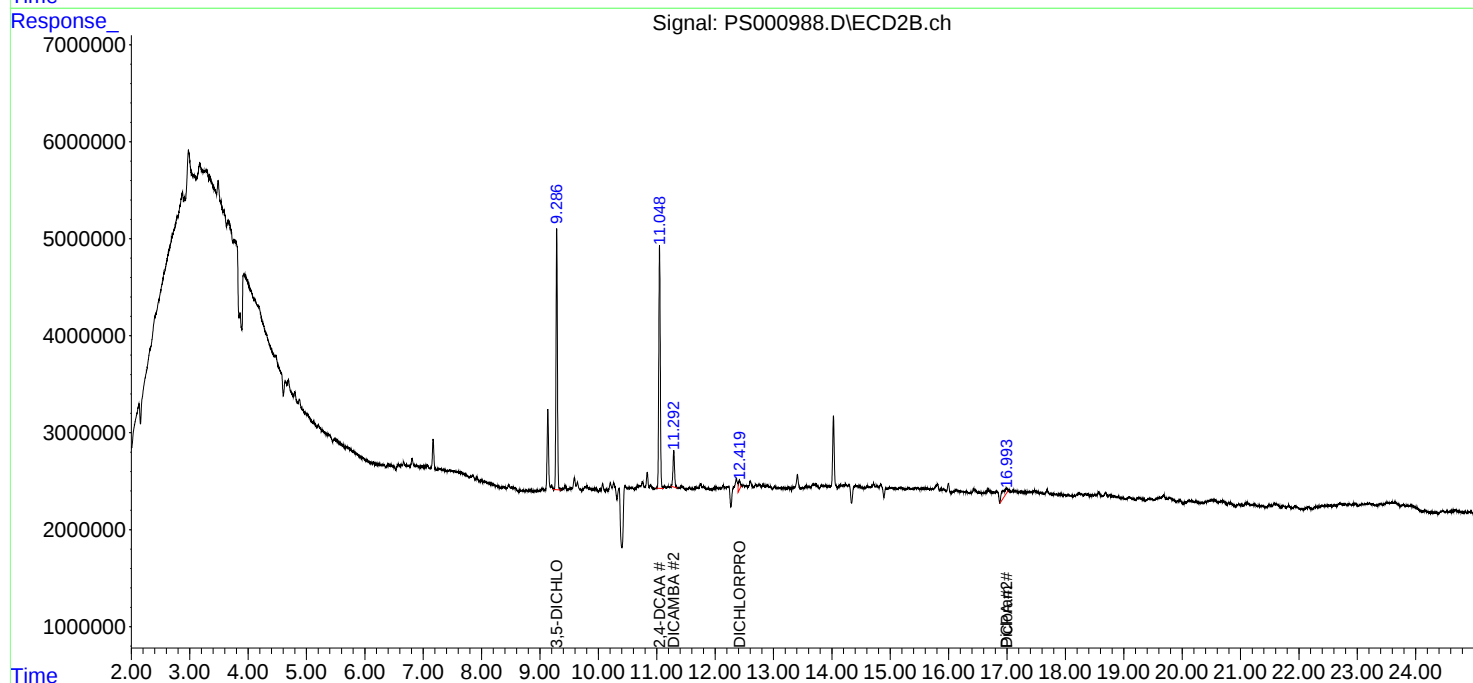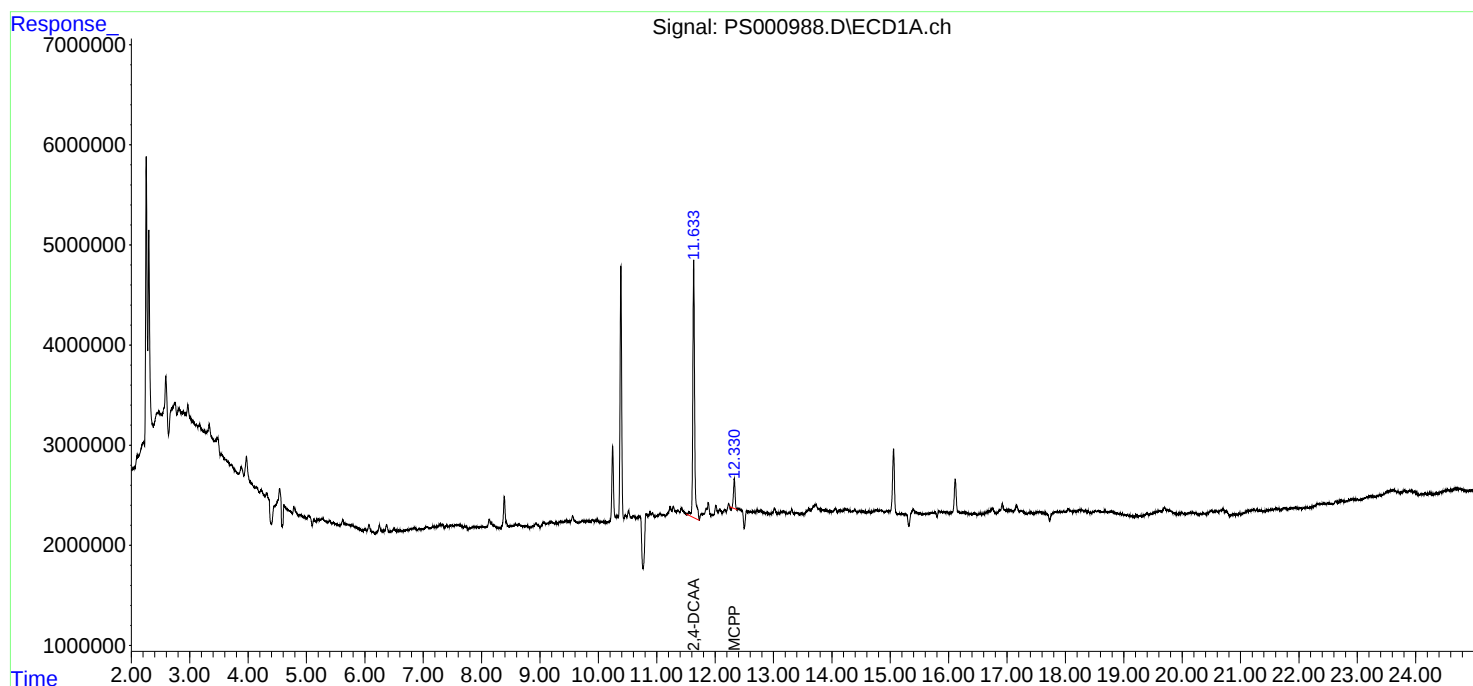


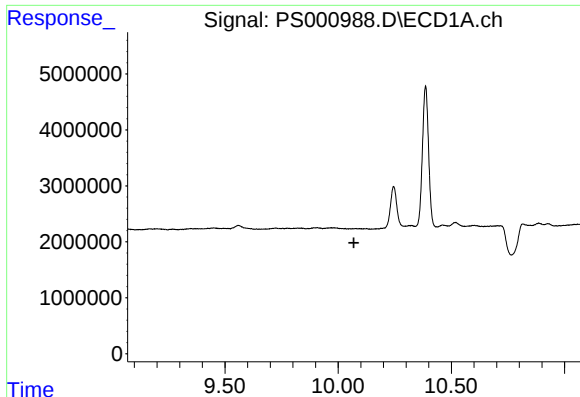

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

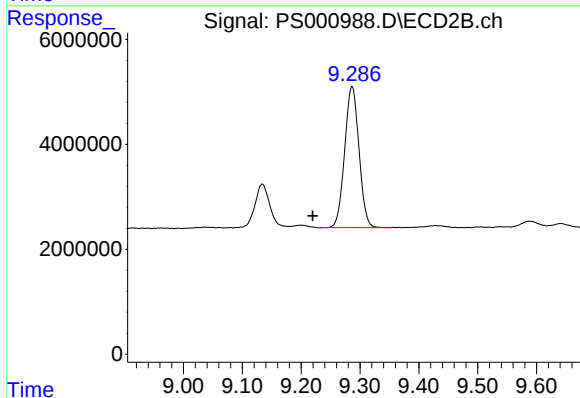


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.286 min
Delta R.T.: 0.067 min
Response: 45481226
Conc: 154.62 ng/ml

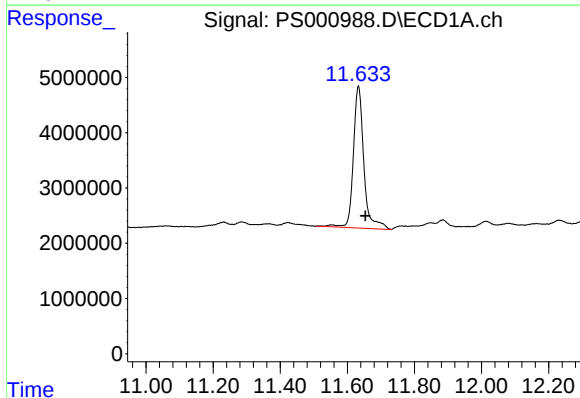


#4 2,4-DCAA

R.T.: 11.633 min
Delta R.T.: -0.020 min
Response: 55529583
Conc: 269.14 ng/ml

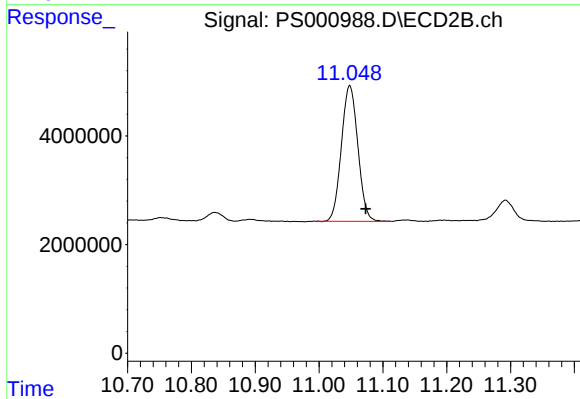

#4 2,4-DCAA


R.T.: 11.048 min
Delta R.T.: -0.026 min
Response: 44848908
Conc: 205.92 ng/ml

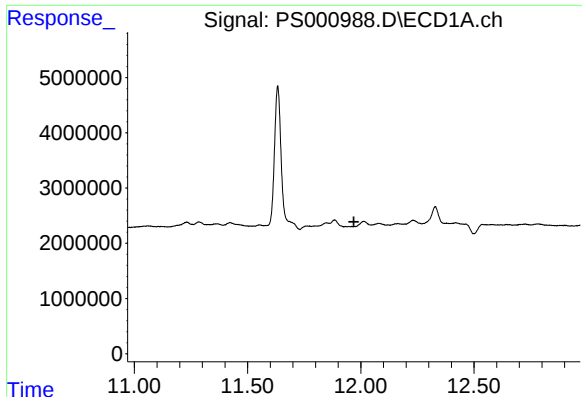

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.970 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

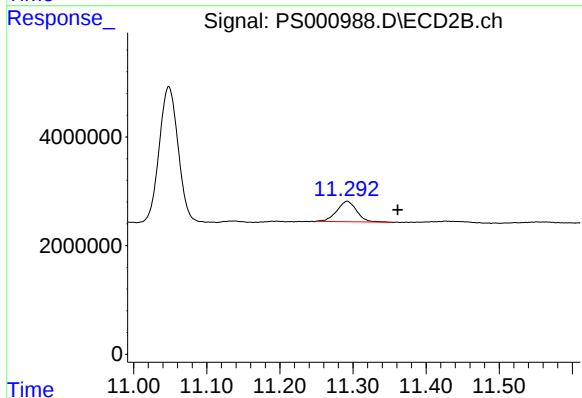


#5 DICAMBA

R.T.: 11.292 min
Delta R.T.: -0.069 min
Response: 7092323
Conc: 9.04 ng/ml

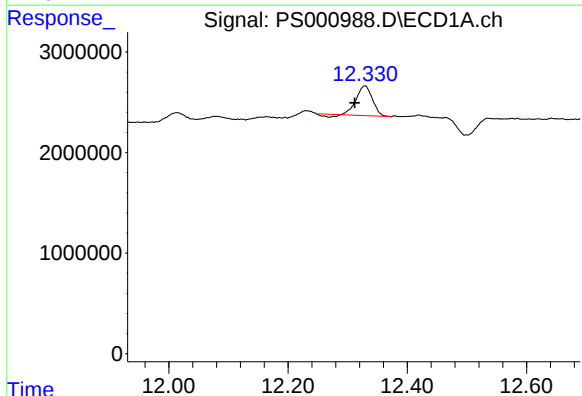


#6 MCP

R.T.: 12.329 min
Delta R.T.: 0.017 min
Response: 5371566
Conc: 9.78 ug/ml

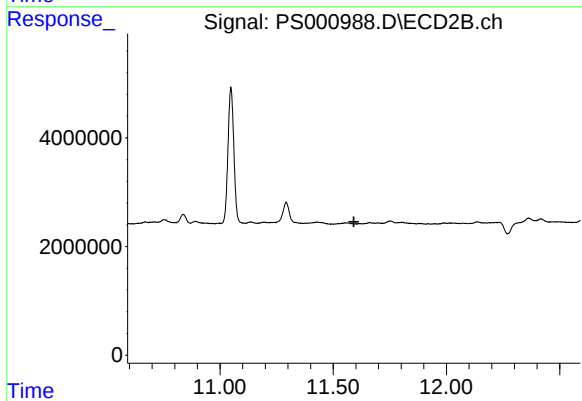

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

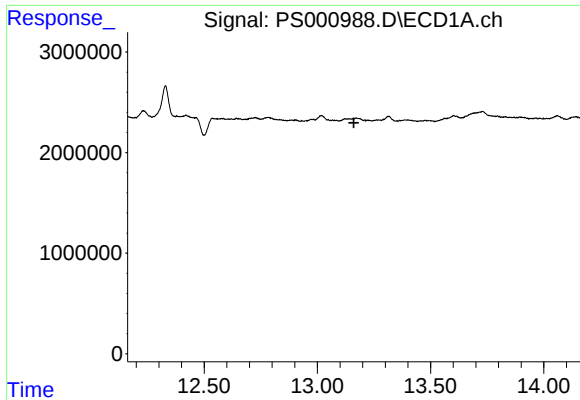

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

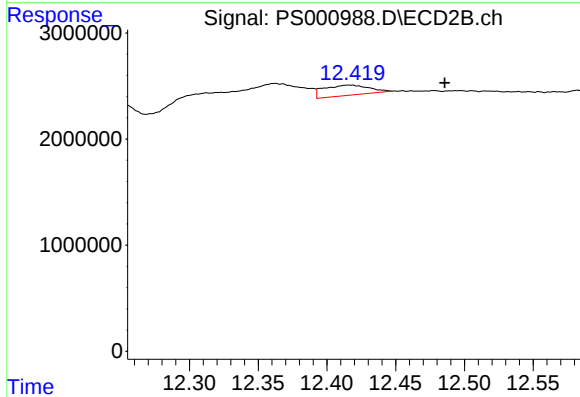


#8 DICHLORPROP

R.T.: 12.417 min
Delta R.T.: -0.068 min
Response: 2184800
Conc: 10.82 ng/ml

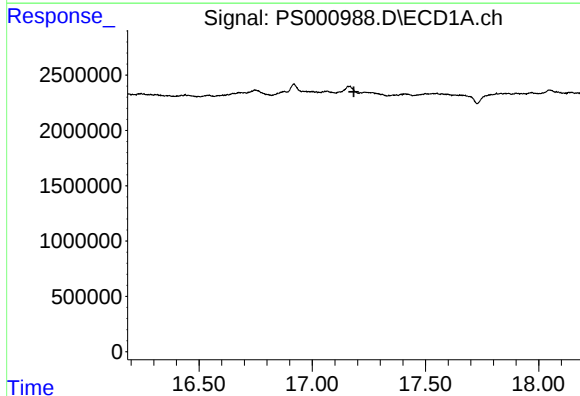


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.184 min
Response: 0
Conc: N.D.

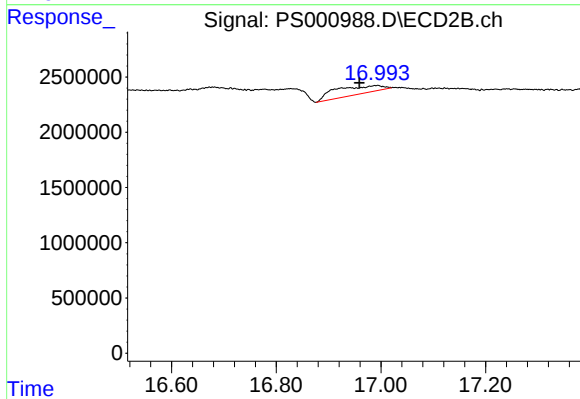

#15 Picloram


R.T.: 16.994 min
Delta R.T.: 0.035 min
Response: 4605877
Conc: 3.02 ng/ml

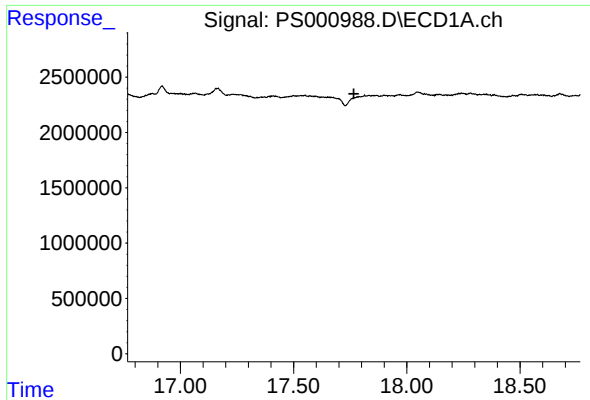

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.766 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

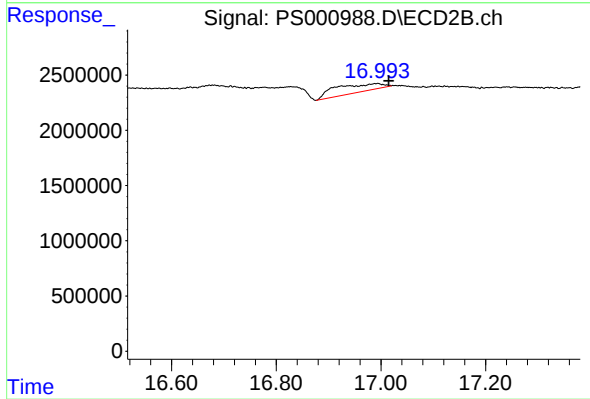

#16 DCPA

R.T.: 16.994 min
Delta R.T.: -0.021 min
Response: 4605877
Conc: 2.68 ng/ml