

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071218\
 Data File : PS000994.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2018 22:23
 Operator : UA
 Sample : J3947-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 00:50:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.651	11.066	42358017	36738955	205.302	168.684
Target Compounds							
1) T	Dalapon	2.987	0.000	2978604	0	11.093	N.D. #
2) T	3,5-DICHL...	0.000	9.152	0	12315944	N.D.	41.869 #
5) T	DICAMBA	0.000	11.310	0	5201371	N.D.	6.626 #
6) T	MCP	12.346	0.000	6964465	0	12.679	N.D. #
8) T	DICHLORPROP	0.000	12.432	0	2466575	N.D.	12.212 #
15) T	Picloram	0.000	17.006	0	5880572	N.D.	3.862 #
16) T	DCPA	0.000	17.006	0	5880572	N.D.	3.421 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071218\
Data File : PS000994.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2018 22:23
Operator : UA
Sample : J3947-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 00:50:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

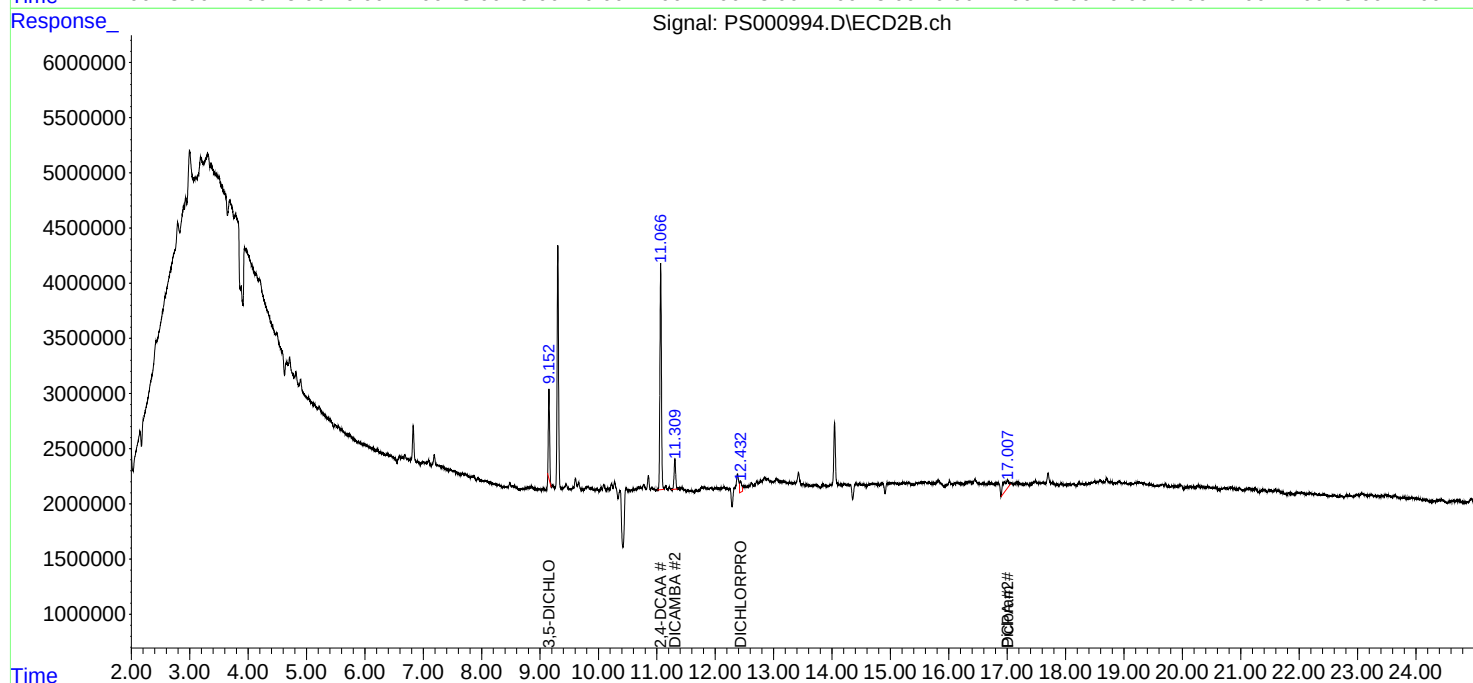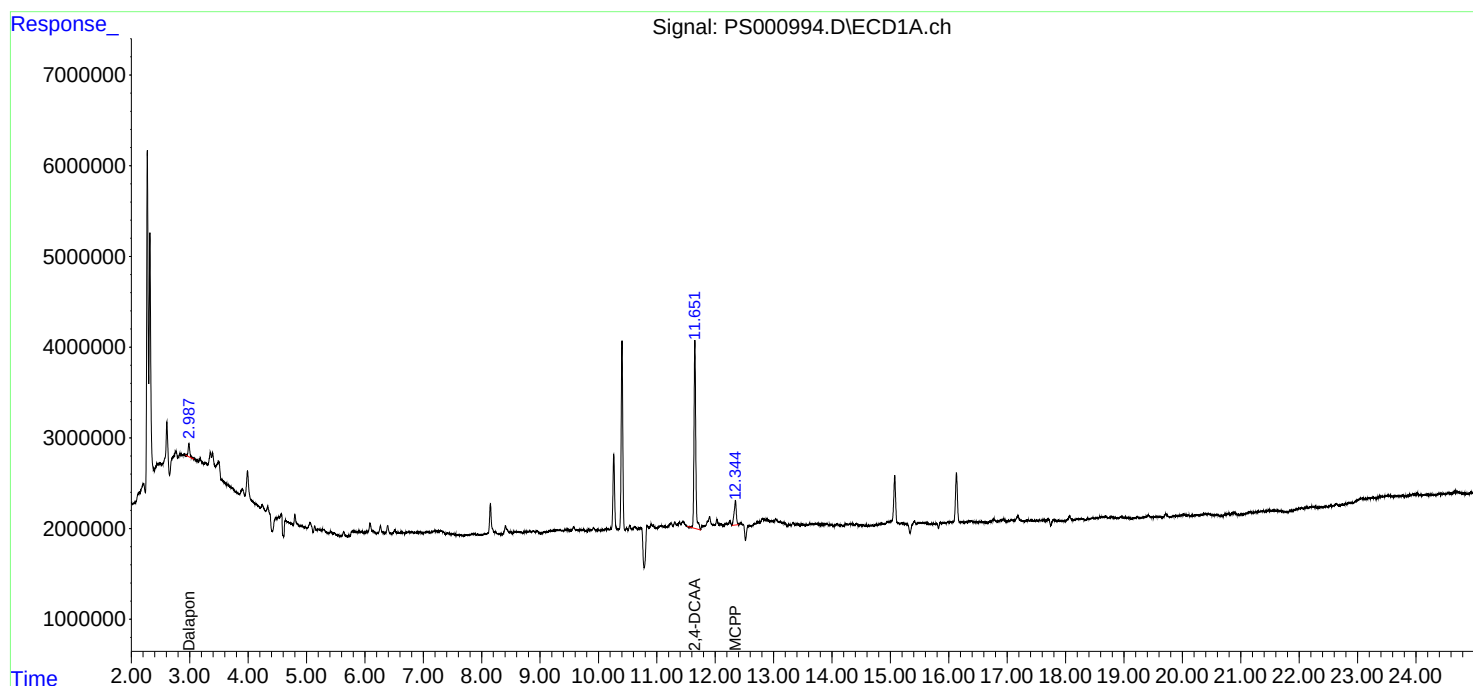


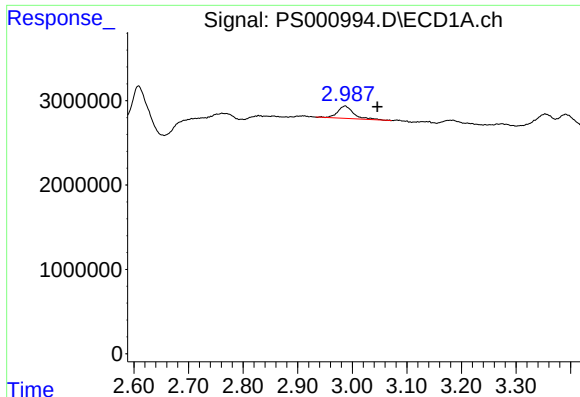

#1 Dalapon


R.T.: 2.987 min
Delta R.T.: -0.059 min
Response: 2978604
Conc: 11.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

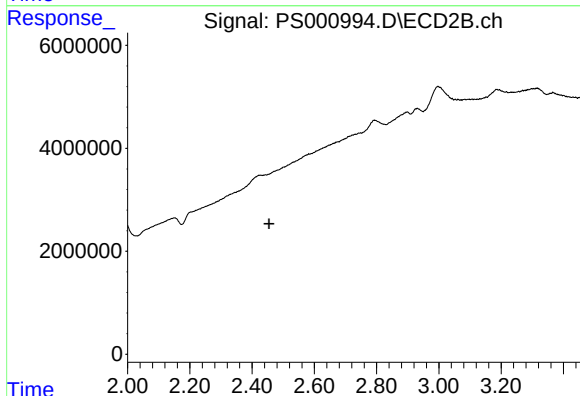


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.455 min
Response: 0
Conc: N.D.

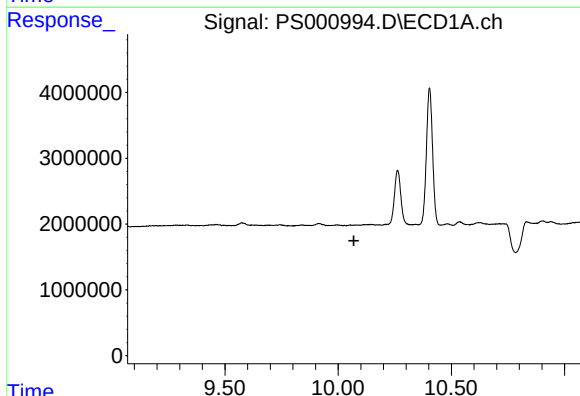


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

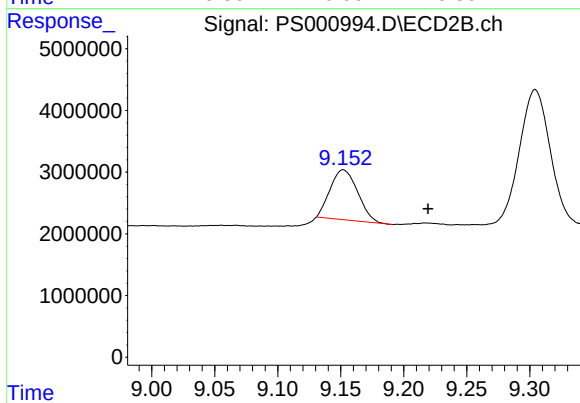

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.152 min
Delta R.T.: -0.067 min
Response: 12315944
Conc: 41.87 ng/ml

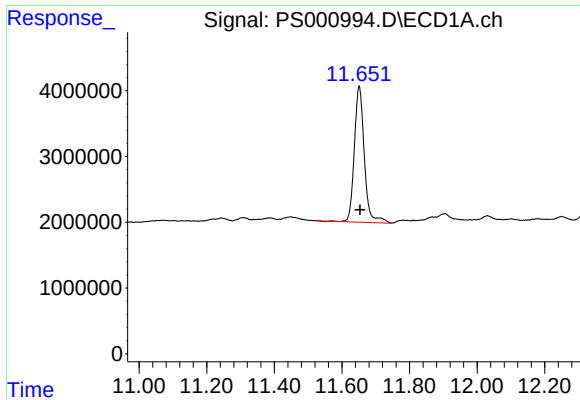

#4 2,4-DCAA


R.T.: 11.651 min
Delta R.T.: -0.002 min
Response: 42358017
Conc: 205.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

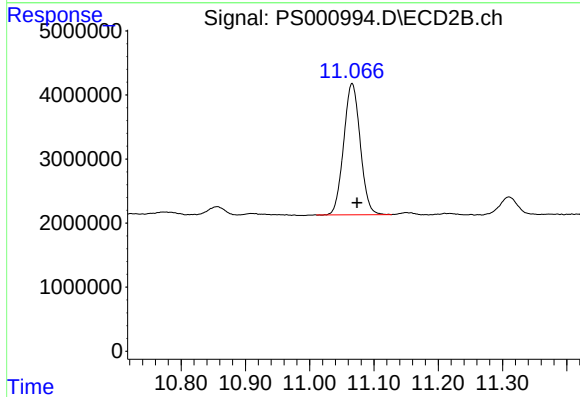


#4 2,4-DCAA

R.T.: 11.066 min
Delta R.T.: -0.008 min
Response: 36738955
Conc: 168.68 ng/ml

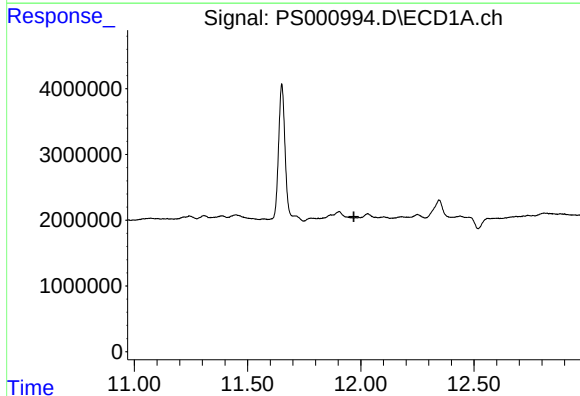


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.970 min
Response: 0
Conc: N.D.

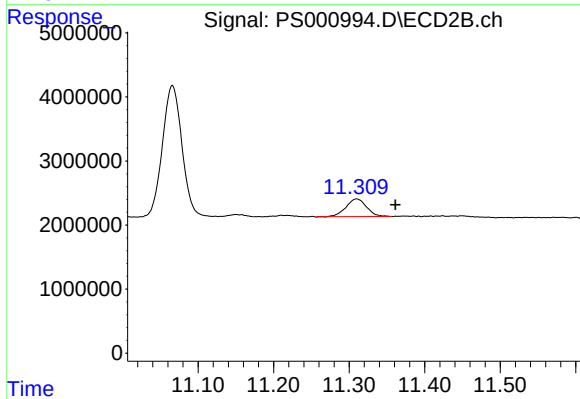

#5 DICAMBA


R.T.: 11.310 min
Delta R.T.: -0.051 min
Response: 5201371
Conc: 6.63 ng/ml

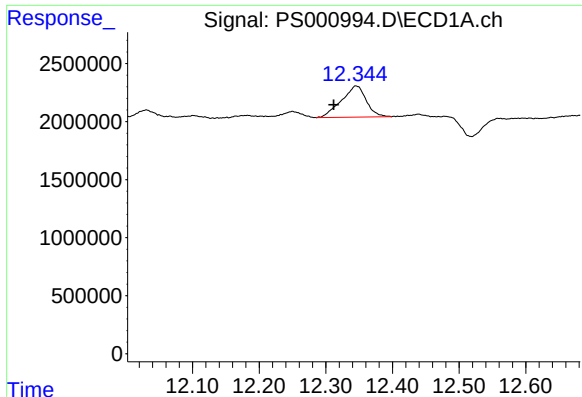

#6 MCP


R.T.: 12.346 min
Delta R.T.: 0.034 min
Response: 6964465
Conc: 12.68 ug/ml

Instrument :
ECD_S
ClientSampleId :

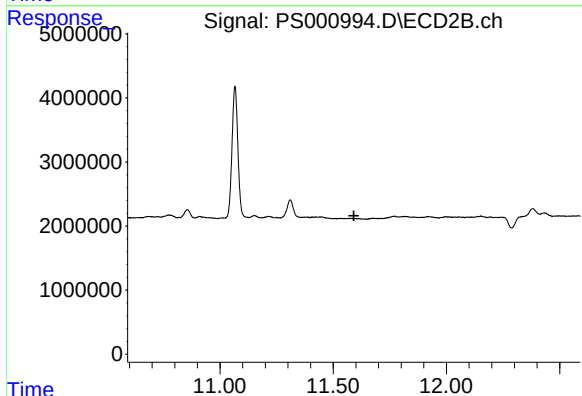


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

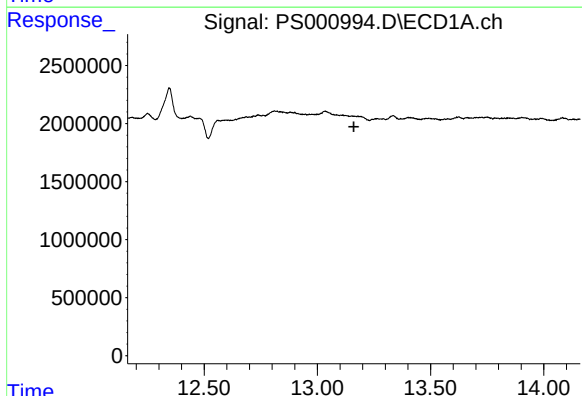


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

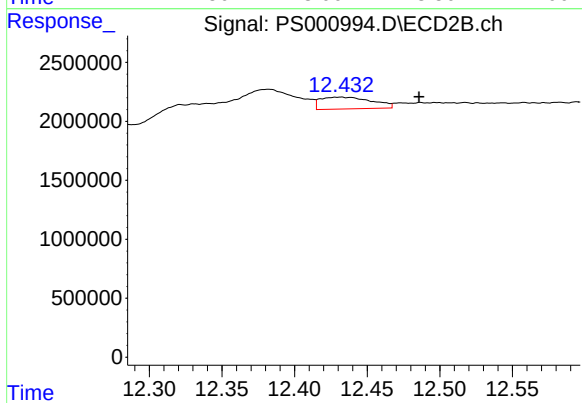

#8 DICHLORPROP


R.T.: 12.432 min
Delta R.T.: -0.054 min
Response: 2466575
Conc: 12.21 ng/ml

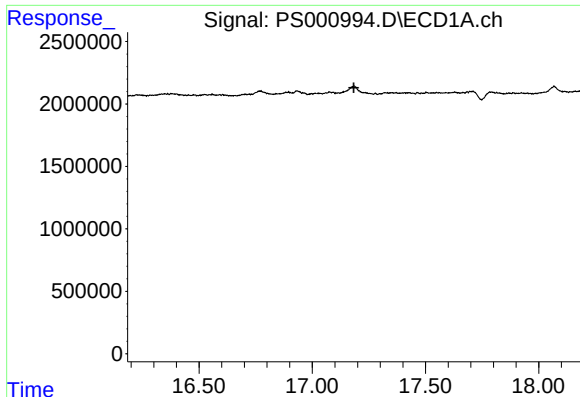

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 17.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

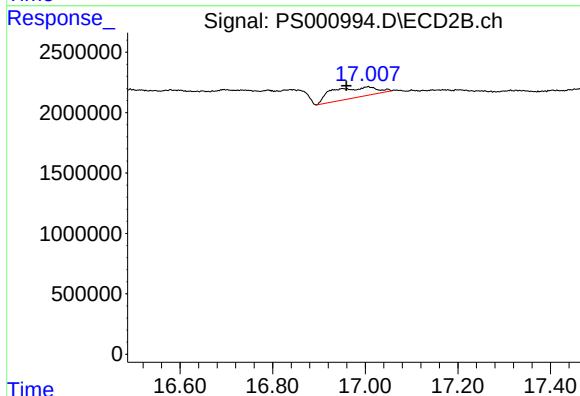


#15 Picloram

R.T.: 17.006 min
Delta R.T.: 0.047 min
Response: 5880572
Conc: 3.86 ng/ml

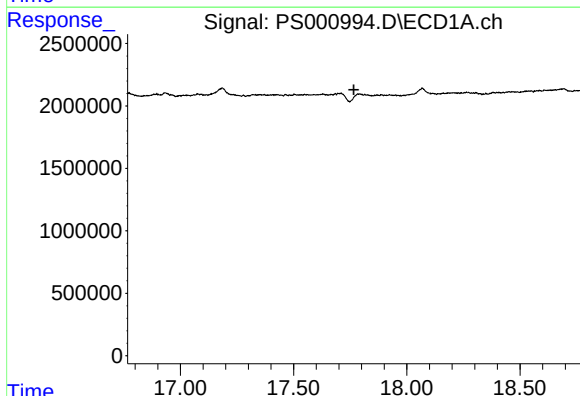

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.766 min
Response: 0
Conc: N.D.

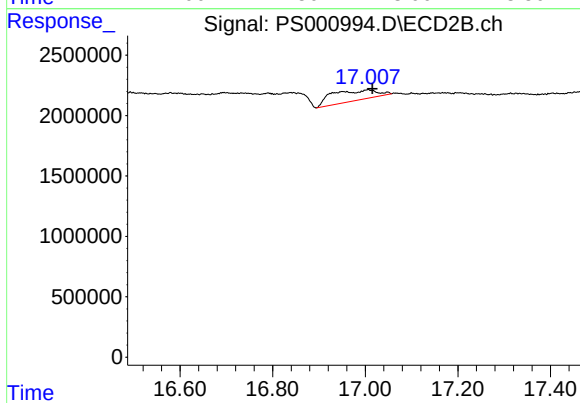

#16 DCPA

R.T.: 17.006 min
Delta R.T.: -0.009 min
Response: 5880572
Conc: 3.42 ng/ml