

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071218\
 Data File : PS000999.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2018 00:57
 Operator : UA
 Sample : J3947-28
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 01:38:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.631	11.045	82675896	69812073	400.717	320.537
Target Compounds							
2) T	3,5-DICHL...	0.000	9.284	0	42861646	N.D.	145.712 #
3) T	4-Nitroph...	11.225	0.000	13858364	0	101.038	N.D. #
5) T	DICAMBA	0.000	11.393	0	9417299	N.D.	11.997 #
6) T	MCP	12.324	0.000	6332361	0	11.528	N.D. #
7) T	MCPA	12.602	0.000	7952839	0	8.714	N.D. #
8) T	DICHLORPROP	0.000	12.416	0	1781853	N.D.	8.822 #
14) T	DINOSEB	0.000	15.742	0	6222247	N.D.	7.430 #
15) T	Picloram	17.161	16.988	528544	13091594	0.292	8.598 #
16) T	DCPA	17.765	16.988	18146689	13091594	12.465	7.615 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071218\
Data File : PS000999.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2018 00:57
Operator : UA
Sample : J3947-28
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 01:38:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

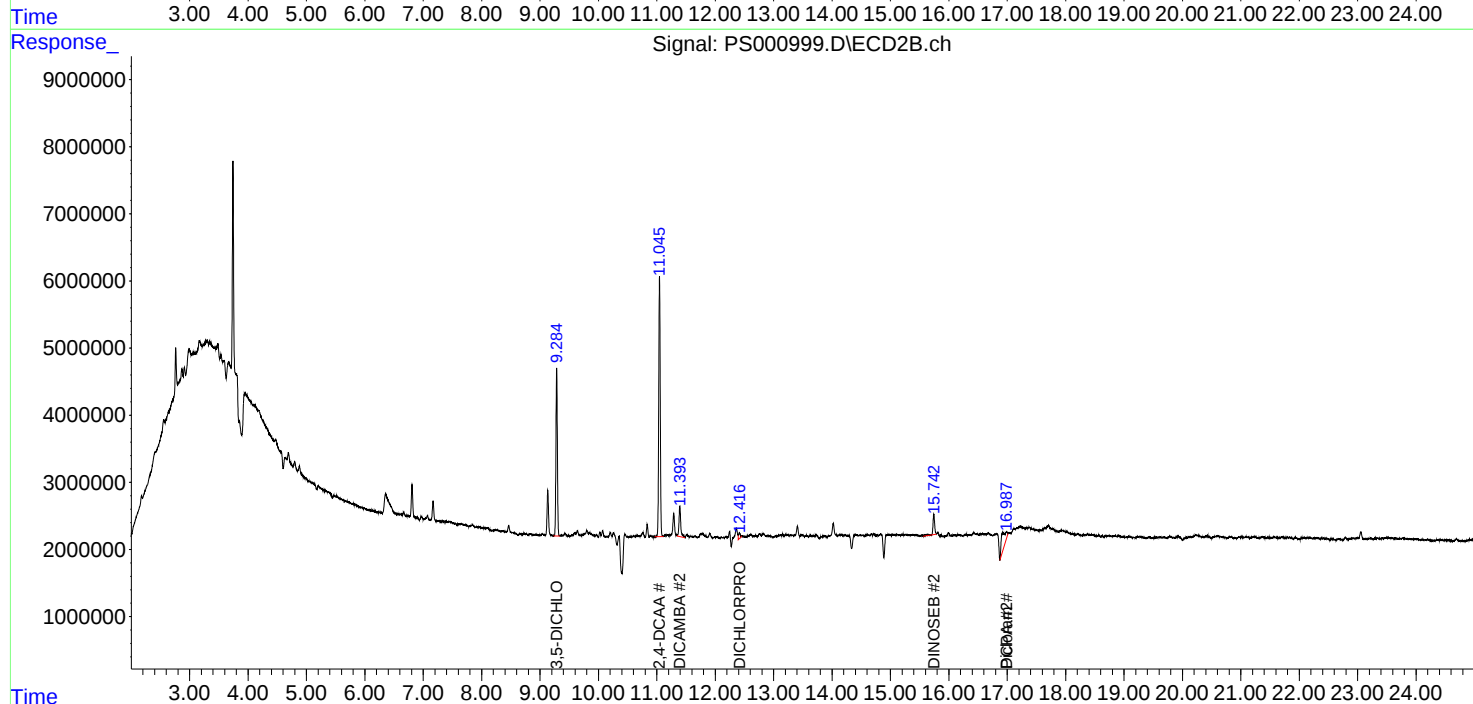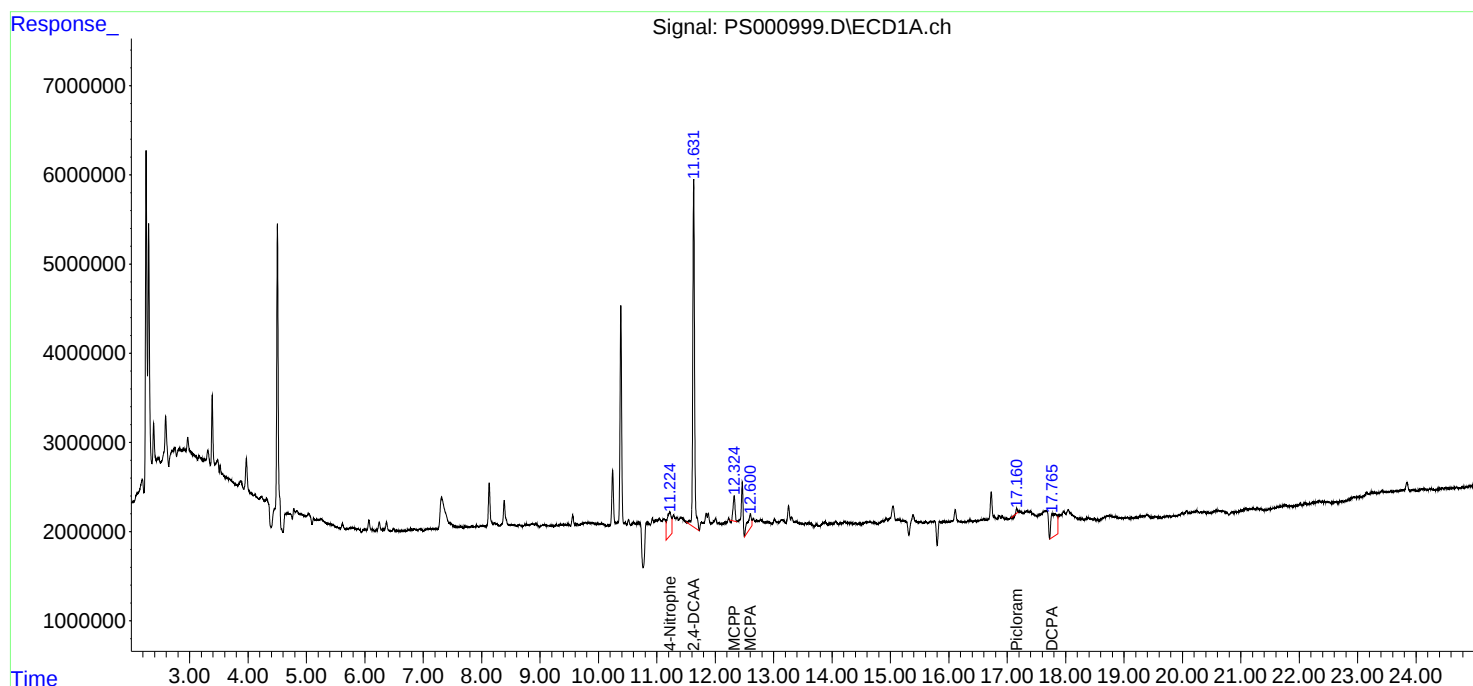


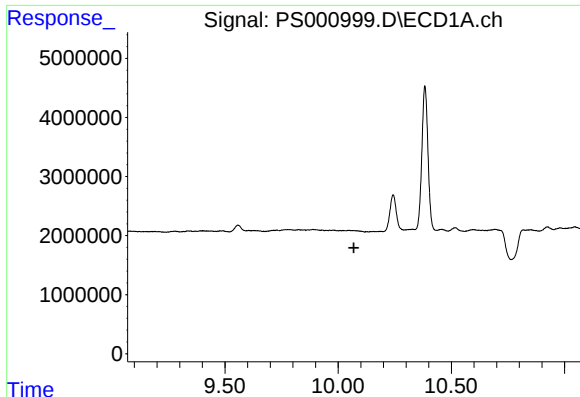

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

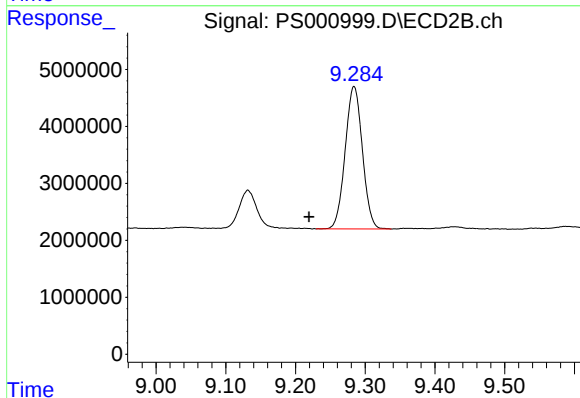


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.284 min
Delta R.T.: 0.065 min
Response: 42861646
Conc: 145.71 ng/ml

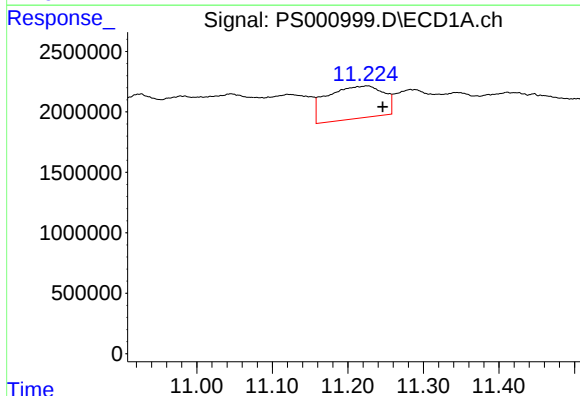


#3 4-Nitrophenol

R.T.: 11.225 min
Delta R.T.: -0.021 min
Response: 13858364
Conc: 101.04 ng/ml

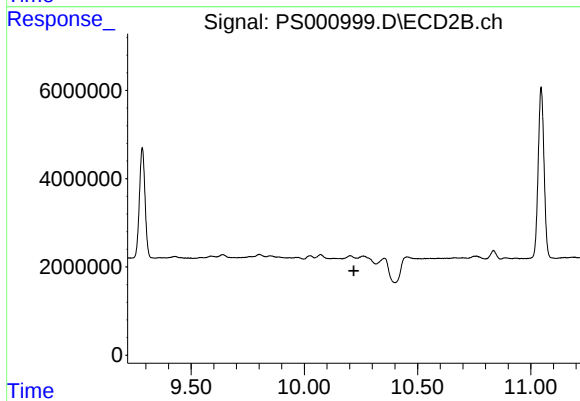

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.219 min
Response: 0
Conc: N.D.

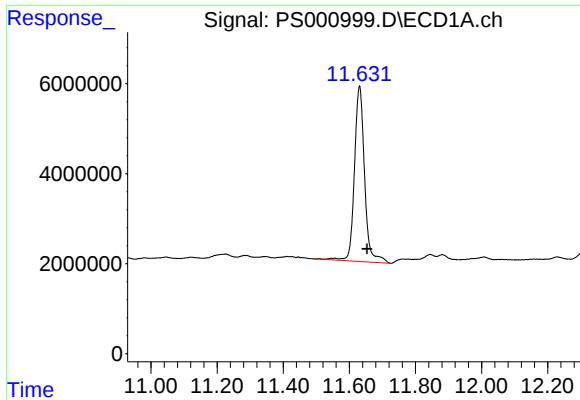

#4 2,4-DCAA


R.T.: 11.631 min
Delta R.T.: -0.023 min
Response: 82675896
Conc: 400.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

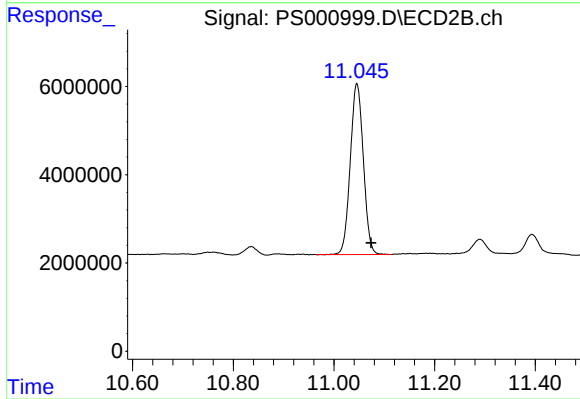


#4 2,4-DCAA

R.T.: 11.045 min
Delta R.T.: -0.028 min
Response: 69812073
Conc: 320.54 ng/ml

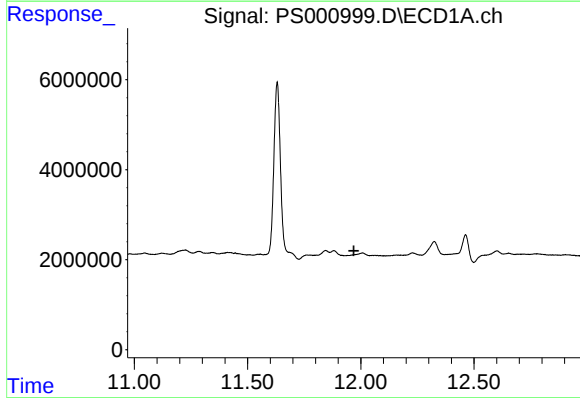


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.970 min
Response: 0
Conc: N.D.

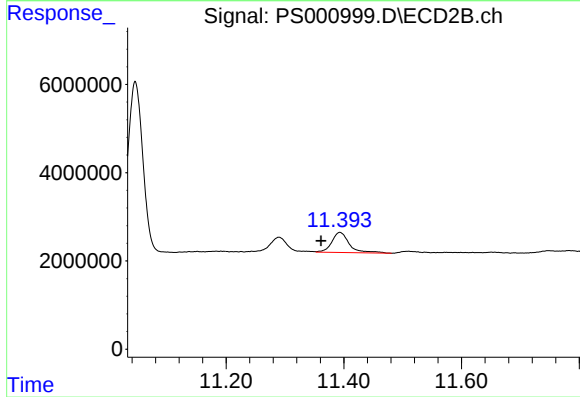

#5 DICAMBA


R.T.: 11.393 min
Delta R.T.: 0.032 min
Response: 9417299
Conc: 12.00 ng/ml

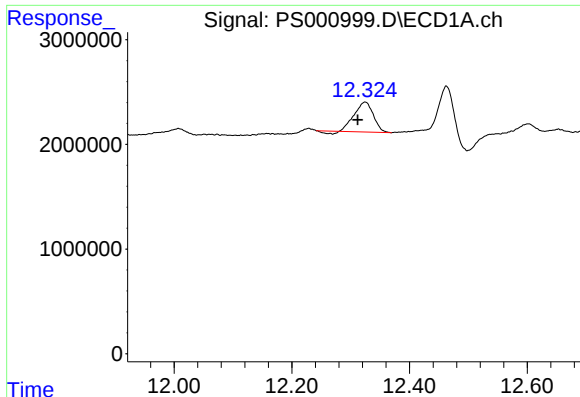

#6 MCPP


R.T.: 12.324 min
Delta R.T.: 0.012 min
Response: 6332361
Conc: 11.53 ug/ml

Instrument :
ECD_S
ClientSampleId :

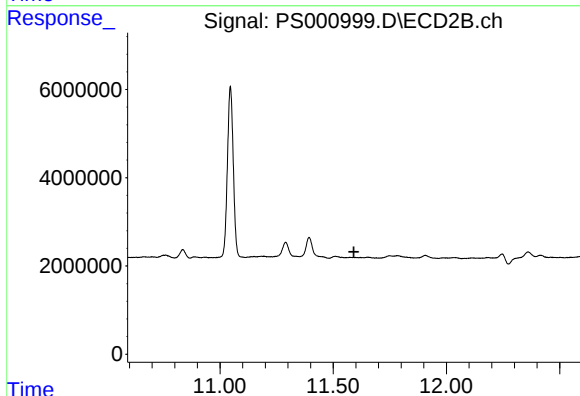


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

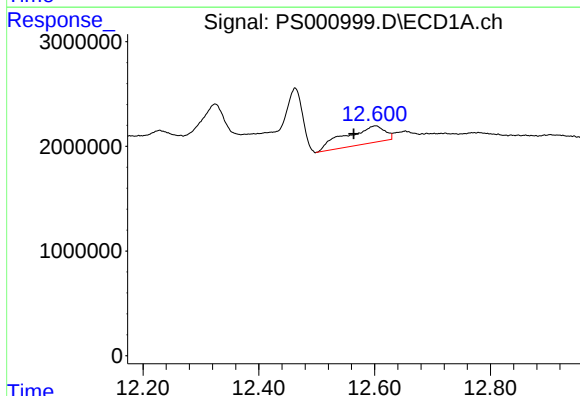


#7 MCPA

R.T.: 12.602 min
Delta R.T.: 0.038 min
Response: 7952839
Conc: 8.71 ug/ml

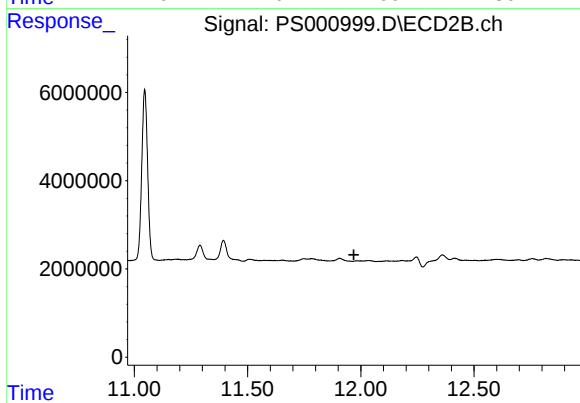

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 11.969 min
Response: 0
Conc: N.D.

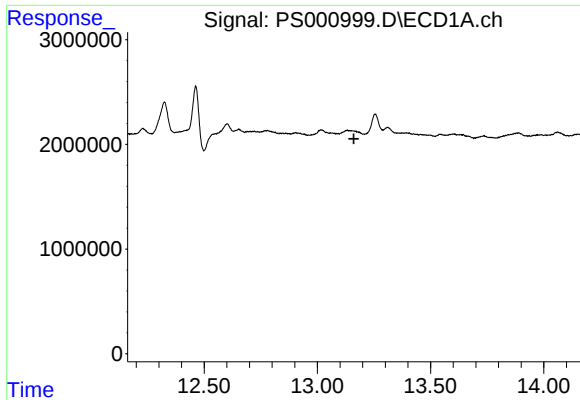

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.161 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

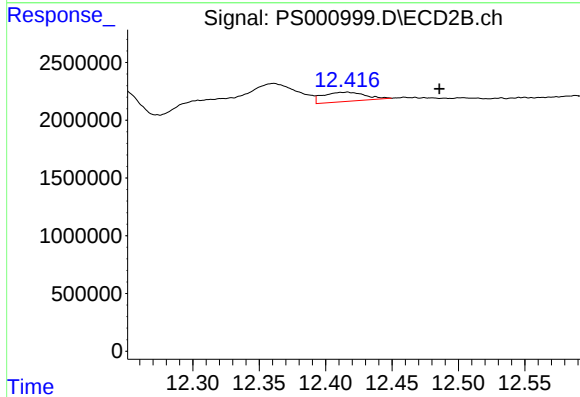


#8 DICHLORPROP

R.T.: 12.416 min
Delta R.T.: -0.069 min
Response: 1781853
Conc: 8.82 ng/ml

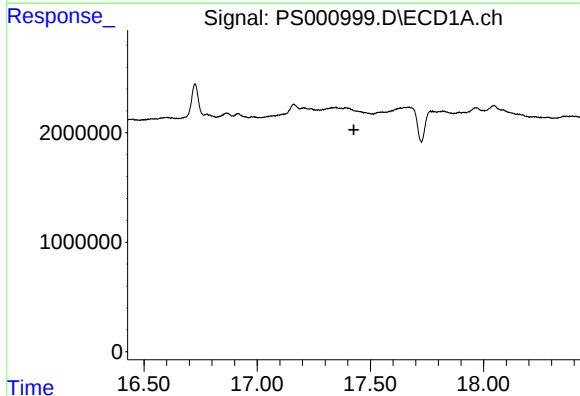


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.427 min
Response: 0
Conc: N.D.

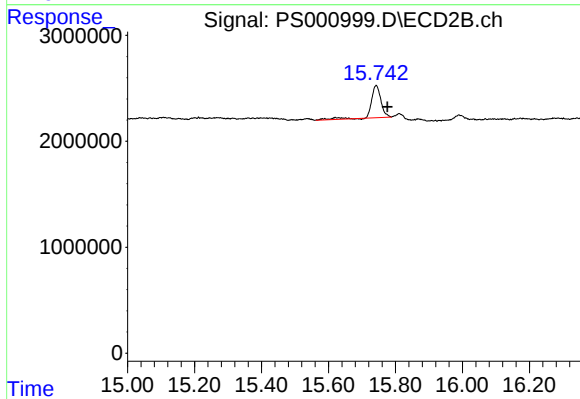

#14 DINOSEB


R.T.: 15.742 min
Delta R.T.: -0.034 min
Response: 6222247
Conc: 7.43 ng/ml

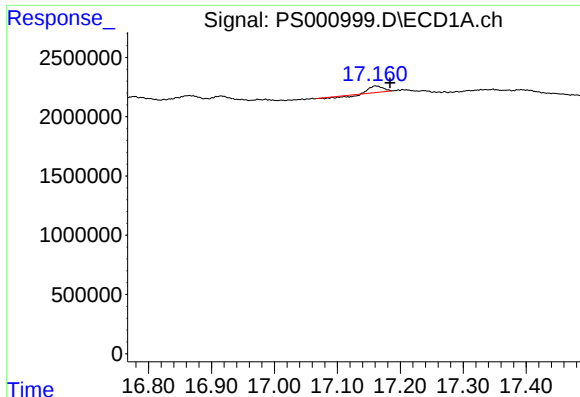

#15 Picloram


R.T.: 17.161 min
Delta R.T.: -0.022 min
Response: 528544
Conc: 0.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

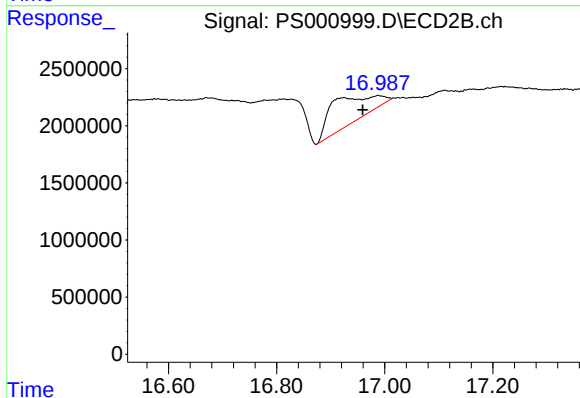


#15 Picloram

R.T.: 16.988 min
Delta R.T.: 0.029 min
Response: 13091594
Conc: 8.60 ng/ml

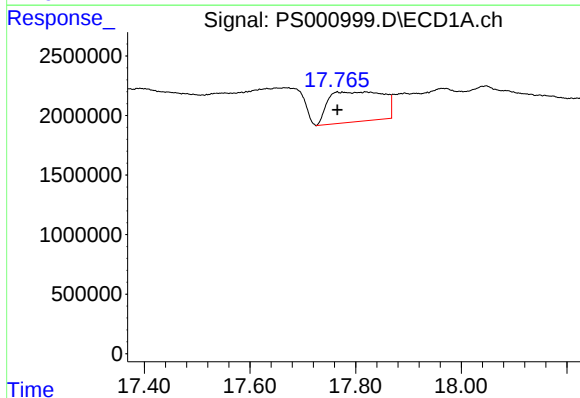

#16 DCPA

R.T.: 17.765 min
Delta R.T.: 0.000 min
Response: 18146689
Conc: 12.46 ng/ml

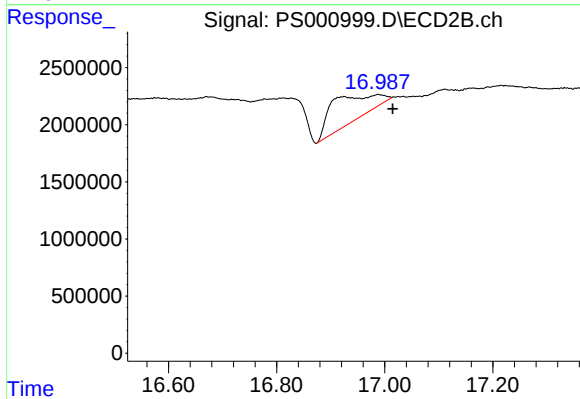

#16 DCPA

R.T.: 16.988 min
Delta R.T.: -0.027 min
Response: 13091594
Conc: 7.62 ng/ml