

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071222\
 Data File : PS019950.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2022 14:17
 Operator : AJ\MA
 Sample : PB146145TB
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 01:43:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 27 17:26:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	6.791	0	2590483	N.D.	3.190
Target Compounds							
2) T	3,5-DICHL...	6.436	0.000	241638	0	<MDL	N.D. #
3) T	4-Nitroph...	6.985f	0.000	1867832	0	1.755	N.D. #
5) T	DICAMBA	7.393	6.948	497582	1585686	<MDL	<MDL #
6) T	MCP	7.545	0.000	2544067	0	<MDL	N.D. #
7) T	MCPA	7.685	0.000	549.0E6	0	46.847	N.D. #
9) T	2,4-D	0.000	7.856	0	484666	N.D.	<MDL
10) T	Pentachlo...	8.616	8.283	2936910	1046120	<MDL	<MDL #
11) T	2,4,5-TP ...	9.181	8.654	2976598	698849	<MDL	<MDL #
12) T	2,4,5-T	9.428	9.060f	91935485	430646	4.996	<MDL #
13) T	2,4-DB	9.973	9.472f	788103	789073	<MDL	1.215 #
14) T	DINOSEB	0.000	9.851	0	665283	N.D.	<MDL
15) T	Picloram	10.967	10.878f	1161721	108.4E6	<MDL	16.670 #
16) T	DCPA	11.418	10.775	3148346	2073514	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071222\
Data File : PS019950.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2022 14:17
Operator : AJ\MA
Sample : PB146145TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 01:43:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
Quant Title : 8080.M
QLast Update : Mon Jun 27 17:26:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

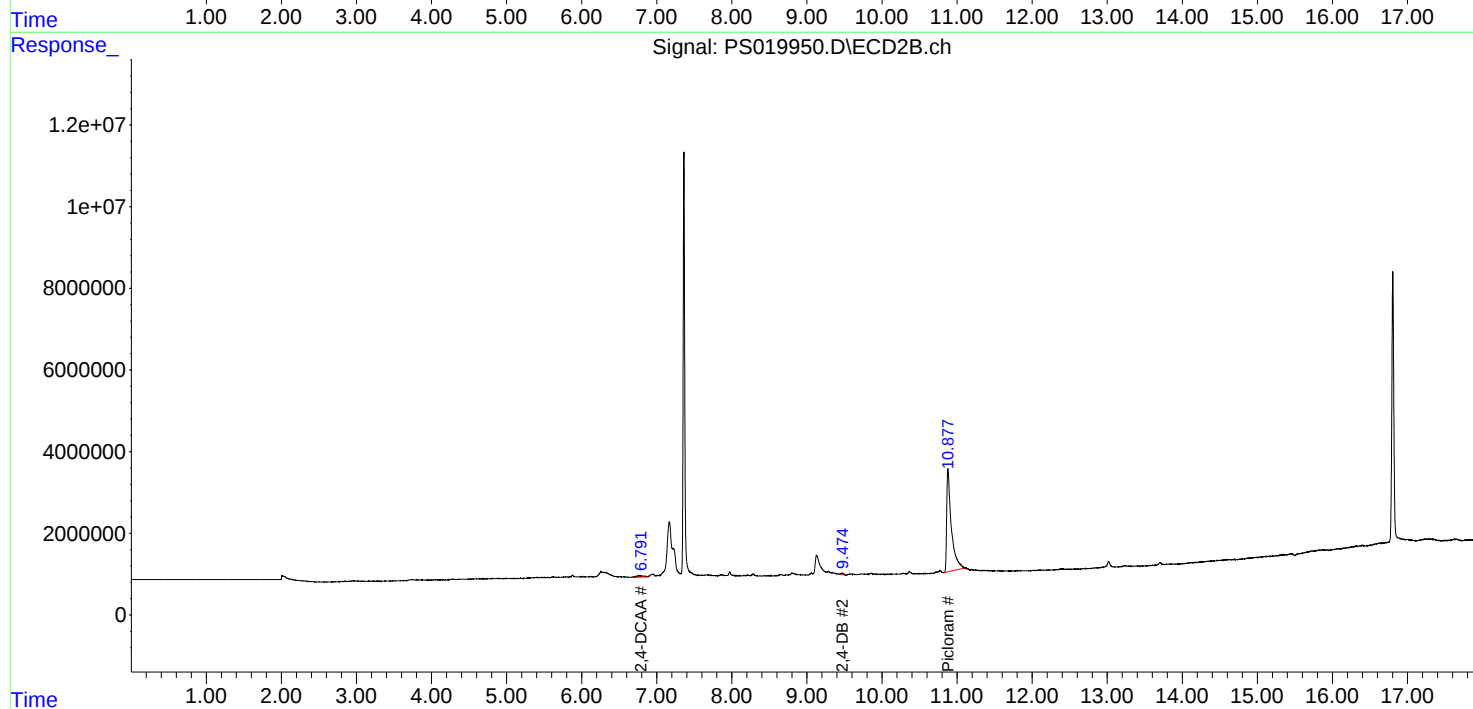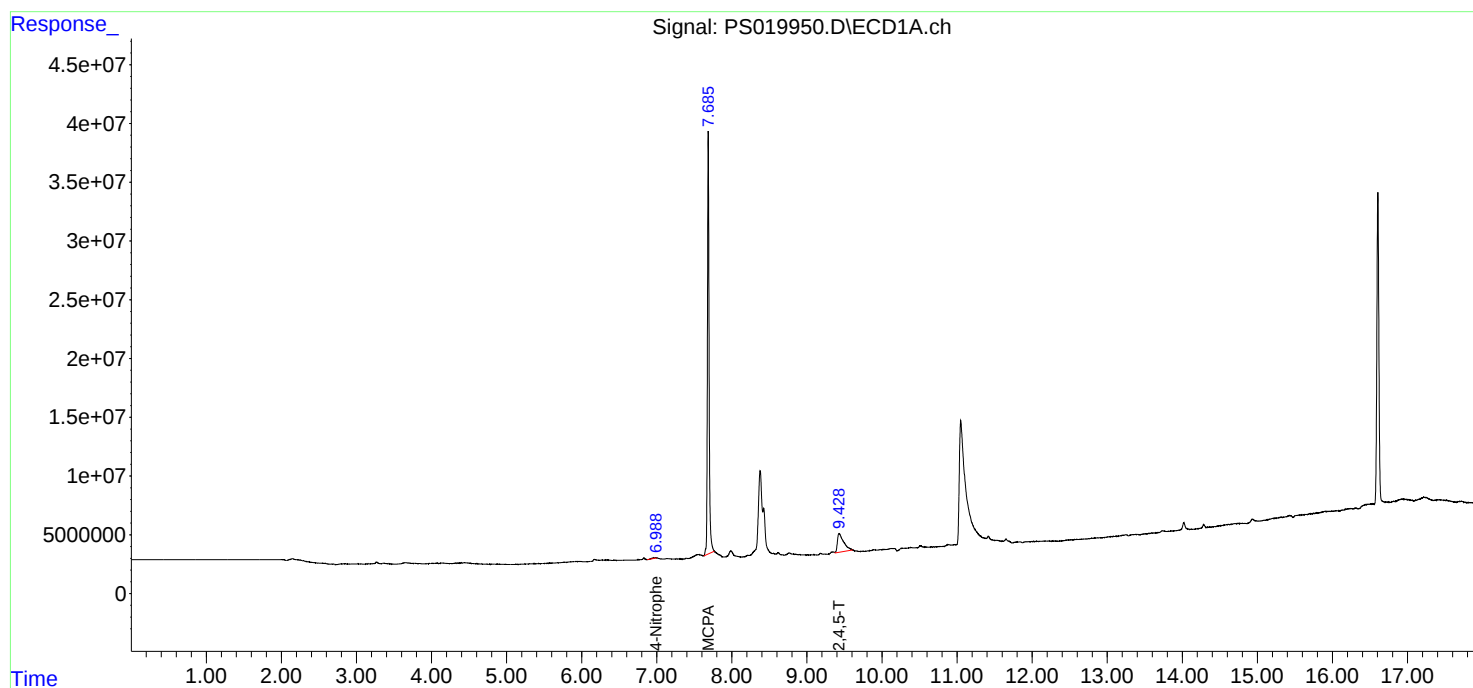


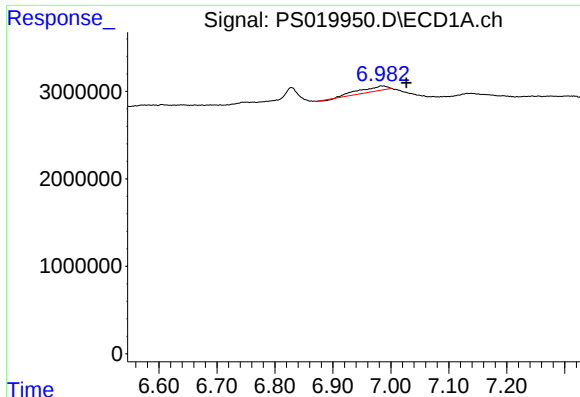

#3 4-Nitrophenol


R.T.: 6.985 min
Delta R.T.: -0.041 min
Response: 1867832
Conc: 1.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

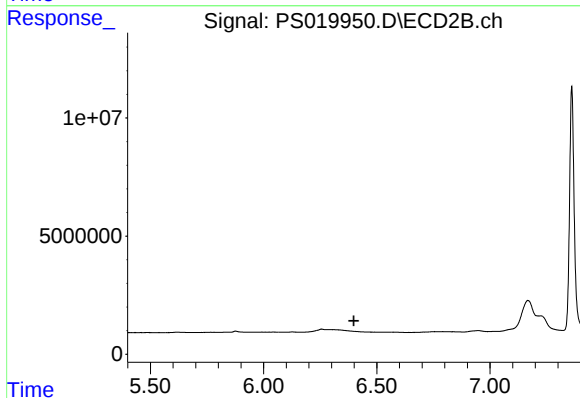


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

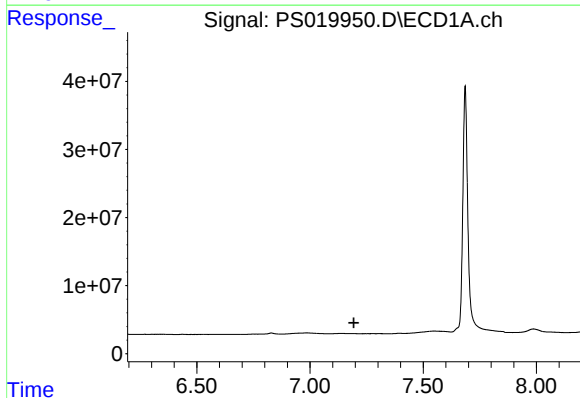


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.194 min
Response: 0
Conc: N.D.

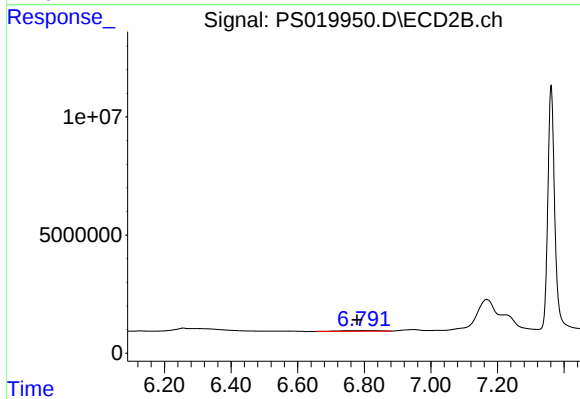

#4 2,4-DCAA


R.T.: 6.791 min
Delta R.T.: 0.013 min
Response: 2590483
Conc: 3.19 ng/ml

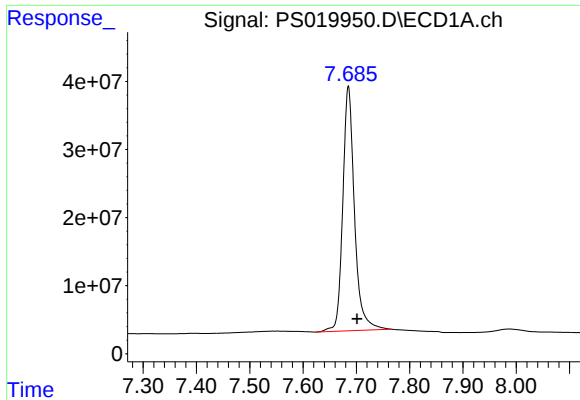

#7 MCPA


R.T.: 7.685 min
Delta R.T.: -0.016 min
Response: 548950095
Conc: 46.85 ug/ml

Instrument :
ECD_S
ClientSampleId :

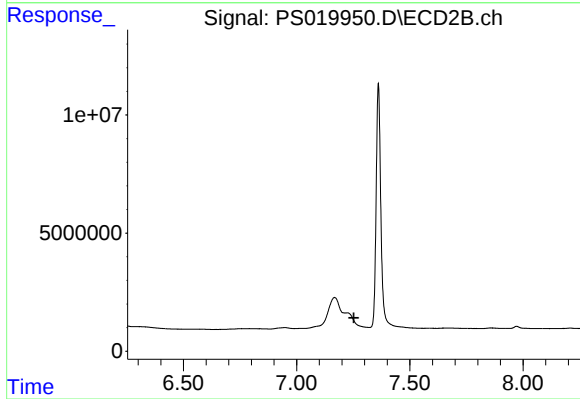


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

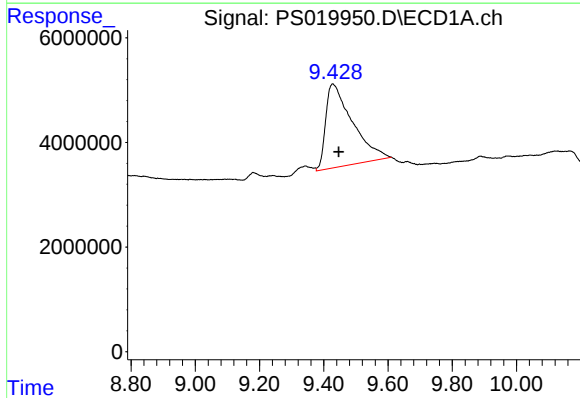


#12 2,4,5-T

R.T.: 9.428 min
Delta R.T.: -0.019 min
Response: 91935485
Conc: 5.00 ng/ml

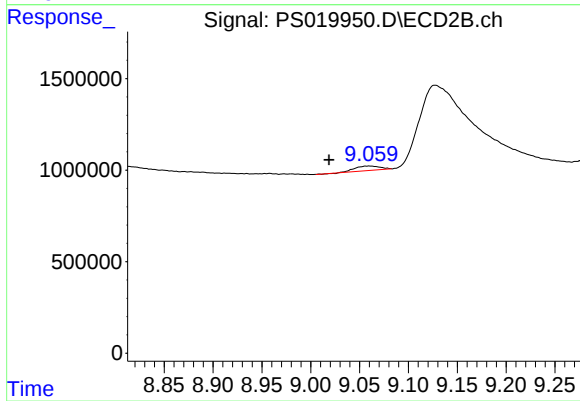

#12 2,4,5-T


R.T.: 9.060 min
Delta R.T.: 0.041 min
Response: 430646
Conc: N.D.

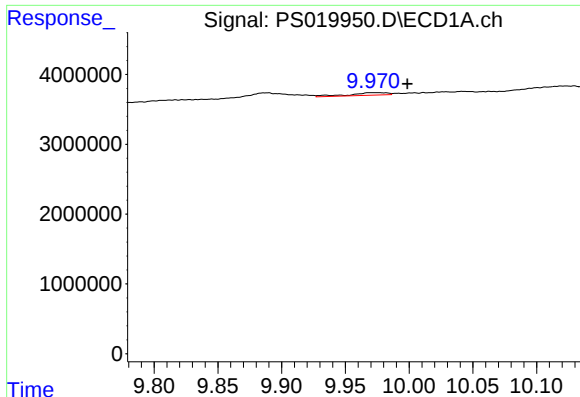

#13 2,4-DB


R.T.: 9.973 min
Delta R.T.: -0.026 min
Response: 788103
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

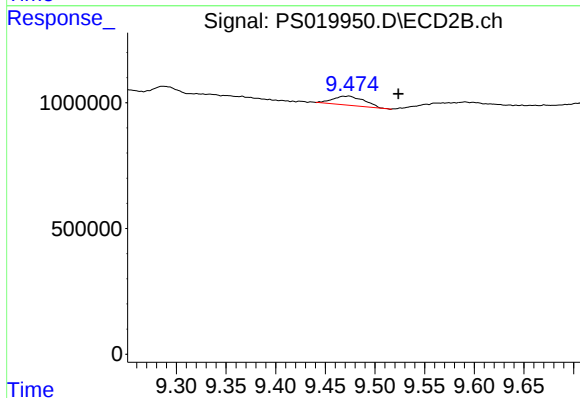


#13 2,4-DB

R.T.: 9.472 min
Delta R.T.: -0.052 min
Response: 789073
Conc: 1.21 ng/ml

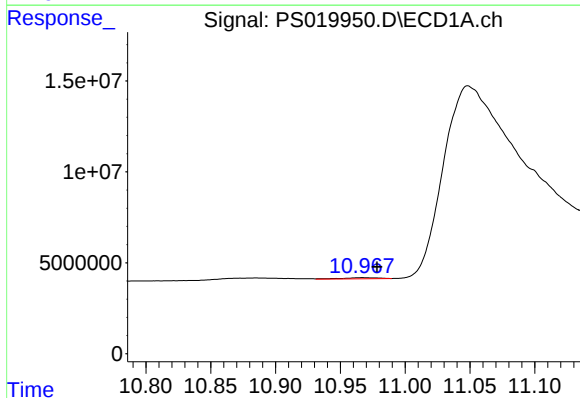

#15 Picloram

R.T.: 10.967 min
Delta R.T.: -0.011 min
Response: 1161721
Conc: N.D.

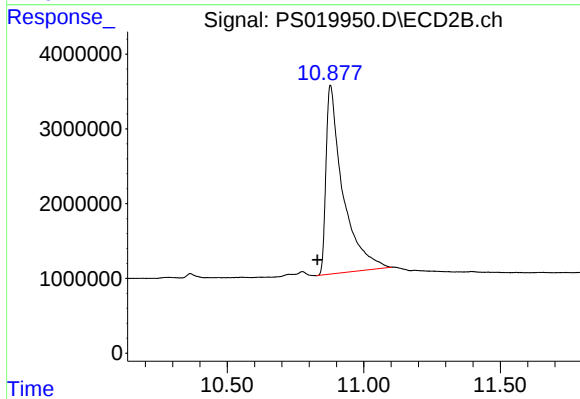

#15 Picloram

R.T.: 10.878 min
Delta R.T.: 0.048 min
Response: 108416368
Conc: 16.67 ng/ml