

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071223\
 Data File : PS023705.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2023 09:41
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 20:32:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070723.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 07 18:46:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.357	0.000	1248602	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.475	2.585	-127213	4831661	N.D.	6.903
2) T	3,5-DICHL...	5.753	0.000	1446007	0	<MDL	N.D. #
3) T	4-Nitroph...	6.208	0.000	2298389	0	2.568	N.D. #
5) T	DICAMBA	6.517	6.988	2748324	1316887	<MDL	<MDL #
8) T	DICHLORPROP	7.114	0.000	14396	0	<MDL	N.D. #
9) T	2,4-D	7.312	0.000	1643903	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.108f	0.000	795790	0	<MDL	N.D. #
12) T	2,4,5-T	8.324	9.078	890575	2724090	<MDL	1.116 #
13) T	2,4-DB	8.828	0.000	1665812	0	1.692	N.D. #
14) T	DINOSEB	9.885	0.000	985187	0	<MDL	N.D. #
15) T	Picloram	9.711	10.828	34422546	10137809	2.936	2.397
16) T	DCPA	10.150	10.777	465682	308511	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071223\
Data File : PS023705.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2023 09:41
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 20:32:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070723.M
Quant Title : 8080.M
QLast Update : Fri Jul 07 18:46:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

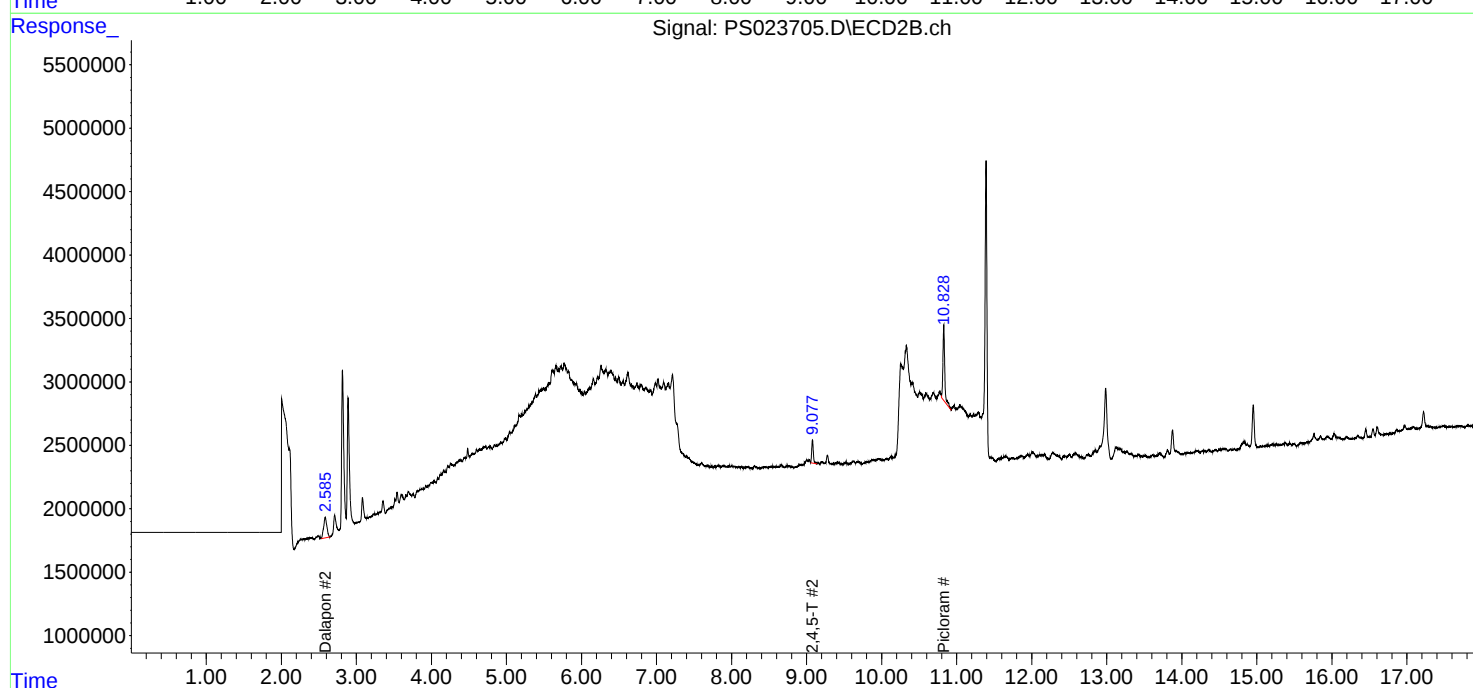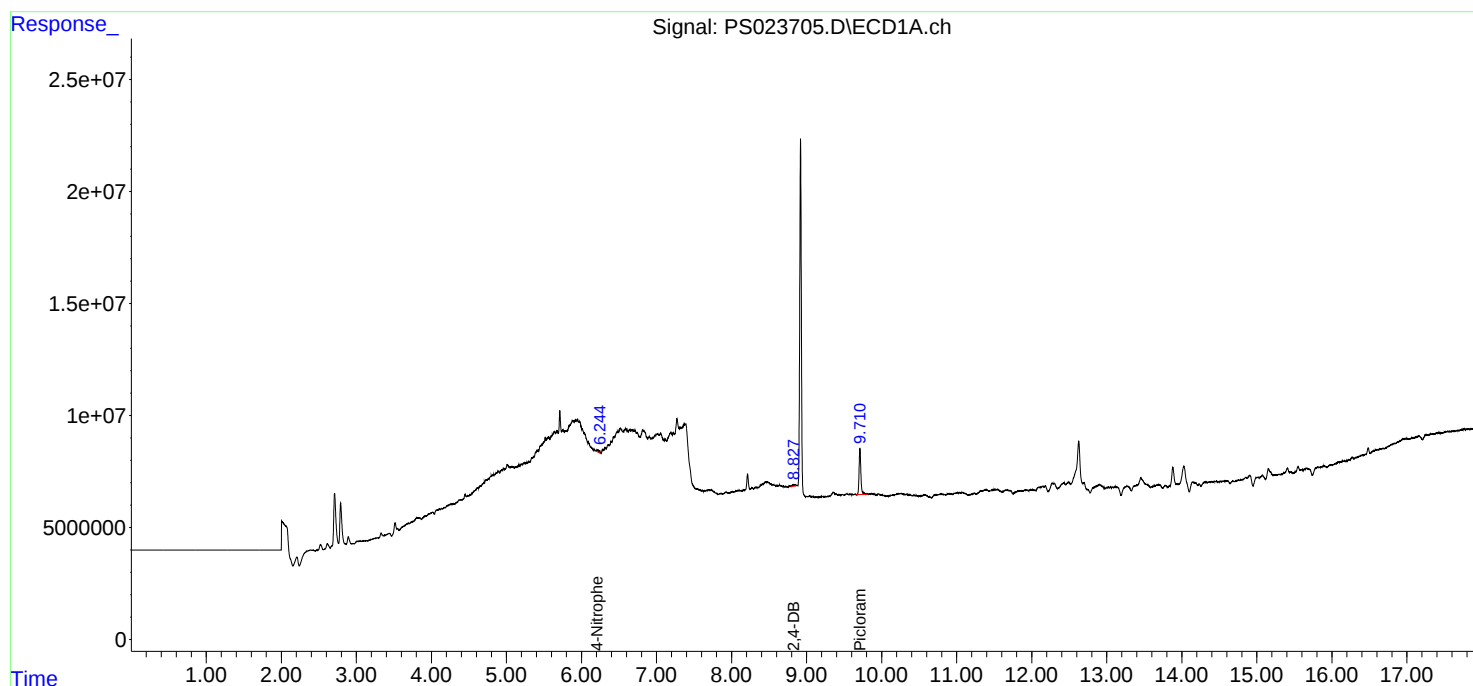


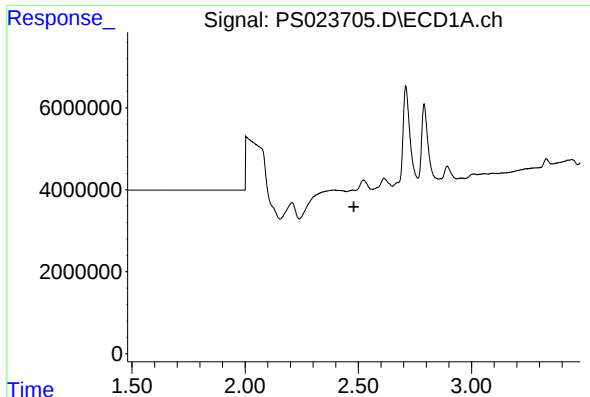

#1 Dalapon


R.T.: 2.475 min
Delta R.T.: -0.005 min
Response: -127213
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

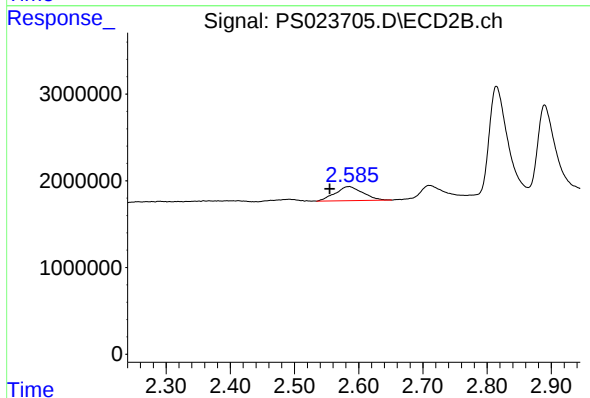


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: 0.030 min
Response: 4831661
Conc: 6.90 ng/ml

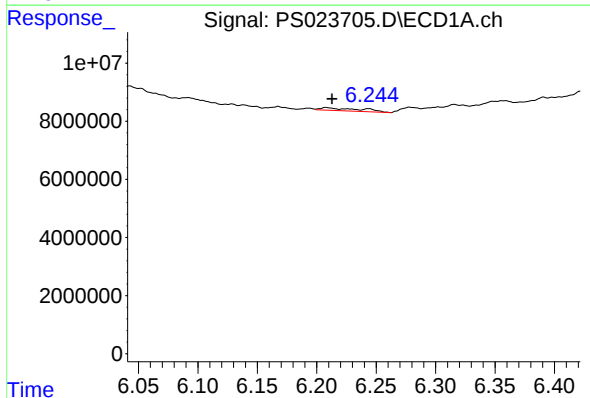


#3 4-Nitrophenol

R.T.: 6.208 min
Delta R.T.: -0.005 min
Response: 2298389
Conc: 2.57 ng/ml

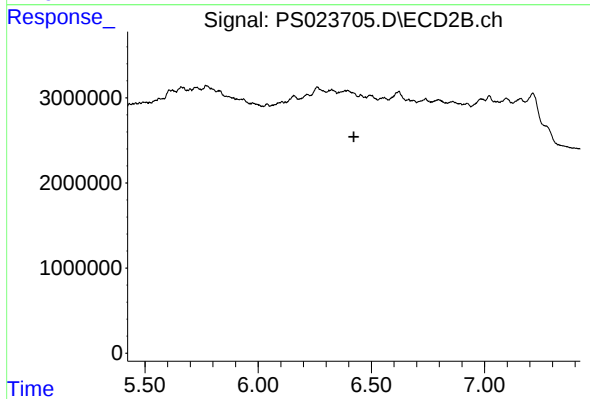

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.423 min
Response: 0
Conc: N.D.

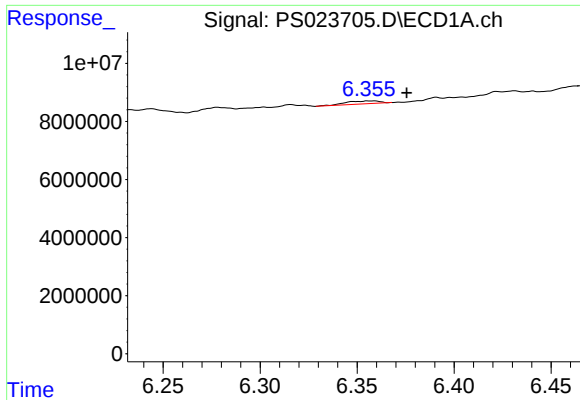

#4 2,4-DCAA


R.T.: 6.357 min
Delta R.T.: -0.019 min
Response: 1248602
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

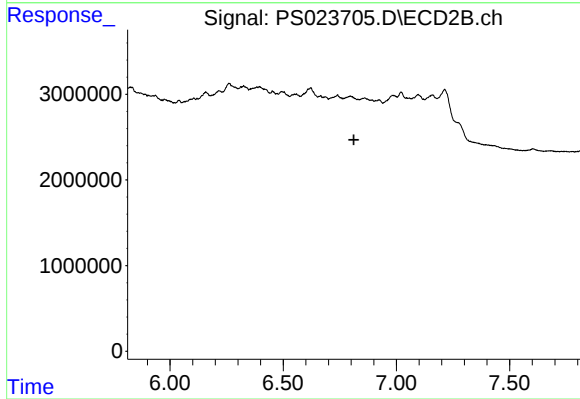


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.812 min
Response: 0
Conc: N.D.

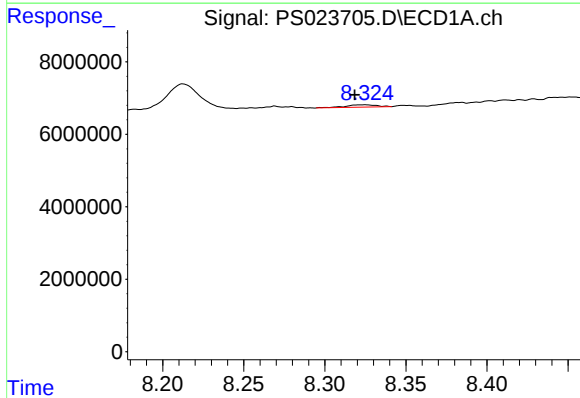


#12 2,4,5-T

R.T.: 8.324 min
Delta R.T.: 0.005 min
Response: 890575
Conc: N.D.

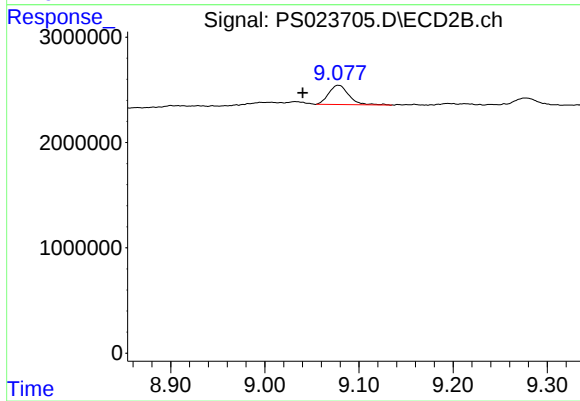

#12 2,4,5-T


R.T.: 9.078 min
Delta R.T.: 0.038 min
Response: 2724090
Conc: 1.12 ng/ml

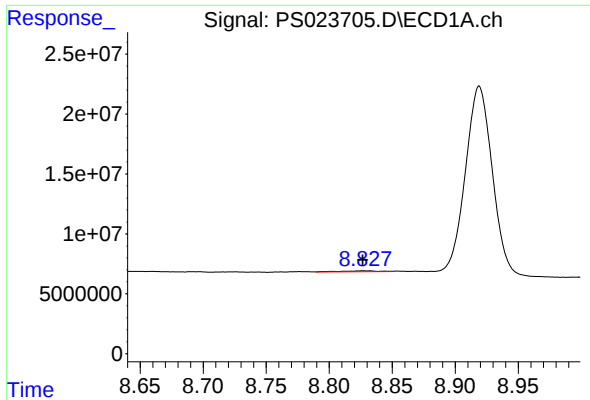

#13 2,4-DB


R.T.: 8.828 min
Delta R.T.: 0.002 min
Response: 1665812
Conc: 1.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

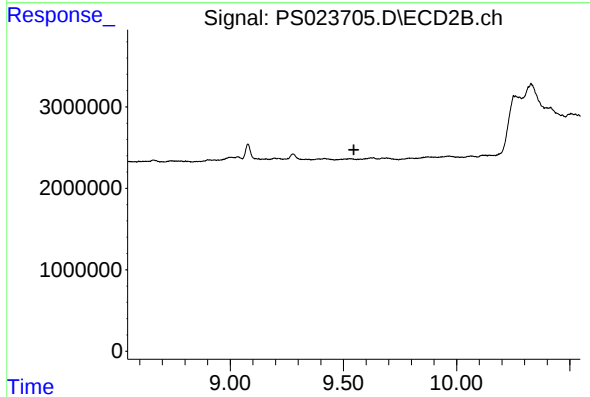


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.546 min
Response: 0
Conc: N.D.

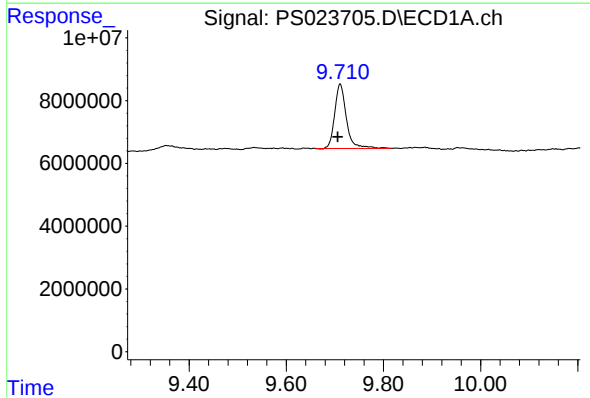

#15 Picloram

R.T.: 9.711 min
Delta R.T.: 0.005 min
Response: 34422546
Conc: 2.94 ng/ml

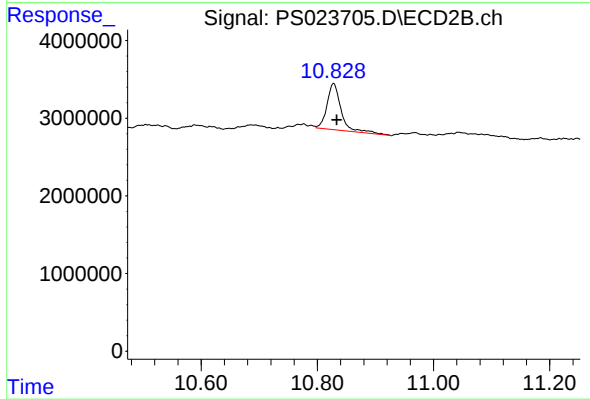

#15 Picloram

R.T.: 10.828 min
Delta R.T.: -0.005 min
Response: 10137809
Conc: 2.40 ng/ml