

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071223\
 Data File : PS023709.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2023 12:35
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 20:37:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070723.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 07 18:46:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.376	6.807	471.4E6	142.3E6	373.240	339.211
Target Compounds							
1) T	Dalapon	0.000	2.584	0	778212	N.D.	1.112
2) T	3,5-DICHL...	5.745	0.000	425261	0	<MDL	N.D. #
3) T	4-Nitroph...	6.216	0.000	3808717	0	4.256	N.D. #
5) T	DICAMBA	6.523	0.000	358713	0	<MDL	N.D. #
8) T	DICHLORPROP	7.130	7.604	-159797	991235	N.D.	2.130
9) T	2,4-D	0.000	7.863	0	540817	N.D.	1.000
10) T	Pentachlo...	7.538	8.301	296689	910343	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	8.626f	0	282829	N.D.	<MDL
12) T	2,4,5-T	8.269f	8.974f	2388229	854582	<MDL	<MDL #
13) T	2,4-DB	8.792	9.497f	34245548	653105	34.778	2.099 #
14) T	DINOSEB	9.878	0.000	1508490	0	<MDL	N.D. #
15) T	Picloram	0.000	10.797	0	8115629	N.D.	1.919
16) T	DCPA	0.000	10.797	0	8115629	N.D.	2.925



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071223\
Data File : PS023709.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2023 12:35
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 20:37:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070723.M
Quant Title : 8080.M
QLast Update : Fri Jul 07 18:46:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

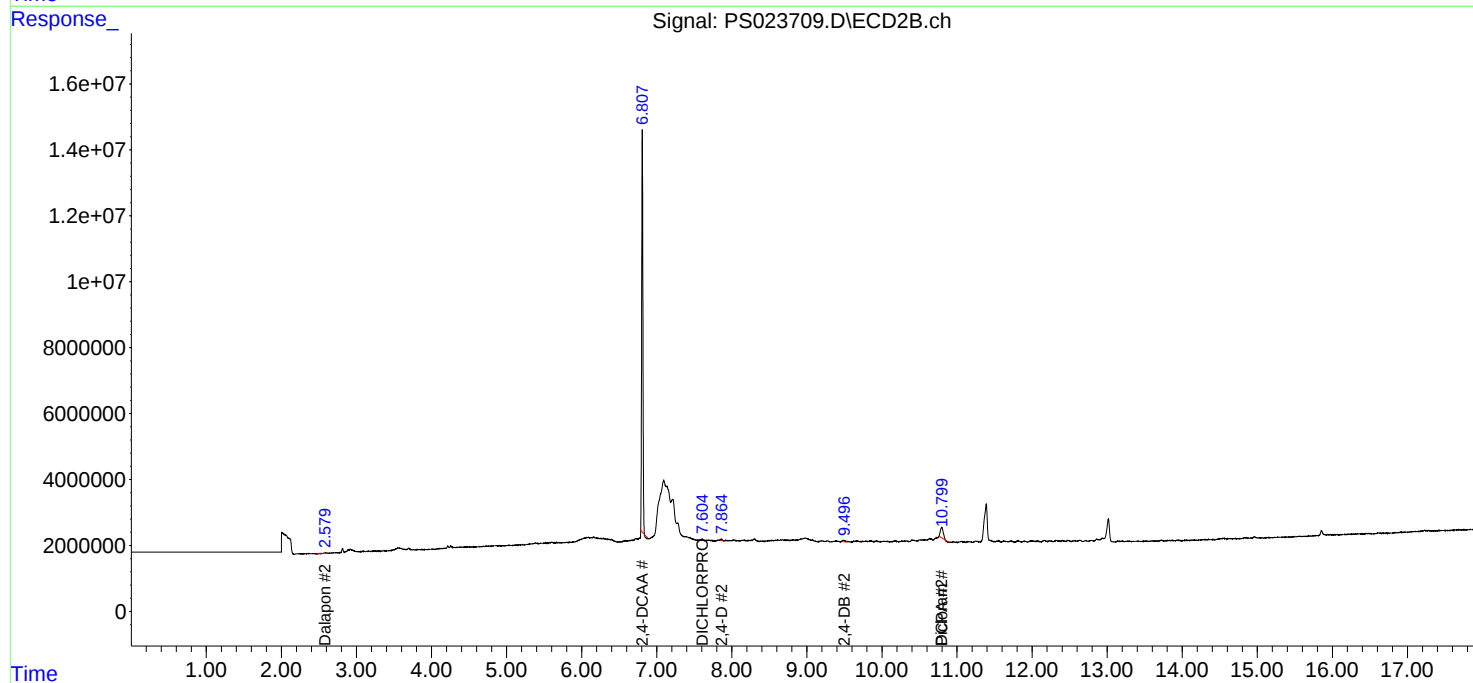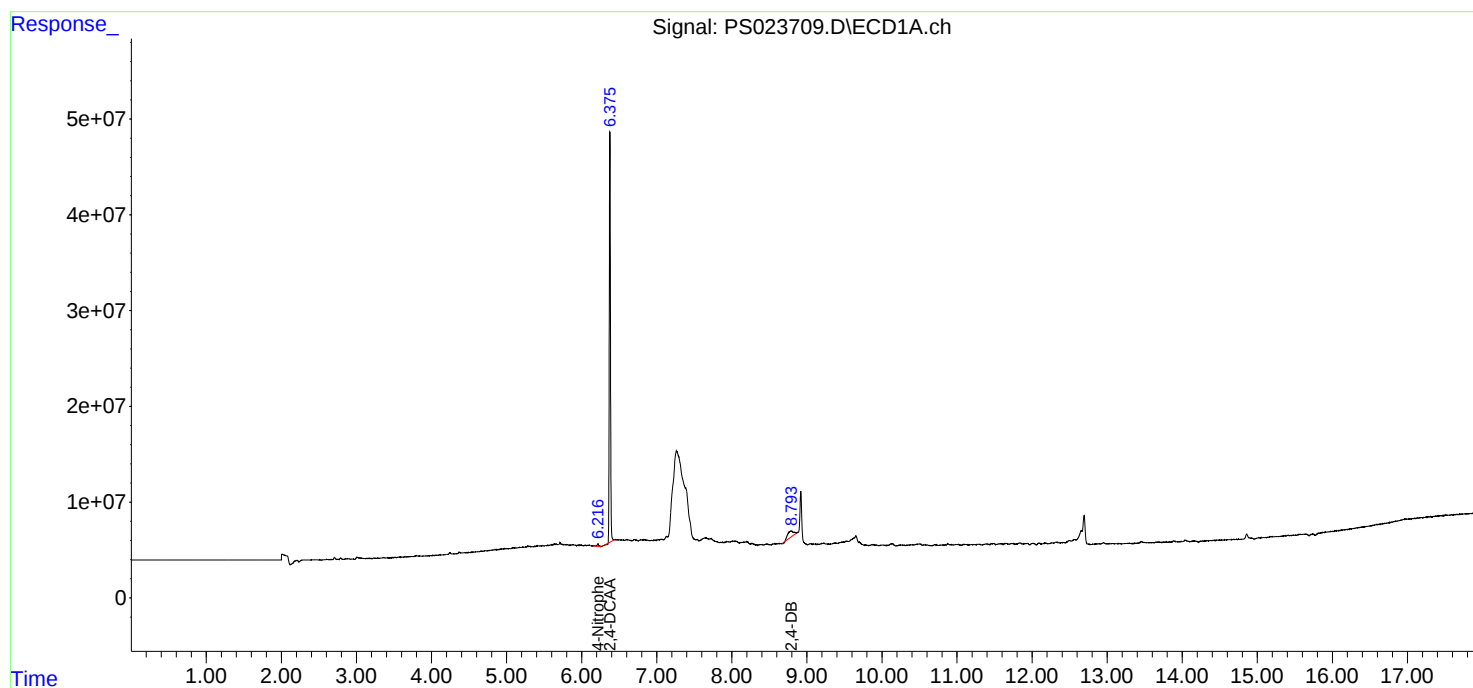


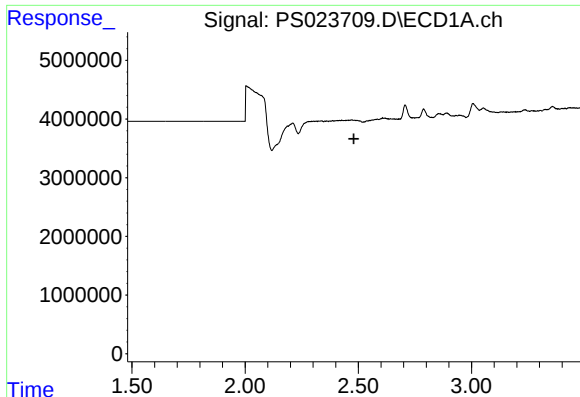

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.480 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

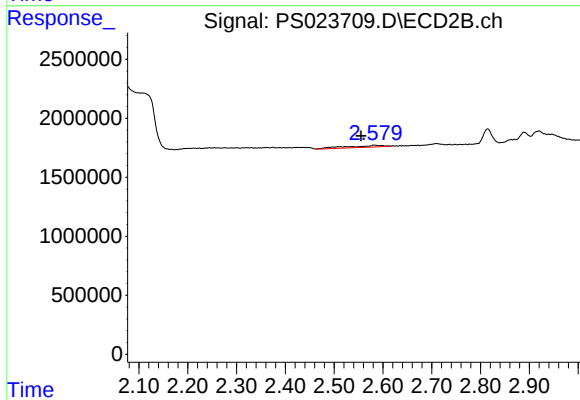


#1 Dalapon

R.T.: 2.584 min
Delta R.T.: 0.029 min
Response: 778212
Conc: 1.11 ng/ml

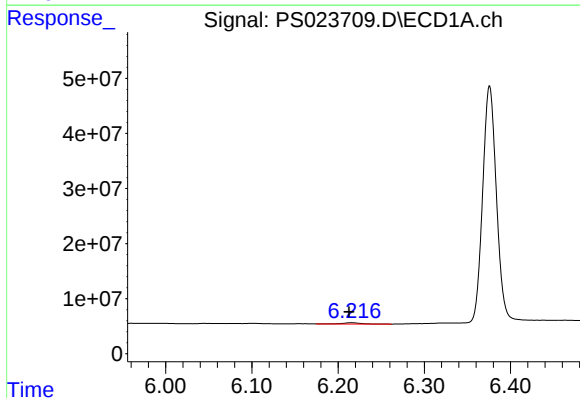


#3 4-Nitrophenol

R.T.: 6.216 min
Delta R.T.: 0.003 min
Response: 3808717
Conc: 4.26 ng/ml

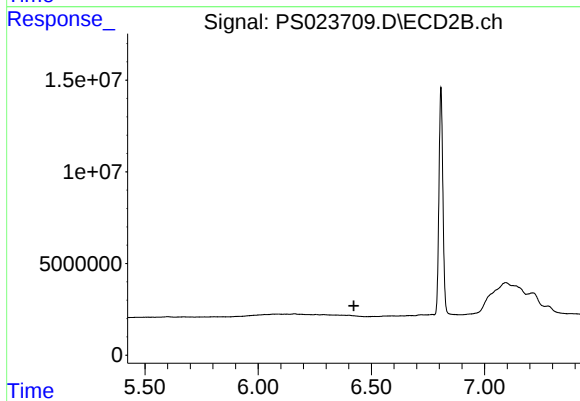

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.423 min
Response: 0
Conc: N.D.

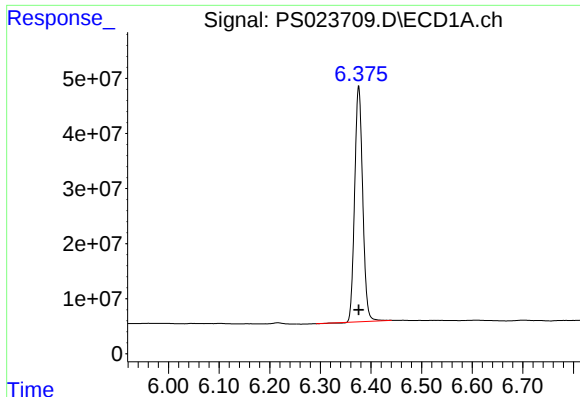

#4 2,4-DCAA


R.T.: 6.376 min
Delta R.T.: 0.000 min
Response: 471404825
Conc: 373.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

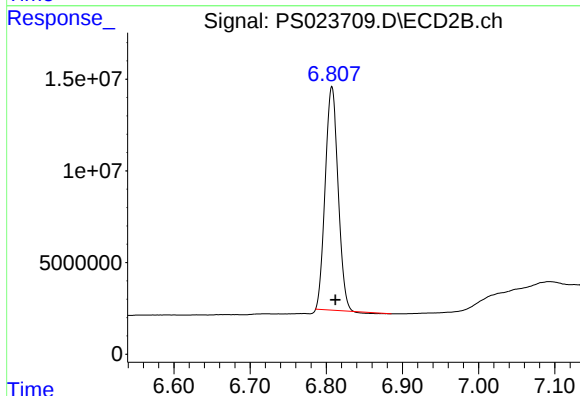


#4 2,4-DCAA

R.T.: 6.807 min
Delta R.T.: -0.005 min
Response: 142279349
Conc: 339.21 ng/ml

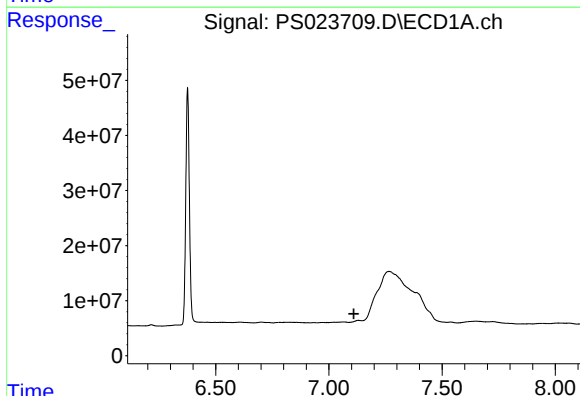


#8 DICHLORPROP

R.T.: 7.130 min
Delta R.T.: 0.020 min
Response: -159797
Conc: N.D.

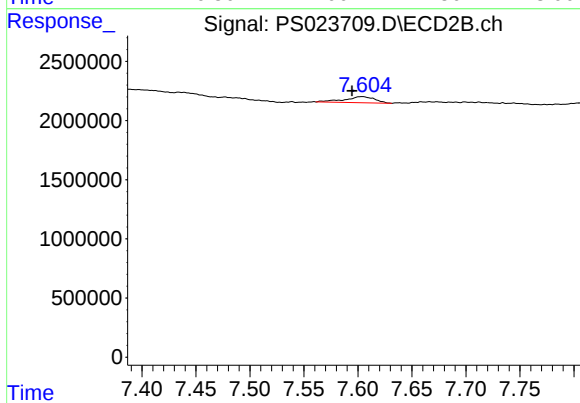

#8 DICHLORPROP


R.T.: 7.604 min
Delta R.T.: 0.009 min
Response: 991235
Conc: 2.13 ng/ml

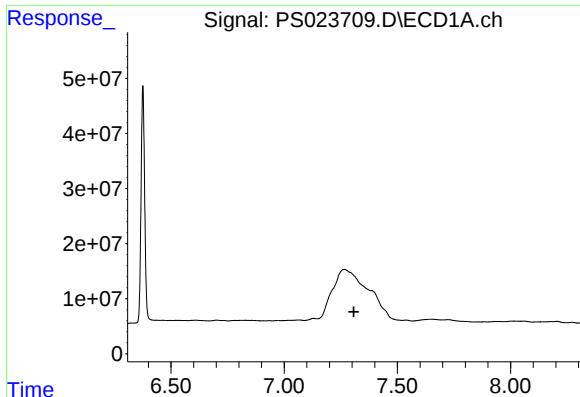

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.308 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

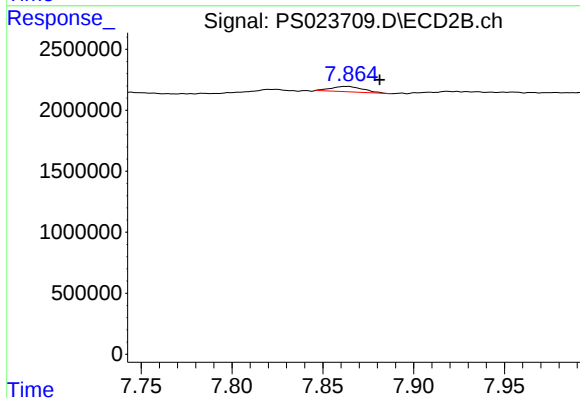


#9 2,4-D

R.T.: 7.863 min
Delta R.T.: -0.018 min
Response: 540817
Conc: 1.00 ng/ml

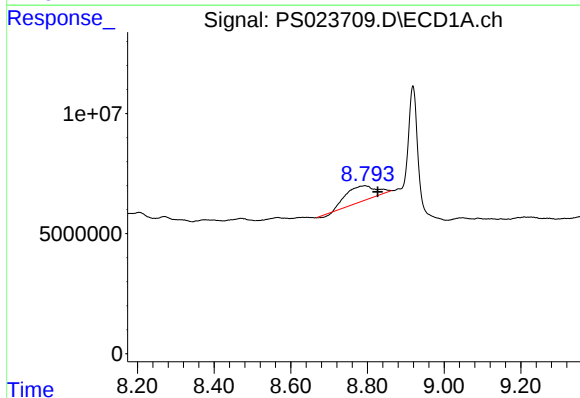


#13 2,4-DB

R.T.: 8.792 min
Delta R.T.: -0.035 min
Response: 34245548
Conc: 34.78 ng/ml

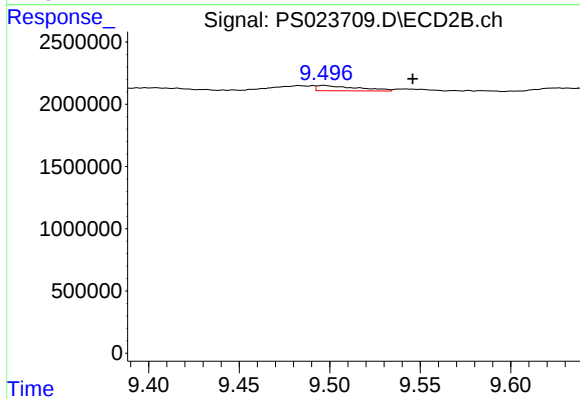

#13 2,4-DB


R.T.: 9.497 min
Delta R.T.: -0.049 min
Response: 653105
Conc: 2.10 ng/ml

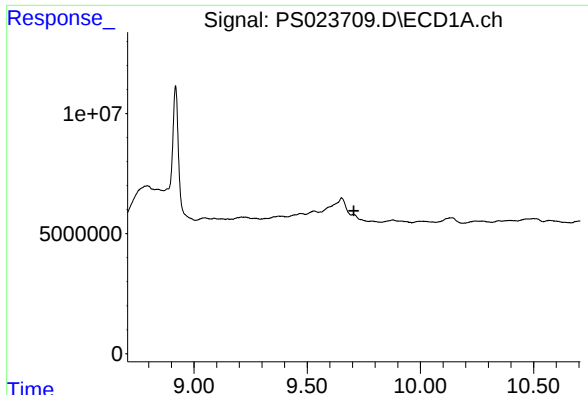

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 9.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

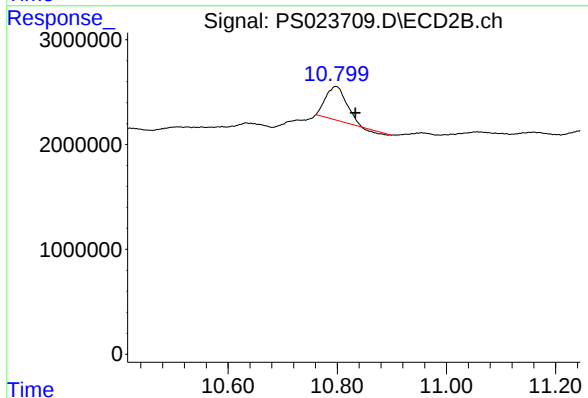


#15 Picloram

R.T.: 10.797 min
Delta R.T.: -0.036 min
Response: 8115629
Conc: 1.92 ng/ml

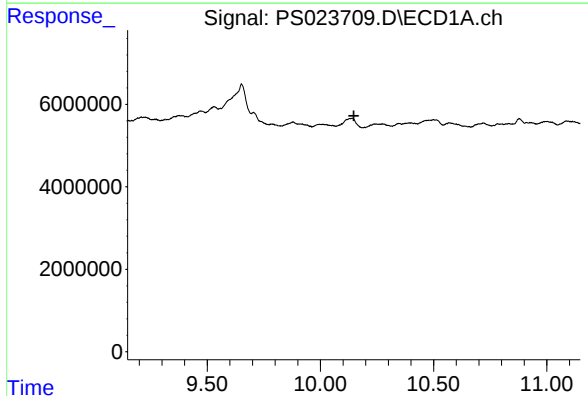

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.148 min
Response: 0
Conc: N.D.

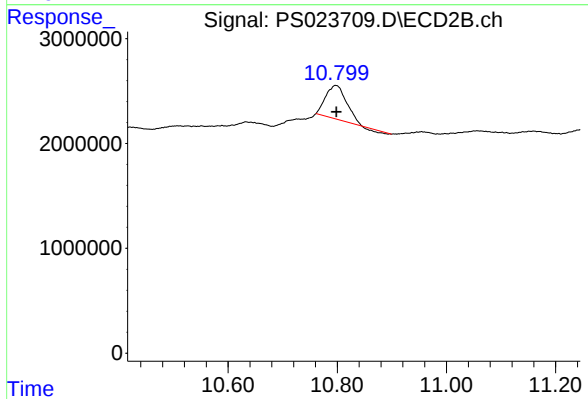

#16 DCPA

R.T.: 10.797 min
Delta R.T.: -0.002 min
Response: 8115629
Conc: 2.93 ng/ml