

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071318\
 Data File : PS001015.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2018 11:35
 Operator : UA
 Sample : J3927-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 15:48:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.649	11.064	59049438	48742764	286.203	223.799
Target Compounds							
1) T	Dalapon	2.987	2.424	4016691	2353994	14.959	8.737 #
2) T	3,5-DICHL...	0.000	9.151	0	4690298	N.D.	15.945 #
5) T	DICAMBA	0.000	11.308	0	6045253	N.D.	7.702 #
6) T	MCP	12.344	0.000	5693615	0	10.365	N.D. #
8) T	DICHLORPROP	0.000	12.477	0	617290	N.D.	3.056 #
15) T	Picloram	0.000	17.008	0	6247622	N.D.	4.103 #
16) T	DCPA	0.000	17.008	0	6247622	N.D.	3.634 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071318\
Data File : PS001015.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2018 11:35
Operator : UA
Sample : J3927-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 15:48:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

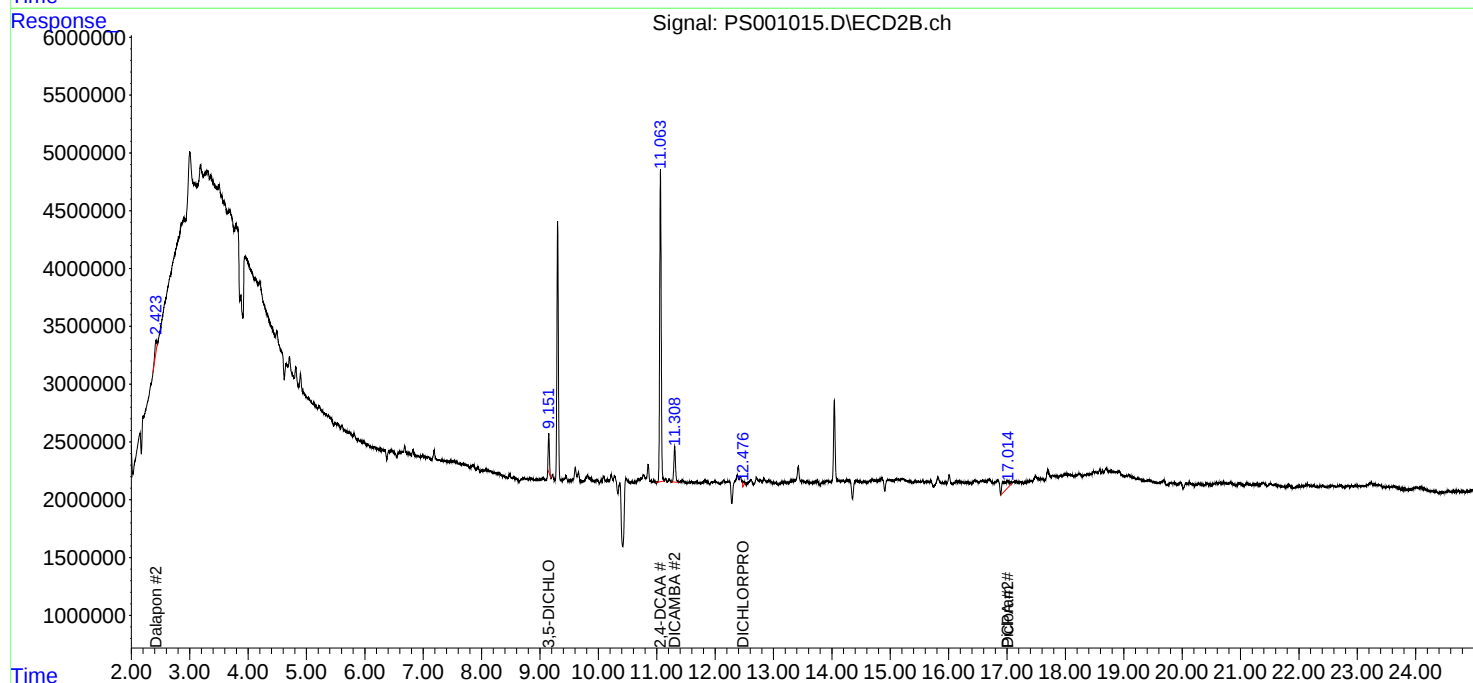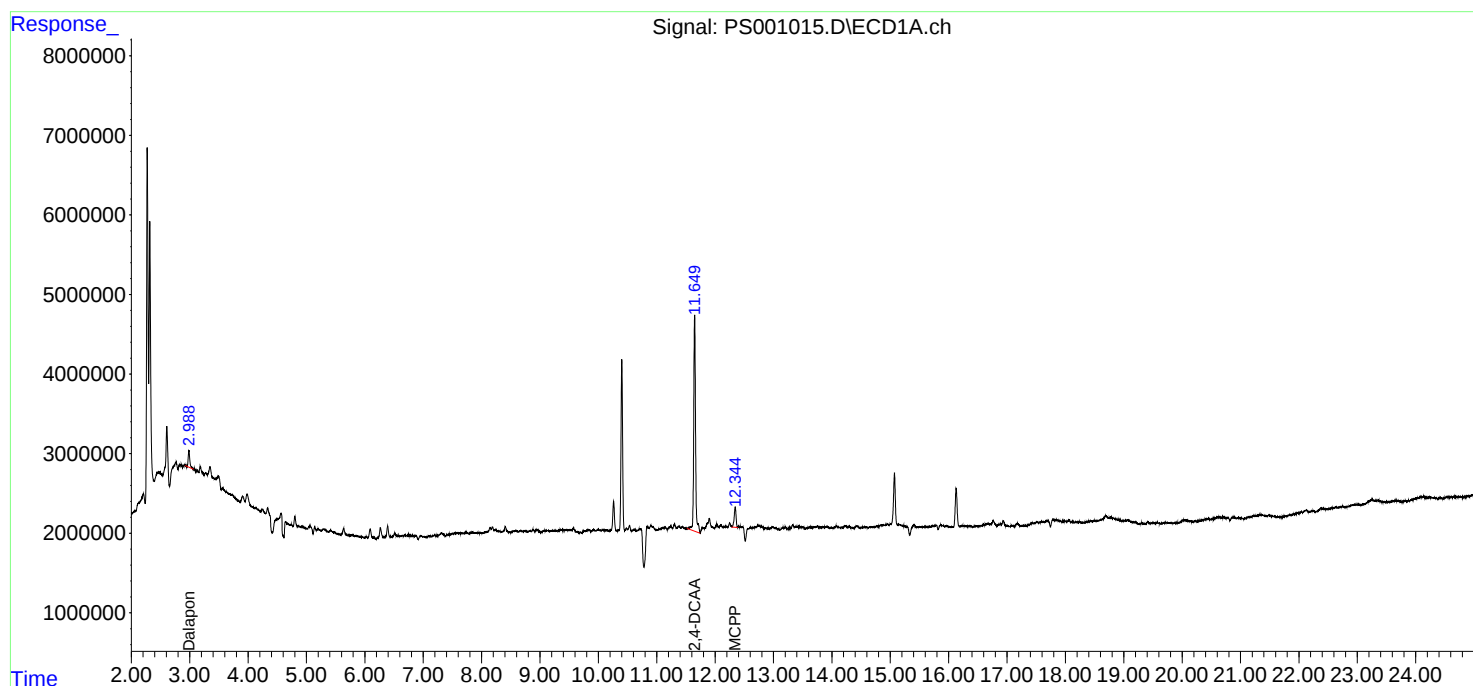


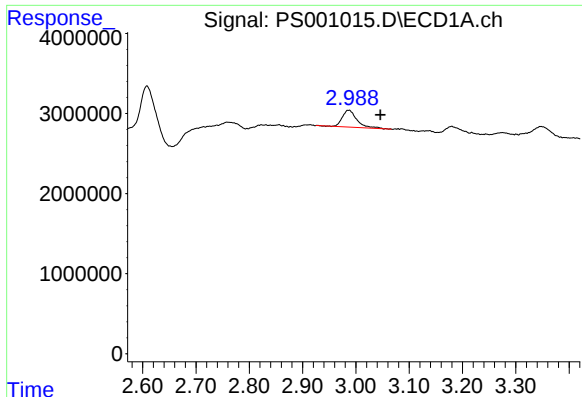

#1 Dalapon


R.T.: 2.987 min
Delta R.T.: -0.059 min
Response: 4016691
Conc: 14.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

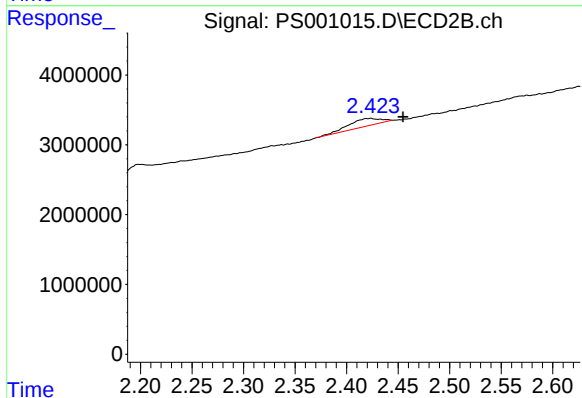


#1 Dalapon

R.T.: 2.424 min
Delta R.T.: -0.031 min
Response: 2353994
Conc: 8.74 ng/ml

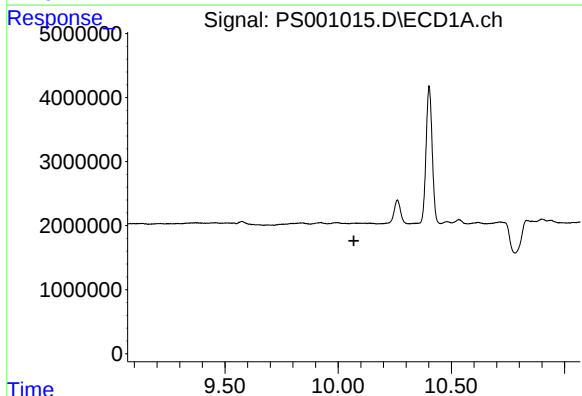


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

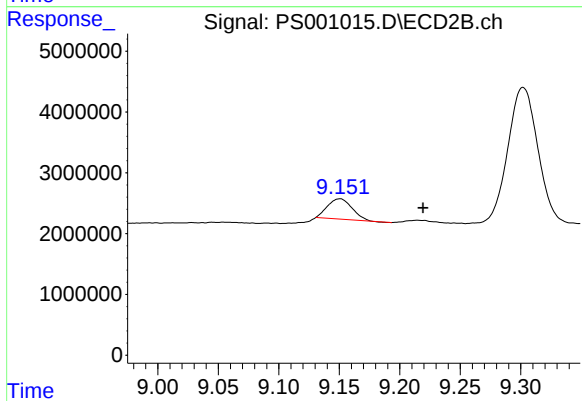

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.151 min
Delta R.T.: -0.069 min
Response: 4690298
Conc: 15.95 ng/ml

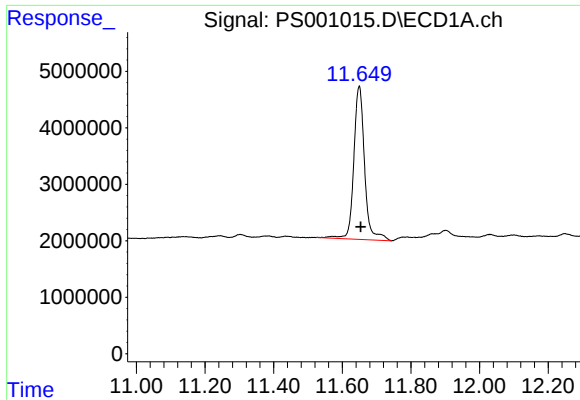

#4 2,4-DCAA


R.T.: 11.649 min
Delta R.T.: -0.004 min
Response: 59049438
Conc: 286.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

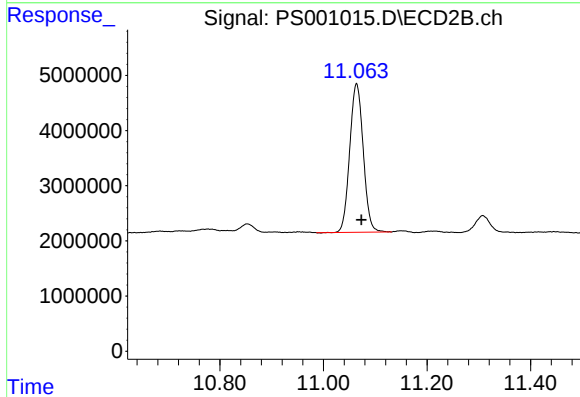


#4 2,4-DCAA

R.T.: 11.064 min
Delta R.T.: -0.010 min
Response: 48742764
Conc: 223.80 ng/ml

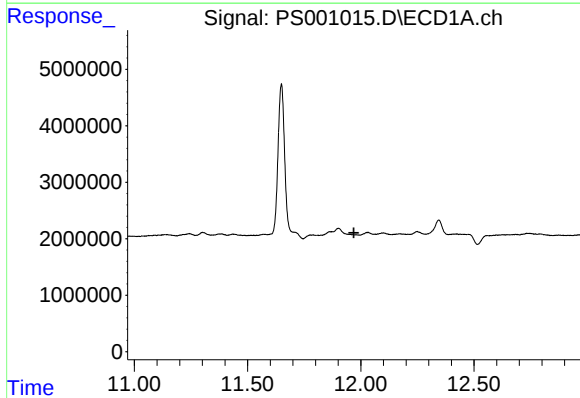


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.970 min
Response: 0
Conc: N.D.

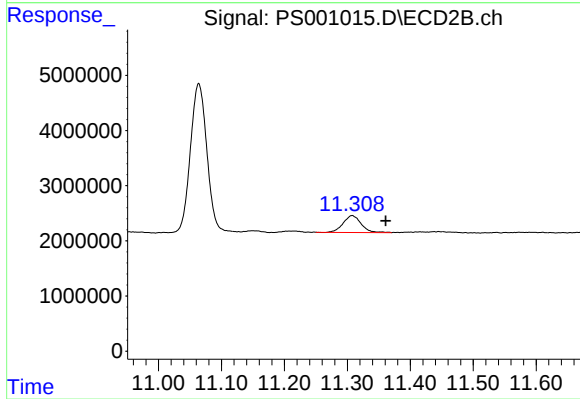

#5 DICAMBA


R.T.: 11.308 min
Delta R.T.: -0.054 min
Response: 6045253
Conc: 7.70 ng/ml

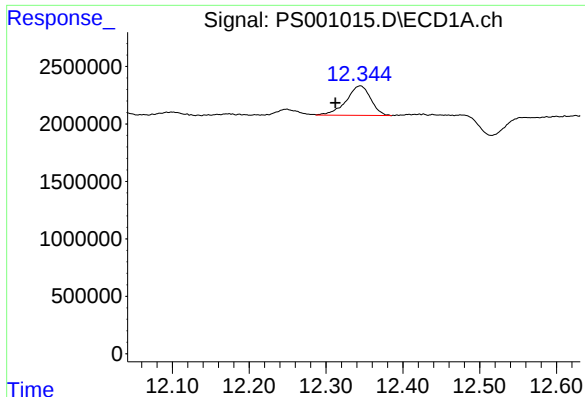

#6 MCP


R.T.: 12.344 min
Delta R.T.: 0.032 min
Response: 5693615
Conc: 10.37 ug/ml

Instrument :
ECD_S
ClientSampleId :

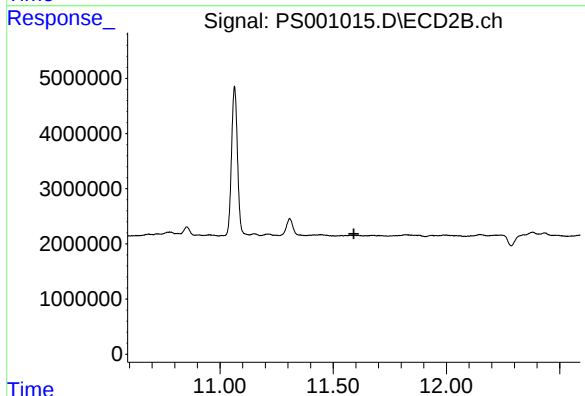


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

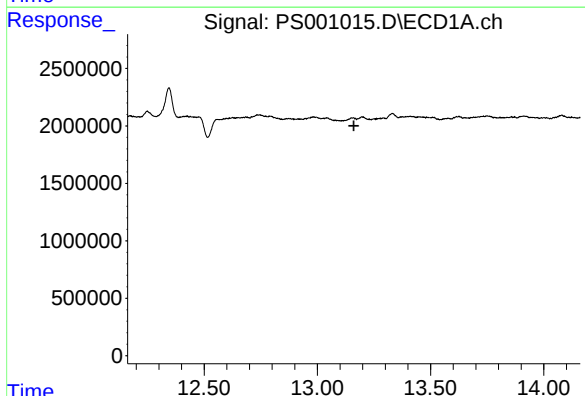


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

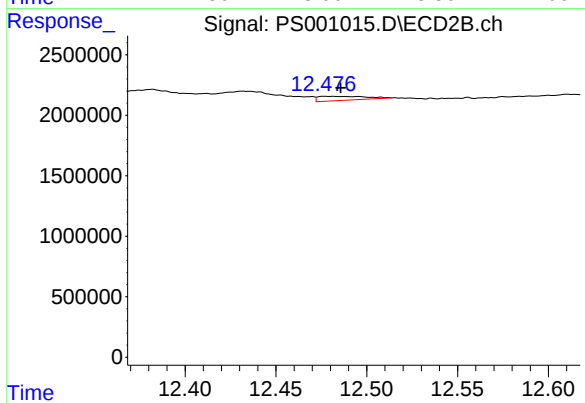

#8 DICHLORPROP


R.T.: 12.477 min
Delta R.T.: -0.008 min
Response: 617290
Conc: 3.06 ng/ml

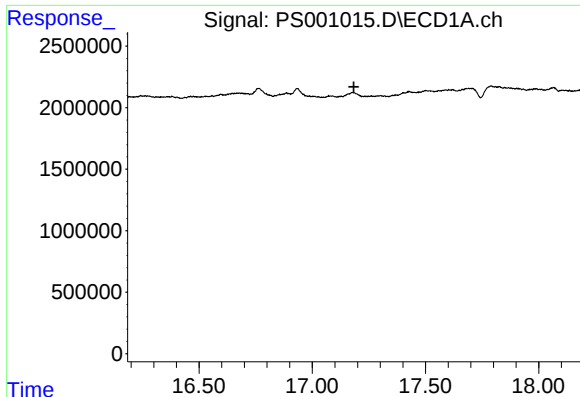

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

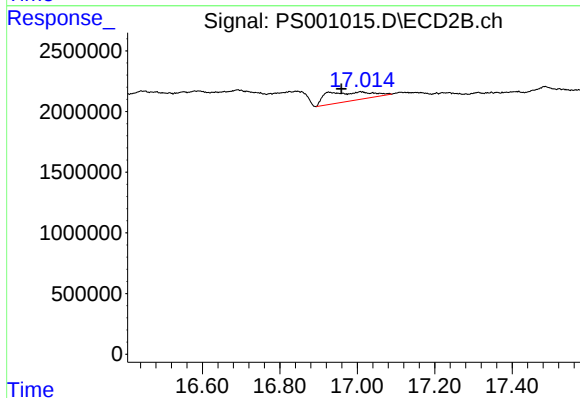


#15 Picloram

R.T.: 17.008 min
Delta R.T.: 0.049 min
Response: 6247622
Conc: 4.10 ng/ml

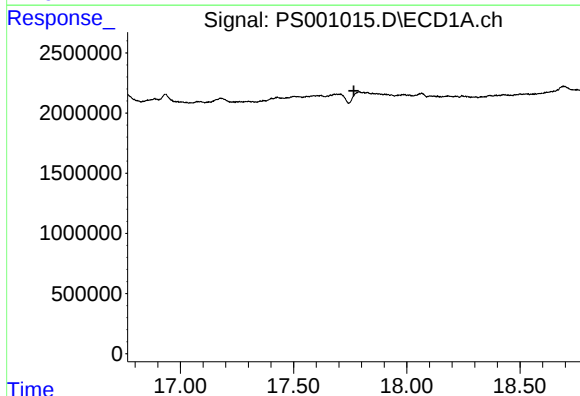

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.766 min
Response: 0
Conc: N.D.

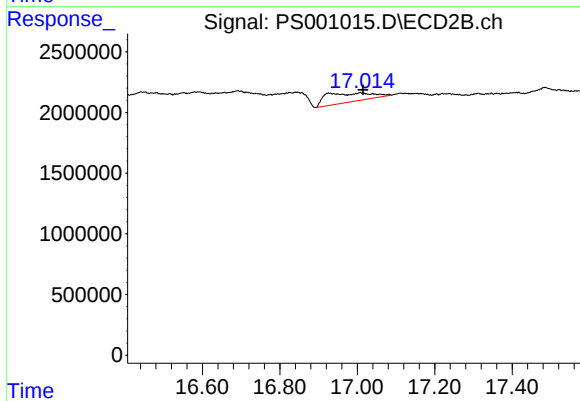

#16 DCPA

R.T.: 17.008 min
Delta R.T.: -0.007 min
Response: 6247622
Conc: 3.63 ng/ml