

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071318\
 Data File : PS001017.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2018 12:38
 Operator : UA
 Sample : J3825-06RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 15:48:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.668	11.083	55069858	45534461	266.915	209.068
Target Compounds							
1) T	Dalapon	0.000	2.451	0	1102027	N.D.	4.090 #
2) T	3,5-DICHL...	0.000	9.169	0	7801300	N.D.	26.521 #
5) T	DICAMBA	11.920	11.327	3533111	6426888	4.487	8.188 #
6) T	MCP	12.362	0.000	9684696	0	17.631	N.D. #
8) T	DICHLORPROP	0.000	12.449	0	2511442	N.D.	12.434 #
10) T	Pentachlo...	0.000	13.443	0	3770933	N.D.	1.202 #
11) T	2,4,5-TP ...	0.000	14.061	0	14309011	N.D.	11.402 #
15) T	Picloram	17.164	0.000	4015511	0	2.217	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071318\
Data File : PS001017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2018 12:38
Operator : UA
Sample : J3825-06RE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 15:48:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

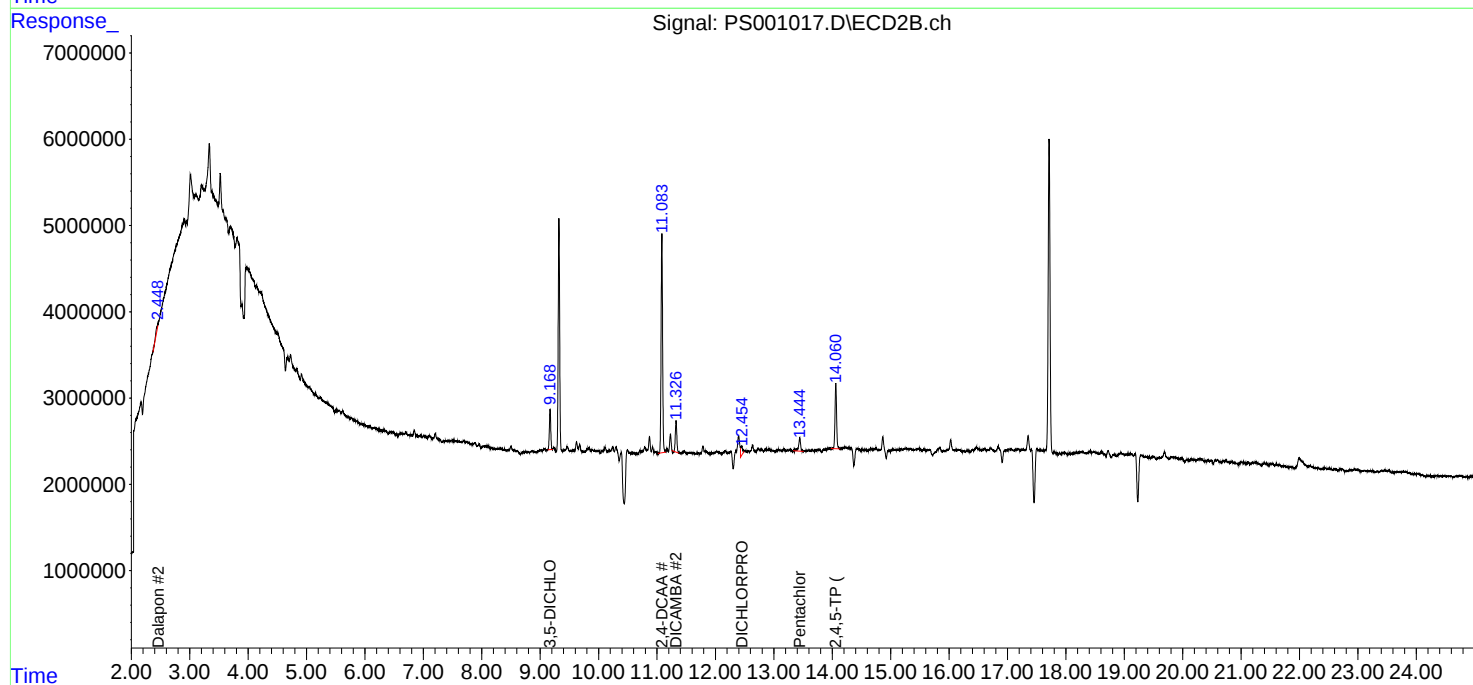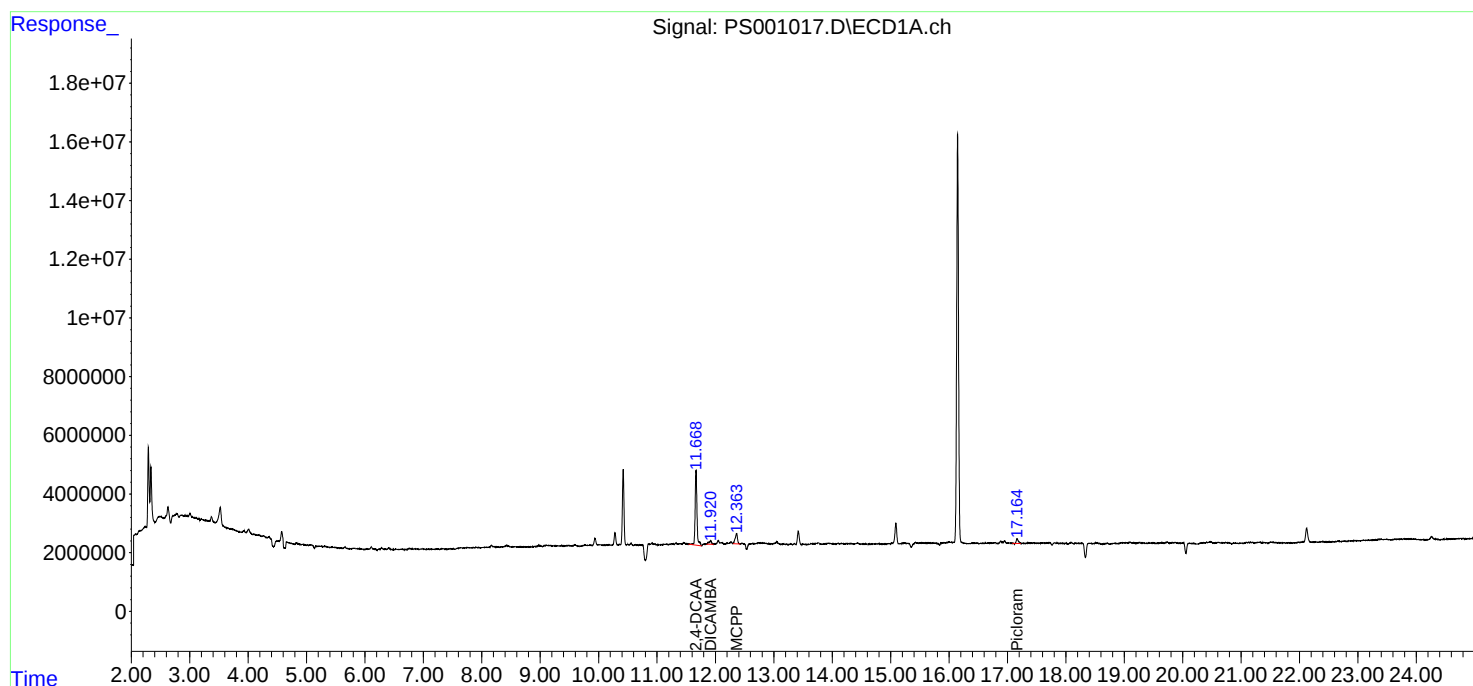


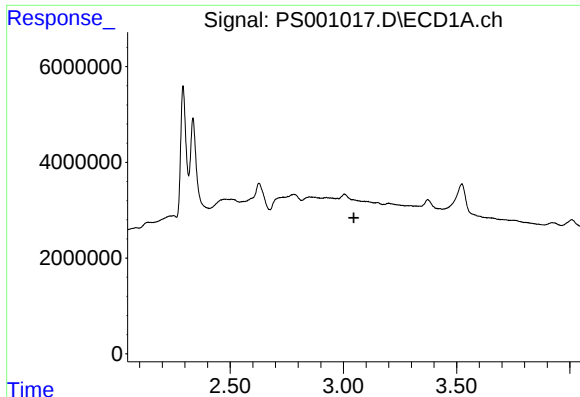

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.046 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

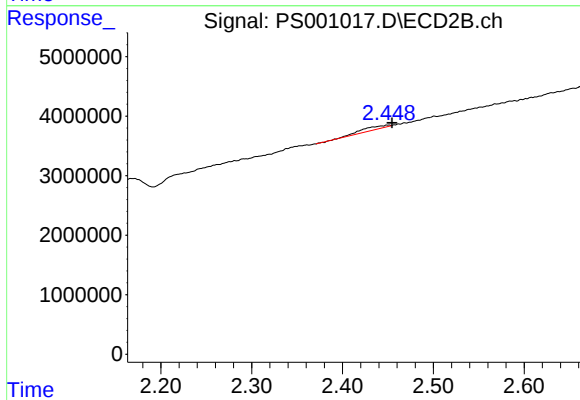


#1 Dalapon

R.T.: 2.451 min
Delta R.T.: -0.003 min
Response: 1102027
Conc: 4.09 ng/ml

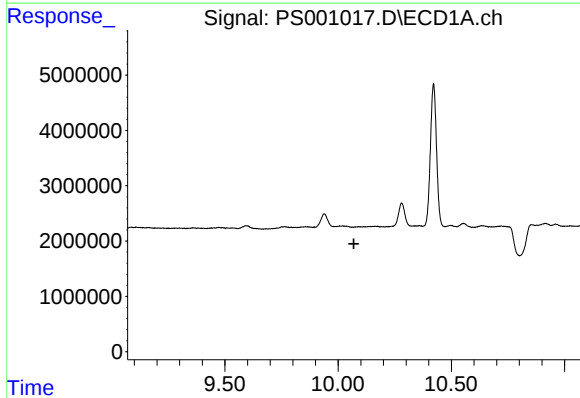


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

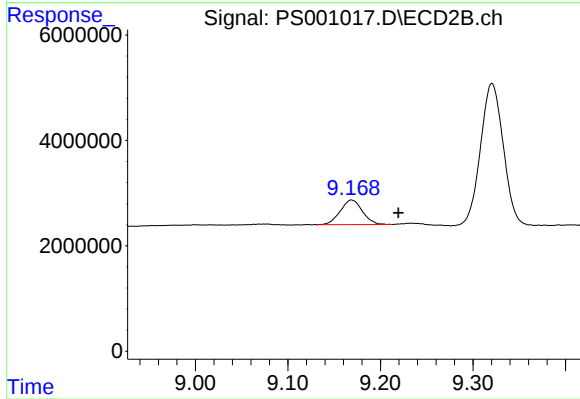

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.169 min
Delta R.T.: -0.051 min
Response: 7801300
Conc: 26.52 ng/ml

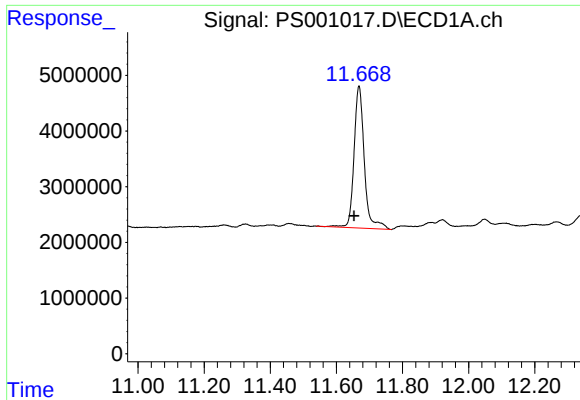

#4 2,4-DCAA


R.T.: 11.668 min
Delta R.T.: 0.015 min
Response: 55069858
Conc: 266.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

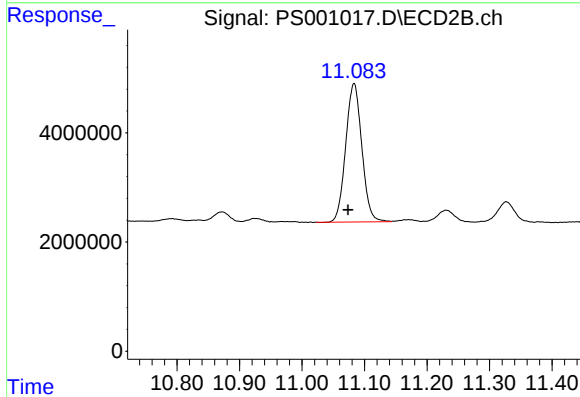


#4 2,4-DCAA

R.T.: 11.083 min
Delta R.T.: 0.010 min
Response: 45534461
Conc: 209.07 ng/ml

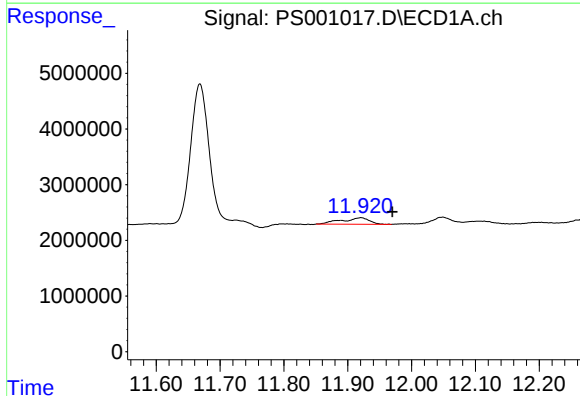


#5 DICAMBA

R.T.: 11.920 min
Delta R.T.: -0.049 min
Response: 3533111
Conc: 4.49 ng/ml

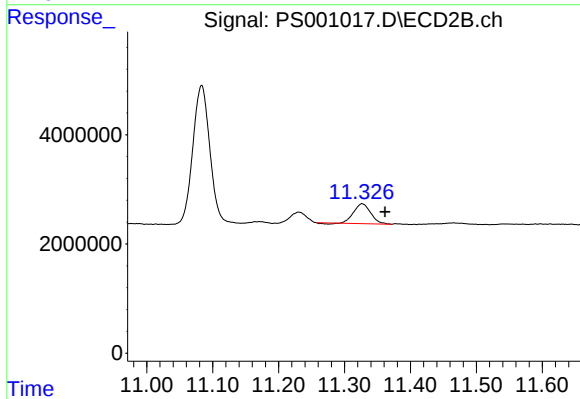

#5 DICAMBA


R.T.: 11.327 min
Delta R.T.: -0.034 min
Response: 6426888
Conc: 8.19 ng/ml

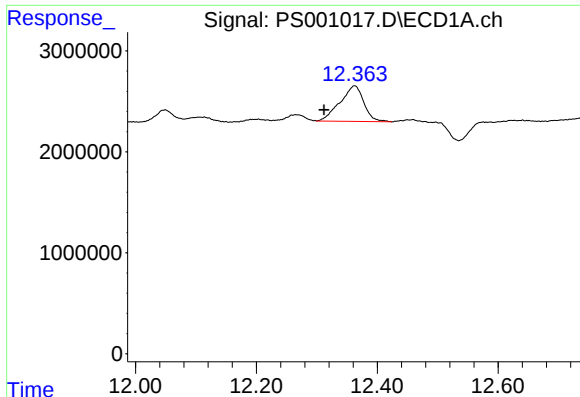

#6 MCP


R.T.: 12.362 min
Delta R.T.: 0.050 min
Response: 9684696
Conc: 17.63 ug/ml

Instrument :
ECD_S
ClientSampleId :

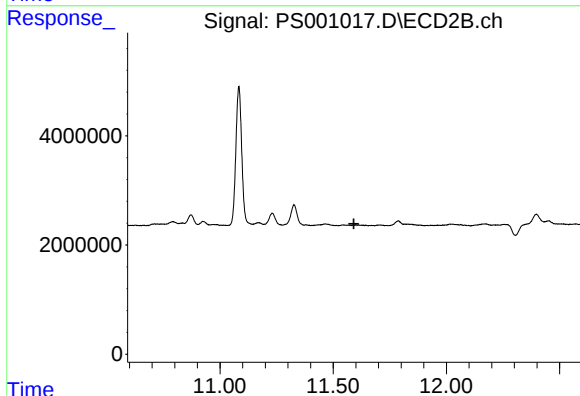


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

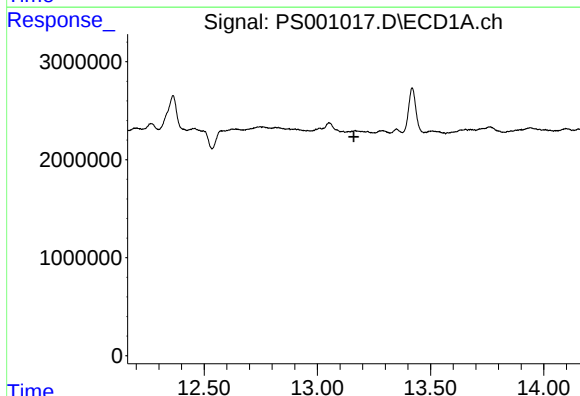


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

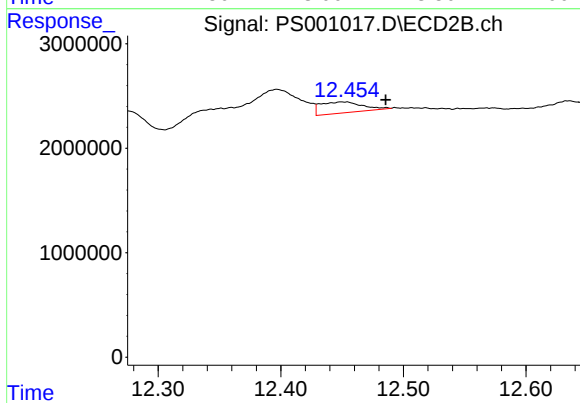

#8 DICHLORPROP


R.T.: 12.449 min
Delta R.T.: -0.036 min
Response: 2511442
Conc: 12.43 ng/ml

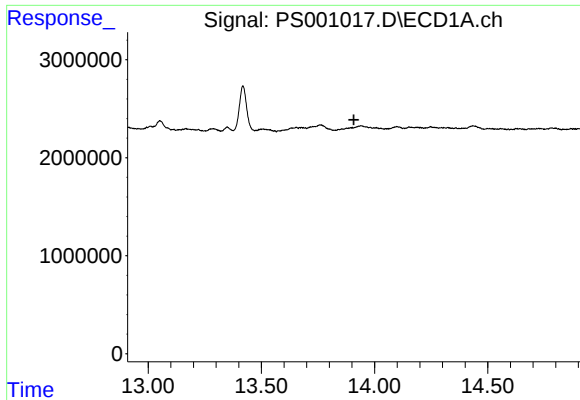

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.908 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

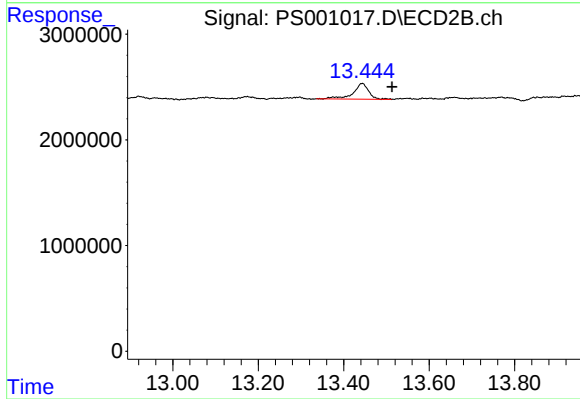


#10 Pentachlorophenol

R.T.: 13.443 min
Delta R.T.: -0.070 min
Response: 3770933
Conc: 1.20 ng/ml

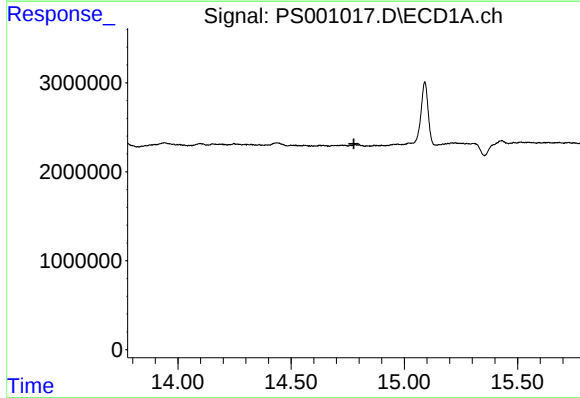


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.777 min
Response: 0
Conc: N.D.

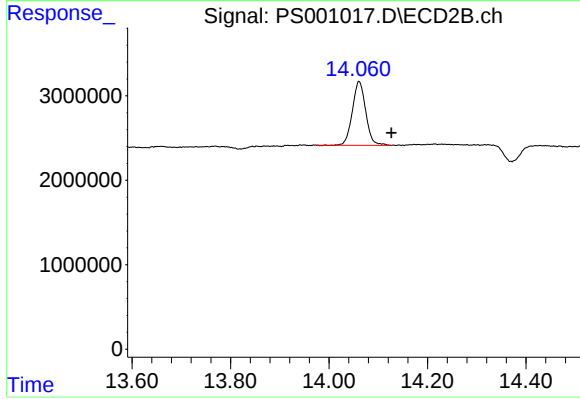

#11 2,4,5-TP (SILVEX)


R.T.: 14.061 min
Delta R.T.: -0.066 min
Response: 14309011
Conc: 11.40 ng/ml

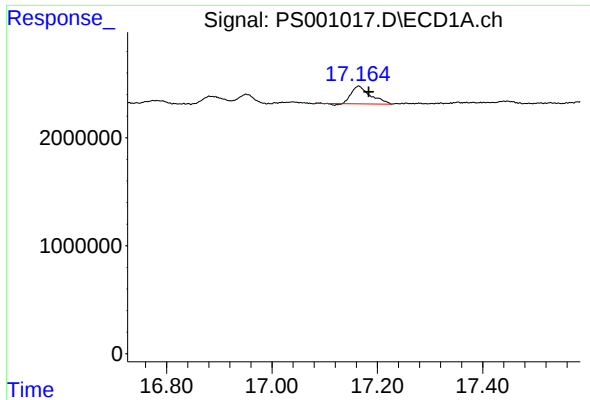

#15 Picloram

R.T.: 17.164 min
Delta R.T.: -0.019 min
Response: 4015511
Conc: 2.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

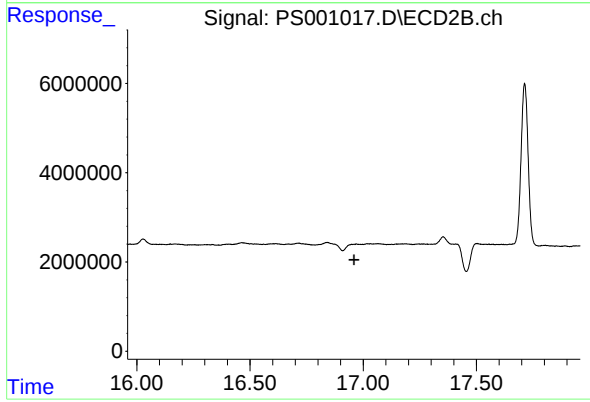

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.959 min
Response: 0
Conc: N.D.