

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071318\
 Data File : PS001019.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2018 13:39
 Operator : UA
 Sample : J3825-10RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 15:49:39 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.639	11.053	55279050	45336192	267.929	208.158
Target Compounds							
1) T	Dalapon	2.976	2.468	3122063	2314040	11.627	8.589 #
5) T	DICAMBA	0.000	11.297	0	7104403	N.D.	9.051 #
6) T	MCPD	12.333	0.000	10275323	0	18.706	N.D. #
7) T	MCPA	12.605	0.000	5914393	0	6.481	N.D. #
8) T	DICHLORPROP	0.000	12.418	0	2438350	N.D.	12.072 #
15) T	Picloram	0.000	16.920	0	1693706	N.D.	1.112 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071318\
Data File : PS001019.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2018 13:39
Operator : UA
Sample : J3825-10RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 15:49:39 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

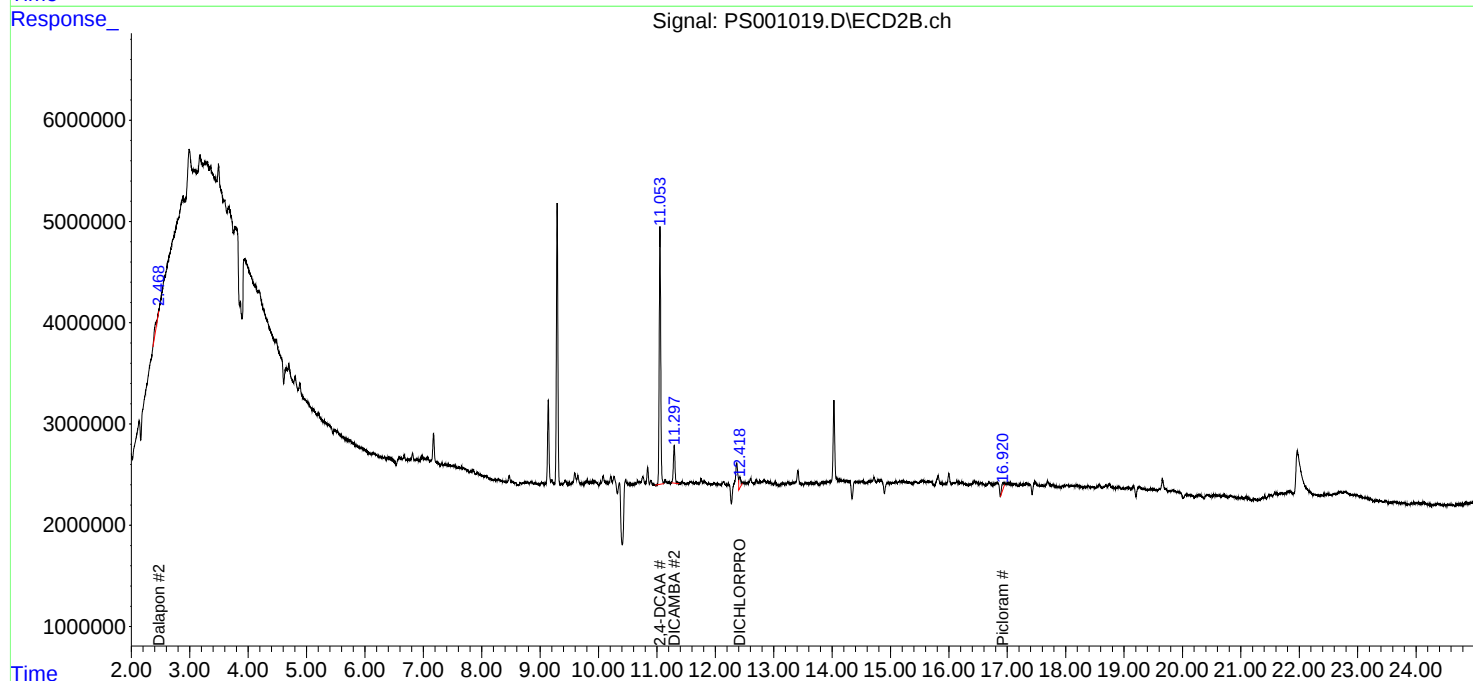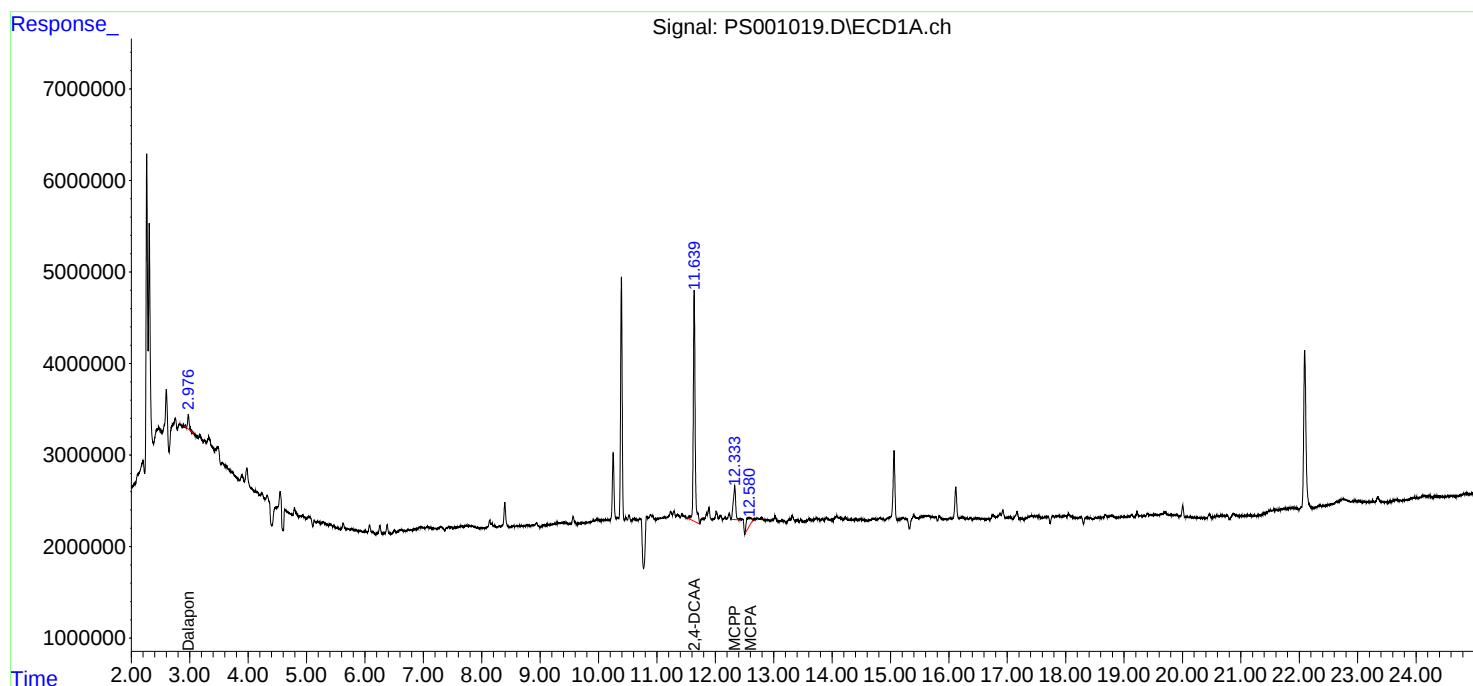


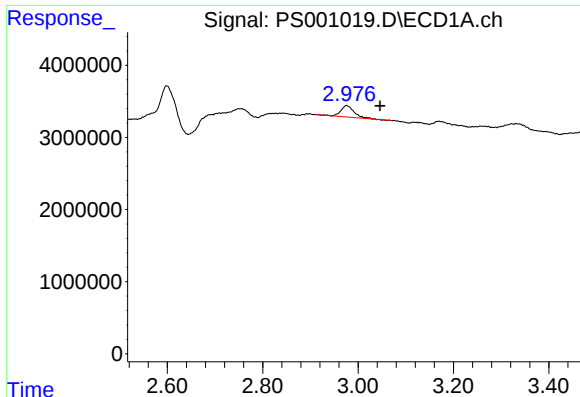

#1 Dalapon


R.T.: 2.976 min
Delta R.T.: -0.070 min
Response: 3122063
Conc: 11.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

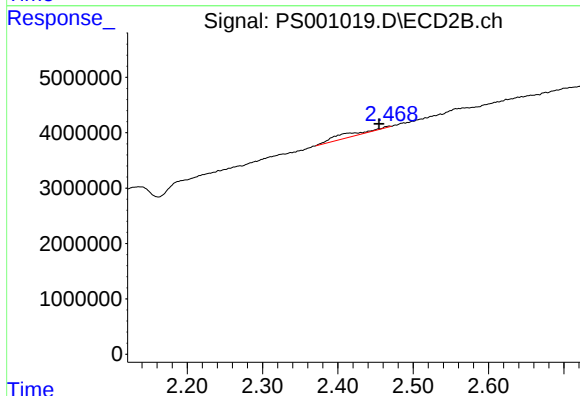


#1 Dalapon

R.T.: 2.468 min
Delta R.T.: 0.014 min
Response: 2314040
Conc: 8.59 ng/ml

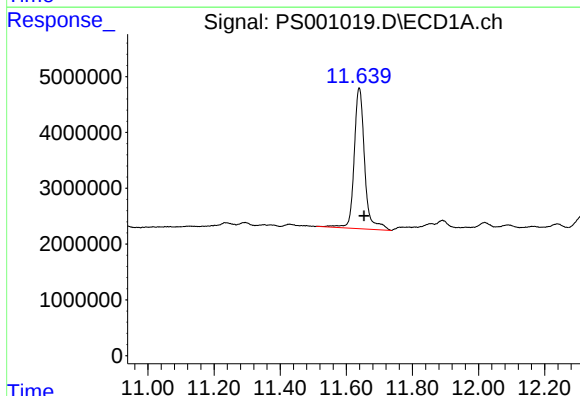


#4 2,4-DCAA

R.T.: 11.639 min
Delta R.T.: -0.014 min
Response: 55279050
Conc: 267.93 ng/ml

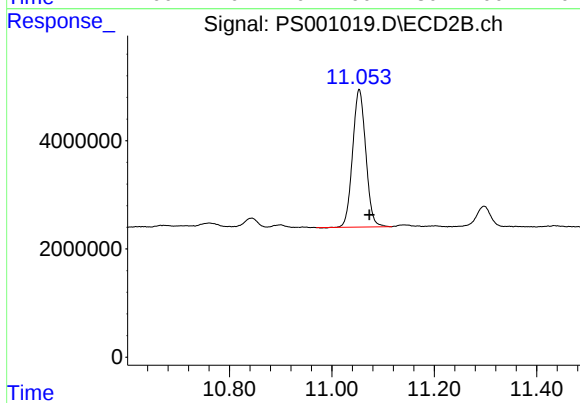

#4 2,4-DCAA


R.T.: 11.053 min
Delta R.T.: -0.020 min
Response: 45336192
Conc: 208.16 ng/ml

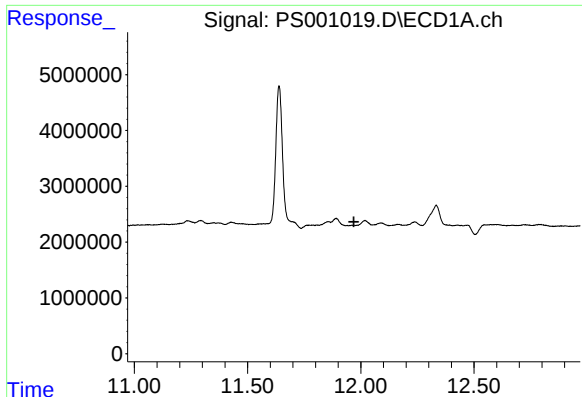

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.970 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

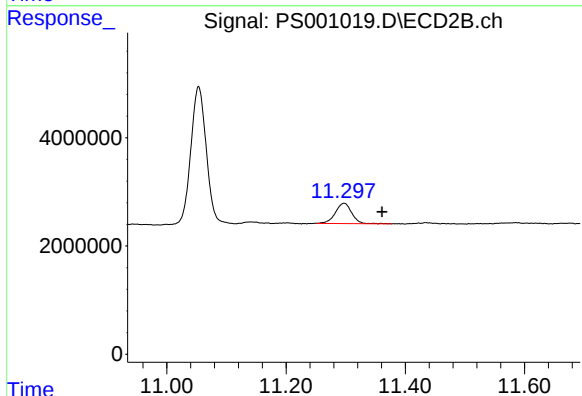


#5 DICAMBA

R.T.: 11.297 min
Delta R.T.: -0.064 min
Response: 7104403
Conc: 9.05 ng/ml

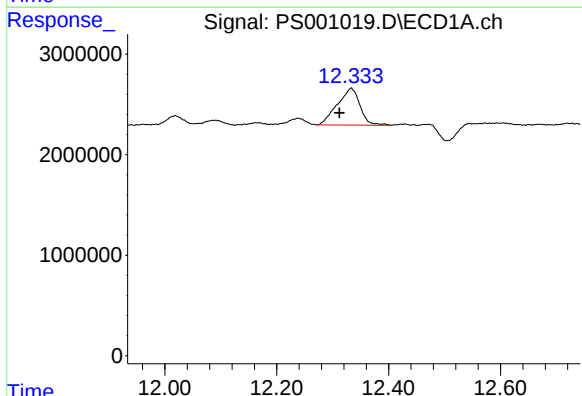


#6 MCP

R.T.: 12.333 min
Delta R.T.: 0.021 min
Response: 10275323
Conc: 18.71 ug/ml

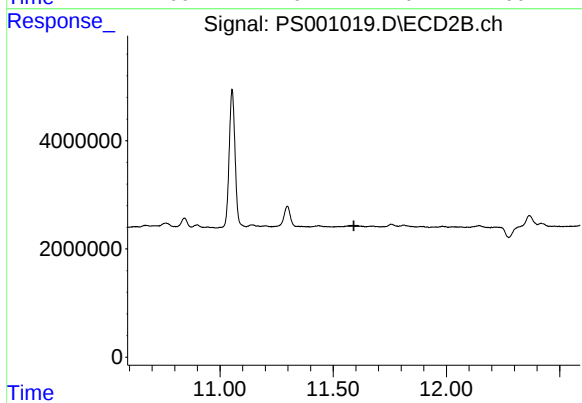

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

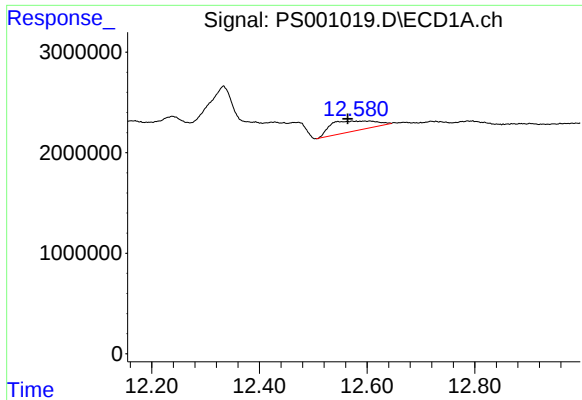

#7 MCPA


R.T.: 12.605 min
Delta R.T.: 0.041 min
Response: 5914393
Conc: 6.48 ug/ml

Instrument :
ECD_S
ClientSampleId :

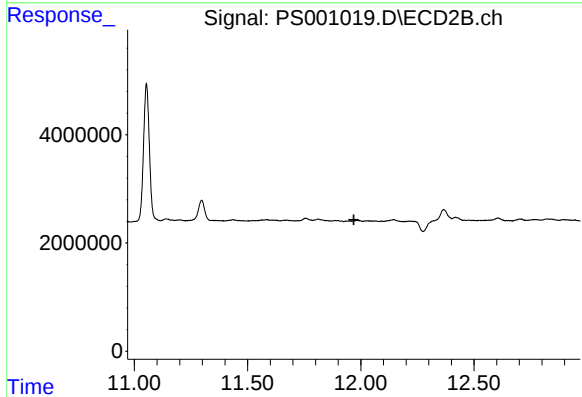


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.969 min
Response: 0
Conc: N.D.

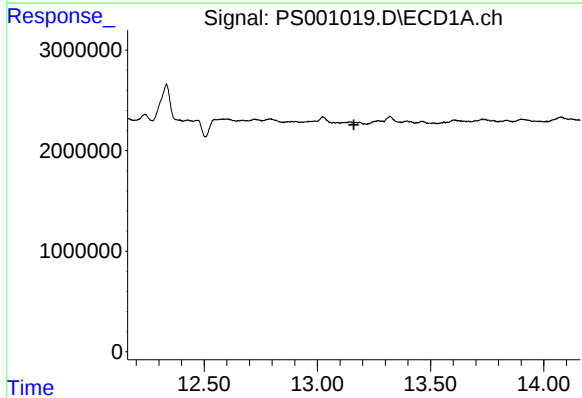


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

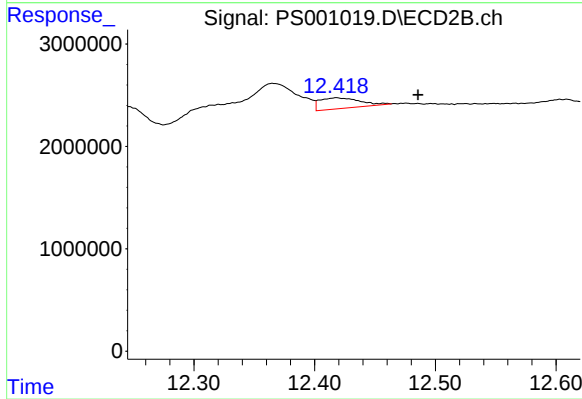

#8 DICHLORPROP


R.T.: 12.418 min
Delta R.T.: -0.068 min
Response: 2438350
Conc: 12.07 ng/ml

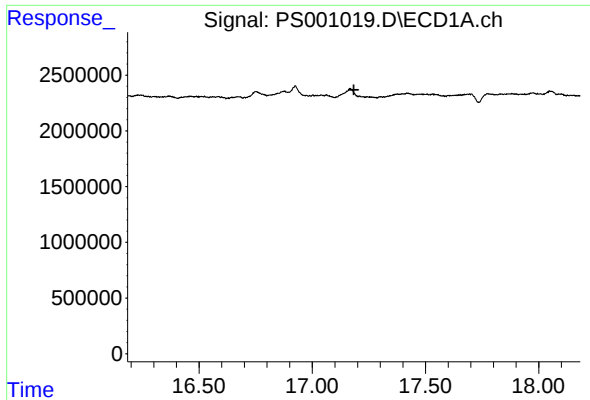

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 17.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

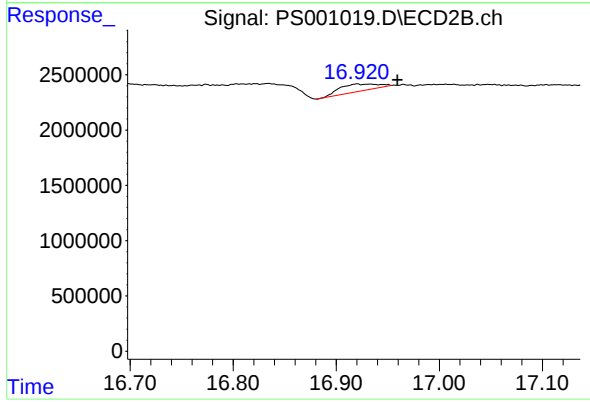

#15 Picloram

R.T.: 16.920 min
Delta R.T.: -0.039 min
Response: 1693706
Conc: 1.11 ng/ml