

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071318\
 Data File : PS001021.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2018 14:41
 Operator : UA
 Sample : J3825-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 15:50:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.651	11.066	52278071	43723719	253.383	200.754
Target Compounds							
1) T	Dalapon	2.987	2.431	2943061	350299	10.961	1.300 #
2) T	3,5-DICHL...	0.000	9.152	0	9476660	N.D.	32.217 #
5) T	DICAMBA	12.029	11.309	2055624	6025724	2.611	7.677 #
6) T	MCP	12.344	0.000	7986638	0	14.540	N.D. #
8) T	DICHLORPROP	0.000	12.433	0	2835090	N.D.	14.037 #
15) T	Picloram	0.000	16.942	0	1587424	N.D.	1.043 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071318\
Data File : PS001021.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2018 14:41
Operator : UA
Sample : J3825-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 15:50:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

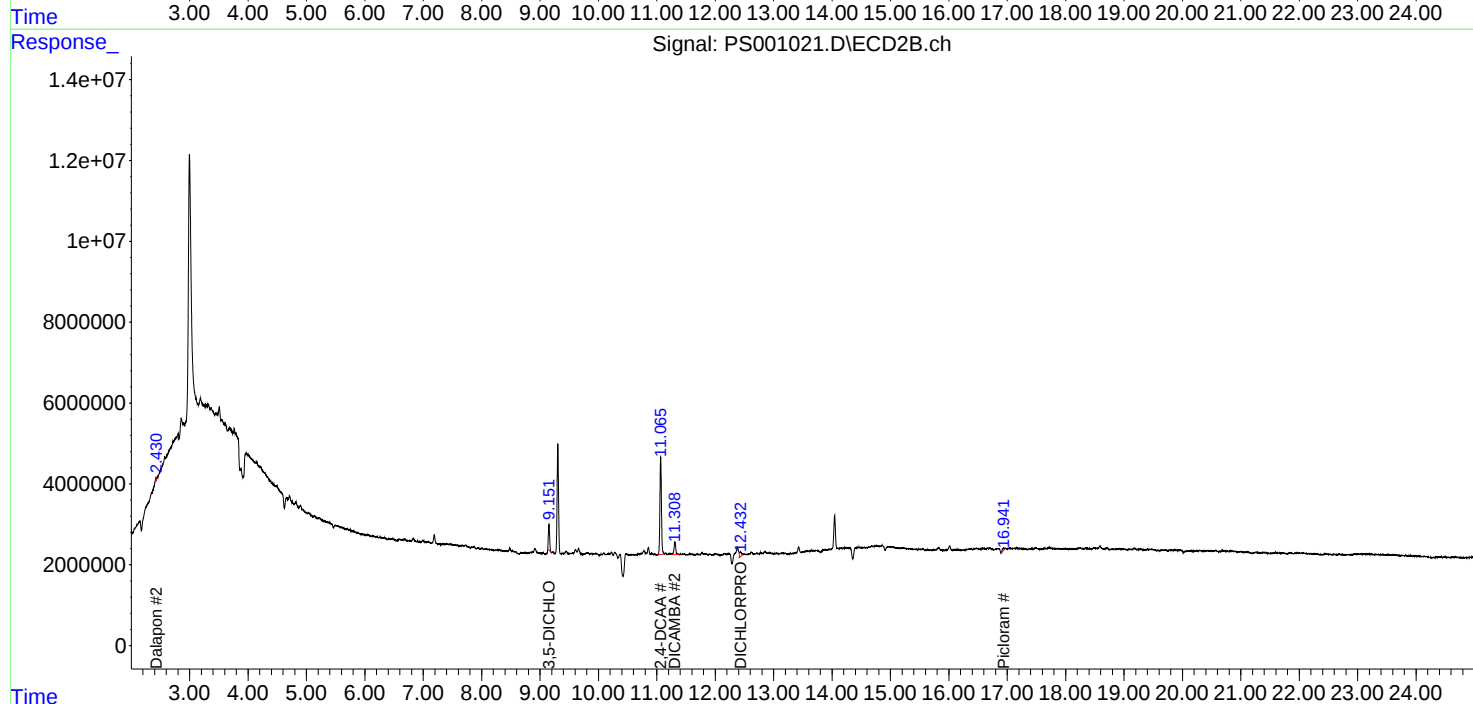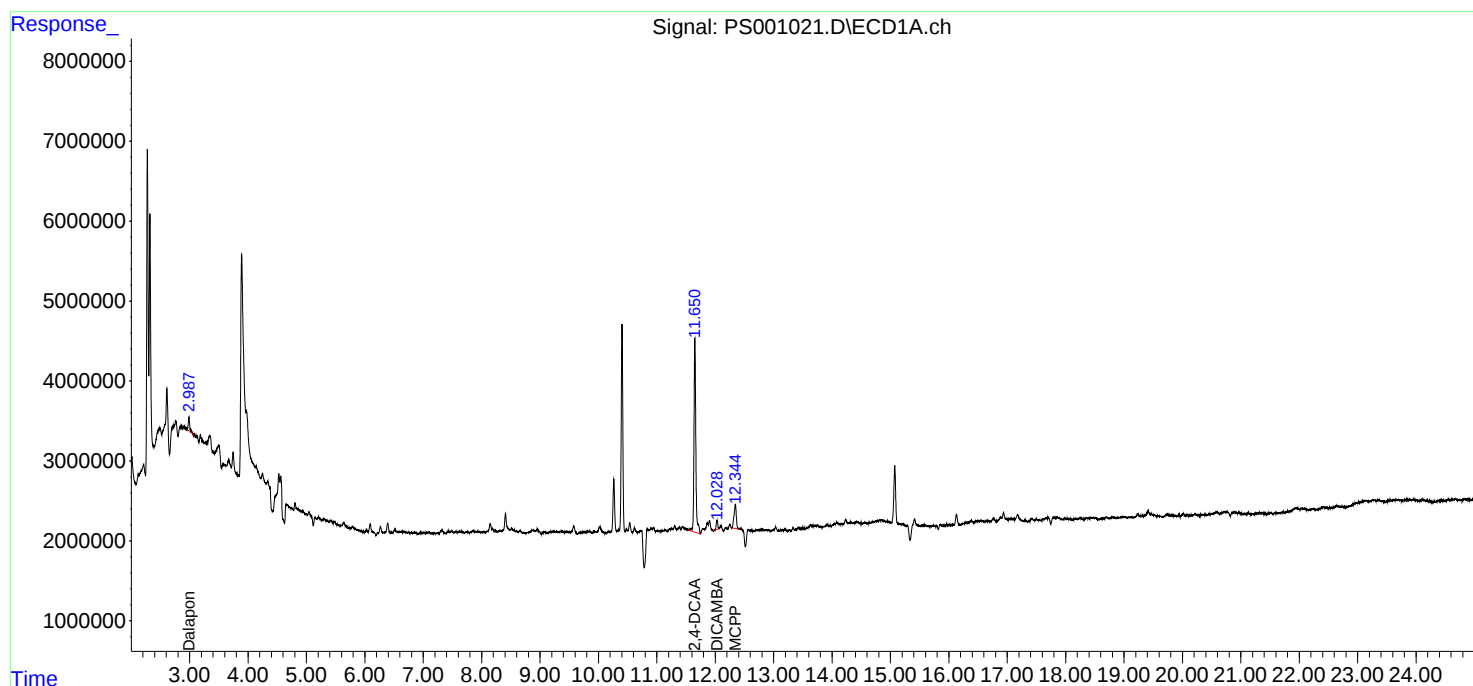


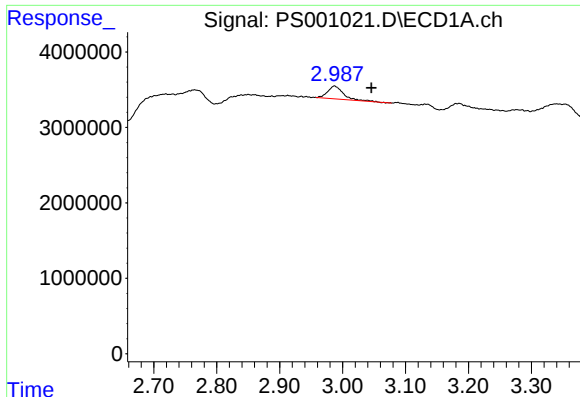

#1 Dalapon


R.T.: 2.987 min
Delta R.T.: -0.059 min
Response: 2943061
Conc: 10.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

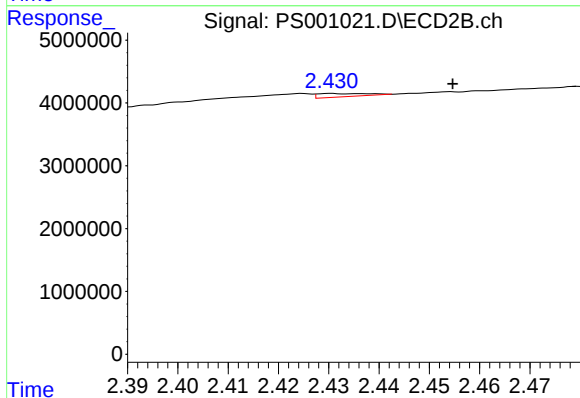


#1 Dalapon

R.T.: 2.431 min
Delta R.T.: -0.024 min
Response: 350299
Conc: 1.30 ng/ml

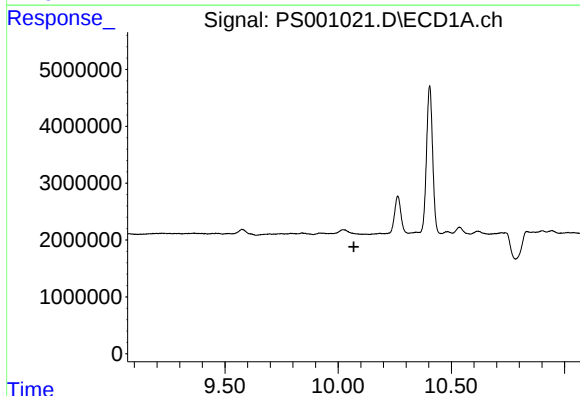


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

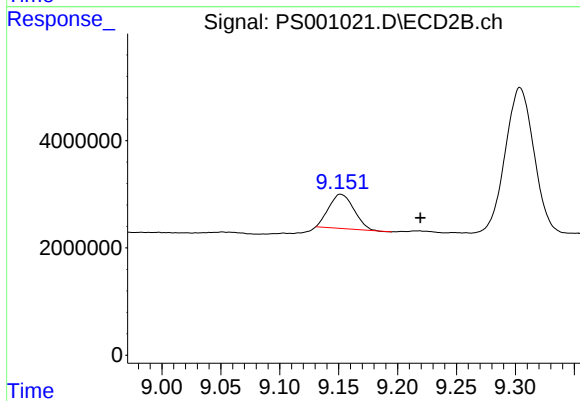

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.152 min
Delta R.T.: -0.068 min
Response: 9476660
Conc: 32.22 ng/ml

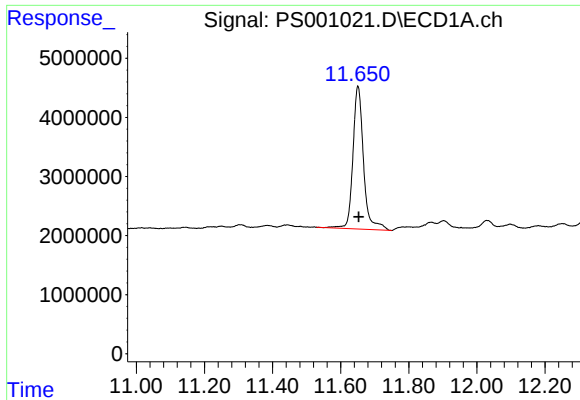

#4 2,4-DCAA


R.T.: 11.651 min
Delta R.T.: -0.003 min
Response: 52278071
Conc: 253.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

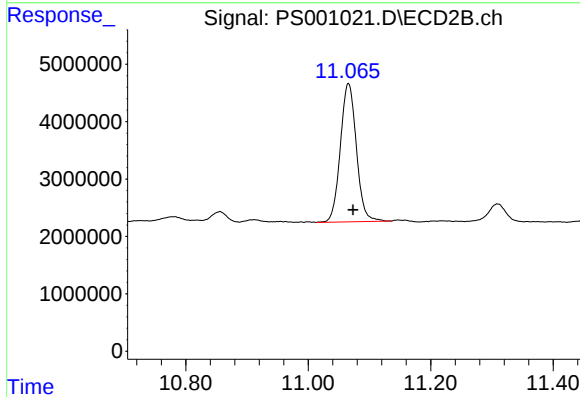


#4 2,4-DCAA

R.T.: 11.066 min
Delta R.T.: -0.008 min
Response: 43723719
Conc: 200.75 ng/ml

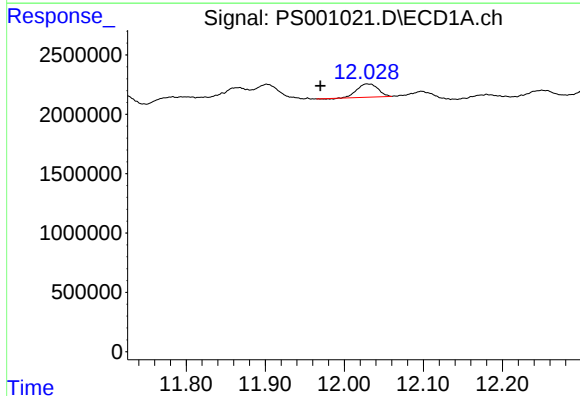


#5 DICAMBA

R.T.: 12.029 min
Delta R.T.: 0.059 min
Response: 2055624
Conc: 2.61 ng/ml

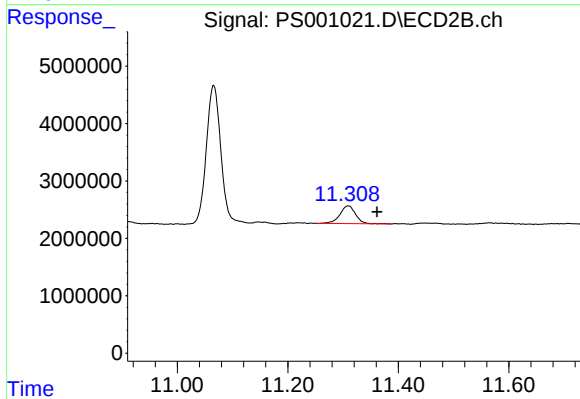

#5 DICAMBA


R.T.: 11.309 min
Delta R.T.: -0.052 min
Response: 6025724
Conc: 7.68 ng/ml

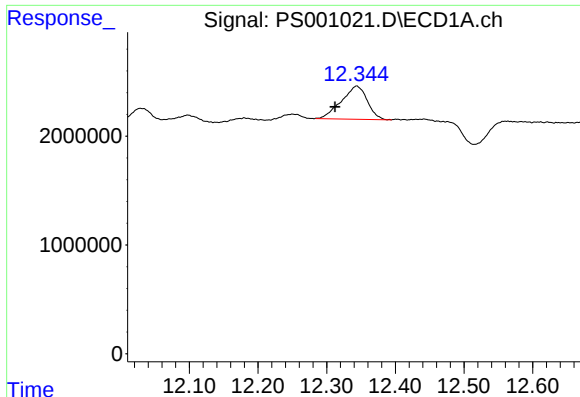

#6 MCP


R.T.: 12.344 min
Delta R.T.: 0.032 min
Response: 7986638
Conc: 14.54 ug/ml

Instrument :
ECD_S
ClientSampleId :

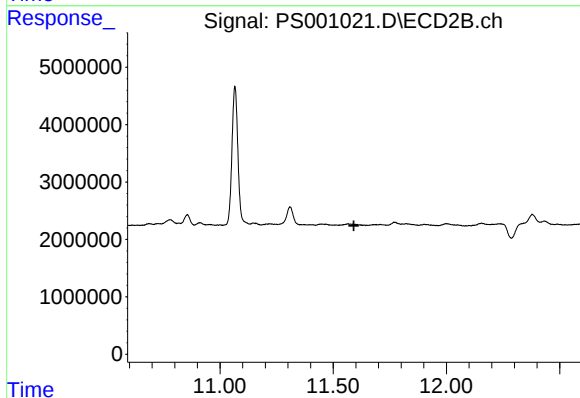


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

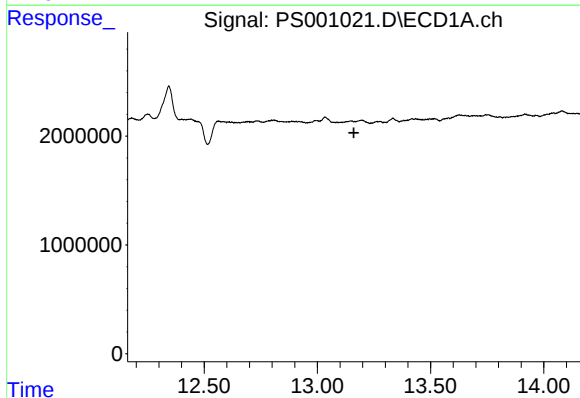


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

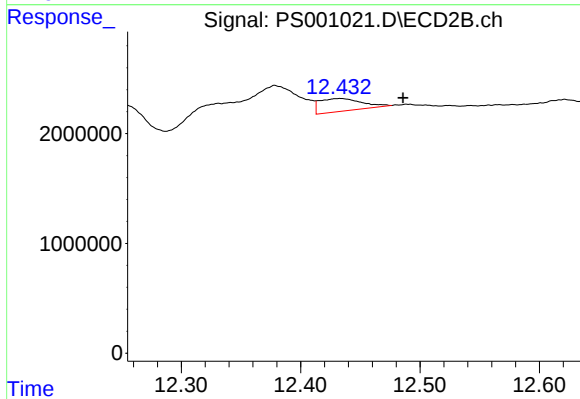

#8 DICHLORPROP


R.T.: 12.433 min
Delta R.T.: -0.053 min
Response: 2835090
Conc: 14.04 ng/ml

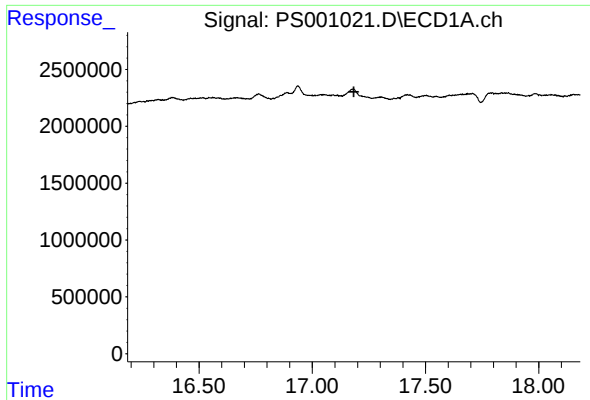

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 17.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

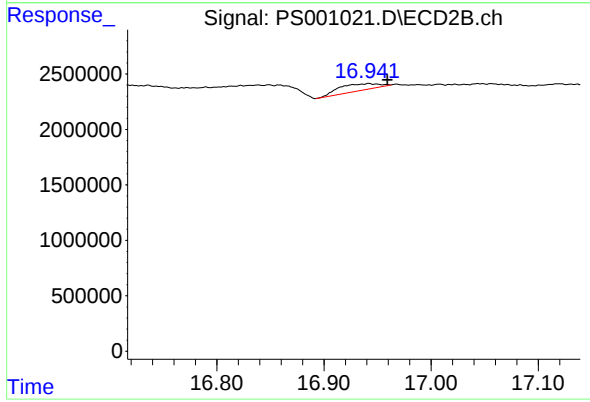

#15 Picloram

R.T.: 16.942 min
Delta R.T.: -0.017 min
Response: 1587424
Conc: 1.04 ng/ml