

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071318\
 Data File : PS001024.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2018 17:14
 Operator : UA
 Sample : J3825-02RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 00:41:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.659	11.062	48508424	40846400	235.112	187.543
Target Compounds							
1) T	Dalapon	2.993	0.000	3309780	0	12.327	N.D. #
5) T	DICAMBA	12.038	11.306	1674877	5554845	2.127	7.077 #
6) T	MCPD	12.346	0.000	11947317	0	21.750	N.D. #
12) T	2,4,5-T	0.000	14.690	0	5625562	N.D.	5.437 #
15) T	Picloram	17.189	17.007	3972458	8497172	2.193	5.580 #
16) T	DCPA	0.000	17.007	0	8497172	N.D.	4.943 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071318\
Data File : PS001024.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2018 17:14
Operator : UA
Sample : J3825-02RE
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 00:41:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

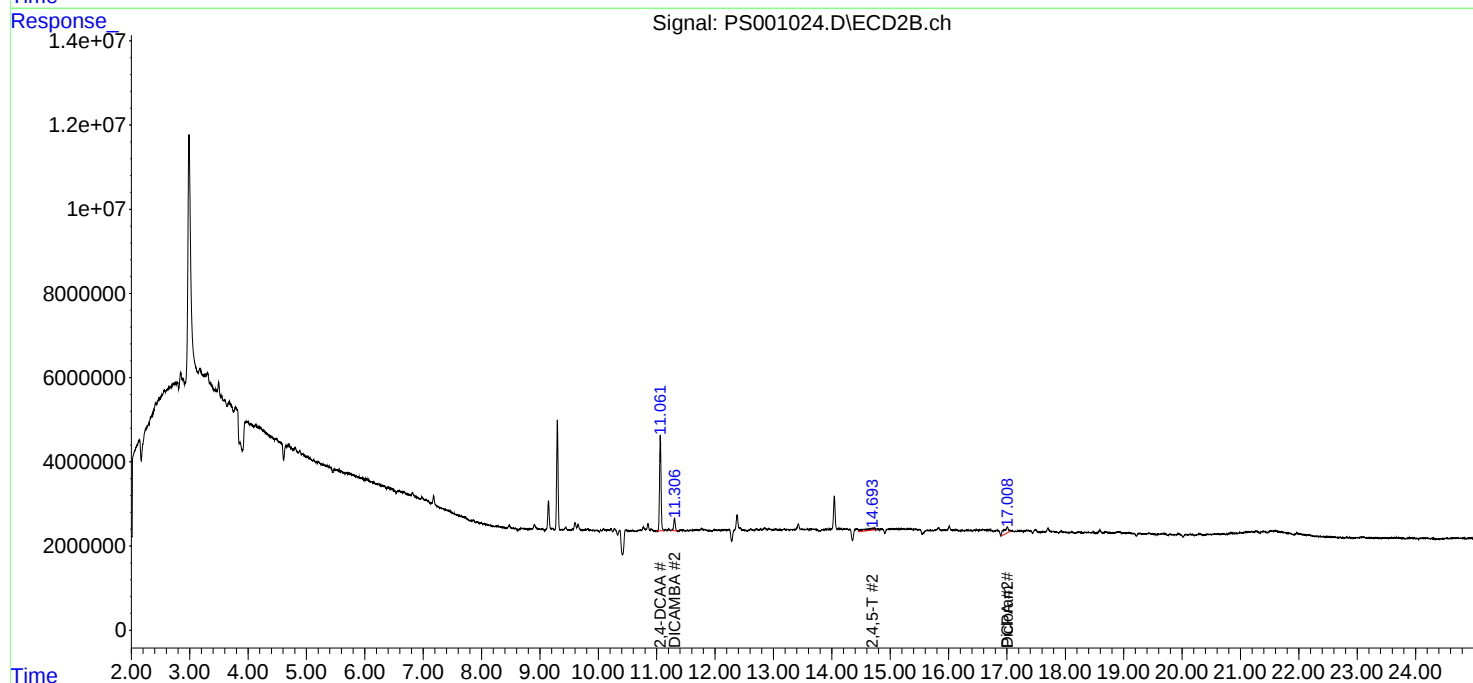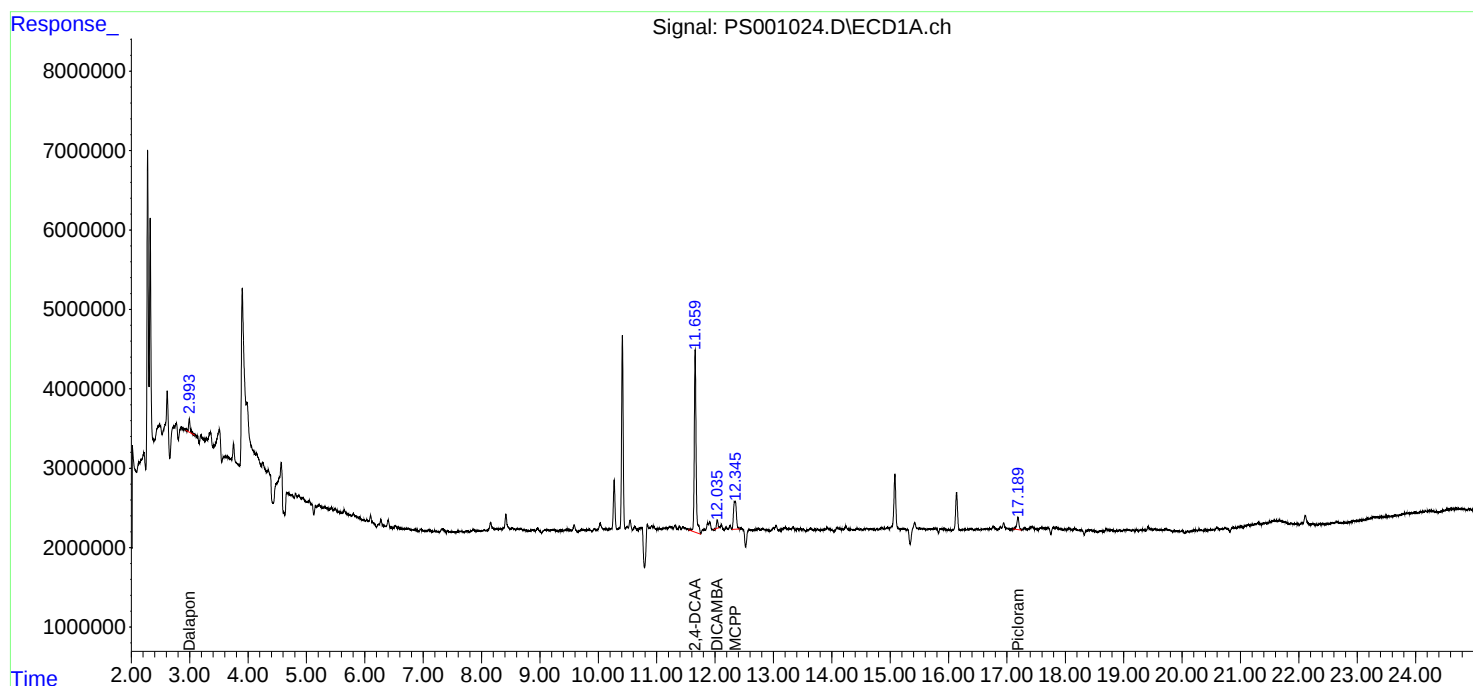


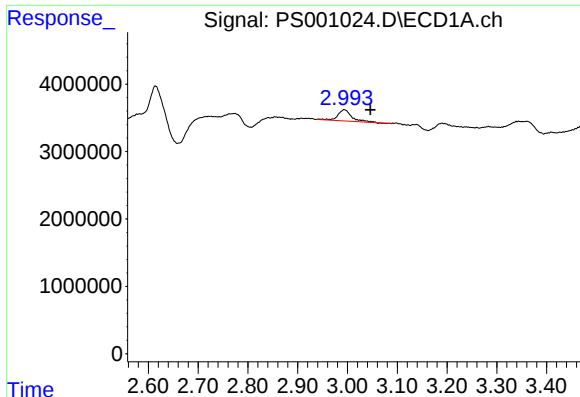

#1 Dalapon


R.T.: 2.993 min
Delta R.T.: -0.053 min
Response: 3309780
Conc: 12.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

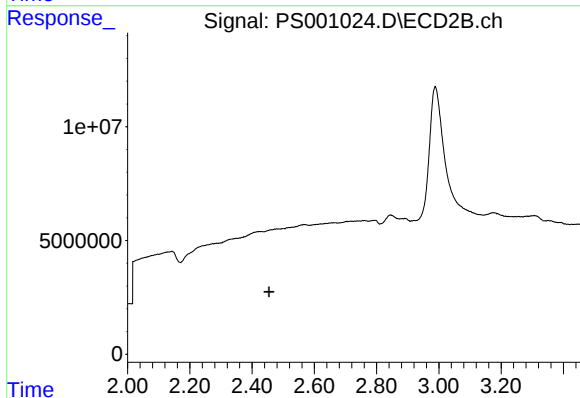


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.455 min
Response: 0
Conc: N.D.

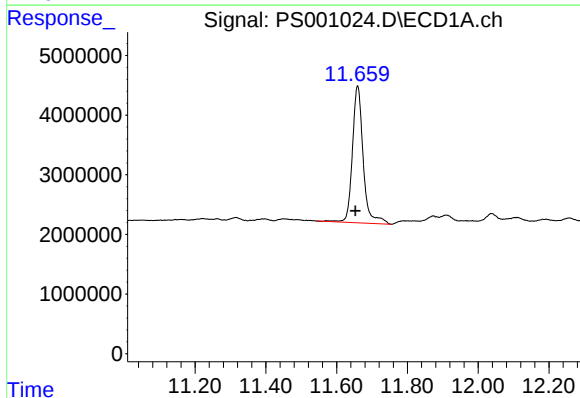


#4 2,4-DCAA

R.T.: 11.659 min
Delta R.T.: 0.006 min
Response: 48508424
Conc: 235.11 ng/ml

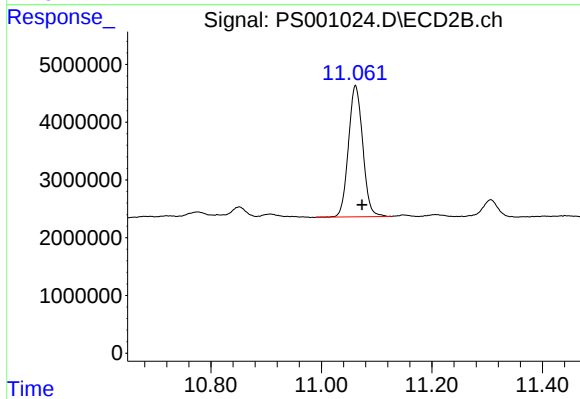

#4 2,4-DCAA


R.T.: 11.062 min
Delta R.T.: -0.012 min
Response: 40846400
Conc: 187.54 ng/ml

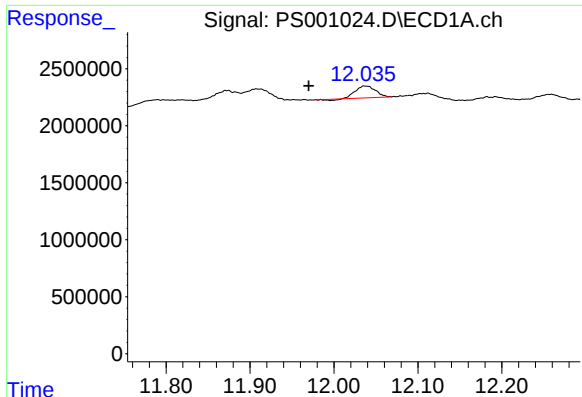

#5 DICAMBA


R.T.: 12.038 min
Delta R.T.: 0.068 min
Response: 1674877
Conc: 2.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

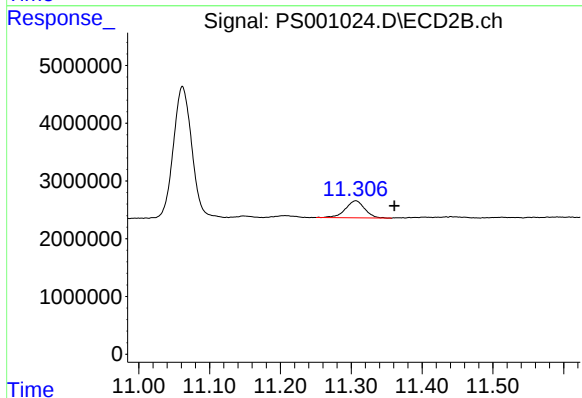


#5 DICAMBA

R.T.: 11.306 min
Delta R.T.: -0.055 min
Response: 5554845
Conc: 7.08 ng/ml

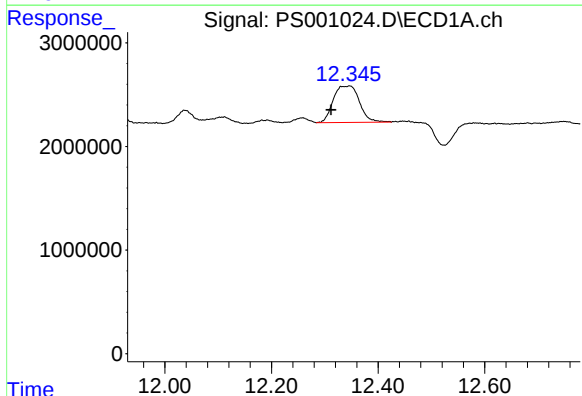


#6 MCP

R.T.: 12.346 min
Delta R.T.: 0.034 min
Response: 11947317
Conc: 21.75 ug/ml

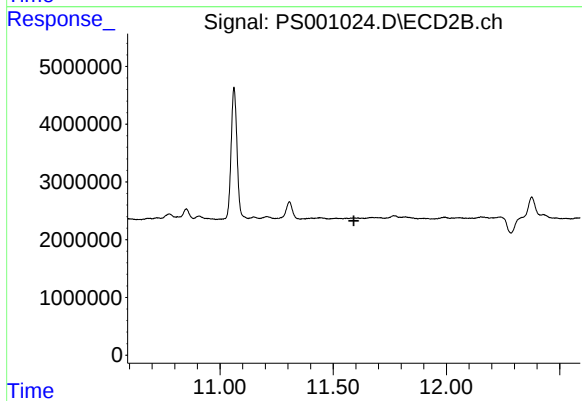

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

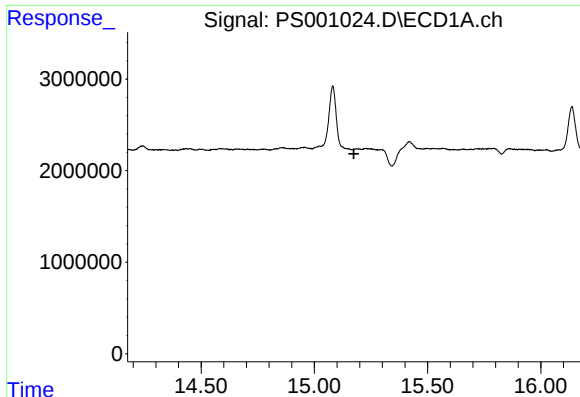

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.174 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

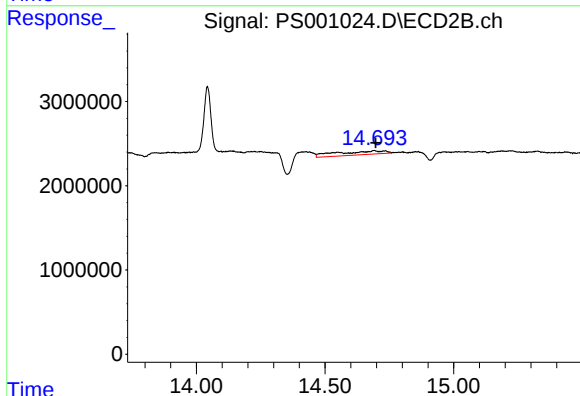


#12 2,4,5-T

R.T.: 14.690 min
Delta R.T.: -0.008 min
Response: 5625562
Conc: 5.44 ng/ml

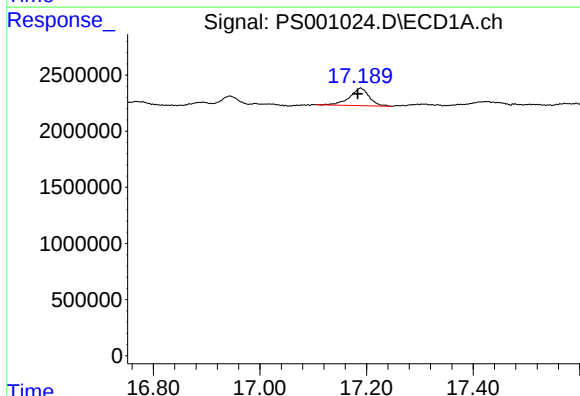


#15 Picloram

R.T.: 17.189 min
Delta R.T.: 0.005 min
Response: 3972458
Conc: 2.19 ng/ml

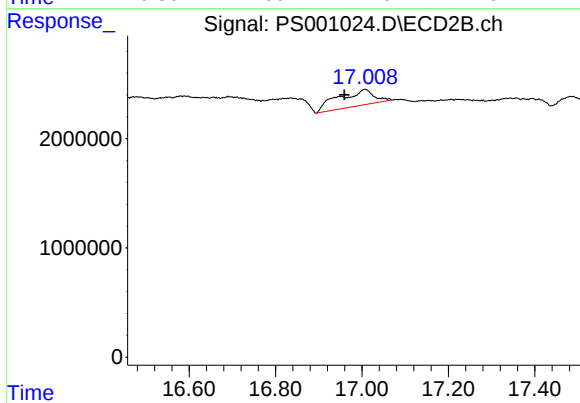

#15 Picloram


R.T.: 17.007 min
Delta R.T.: 0.048 min
Response: 8497172
Conc: 5.58 ng/ml

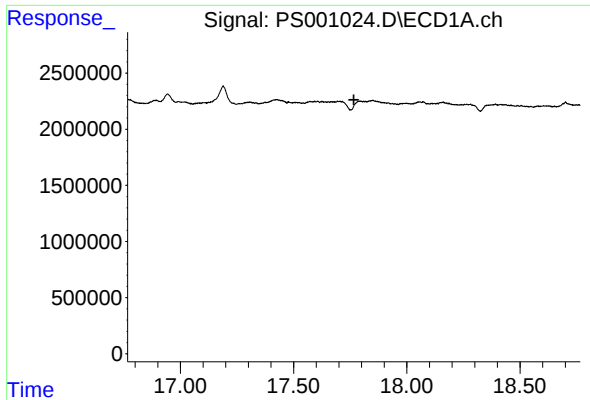

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.766 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

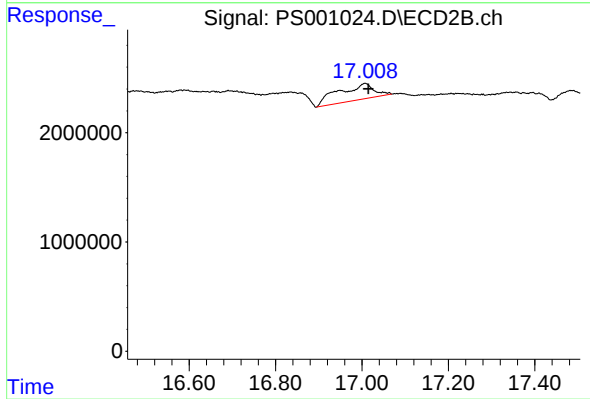

#16 DCPA

R.T.: 17.007 min
Delta R.T.: -0.008 min
Response: 8497172
Conc: 4.94 ng/ml