

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071318\
 Data File : PS001028.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2018 19:18
 Operator : UA
 Sample : J3947-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 00:43:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.649	11.065	45998317	38330911	222.946	175.994
Target Compounds							
1) T	Dalapon	2.986	0.000	7026821	0	26.170	N.D. #
2) T	3,5-DICHL...	0.000	9.150	0	6415646	N.D.	21.811 #
5) T	DICAMBA	0.000	11.308	0	5472173	N.D.	6.971 #
6) T	MCP	12.343	0.000	6280534	0	11.434	N.D. #
8) T	DICHLORPROP	0.000	12.433	0	1453759	N.D.	7.198 #
15) T	Picloram	17.180	17.004	4289946	6905961	2.369	4.535 #
16) T	DCPA	0.000	17.004	0	6905961	N.D.	4.017 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071318\
Data File : PS001028.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2018 19:18
Operator : UA
Sample : J3947-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 00:43:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

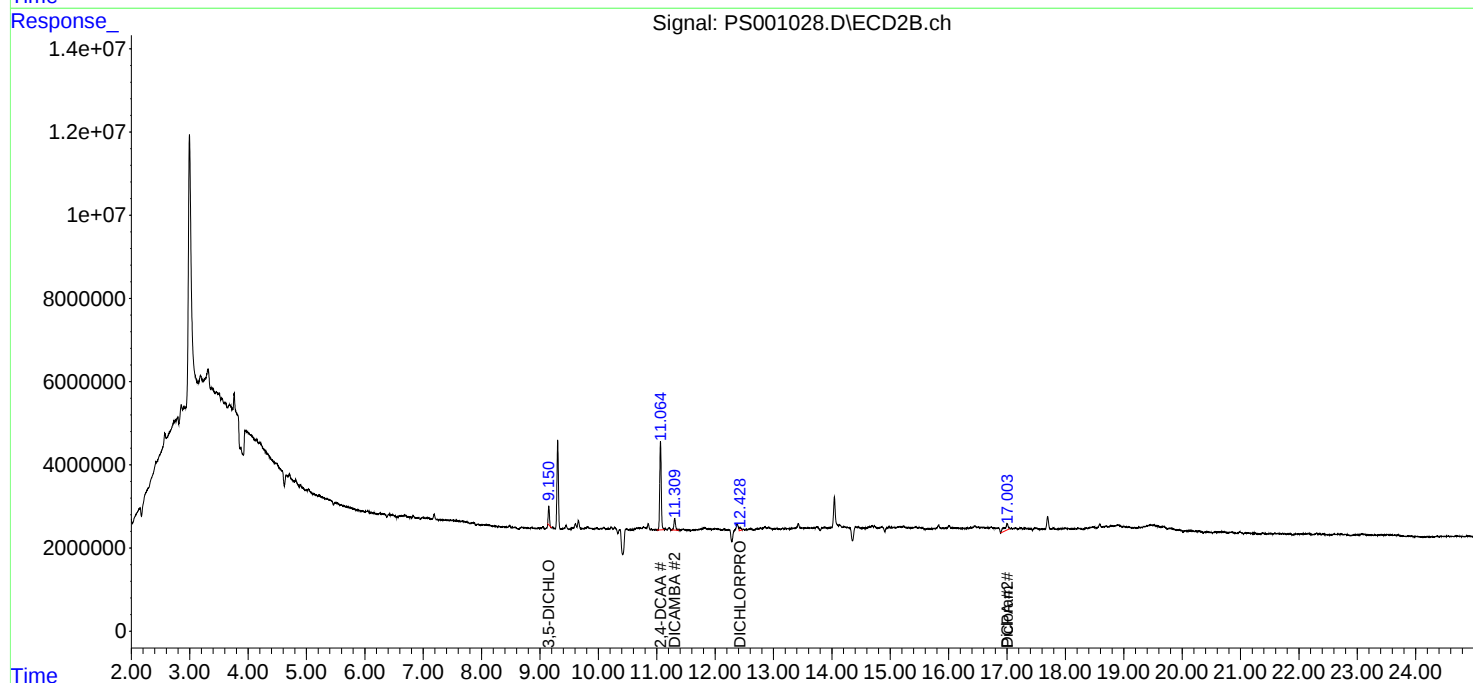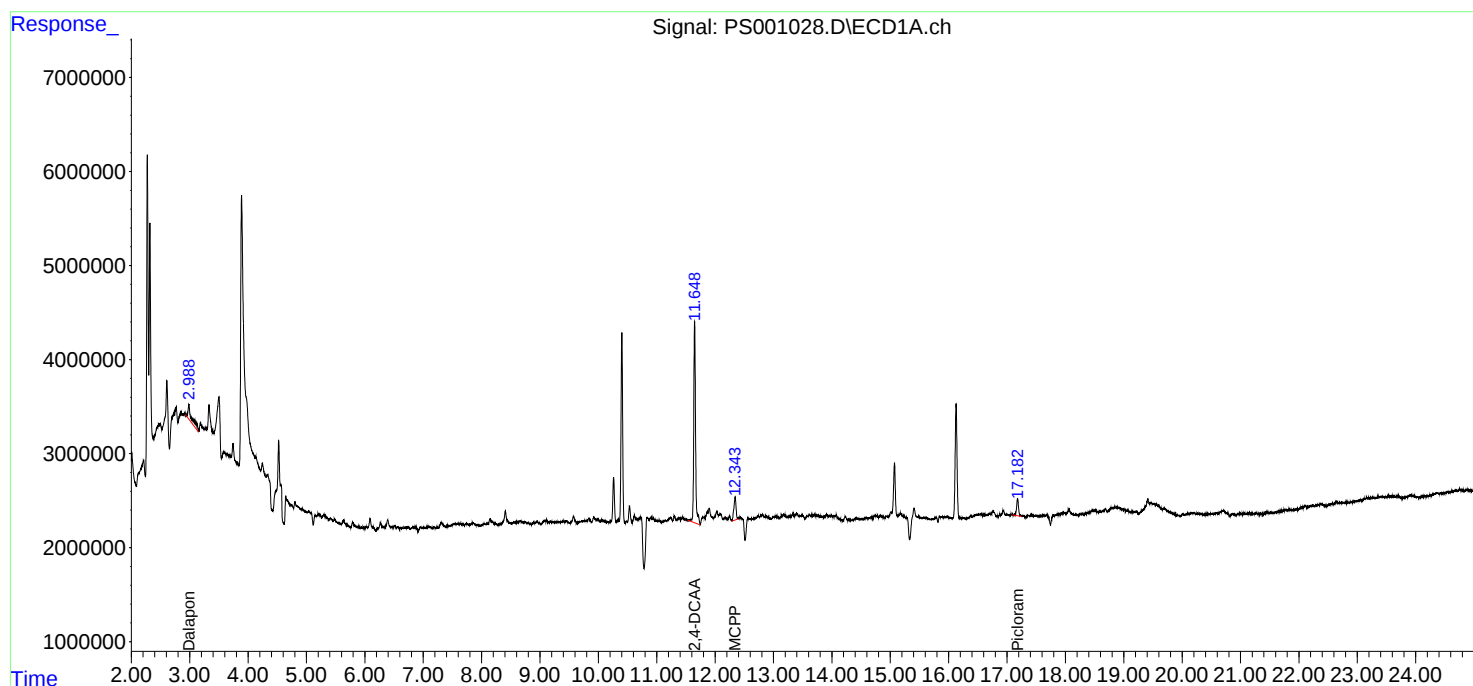


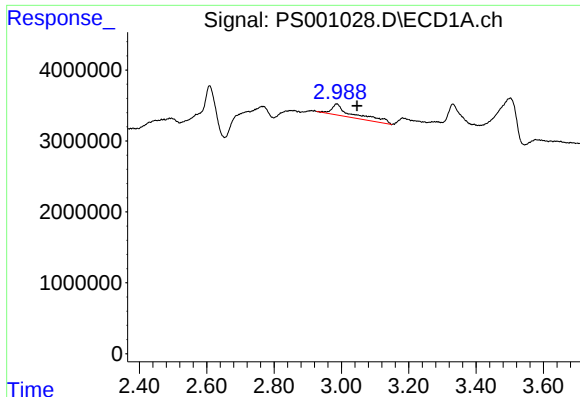

#1 Dalapon


R.T.: 2.986 min
Delta R.T.: -0.060 min
Response: 7026821
Conc: 26.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

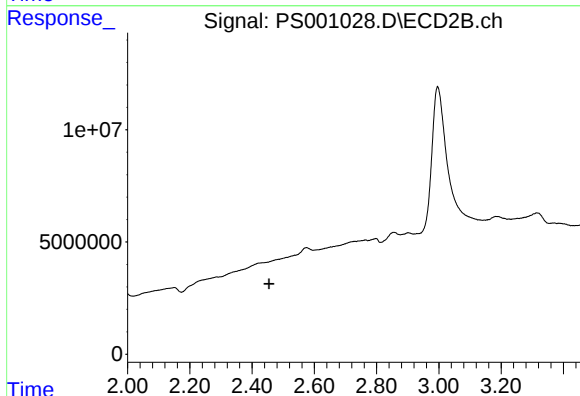


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.455 min
Response: 0
Conc: N.D.

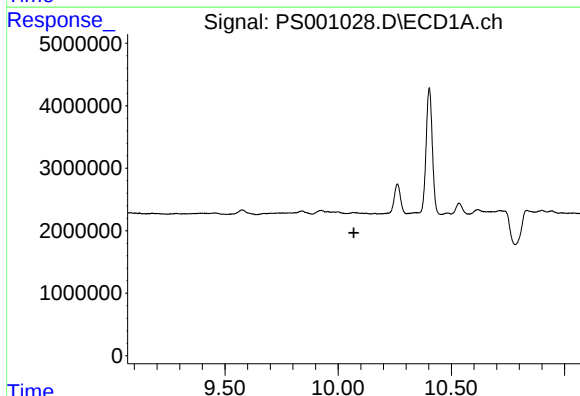


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

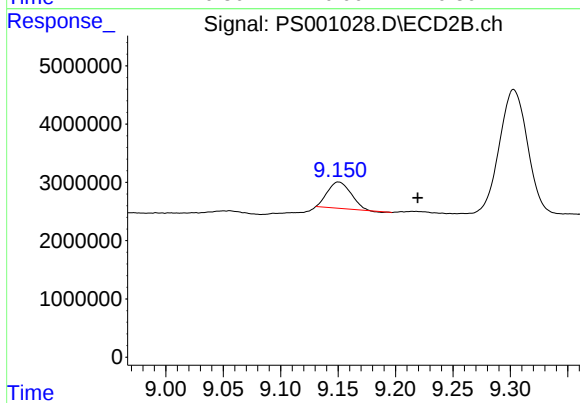

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.150 min
Delta R.T.: -0.069 min
Response: 6415646
Conc: 21.81 ng/ml

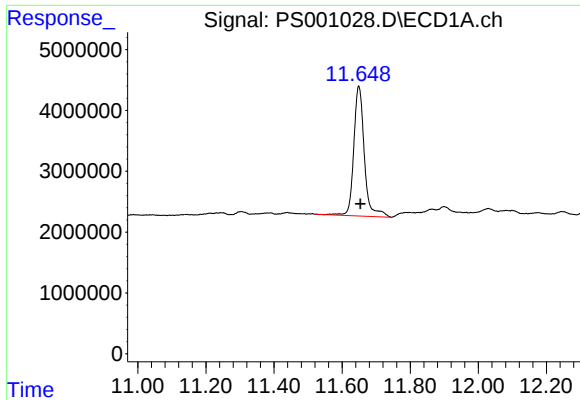

#4 2,4-DCAA


R.T.: 11.649 min
Delta R.T.: -0.004 min
Response: 45998317
Conc: 222.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

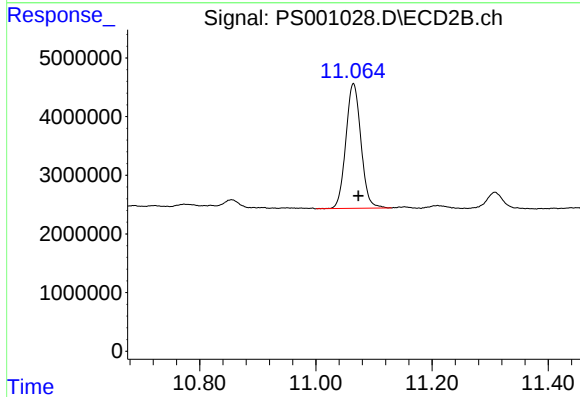


#4 2,4-DCAA

R.T.: 11.065 min
Delta R.T.: -0.009 min
Response: 38330911
Conc: 175.99 ng/ml

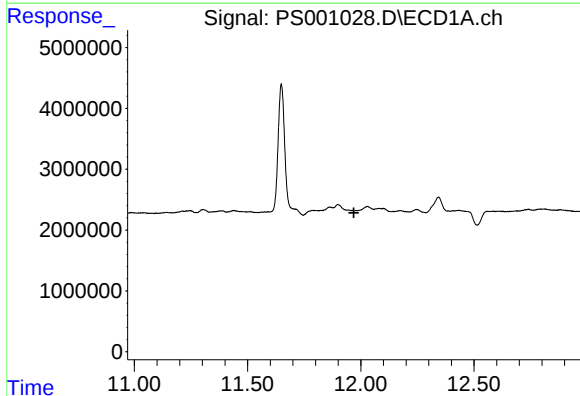


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.970 min
Response: 0
Conc: N.D.

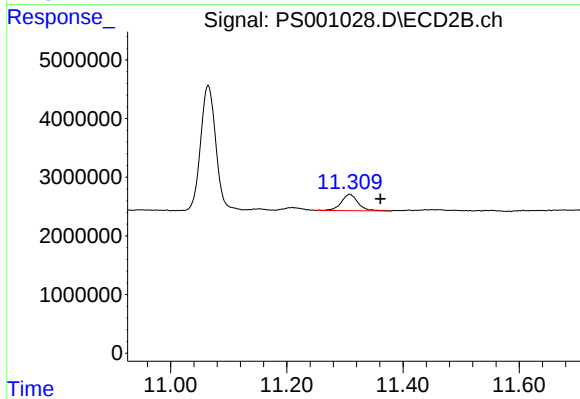

#5 DICAMBA


R.T.: 11.308 min
Delta R.T.: -0.053 min
Response: 5472173
Conc: 6.97 ng/ml

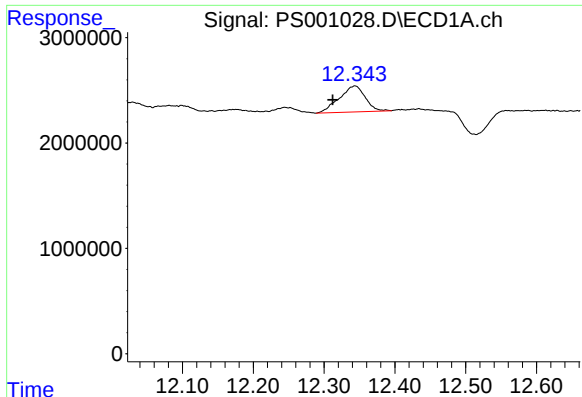

#6 MCP


R.T.: 12.343 min
Delta R.T.: 0.031 min
Response: 6280534
Conc: 11.43 ug/ml

Instrument :
ECD_S
ClientSampleId :

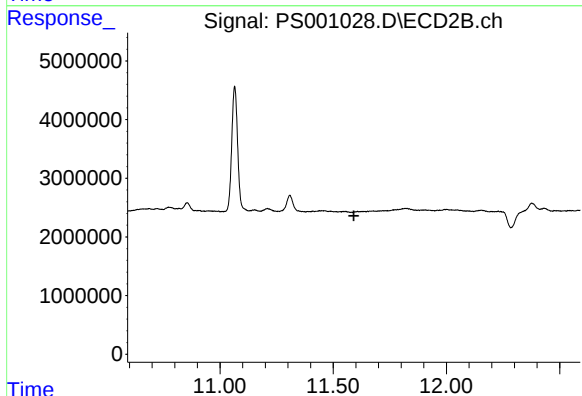


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

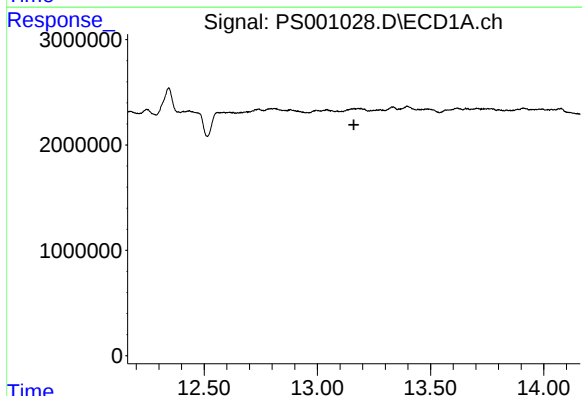


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

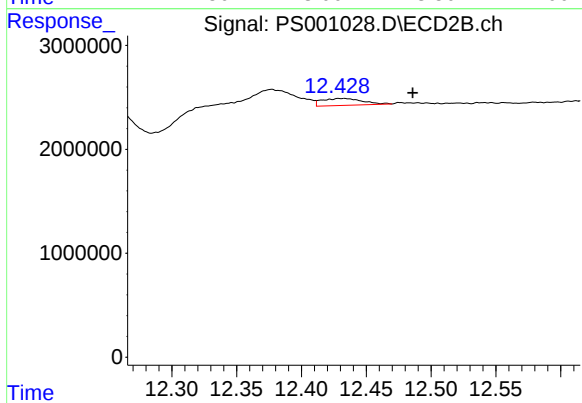

#8 DICHLORPROP


R.T.: 12.433 min
Delta R.T.: -0.053 min
Response: 1453759
Conc: 7.20 ng/ml

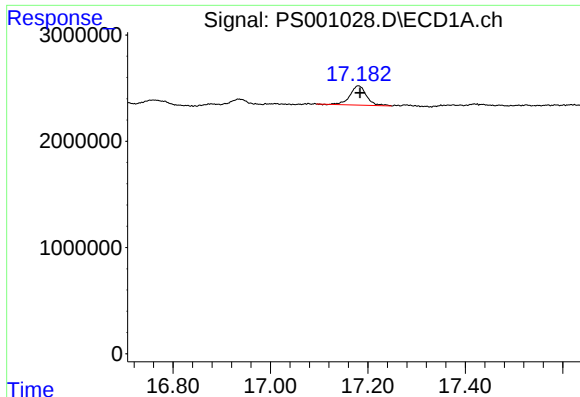

#15 Picloram


R.T.: 17.180 min
Delta R.T.: -0.003 min
Response: 4289946
Conc: 2.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

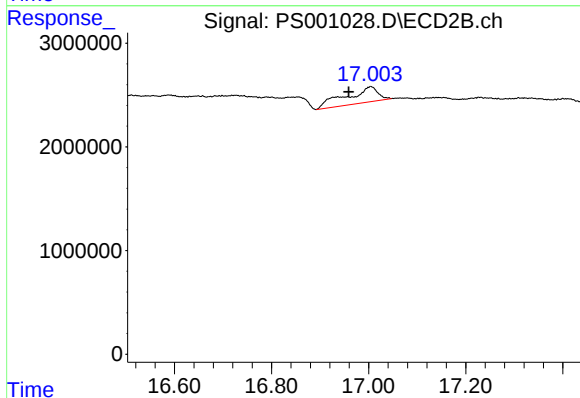


#15 Picloram

R.T.: 17.004 min
Delta R.T.: 0.045 min
Response: 6905961
Conc: 4.54 ng/ml

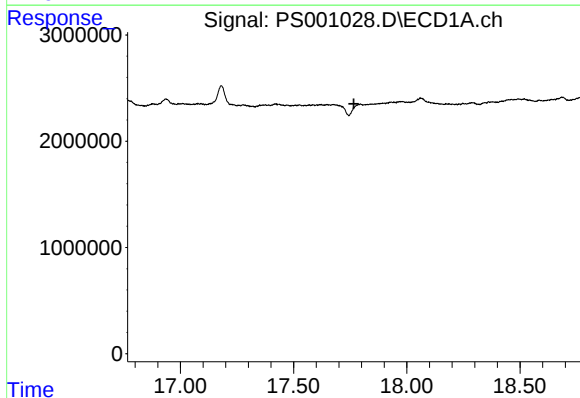

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.766 min
Response: 0
Conc: N.D.

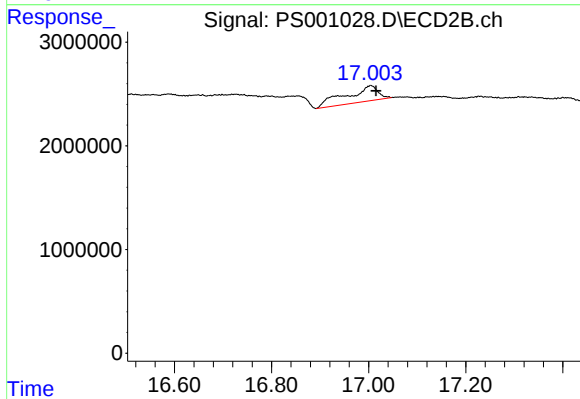

#16 DCPA

R.T.: 17.004 min
Delta R.T.: -0.011 min
Response: 6905961
Conc: 4.02 ng/ml