

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071320\
 Data File : PS011176.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2020 17:47
 Operator : DD\AJ
 Sample : PB130012BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 18:45:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	6.918	258.8E6	181.7E6	266.735	322.810
Target Compounds							
1) T	Dalapon	2.992	2.583	51993866	184.6E6	43.207	240.492 #
2) T	3,5-DICHL...	0.000	6.098	0	71545217	N.D.	85.189
3) T	4-Nitroph...	6.996	0.000	6295000	0	14.279	N.D. #
5) T	DICAMBA	7.407	0.000	6977155	0	1.800	N.D. #
6) T	MCPD	7.638	0.000	5187002	0	1.713	N.D. #
7) T	MCPA	7.689	7.457	236.4E6	227.0E6	55.428	78.742 #
8) T	DICHLORPROP	0.000	7.739	0	9855436	N.D.	16.373
10) T	Pentachlo...	8.706	0.000	12726444	0	<MDL	N.D. #
12) T	2,4,5-T	9.424	0.000	26285371	0	5.209	N.D. #
15) T	Picloram	11.030	11.010	20326594	12075670	3.221	2.761
16) T	DCPA	0.000	11.010	0	12075670	N.D.	3.193



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071320\
Data File : PS011176.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2020 17:47
Operator : DD\AJ
Sample : PB130012BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 18:45:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

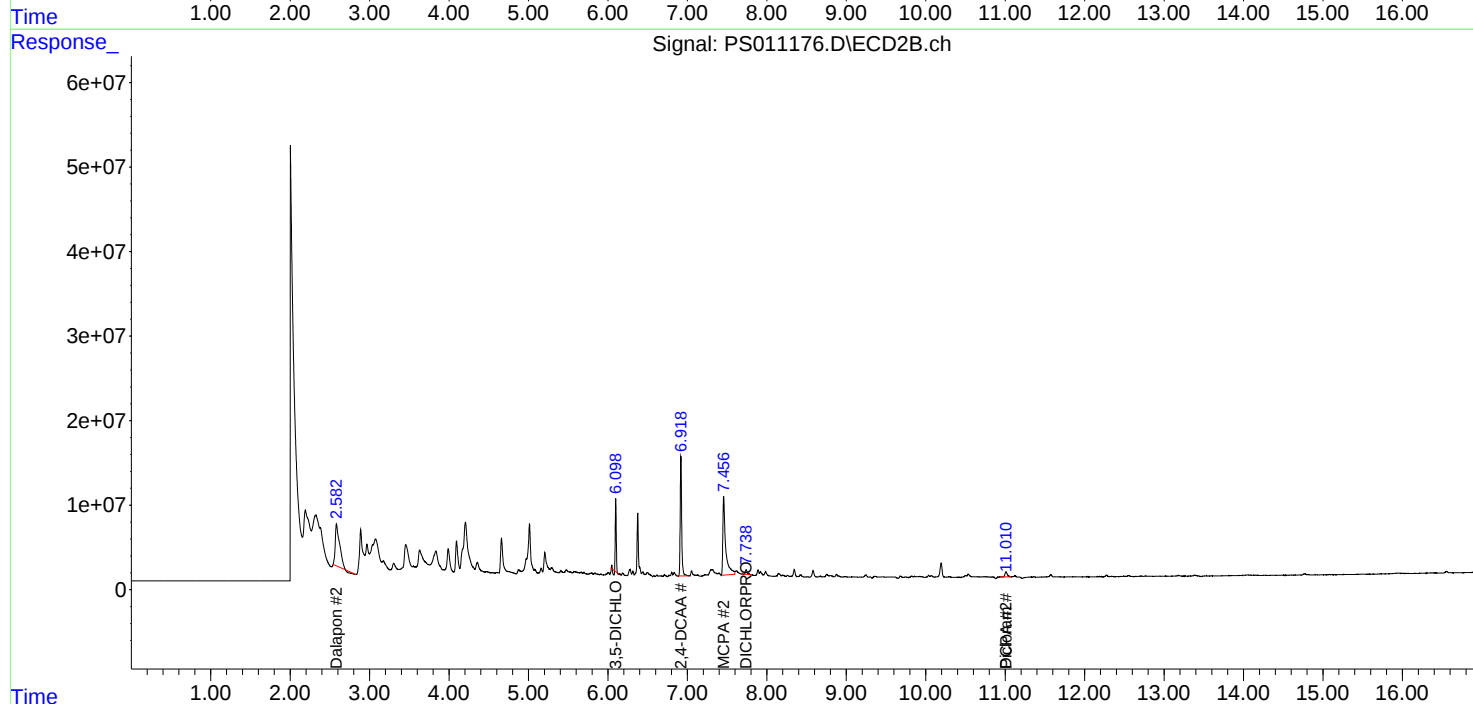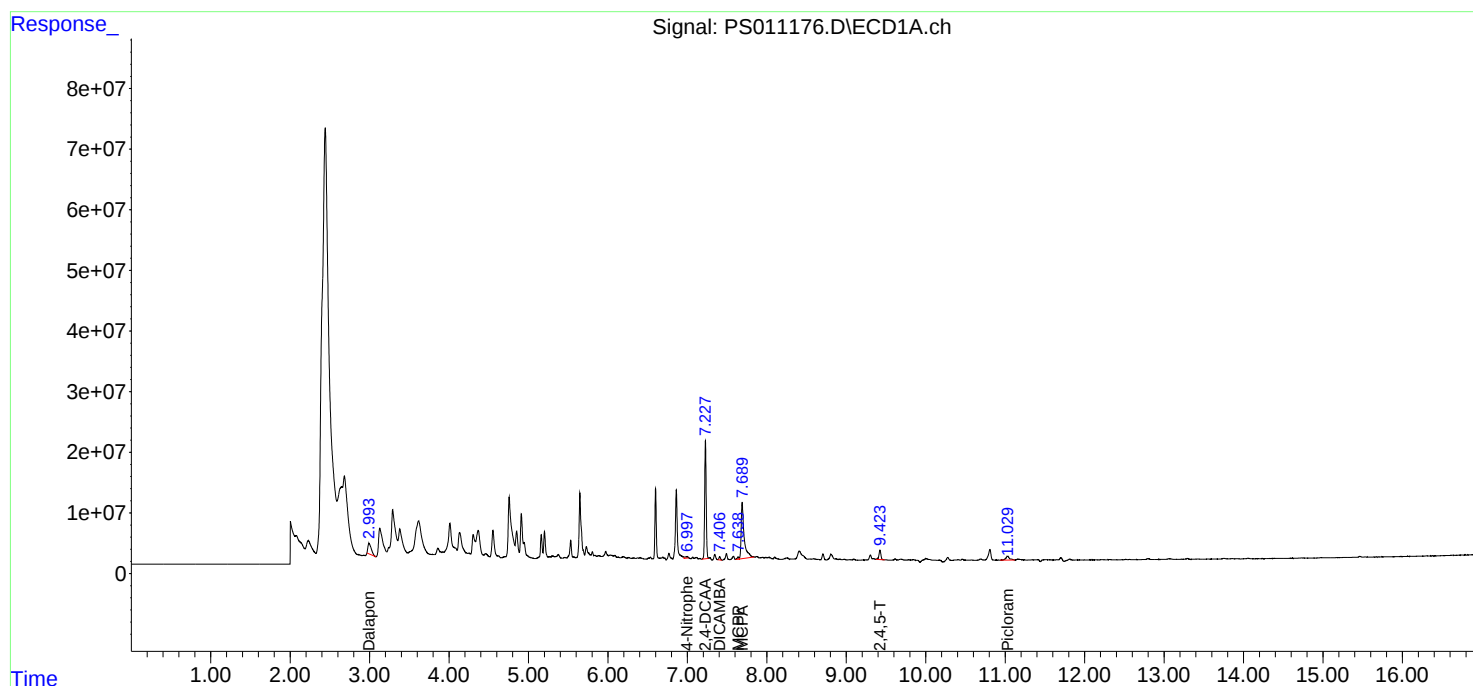


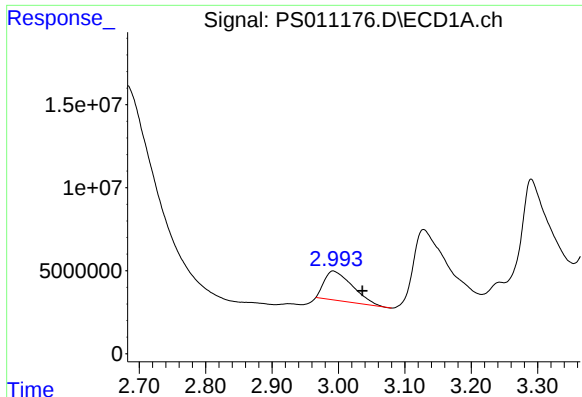

#1 Dalapon


R.T.: 2.992 min
Delta R.T.: -0.044 min
Response: 51993866
Conc: 43.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

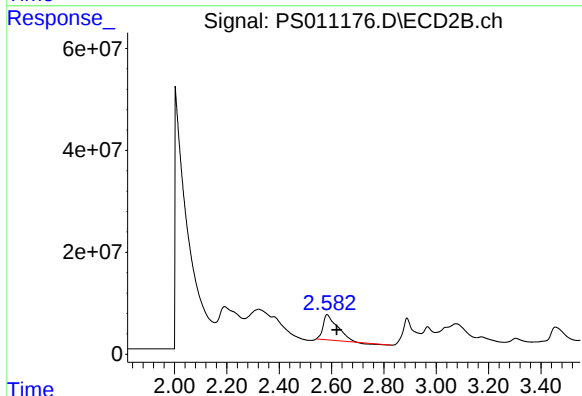


#1 Dalapon

R.T.: 2.583 min
Delta R.T.: -0.037 min
Response: 184619157
Conc: 240.49 ng/ml

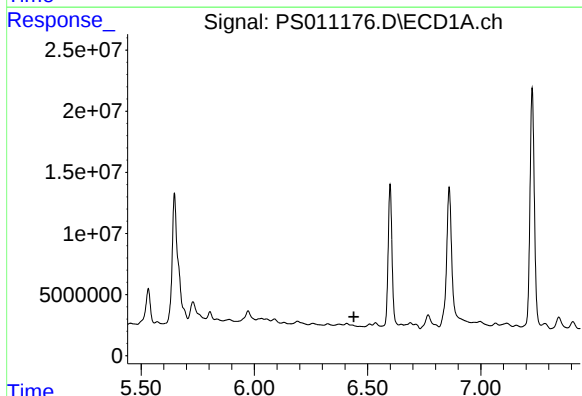


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.439 min
Response: 0
Conc: N.D.

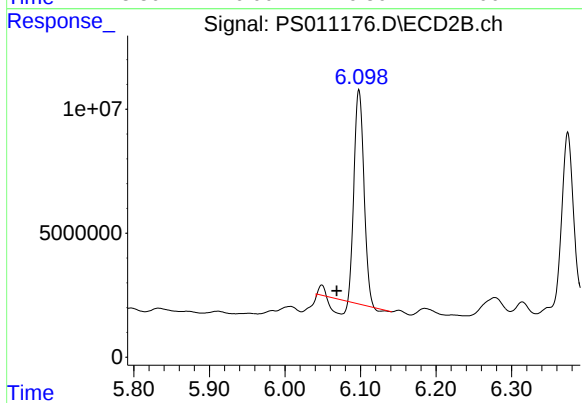

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.098 min
Delta R.T.: 0.030 min
Response: 71545217
Conc: 85.19 ng/ml

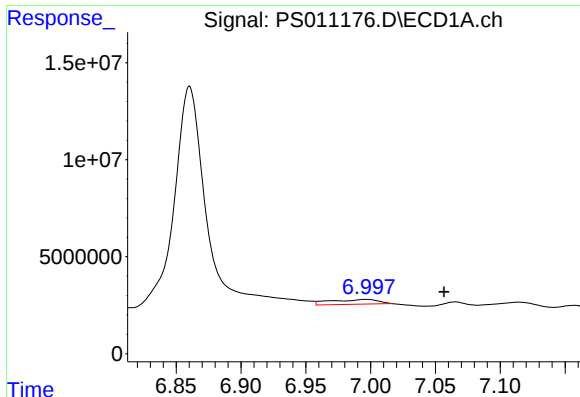

#3 4-Nitrophenol


R.T.: 6.996 min
Delta R.T.: -0.061 min
Response: 6295000
Conc: 14.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

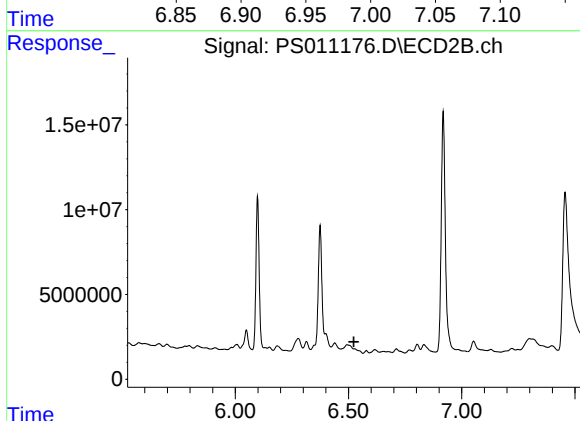


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.524 min
Response: 0
Conc: N.D.

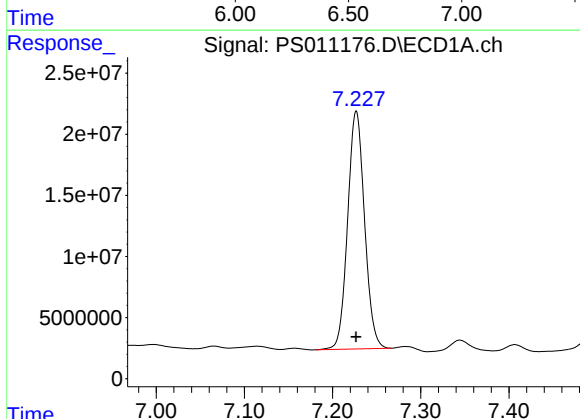


#4 2,4-DCAA

R.T.: 7.227 min
Delta R.T.: 0.000 min
Response: 258823224
Conc: 266.74 ng/ml

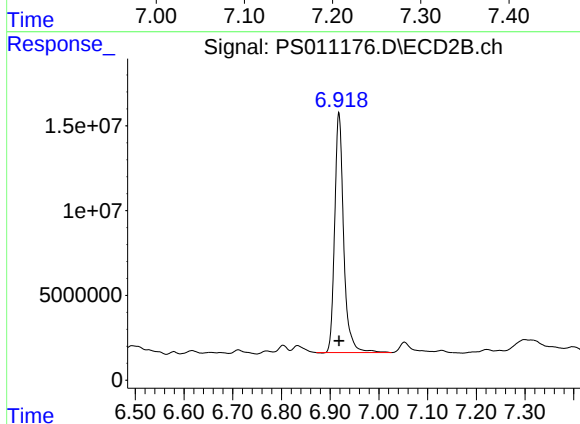

#4 2,4-DCAA


R.T.: 6.918 min
Delta R.T.: 0.000 min
Response: 181749345
Conc: 322.81 ng/ml

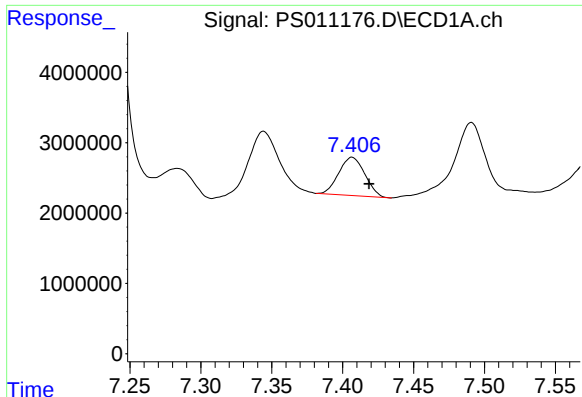

#5 DICAMBA


R.T.: 7.407 min
Delta R.T.: -0.012 min
Response: 6977155
Conc: 1.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

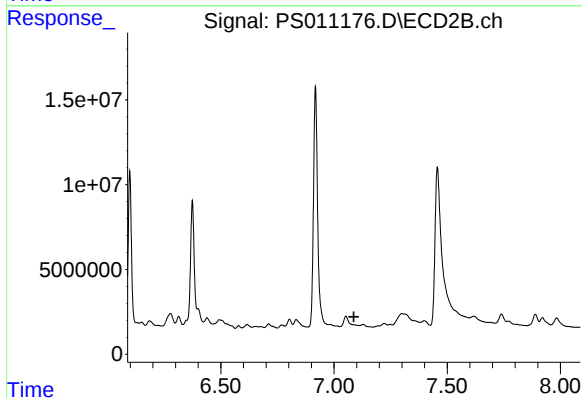


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.088 min
Response: 0
Conc: N.D.

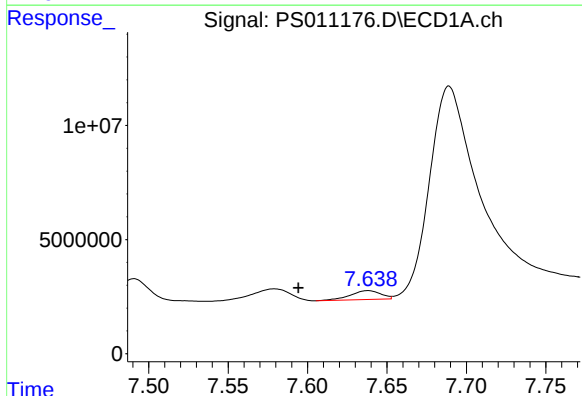


#6 MCP

R.T.: 7.638 min
Delta R.T.: 0.044 min
Response: 5187002
Conc: 1.71 ug/ml

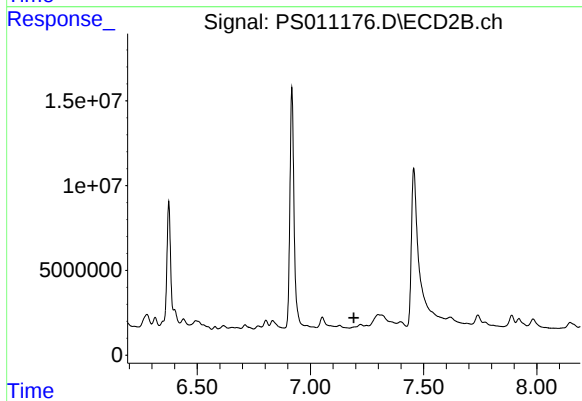

#6 MCP


R.T.: 0.000 min
Exp R.T. : 7.192 min
Response: 0
Conc: N.D.

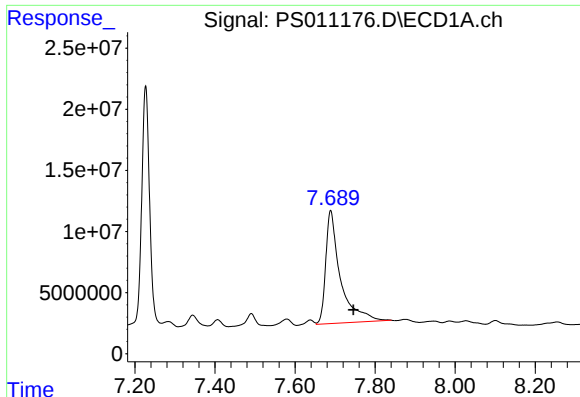

#7 MCPA


R.T.: 7.689 min
Delta R.T.: -0.057 min
Response: 236382899
Conc: 55.43 ug/ml

Instrument :
ECD_S
ClientSampleId :

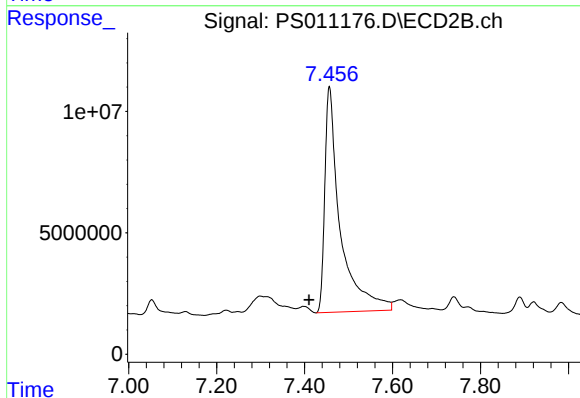


#7 MCPA

R.T.: 7.457 min
Delta R.T.: 0.047 min
Response: 226960001
Conc: 78.74 ug/ml

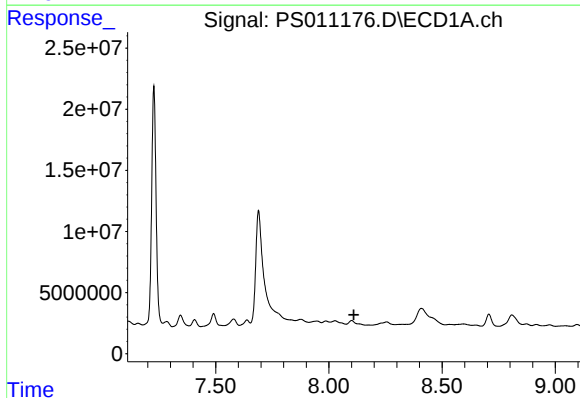


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.110 min
Response: 0
Conc: N.D.

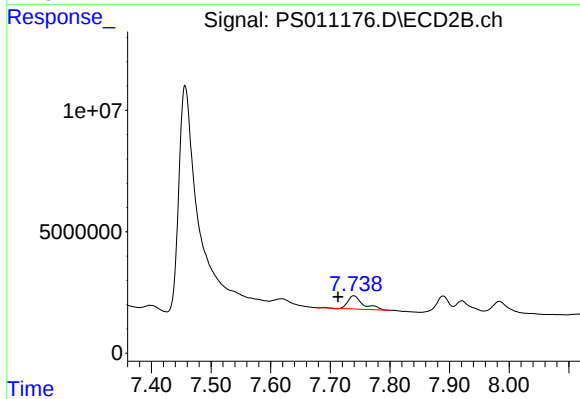

#8 DICHLORPROP


R.T.: 7.739 min
Delta R.T.: 0.026 min
Response: 9855436
Conc: 16.37 ng/ml

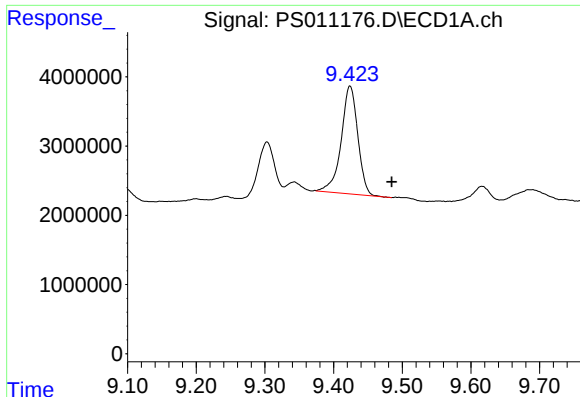

#12 2,4,5-T


R.T.: 9.424 min
Delta R.T.: -0.061 min
Response: 26285371
Conc: 5.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

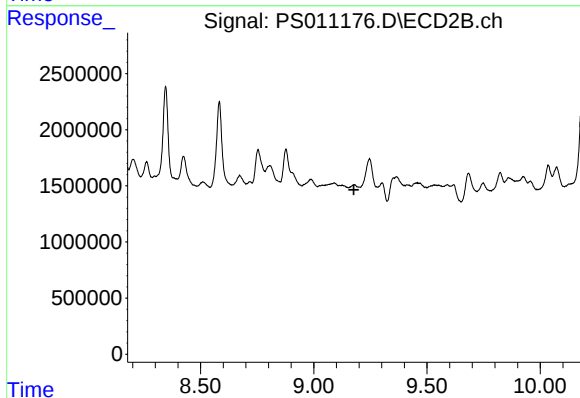


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.177 min
Response: 0
Conc: N.D.

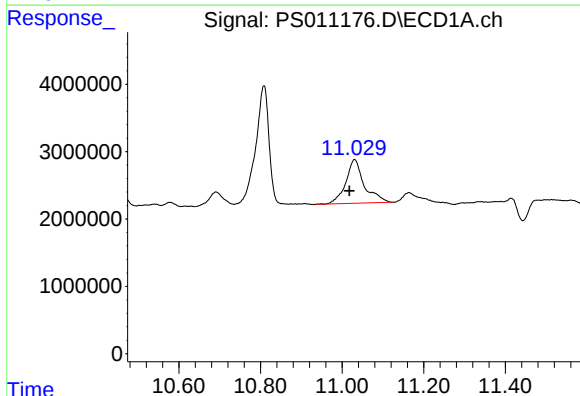


#15 Picloram

R.T.: 11.030 min
Delta R.T.: 0.012 min
Response: 20326594
Conc: 3.22 ng/ml

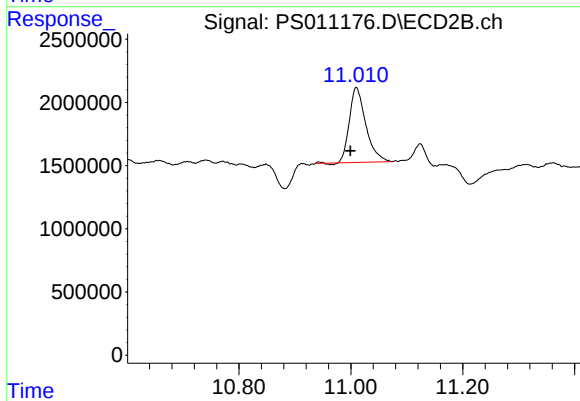

#15 Picloram


R.T.: 11.010 min
Delta R.T.: 0.010 min
Response: 12075670
Conc: 2.76 ng/ml

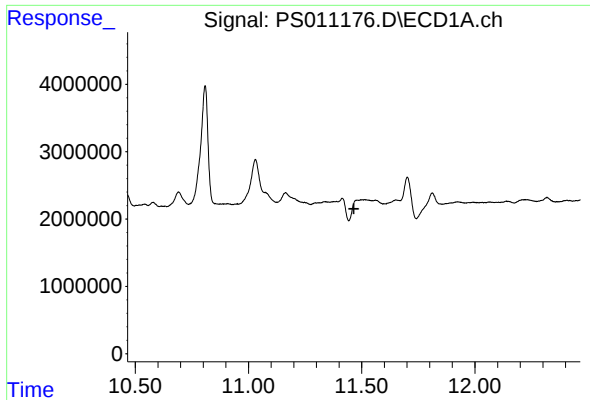

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.466 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

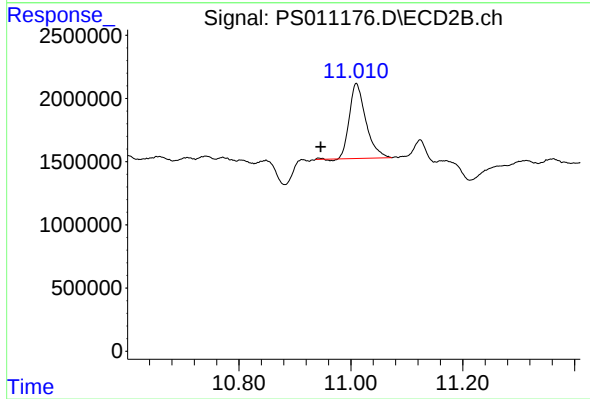

#16 DCPA

R.T.: 11.010 min
Delta R.T.: 0.064 min
Response: 12075670
Conc: 3.19 ng/ml