

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071320\
 Data File : PS011188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2020 22:23
 Operator : DD\AJ
 Sample : L3255-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 01:59:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.226	6.917	87169433	40288582	89.834	71.558
Target Compounds							
2) T	3,5-DICHL...	0.000	6.098	0	52544423	N.D.	62.565
6) T	MCP	7.576	0.000	6545347	0	2.161	N.D. #
7) T	MCPA	7.739	7.382	6255607	32232930	1.467	11.183 #
8) T	DICHLORPROP	8.125	7.719	8216767	8614103	8.764	14.311 #
9) T	2,4-D	8.374	7.986	-6351204	16753652	N.D.	22.348
10) T	Pentachlo...	8.713	8.468	35269046	8562905	2.668	1.229 #
12) T	2,4,5-T	9.530	9.167	26413938	6673313	5.235	2.200 #
13) T	2,4-DB	0.000	9.707	0	26916852	N.D.	62.964
14) T	DINOSEB	11.166	10.032	47437895	35607846	12.307	16.601 #
15) T	Picloram	10.990	11.022	179.4E6	20928222	28.435	4.785 #
16) T	DCPA	11.497	0.000	10689415	0	1.659	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071320\
Data File : PS011188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2020 22:23
Operator : DD\AJ
Sample : L3255-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 01:59:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

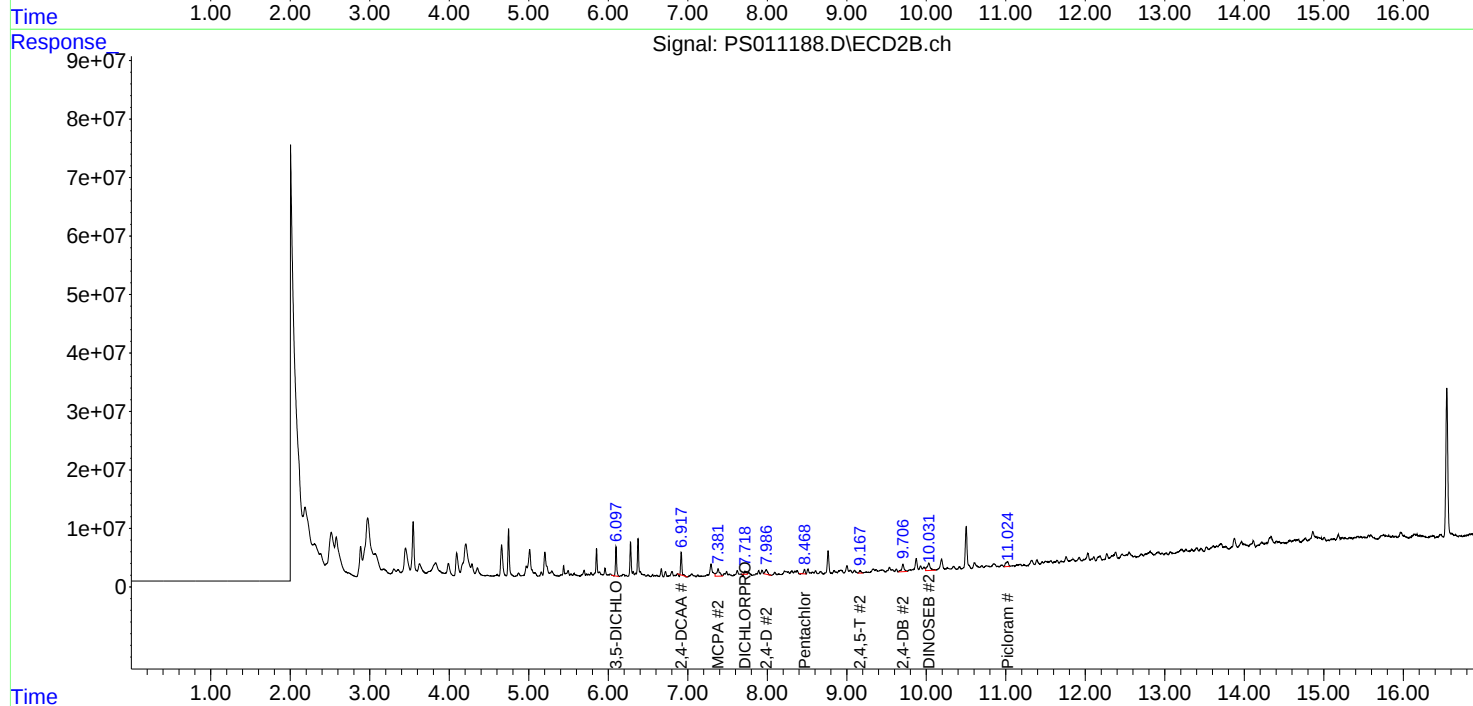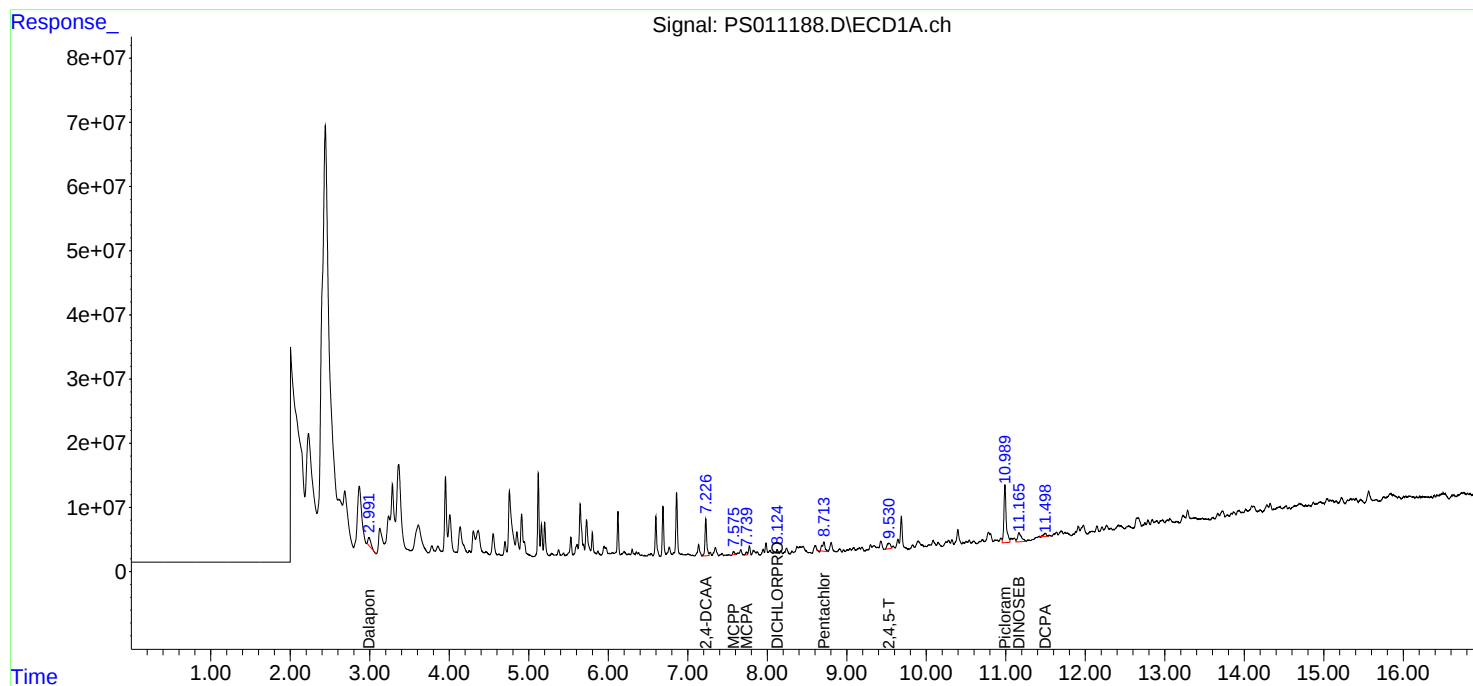


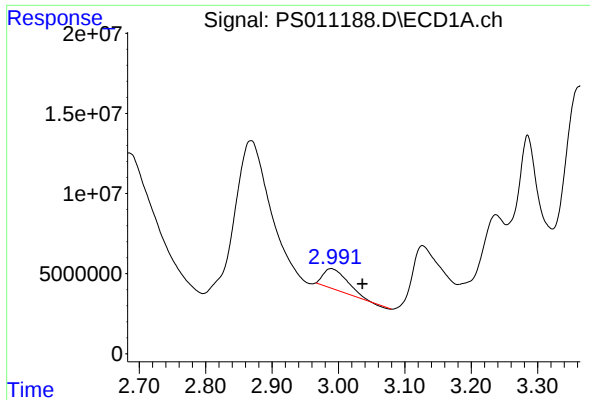

#1 Dalapon


R.T.: 2.989 min
Delta R.T.: -0.047 min
Response: 31384689
Conc: 26.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

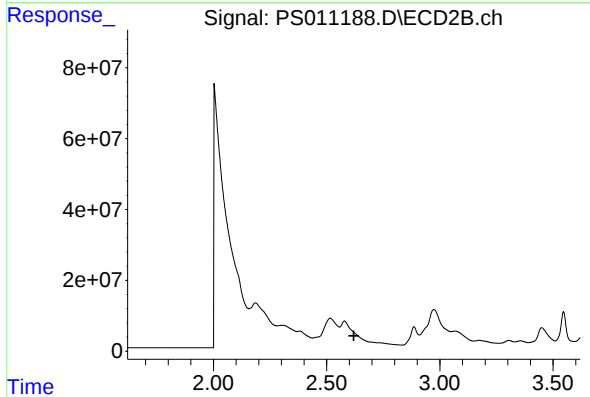


#1 Dalapon

R.T.: 2.579 min
Delta R.T.: -0.042 min
Response: -145284549
Conc: N.D.

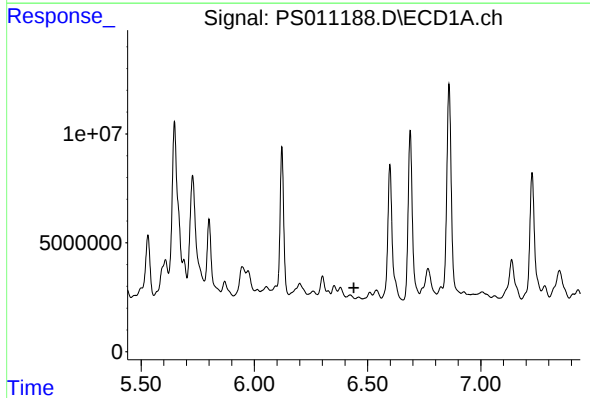


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.439 min
Response: 0
Conc: N.D.

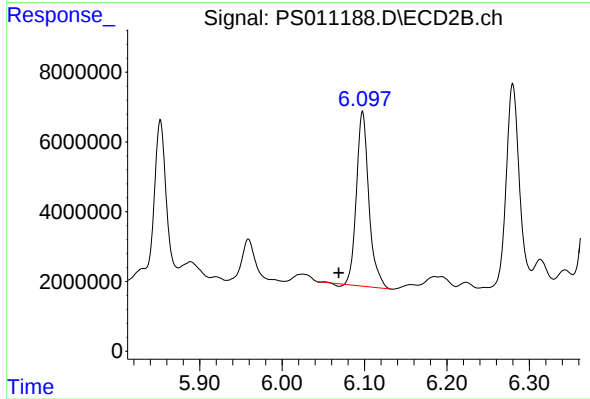

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.098 min
Delta R.T.: 0.029 min
Response: 52544423
Conc: 62.56 ng/ml

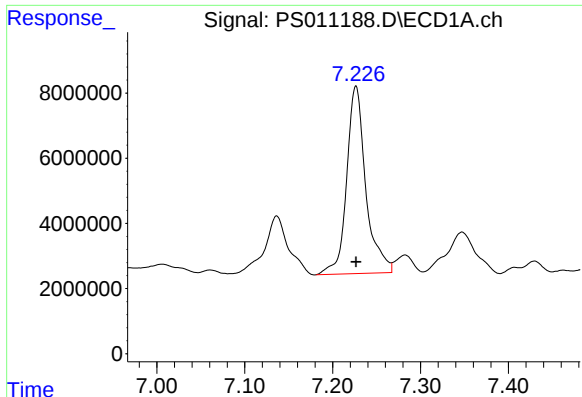

#4 2,4-DCAA


R.T.: 7.226 min
Delta R.T.: 0.000 min
Response: 87169433
Conc: 89.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

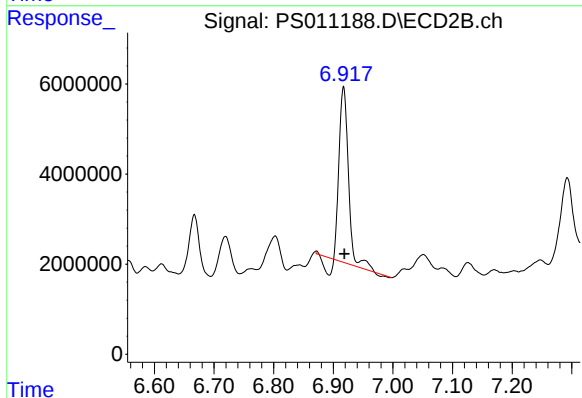


#4 2,4-DCAA

R.T.: 6.917 min
Delta R.T.: -0.001 min
Response: 40288582
Conc: 71.56 ng/ml

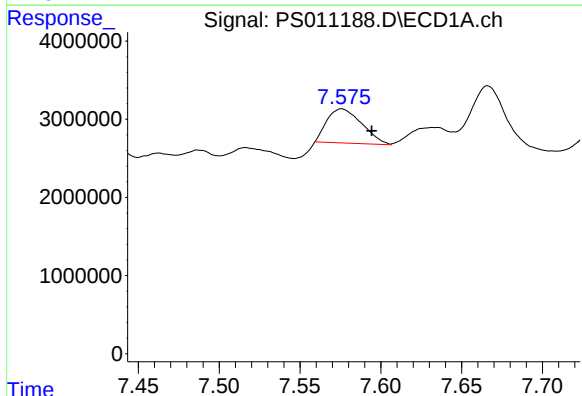


#6 MCP

R.T.: 7.576 min
Delta R.T.: -0.018 min
Response: 6545347
Conc: 2.16 ug/ml

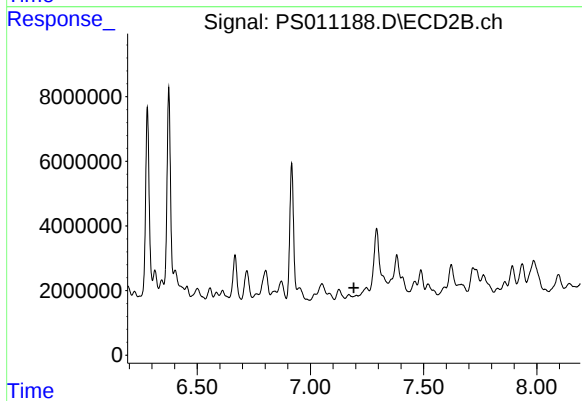

#6 MCP


R.T.: 0.000 min
Exp R.T. : 7.192 min
Response: 0
Conc: N.D.

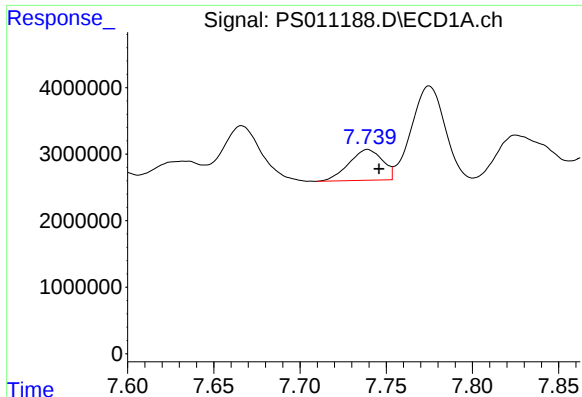

#7 MCPA


R.T.: 7.739 min
Delta R.T.: -0.006 min
Response: 6255607
Conc: 1.47 ug/ml

Instrument :
ECD_S
ClientSampleId :

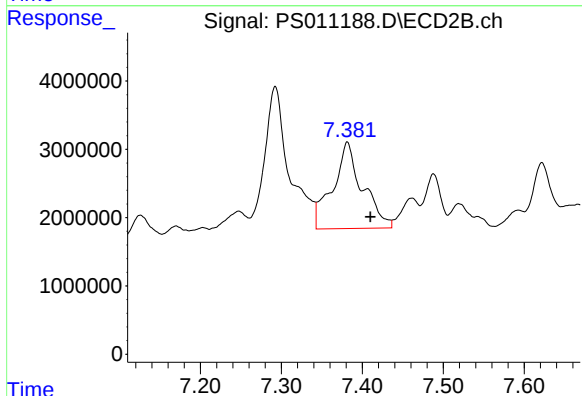


#7 MCPA

R.T.: 7.382 min
Delta R.T.: -0.028 min
Response: 32232930
Conc: 11.18 ug/ml

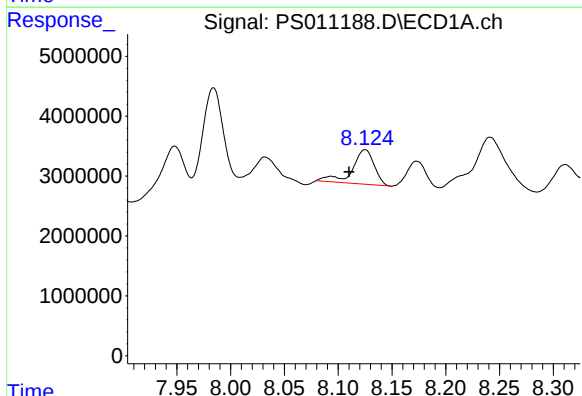


#8 DICHLORPROP

R.T.: 8.125 min
Delta R.T.: 0.015 min
Response: 8216767
Conc: 8.76 ng/ml

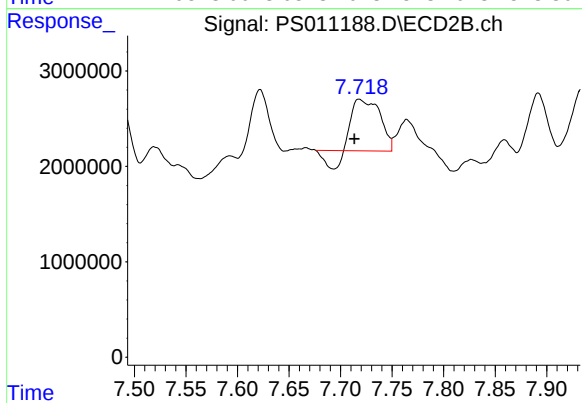

#8 DICHLORPROP


R.T.: 7.719 min
Delta R.T.: 0.006 min
Response: 8614103
Conc: 14.31 ng/ml

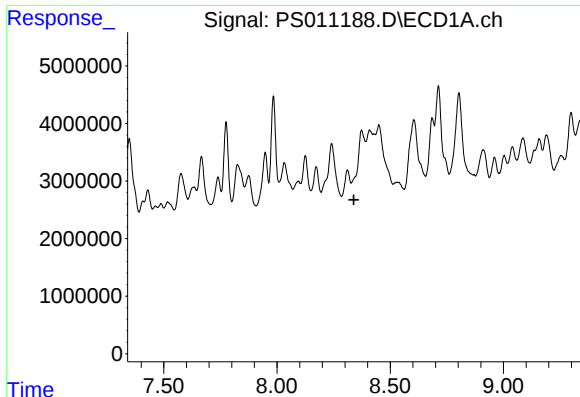

#9 2,4-D


R.T.: 8.374 min
Delta R.T.: 0.034 min
Response: -6351204
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

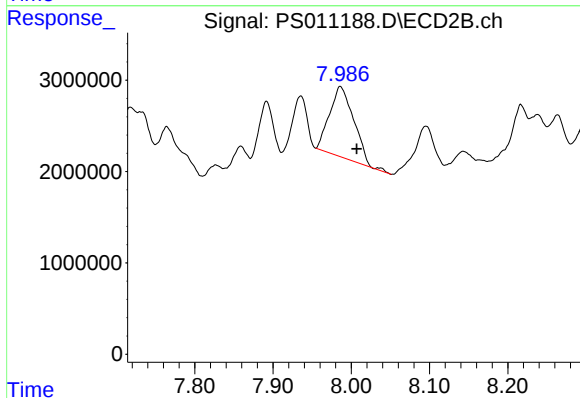


#9 2,4-D

R.T.: 7.986 min
Delta R.T.: -0.021 min
Response: 16753652
Conc: 22.35 ng/ml

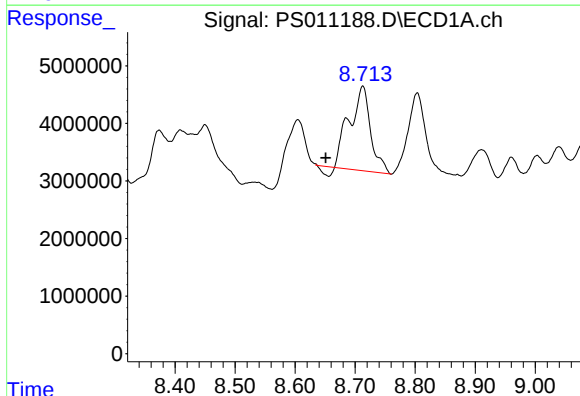


#10 Pentachlorophenol

R.T.: 8.713 min
Delta R.T.: 0.061 min
Response: 35269046
Conc: 2.67 ng/ml

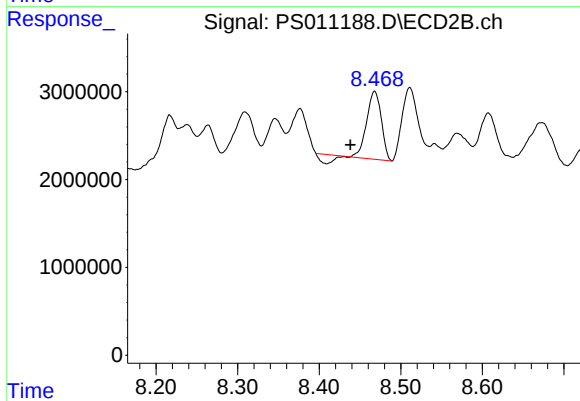

#10 Pentachlorophenol


R.T.: 8.468 min
Delta R.T.: 0.030 min
Response: 8562905
Conc: 1.23 ng/ml

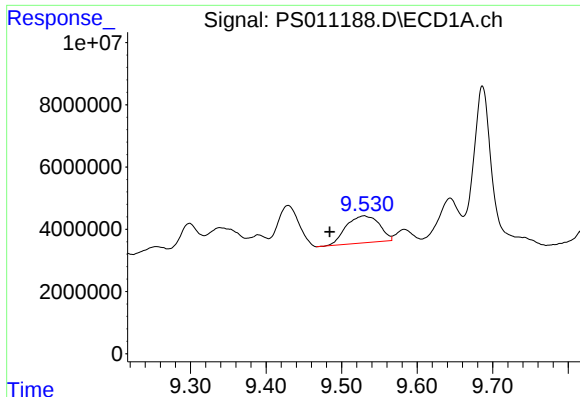

#12 2,4,5-T


R.T.: 9.530 min
Delta R.T.: 0.045 min
Response: 26413938
Conc: 5.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

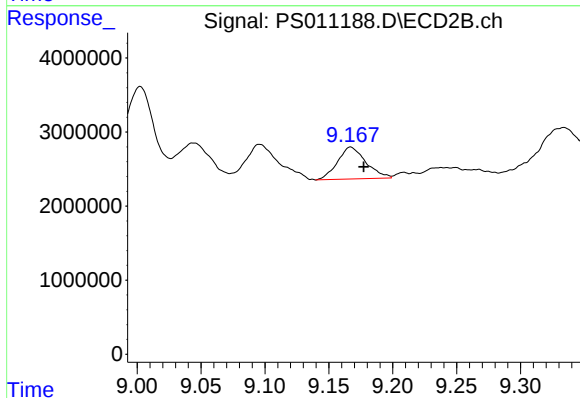


#12 2,4,5-T

R.T.: 9.167 min
Delta R.T.: -0.010 min
Response: 6673313
Conc: 2.20 ng/ml

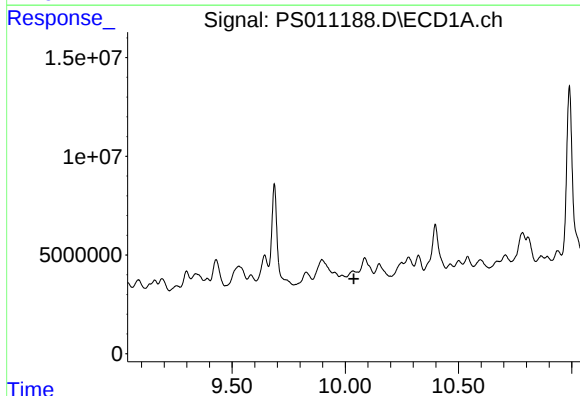


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.038 min
Response: 0
Conc: N.D.

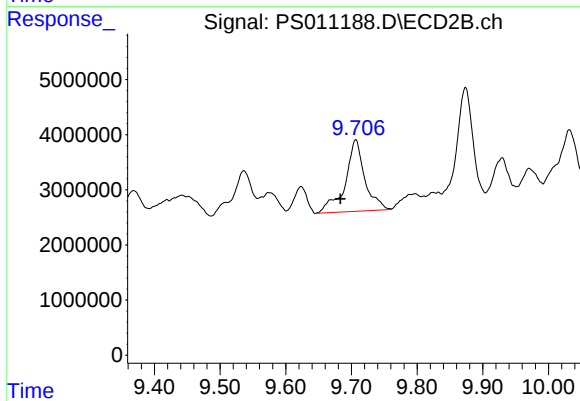

#13 2,4-DB


R.T.: 9.707 min
Delta R.T.: 0.024 min
Response: 26916852
Conc: 62.96 ng/ml

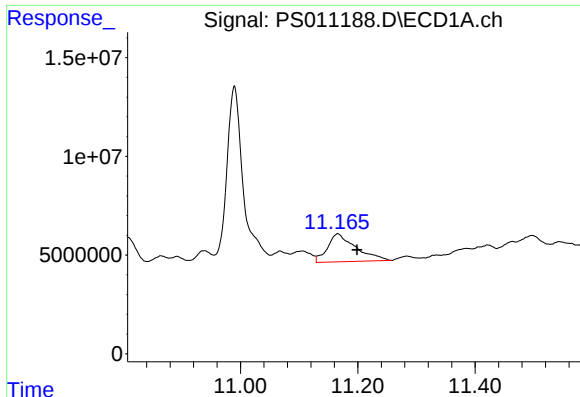

#14 DINOSEB


R.T.: 11.166 min
Delta R.T.: -0.033 min
Response: 47437895
Conc: 12.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

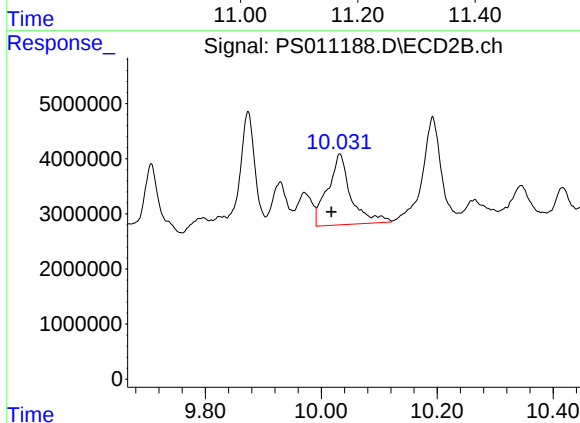


#14 DINOSEB

R.T.: 10.032 min
Delta R.T.: 0.015 min
Response: 35607846
Conc: 16.60 ng/ml

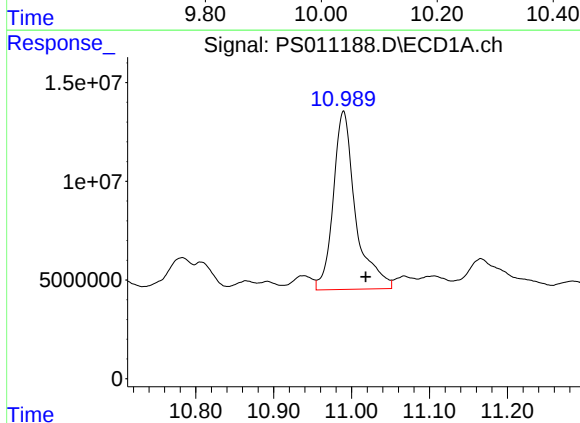


#15 Picloram

R.T.: 10.990 min
Delta R.T.: -0.029 min
Response: 179423209
Conc: 28.44 ng/ml

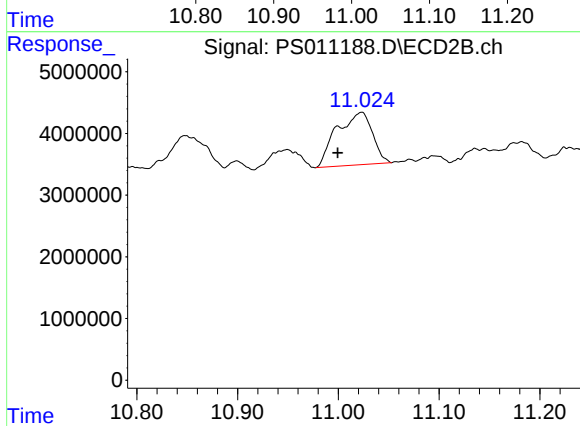

#15 Picloram


R.T.: 11.022 min
Delta R.T.: 0.023 min
Response: 20928222
Conc: 4.79 ng/ml

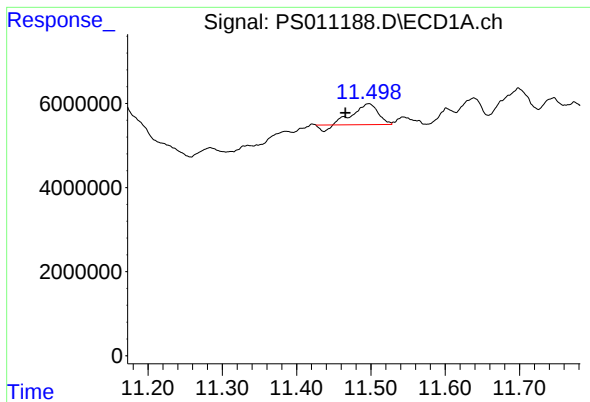

#16 DCPA

R.T.: 11.497 min
Delta R.T.: 0.031 min
Response: 10689415
Conc: 1.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

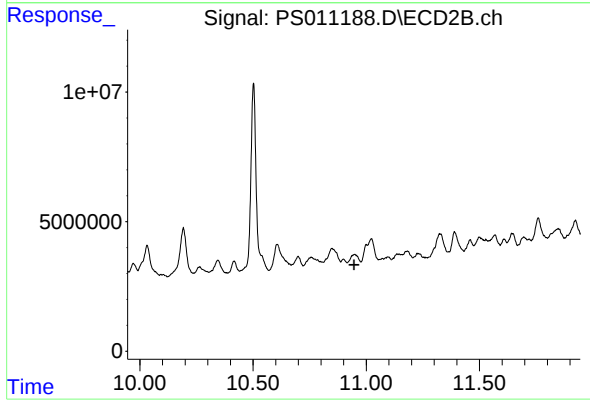

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.946 min
Response: 0
Conc: N.D.