

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071320\
 Data File : PS011190.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2020 23:09
 Operator : DD\AJ
 Sample : L3255-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 01:59:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.226	6.917	245.3E6	148.0E6	252.823	262.952
Target Compounds							
1) T	Dalapon	2.990	2.580	38068348	6390200	31.635	8.324 #
2) T	3,5-DICHL...	0.000	6.098	0	50327520	N.D.	59.925
6) T	MCP	7.585	0.000	8845245	0	2.921	N.D. #
7) T	MCPA	7.774	7.381	18624736	32115256	4.367	11.142 #
8) T	DICHLORPROP	0.000	7.735	0	5948139	N.D.	9.882
10) T	Pentachlo...	8.706	0.000	17859592	0	1.351	N.D. #
12) T	2,4,5-T	9.506	0.000	5881011	0	1.166	N.D. #
13) T	2,4-DB	9.987	9.706	9512870	9508909	14.759	22.243 #
14) T	DINOSEB	11.163	10.032	38494650	28091514	9.987	13.097 #
15) T	Picloram	10.990	0.000	149.2E6	0	23.644	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071320\
Data File : PS011190.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2020 23:09
Operator : DD\AJ
Sample : L3255-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 01:59:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

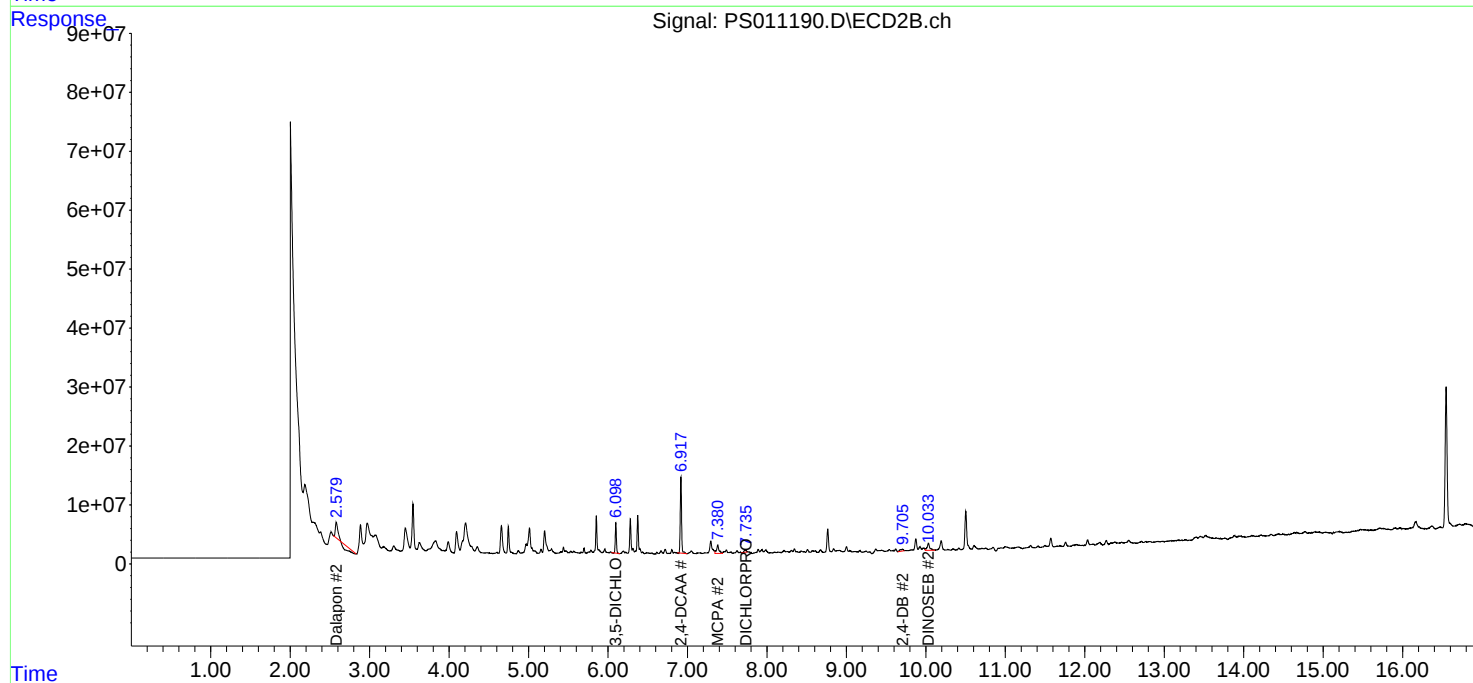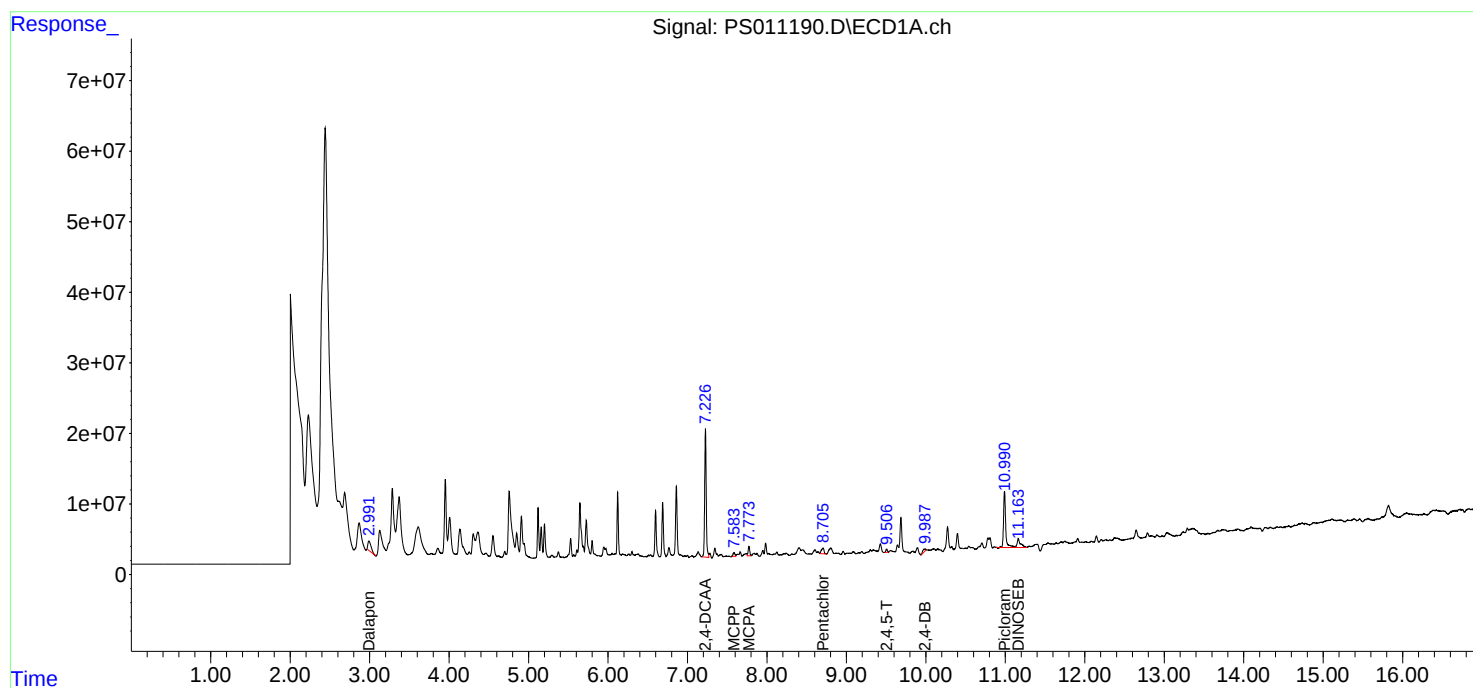


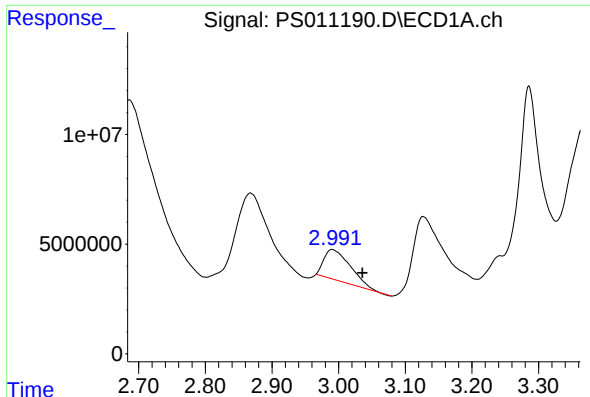

#1 Dalapon


R.T.: 2.990 min
Delta R.T.: -0.046 min
Response: 38068348
Conc: 31.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

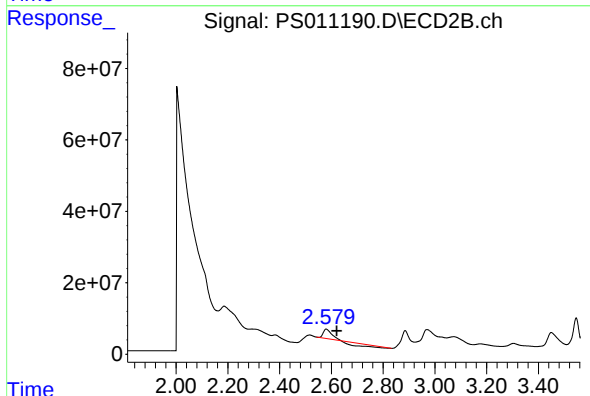


#1 Dalapon

R.T.: 2.580 min
Delta R.T.: -0.040 min
Response: 6390200
Conc: 8.32 ng/ml

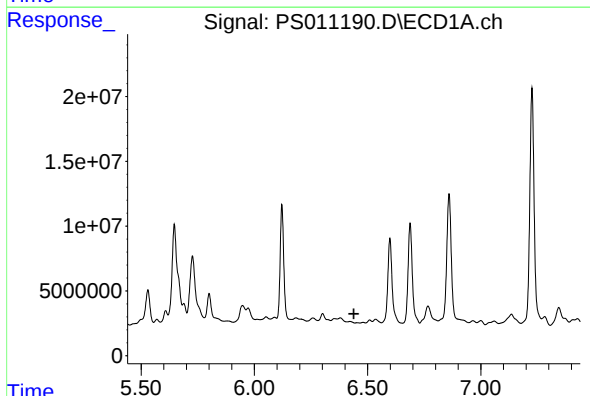


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.439 min
Response: 0
Conc: N.D.

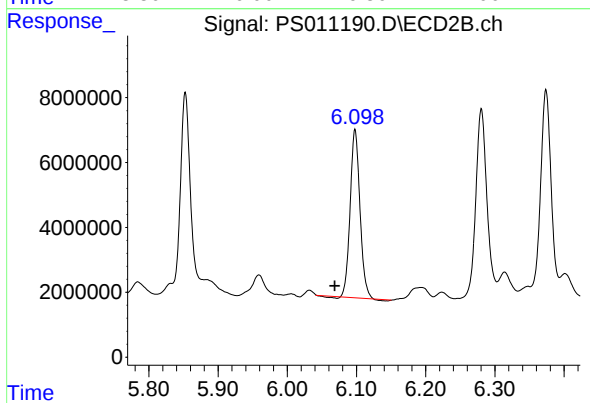

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.098 min
Delta R.T.: 0.030 min
Response: 50327520
Conc: 59.92 ng/ml

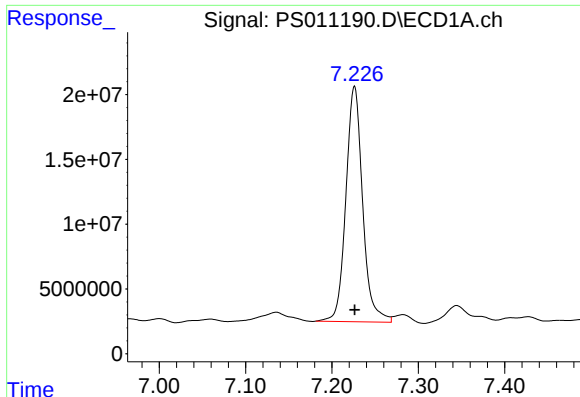

#4 2,4-DCAA


R.T.: 7.226 min
Delta R.T.: 0.000 min
Response: 245323906
Conc: 252.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

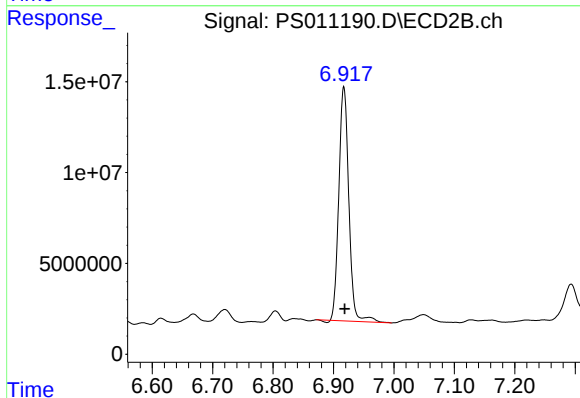


#4 2,4-DCAA

R.T.: 6.917 min
Delta R.T.: -0.001 min
Response: 148048122
Conc: 262.95 ng/ml

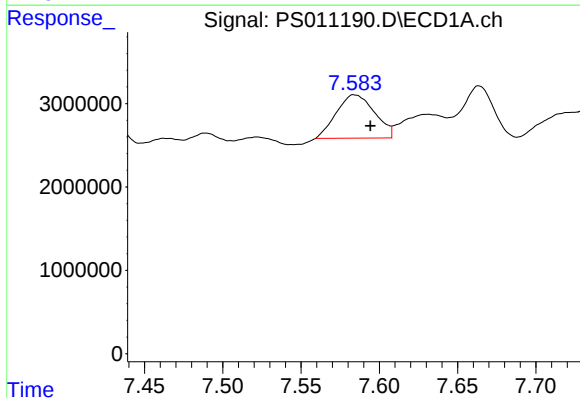


#6 MCP

R.T.: 7.585 min
Delta R.T.: -0.010 min
Response: 8845245
Conc: 2.92 ug/ml

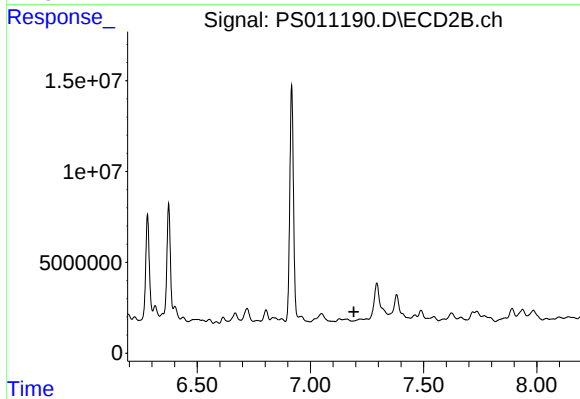

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.192 min
Response: 0
Conc: N.D.

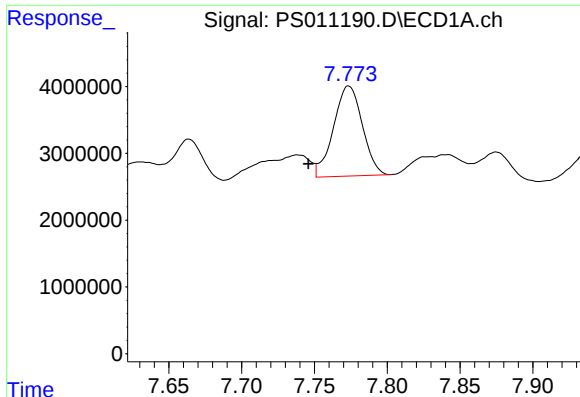

#7 MCPA


R.T.: 7.774 min
Delta R.T.: 0.028 min
Response: 18624736
Conc: 4.37 ug/ml

Instrument :
ECD_S
ClientSampleId :

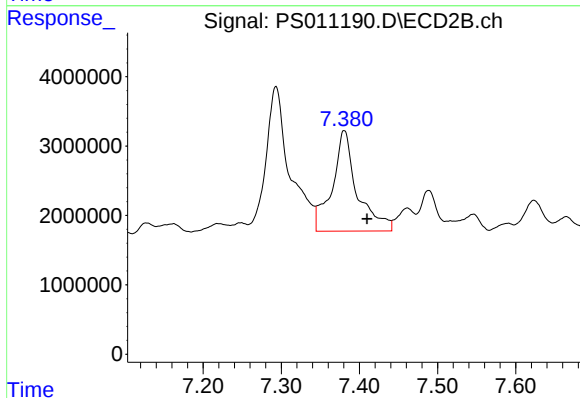


#7 MCPA

R.T.: 7.381 min
Delta R.T.: -0.029 min
Response: 32115256
Conc: 11.14 ug/ml

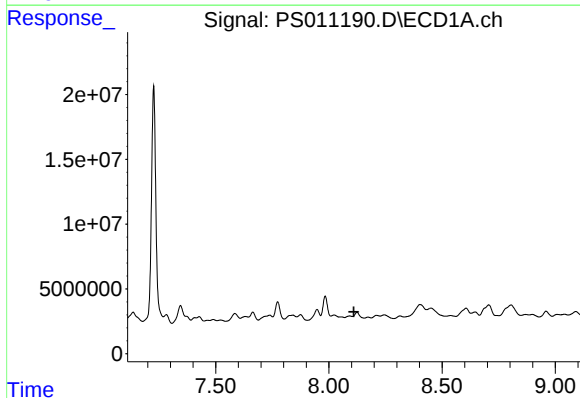


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.110 min
Response: 0
Conc: N.D.

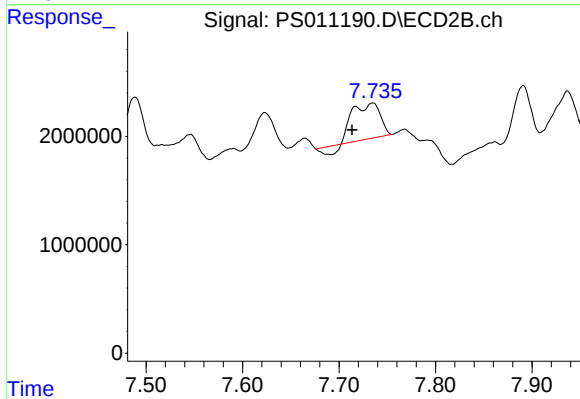

#8 DICHLORPROP


R.T.: 7.735 min
Delta R.T.: 0.021 min
Response: 5948139
Conc: 9.88 ng/ml

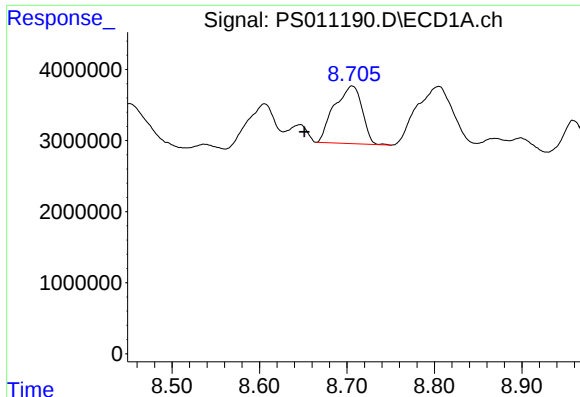

#10 Pentachlorophenol


R.T.: 8.706 min
Delta R.T.: 0.055 min
Response: 17859592
Conc: 1.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

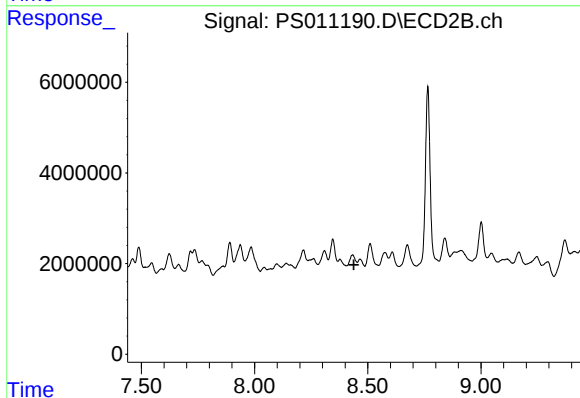


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.438 min
Response: 0
Conc: N.D.

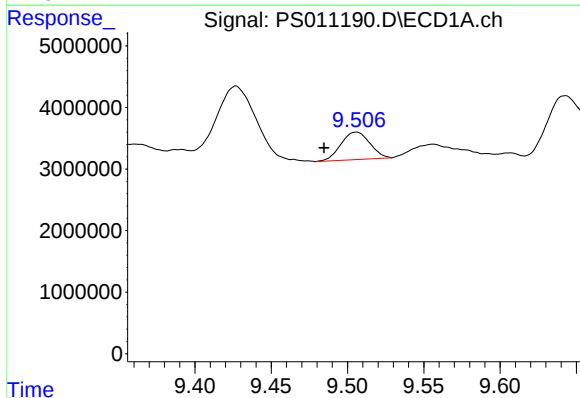


#12 2,4,5-T

R.T.: 9.506 min
Delta R.T.: 0.021 min
Response: 5881011
Conc: 1.17 ng/ml

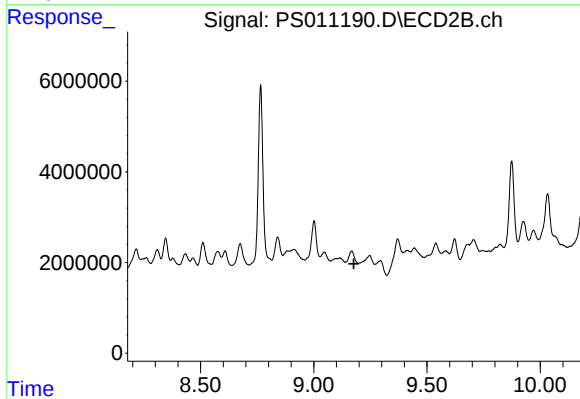

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.177 min
Response: 0
Conc: N.D.

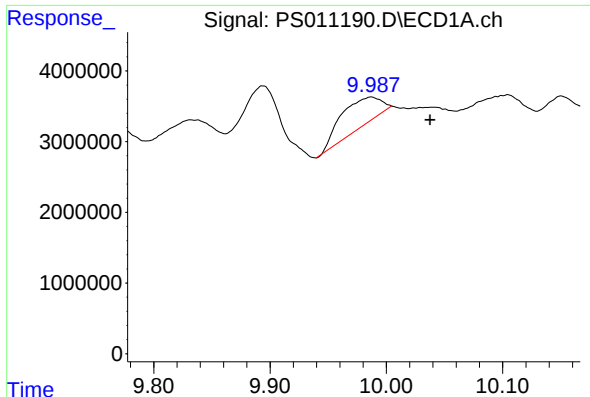

#13 2,4-DB


R.T.: 9.987 min
Delta R.T.: -0.051 min
Response: 9512870
Conc: 14.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

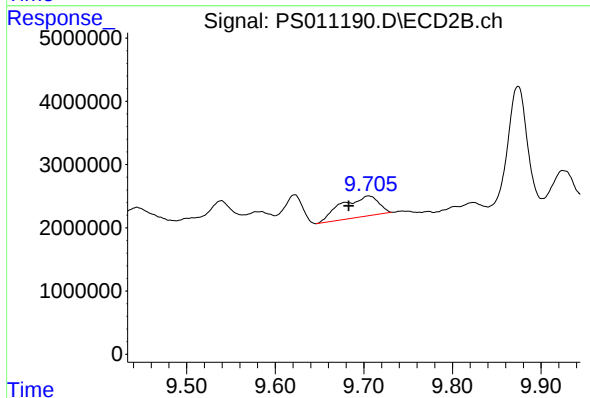


#13 2,4-DB

R.T.: 9.706 min
Delta R.T.: 0.023 min
Response: 9508909
Conc: 22.24 ng/ml

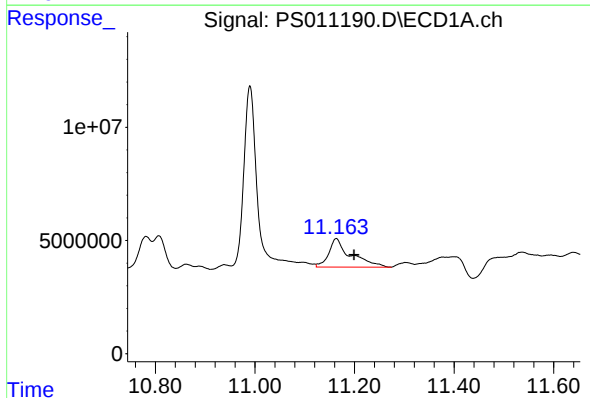


#14 DINOSEB

R.T.: 11.163 min
Delta R.T.: -0.036 min
Response: 38494650
Conc: 9.99 ng/ml

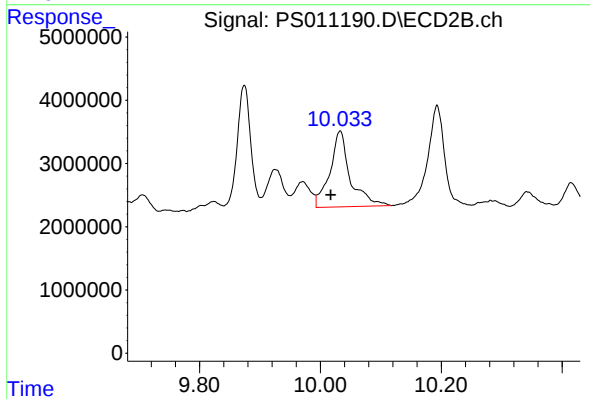

#14 DINOSEB


R.T.: 10.032 min
Delta R.T.: 0.015 min
Response: 28091514
Conc: 13.10 ng/ml

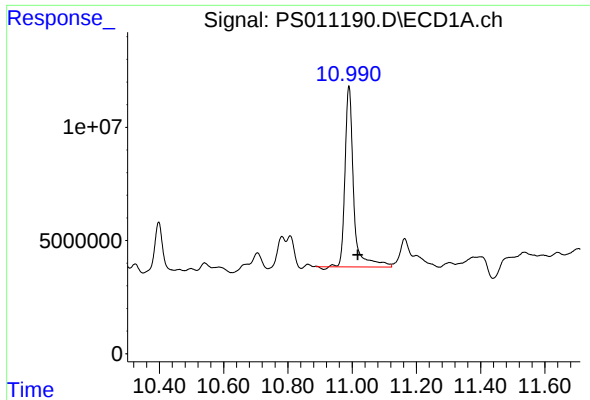

#15 Picloram

R.T.: 10.990 min
Delta R.T.: -0.028 min
Response: 149187915
Conc: 23.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

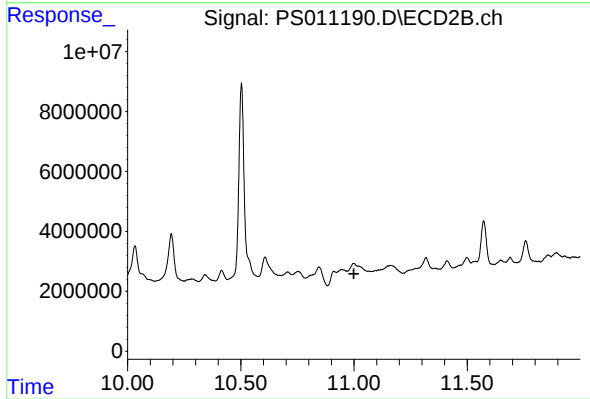

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.999 min
Response: 0
Conc: N.D.