

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071420\
 Data File : PS011211.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2020 10:26
 Operator : DD\AJ
 Sample : PB130039BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 12:16:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	6.918	262.7E6	186.3E6	270.706	330.922
Target Compounds							
1) T	Dalapon	2.993	2.584	52084388	149.2E6	43.282	194.353 #
2) T	3,5-DICHL...	0.000	6.098	0	73768351	N.D.	87.836
3) T	4-Nitroph...	6.995	0.000	8158972	0	18.508	N.D. #
5) T	DICAMBA	7.407	0.000	6640316	0	1.713	N.D. #
6) T	MCPD	7.639	0.000	5903874	0	1.950	N.D. #
7) T	MCPA	7.691	7.458	200.9E6	190.5E6	47.104	66.110 #
8) T	DICHLORPROP	0.000	7.739	0	12830435	N.D.	21.316
9) T	2,4-D	0.000	7.983	0	7454182	N.D.	9.943
10) T	Pentachlo...	8.707	0.000	15469127	0	1.170	N.D. #
12) T	2,4,5-T	9.425	0.000	31562089	0	6.255	N.D. #
15) T	Picloram	11.027	0.000	16679216	0	2.643	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071420\
Data File : PS011211.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2020 10:26
Operator : DD\AJ
Sample : PB130039BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 12:16:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

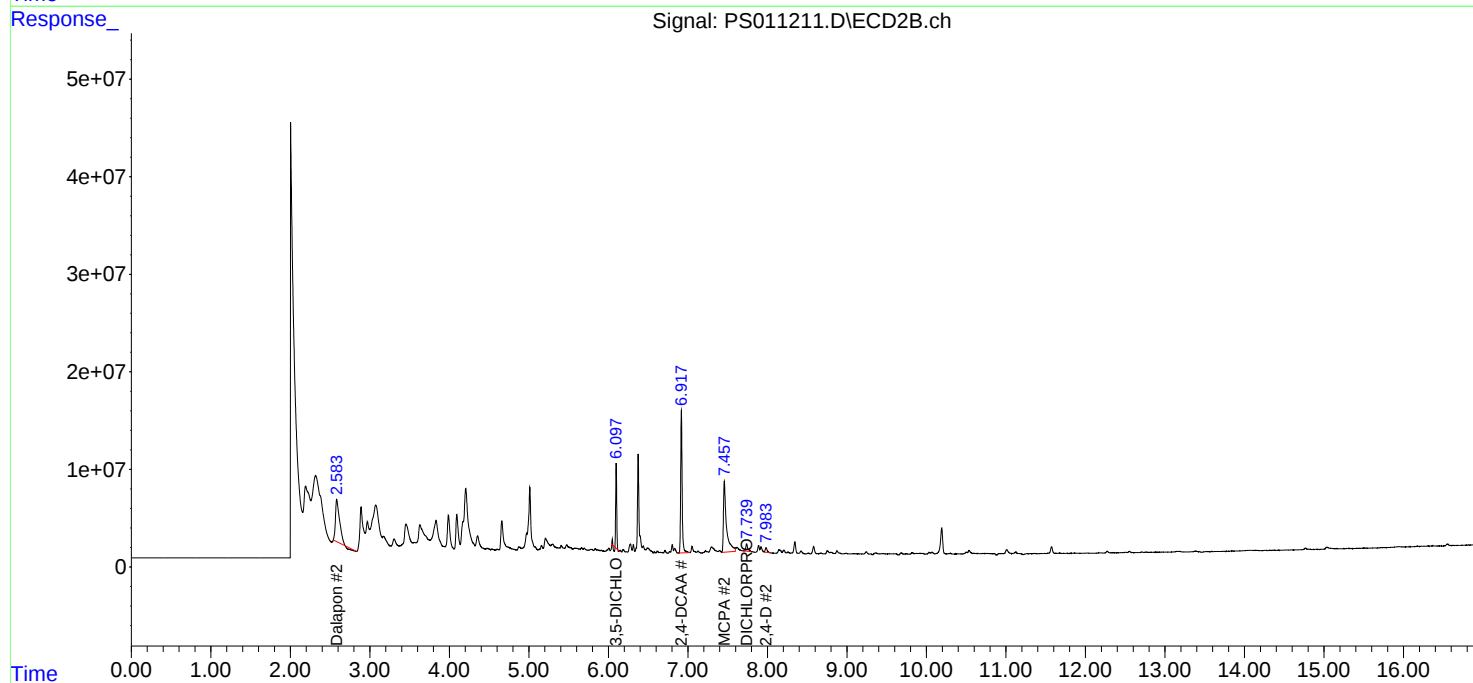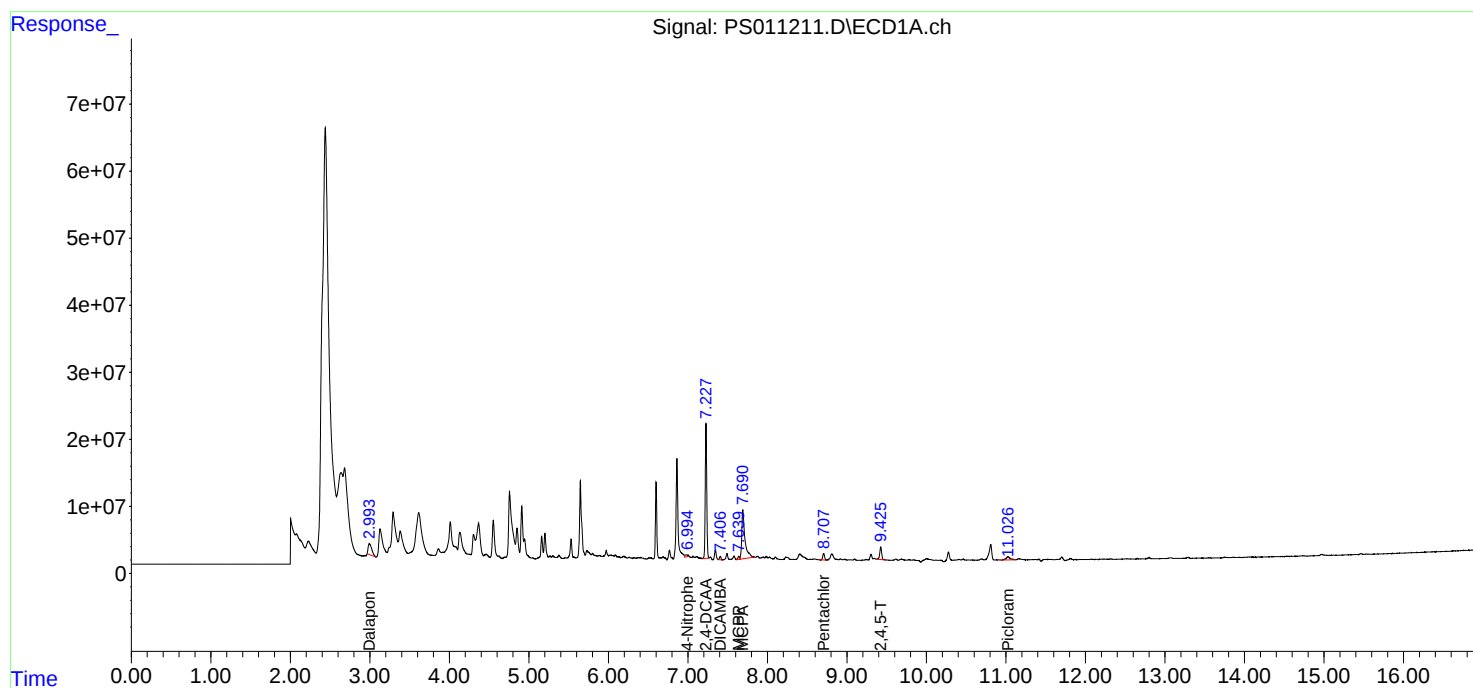


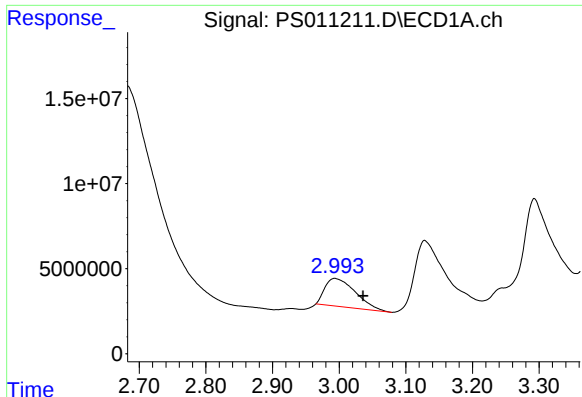

#1 Dalapon


R.T.: 2.993 min
Delta R.T.: -0.043 min
Response: 52084388
Conc: 43.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

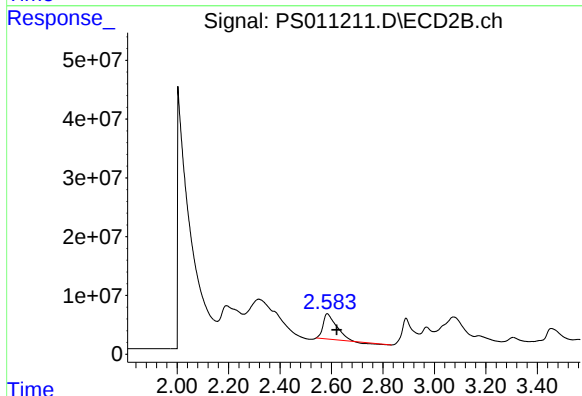


#1 Dalapon

R.T.: 2.584 min
Delta R.T.: -0.037 min
Response: 149199190
Conc: 194.35 ng/ml

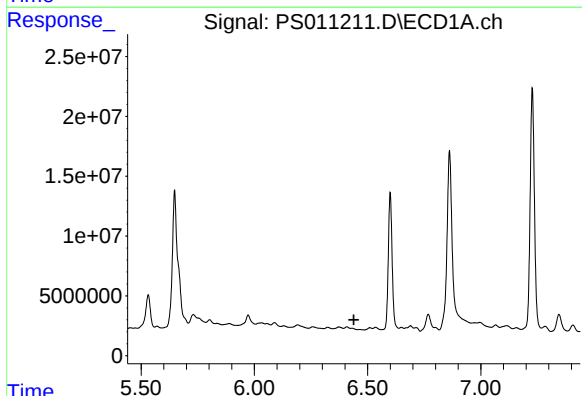


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.439 min
Response: 0
Conc: N.D.

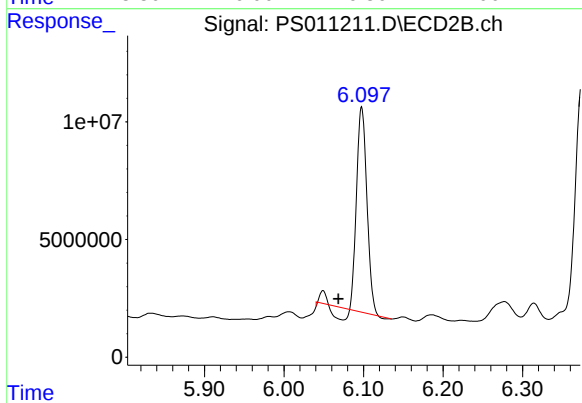

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.098 min
Delta R.T.: 0.029 min
Response: 73768351
Conc: 87.84 ng/ml

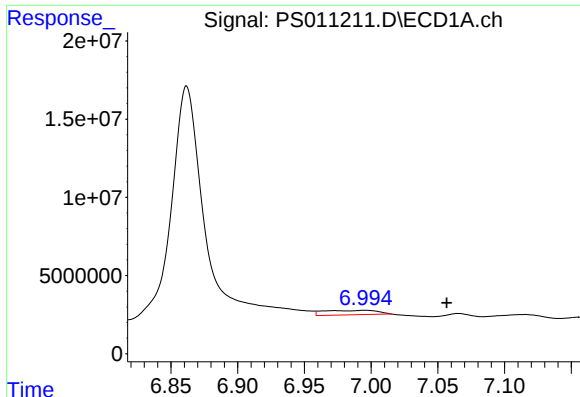

#3 4-Nitrophenol


R.T.: 6.995 min
Delta R.T.: -0.061 min
Response: 8158972
Conc: 18.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

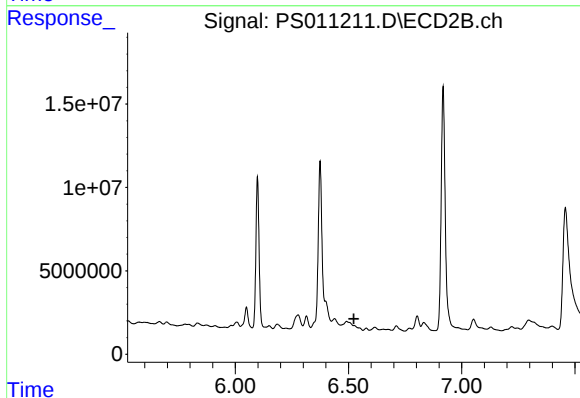


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.524 min
Response: 0
Conc: N.D.

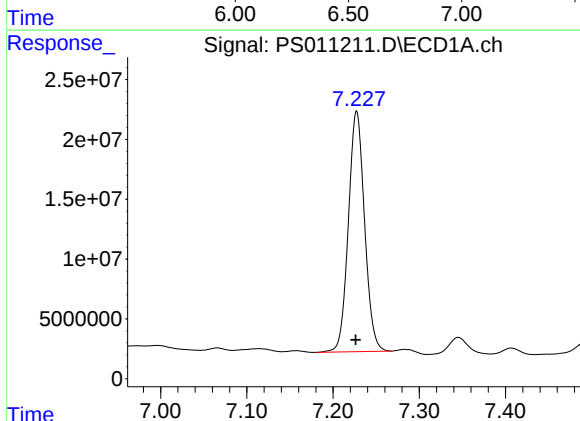


#4 2,4-DCAA

R.T.: 7.227 min
Delta R.T.: 0.000 min
Response: 262676192
Conc: 270.71 ng/ml

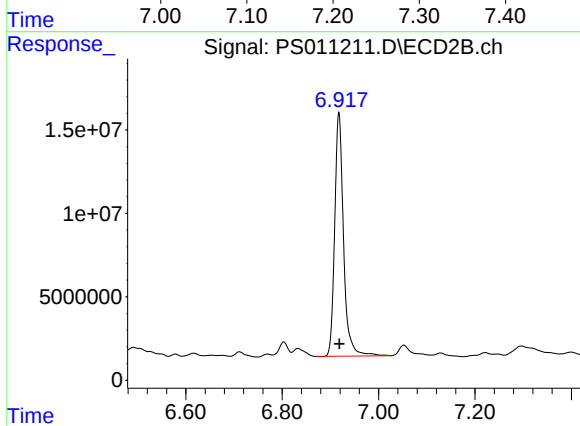

#4 2,4-DCAA


R.T.: 6.918 min
Delta R.T.: 0.000 min
Response: 186316621
Conc: 330.92 ng/ml

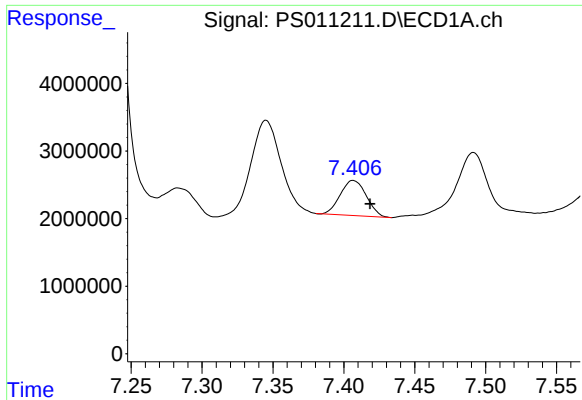

#5 DICAMBA


R.T.: 7.407 min
Delta R.T.: -0.012 min
Response: 6640316
Conc: 1.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

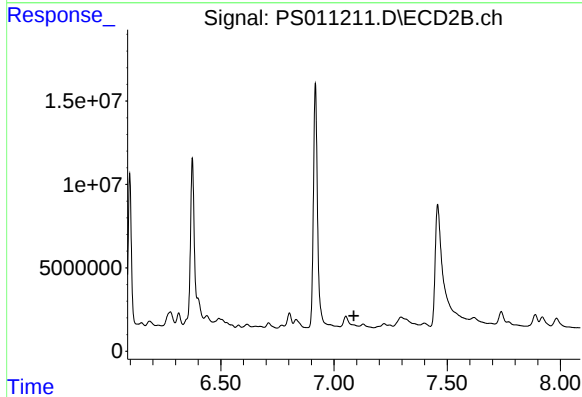


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.088 min
Response: 0
Conc: N.D.

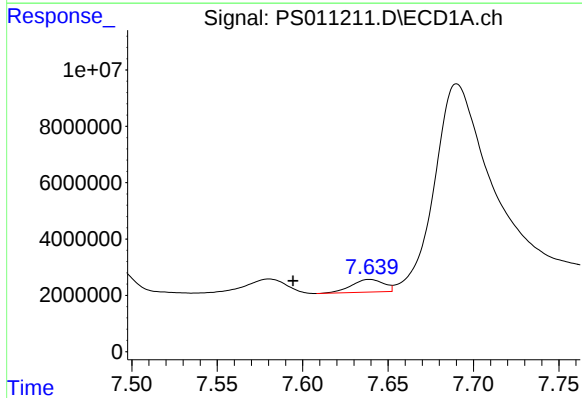


#6 MCP

R.T.: 7.639 min
Delta R.T.: 0.045 min
Response: 5903874
Conc: 1.95 ug/ml

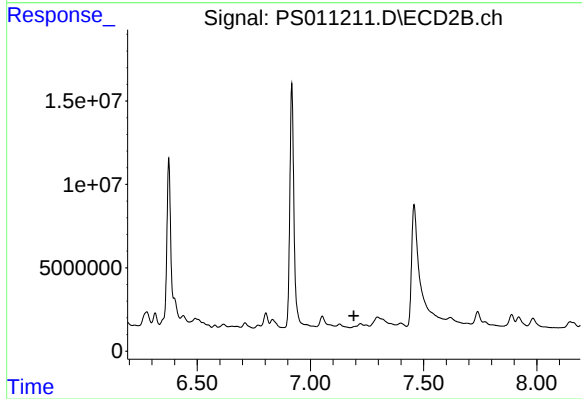

#6 MCP


R.T.: 0.000 min
Exp R.T. : 7.192 min
Response: 0
Conc: N.D.

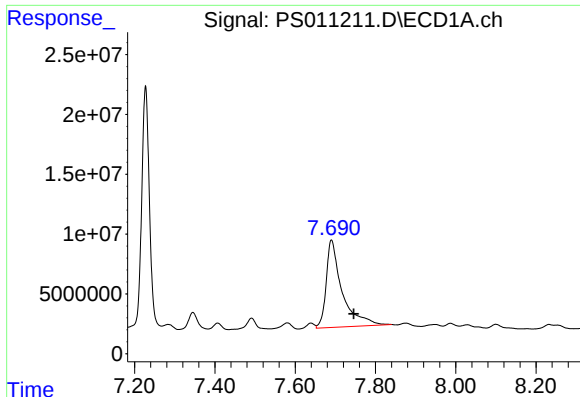

#7 MCPA


R.T.: 7.691 min
Delta R.T.: -0.055 min
Response: 200886450
Conc: 47.10 ug/ml

Instrument :
ECD_S
ClientSampleId :

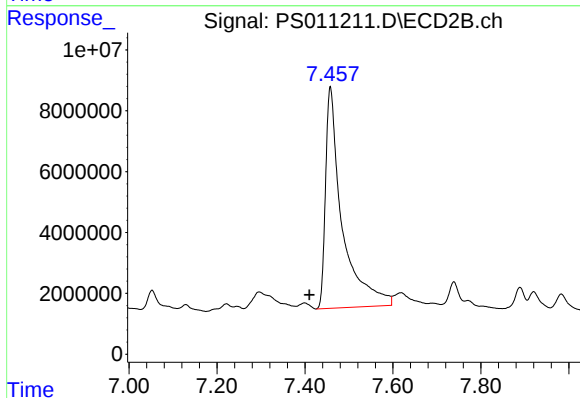


#7 MCPA

R.T.: 7.458 min
Delta R.T.: 0.048 min
Response: 190549392
Conc: 66.11 ug/ml

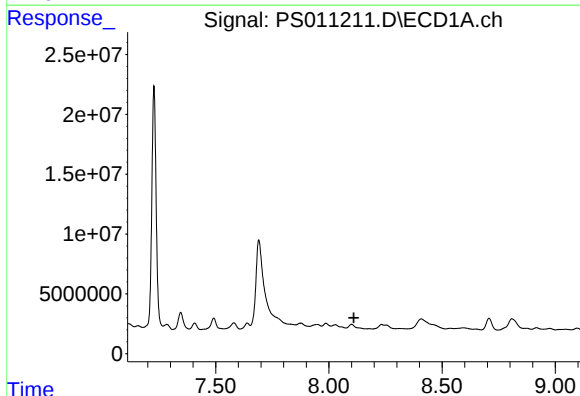


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.110 min
Response: 0
Conc: N.D.

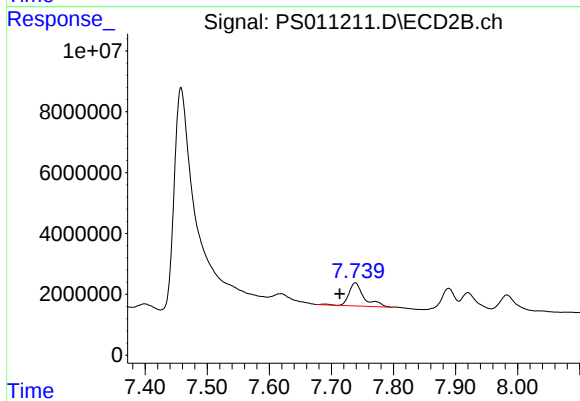

#8 DICHLORPROP


R.T.: 7.739 min
Delta R.T.: 0.025 min
Response: 12830435
Conc: 21.32 ng/ml

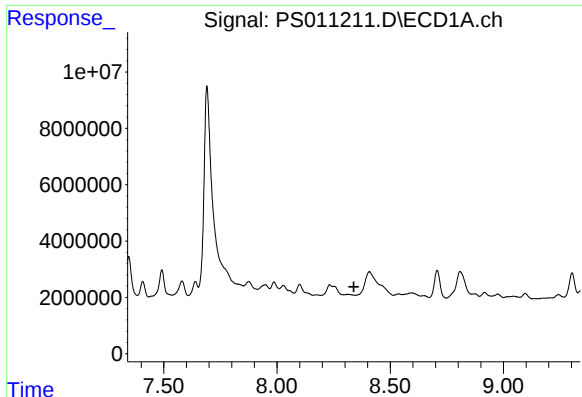

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.339 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

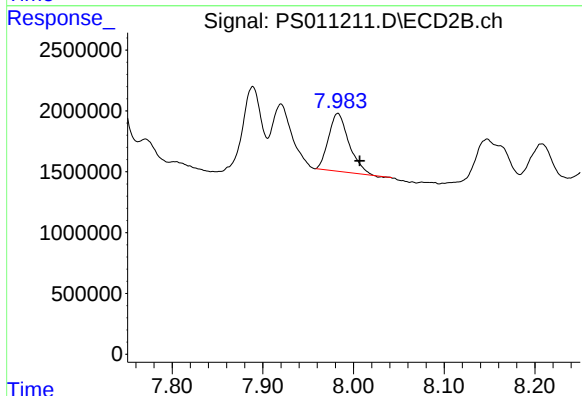


#9 2,4-D

R.T.: 7.983 min
Delta R.T.: -0.024 min
Response: 7454182
Conc: 9.94 ng/ml

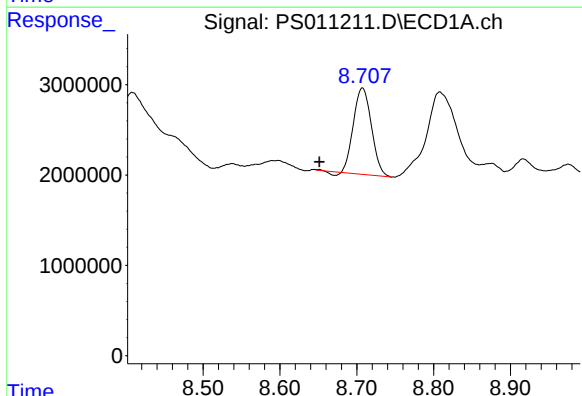


#10 Pentachlorophenol

R.T.: 8.707 min
Delta R.T.: 0.056 min
Response: 15469127
Conc: 1.17 ng/ml

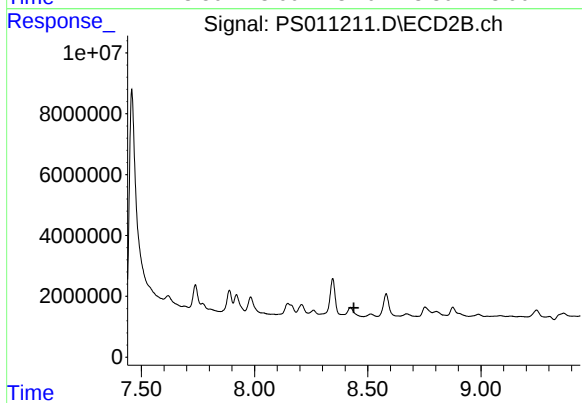

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.438 min
Response: 0
Conc: N.D.

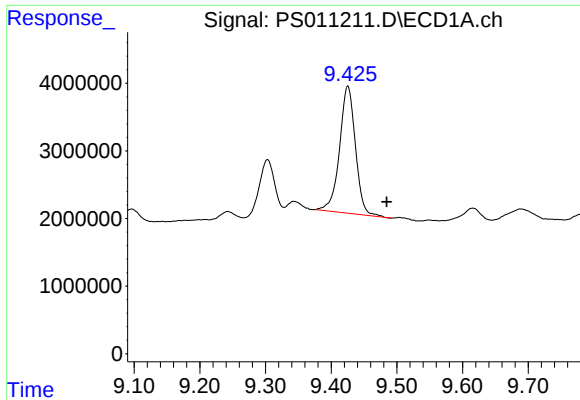

#12 2,4,5-T


R.T.: 9.425 min
Delta R.T.: -0.059 min
Response: 31562089
Conc: 6.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

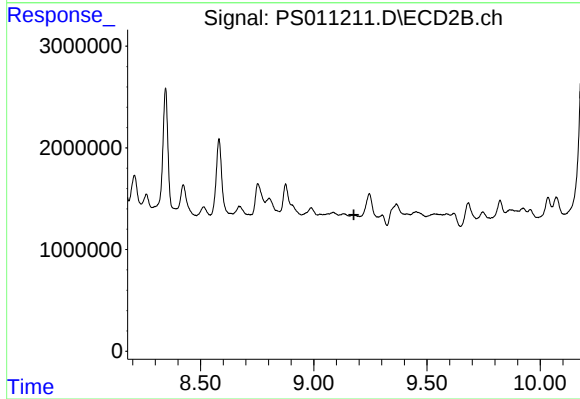


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.177 min
Response: 0
Conc: N.D.

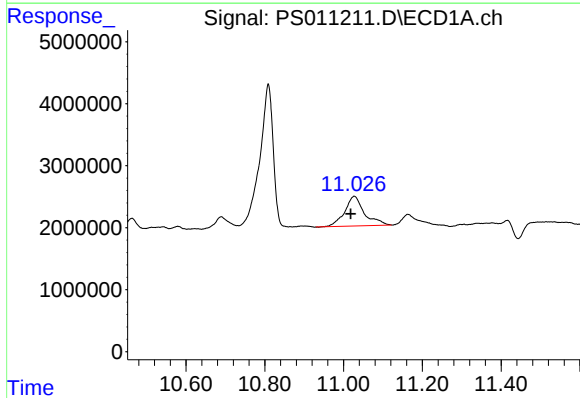

#15 Picloram

R.T.: 11.027 min
Delta R.T.: 0.009 min
Response: 16679216
Conc: 2.64 ng/ml

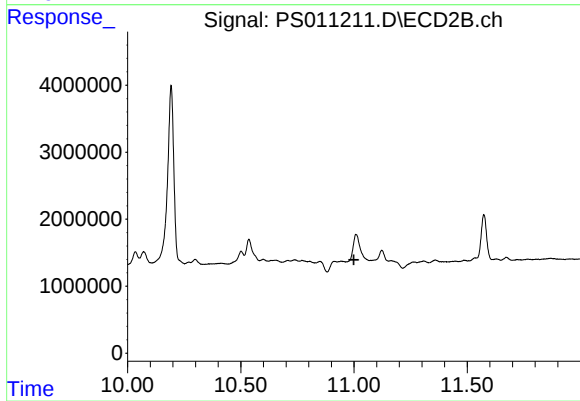

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.999 min
Response: 0
Conc: N.D.