

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071421\
 Data File : PS016095.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2021 15:47
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 06:49:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
 Quant Title : 8080.M
 QLast Update : Wed Jun 30 00:31:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
8) T	DICHLORPROP	8.021f	0.000	8645932	0	6.216	N.D. #
15) T	Picloram	10.993	10.824	57031094	24355371	5.185	5.854
16) T	DCPA	0.000	10.824f	0	24355371	N.D.	5.663



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071421\
Data File : PS016095.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2021 15:47
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 06:49:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
Quant Title : 8080.M
QLast Update : Wed Jun 30 00:31:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

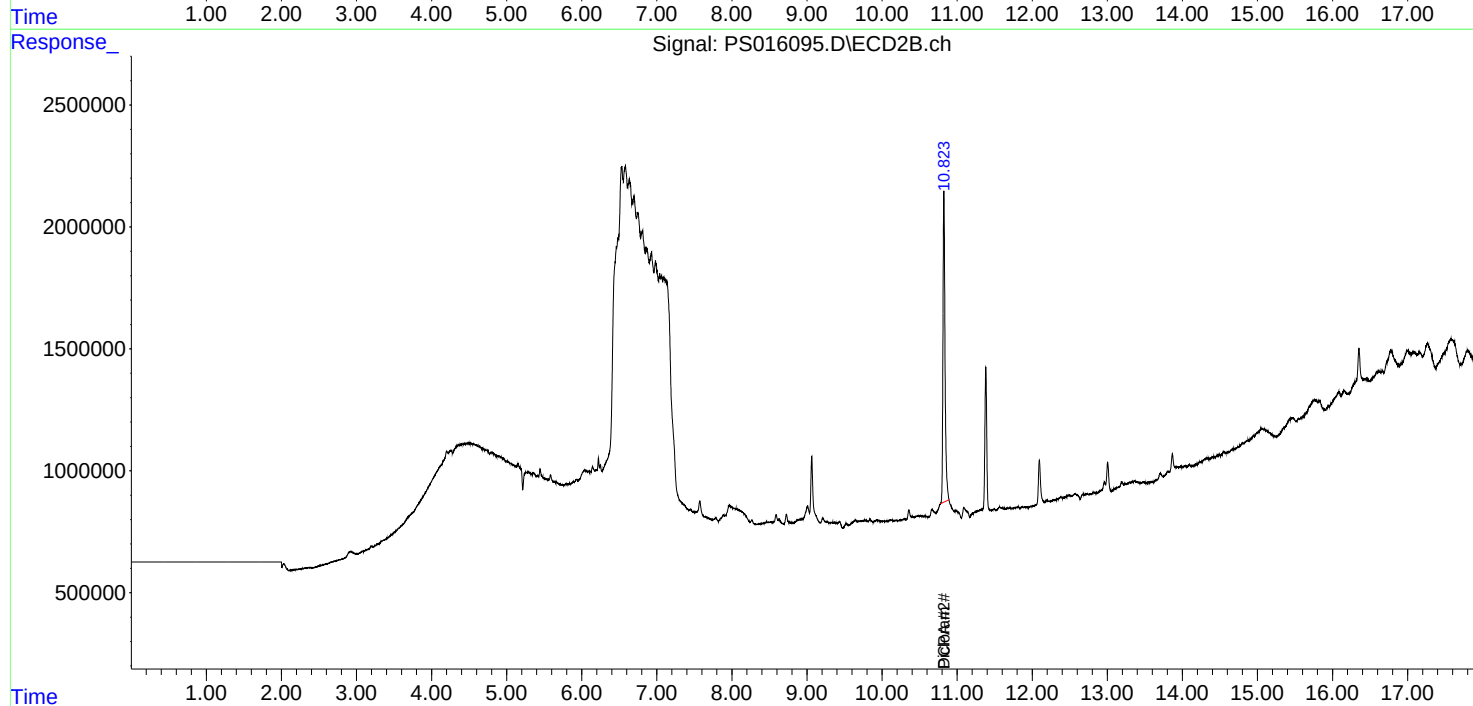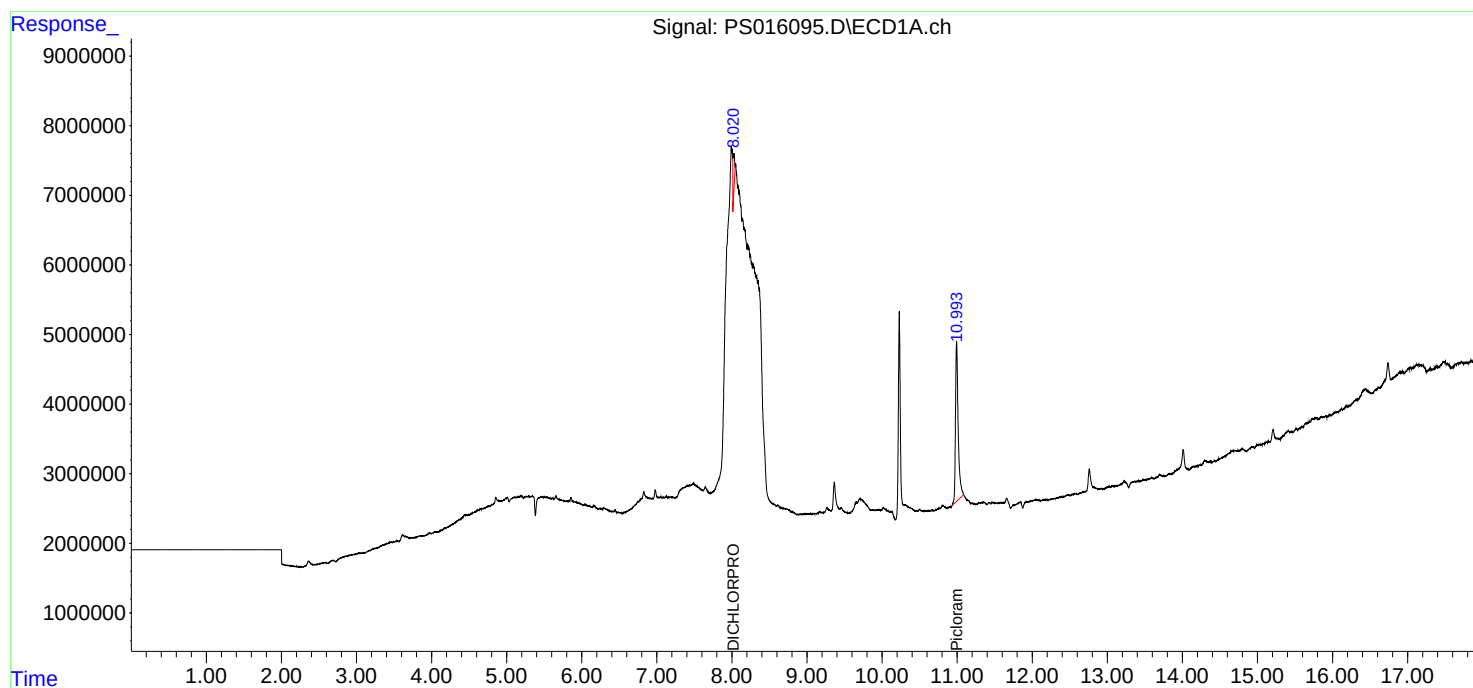


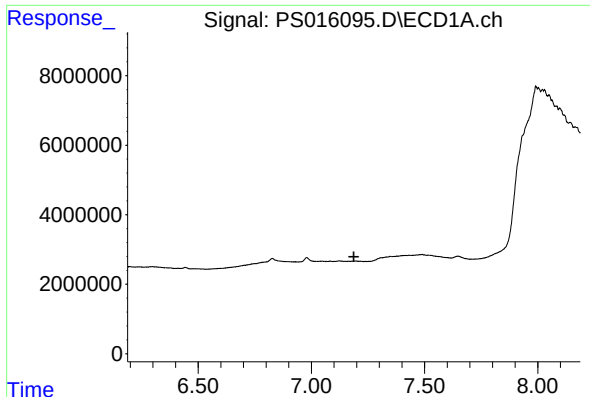

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

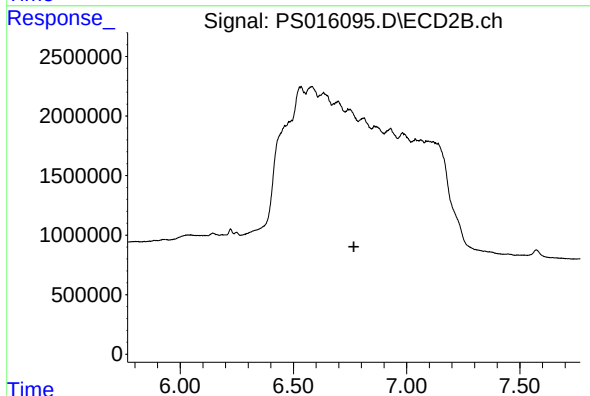


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.767 min
Response: 0
Conc: N.D.

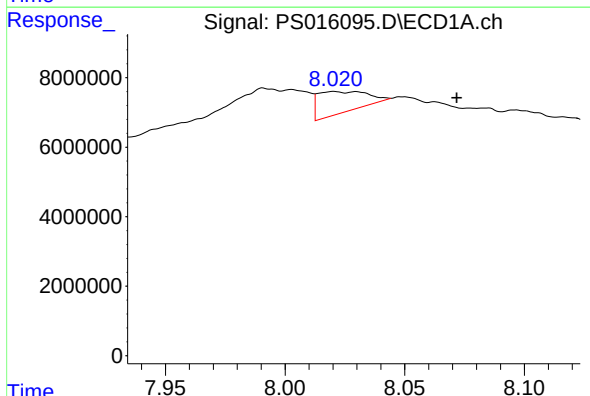


#8 DICHLORPROP

R.T.: 8.021 min
Delta R.T.: -0.051 min
Response: 8645932
Conc: 6.22 ng/ml

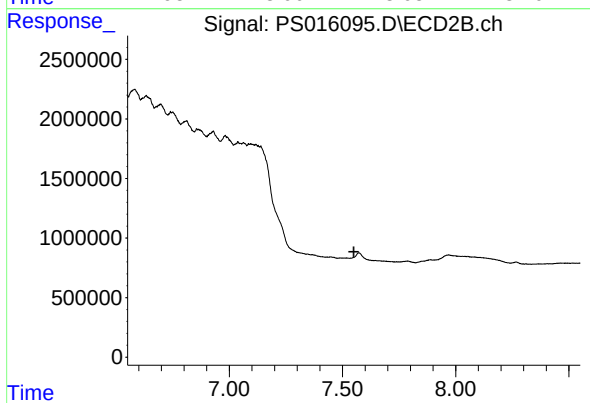

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.550 min
Response: 0
Conc: N.D.

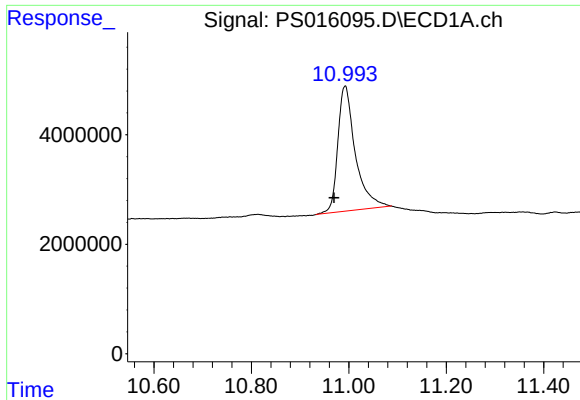

#15 Picloram


R.T.: 10.993 min
Delta R.T.: 0.023 min
Response: 57031094
Conc: 5.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

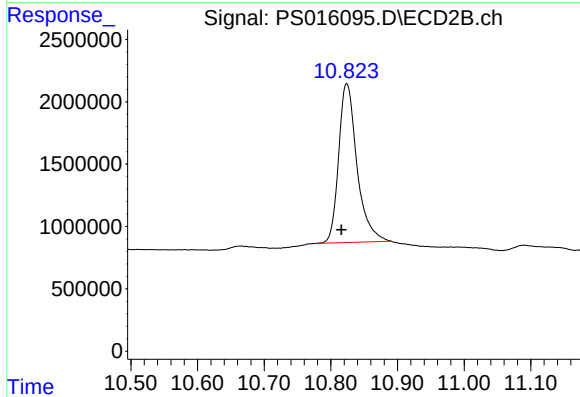


#15 Picloram

R.T.: 10.824 min
Delta R.T.: 0.008 min
Response: 24355371
Conc: 5.85 ng/ml

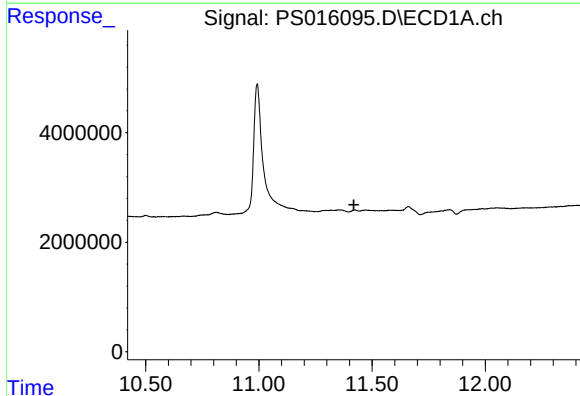

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.420 min
Response: 0
Conc: N.D.

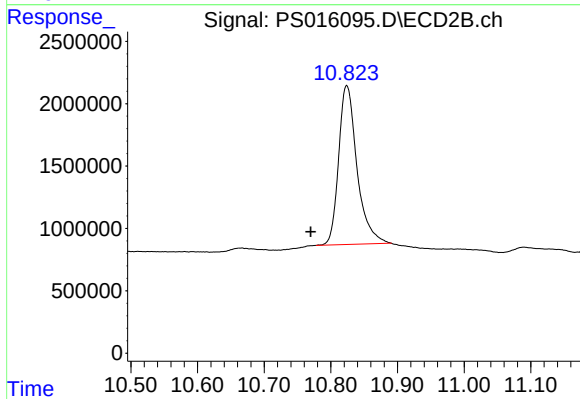

#16 DCPA

R.T.: 10.824 min
Delta R.T.: 0.054 min
Response: 24355371
Conc: 5.66 ng/ml