

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071520\
 Data File : PS011231.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2020 11:56
 Operator : DD\AJ
 Sample : L3287-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 12:46:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.226	6.917	228.8E6	107.5E6	235.808	190.868
Target Compounds							
1) T	Dalapon	2.989	2.582	44995167	45654879	37.391	59.472 #
2) T	3,5-DICHL...	0.000	6.098	0	64622160	N.D.	76.945
6) T	MCPD	7.586	0.000	11380041	0	3.758	N.D. #
7) T	MCPA	7.774	7.381	24164387	47594826	5.666	16.513 #
8) T	DICHLORPROP	8.174	7.735	7717350	19706228	8.232	32.738 #
9) T	2,4-D	0.000	7.984	0	14128371	N.D.	18.846
10) T	Pentachlo...	8.649	8.436	14569715	30870029	1.102	4.429 #
12) T	2,4,5-T	9.427	9.168	27413451	19040687	5.433	6.278
13) T	2,4-DB	9.987	9.702	11626927	39969797	18.039	93.497 #
14) T	DINOSEB	11.162	10.032	86922896	41054254	22.550	19.140
15) T	Picloram	10.988	0.000	296.4E6	0	46.972	N.D. #
16) T	DCPA	11.482	0.000	15791118	0	2.451	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071520\
Data File : PS011231.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2020 11:56
Operator : DD\AJ
Sample : L3287-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 12:46:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

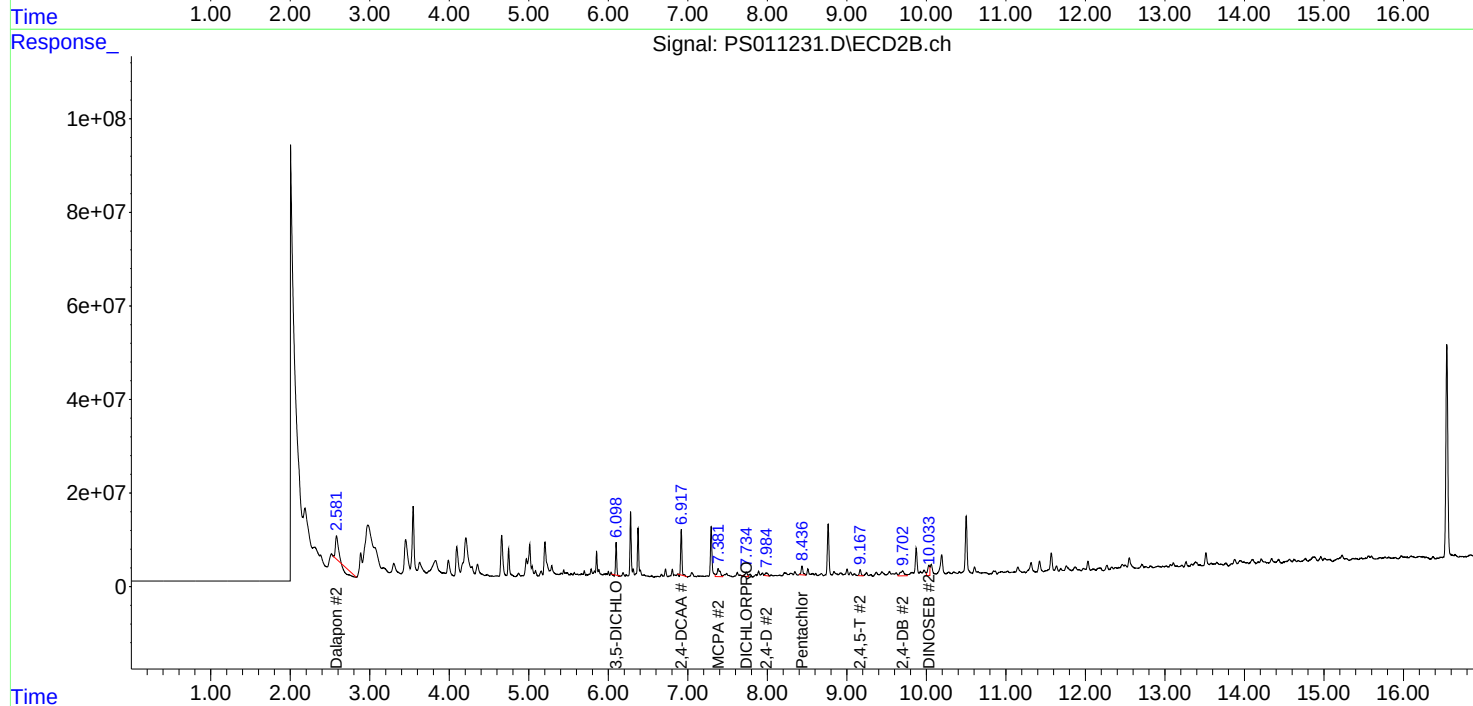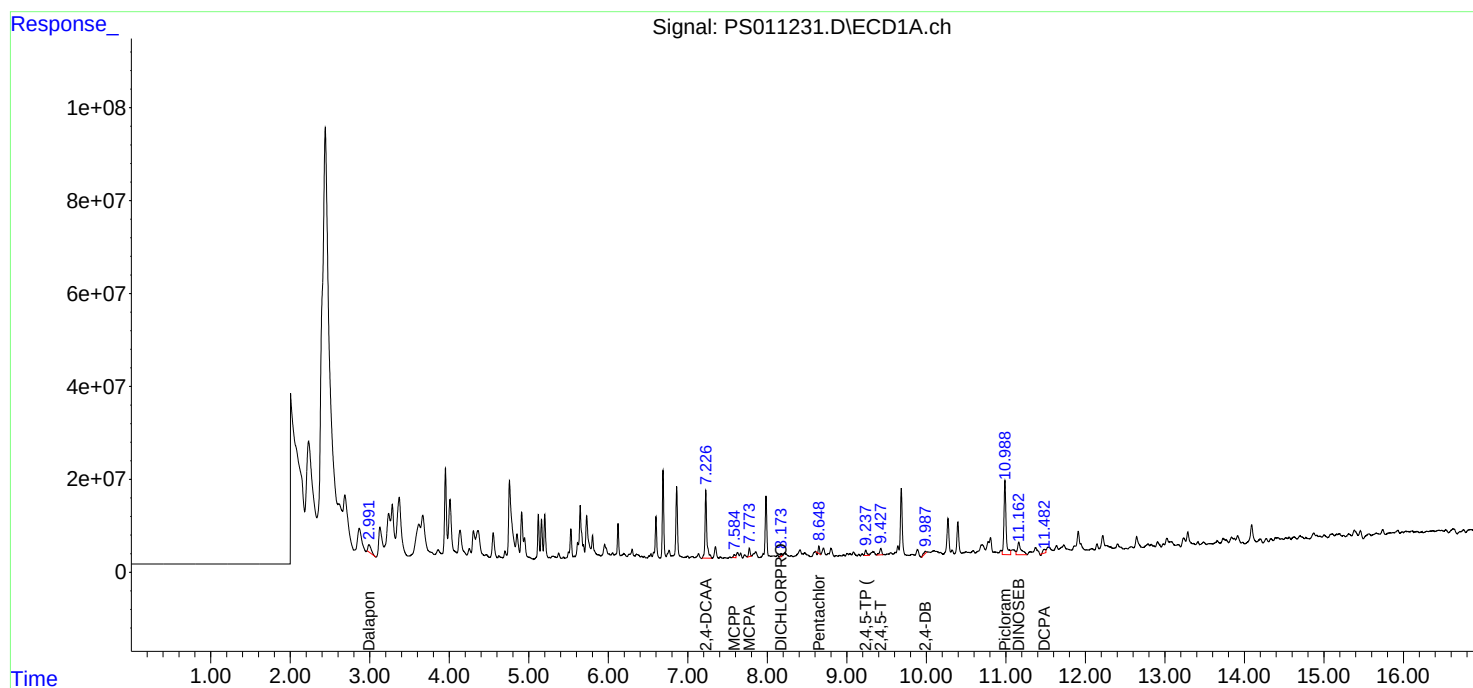


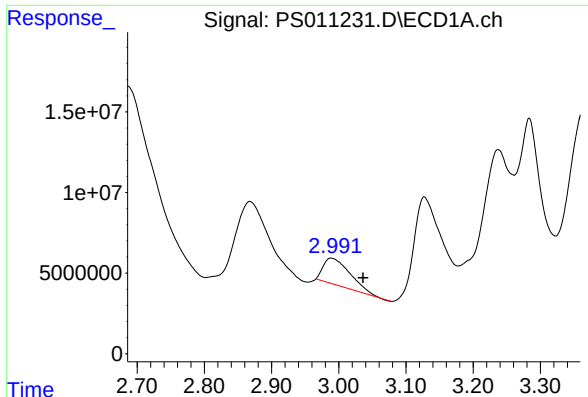

#1 Dalapon


R.T.: 2.989 min
Delta R.T.: -0.047 min
Response: 44995167
Conc: 37.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

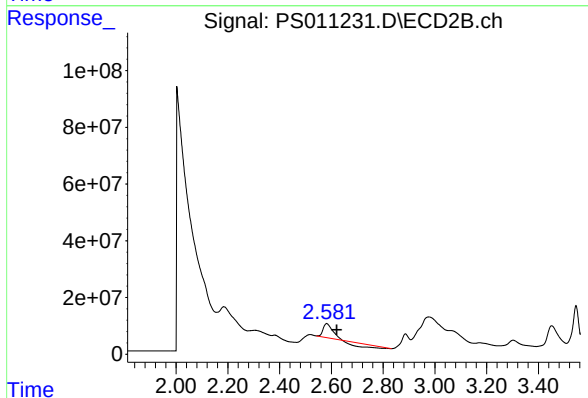


#1 Dalapon

R.T.: 2.582 min
Delta R.T.: -0.038 min
Response: 45654879
Conc: 59.47 ng/ml

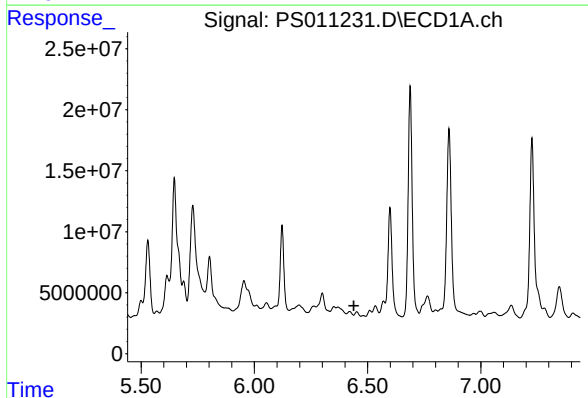


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.439 min
Response: 0
Conc: N.D.

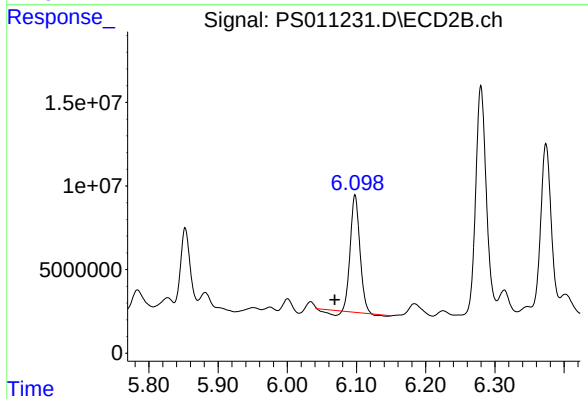

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.098 min
Delta R.T.: 0.029 min
Response: 64622160
Conc: 76.95 ng/ml

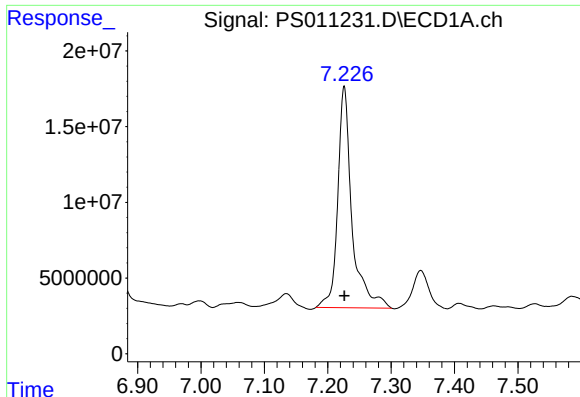

#4 2,4-DCAA


R.T.: 7.226 min
Delta R.T.: 0.000 min
Response: 228813798
Conc: 235.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

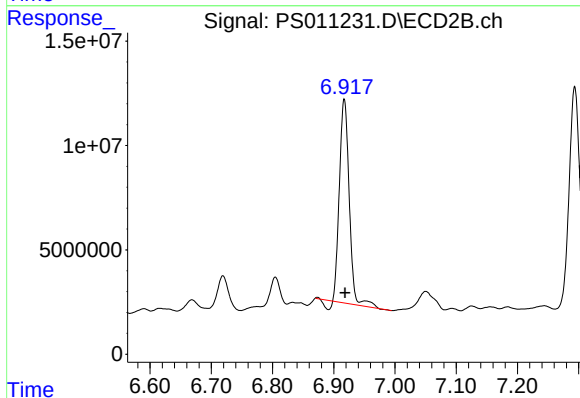


#4 2,4-DCAA

R.T.: 6.917 min
Delta R.T.: -0.001 min
Response: 107463076
Conc: 190.87 ng/ml

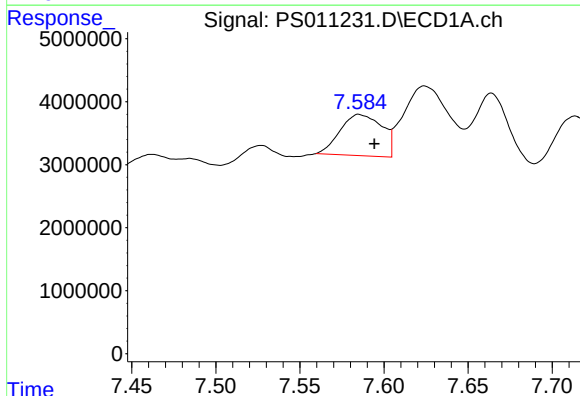


#6 MCP

R.T.: 7.586 min
Delta R.T.: -0.009 min
Response: 11380041
Conc: 3.76 ug/ml

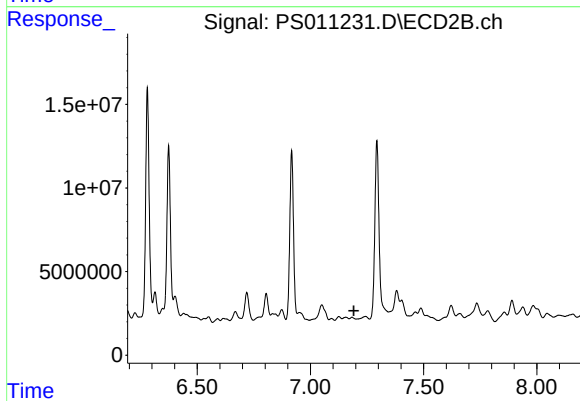

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.192 min
Response: 0
Conc: N.D.

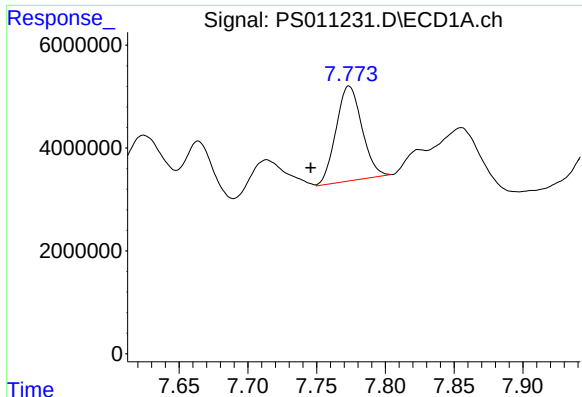

#7 MCPA


R.T.: 7.774 min
Delta R.T.: 0.028 min
Response: 24164387
Conc: 5.67 ug/ml

Instrument :
ECD_S
ClientSampleId :

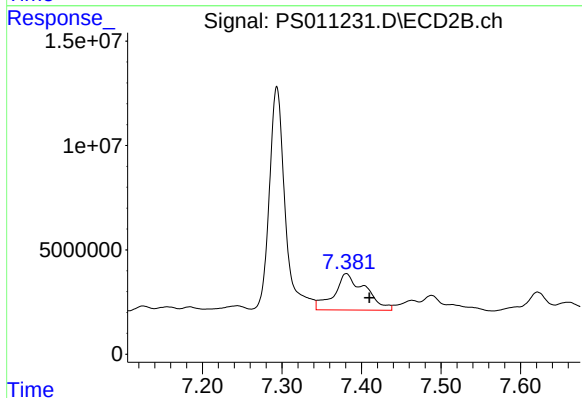


#7 MCPA

R.T.: 7.381 min
Delta R.T.: -0.029 min
Response: 47594826
Conc: 16.51 ug/ml

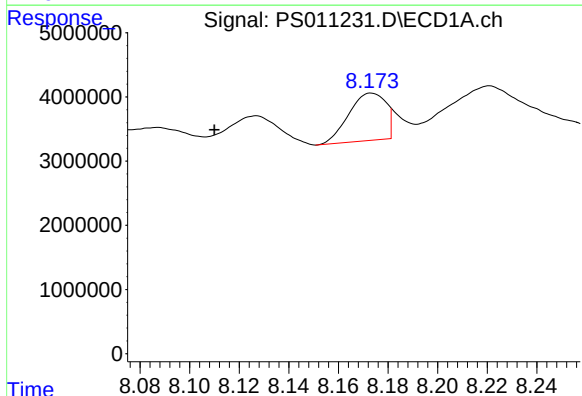


#8 DICHLORPROP

R.T.: 8.174 min
Delta R.T.: 0.063 min
Response: 7717350
Conc: 8.23 ng/ml

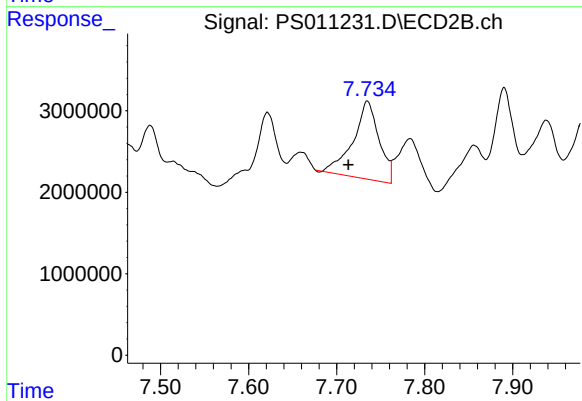

#8 DICHLORPROP


R.T.: 7.735 min
Delta R.T.: 0.022 min
Response: 19706228
Conc: 32.74 ng/ml

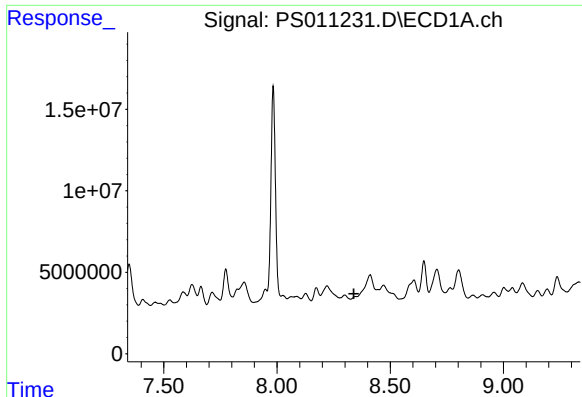

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.339 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

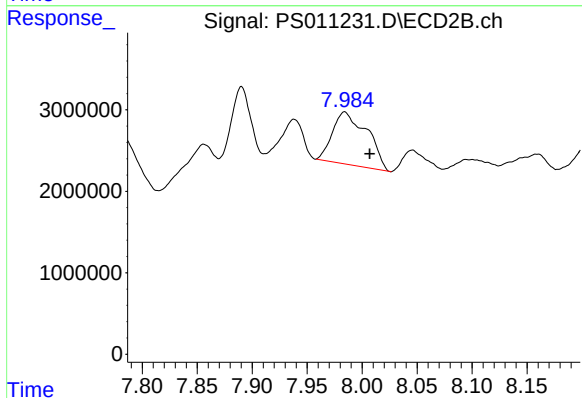


#9 2,4-D

R.T.: 7.984 min
Delta R.T.: -0.023 min
Response: 14128371
Conc: 18.85 ng/ml

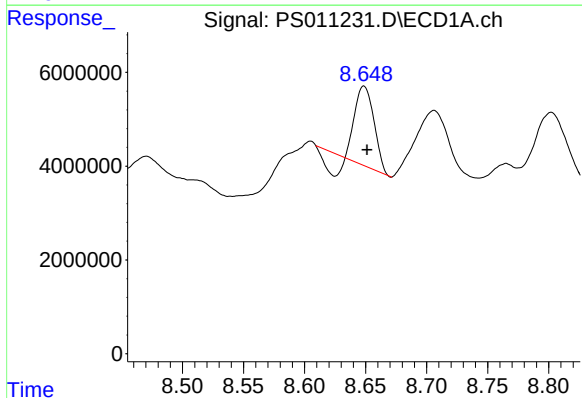


#10 Pentachlorophenol

R.T.: 8.649 min
Delta R.T.: -0.003 min
Response: 14569715
Conc: 1.10 ng/ml

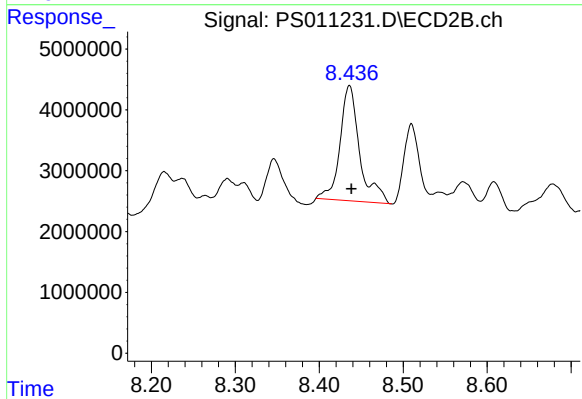

#10 Pentachlorophenol


R.T.: 8.436 min
Delta R.T.: -0.003 min
Response: 30870029
Conc: 4.43 ng/ml

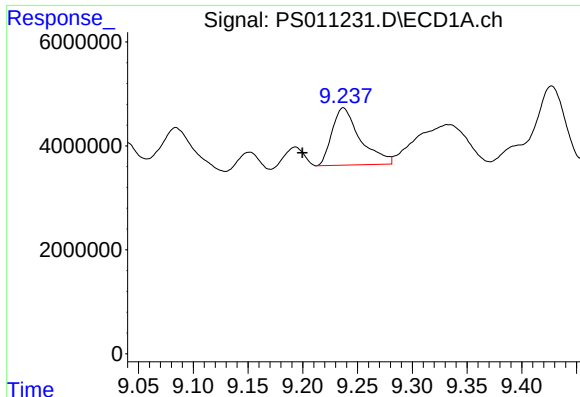

#11 2,4,5-TP (SILVEX)


R.T.: 9.237 min
Delta R.T.: 0.037 min
Response: 19802841
Conc: 3.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

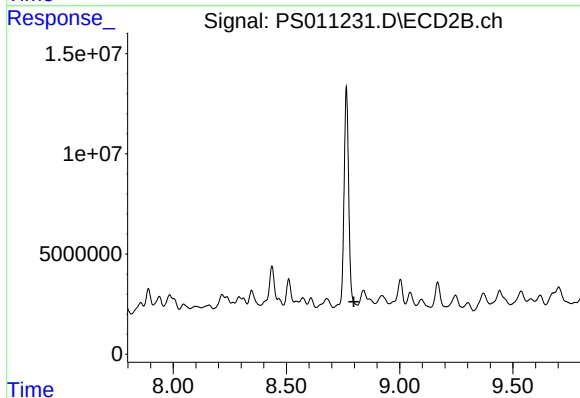


#11 2,4,5-TP (SILVEX)

R.T.: 8.840 min
Delta R.T.: 0.042 min
Response: -36883613
Conc: N.D.

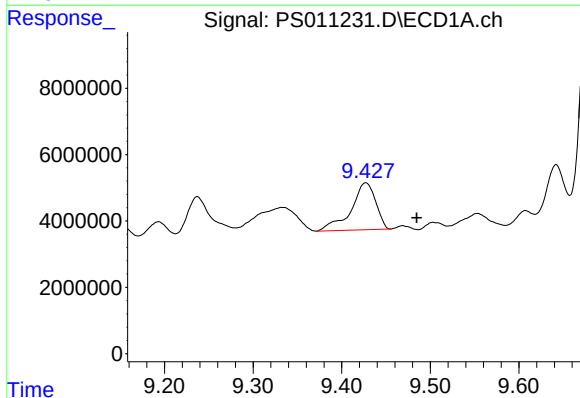


#12 2,4,5-T

R.T.: 9.427 min
Delta R.T.: -0.057 min
Response: 27413451
Conc: 5.43 ng/ml

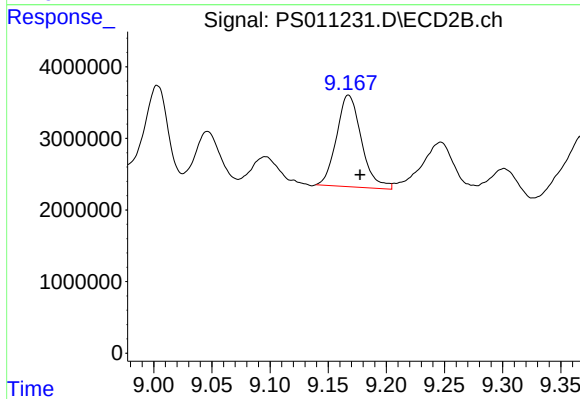

#12 2,4,5-T


R.T.: 9.168 min
Delta R.T.: -0.010 min
Response: 19040687
Conc: 6.28 ng/ml

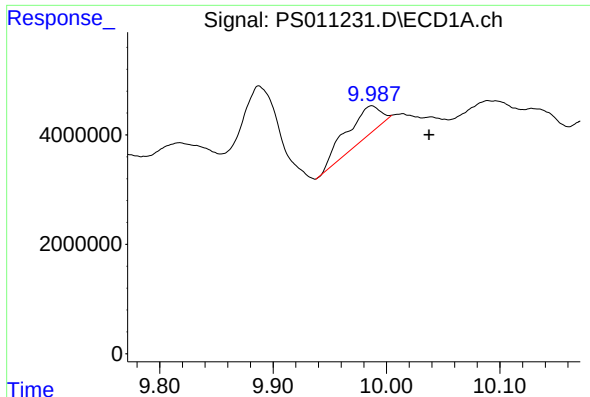

#13 2,4-DB


R.T.: 9.987 min
Delta R.T.: -0.051 min
Response: 11626927
Conc: 18.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

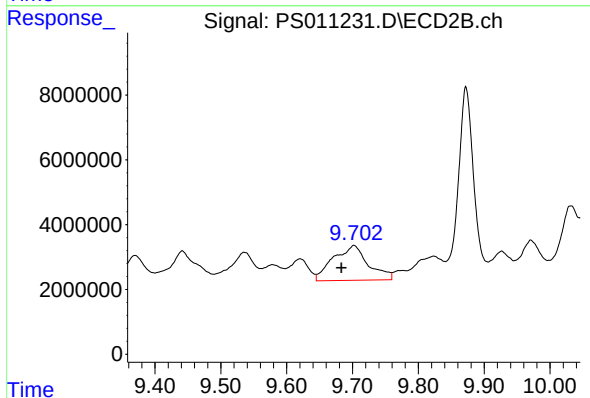


#13 2,4-DB

R.T.: 9.702 min
Delta R.T.: 0.019 min
Response: 39969797
Conc: 93.50 ng/ml

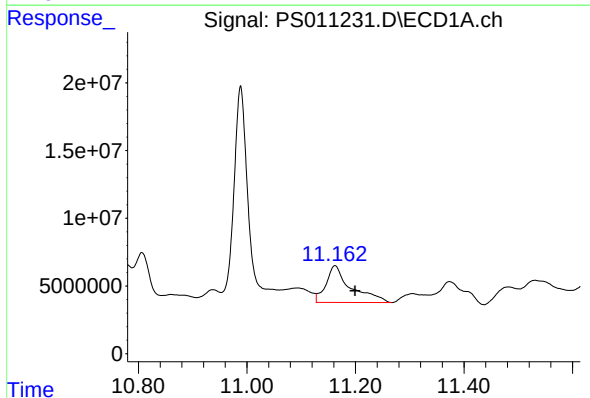


#14 DINOSEB

R.T.: 11.162 min
Delta R.T.: -0.037 min
Response: 86922896
Conc: 22.55 ng/ml

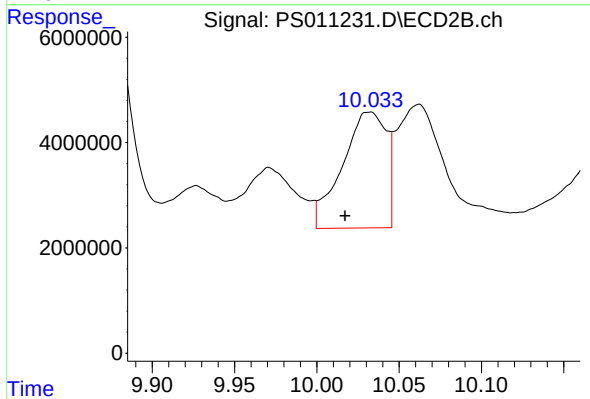

#14 DINOSEB


R.T.: 10.032 min
Delta R.T.: 0.015 min
Response: 41054254
Conc: 19.14 ng/ml

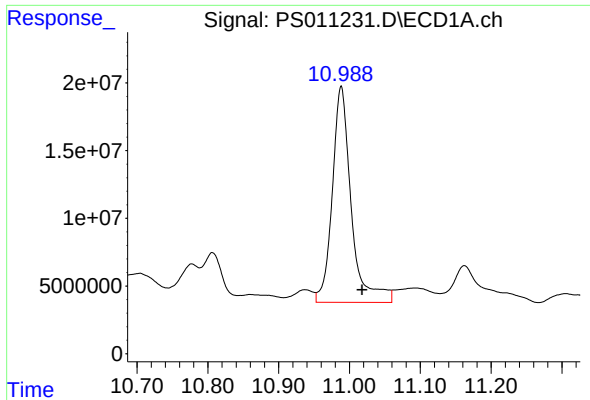

#15 Picloram


R.T.: 10.988 min
Delta R.T.: -0.030 min
Response: 296385710
Conc: 46.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

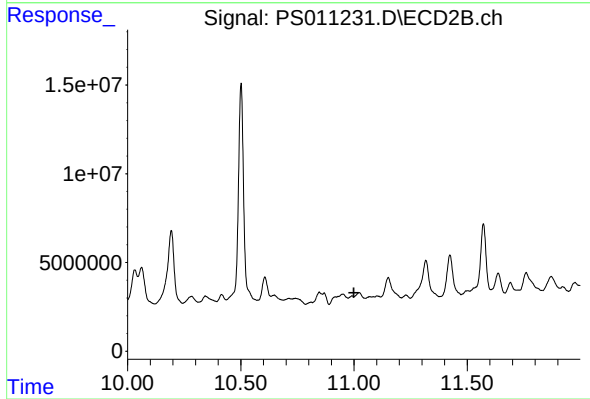


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.999 min
Response: 0
Conc: N.D.

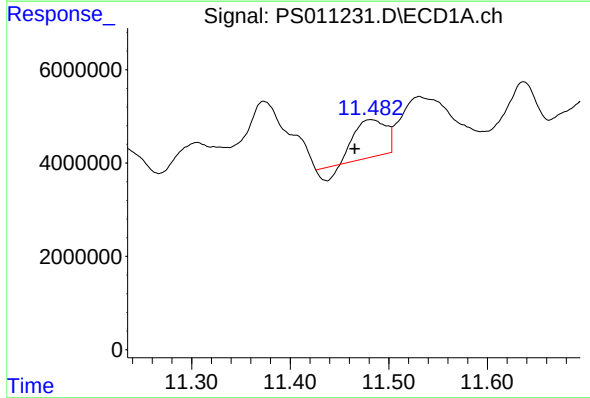

#16 DCPA

R.T.: 11.482 min
Delta R.T.: 0.016 min
Response: 15791118
Conc: 2.45 ng/ml

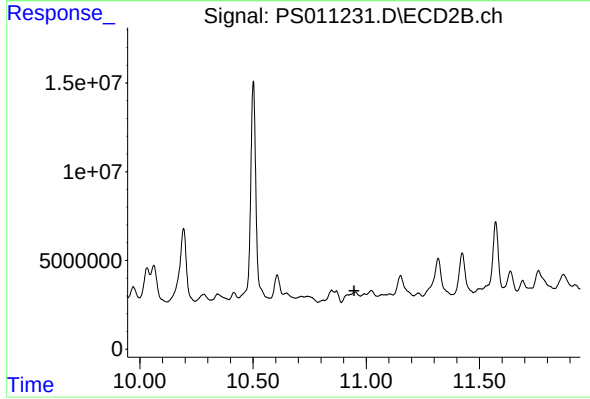

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.946 min
Response: 0
Conc: N.D.