

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071521\
 Data File : PS016114.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2021 12:09
 Operator : DD\AJ
 Sample : M3026-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 01:10:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
 Quant Title : 8080.M
 QLast Update : Wed Jun 30 00:31:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.187	6.766	339.3E6	120.8E6	221.026	235.429
Target Compounds							
1) T	Dalapon	2.980	2.483	49756591	67839562	22.941	97.063 #
2) T	3,5-DICHL...	0.000	5.982	0	56664455	N.D.	73.615
3) T	4-Nitroph...	6.954f	6.417	4461041	9824643	5.045	31.128 #
5) T	DICAMBA	7.363	6.890f	9029546	3917703	1.576	1.860
6) T	MCPD	7.541	0.000	10450202	0	2.384	N.D. #
7) T	MCPA	7.655f	7.297f	421.6E6	101.9E6	66.298	38.662 #
8) T	DICHLORPROP	8.018f	7.568	35633095	23610943	25.617	44.838 #
10) T	Pentachlo...	8.670f	0.000	25621275	0	1.293	N.D. #
12) T	2,4,5-T	9.381f	0.000	73427736	0	9.403	N.D. #
15) T	Picloram	10.965	0.000	10965934	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071521\
Data File : PS016114.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2021 12:09
Operator : DD\AJ
Sample : M3026-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 01:10:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
Quant Title : 8080.M
QLast Update : Wed Jun 30 00:31:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

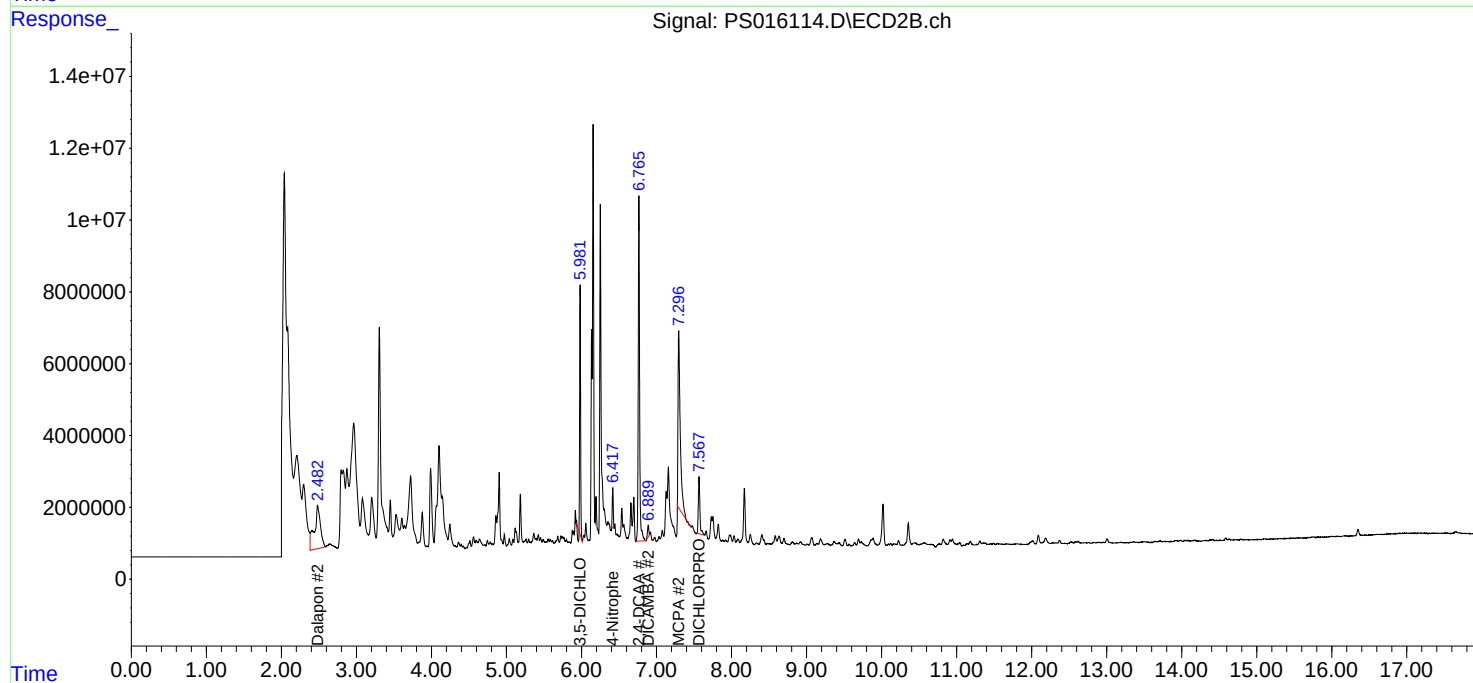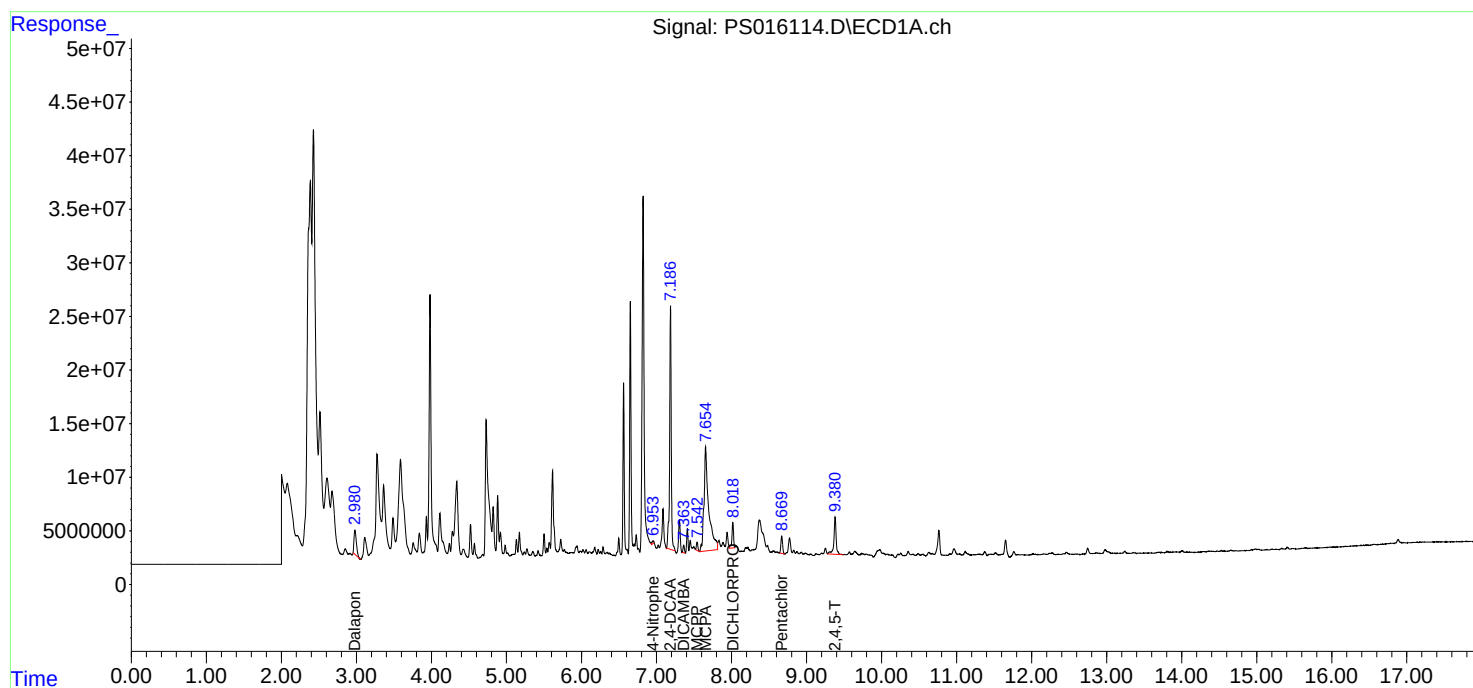


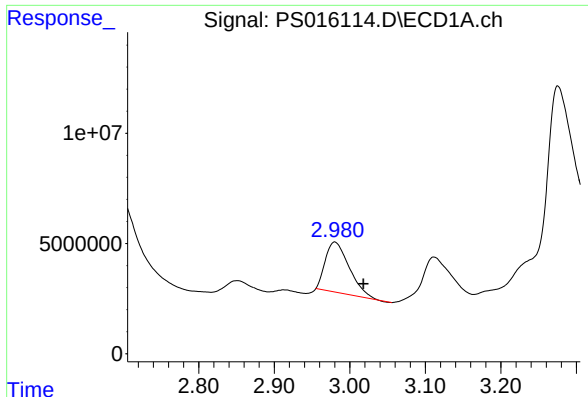

#1 Dalapon


R.T.: 2.980 min
Delta R.T.: -0.038 min
Response: 49756591
Conc: 22.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

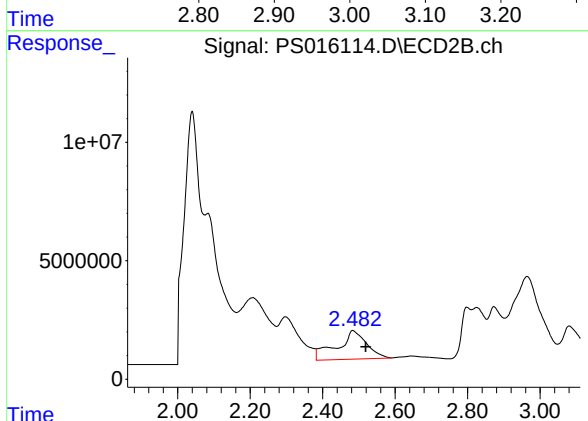


#1 Dalapon

R.T.: 2.483 min
Delta R.T.: -0.036 min
Response: 67839562
Conc: 97.06 ng/ml

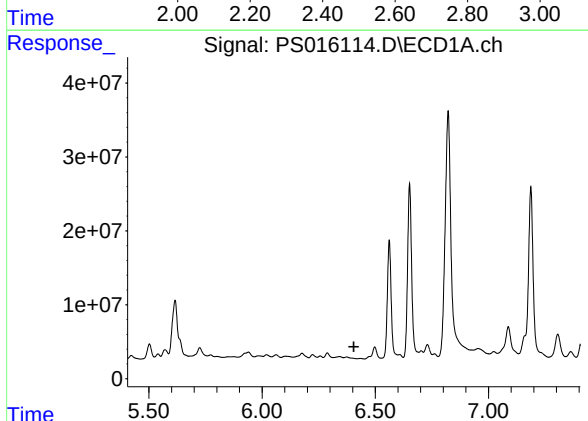


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.406 min
Response: 0
Conc: N.D.

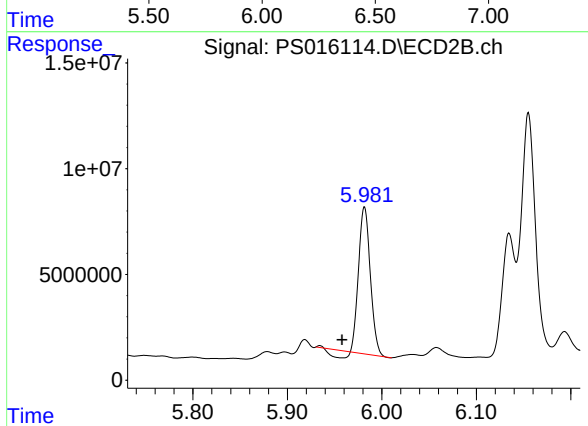

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.982 min
Delta R.T.: 0.024 min
Response: 56664455
Conc: 73.61 ng/ml

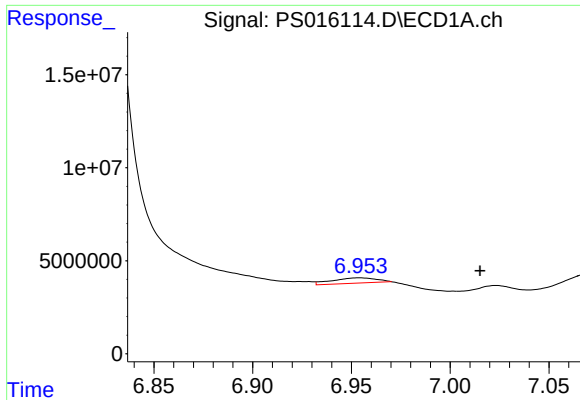

#3 4-Nitrophenol


R.T.: 6.954 min
Delta R.T.: -0.061 min
Response: 4461041
Conc: 5.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

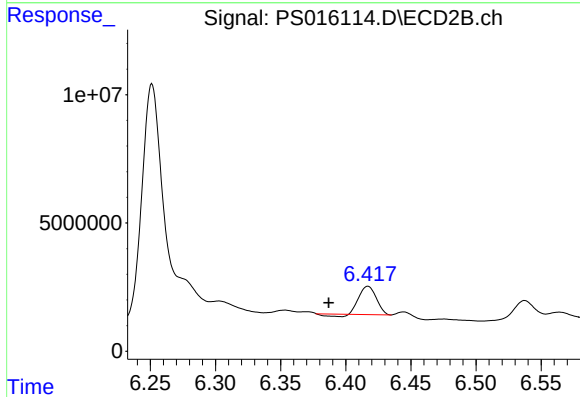


#3 4-Nitrophenol

R.T.: 6.417 min
Delta R.T.: 0.030 min
Response: 9824643
Conc: 31.13 ng/ml

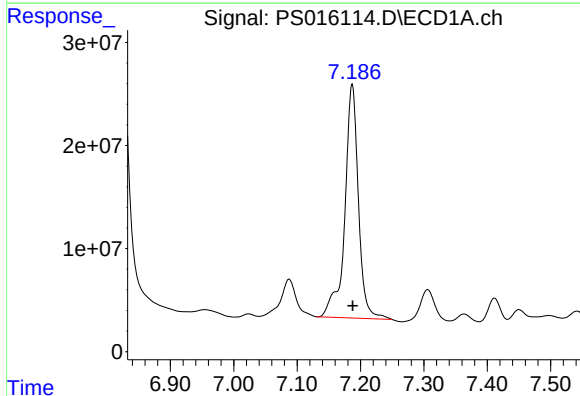


#4 2,4-DCAA

R.T.: 7.187 min
Delta R.T.: -0.001 min
Response: 339319579
Conc: 221.03 ng/ml

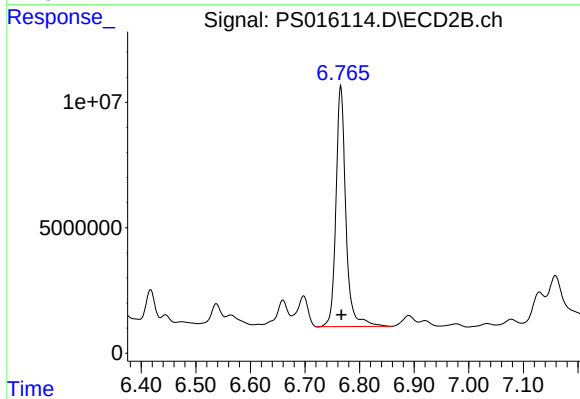

#4 2,4-DCAA


R.T.: 6.766 min
Delta R.T.: -0.001 min
Response: 120849977
Conc: 235.43 ng/ml

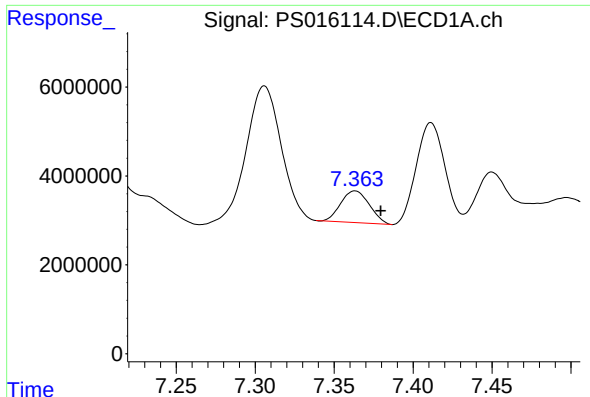

#5 DICAMBA


R.T.: 7.363 min
Delta R.T.: -0.016 min
Response: 9029546
Conc: 1.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

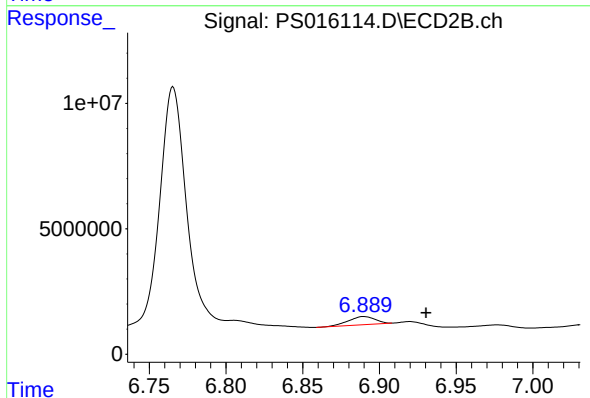


#5 DICAMBA

R.T.: 6.890 min
Delta R.T.: -0.040 min
Response: 3917703
Conc: 1.86 ng/ml

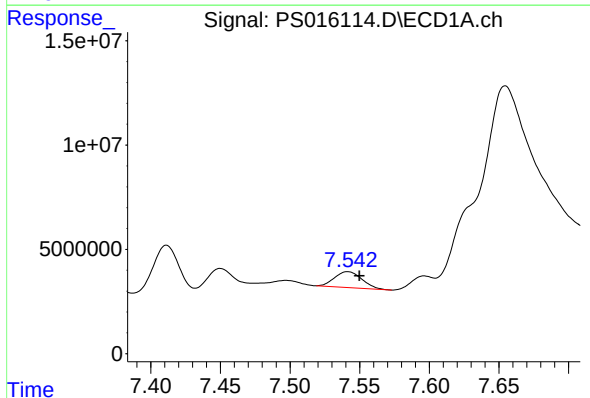


#6 MCP

R.T.: 7.541 min
Delta R.T.: -0.008 min
Response: 10450202
Conc: 2.38 ug/ml

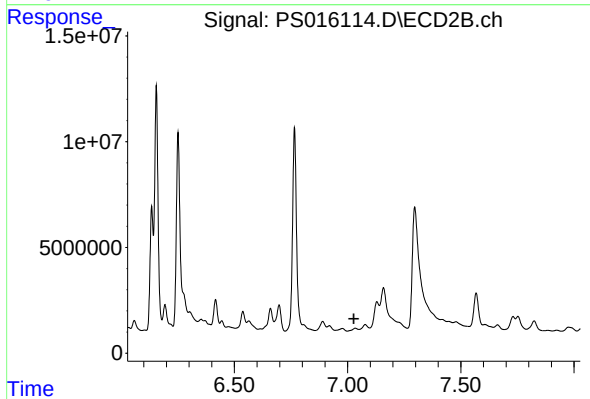

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.028 min
Response: 0
Conc: N.D.

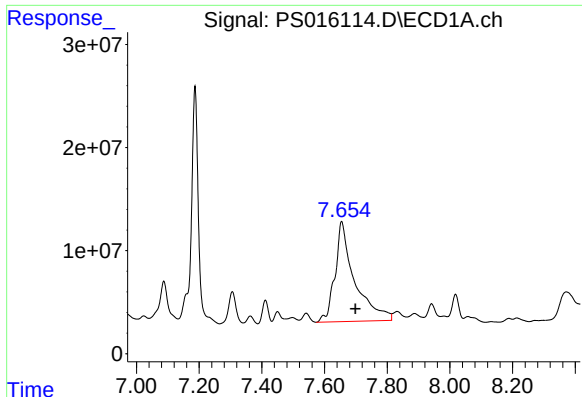

#7 MCPA


R.T.: 7.655 min
Delta R.T.: -0.044 min
Response: 421599081
Conc: 66.30 ug/ml

Instrument :
ECD_S
ClientSampleId :

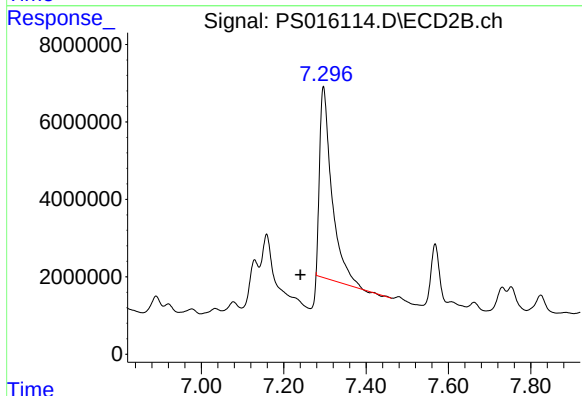


#7 MCPA

R.T.: 7.297 min
Delta R.T.: 0.056 min
Response: 101904533
Conc: 38.66 ug/ml

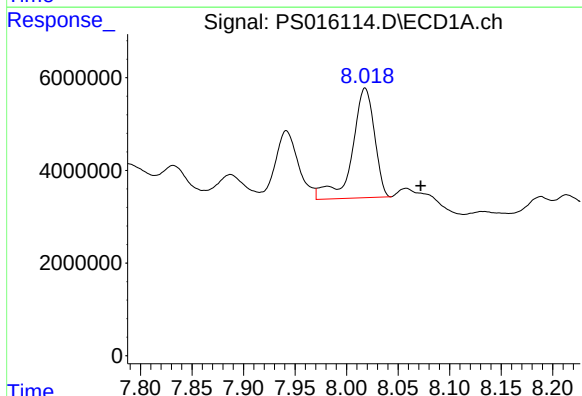


#8 DICHLORPROP

R.T.: 8.018 min
Delta R.T.: -0.054 min
Response: 35633095
Conc: 25.62 ng/ml

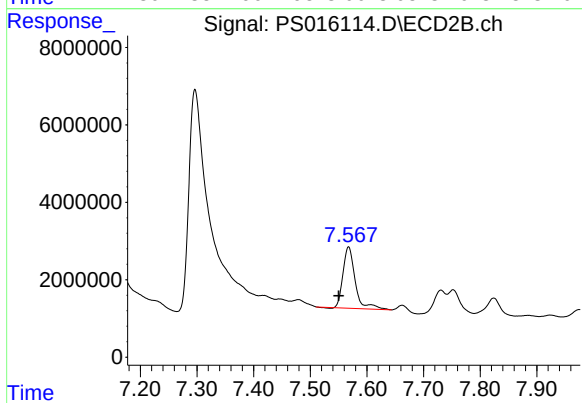

#8 DICHLORPROP


R.T.: 7.568 min
Delta R.T.: 0.018 min
Response: 23610943
Conc: 44.84 ng/ml

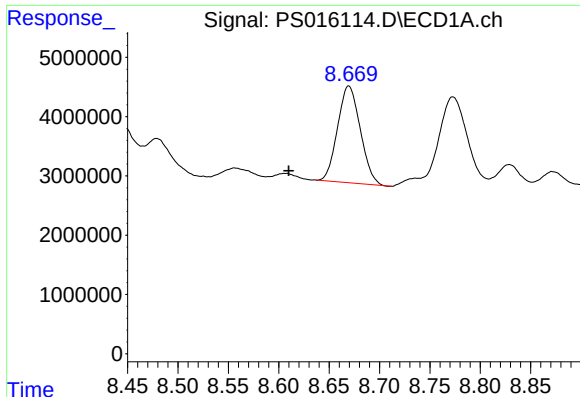

#10 Pentachlorophenol


R.T.: 8.670 min
Delta R.T.: 0.060 min
Response: 25621275
Conc: 1.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

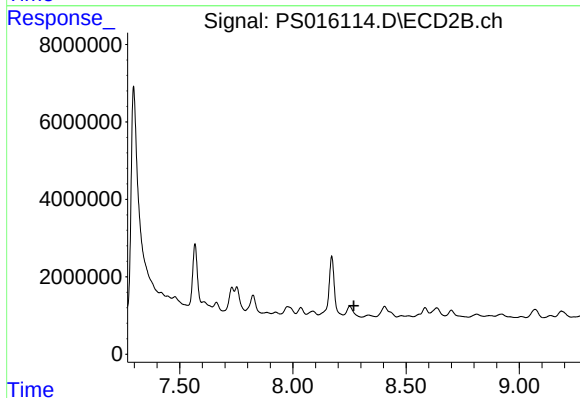


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.269 min
Response: 0
Conc: N.D.

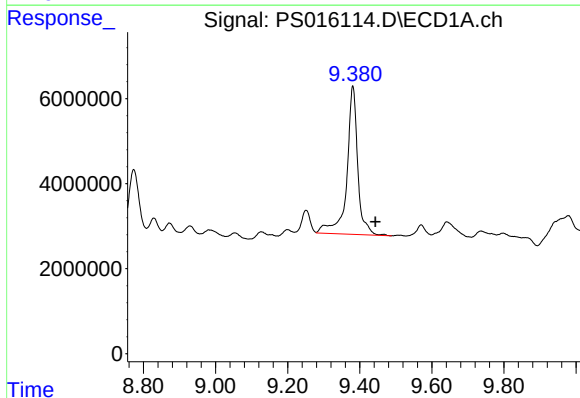

#12 2,4,5-T

R.T.: 9.381 min
Delta R.T.: -0.063 min
Response: 73427736
Conc: 9.40 ng/ml

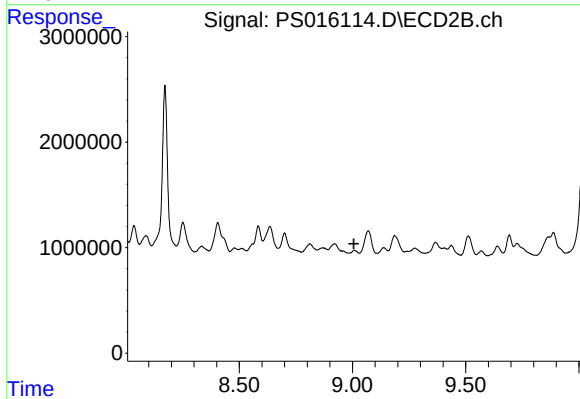

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.006 min
Response: 0
Conc: N.D.