

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071522\
 Data File : PS019962.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2022 08:27
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 01:32:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 27 17:26:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	6.795	1691955	199388	<MDL	<MDL #
Target Compounds							
2) T	3,5-DICHL...	6.392	5.974	-28900	627486	N.D.	<MDL
5) T	DICAMBA	7.377	6.945	787375	513985	<MDL	<MDL #
6) T	MCP	7.581	6.996f	-134632	265.6E6	N.D.	92.522
7) T	MCPA	7.673	0.000	36544437	0	3.119	N.D. #
8) T	DICHLORPROP	8.099	7.534	2755638	387415	1.018	<MDL #
9) T	2,4-D	8.249f	7.859	10799534	1162117	3.636	1.031 #
10) T	Pentachlo...	8.631	8.276	1654210	175740	<MDL	<MDL #
11) T	2,4,5-TP ...	9.173	8.656	1327484	899458	<MDL	<MDL #
12) T	2,4,5-T	9.490f	9.037	859076	543710	<MDL	<MDL #
13) T	2,4-DB	9.994	9.542	26302427	1288098	6.573	1.983 #
14) T	DINOSEB	11.194f	9.845	6808109	998635	<MDL	<MDL #
15) T	Picloram	10.948	10.871f	997.4E6	21146546	31.984	3.252 #
16) T	DCPA	11.426	10.787	1872829	16542845	<MDL	2.553 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071522\
Data File : PS019962.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2022 08:27
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 01:32:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
Quant Title : 8080.M
QLast Update : Mon Jun 27 17:26:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

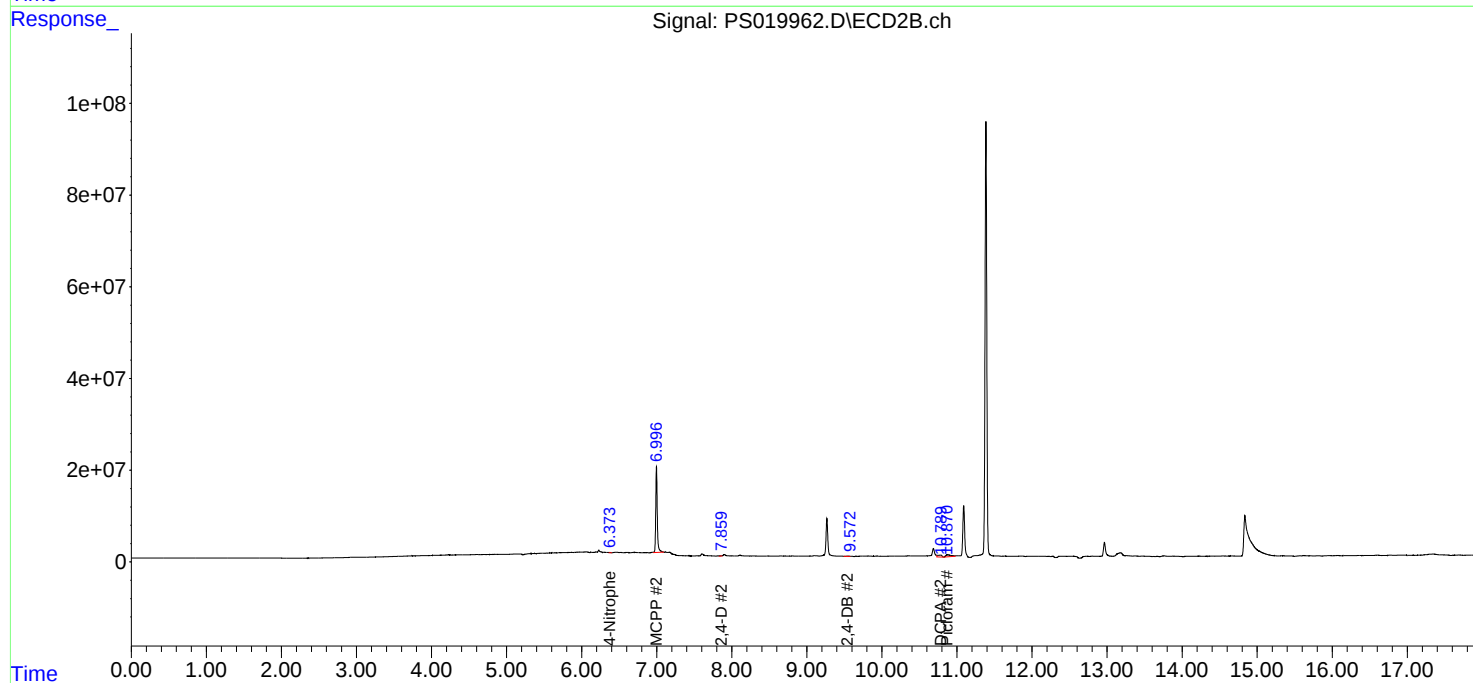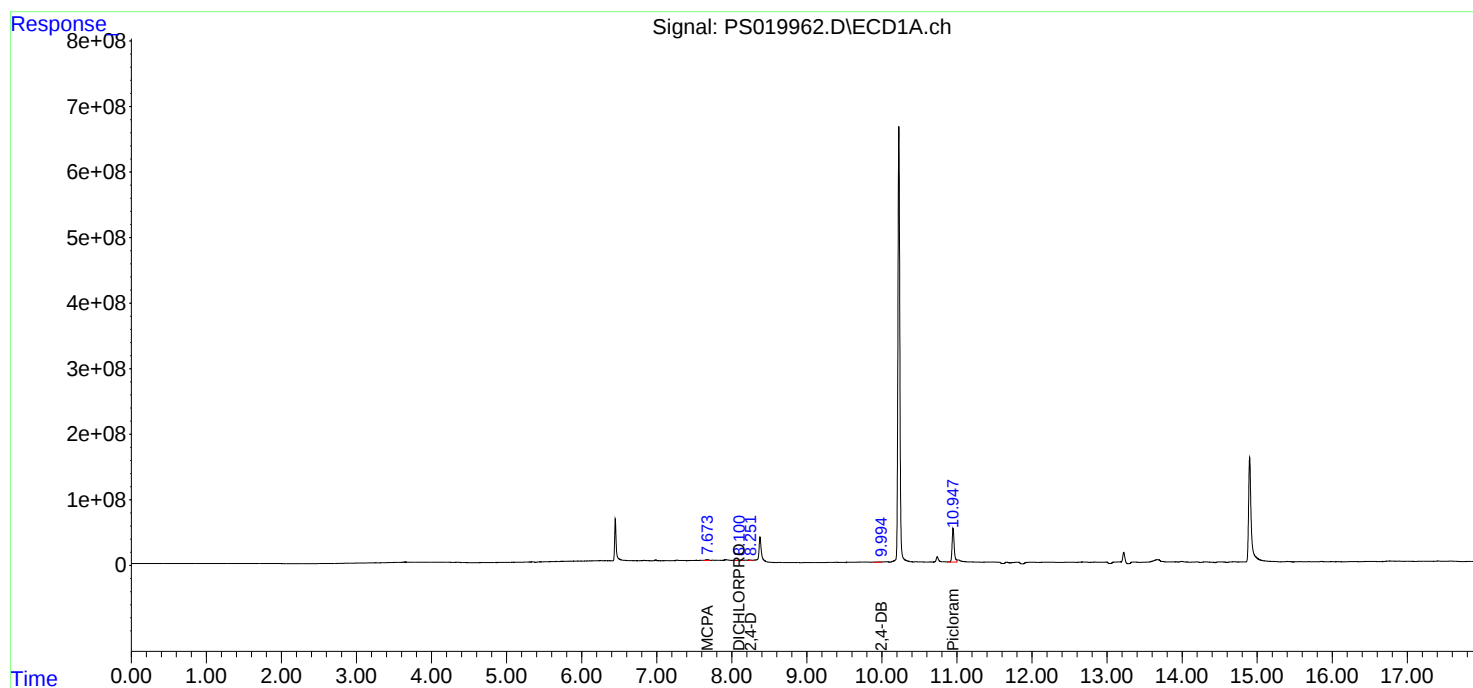


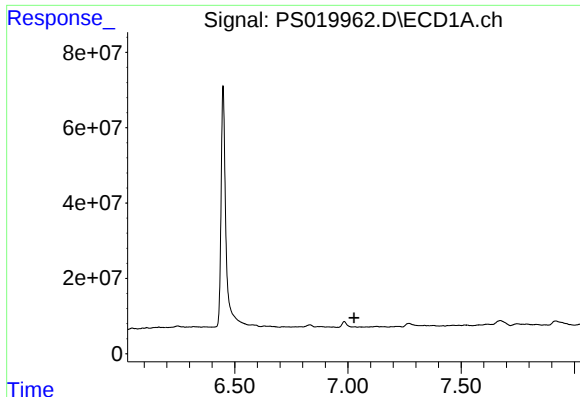

#3 4-Nitrophenol


R.T.: 7.031 min
Delta R.T.: 0.005 min
Response: -2327945
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

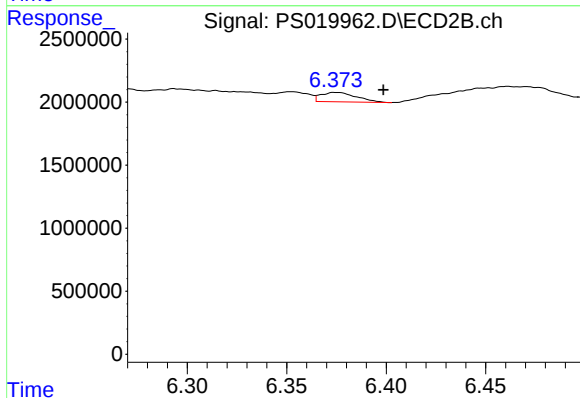


#3 4-Nitrophenol

R.T.: 6.375 min
Delta R.T.: -0.024 min
Response: 922649
Conc: 2.13 ng/ml

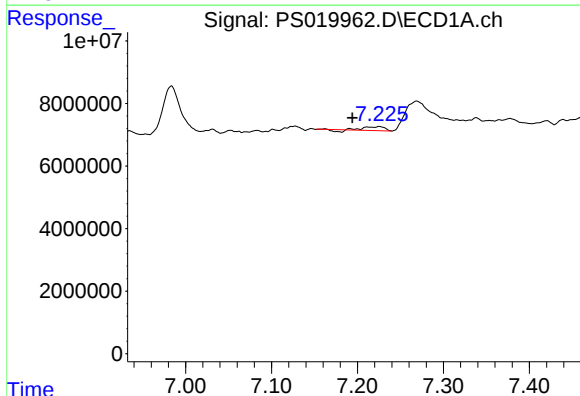


#4 2,4-DCAA

R.T.: 7.225 min
Delta R.T.: 0.031 min
Response: 1691955
Conc: N.D.

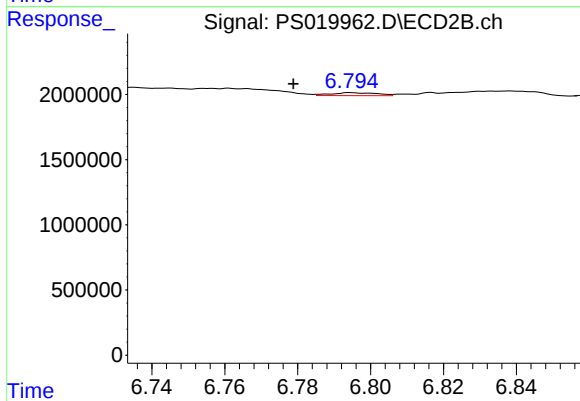

#4 2,4-DCAA


R.T.: 6.795 min
Delta R.T.: 0.016 min
Response: 199388
Conc: N.D.

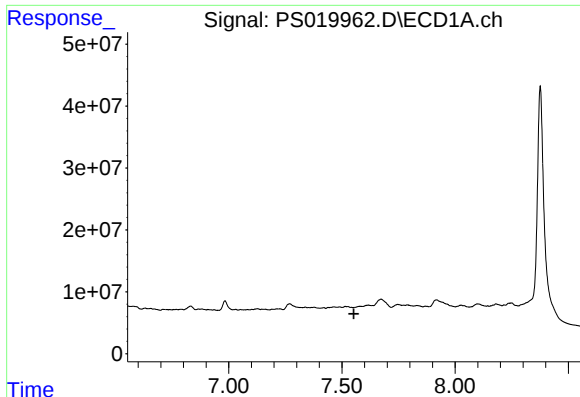

#6 MCPP


R.T.: 7.581 min
Delta R.T.: 0.028 min
Response: -134632
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

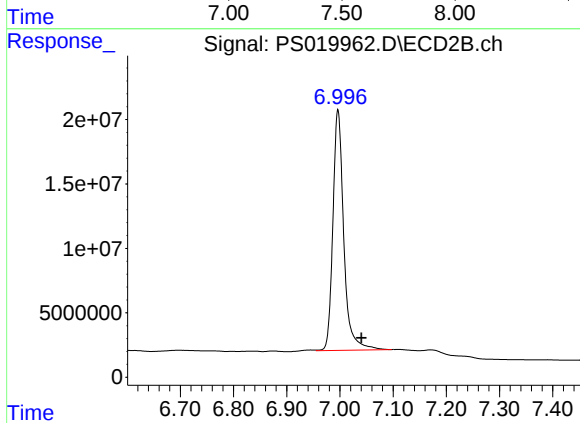


#6 MCPP

R.T.: 6.996 min
Delta R.T.: -0.044 min
Response: 265577702
Conc: 92.52 ug/ml

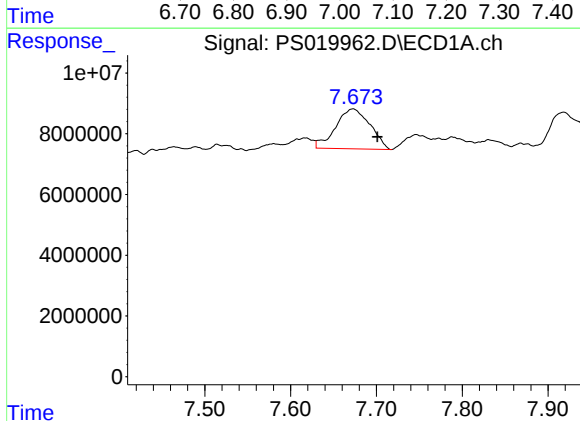


#7 MCPA

R.T.: 7.673 min
Delta R.T.: -0.029 min
Response: 36544437
Conc: 3.12 ug/ml

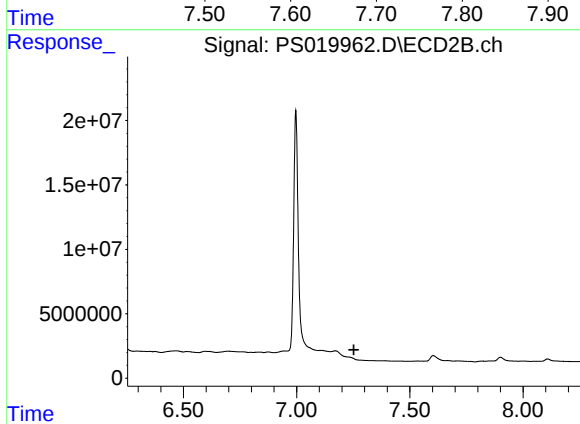

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.253 min
Response: 0
Conc: N.D.

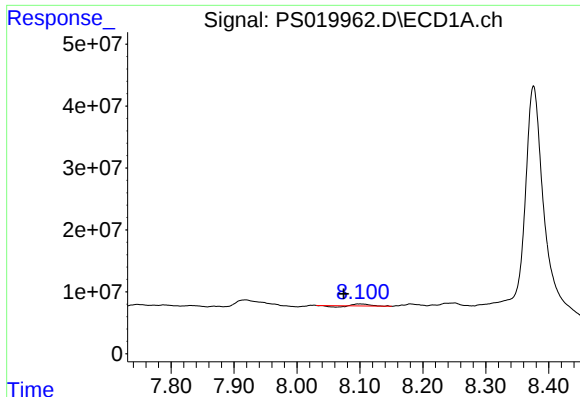

#8 DICHLORPROP


R.T.: 8.099 min
Delta R.T.: 0.025 min
Response: 2755638
Conc: 1.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

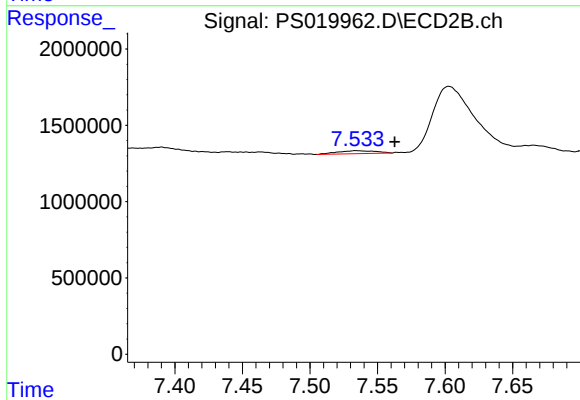


#8 DICHLORPROP

R.T.: 7.534 min
Delta R.T.: -0.029 min
Response: 387415
Conc: N.D.

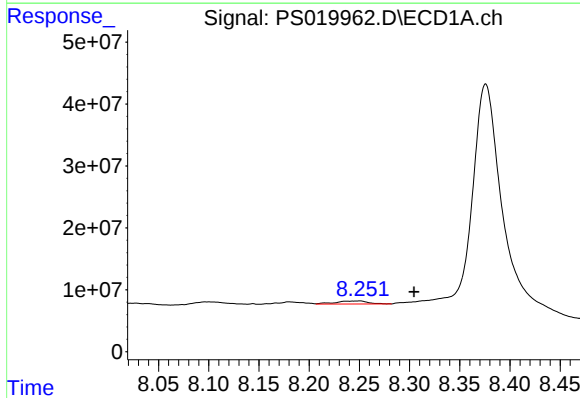


#9 2,4-D

R.T.: 8.249 min
Delta R.T.: -0.056 min
Response: 10799534
Conc: 3.64 ng/ml

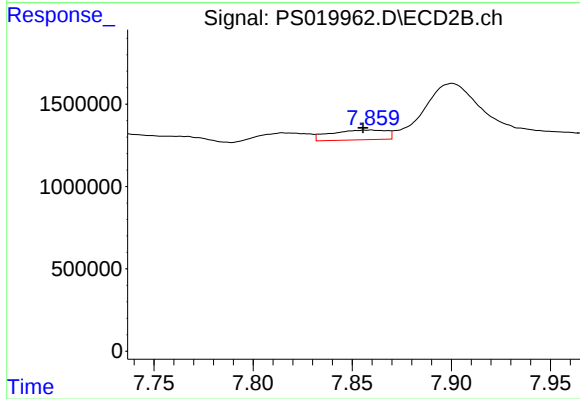

#9 2,4-D


R.T.: 7.859 min
Delta R.T.: 0.004 min
Response: 1162117
Conc: 1.03 ng/ml

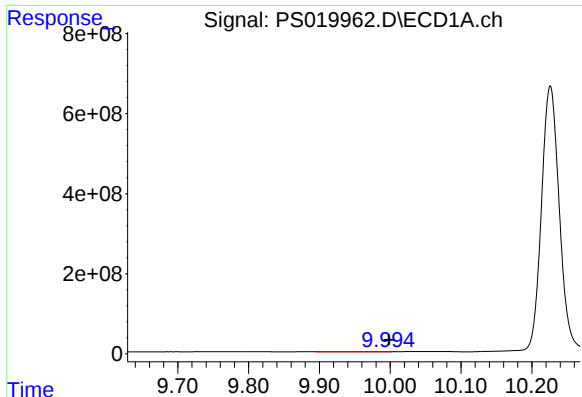

#13 2,4-DB


R.T.: 9.994 min
Delta R.T.: -0.004 min
Response: 26302427
Conc: 6.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

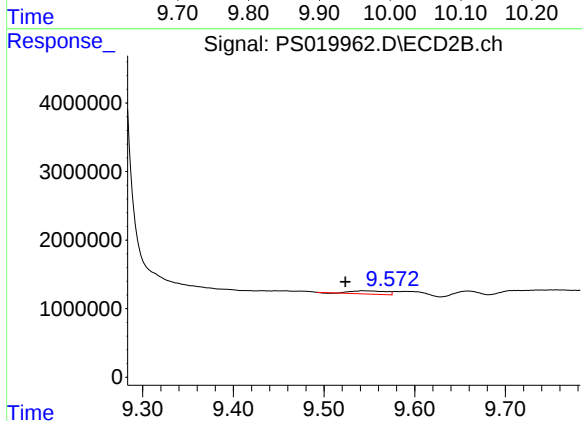


#13 2,4-DB

R.T.: 9.542 min
Delta R.T.: 0.019 min
Response: 1288098
Conc: 1.98 ng/ml

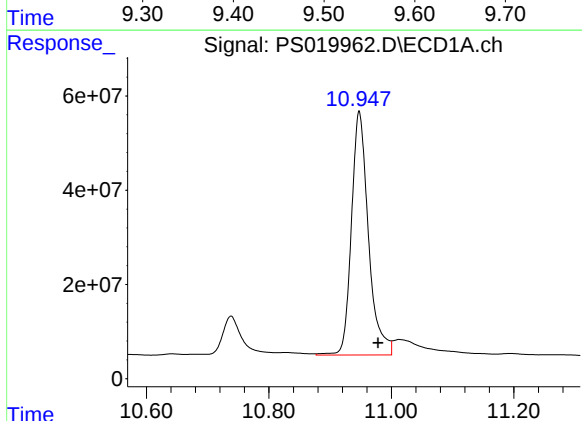


#15 Picloram

R.T.: 10.948 min
Delta R.T.: -0.031 min
Response: 997362069
Conc: 31.98 ng/ml

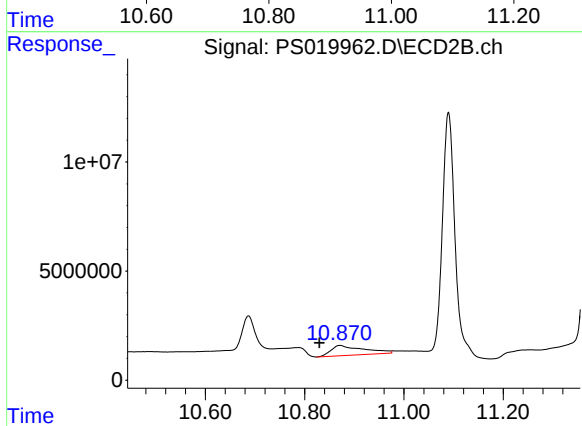

#15 Picloram


R.T.: 10.871 min
Delta R.T.: 0.041 min
Response: 21146546
Conc: 3.25 ng/ml

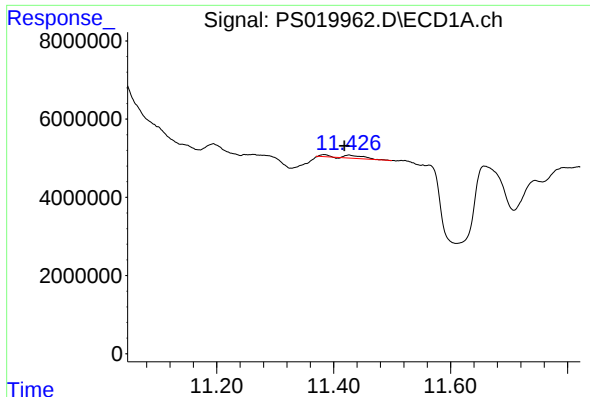

#16 DCPA

R.T.: 11.426 min
Delta R.T.: 0.007 min
Response: 1872829
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

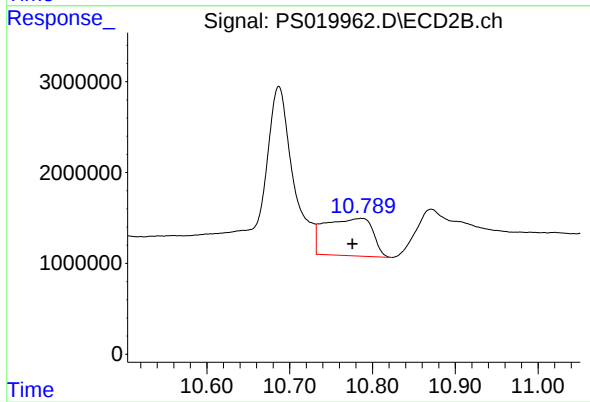

#16 DCPA

R.T.: 10.787 min
Delta R.T.: 0.011 min
Response: 16542845
Conc: 2.55 ng/ml