

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071522\
 Data File : PS019965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2022 10:14
 Operator : AJ\MA
 Sample : PB146244BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 01:33:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 27 17:26:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	6.754	0	401633	N.D.	<MDL
Target Compounds							
2) T	3,5-DICHL...	6.438	0.000	300533	0	<MDL	N.D. #
3) T	4-Nitroph...	6.991	0.000	1548053	0	1.454	N.D. #
5) T	DICAMBA	0.000	6.946	0	314675	N.D.	<MDL
7) T	MCPA	7.688	0.000	464.3E6	0	39.620	N.D. #
10) T	Pentachlo...	8.620	8.283	2293459	906785	<MDL	<MDL #
11) T	2,4,5-TP ...	9.190	8.660	2828750	759201	<MDL	<MDL #
12) T	2,4,5-T	9.474	9.077f	24623452	448986	1.338	<MDL #
13) T	2,4-DB	9.998	0.000	73292	0	<MDL	N.D. #
14) T	DINOSEB	11.106f	9.852	87659794	473753	5.392	<MDL #
15) T	Picloram	10.976	10.776f	2123564	1510183	<MDL	<MDL #
16) T	DCPA	11.421	10.776	5563127	1510183	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071522\
Data File : PS019965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2022 10:14
Operator : AJ\MA
Sample : PB146244BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 01:33:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
Quant Title : 8080.M
QLast Update : Mon Jun 27 17:26:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

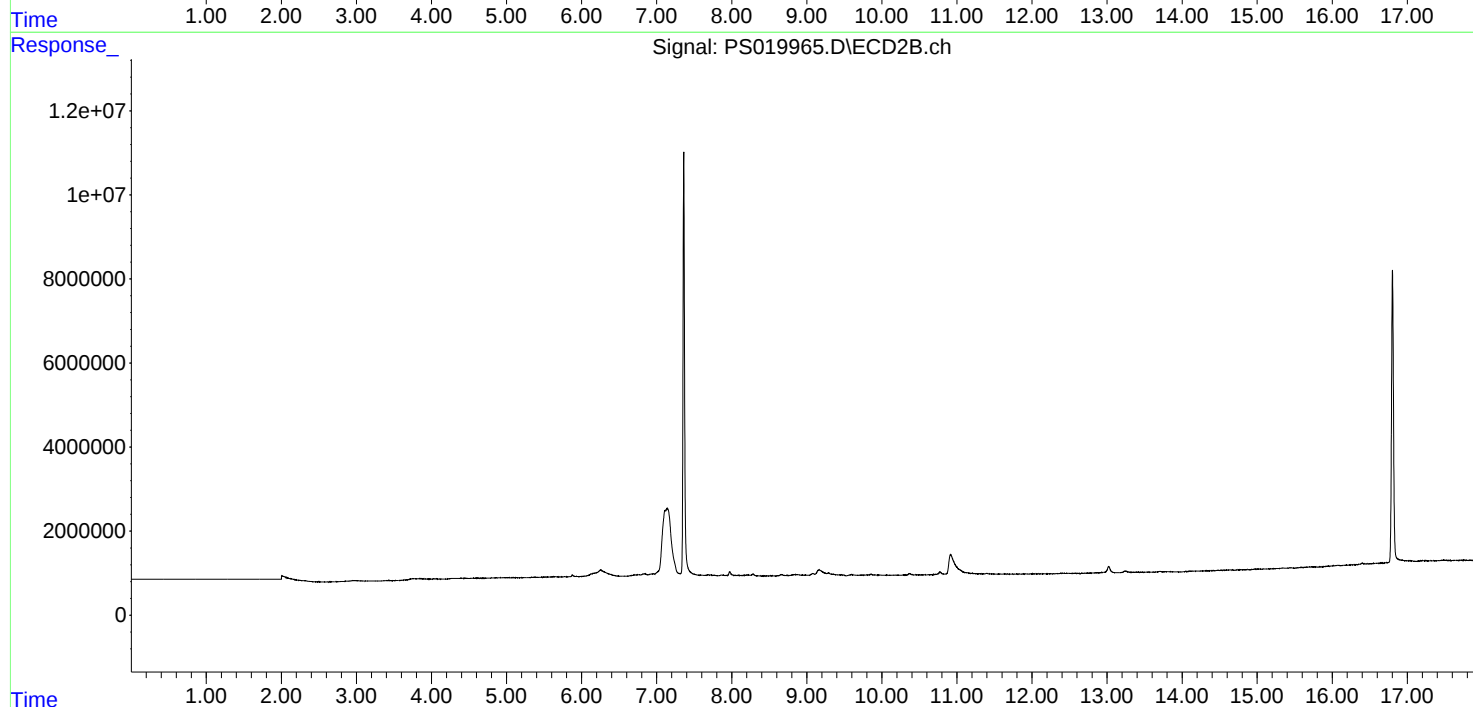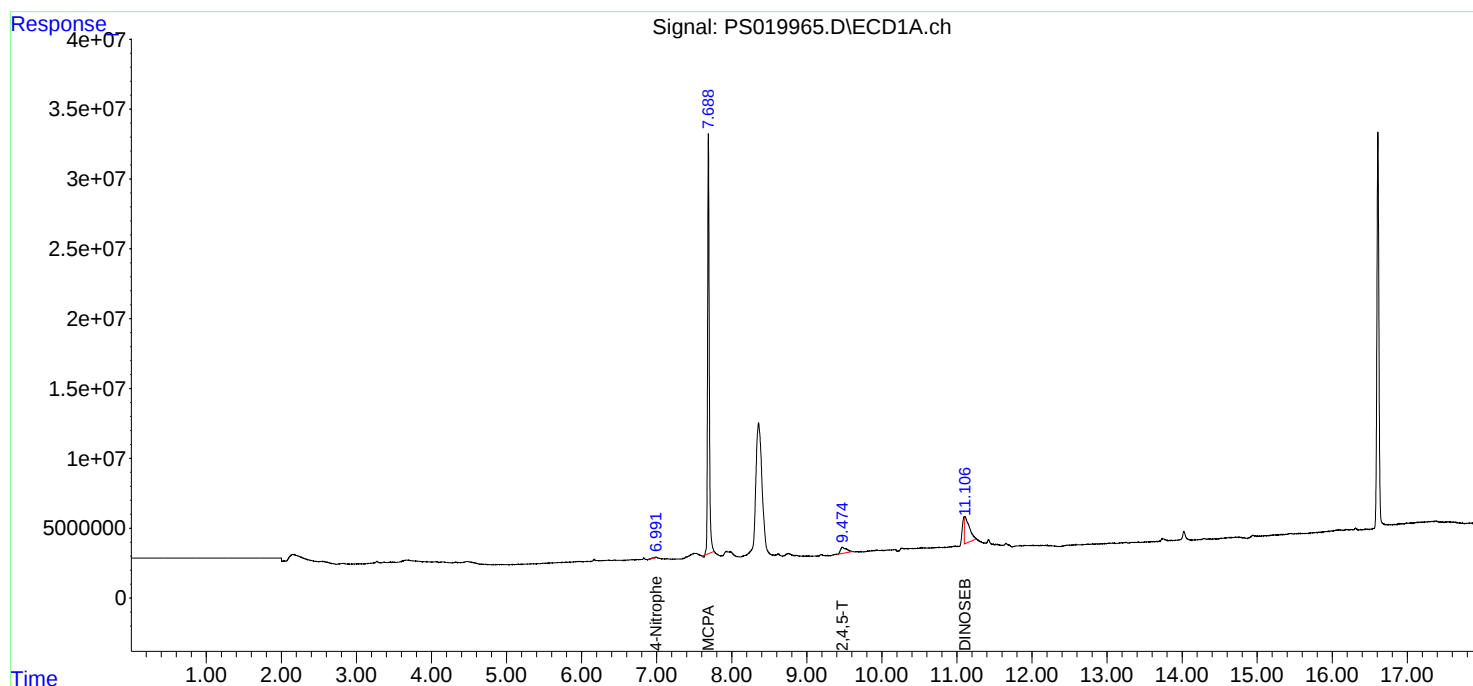


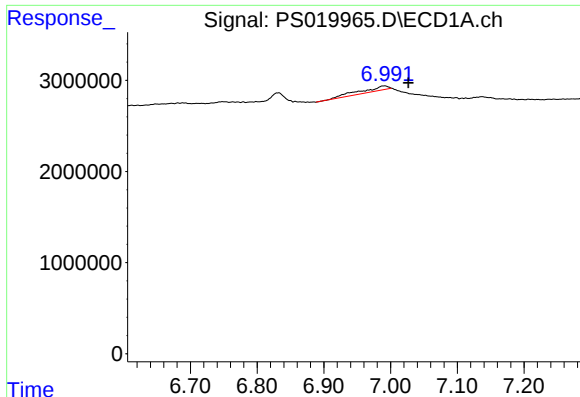

#3 4-Nitrophenol


R.T.: 6.991 min
Delta R.T.: -0.036 min
Response: 1548053
Conc: 1.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

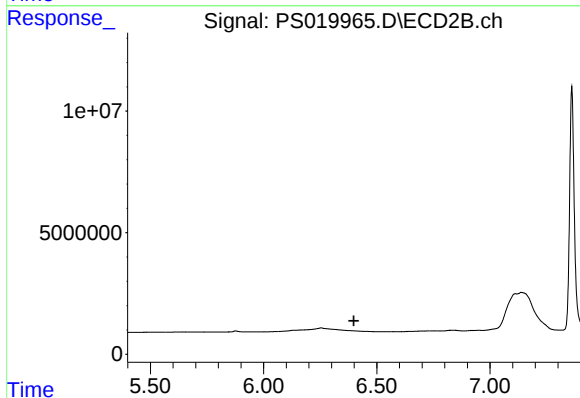


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

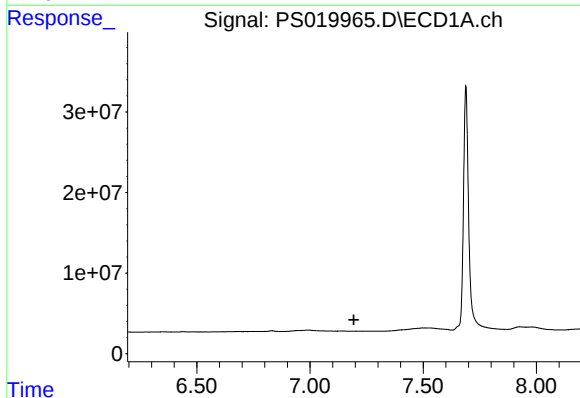


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.194 min
Response: 0
Conc: N.D.

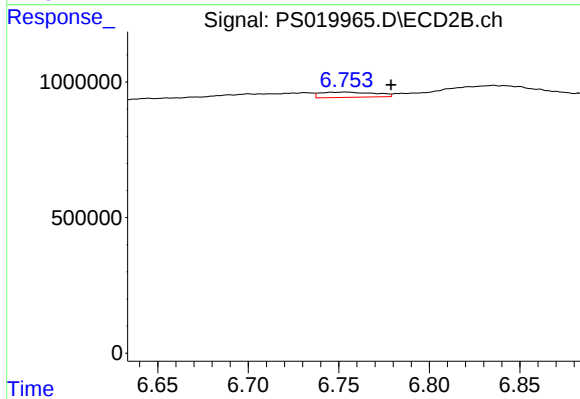

#4 2,4-DCAA


R.T.: 6.754 min
Delta R.T.: -0.025 min
Response: 401633
Conc: N.D.

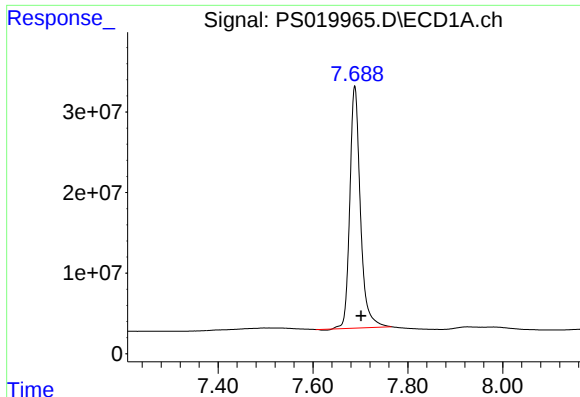

#7 MCPA


R.T.: 7.688 min
Delta R.T.: -0.013 min
Response: 464263832
Conc: 39.62 ug/ml

Instrument :
ECD_S
ClientSampleId :

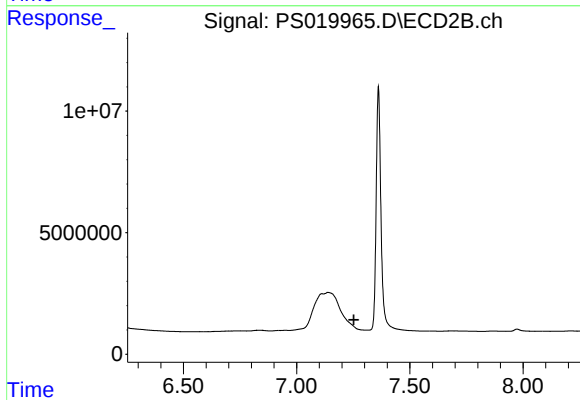


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

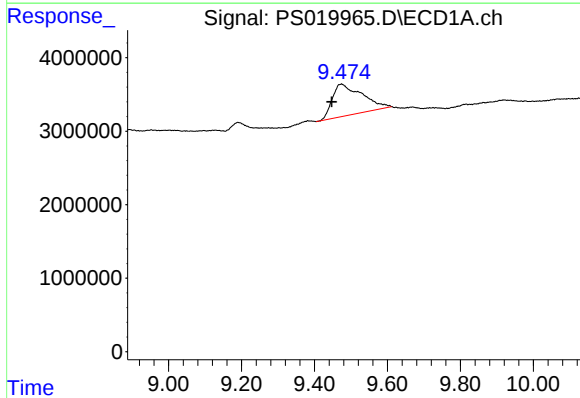


#12 2,4,5-T

R.T.: 9.474 min
Delta R.T.: 0.027 min
Response: 24623452
Conc: 1.34 ng/ml

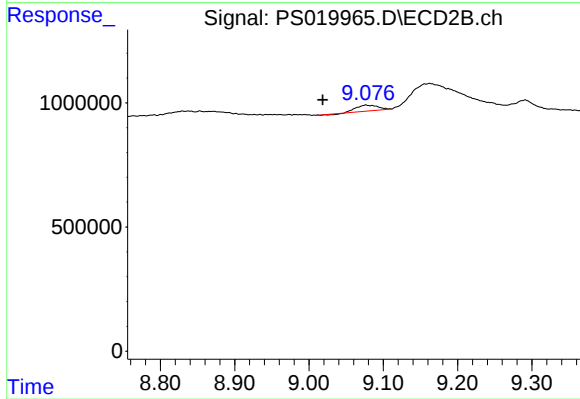

#12 2,4,5-T


R.T.: 9.077 min
Delta R.T.: 0.058 min
Response: 448986
Conc: N.D.

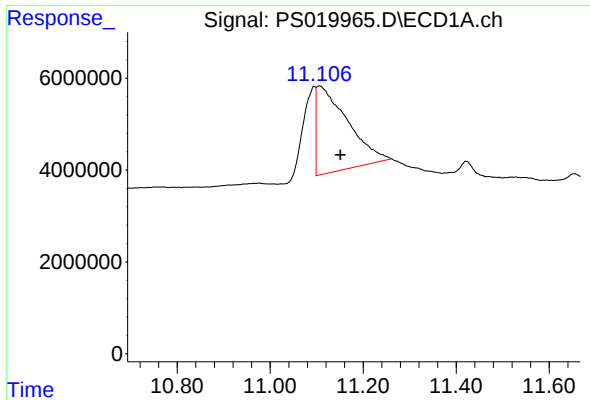

#14 DINOSEB

R.T.: 11.106 min
Delta R.T.: -0.045 min
Response: 87659794
Conc: 5.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

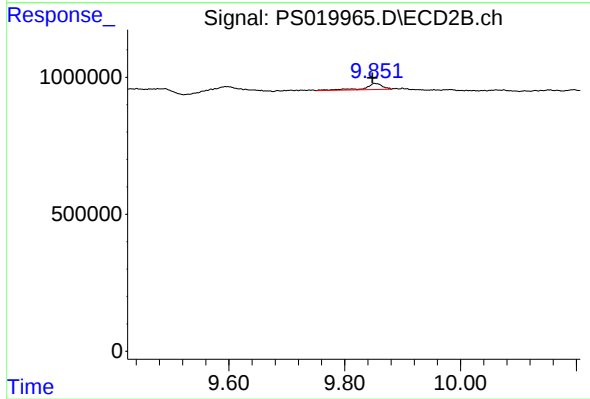

#14 DINOSEB

R.T.: 9.852 min
Delta R.T.: 0.004 min
Response: 473753
Conc: N.D.