

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071522\
 Data File : PS019967.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2022 11:02
 Operator : AJ\MA
 Sample : PB146202TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 01:34:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 27 17:26:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	6.787	0	960139	N.D.	1.182
Target Compounds							
1) T	Dalapon	3.021	0.000	141375	0	<MDL	N.D. #
3) T	4-Nitroph...	6.990	0.000	615524	0	<MDL	N.D. #
5) T	DICAMBA	7.401	6.954	31479	1385325	<MDL	<MDL #
6) T	MCP	7.559	0.000	1833562	0	<MDL	N.D. #
7) T	MCPA	7.686	0.000	470.4E6	0	40.147	N.D. #
10) T	Pentachlo...	8.621	8.286	1475336	927010	<MDL	<MDL #
11) T	2,4,5-TP ...	9.197	8.665	2488644	566735	<MDL	<MDL #
12) T	2,4,5-T	9.483	0.000	14421262	0	<MDL	N.D. #
13) T	2,4-DB	9.974	0.000	339677	0	<MDL	N.D. #
14) T	DINOSEB	11.127	9.856	66382576	245423	4.083	<MDL #
15) T	Picloram	10.974	10.778f	1349001	965128	<MDL	<MDL #
16) T	DCPA	11.419	10.778	3354344	965128	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071522\
Data File : PS019967.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2022 11:02
Operator : AJ\MA
Sample : PB146202TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 01:34:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
Quant Title : 8080.M
QLast Update : Mon Jun 27 17:26:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

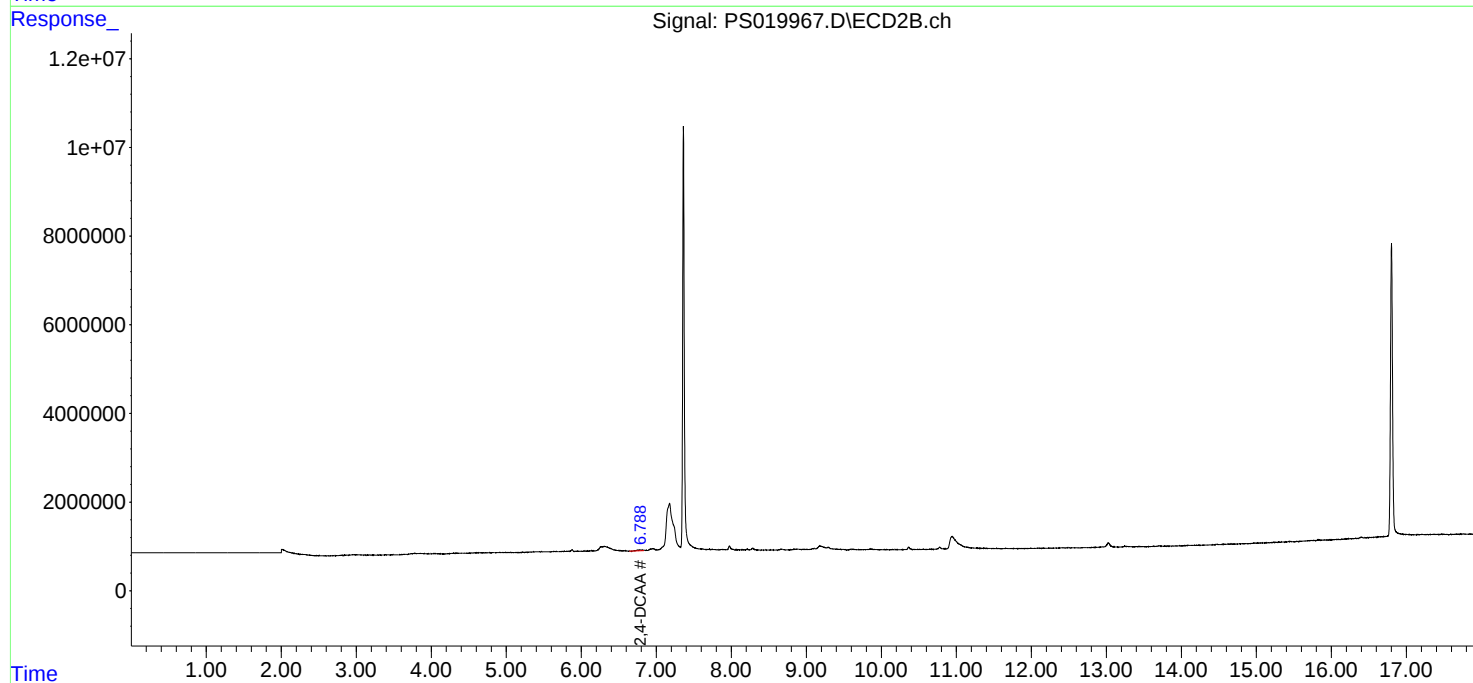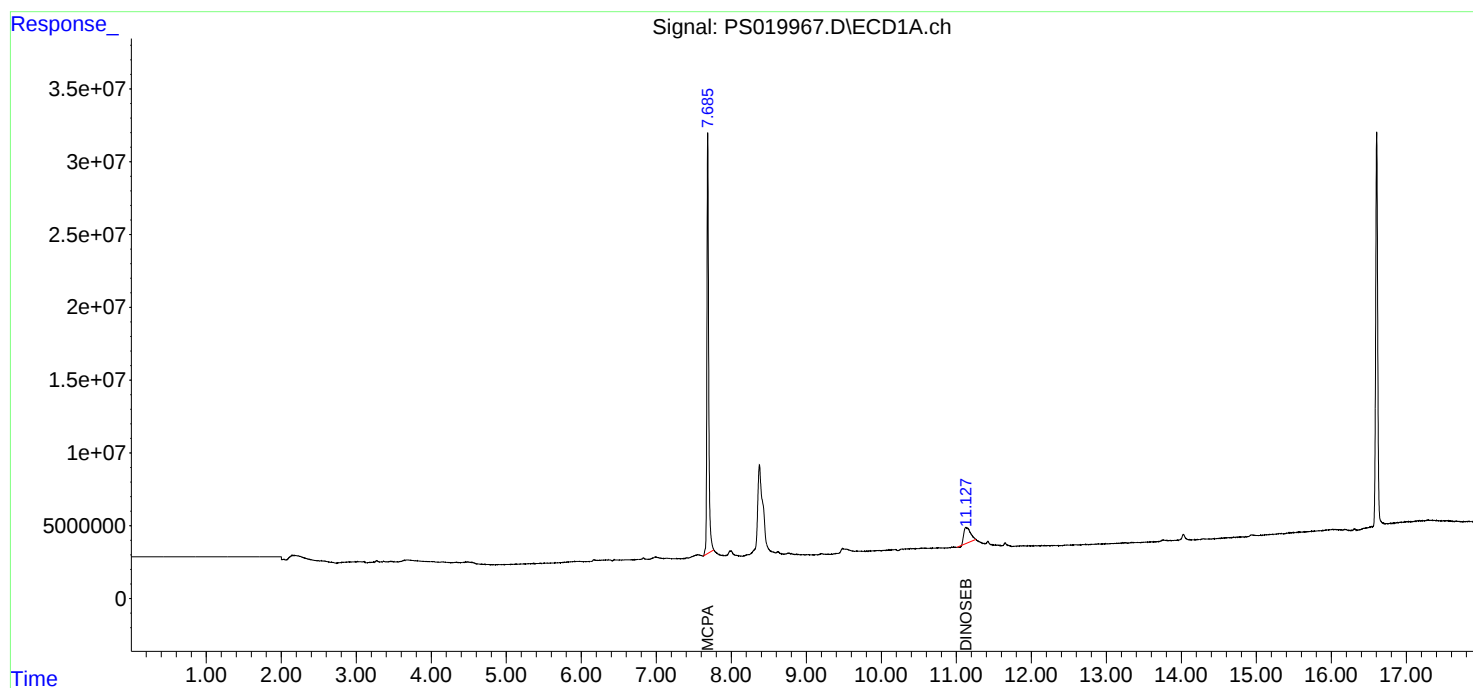


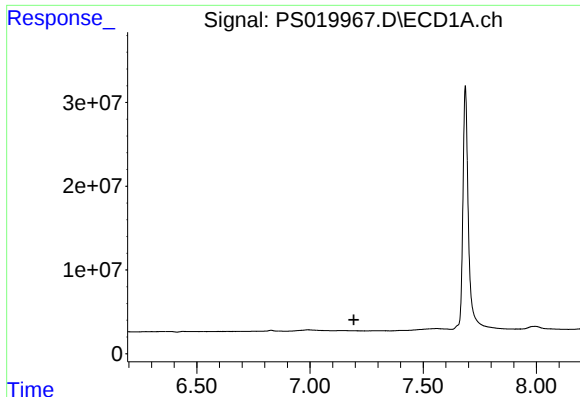

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.194 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

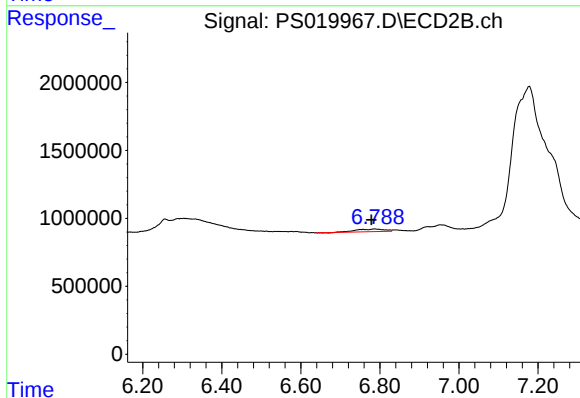


#4 2,4-DCAA

R.T.: 6.787 min
Delta R.T.: 0.009 min
Response: 960139
Conc: 1.18 ng/ml

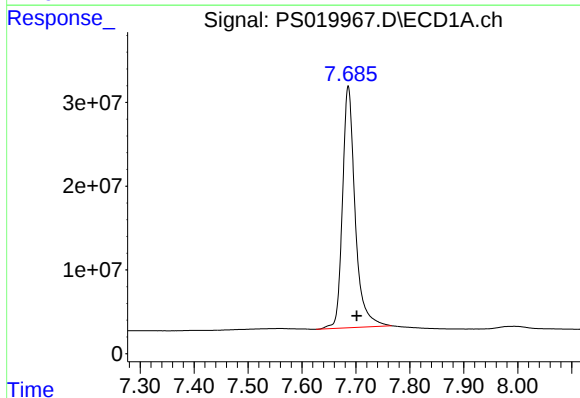


#7 MCPA

R.T.: 7.686 min
Delta R.T.: -0.015 min
Response: 470445233
Conc: 40.15 ug/ml

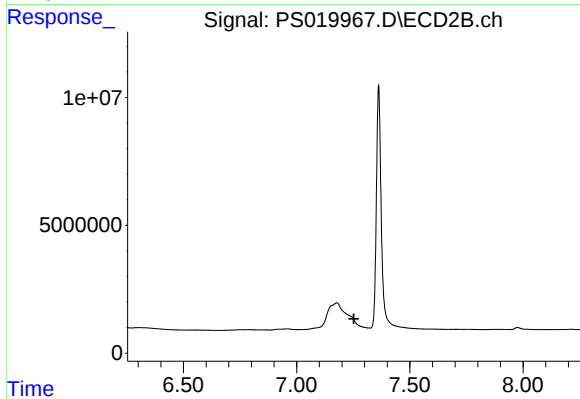

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.253 min
Response: 0
Conc: N.D.

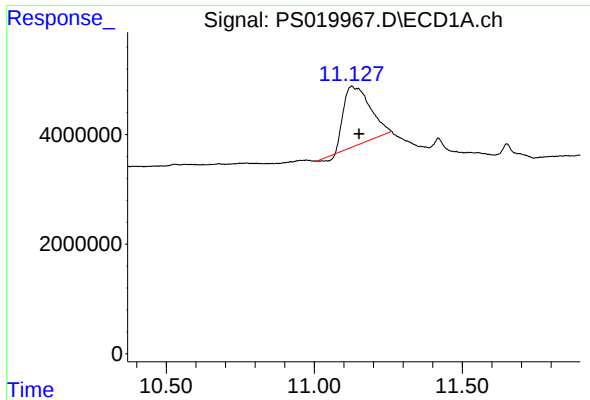

#14 DINOSEB

R.T.: 11.127 min
Delta R.T.: -0.024 min
Response: 66382576
Conc: 4.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

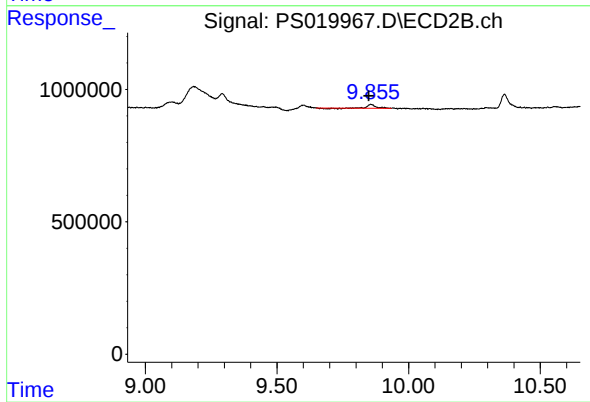

#14 DINOSEB

R.T.: 9.856 min
Delta R.T.: 0.008 min
Response: 245423
Conc: N.D.