

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071522\
 Data File : PS019972.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2022 13:04
 Operator : AJ\MA
 Sample : PB146245BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 01:35:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 27 17:26:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.135f	6.787	504638	664954	<MDL	<MDL	#
Target Compounds								
2) T	3,5-DICHL...	6.431	0.000	553768	0	<MDL	N.D.	#
3) T	4-Nitroph...	6.985f	0.000	1005378	0	<MDL	N.D.	#
5) T	DICAMBA	7.382	6.933	46021	1106435	<MDL	<MDL	#
6) T	MCP	7.560	0.000	2225647	0	<MDL	N.D.	#
7) T	MCPA	7.683	0.000	511.3E6	0	43.633	N.D.	#
9) T	2,4-D	0.000	7.841	0	503949	N.D.	<MDL	
11) T	2,4,5-TP ...	9.187	8.702f	331477	165432	<MDL	<MDL	#
12) T	2,4,5-T	9.461	0.000	7873091	0	<MDL	N.D.	#
13) T	2,4-DB	9.977	0.000	2609591	0	<MDL	N.D.	#
14) T	DINOSEB	0.000	9.883	0	375344	N.D.	<MDL	
15) T	Picloram	11.034f	10.776f	41977998	898571	1.346	<MDL	#
16) T	DCPA	11.417	10.776	1013999	898571	<MDL	<MDL	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071522\
Data File : PS019972.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2022 13:04
Operator : AJ\MA
Sample : PB146245BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 01:35:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
Quant Title : 8080.M
QLast Update : Mon Jun 27 17:26:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

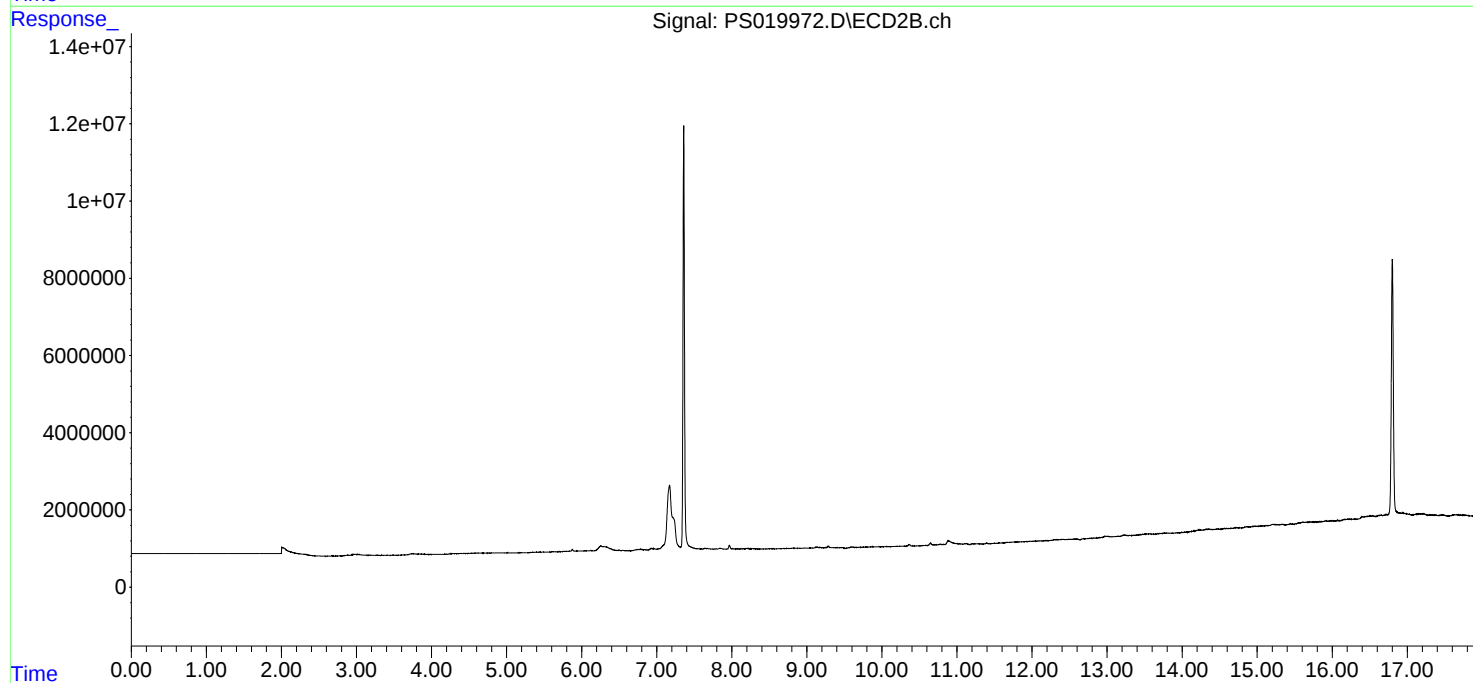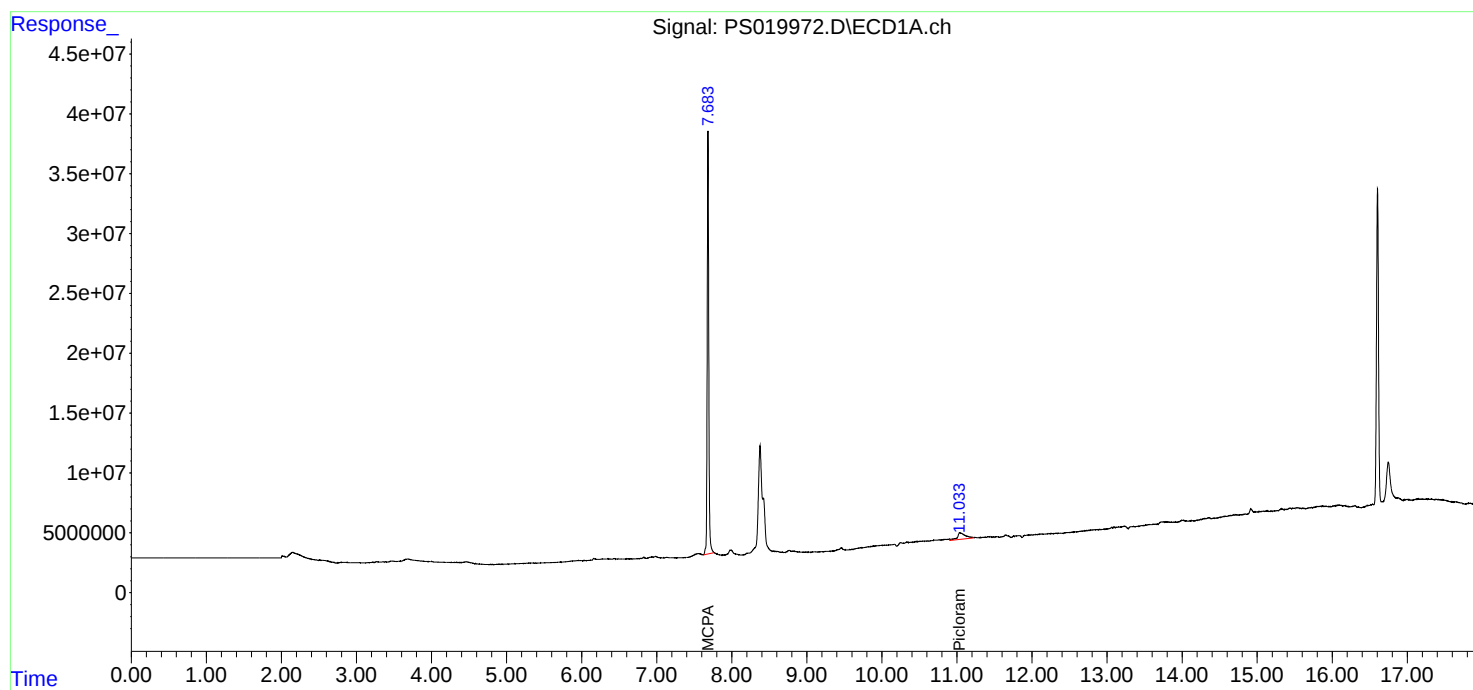


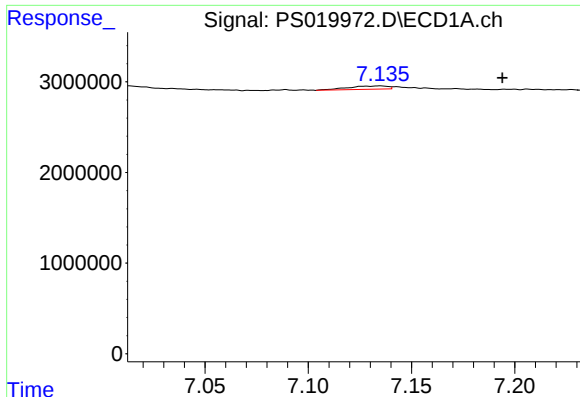

#4 2,4-DCAA


R.T.: 7.135 min
Delta R.T.: -0.059 min
Response: 504638
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

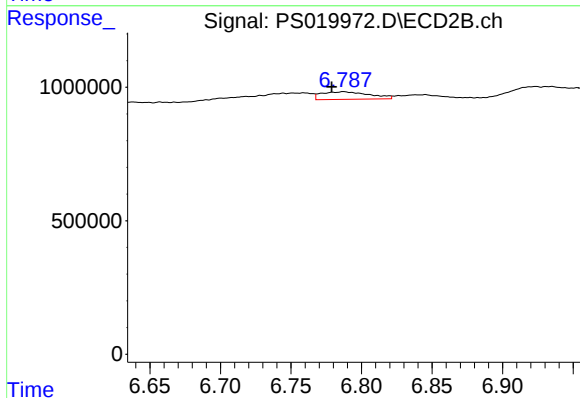


#4 2,4-DCAA

R.T.: 6.787 min
Delta R.T.: 0.008 min
Response: 664954
Conc: N.D.

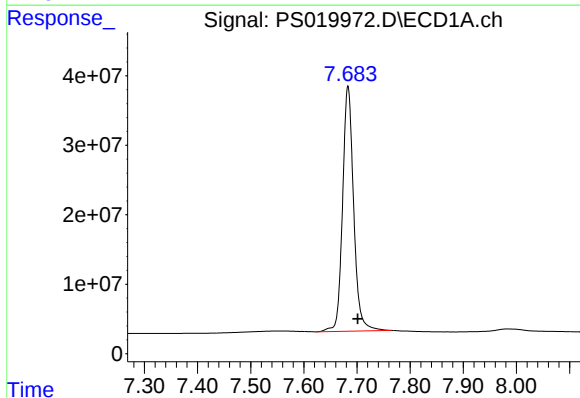


#7 MCPA

R.T.: 7.683 min
Delta R.T.: -0.018 min
Response: 511290326
Conc: 43.63 ug/ml

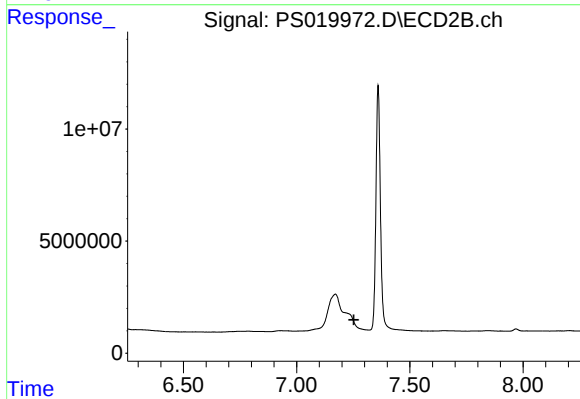

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

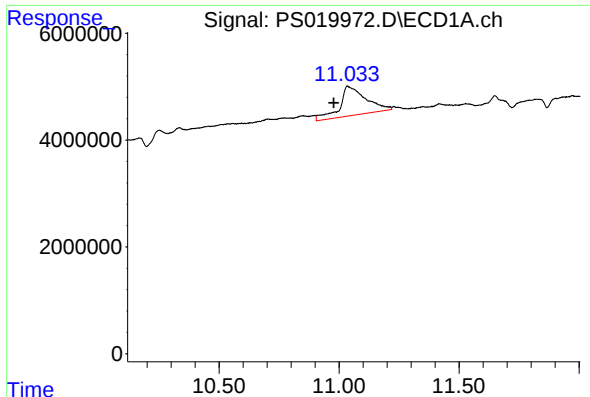

#15 Picloram

R.T.: 11.034 min
Delta R.T.: 0.056 min
Response: 41977998
Conc: 1.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

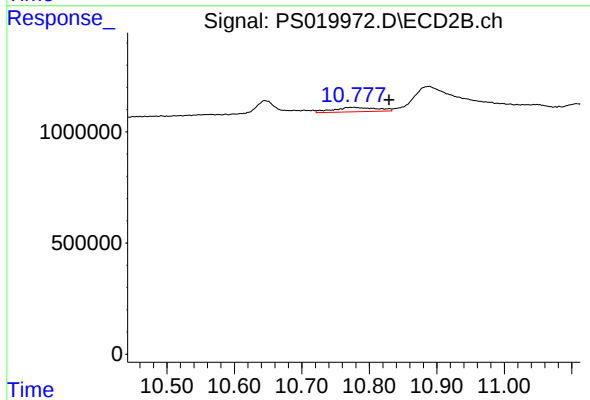

#15 Picloram

R.T.: 10.776 min
Delta R.T.: -0.053 min
Response: 898571
Conc: N.D.