

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071522\
 Data File : PS019974.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2022 14:16
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 01:36:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 27 17:26:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.196	6.780	1239.4E6	396.8E6	477.864	488.540
Target Compounds							
1) T	Dalapon	3.030	0.000	452706	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.363f	0.000	384780	0	<MDL	N.D. #
7) T	MCPA	7.662	0.000	1381301	0	<MDL	N.D. #
10) T	Pentachlo...	0.000	8.282	0	797470	N.D.	<MDL
11) T	2,4,5-TP ...	9.187	0.000	2709980	0	<MDL	N.D. #
13) T	2,4-DB	10.034	0.000	4263591	0	1.065	N.D. #
15) T	Picloram	10.974	0.000	140.9E6	0	4.519	N.D. #
16) T	DCPA	11.417	10.712f	2457895	3509254	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071522\
Data File : PS019974.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2022 14:16
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 01:36:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
Quant Title : 8080.M
QLast Update : Mon Jun 27 17:26:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

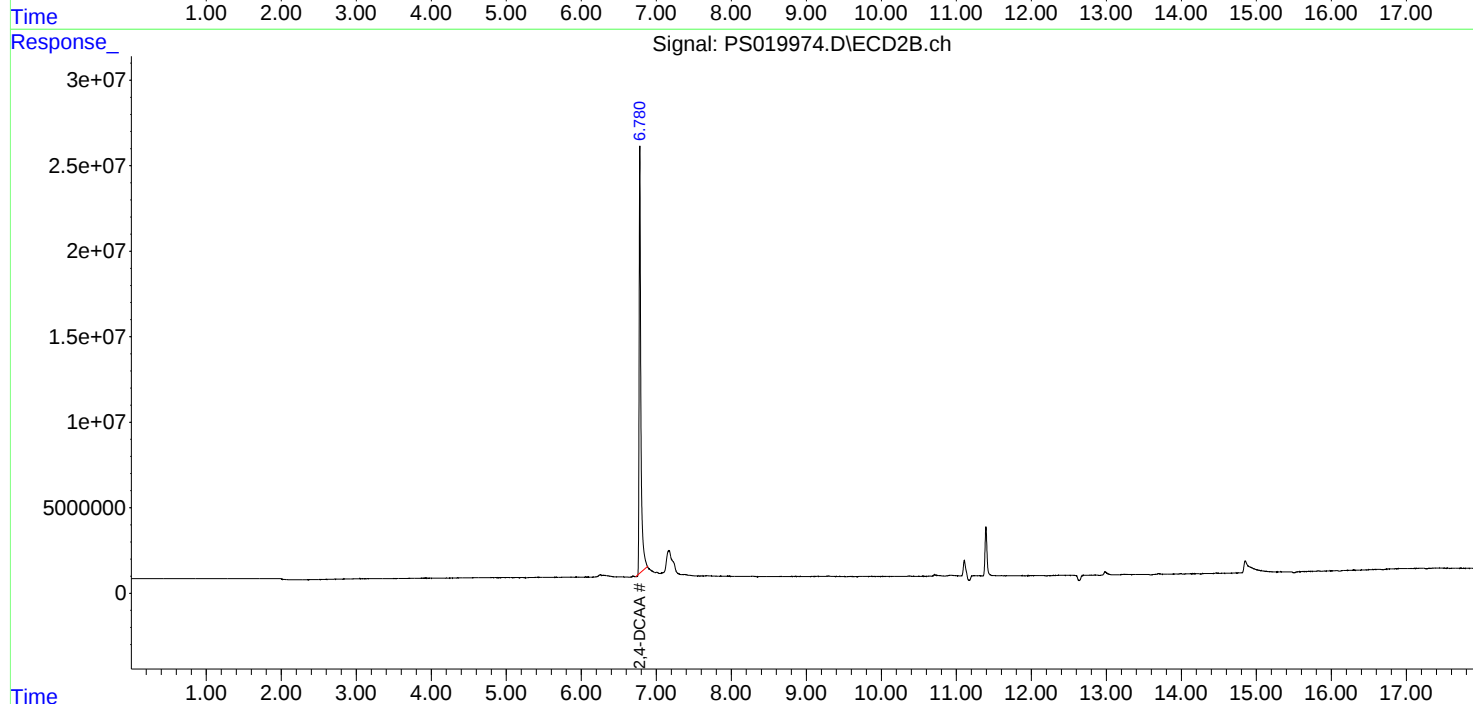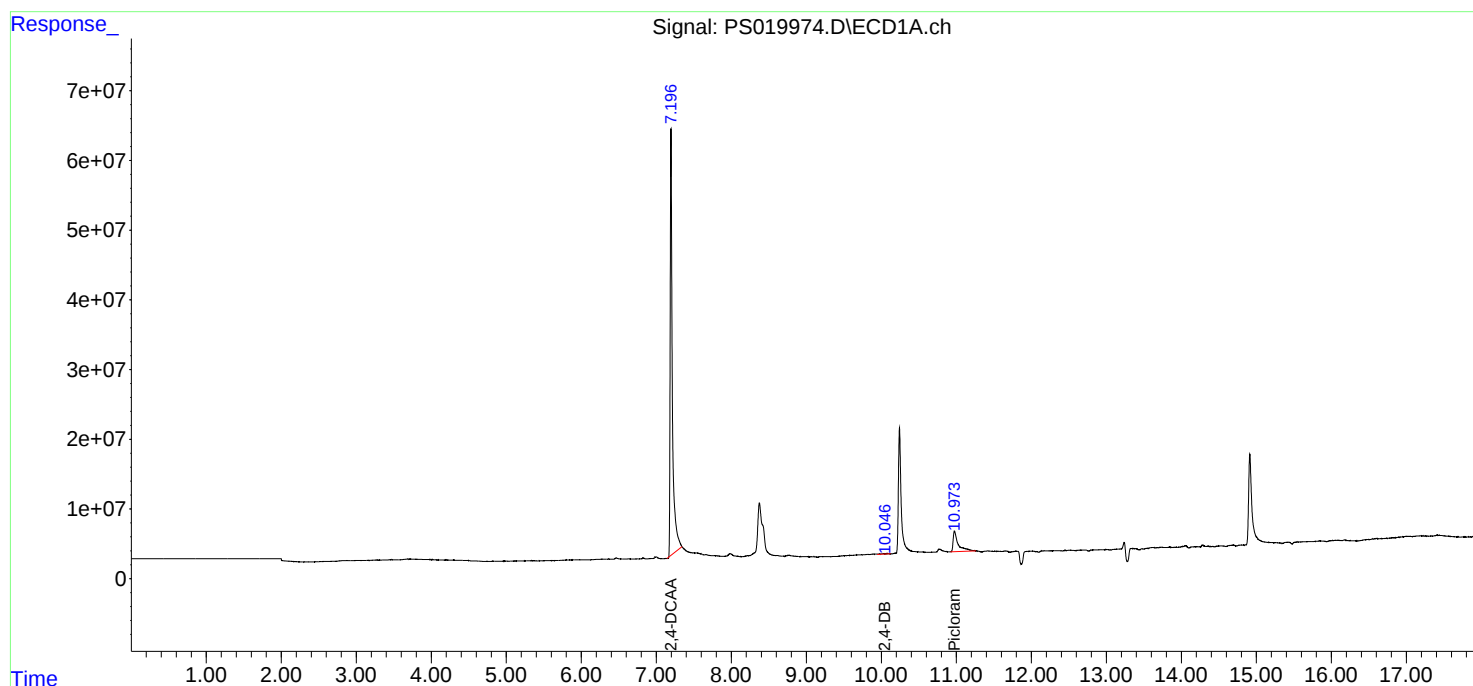


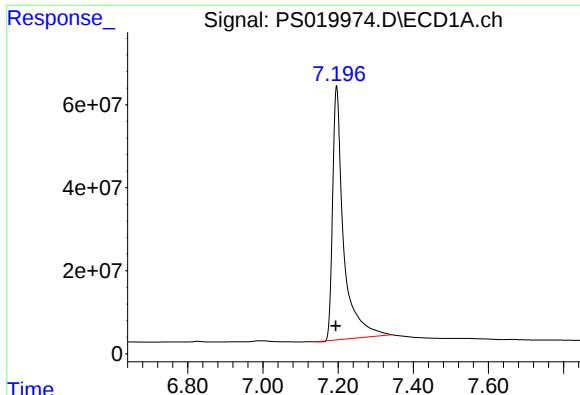

#4 2,4-DCAA


R.T.: 7.196 min
Delta R.T.: 0.002 min
Response: 1239411544
Conc: 477.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

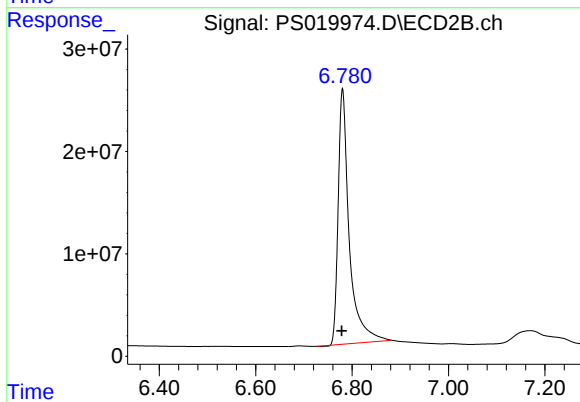


#4 2,4-DCAA

R.T.: 6.780 min
Delta R.T.: 0.002 min
Response: 396765821
Conc: 488.54 ng/ml

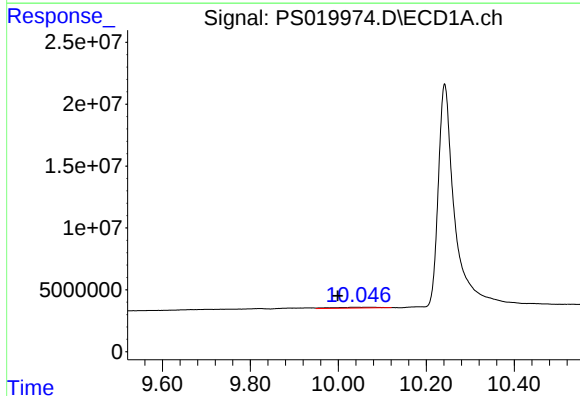


#13 2,4-DB

R.T.: 10.034 min
Delta R.T.: 0.035 min
Response: 4263591
Conc: 1.07 ng/ml

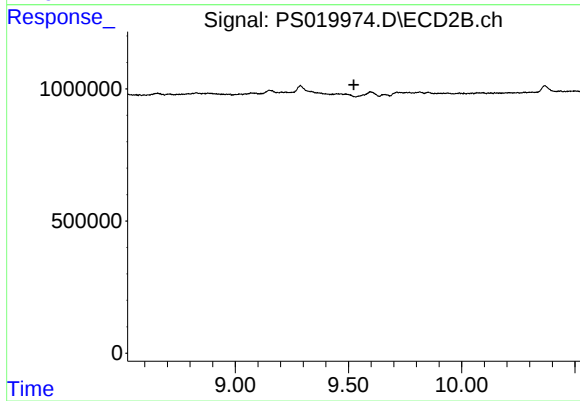

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.524 min
Response: 0
Conc: N.D.

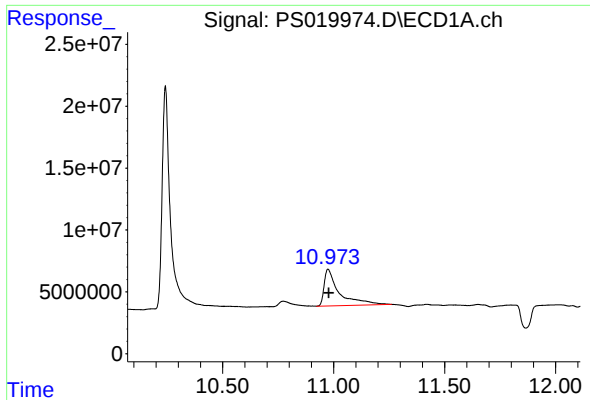

#15 Picloram

R.T.: 10.974 min
Delta R.T.: -0.004 min
Response: 140913472
Conc: 4.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

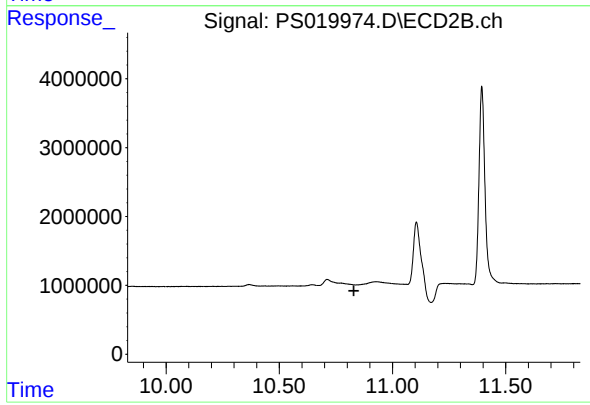

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.829 min
Response: 0
Conc: N.D.