

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071522\
 Data File : PS019986.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2022 20:25
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 01:40:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 27 17:26:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.193	6.779	1319.1E6	430.1E6	508.576	529.631
Target Compounds							
1) T	Dalapon	3.046	0.000	925657	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.458f	0.000	6975664	0	2.036	N.D. #
5) T	DICAMBA	0.000	7.005f	0	938631	N.D.	<MDL
6) T	MCP	0.000	7.005	0	938631	N.D.	<MDL
7) T	MCPA	7.718	0.000	1518480	0	<MDL	N.D. #
9) T	2,4-D	0.000	7.840	0	135621	N.D.	<MDL
10) T	Pentachlo...	8.609	8.280	-327943	1678648	N.D.	<MDL
11) T	2,4,5-TP ...	9.114f	8.614	9055114	379229	<MDL	<MDL #
12) T	2,4,5-T	0.000	9.055	0	253031	N.D.	<MDL
13) T	2,4-DB	0.000	9.467f	0	1360200	N.D.	2.094
14) T	DINOSEB	11.138	0.000	4227369	0	<MDL	N.D. #
15) T	Picloram	10.955	10.878f	136.7E6	2737362	4.385	<MDL #
16) T	DCPA	11.441	10.774	4036717	1081469	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071522\
Data File : PS019986.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2022 20:25
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 01:40:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
Quant Title : 8080.M
QLast Update : Mon Jun 27 17:26:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

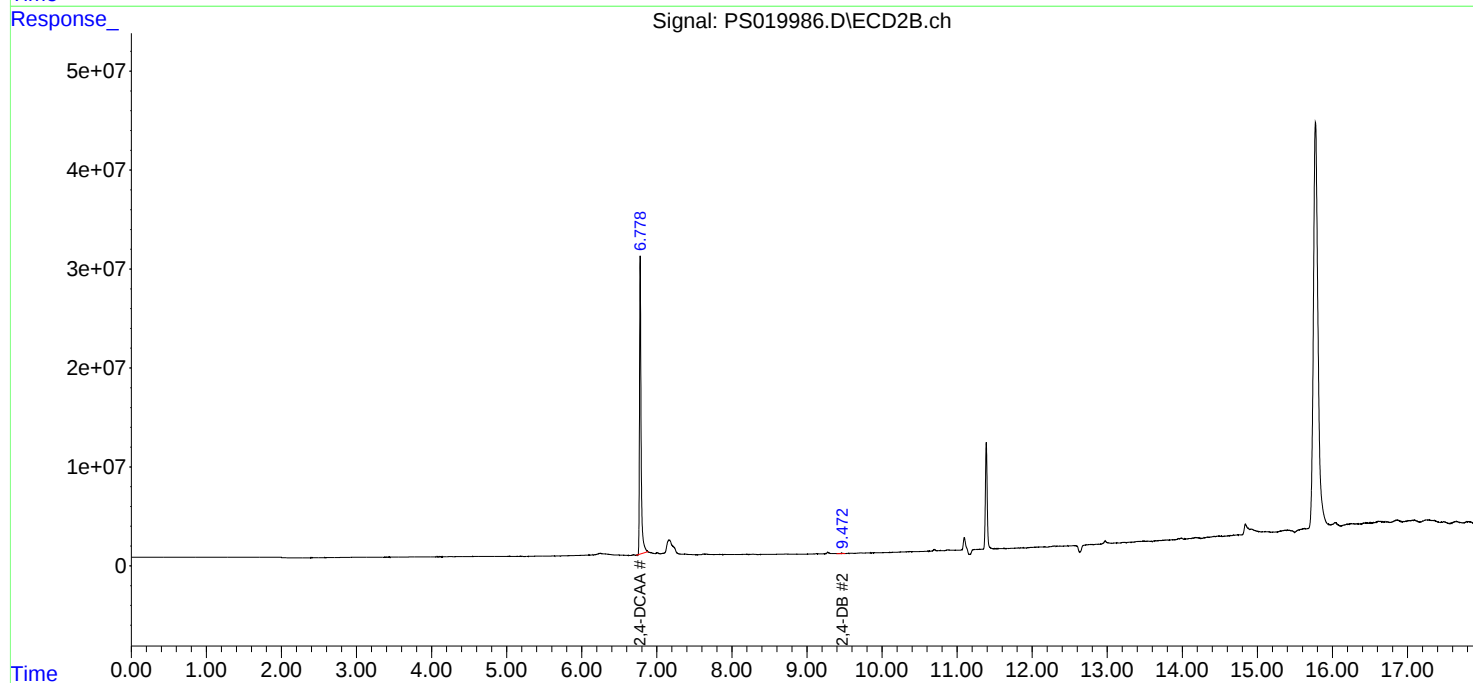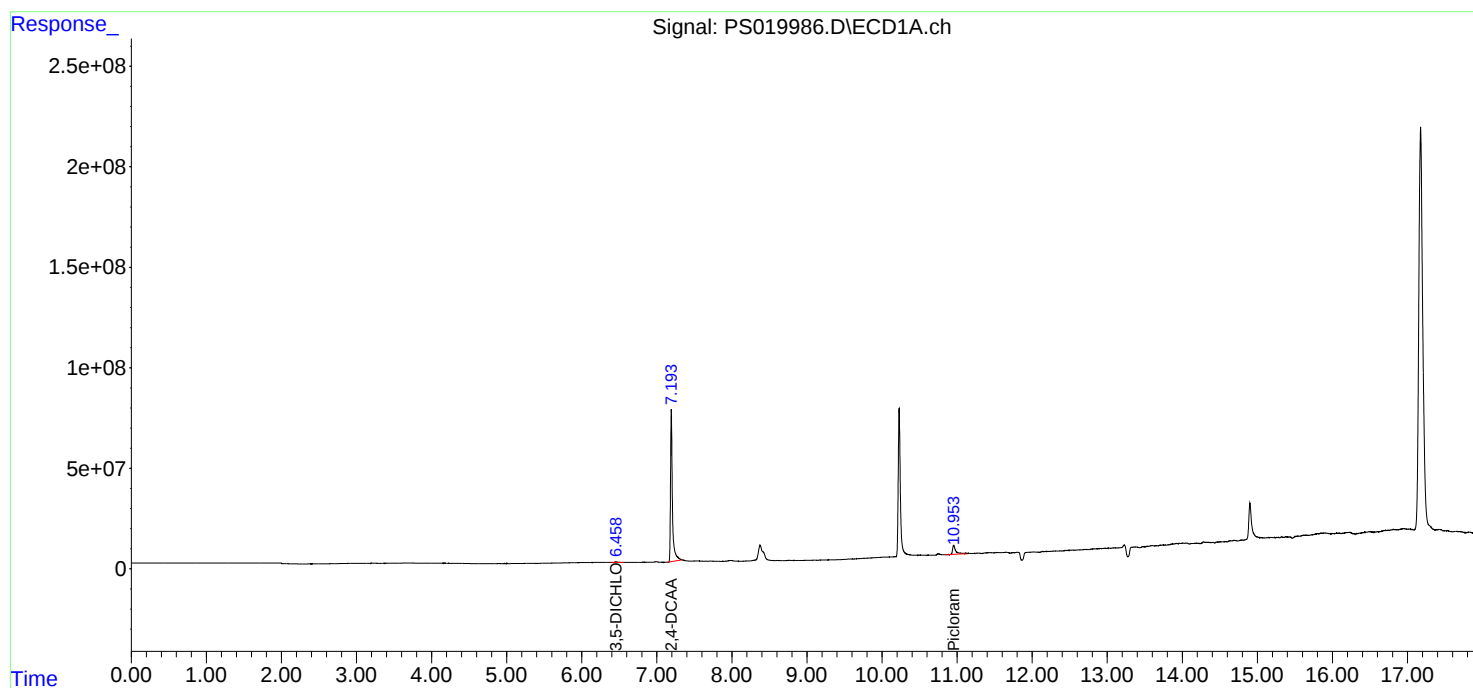


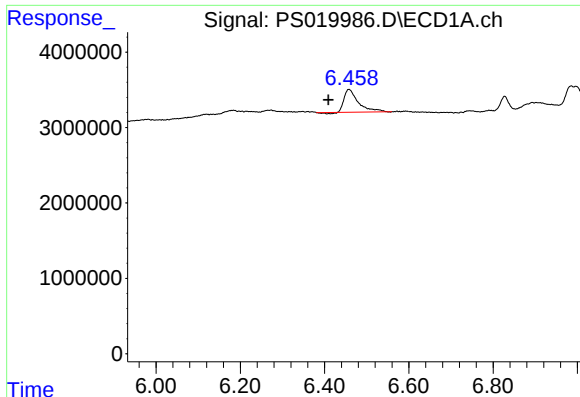

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.458 min
Delta R.T.: 0.049 min
Response: 6975664
Conc: 2.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

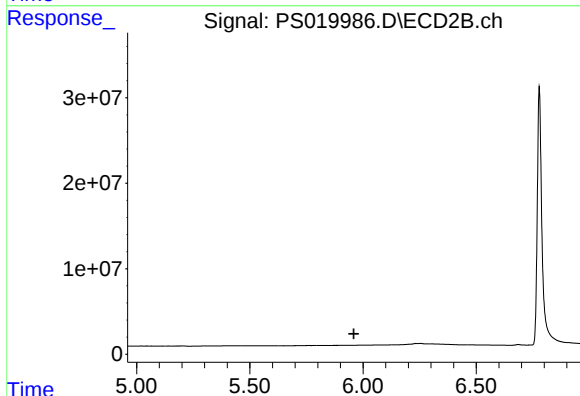


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.960 min
Response: 0
Conc: N.D.

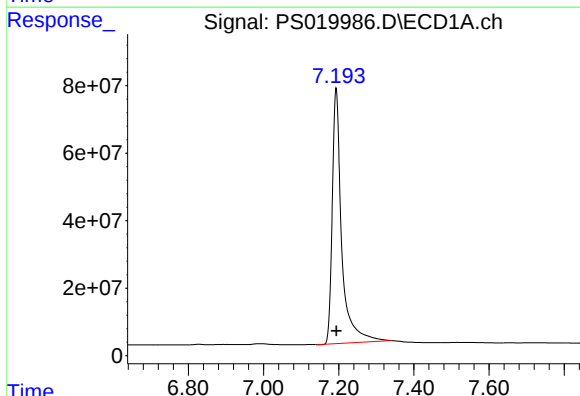


#4 2,4-DCAA

R.T.: 7.193 min
Delta R.T.: 0.000 min
Response: 1319068298
Conc: 508.58 ng/ml

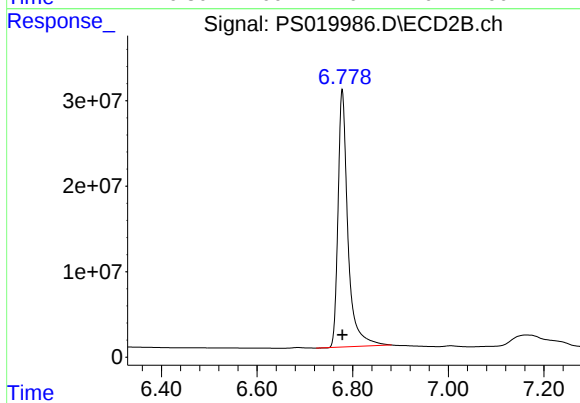

#4 2,4-DCAA


R.T.: 6.779 min
Delta R.T.: 0.000 min
Response: 430137835
Conc: 529.63 ng/ml

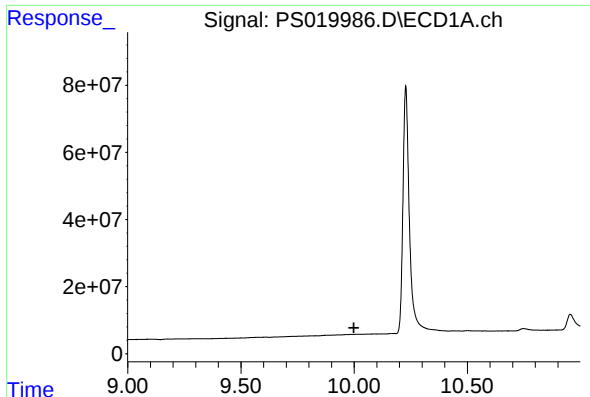

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.999 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

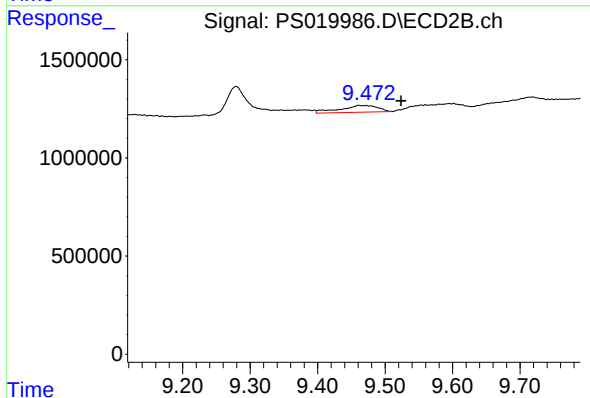


#13 2,4-DB

R.T.: 9.467 min
Delta R.T.: -0.056 min
Response: 1360200
Conc: 2.09 ng/ml

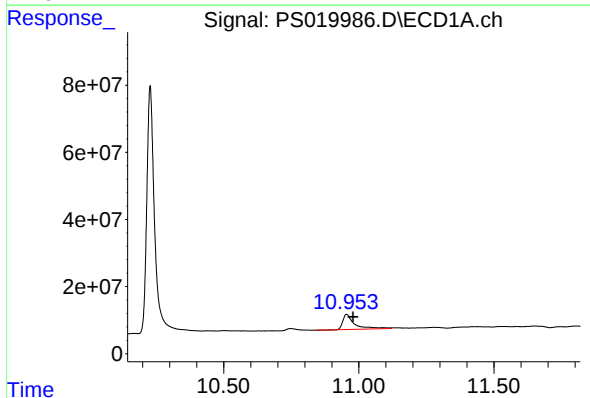

#15 Picloram

R.T.: 10.955 min
Delta R.T.: -0.023 min
Response: 136734663
Conc: 4.38 ng/ml

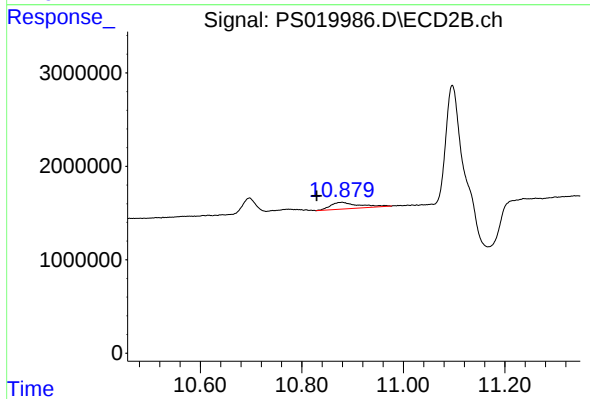

#15 Picloram

R.T.: 10.878 min
Delta R.T.: 0.049 min
Response: 2737362
Conc: N.D.