

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071522\
 Data File : PS019998.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2022 03:19
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 04:30:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 27 17:26:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.194	6.778	1454.5E6	444.1E6	560.792	546.835
Target Compounds							
1) T	Dalapon	3.052f	0.000	1136416	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.370	0.000	564263	0	<MDL	N.D. #
3) T	4-Nitroph...	6.985f	0.000	2873355	0	2.700	N.D. #
5) T	DICAMBA	0.000	7.005f	0	668176	N.D.	<MDL
6) T	MCPD	0.000	7.005	0	668176	N.D.	<MDL
7) T	MCPA	7.717	0.000	3702730	0	<MDL	N.D. #
9) T	2,4-D	0.000	7.851	0	475736	N.D.	<MDL
10) T	Pentachlo...	8.610	8.283	-272602	1361802	N.D.	<MDL
11) T	2,4,5-TP ...	9.111f	8.618	8566870	265766	<MDL	<MDL #
12) T	2,4,5-T	9.428	9.054	13087224	244760	<MDL	<MDL #
13) T	2,4-DB	0.000	9.466f	0	891174	N.D.	1.372
14) T	DINOSEB	0.000	9.855	0	202012	N.D.	<MDL
15) T	Picloram	10.955	10.878f	209.6E6	4647000	6.722	<MDL #
16) T	DCPA	11.415	10.771	2100028	975326	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071522\
Data File : PS019998.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2022 03:19
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 04:30:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
Quant Title : 8080.M
QLast Update : Mon Jun 27 17:26:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

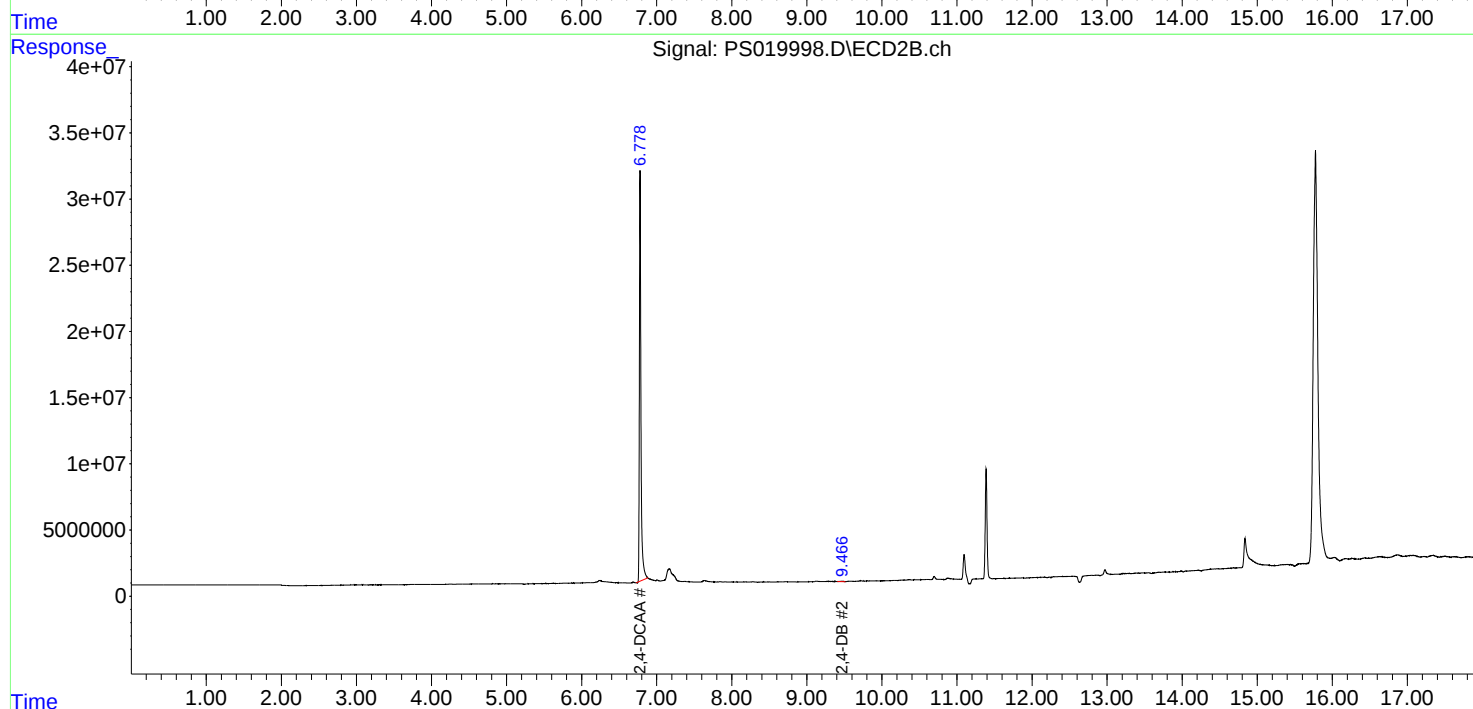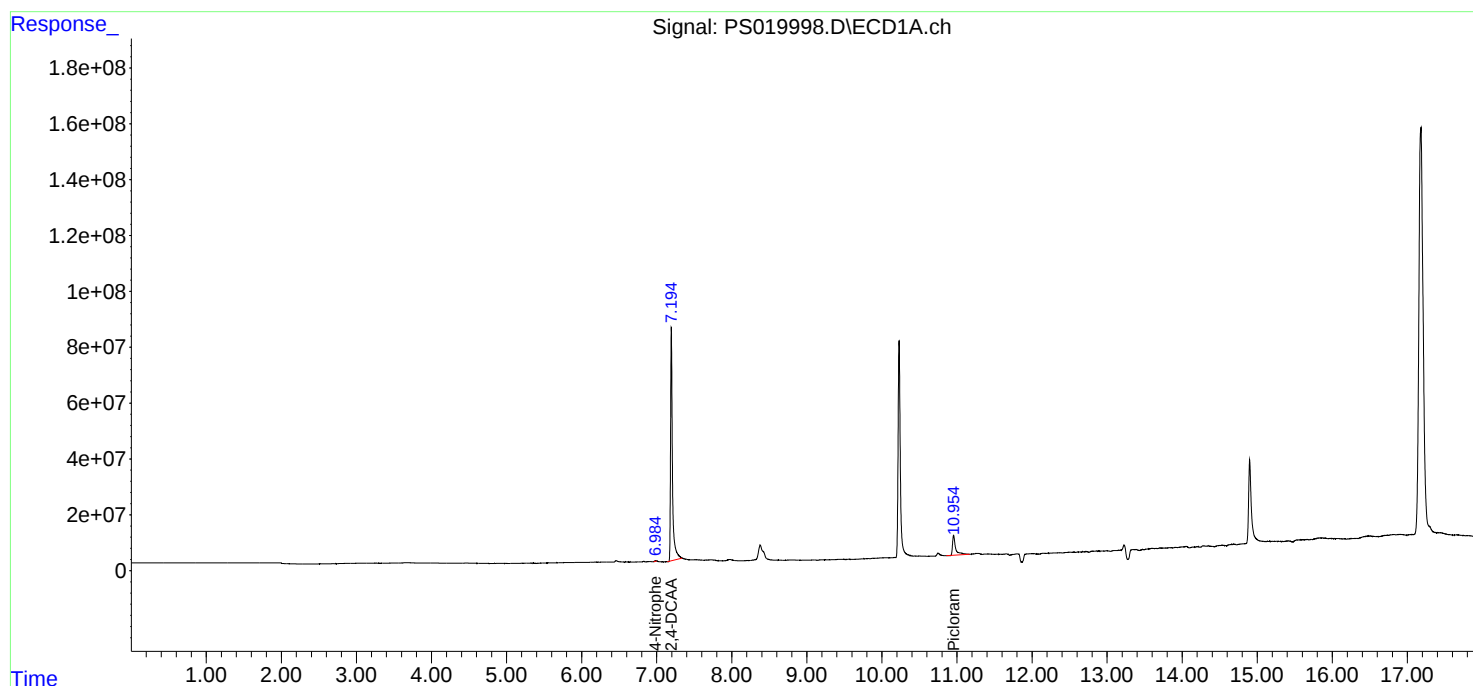


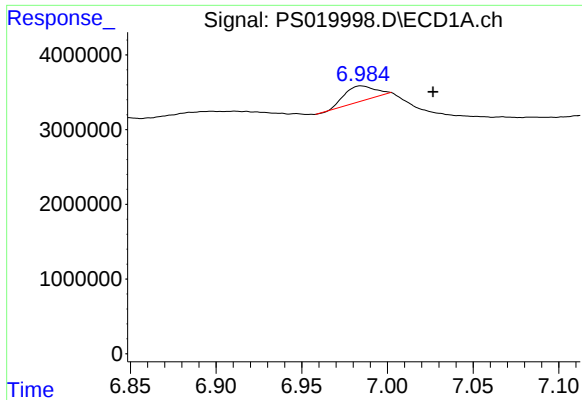

#3 4-Nitrophenol


R.T.: 6.985 min
Delta R.T.: -0.041 min
Response: 2873355
Conc: 2.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

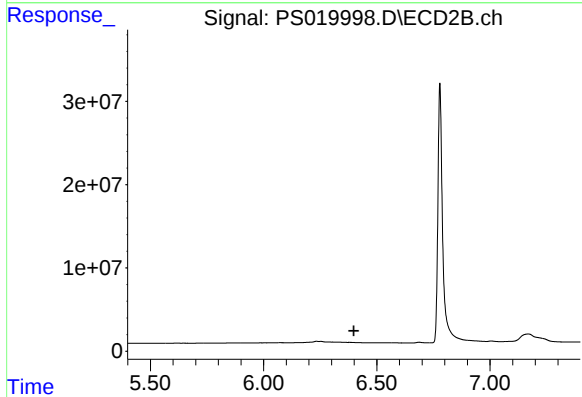


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

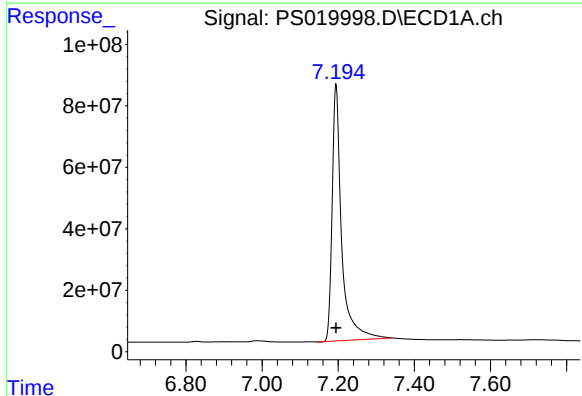


#4 2,4-DCAA

R.T.: 7.194 min
Delta R.T.: 0.000 min
Response: 1454498773
Conc: 560.79 ng/ml

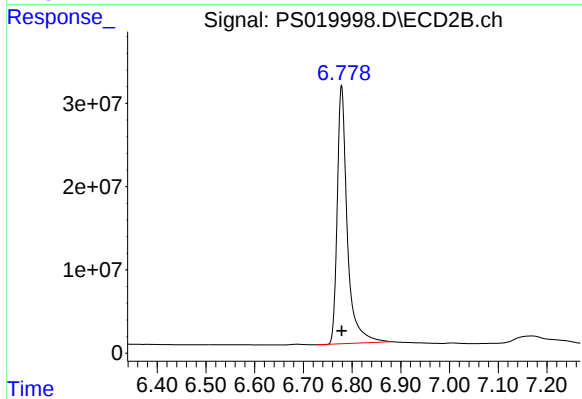

#4 2,4-DCAA


R.T.: 6.778 min
Delta R.T.: 0.000 min
Response: 444110067
Conc: 546.84 ng/ml

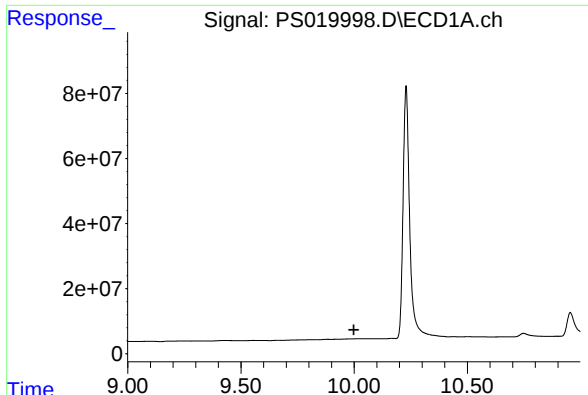

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.999 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

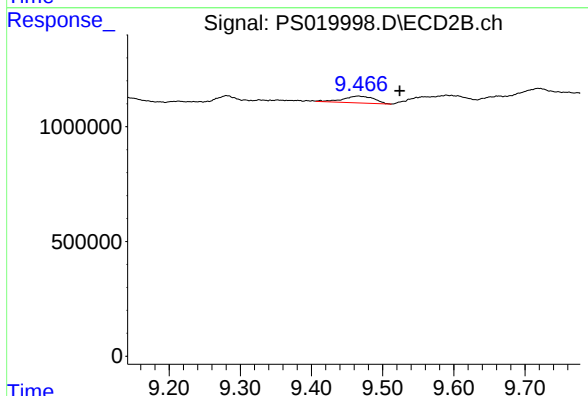


#13 2,4-DB

R.T.: 9.466 min
Delta R.T.: -0.058 min
Response: 891174
Conc: 1.37 ng/ml

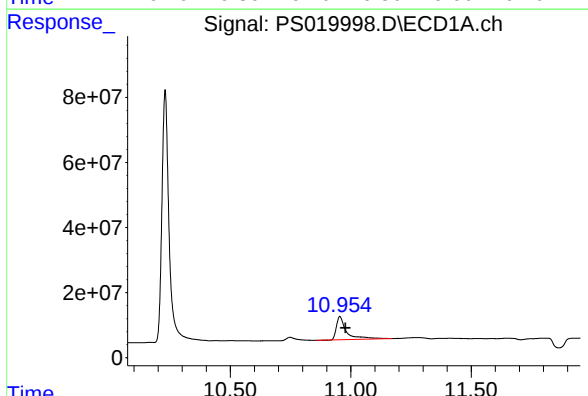

#15 Picloram

R.T.: 10.955 min
Delta R.T.: -0.023 min
Response: 209613787
Conc: 6.72 ng/ml

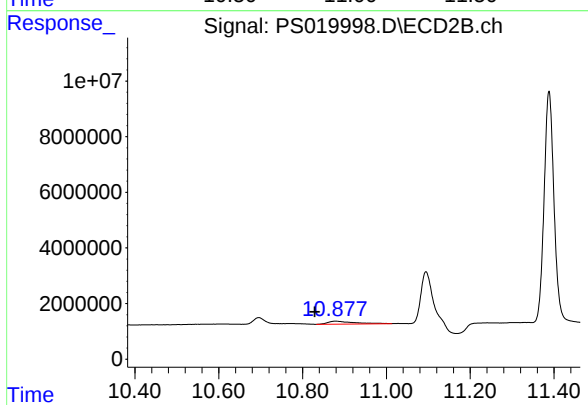

#15 Picloram

R.T.: 10.878 min
Delta R.T.: 0.049 min
Response: 4647000
Conc: N.D.