

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071522\
 Data File : PS020003.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2022 05:45
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 06:19:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 27 17:26:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.194	6.779	1469.6E6	449.9E6	566.613	554.015
Target Compounds							
1) T	Dalapon	3.018	0.000	1086295	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.372	5.913f	375794	349858	<MDL	<MDL #
3) T	4-Nitroph...	6.983f	6.384	4742782	1156350	4.456	2.674 #
5) T	DICAMBA	0.000	7.004f	0	1821336	N.D.	<MDL
6) T	MCP	0.000	7.004	0	1821336	N.D.	<MDL
7) T	MCPA	7.716	0.000	9619739	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.629f	0	4969329	N.D.	5.282
9) T	2,4-D	0.000	7.832	0	771202	N.D.	<MDL
10) T	Pentachlo...	8.610	8.281	1768293	1695260	<MDL	<MDL #
11) T	2,4,5-TP ...	9.175	8.614	3582233	487850	<MDL	<MDL #
12) T	2,4,5-T	9.431	9.052	17600156	372657	<MDL	<MDL #
13) T	2,4-DB	10.012	9.465f	7840314	1710852	1.959	2.634 #
14) T	DINOSEB	0.000	9.851	0	785653	N.D.	<MDL
15) T	Picloram	10.950	10.877f	285.2E6	8172347	9.146	1.257 #
16) T	DCPA	11.416	10.770	2321362	1745166	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071522\
Data File : PS020003.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2022 05:45
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 06:19:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
Quant Title : 8080.M
QLast Update : Mon Jun 27 17:26:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

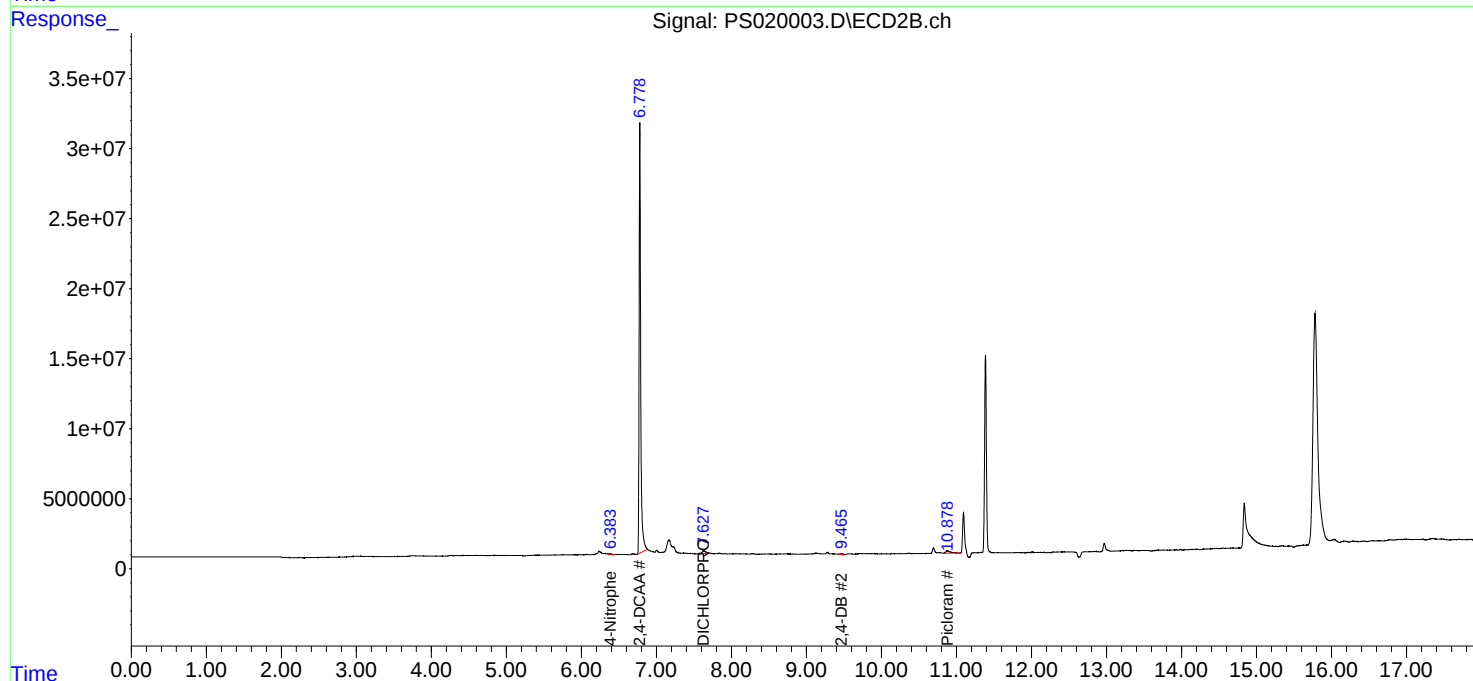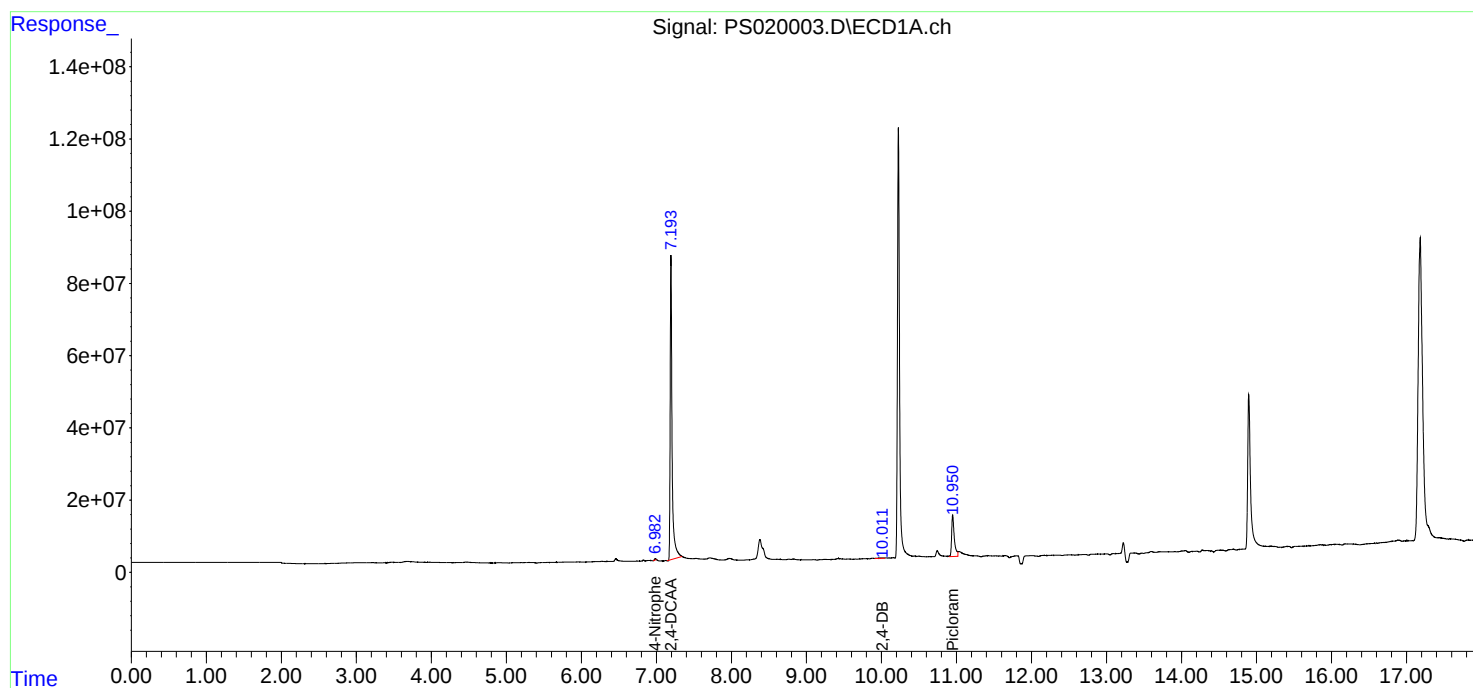


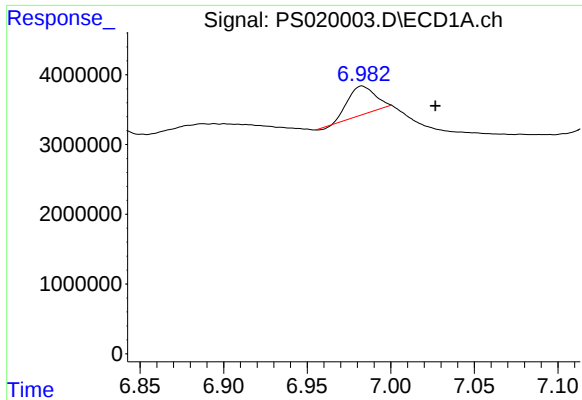

#3 4-Nitrophenol


R.T.: 6.983 min
Delta R.T.: -0.043 min
Response: 4742782
Conc: 4.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

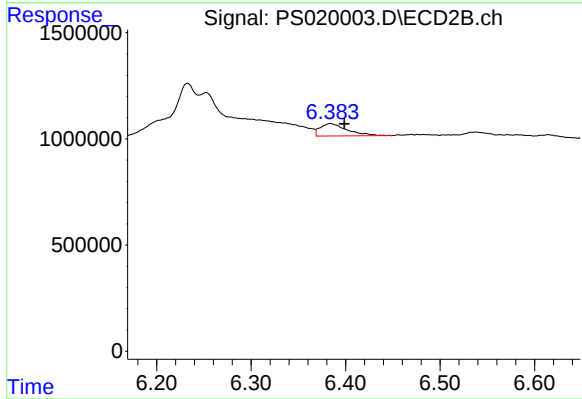


#3 4-Nitrophenol

R.T.: 6.384 min
Delta R.T.: -0.014 min
Response: 1156350
Conc: 2.67 ng/ml

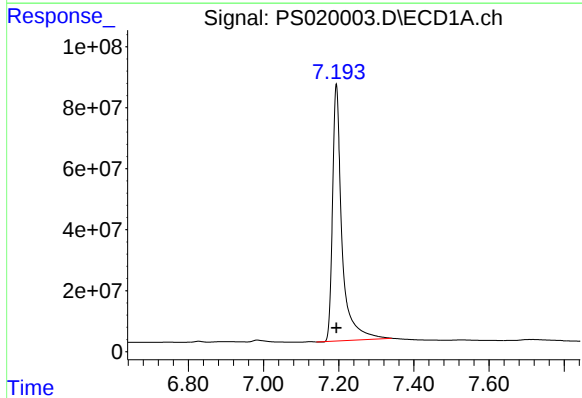


#4 2,4-DCAA

R.T.: 7.194 min
Delta R.T.: 0.000 min
Response: 1469597324
Conc: 566.61 ng/ml

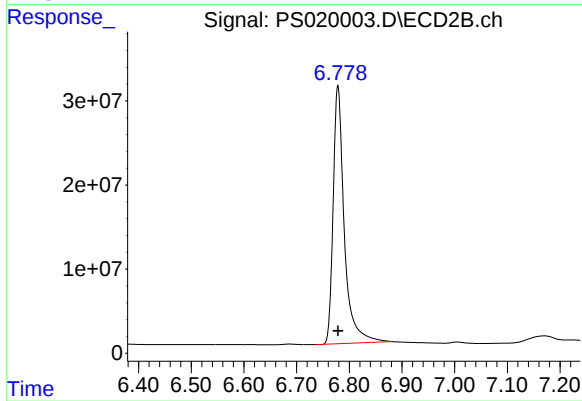

#4 2,4-DCAA


R.T.: 6.779 min
Delta R.T.: 0.000 min
Response: 449941416
Conc: 554.02 ng/ml

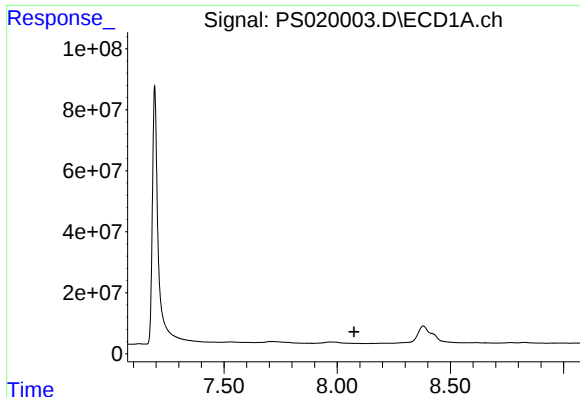

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.074 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

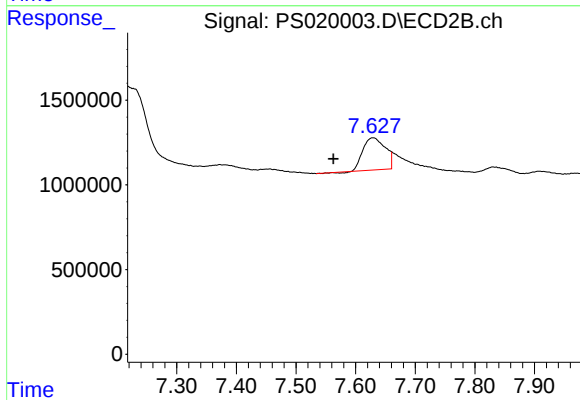


#8 DICHLORPROP

R.T.: 7.629 min
Delta R.T.: 0.066 min
Response: 4969329
Conc: 5.28 ng/ml

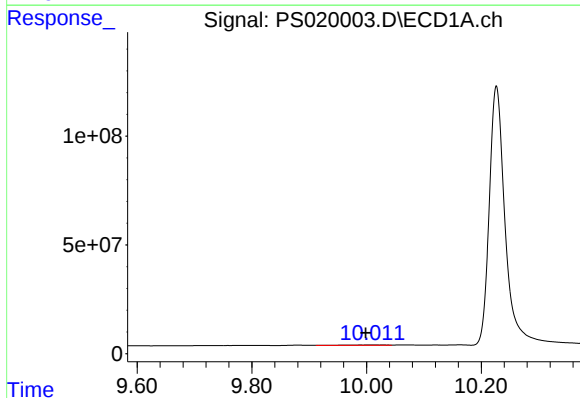


#13 2,4-DB

R.T.: 10.012 min
Delta R.T.: 0.014 min
Response: 7840314
Conc: 1.96 ng/ml

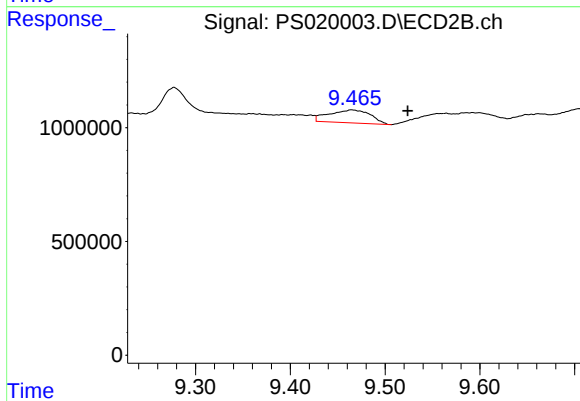

#13 2,4-DB


R.T.: 9.465 min
Delta R.T.: -0.059 min
Response: 1710852
Conc: 2.63 ng/ml

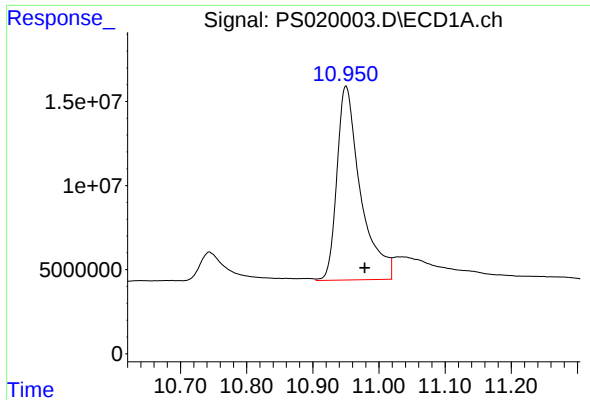

#15 Picloram

R.T.: 10.950 min
Delta R.T.: -0.028 min
Response: 285207414
Conc: 9.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

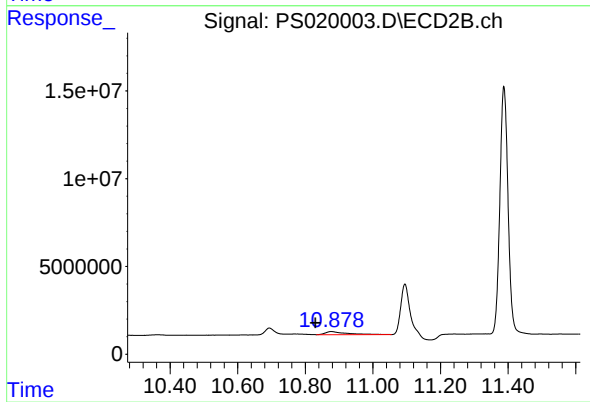

#15 Picloram

R.T.: 10.877 min
Delta R.T.: 0.048 min
Response: 8172347
Conc: 1.26 ng/ml