Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071525\
Data File : PS031048.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2025 01:36
Operator : AR\AJ
Sample : PB168825BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB168825BL

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 07/16/2025
Supervised By :mohammad ahmed 07/18/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 02:52:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071125.M
Quant Title : 8080.M
QLast Update : Mon Jul 14 05:51:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
	System Monitoring Compounds						
4) S	2,4-DCAA	7.330	7.767	1448.4E6	457.6E6	366.224	441.707m
	Target Compounds						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071525\
Data File : PS031048.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2025 01:36
Operator : AR\AJ
Sample : PB168825BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB168825BL

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 07/16/2025
Supervised By :mohammad ahmed 07/18/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 02:52:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071125.M
Quant Title : 8080.M
QLast Update : Mon Jul 14 05:51:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

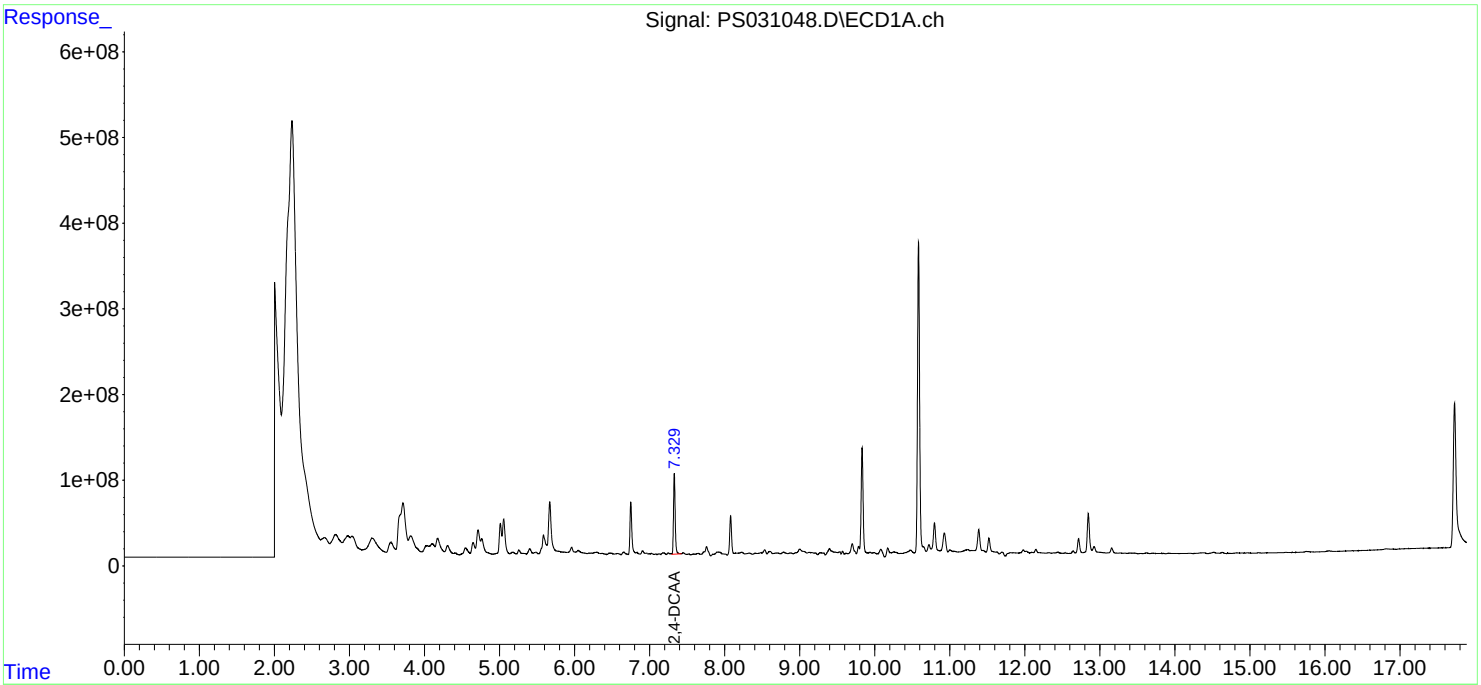

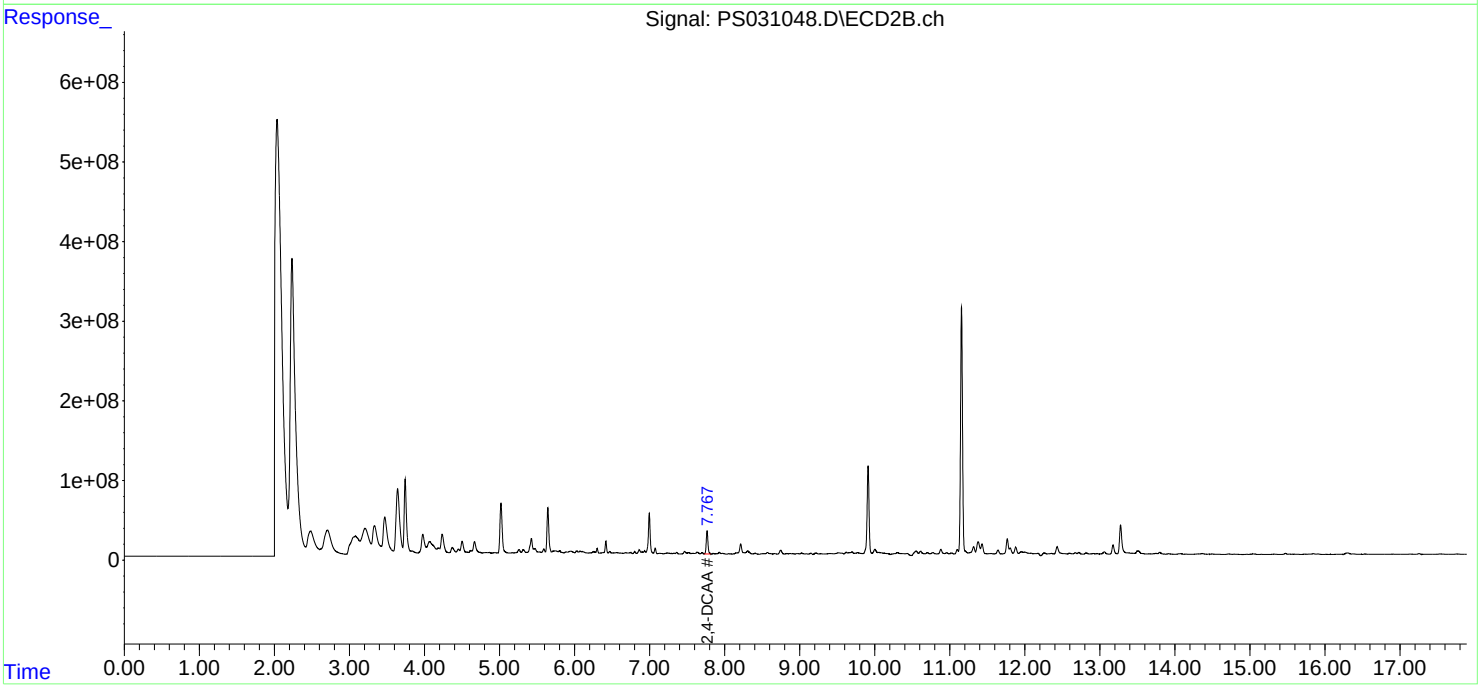

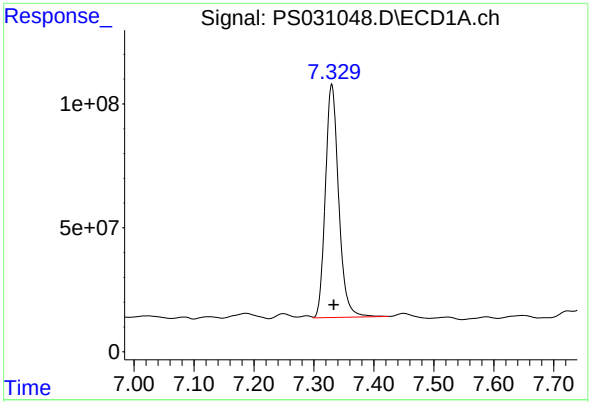

#4 2,4-DCAA

R.T.: 7.330 min
Delta R.T.: -0.003 min
Response: 1448444218
Conc: 366.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB168825BL

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 07/16/2025
Supervised By :mohammad ahmed 07/18/2025

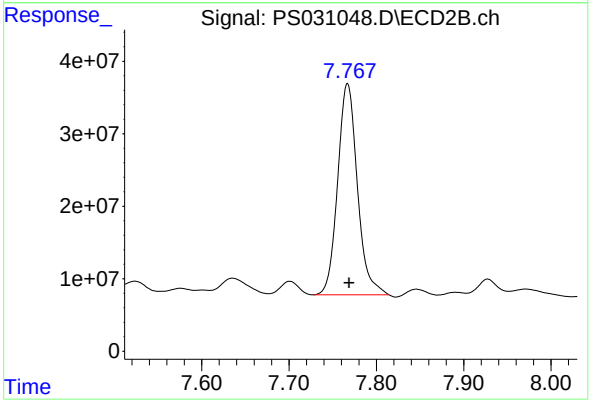

#4 2,4-DCAA

R.T.: 7.767 min
Delta R.T.: -0.002 min
Response: 457623178
Conc: 441.71 ng/ml m