

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071618\
 Data File : PS001048.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2018 13:05
 Operator : UA
 Sample : J3947-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 15:51:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.632	11.045	94785984	84104500	459.412	386.160
Target Compounds							
1) T	Dalapon	0.000	2.438	0	820162	N.D.	3.044 #
2) T	3,5-DICHL...	0.000	9.282	0	35163210	N.D.	119.540 #
6) T	MCP	12.325	0.000	7091022	0	12.909	N.D. #
12) T	2,4,5-T	0.000	14.705	0	1796192	N.D.	1.736 #
15) T	Picloram	17.165	16.987	4459545	8449155	2.462	5.549 #
16) T	DCPA	0.000	16.987	0	8449155	N.D.	4.915 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071618\
Data File : PS001048.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2018 13:05
Operator : UA
Sample : J3947-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 15:51:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

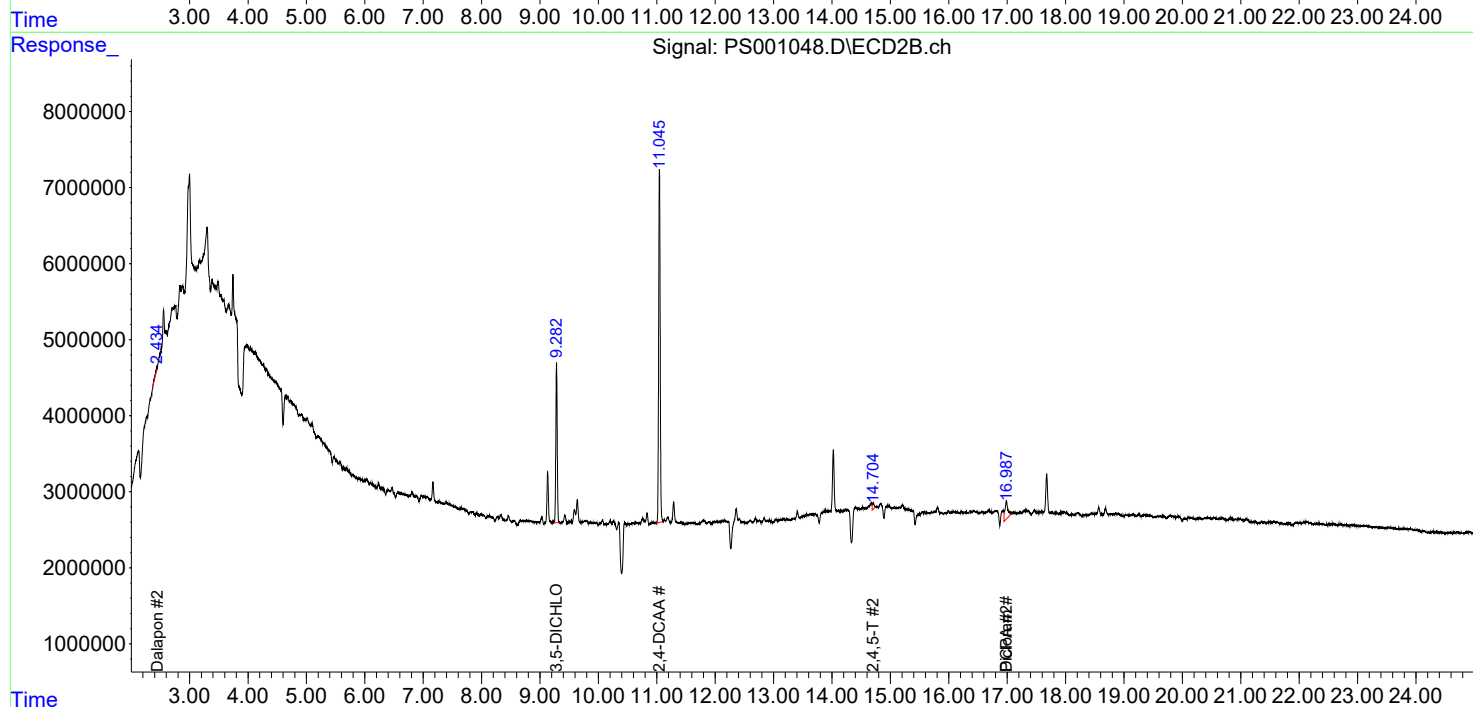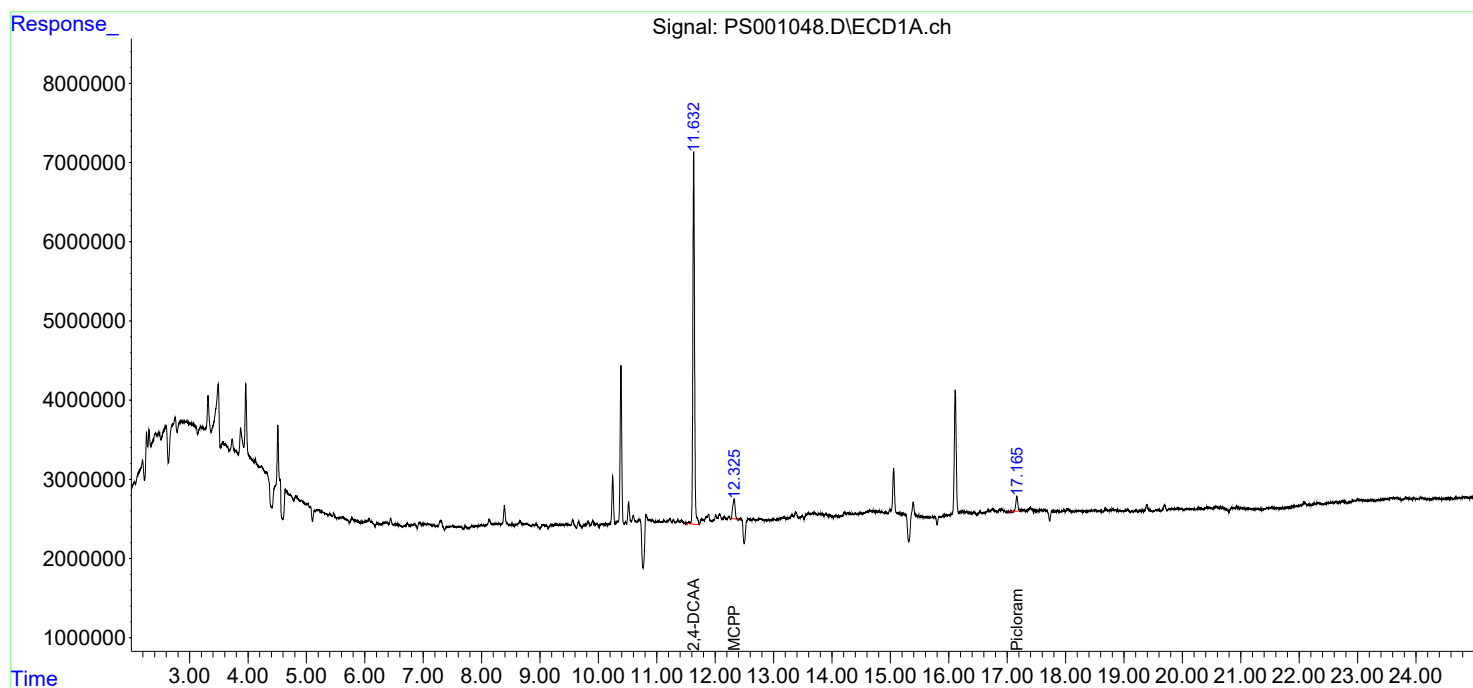


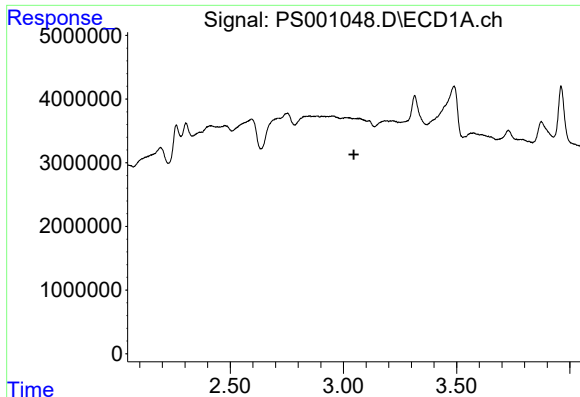

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.046 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

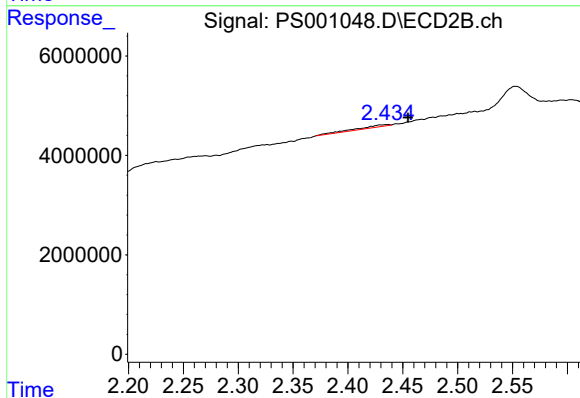


#1 Dalapon

R.T.: 2.438 min
Delta R.T.: -0.017 min
Response: 820162
Conc: 3.04 ng/ml

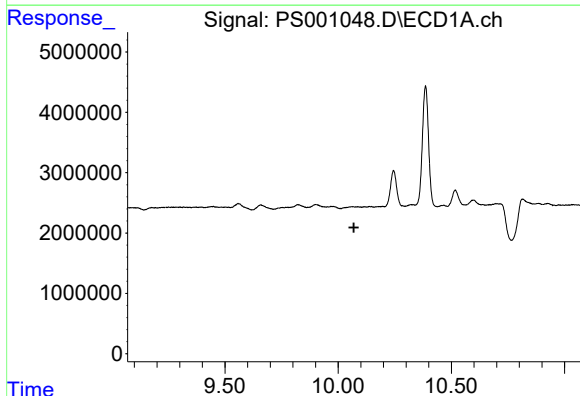


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 10.070 min
Response: 0
Conc: N.D.

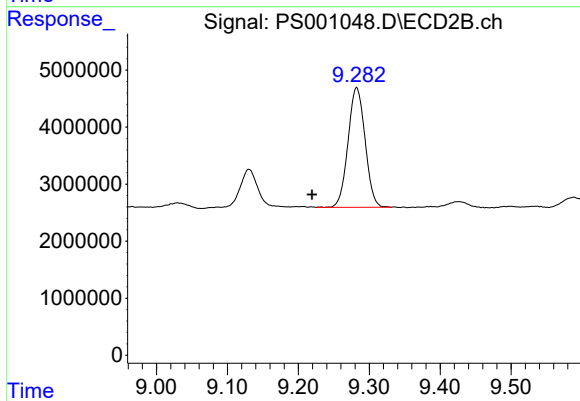

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.282 min
Delta R.T.: 0.063 min
Response: 35163210
Conc: 119.54 ng/ml

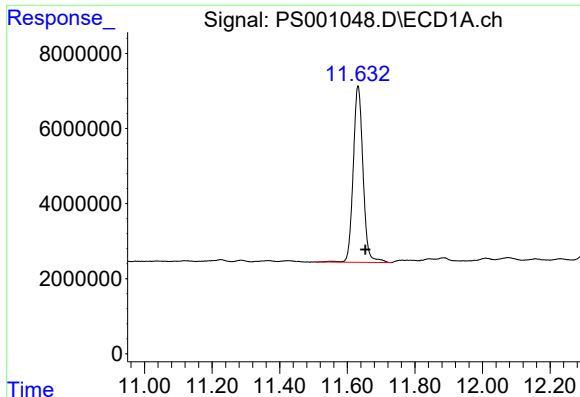

#4 2,4-DCAA


R.T.: 11.632 min
Delta R.T.: -0.021 min
Response: 94785984
Conc: 459.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

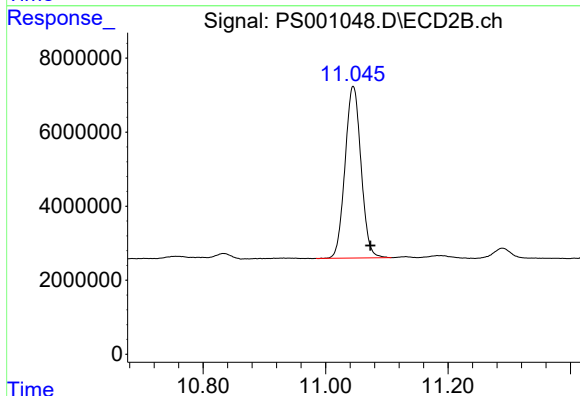


#4 2,4-DCAA

R.T.: 11.045 min
Delta R.T.: -0.028 min
Response: 84104500
Conc: 386.16 ng/ml

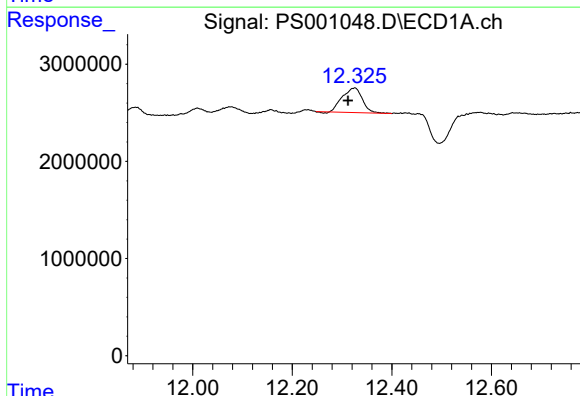


#6 MCP

R.T.: 12.325 min
Delta R.T.: 0.013 min
Response: 7091022
Conc: 12.91 ug/ml

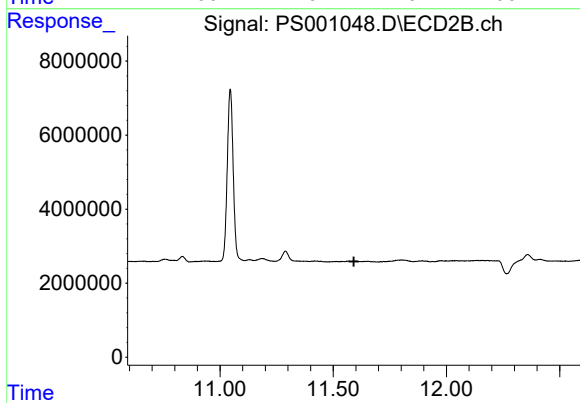

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

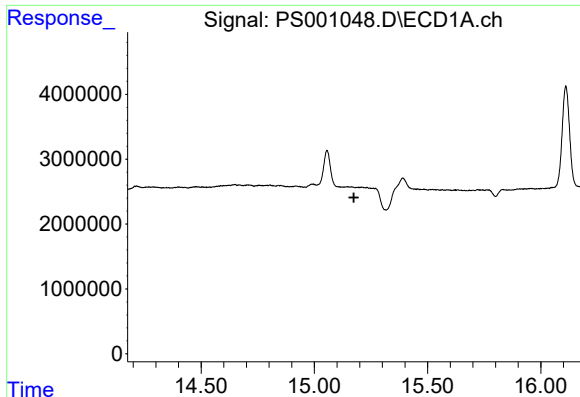

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.174 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

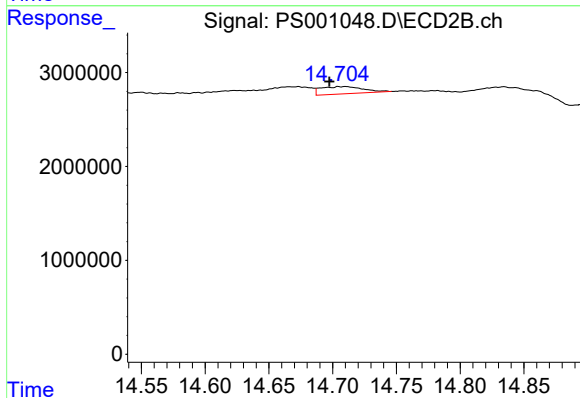


#12 2,4,5-T

R.T.: 14.705 min
Delta R.T.: 0.007 min
Response: 1796192
Conc: 1.74 ng/ml

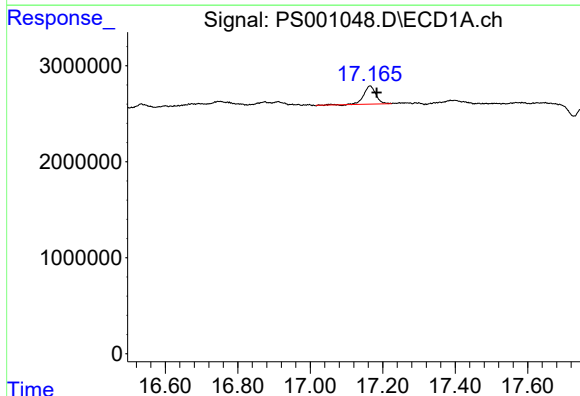


#15 Picloram

R.T.: 17.165 min
Delta R.T.: -0.019 min
Response: 4459545
Conc: 2.46 ng/ml

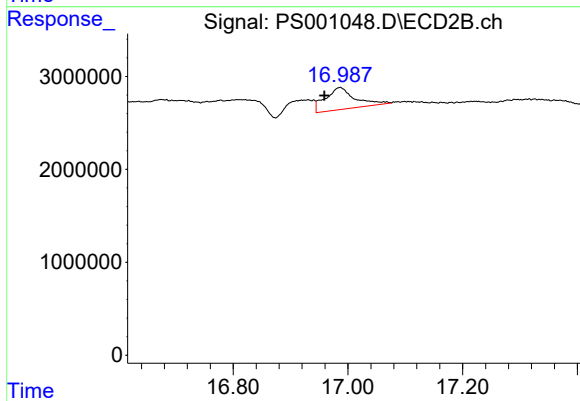

#15 Picloram


R.T.: 16.987 min
Delta R.T.: 0.028 min
Response: 8449155
Conc: 5.55 ng/ml

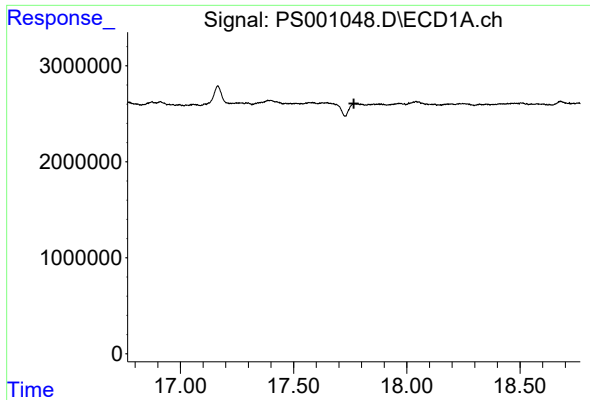

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.766 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

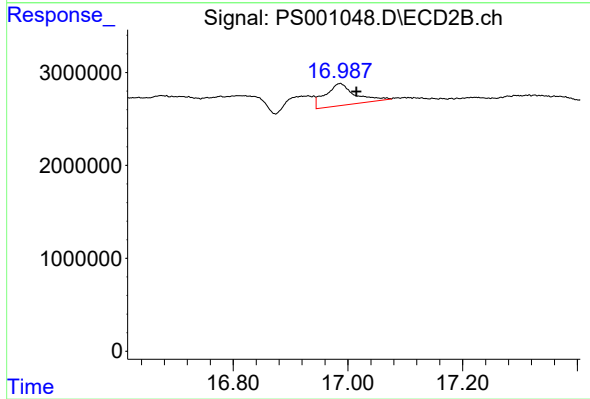

#16 DCPA

R.T.: 16.987 min
Delta R.T.: -0.028 min
Response: 8449155
Conc: 4.91 ng/ml