

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071618\
 Data File : PS001049.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2018 13:37
 Operator : UA
 Sample : J3947-04RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 15:51:24 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.648	11.060	69934262	58953700	338.960	270.682
Target Compounds							
5) T	DICAMBA	12.025	11.304	2013338	6928166	2.557	8.826 #
6) T	MCPP	12.341	0.000	8813279	0	16.045	N.D. #
8) T	DICHLORPROP	0.000	12.428	0	1577670	N.D.	7.811 #
15) T	Picloram	0.000	16.928	0	4605595	N.D.	3.025 #
16) T	DCPA	0.000	17.001	0	3342214	N.D.	1.944 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071618\
Data File : PS001049.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2018 13:37
Operator : UA
Sample : J3947-04RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 15:51:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

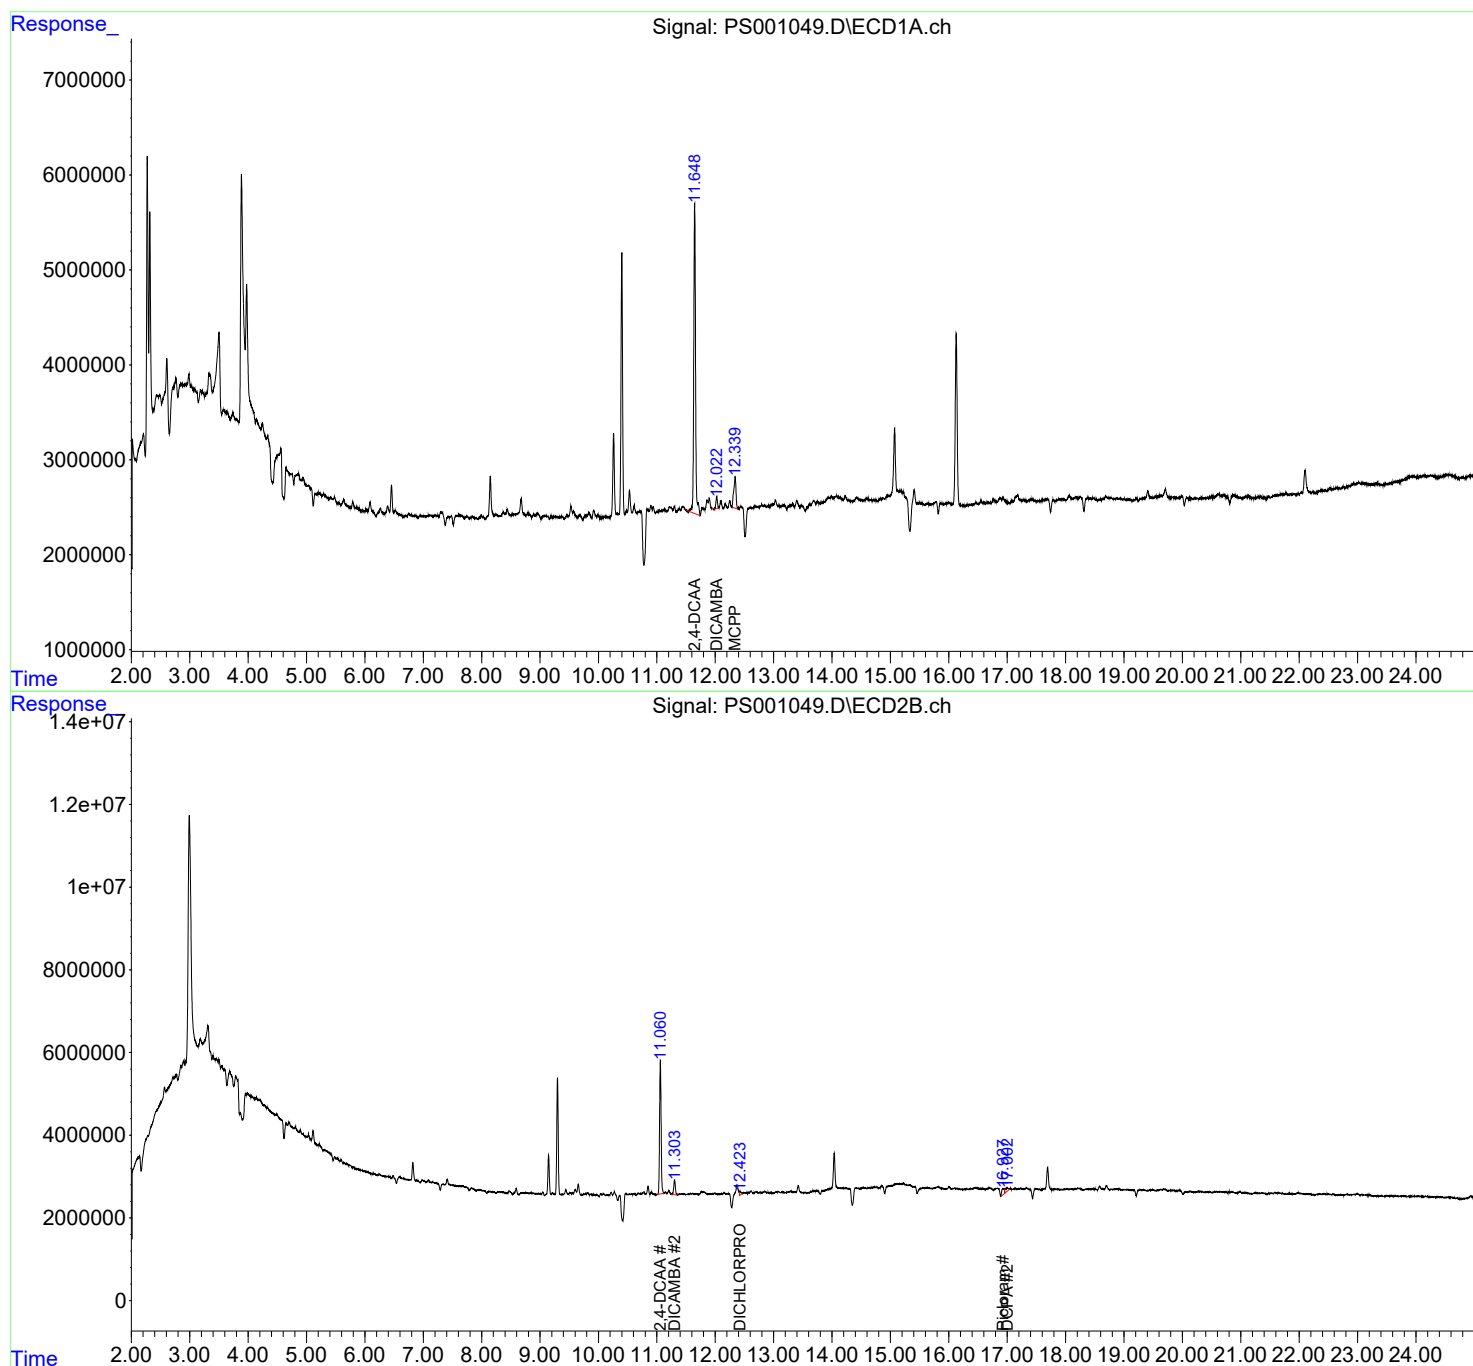


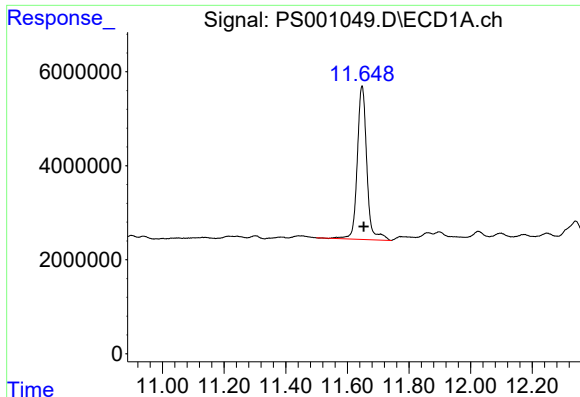

#4 2,4-DCAA


R.T.: 11.648 min
Delta R.T.: -0.006 min
Response: 69934262
Conc: 338.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

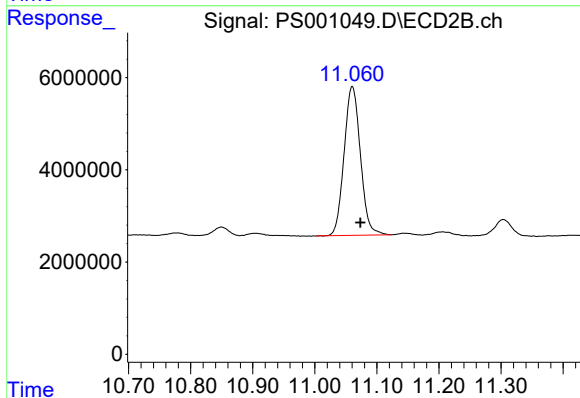


#4 2,4-DCAA

R.T.: 11.060 min
Delta R.T.: -0.013 min
Response: 58953700
Conc: 270.68 ng/ml

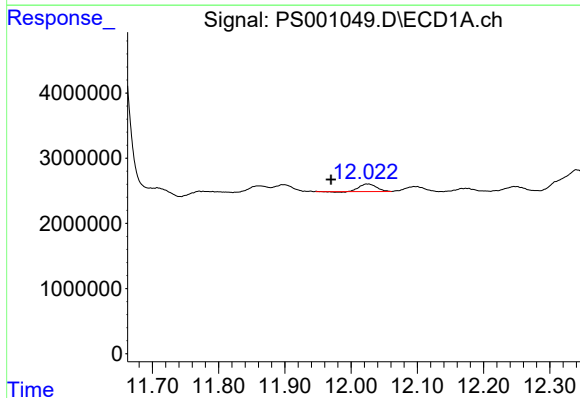


#5 DICAMBA

R.T.: 12.025 min
Delta R.T.: 0.055 min
Response: 2013338
Conc: 2.56 ng/ml

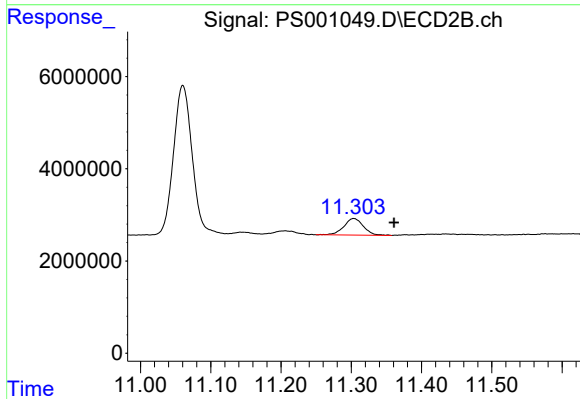

#5 DICAMBA


R.T.: 11.304 min
Delta R.T.: -0.058 min
Response: 6928166
Conc: 8.83 ng/ml

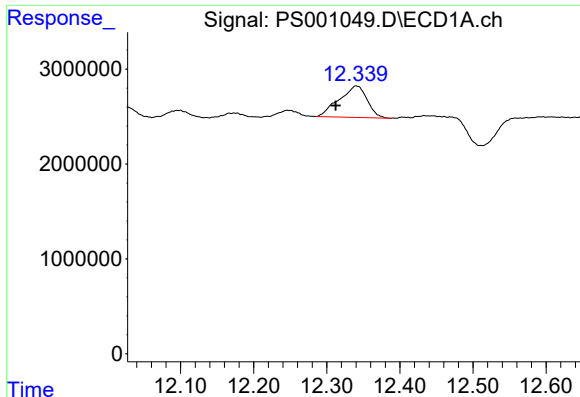

#6 MCP


R.T.: 12.341 min
Delta R.T.: 0.029 min
Response: 8813279
Conc: 16.04 ug/ml

Instrument :
ECD_S
ClientSampleId :

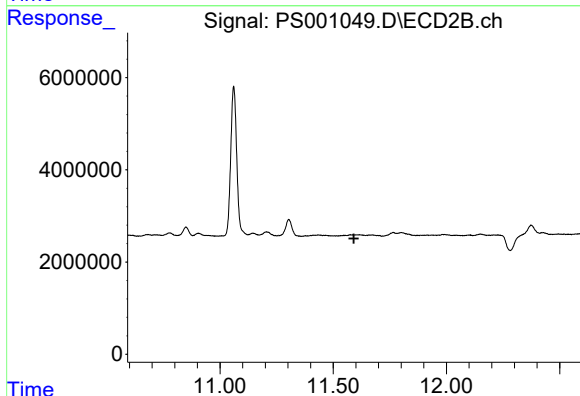


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

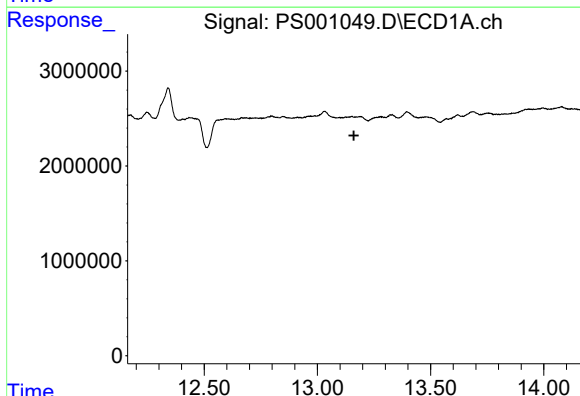


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

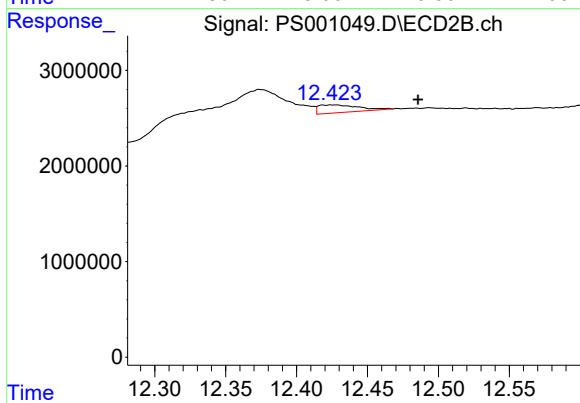

#8 DICHLORPROP


R.T.: 12.428 min
Delta R.T.: -0.058 min
Response: 1577670
Conc: 7.81 ng/ml

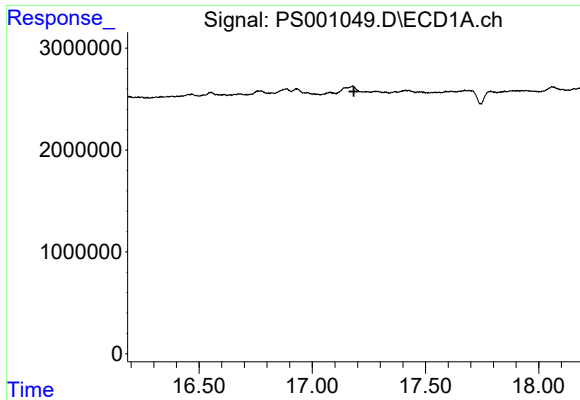

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

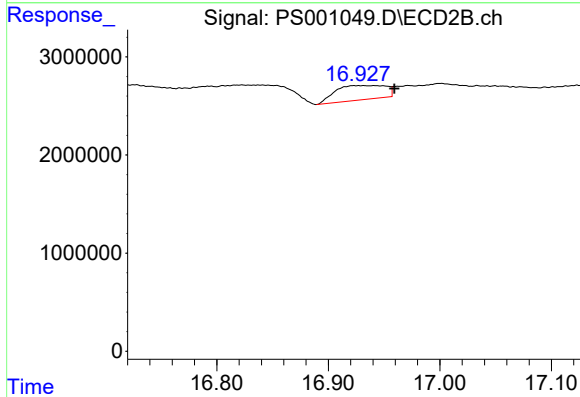


#15 Picloram

R.T.: 16.928 min
Delta R.T.: -0.032 min
Response: 4605595
Conc: 3.02 ng/ml

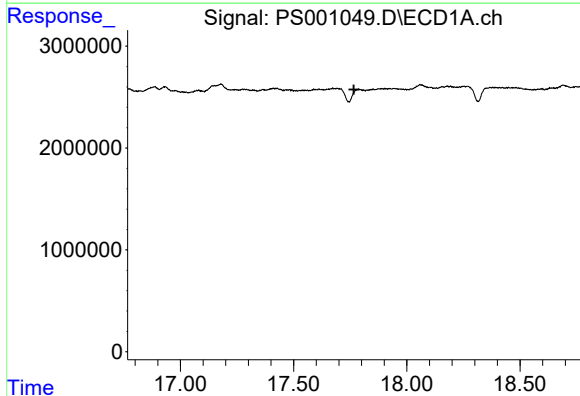

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.766 min
Response: 0
Conc: N.D.

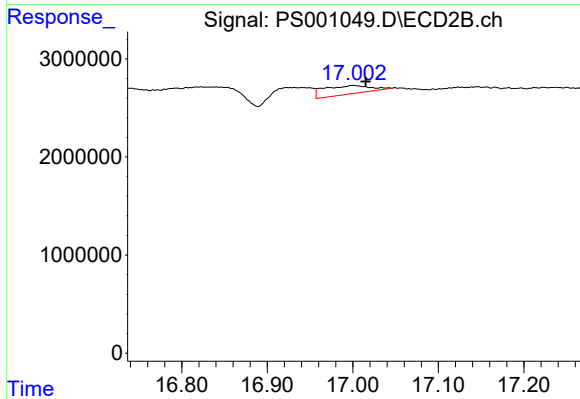

#16 DCPA

R.T.: 17.001 min
Delta R.T.: -0.014 min
Response: 3342214
Conc: 1.94 ng/ml