

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071618\
 Data File : PS001065.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2018 23:59
 Operator : UA
 Sample : J3958-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 00:49:17 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.665	11.079	27117048	19622733	131.432	90.096 #
Target Compounds							
2) T	3,5-DICHL...	0.000	9.231	0	2705403	N.D.	9.197 #
5) T	DICAMBA	0.000	11.322	0	5500691	N.D.	7.008 #
6) T	MCP	12.355	0.000	6324397	0	11.514	N.D. #
8) T	DICHLORPROP	0.000	12.485	0	1397345	N.D.	6.918 #
9) T	2,4-D	13.531	12.962	28394426	27806271	104.319	100.398
15) T	Picloram	17.198	17.020	9002187	9150724	4.971	6.010
16) T	DCPA	0.000	17.020	0	9150724	N.D.	5.323 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071618\
Data File : PS001065.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2018 23:59
Operator : UA
Sample : J3958-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 00:49:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

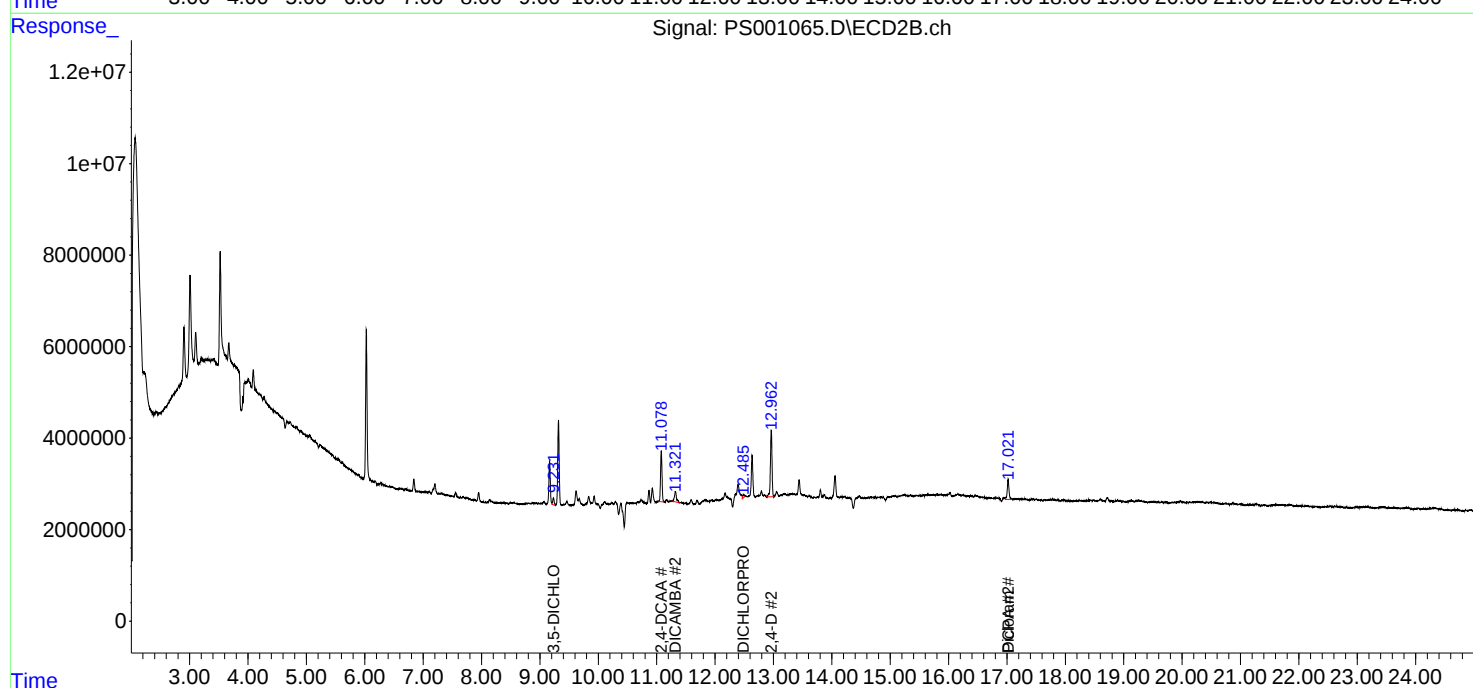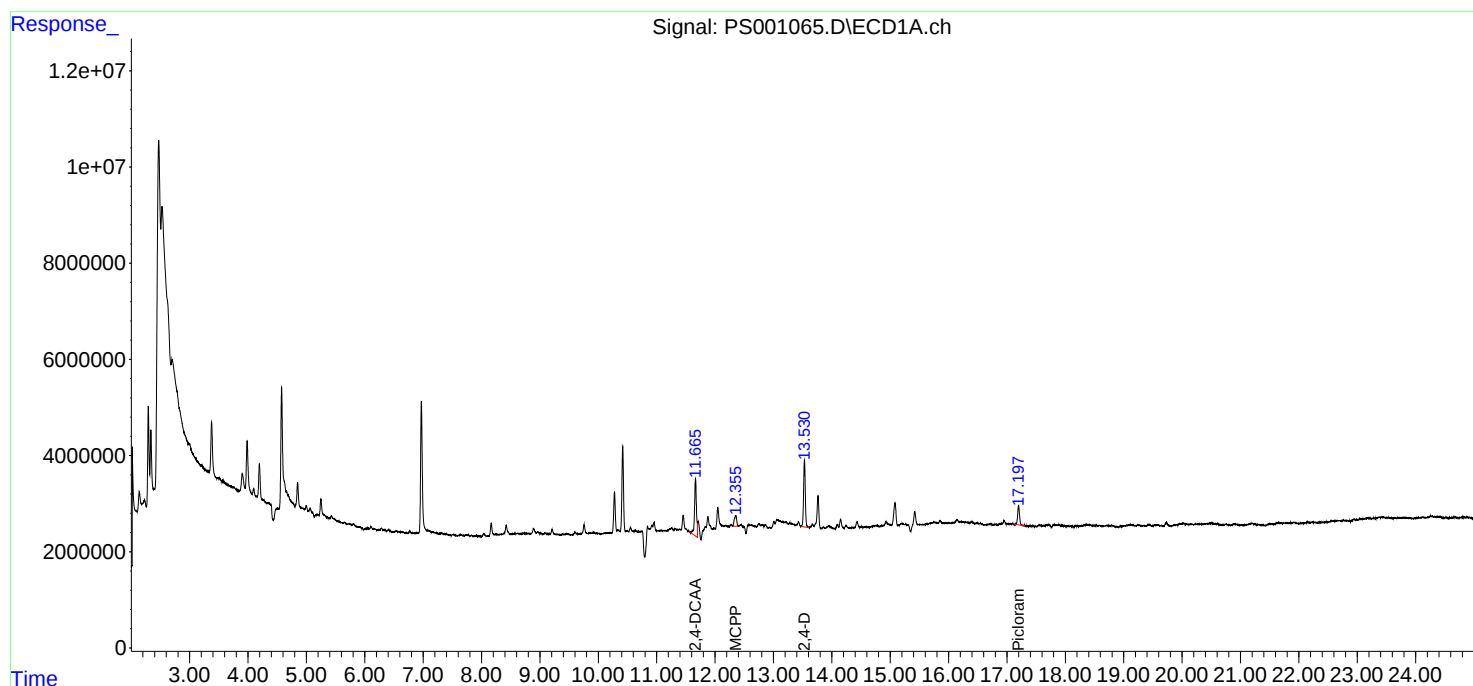


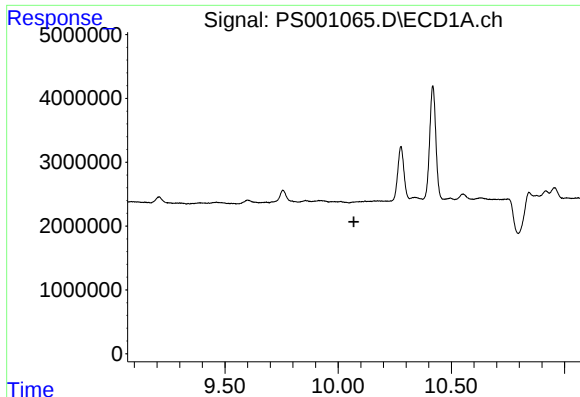

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

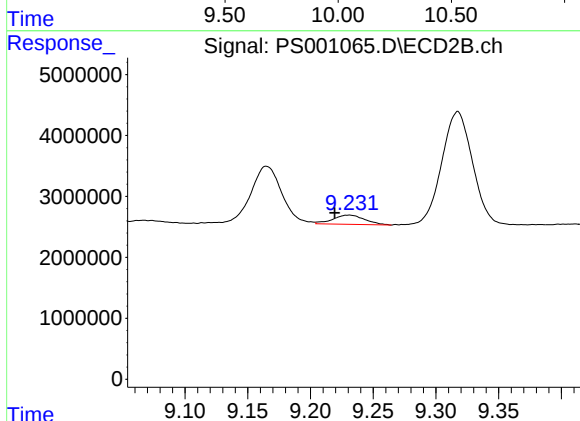


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.231 min
Delta R.T.: 0.012 min
Response: 2705403
Conc: 9.20 ng/ml

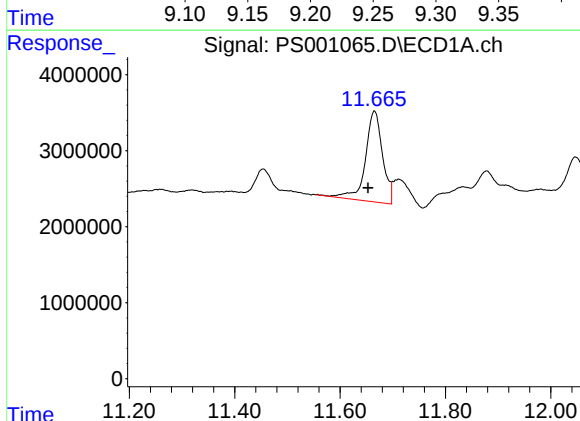


#4 2,4-DCAA

R.T.: 11.665 min
Delta R.T.: 0.012 min
Response: 27117048
Conc: 131.43 ng/ml

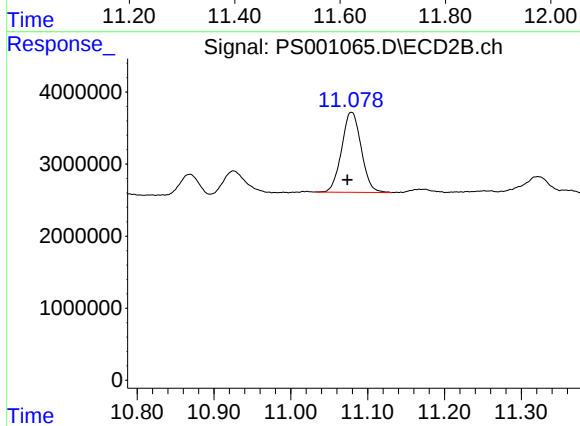

#4 2,4-DCAA


R.T.: 11.079 min
Delta R.T.: 0.005 min
Response: 19622733
Conc: 90.10 ng/ml

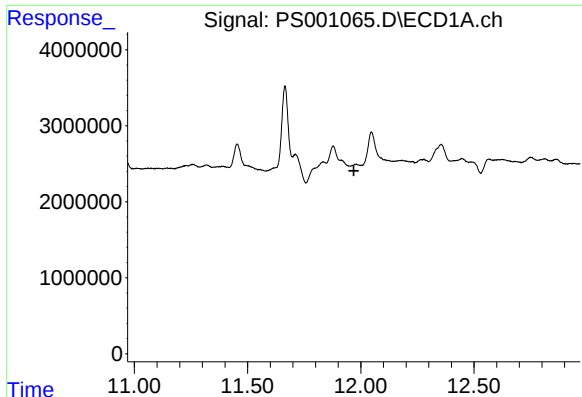

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.970 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

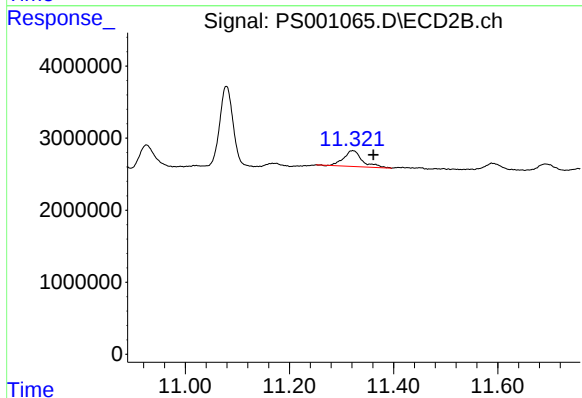


#5 DICAMBA

R.T.: 11.322 min
Delta R.T.: -0.039 min
Response: 5500691
Conc: 7.01 ng/ml

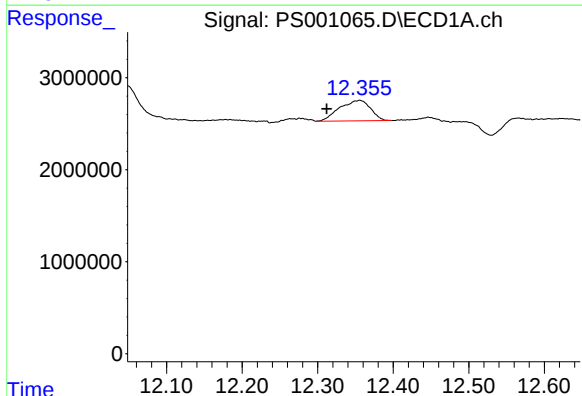


#6 MCP

R.T.: 12.355 min
Delta R.T.: 0.043 min
Response: 6324397
Conc: 11.51 ug/ml

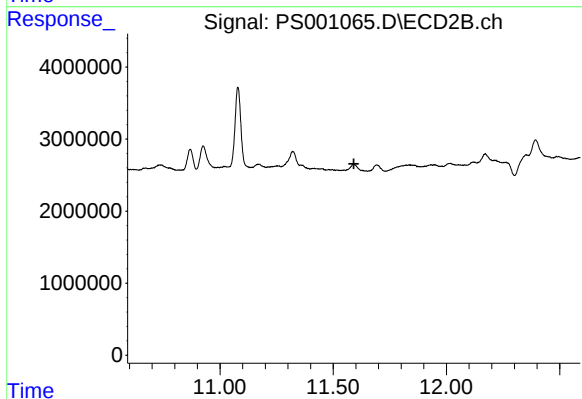

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

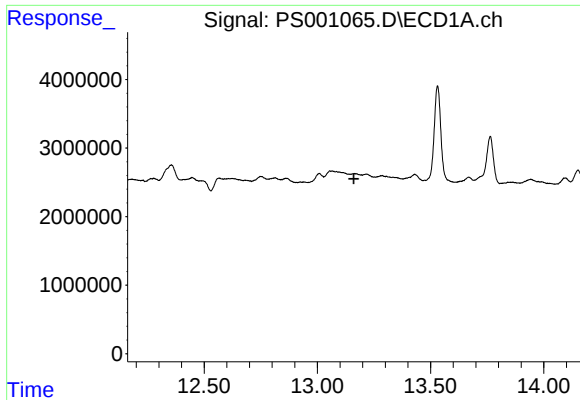

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.161 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

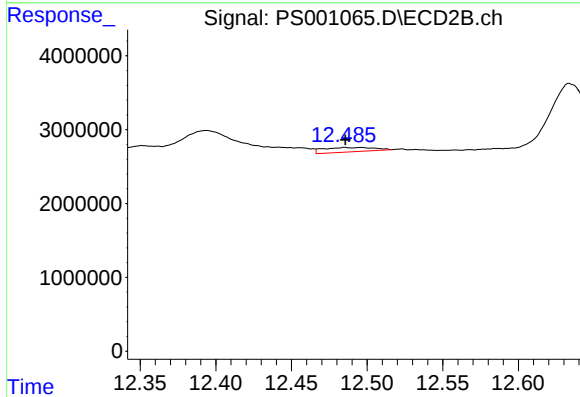


#8 DICHLORPROP

R.T.: 12.485 min
Delta R.T.: 0.000 min
Response: 1397345
Conc: 6.92 ng/ml

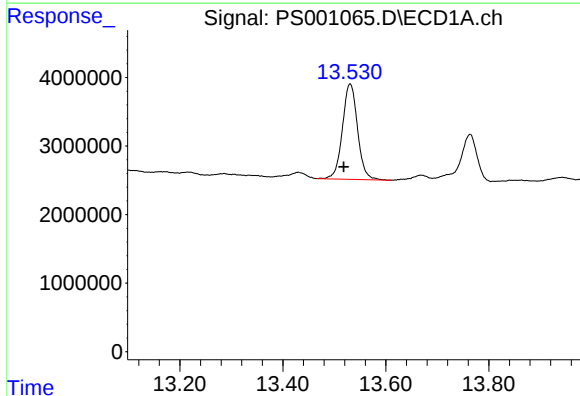


#9 2,4-D

R.T.: 13.531 min
Delta R.T.: 0.013 min
Response: 28394426
Conc: 104.32 ng/ml

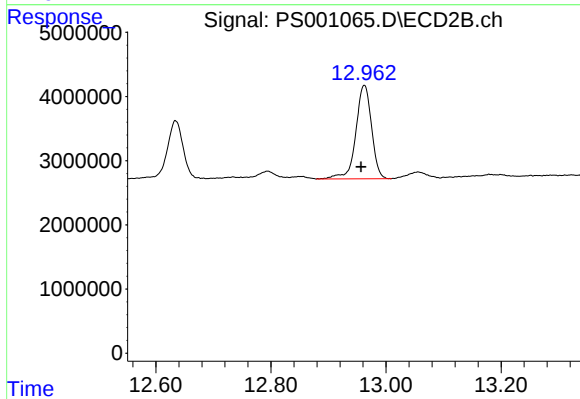

#9 2,4-D


R.T.: 12.962 min
Delta R.T.: 0.006 min
Response: 27806271
Conc: 100.40 ng/ml

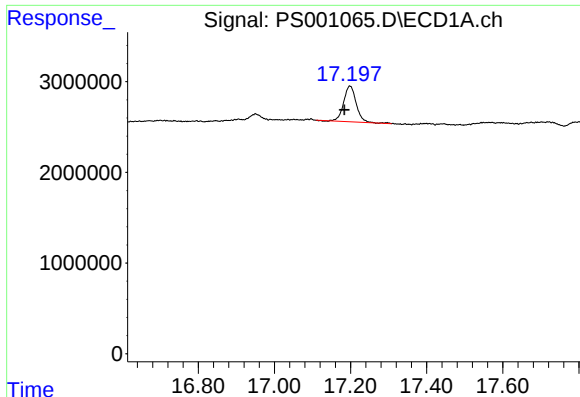

#15 Picloram


R.T.: 17.198 min
Delta R.T.: 0.014 min
Response: 9002187
Conc: 4.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

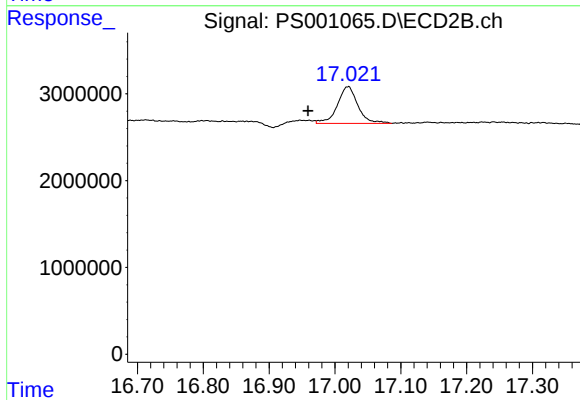


#15 Picloram

R.T.: 17.020 min
Delta R.T.: 0.061 min
Response: 9150724
Conc: 6.01 ng/ml

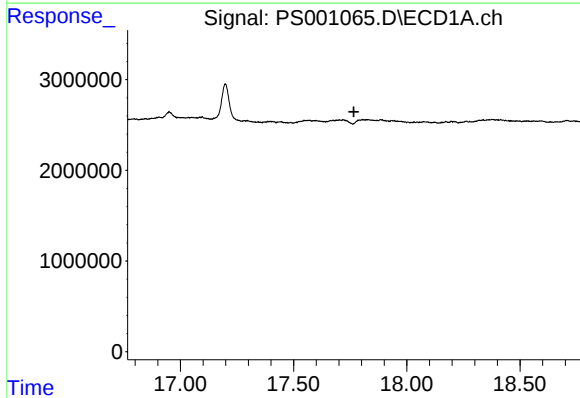

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.766 min
Response: 0
Conc: N.D.

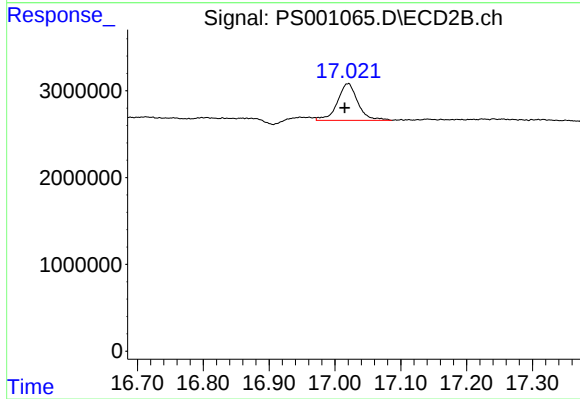

#16 DCPA

R.T.: 17.020 min
Delta R.T.: 0.005 min
Response: 9150724
Conc: 5.32 ng/ml