

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071618\
 Data File : PS001071.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2018 03:05
 Operator : UA
 Sample : J3820-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 04:29:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.688	11.102	27640452	20253352	133.969	92.992 #
Target Compounds							
2) T	3,5-DICHL...	0.000	9.188	0	8214222	N.D.	27.925 #
5) T	DICAMBA	11.901	11.346	1435130	4213192	1.823	5.368 #
6) T	MCPD	12.381	0.000	5846547	0	10.644	N.D. #
7) T	MCPA	12.620	0.000	3002257	0	3.290	N.D. #
10) T	Pentachlo...	0.000	13.463	0	3479280	N.D.	1.109 #
11) T	2,4,5-TP ...	0.000	14.079	0	7398688	N.D.	5.896 #
12) T	2,4,5-T	15.108	14.728	9084305	3982494	7.460	3.849 #
15) T	Picloram	17.220	0.000	2335253	0	1.289	N.D. #
16) T	DCPA	0.000	17.040	0	5175518	N.D.	3.011 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071618\
Data File : PS001071.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2018 03:05
Operator : UA
Sample : J3820-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 04:29:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

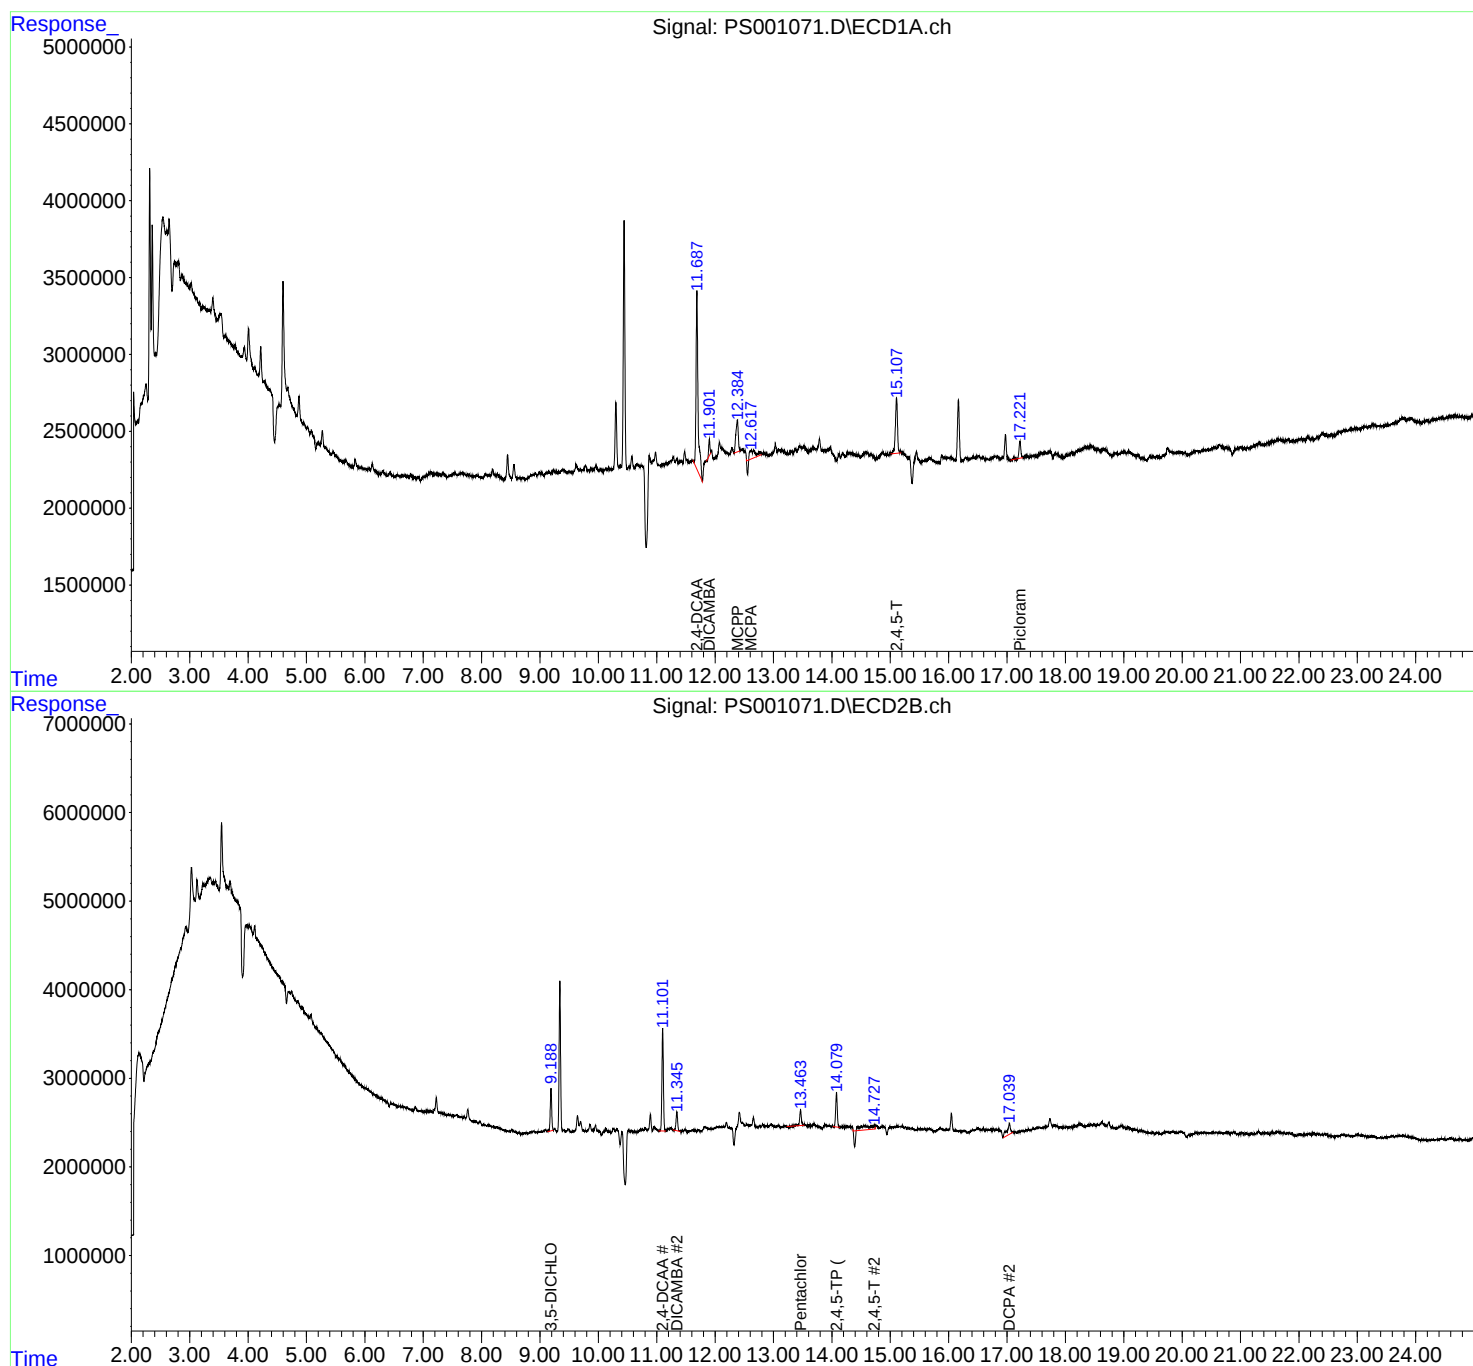


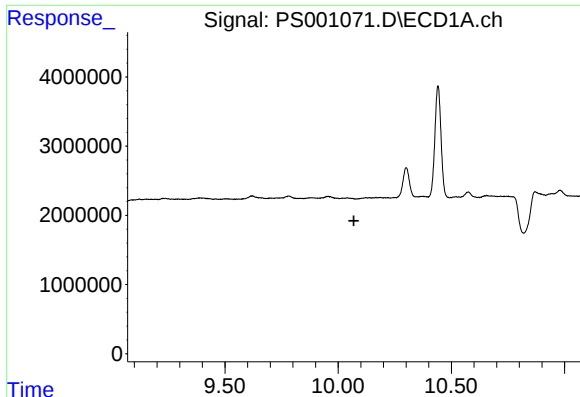

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

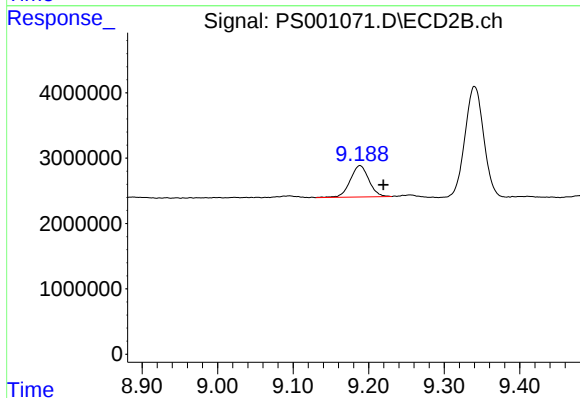


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.188 min
Delta R.T.: -0.031 min
Response: 8214222
Conc: 27.92 ng/ml

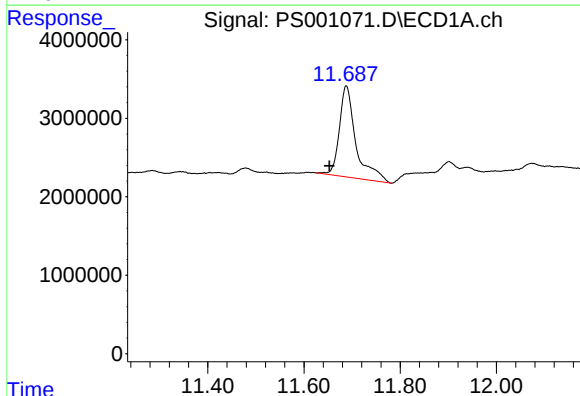


#4 2,4-DCAA

R.T.: 11.688 min
Delta R.T.: 0.035 min
Response: 27640452
Conc: 133.97 ng/ml

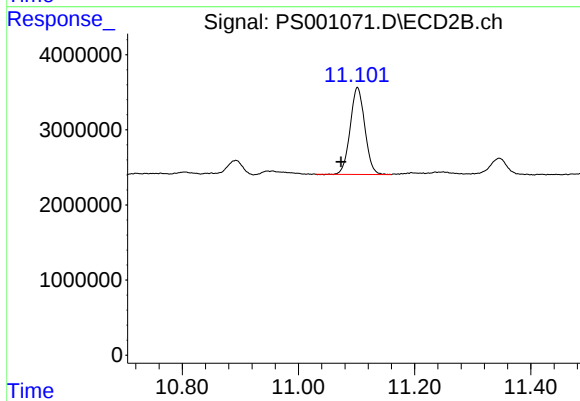

#4 2,4-DCAA


R.T.: 11.102 min
Delta R.T.: 0.028 min
Response: 20253352
Conc: 92.99 ng/ml

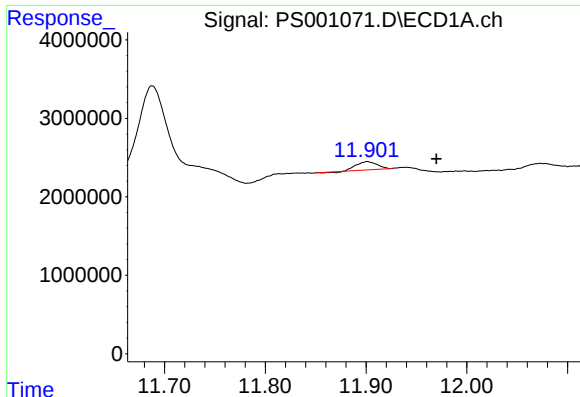

#5 DICAMBA


R.T.: 11.901 min
Delta R.T.: -0.069 min
Response: 1435130
Conc: 1.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

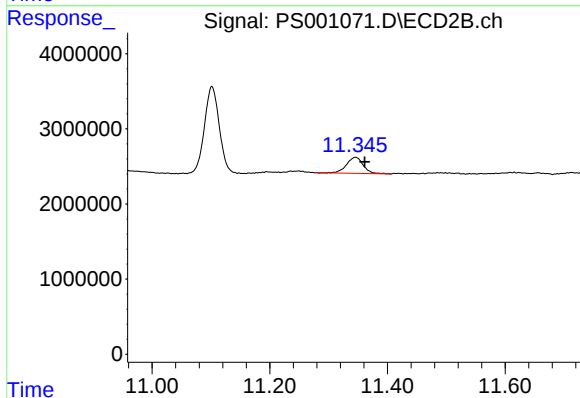


#5 DICAMBA

R.T.: 11.346 min
Delta R.T.: -0.016 min
Response: 4213192
Conc: 5.37 ng/ml

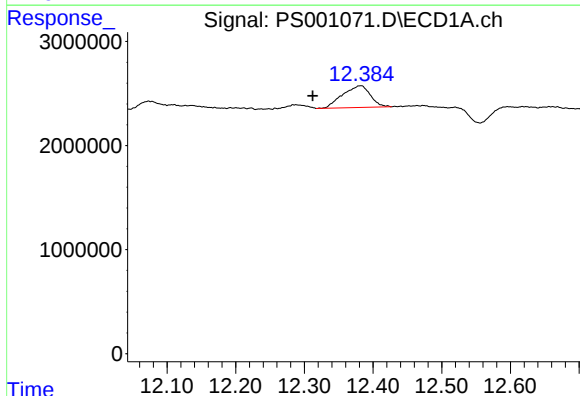


#6 MCP

R.T.: 12.381 min
Delta R.T.: 0.069 min
Response: 5846547
Conc: 10.64 ug/ml

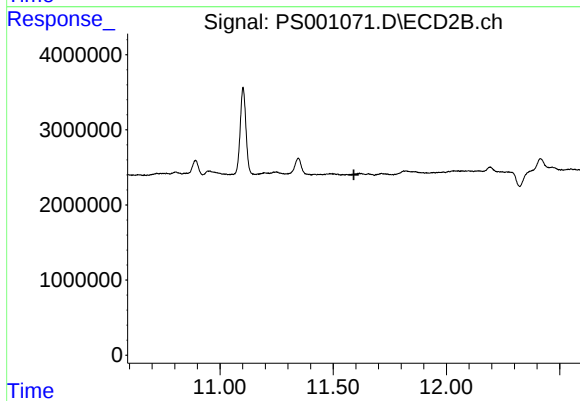

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

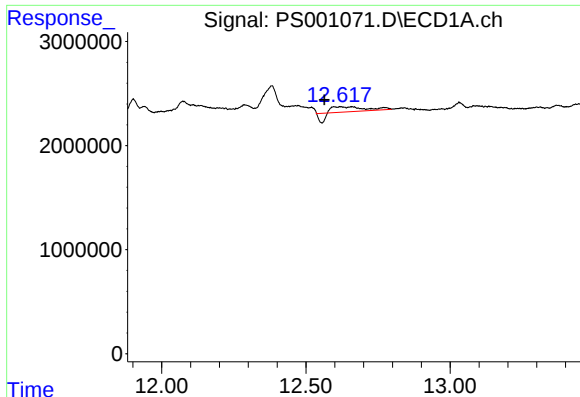

#7 MCPA


R.T.: 12.620 min
Delta R.T.: 0.056 min
Response: 3002257
Conc: 3.29 ug/ml

Instrument :
ECD_S
ClientSampleId :

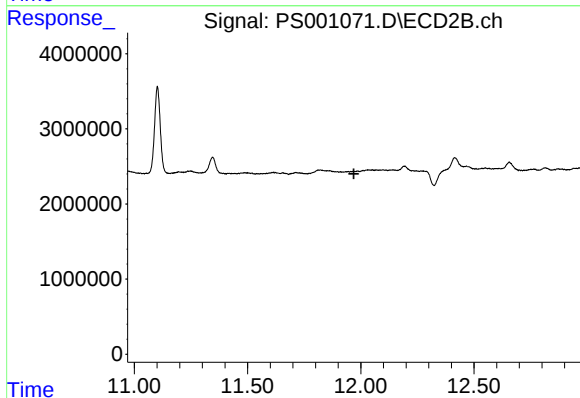


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.969 min
Response: 0
Conc: N.D.

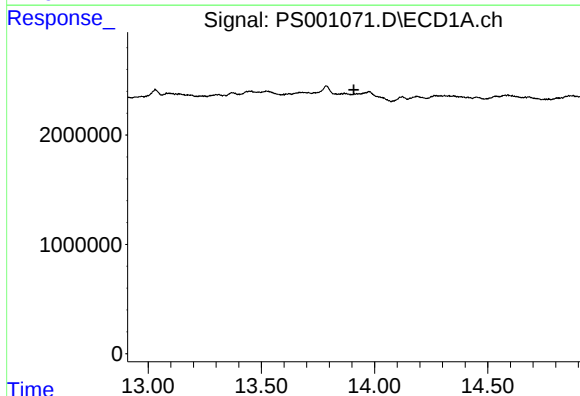


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.908 min
Response: 0
Conc: N.D.

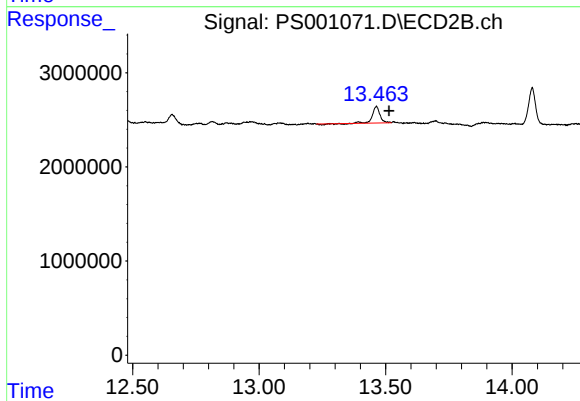

#10 Pentachlorophenol


R.T.: 13.463 min
Delta R.T.: -0.050 min
Response: 3479280
Conc: 1.11 ng/ml

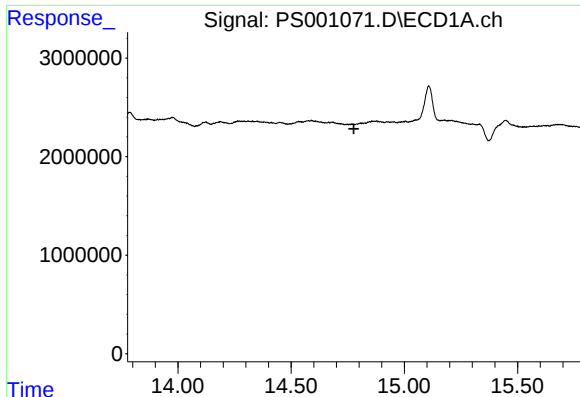

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.777 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

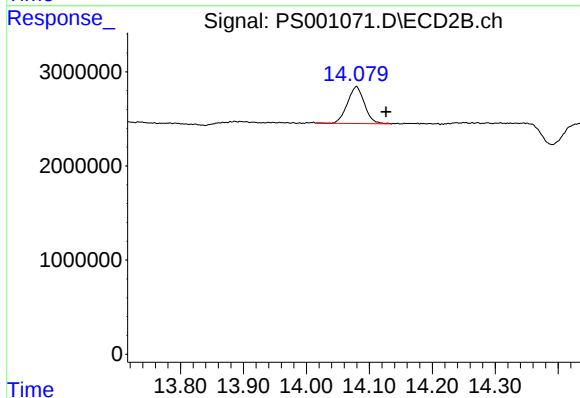


#11 2,4,5-TP (SILVEX)

R.T.: 14.079 min
Delta R.T.: -0.047 min
Response: 7398688
Conc: 5.90 ng/ml

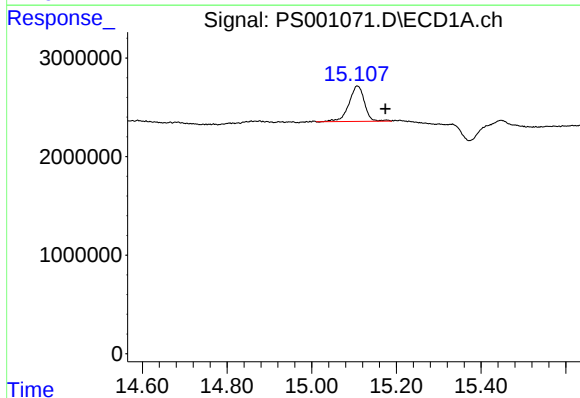


#12 2,4,5-T

R.T.: 15.108 min
Delta R.T.: -0.066 min
Response: 9084305
Conc: 7.46 ng/ml

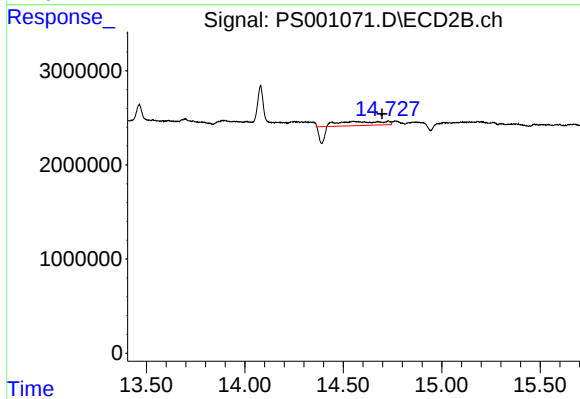

#12 2,4,5-T


R.T.: 14.728 min
Delta R.T.: 0.030 min
Response: 3982494
Conc: 3.85 ng/ml

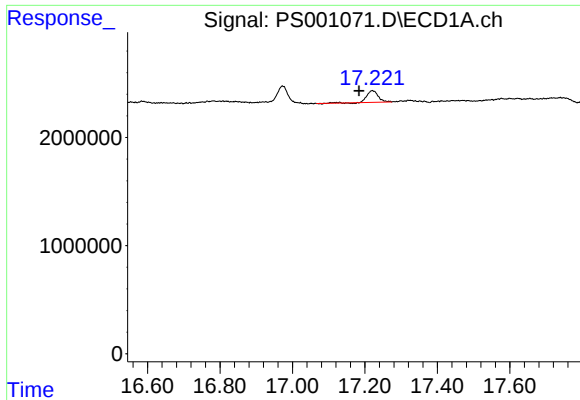

#15 Picloram


R.T.: 17.220 min
Delta R.T.: 0.037 min
Response: 2335253
Conc: 1.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

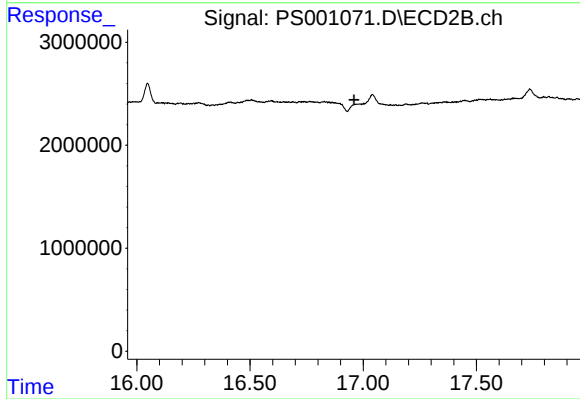


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.959 min
Response: 0
Conc: N.D.

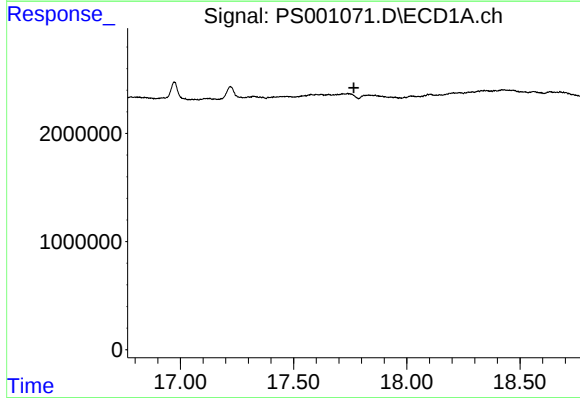

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.766 min
Response: 0
Conc: N.D.

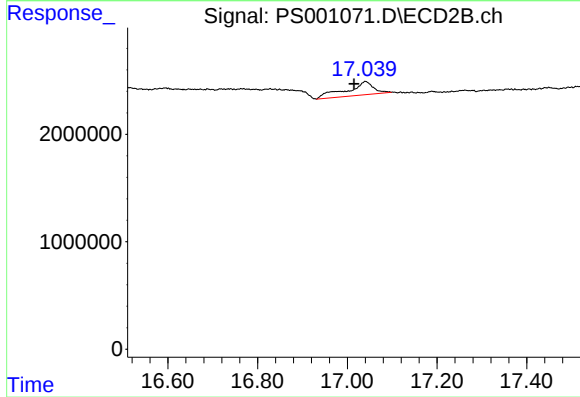

#16 DCPA

R.T.: 17.040 min
Delta R.T.: 0.025 min
Response: 5175518
Conc: 3.01 ng/ml